

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 16:54
 Operator : AR\AJ
 Sample : N1099-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:40:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	5843659	16835223	10.526	10.366
28)	SA Decachlor...	10.318	11.386	10084548	17238571	11.351	10.684
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	1102264	N.D.	0.448 #
9)	A Endosulfan I	0.000	8.372	0	43515	N.D.	0.024 #
10)	B gamma-Chl...	0.000	8.230	0	106282	N.D.	0.053 #
11)	B alpha-Chl...	0.000	8.338f	0	80678	N.D.	0.041 #
15)	B Endosulfa...	0.000	9.123	0	117108	N.D.	0.068 #
18)	B Endrin al...	0.000	9.283f	0	94859	N.D.	0.076 #
25)	Chlordane-3	0.000	8.230	0	106282	N.D.	0.383 #
26)	Chlordane-4	0.000	8.338f	0	80678	N.D.	0.243 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 16:54
Operator : AR\AJ
Sample : N1099-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:40:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

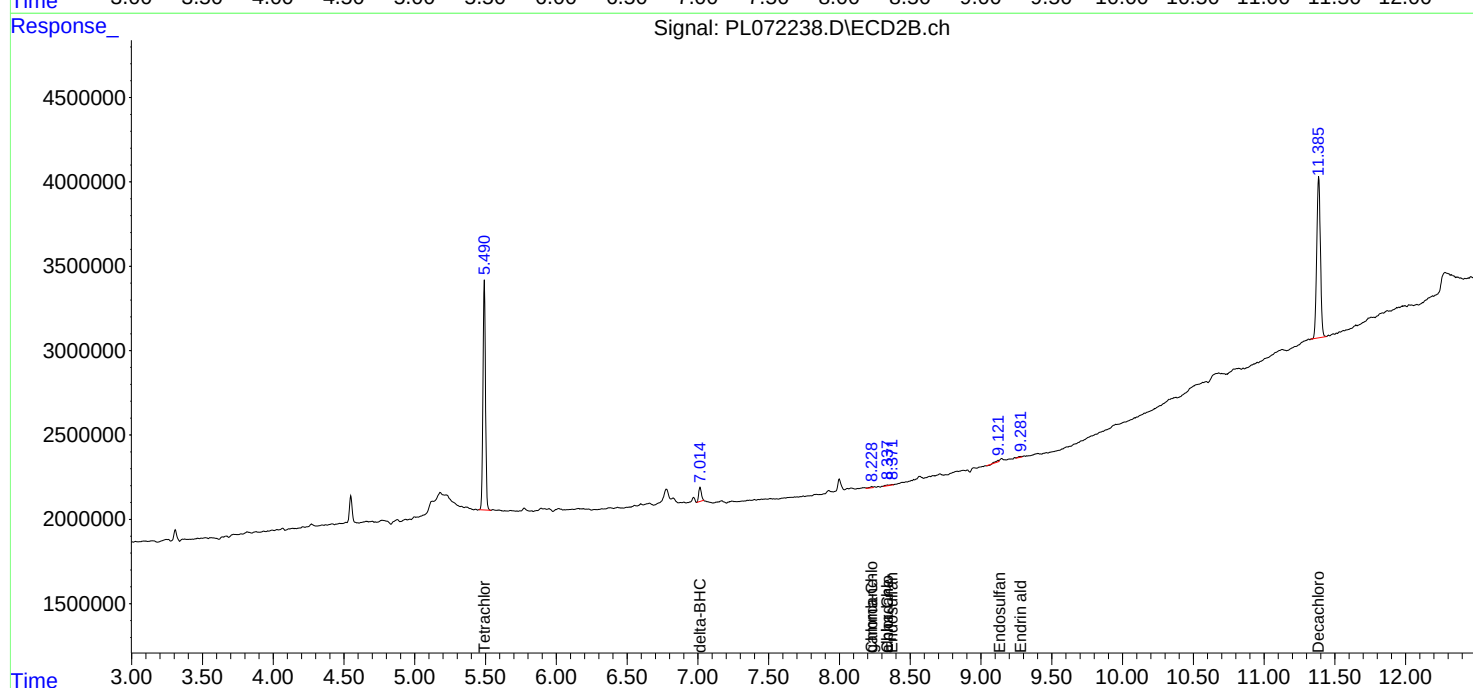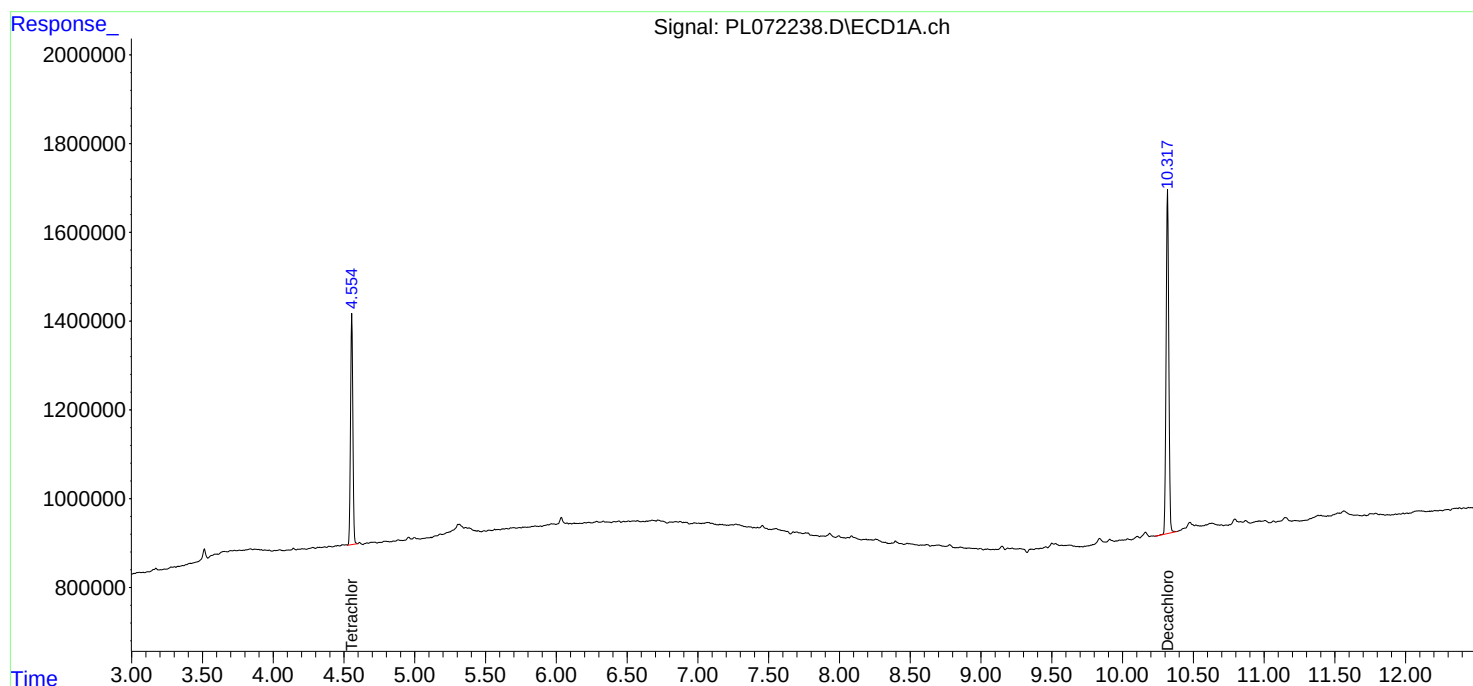


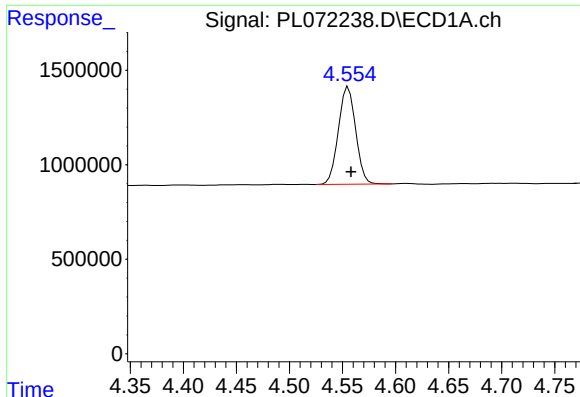

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 5843659
Conc: 10.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

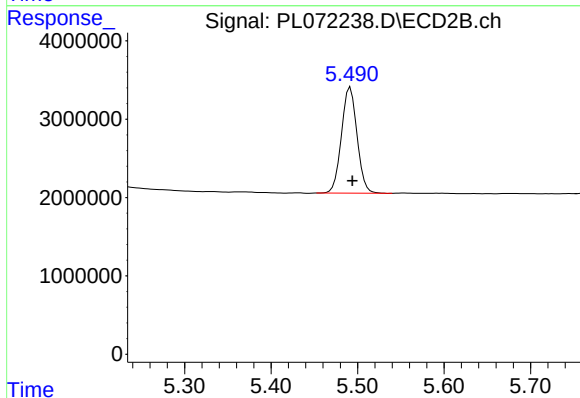


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 16835223
Conc: 10.37 ng/ml

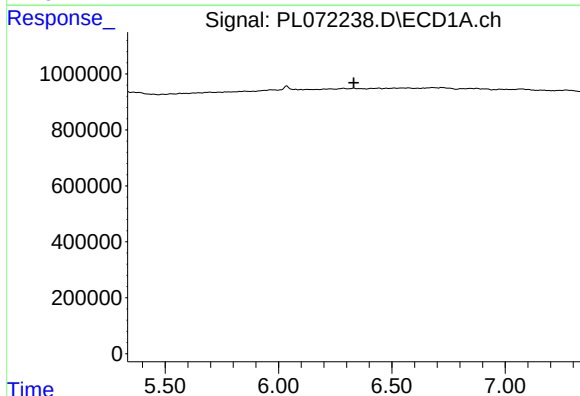


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

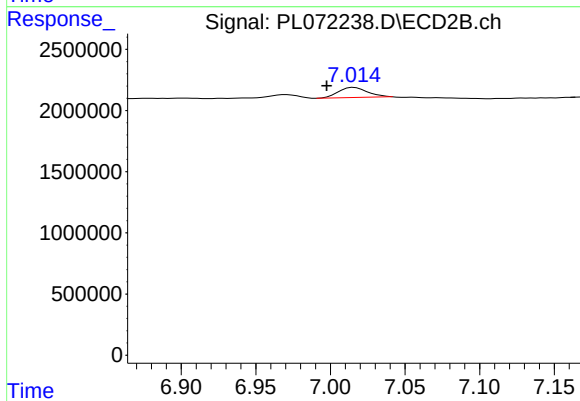

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.018 min
Response: 1102264
Conc: 0.45 ng/ml

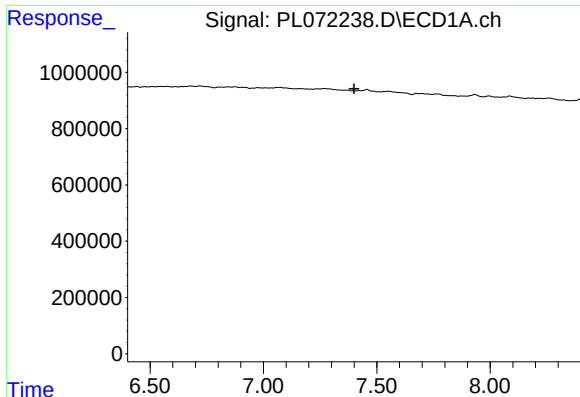

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

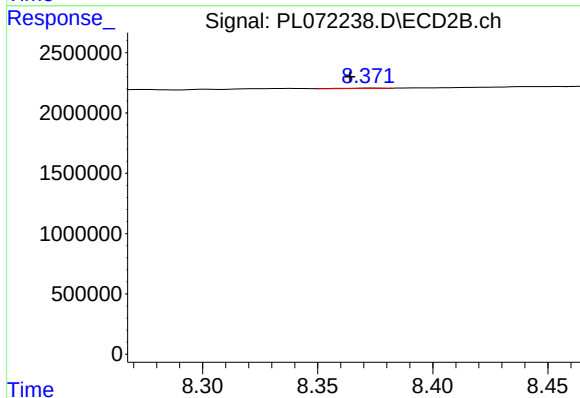


#9 Endosulfan I

R.T.: 8.372 min
Delta R.T.: 0.008 min
Response: 43515
Conc: 0.02 ng/ml

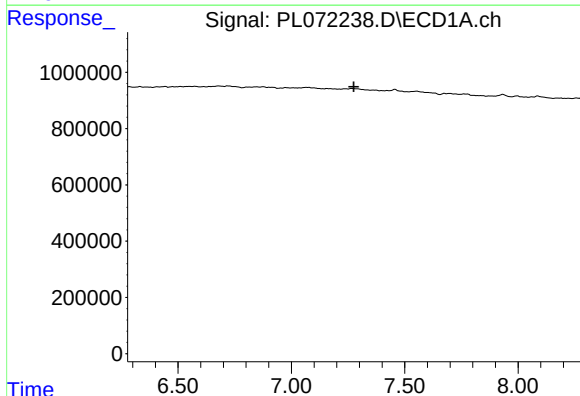


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

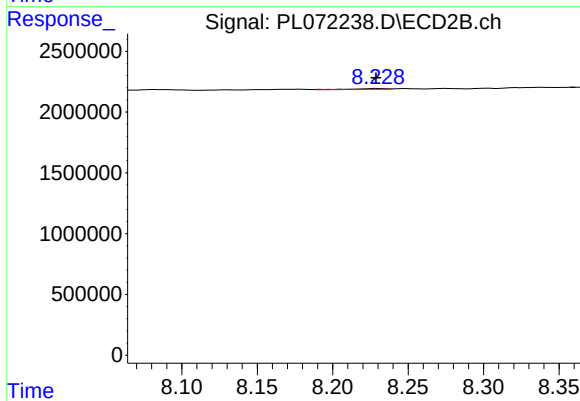

#10 gamma-Chlordane


R.T.: 8.230 min
Delta R.T.: 0.001 min
Response: 106282
Conc: 0.05 ng/ml

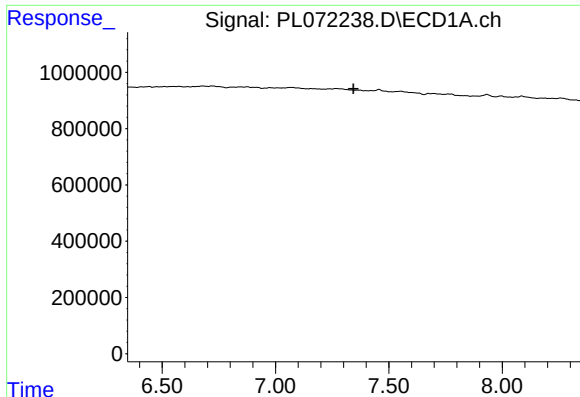

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

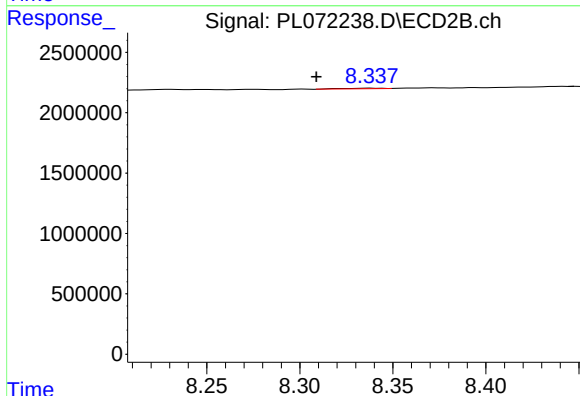


#11 alpha-Chlordane

R.T.: 8.338 min
Delta R.T.: 0.030 min
Response: 80678
Conc: 0.04 ng/ml

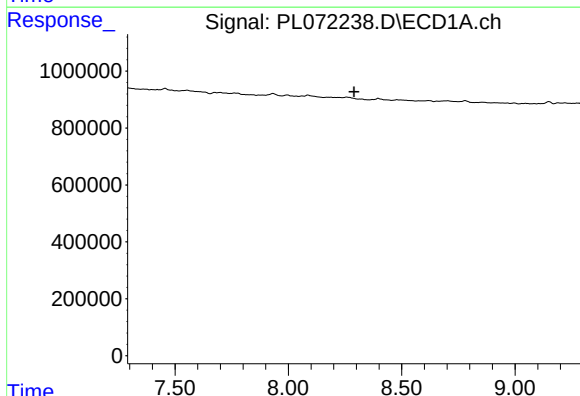


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

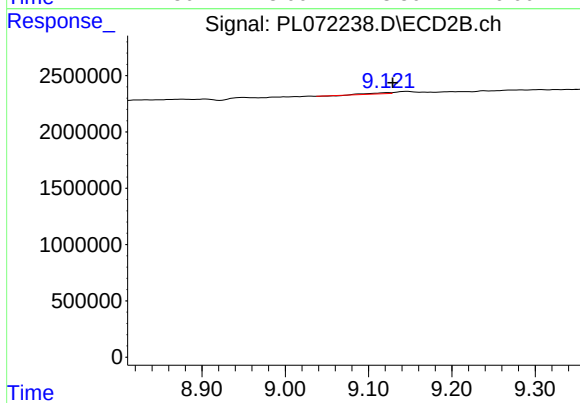

#15 Endosulfan II


R.T.: 9.123 min
Delta R.T.: -0.006 min
Response: 117108
Conc: 0.07 ng/ml

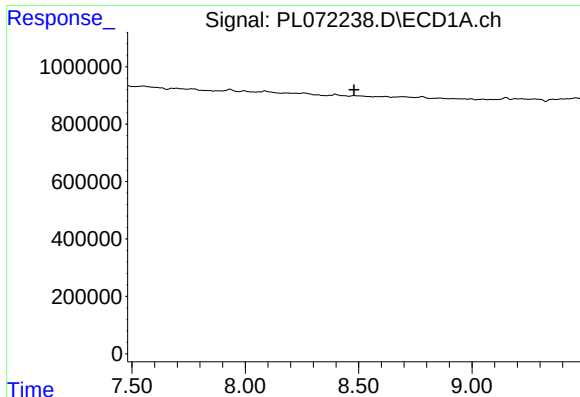

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

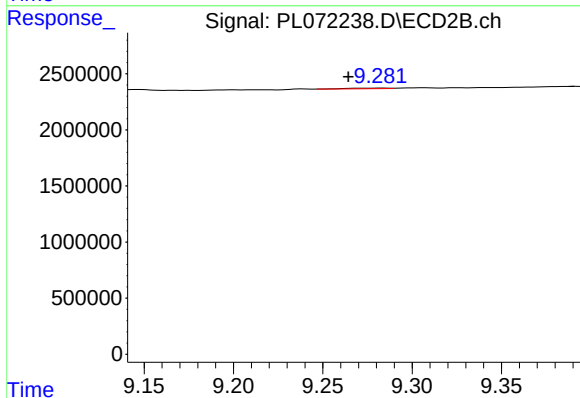


#18 Endrin aldehyde

R.T.: 9.283 min
Delta R.T.: 0.019 min
Response: 94859
Conc: 0.08 ng/ml

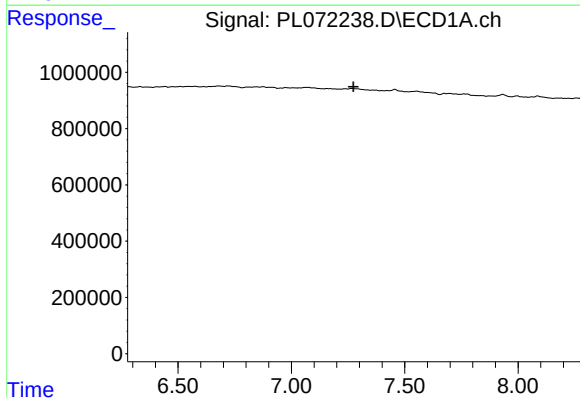


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

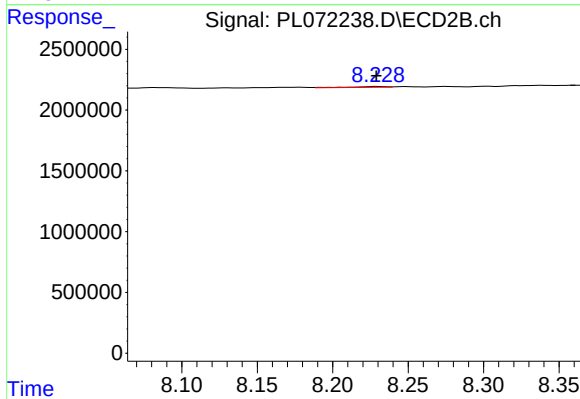

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.001 min
Response: 106282
Conc: 0.38 ng/ml

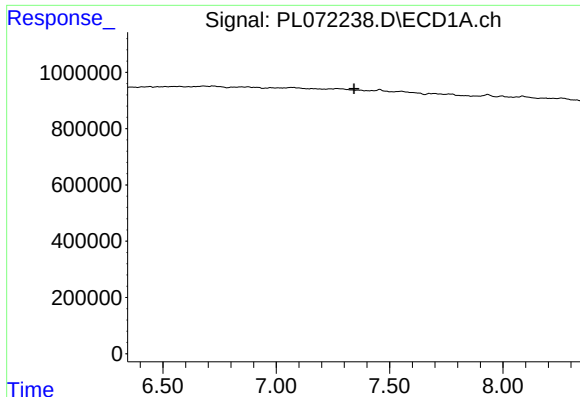

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-05

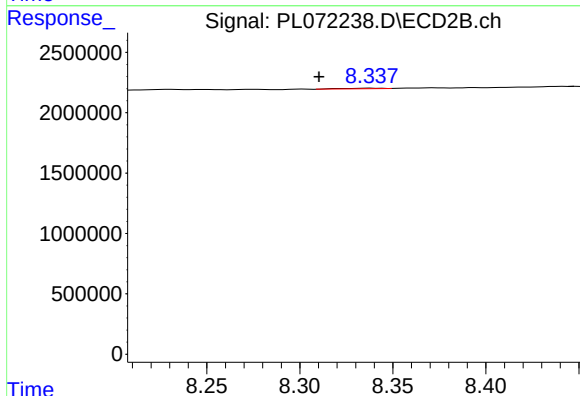


#26 Chlordane-4

R.T.: 8.338 min
Delta R.T.: 0.028 min
Response: 80678
Conc: 0.24 ng/ml

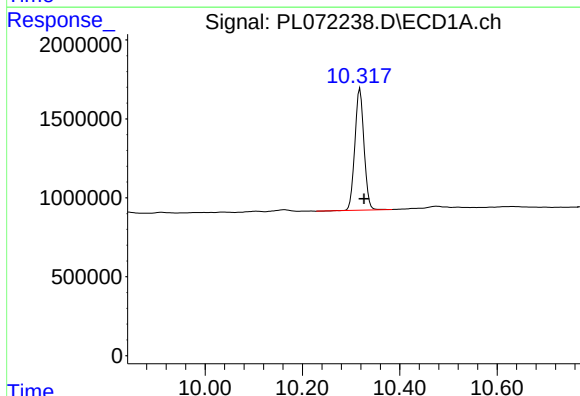

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 10084548
Conc: 11.35 ng/ml

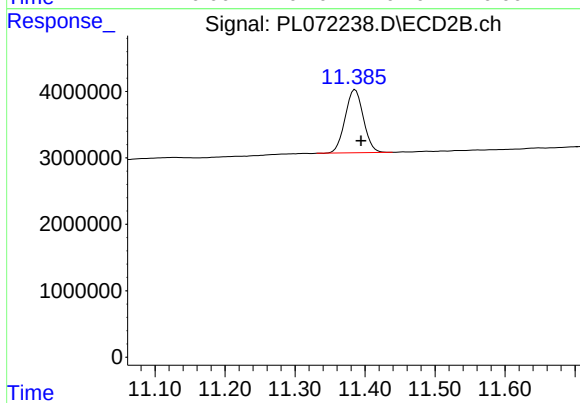

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 17238571
Conc: 10.68 ng/ml