

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 17:10
 Operator : AR\AJ
 Sample : N1099-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:40:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	6600517	18804557	11.889	11.578
28)	SA Decachlor...	10.319	11.385	12087380	20739196	13.605	12.854
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	1097804	N.D.	0.446 #
9)	A Endosulfan I	0.000	8.344f	0	96951	N.D.	0.054 #
10)	B gamma-Chl...	0.000	8.228	0	124960	N.D.	0.062 #
15)	B Endosulfa...	0.000	9.145f	0	365421	N.D.	0.213 #
16)	A 4,4'-DDD	0.000	9.031	0	68362	N.D.	0.048 #
25)	Chlordane-3	0.000	8.228	0	124960	N.D.	0.450 #
27)	Chlordane-5	0.000	9.203	0	104837	N.D.	1.718 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 17:10
Operator : AR\AJ
Sample : N1099-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:40:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

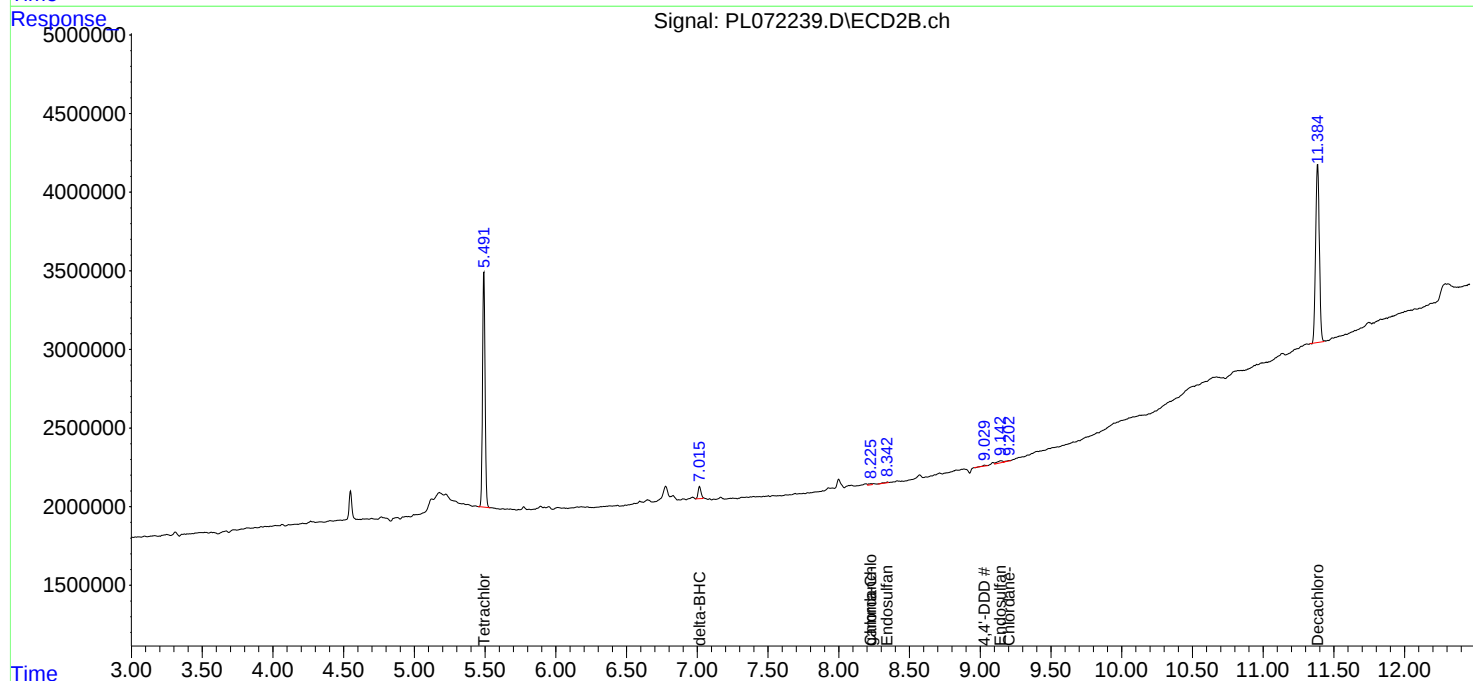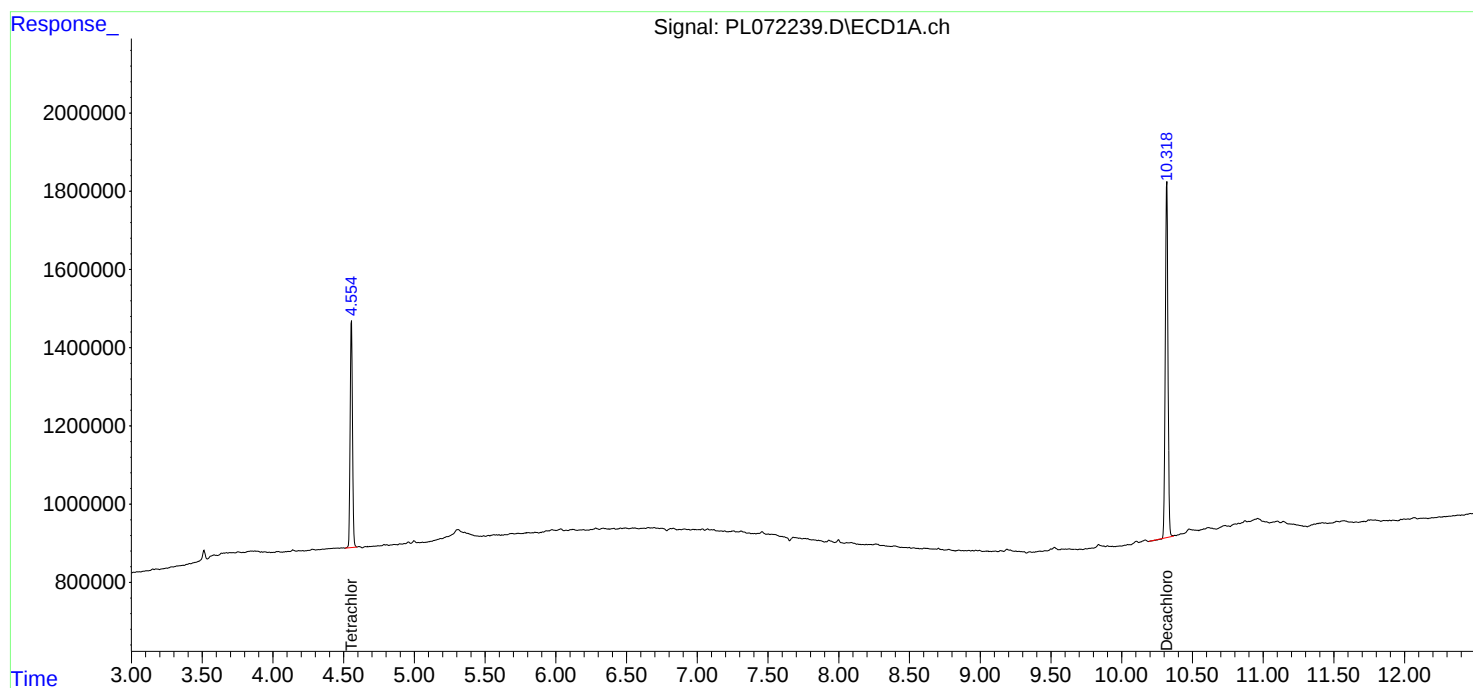


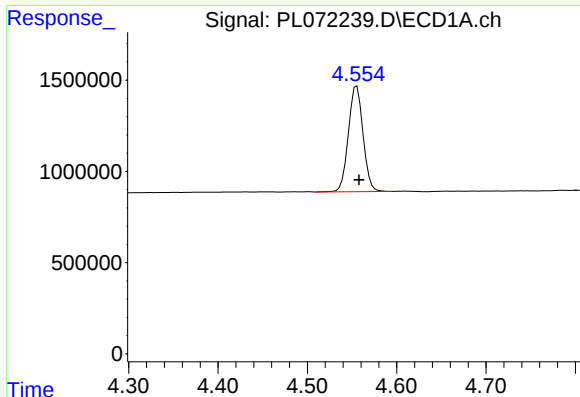

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 6600517
Conc: 11.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

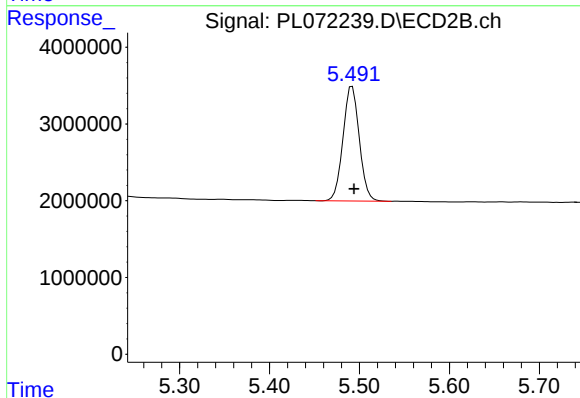


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 18804557
Conc: 11.58 ng/ml

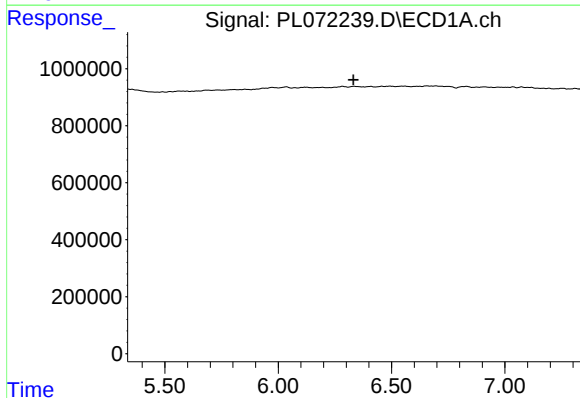


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

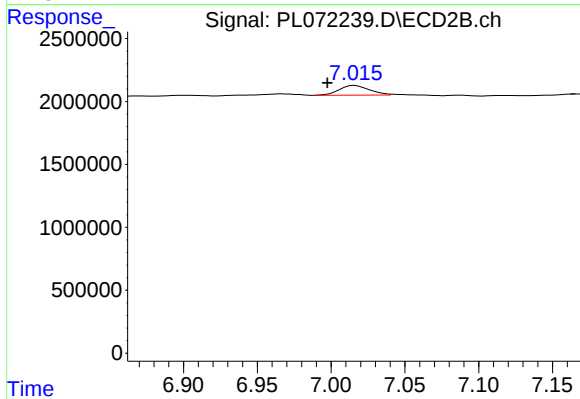

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.019 min
Response: 1097804
Conc: 0.45 ng/ml

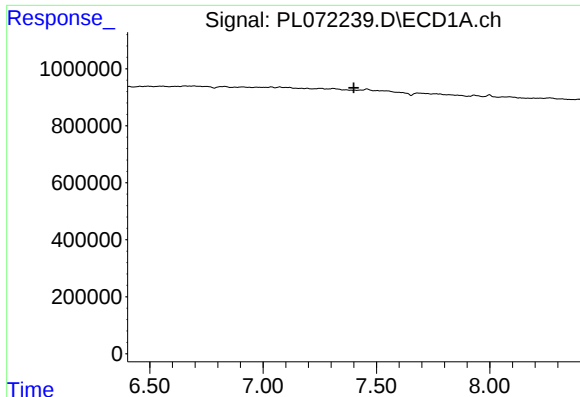

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

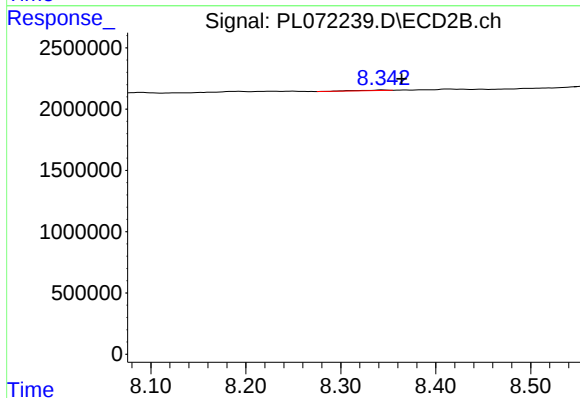


#9 Endosulfan I

R.T.: 8.344 min
Delta R.T.: -0.020 min
Response: 96951
Conc: 0.05 ng/ml

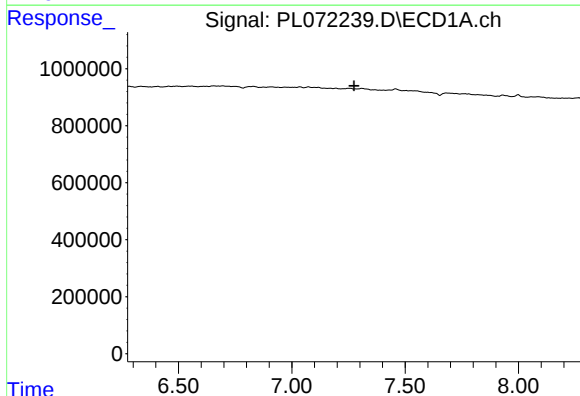


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

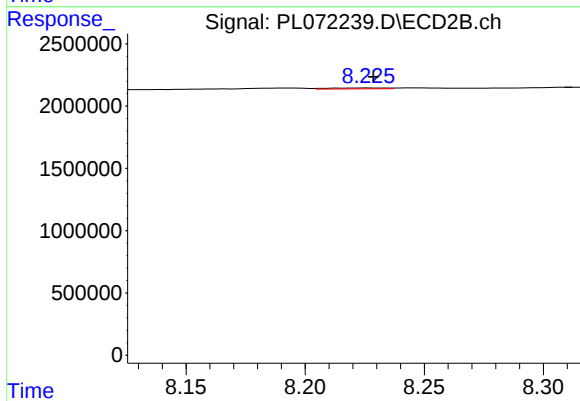

#10 gamma-Chlordane


R.T.: 8.228 min
Delta R.T.: -0.001 min
Response: 124960
Conc: 0.06 ng/ml

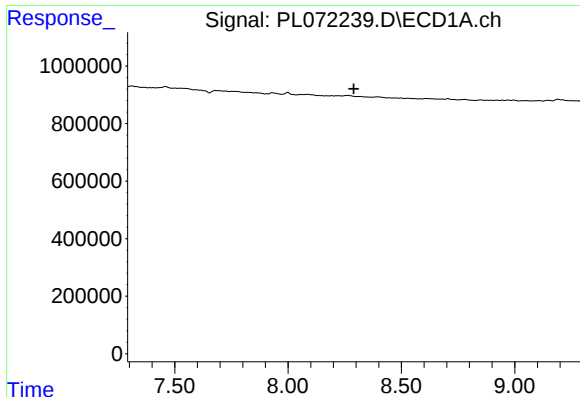

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

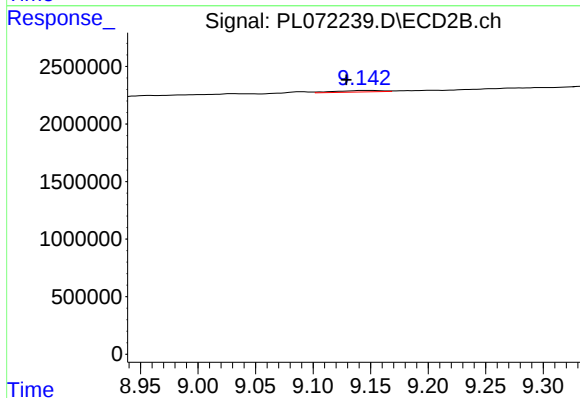


#15 Endosulfan II

R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 365421
Conc: 0.21 ng/ml

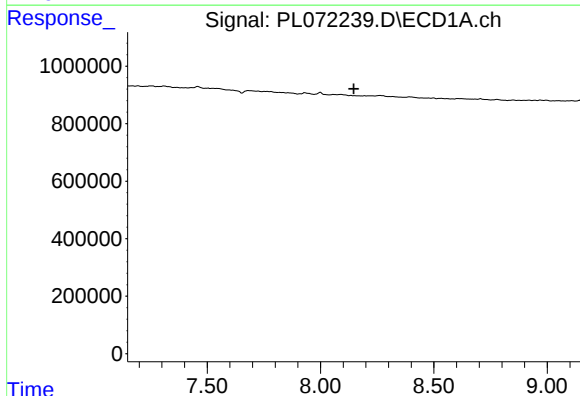


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

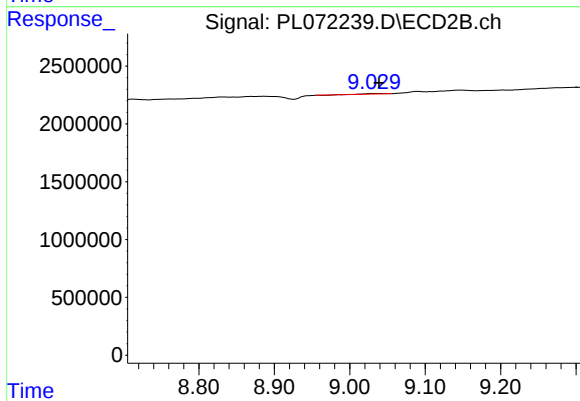

#16 4,4'-DDD


R.T.: 9.031 min
Delta R.T.: -0.008 min
Response: 68362
Conc: 0.05 ng/ml

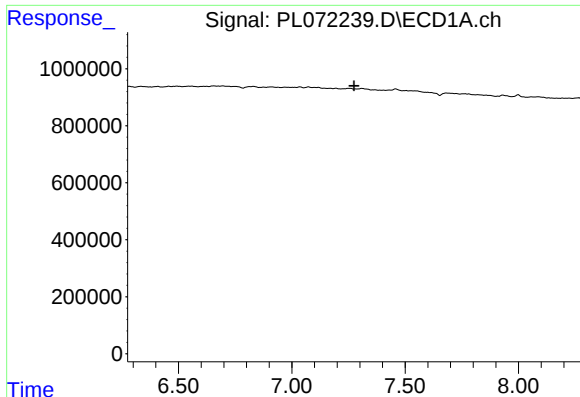

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

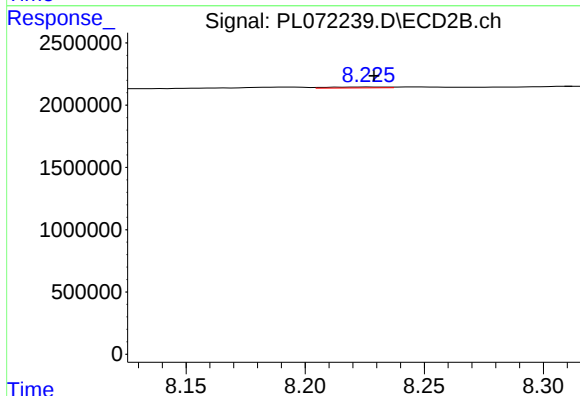


#25 Chlordane-3

R.T.: 8.228 min
Delta R.T.: -0.001 min
Response: 124960
Conc: 0.45 ng/ml

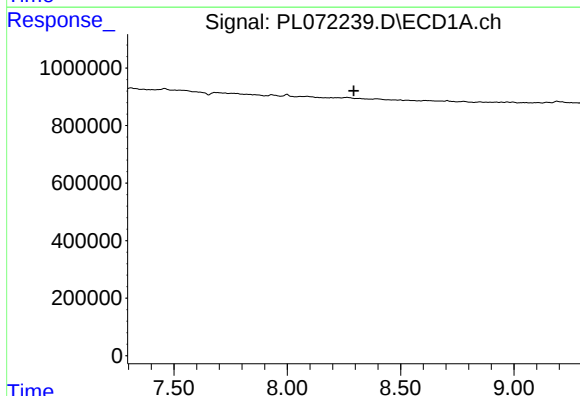


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

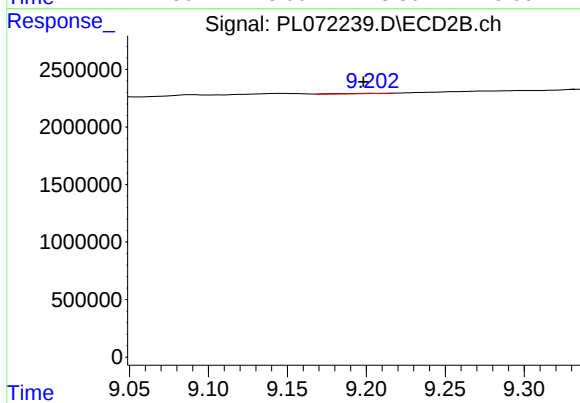

#27 Chlordane-5


R.T.: 9.203 min
Delta R.T.: 0.005 min
Response: 104837
Conc: 1.72 ng/ml

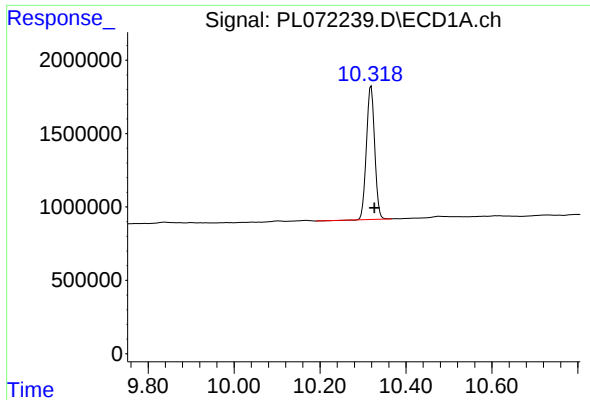

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.008 min
Response: 12087380
Conc: 13.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06

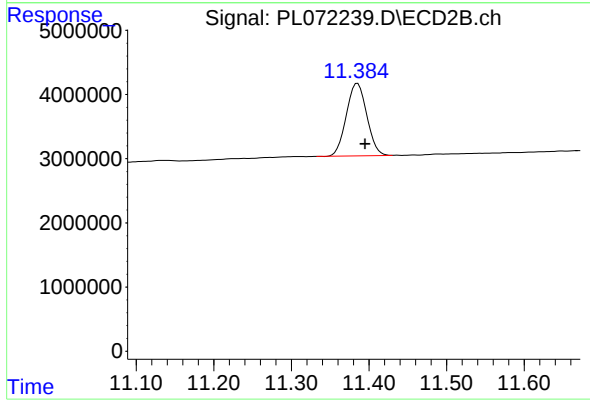

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.009 min
Response: 20739196
Conc: 12.85 ng/ml