

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 17:26
 Operator : AR\AJ
 Sample : N1099-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:40:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	6272005	18377142	11.297	11.315
28)	SA Decachlor...	10.318	11.386	11919487	20910526	13.416	12.960
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	1025300	N.D.	0.417 #
9)	A Endosulfan I	0.000	8.342f	0	43900	N.D.	0.024 #
15)	B Endosulfa...	0.000	9.149f	0	266860	N.D.	0.156 #
16)	A 4,4'-DDD	0.000	9.039	0	93772	N.D.	0.066 #
19)	B Endosulfa...	0.000	9.504	0	61688	N.D.	0.040 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 17:26
Operator : AR\AJ
Sample : N1099-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:40:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

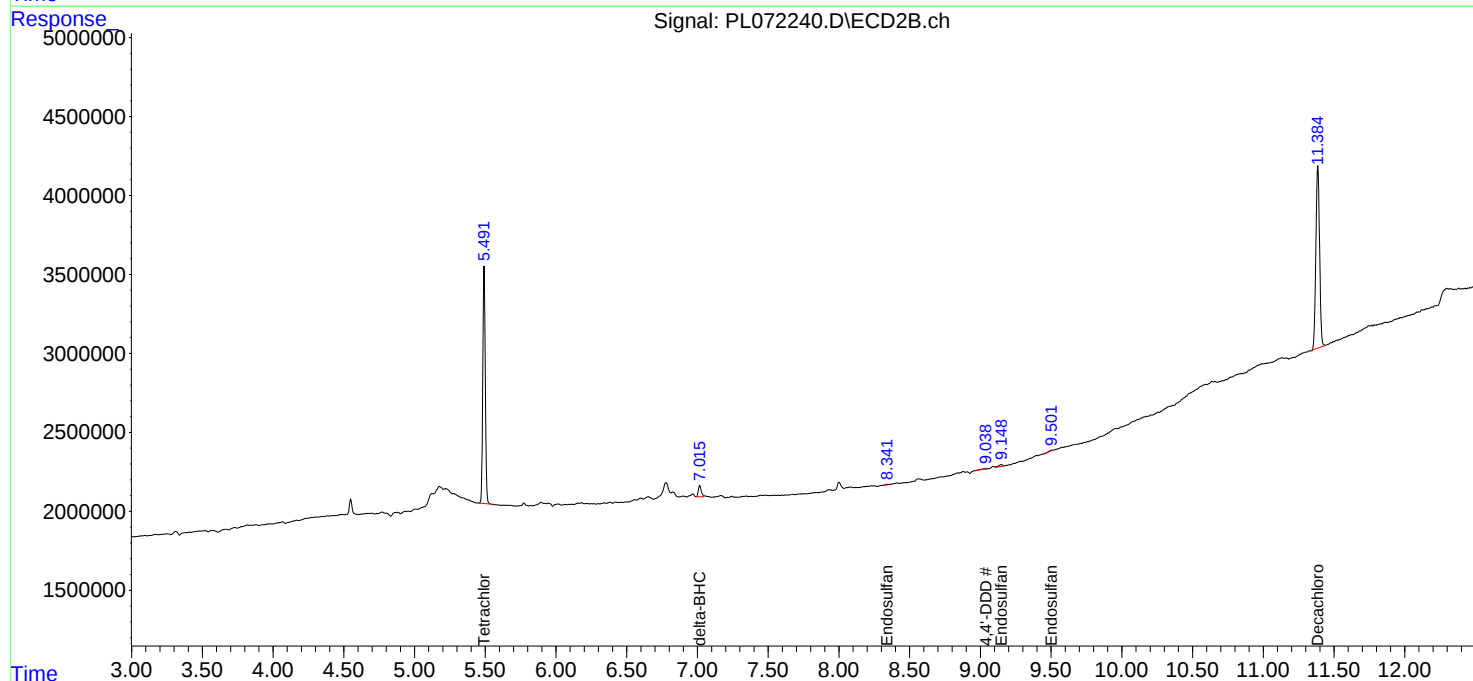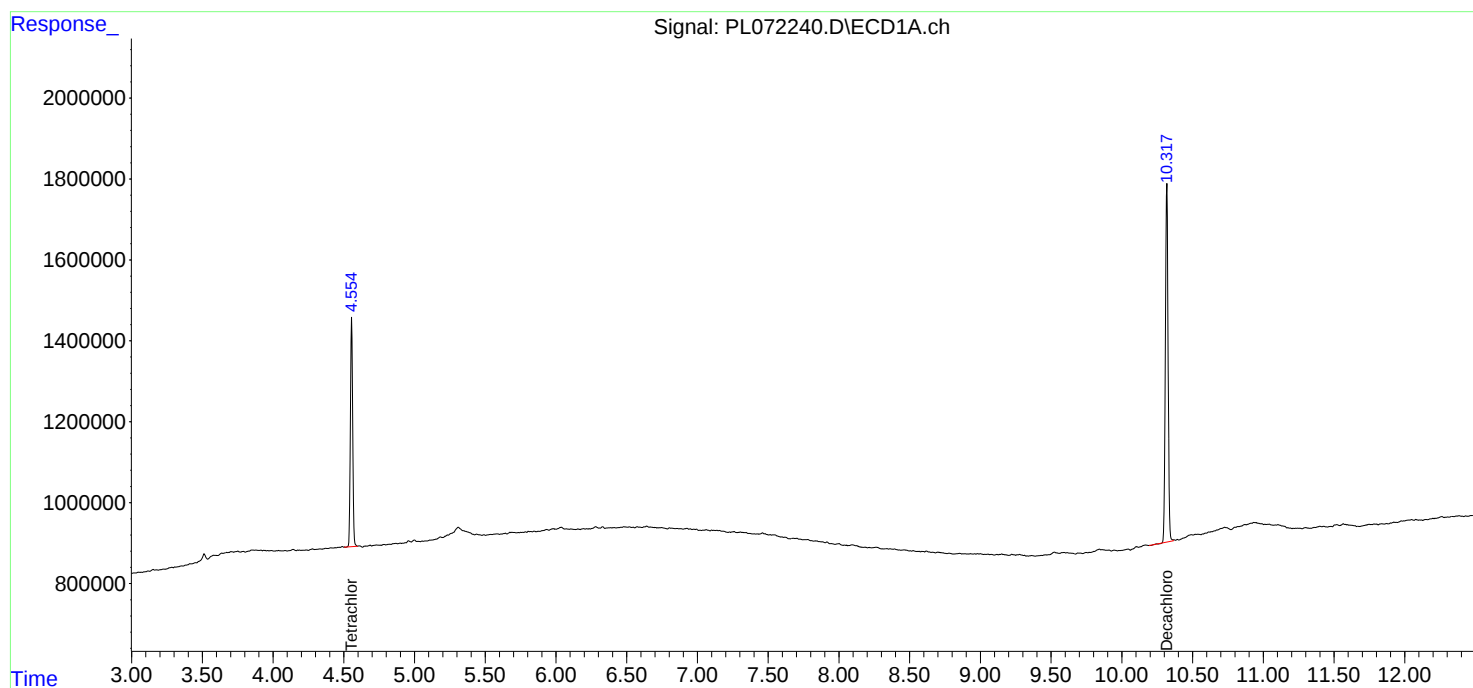


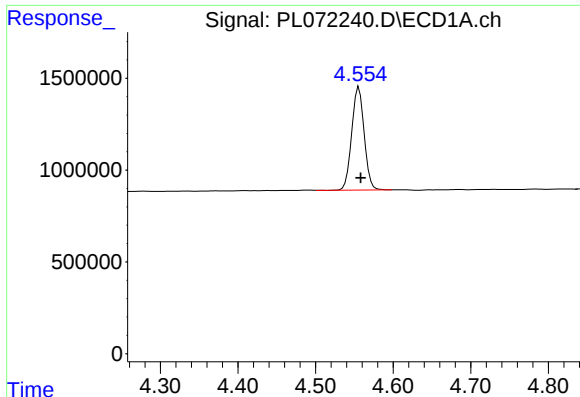

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 6272005
Conc: 11.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

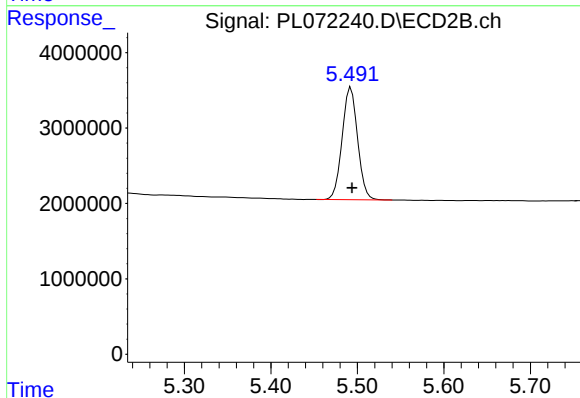


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 18377142
Conc: 11.32 ng/ml

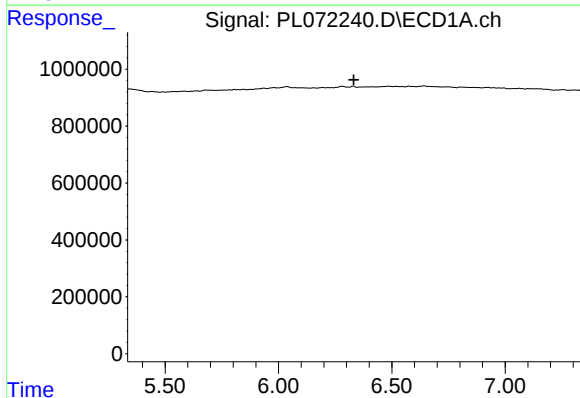


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

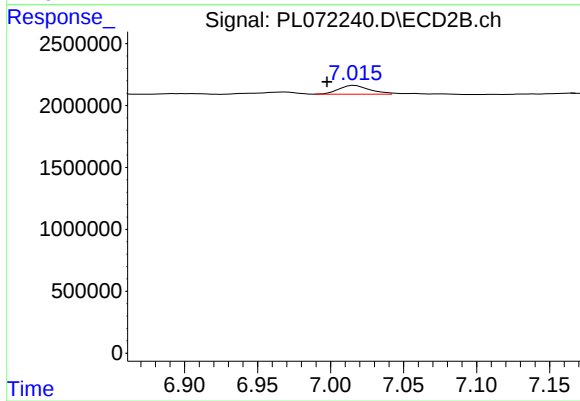

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 1025300
Conc: 0.42 ng/ml

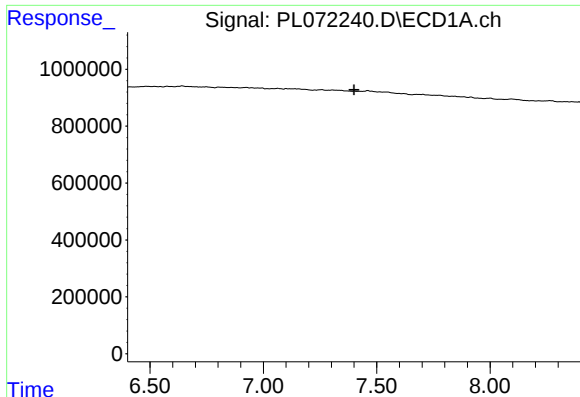

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

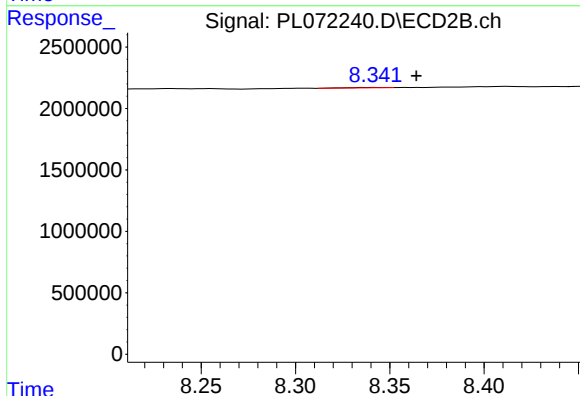


#9 Endosulfan I

R.T.: 8.342 min
Delta R.T.: -0.022 min
Response: 43900
Conc: 0.02 ng/ml

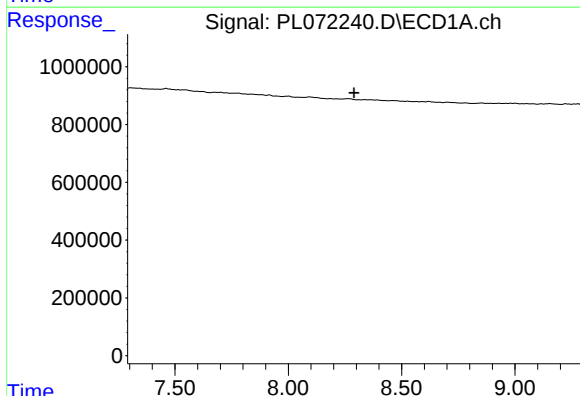


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

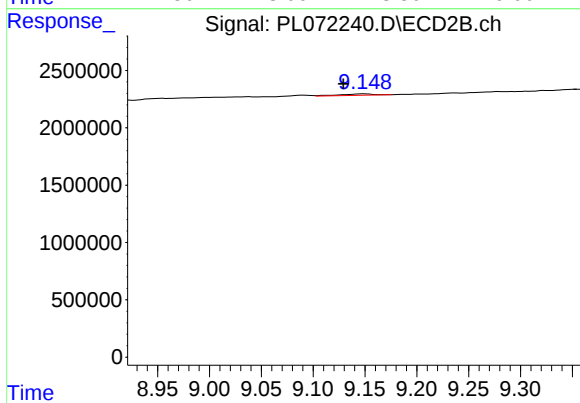

#15 Endosulfan II


R.T.: 9.149 min
Delta R.T.: 0.020 min
Response: 266860
Conc: 0.16 ng/ml

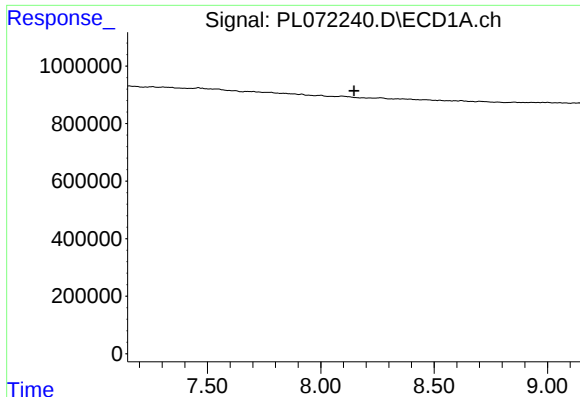

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

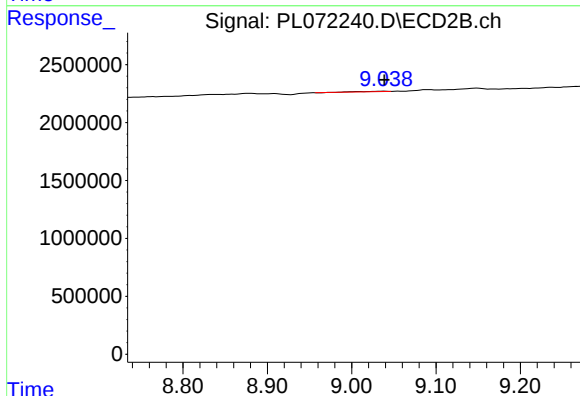


#16 4,4'-DDD

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 93772
Conc: 0.07 ng/ml

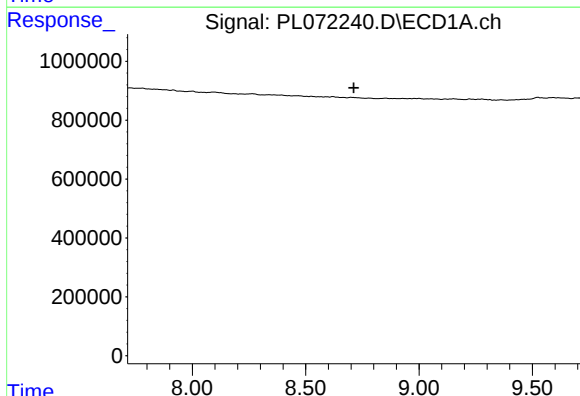


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

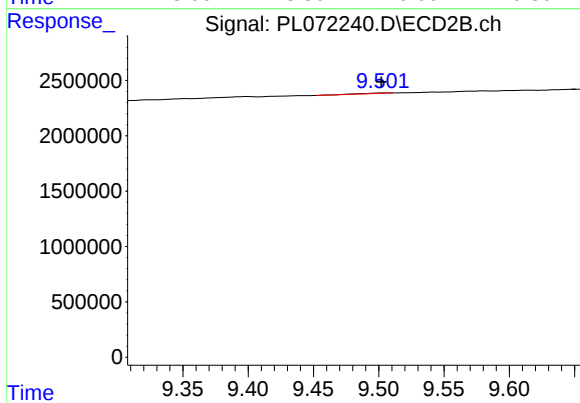

#19 Endosulfan Sulfate


R.T.: 9.504 min
Delta R.T.: 0.002 min
Response: 61688
Conc: 0.04 ng/ml

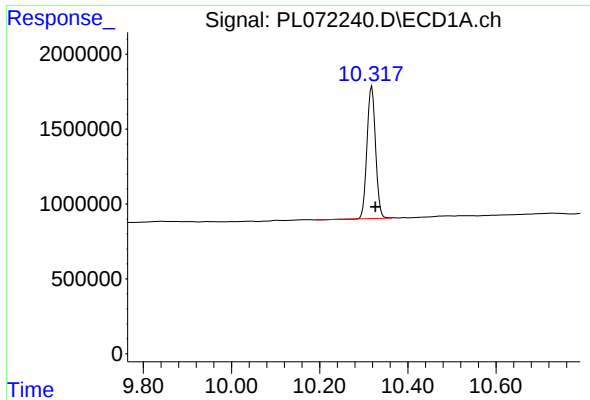

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 11919487
Conc: 13.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-07

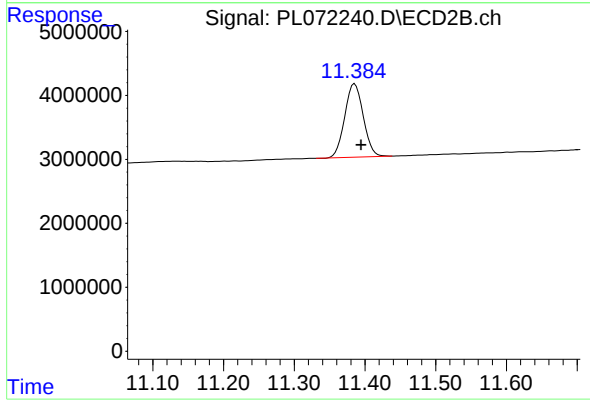

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 20910526
Conc: 12.96 ng/ml