

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 18:15
 Operator : AR\AJ
 Sample : N1099-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:40:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	6122518	18456713	11.028	11.364
28)	SA Decachlor...	10.317	11.385	12054408	21338920	13.568	13.225
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	1329299	N.D.	0.540 #
10)	B gamma-Chl...	0.000	8.226	0	38859	N.D.	0.019 #
15)	B Endosulfa...	0.000	9.147f	0	265440	N.D.	0.155 #
18)	B Endrin al...	0.000	9.293f	0	165408	N.D.	0.133 #
19)	B Endosulfa...	0.000	9.522f	0	139480	N.D.	0.089 #
20)	A Methoxychlor	0.000	9.827f	0	141601	N.D.	0.171 #
21)	B Endrin ke...	0.000	9.978f	0	44272	N.D.	0.027 #
25)	Chlordane-3	0.000	8.226	0	38859	N.D.	0.140 #
27)	Chlordane-5	0.000	9.175f	0	20637	N.D.	0.338 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 18:15
Operator : AR\AJ
Sample : N1099-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:40:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

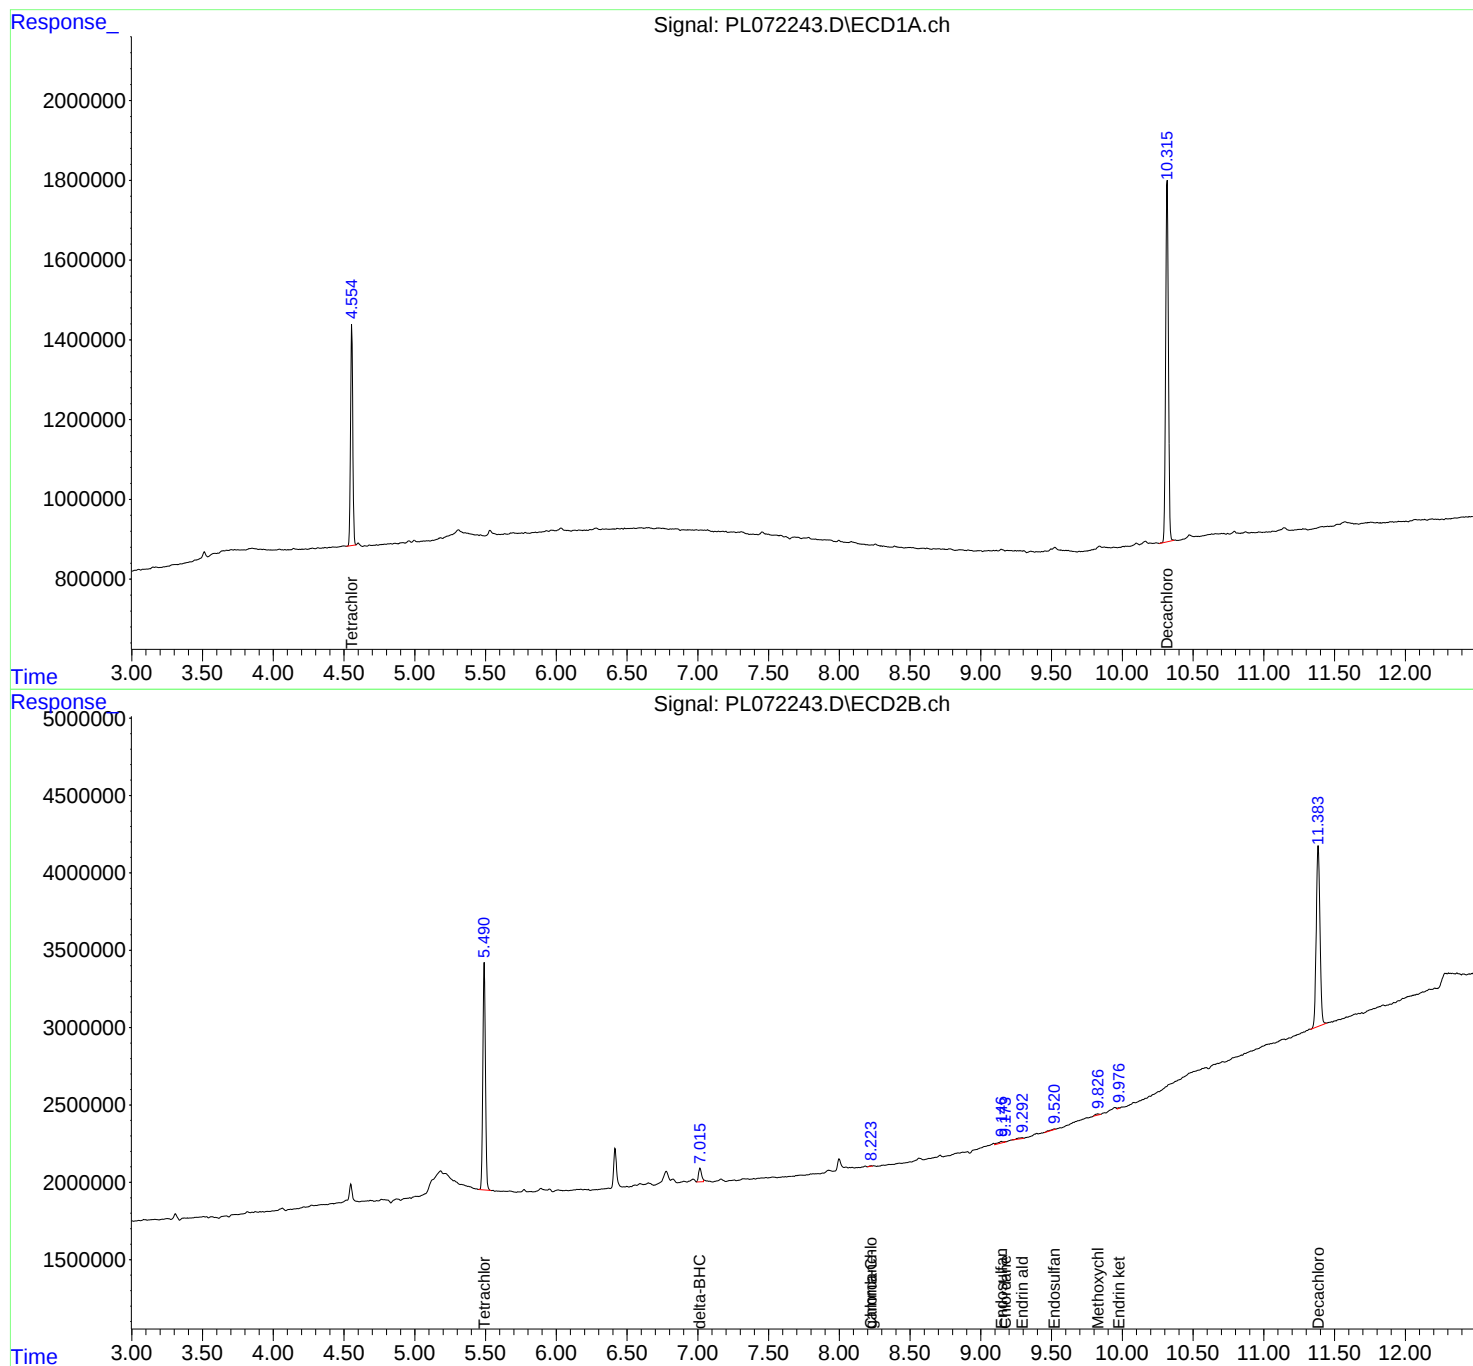


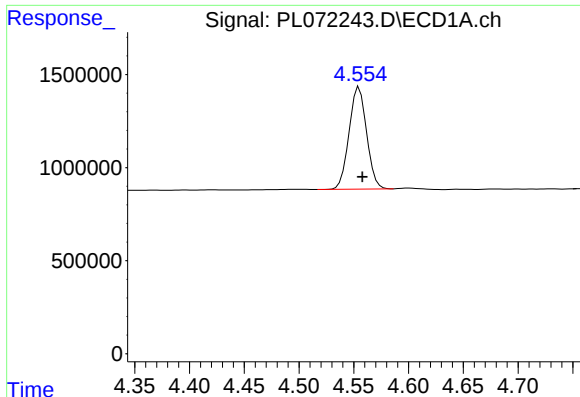

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 6122518
Conc: 11.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

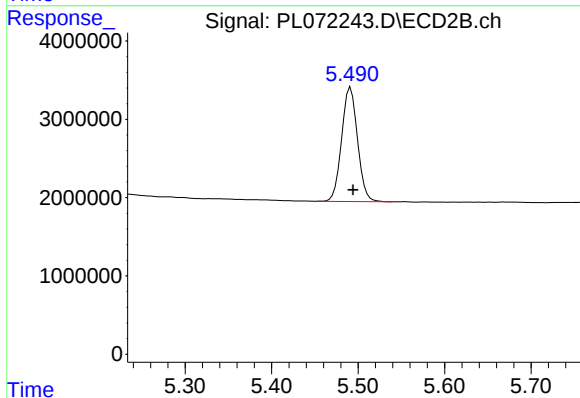


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 18456713
Conc: 11.36 ng/ml

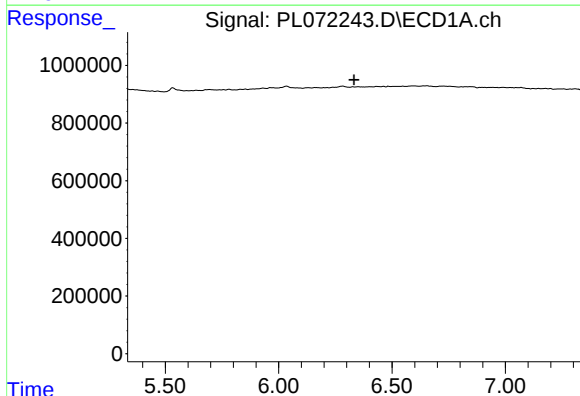


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

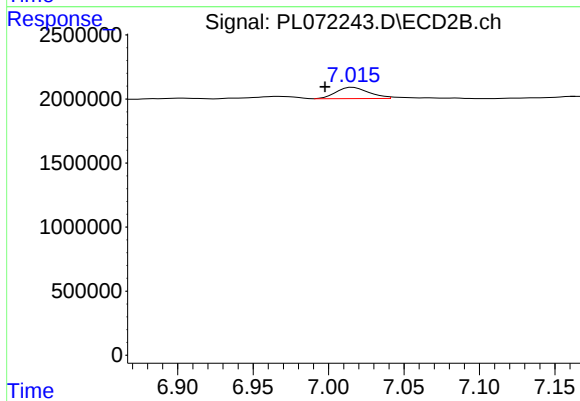

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.019 min
Response: 1329299
Conc: 0.54 ng/ml

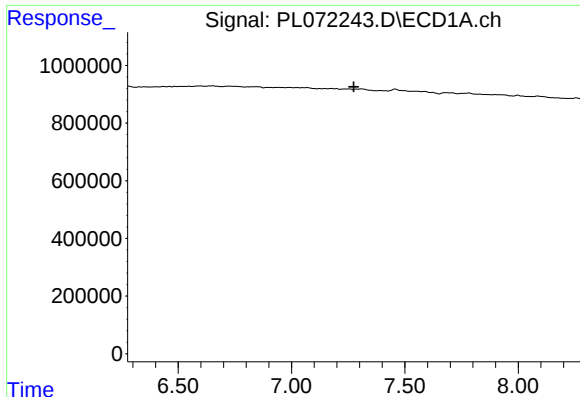

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

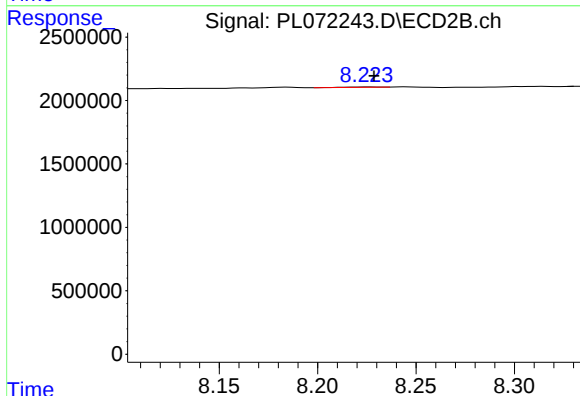


#10 gamma-Chlordane

R.T.: 8.226 min
Delta R.T.: -0.002 min
Response: 38859
Conc: 0.02 ng/ml

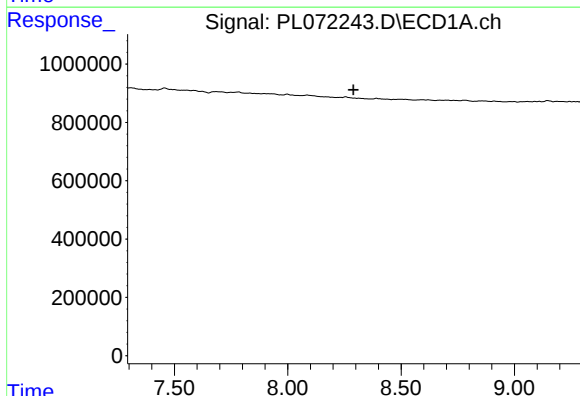


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

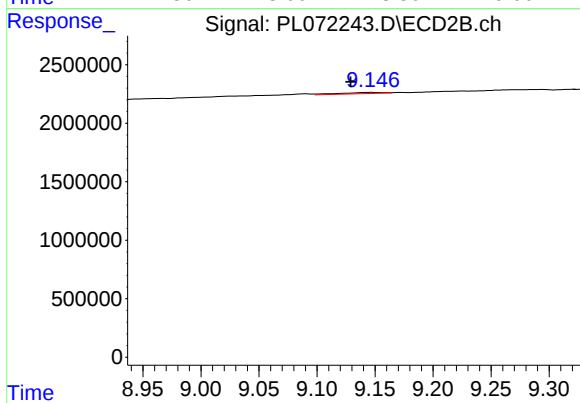

#15 Endosulfan II


R.T.: 9.147 min
Delta R.T.: 0.018 min
Response: 265440
Conc: 0.15 ng/ml

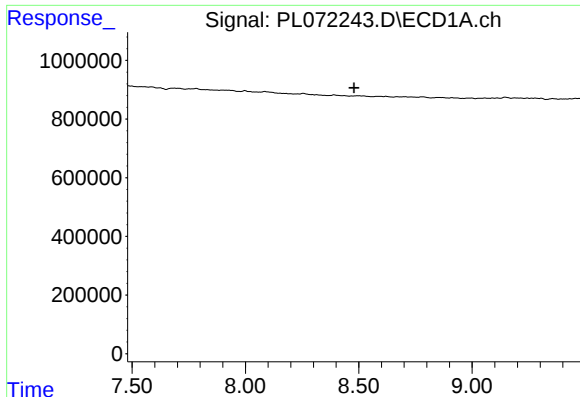

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

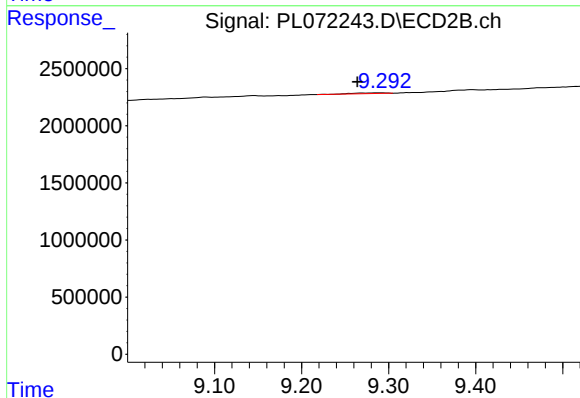


#18 Endrin aldehyde

R.T.: 9.293 min
Delta R.T.: 0.029 min
Response: 165408
Conc: 0.13 ng/ml

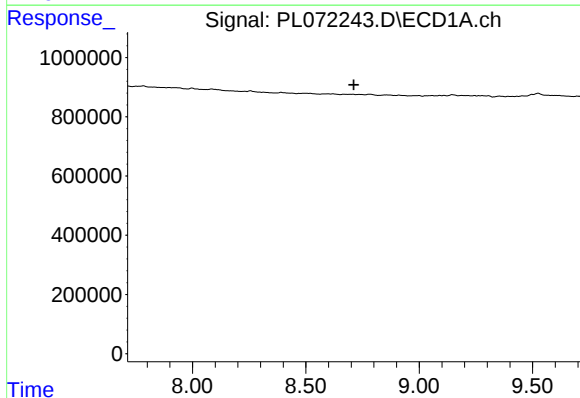


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

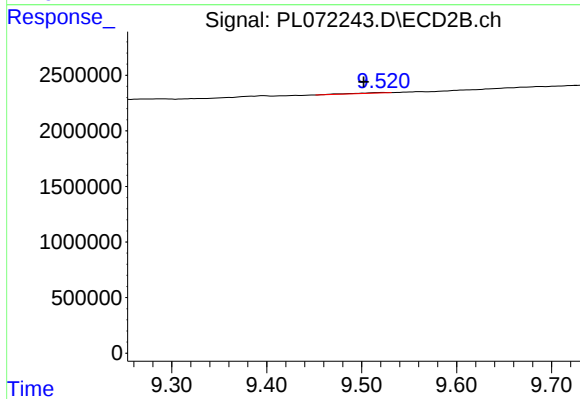

#19 Endosulfan Sulfate


R.T.: 9.522 min
Delta R.T.: 0.020 min
Response: 139480
Conc: 0.09 ng/ml

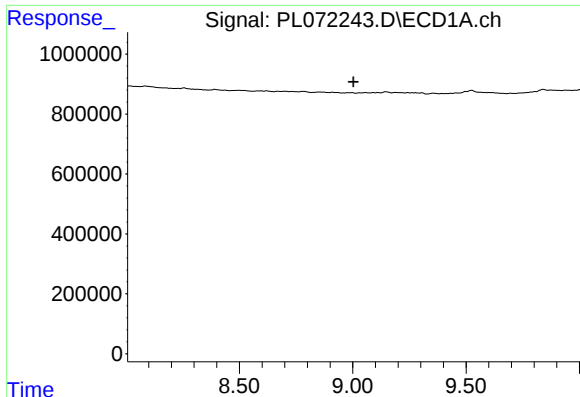

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

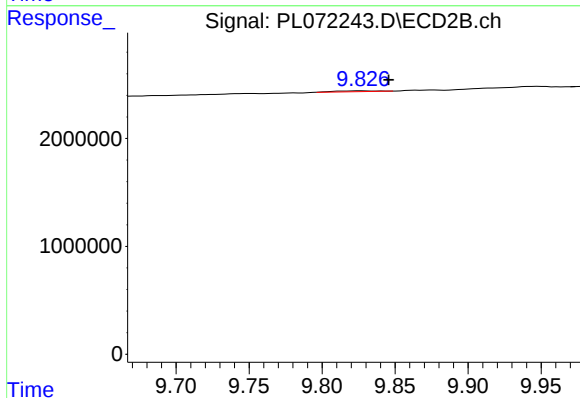


#20 Methoxychlor

R.T.: 9.827 min
Delta R.T.: -0.018 min
Response: 141601
Conc: 0.17 ng/ml

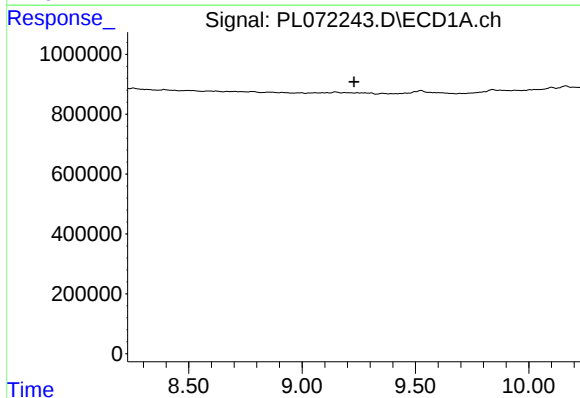


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

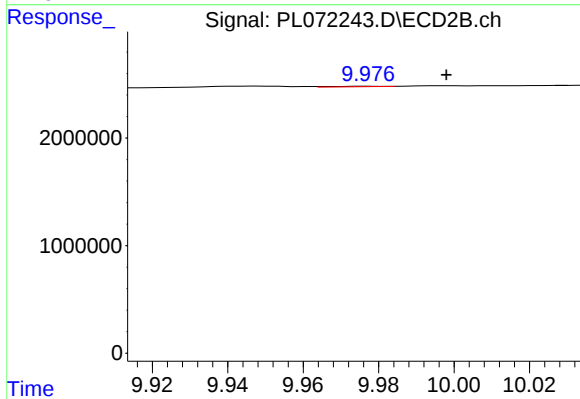

#21 Endrin ketone


R.T.: 9.978 min
Delta R.T.: -0.020 min
Response: 44272
Conc: 0.03 ng/ml

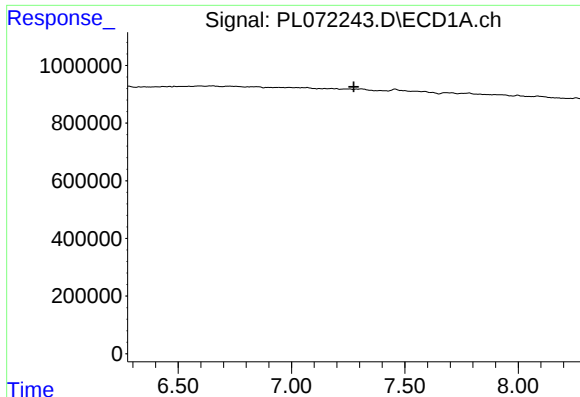

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

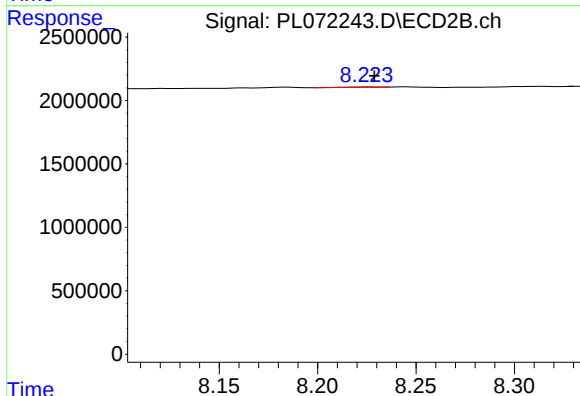


#25 Chlordane-3

R.T.: 8.226 min
Delta R.T.: -0.003 min
Response: 38859
Conc: 0.14 ng/ml

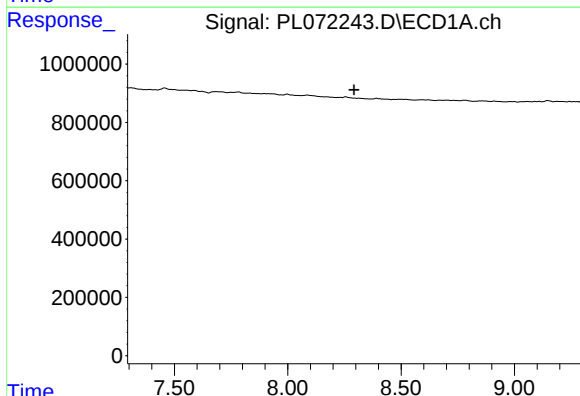


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

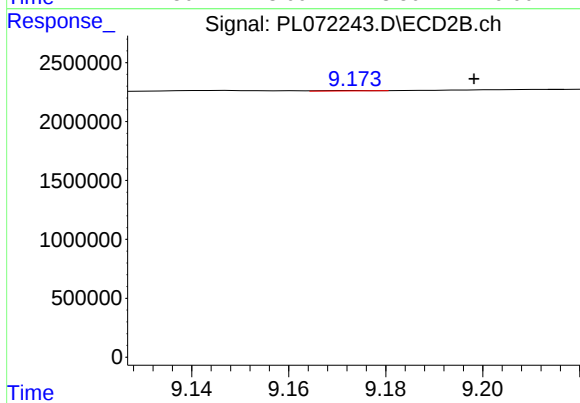

#27 Chlordane-5


R.T.: 9.175 min
Delta R.T.: -0.024 min
Response: 20637
Conc: 0.34 ng/ml

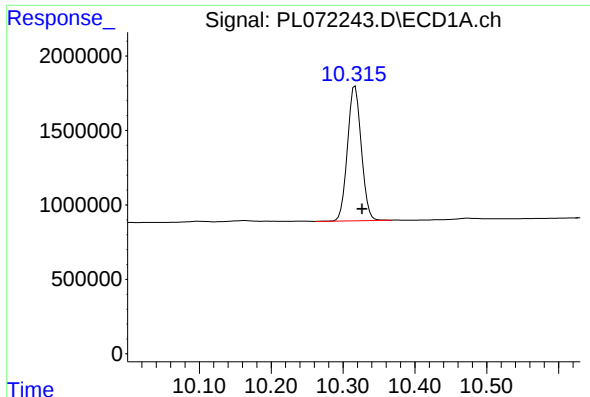

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 12054408
Conc: 13.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-10

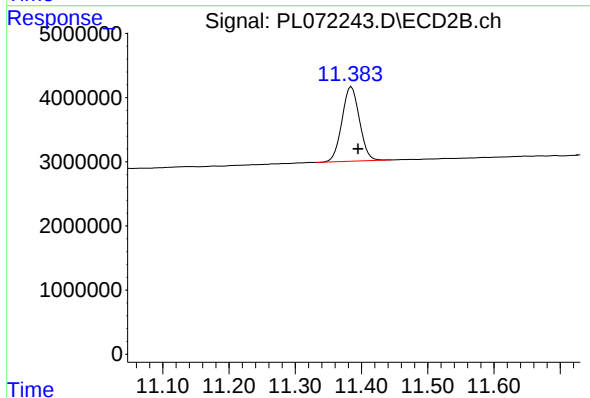

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 21338920
Conc: 13.23 ng/ml