

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 18:48
 Operator : AR\AJ
 Sample : PB142255BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB142255BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:41:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	10170862	30426977	18.320	18.734
28)	SA Decachlor...	10.317	11.385	17259748	29903244	19.427	18.533
Target Compounds							
3)	MA gamma-BHC...	0.000	6.494f	0	98523	N.D.	0.044 #
7)	B delta-BHC	0.000	7.014f	0	6263331	N.D.	2.546 #
9)	A Endosulfan I	0.000	8.342f	0	1058578	N.D.	0.585 #
11)	B alpha-Chl...	0.000	8.309	0	558748	N.D.	0.282 #
14)	MA Endrin	0.000	8.907	0	272477	N.D.	0.164 #
15)	B Endosulfa...	0.000	9.141	0	151545	N.D.	0.088 #
16)	A 4,4'-DDD	0.000	9.038	0	11991960	N.D.	8.387 #
17)	MA 4,4'-DDT	0.000	9.386f	0	43991	N.D.	0.028 #
22)	Mirex	9.395f	0.000	19601	0	0.027	N.D. #
26)	Chlordane-4	0.000	8.309	0	558748	N.D.	1.683 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 18:48
Operator : AR\AJ
Sample : PB142255BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB142255BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:41:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

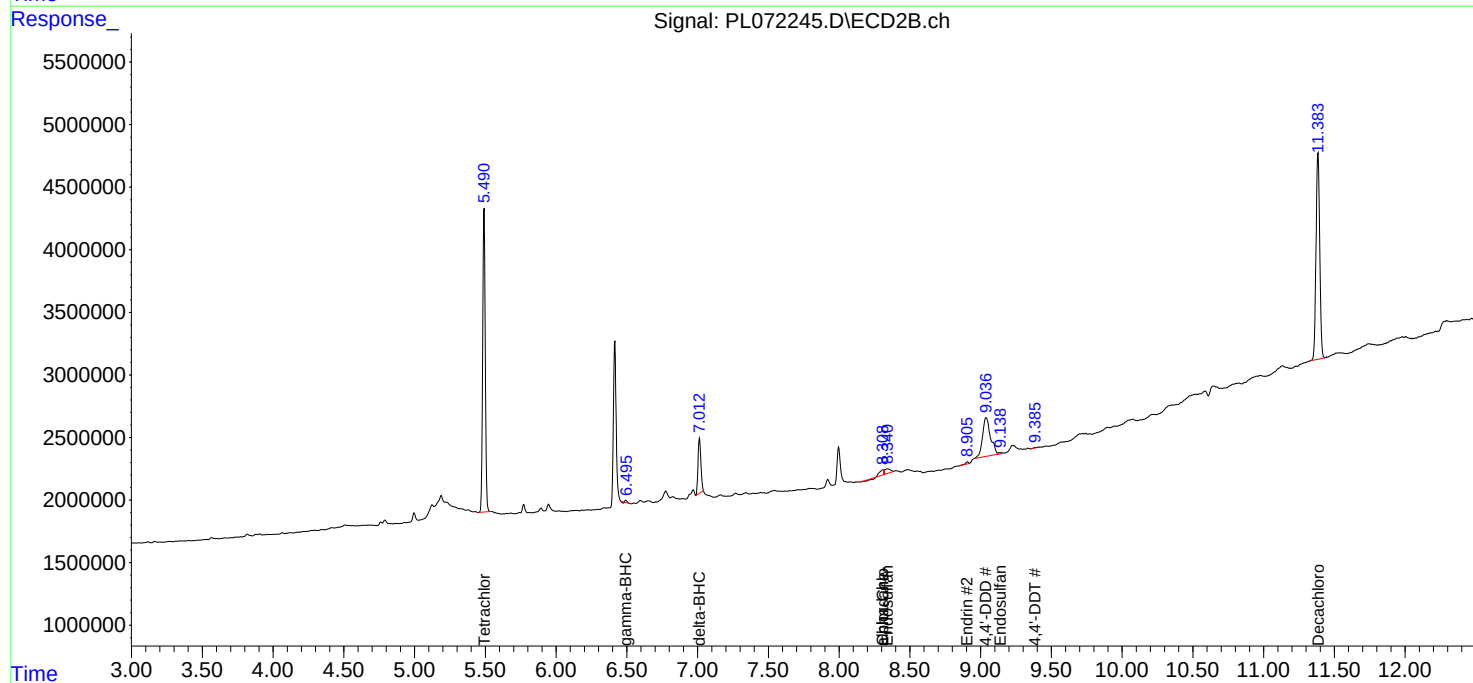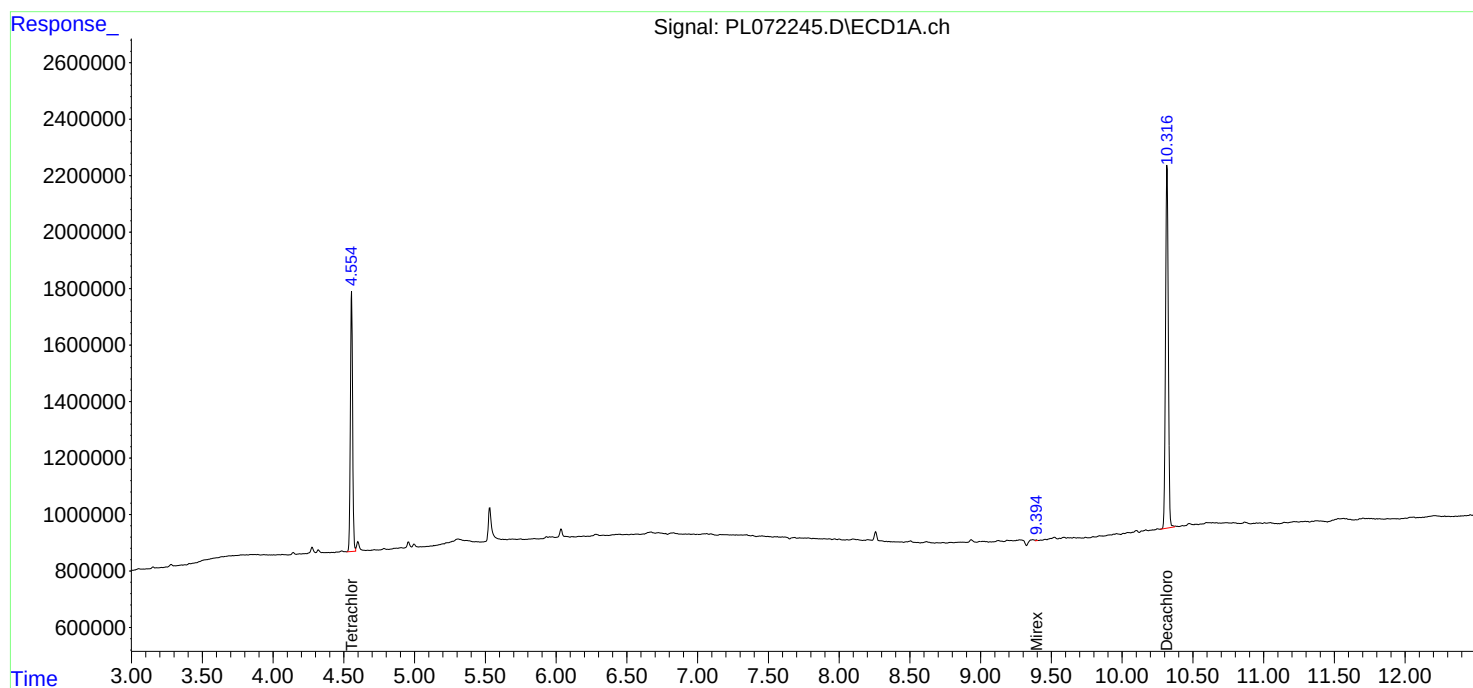


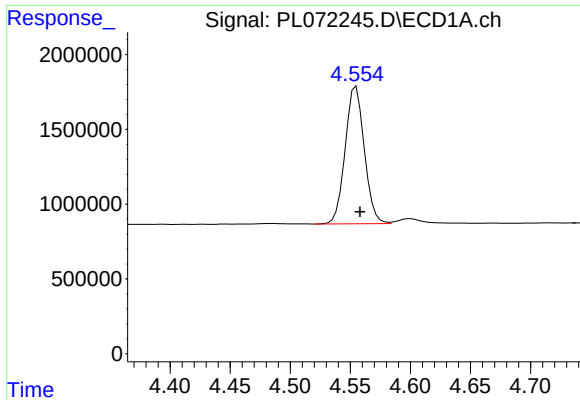

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 10170862
Conc: 18.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB142255BL

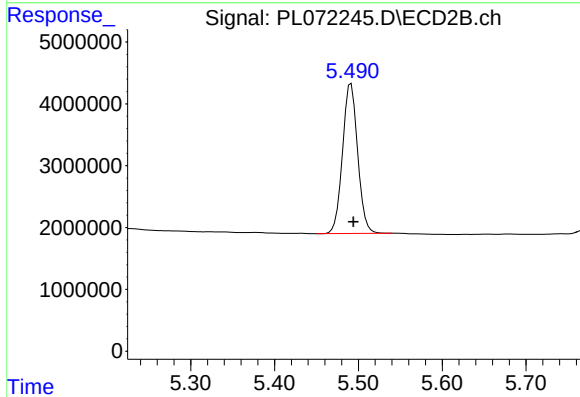


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 30426977
Conc: 18.73 ng/ml

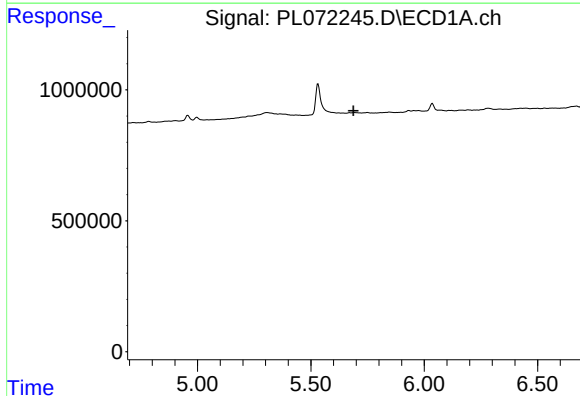


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

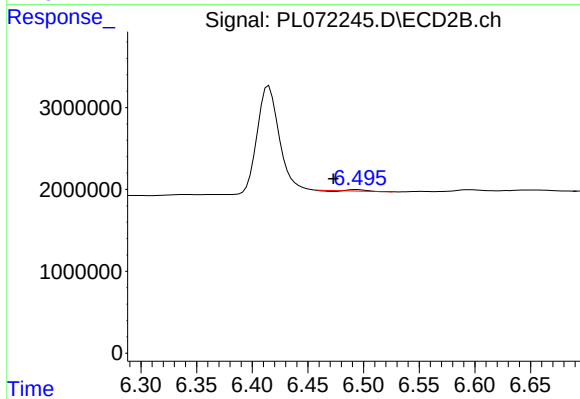

#3 gamma-BHC (Lindane)


R.T.: 6.494 min
Delta R.T.: 0.021 min
Response: 98523
Conc: 0.04 ng/ml

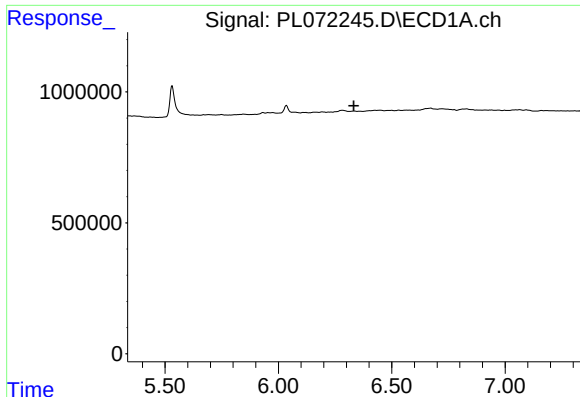

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142255BL

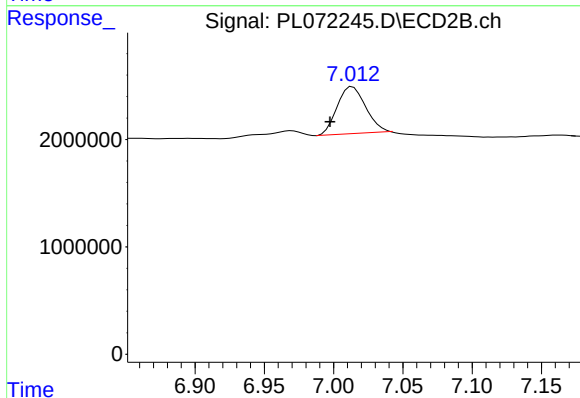


#7 delta-BHC

R.T.: 7.014 min
Delta R.T.: 0.016 min
Response: 6263331
Conc: 2.55 ng/ml

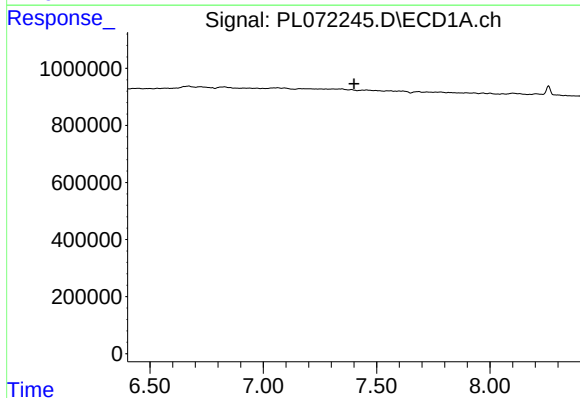


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

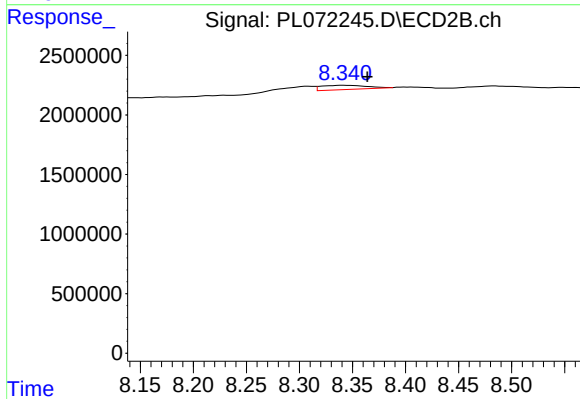

#9 Endosulfan I


R.T.: 8.342 min
Delta R.T.: -0.022 min
Response: 1058578
Conc: 0.58 ng/ml

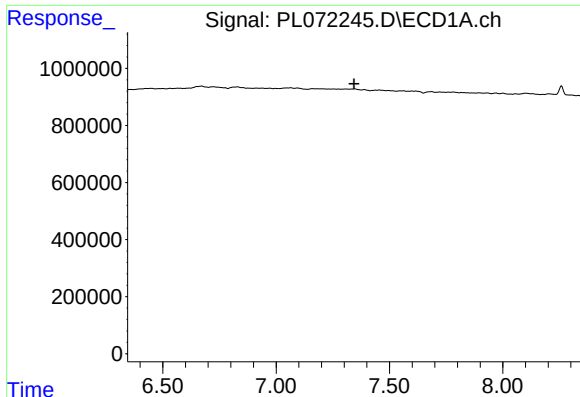

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142255BL

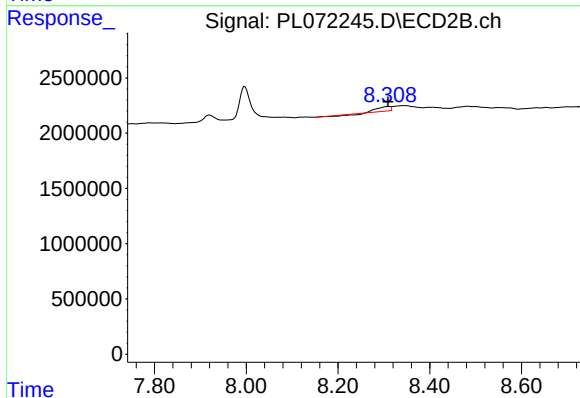


#11 alpha-Chlordane

R.T.: 8.309 min
Delta R.T.: 0.000 min
Response: 558748
Conc: 0.28 ng/ml

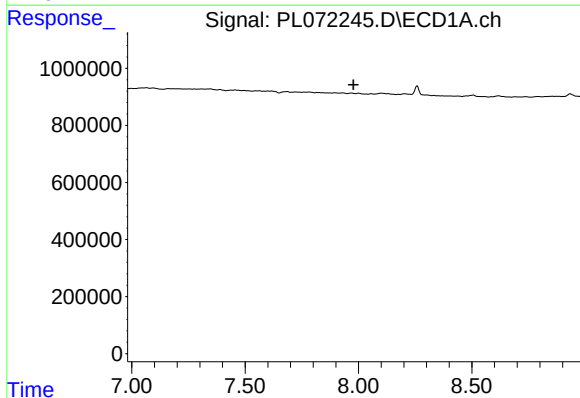


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.978 min
Response: 0
Conc: N.D.

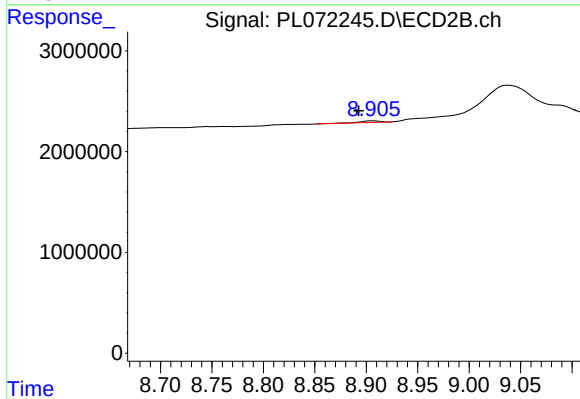

#14 Endrin


R.T.: 8.907 min
Delta R.T.: 0.014 min
Response: 272477
Conc: 0.16 ng/ml

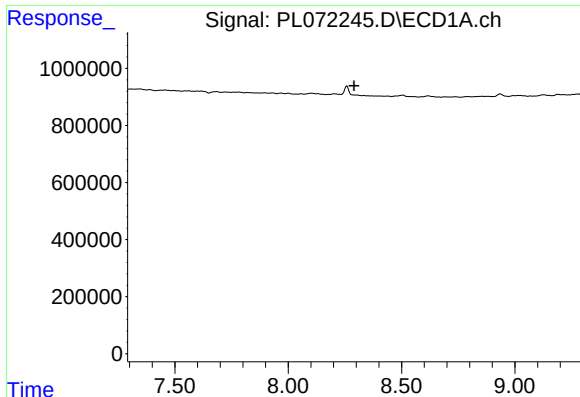

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142255BL

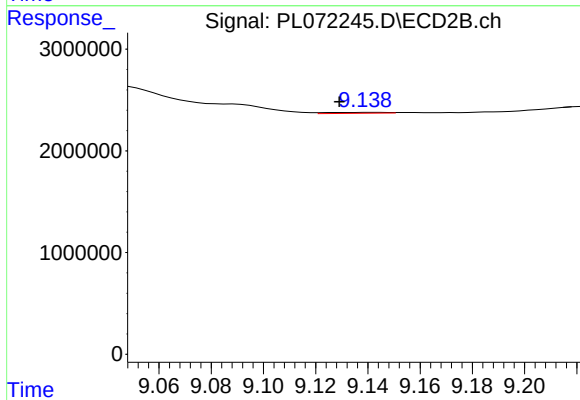


#15 Endosulfan II

R.T.: 9.141 min
Delta R.T.: 0.012 min
Response: 151545
Conc: 0.09 ng/ml

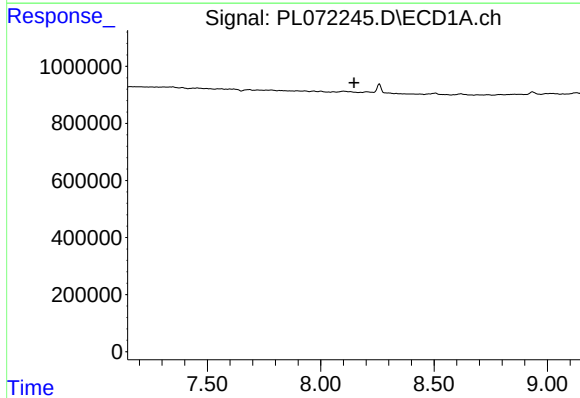


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

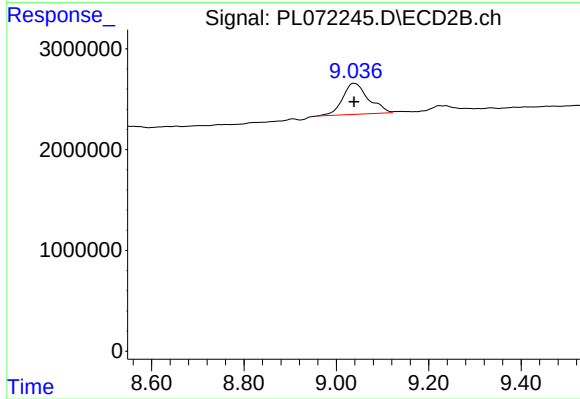

#16 4,4'-DDD


R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 11991960
Conc: 8.39 ng/ml

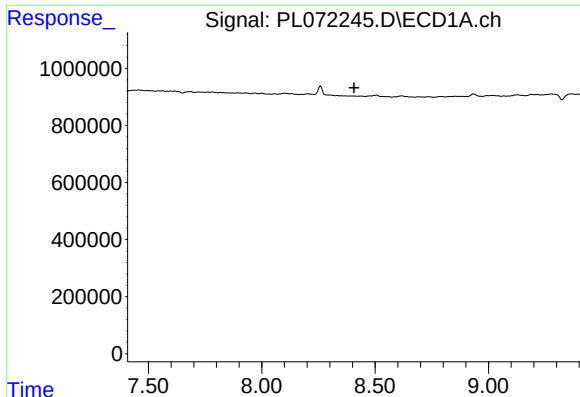

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142255BL

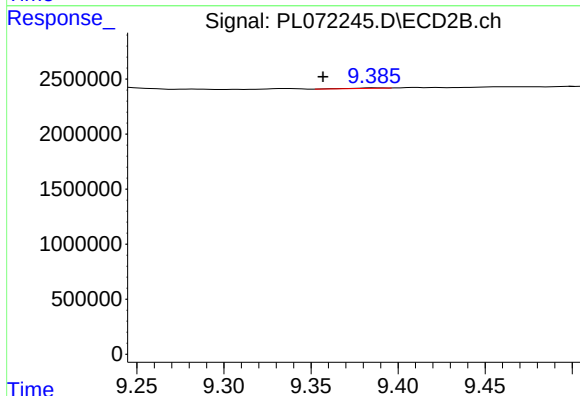


#17 4,4'-DDT

R.T.: 9.386 min
Delta R.T.: 0.029 min
Response: 43991
Conc: 0.03 ng/ml

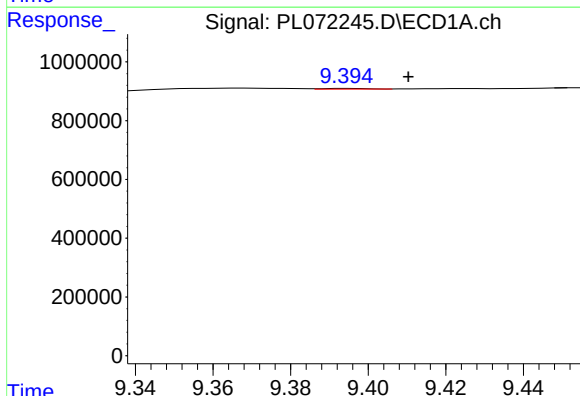


#22 Mirex

R.T.: 9.395 min
Delta R.T.: -0.015 min
Response: 19601
Conc: 0.03 ng/ml

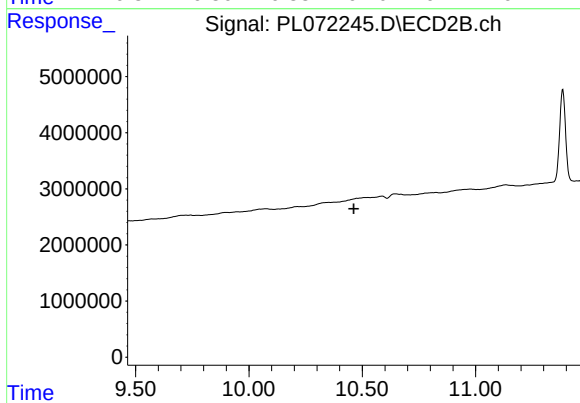

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 10.463 min
Response: 0
Conc: N.D.

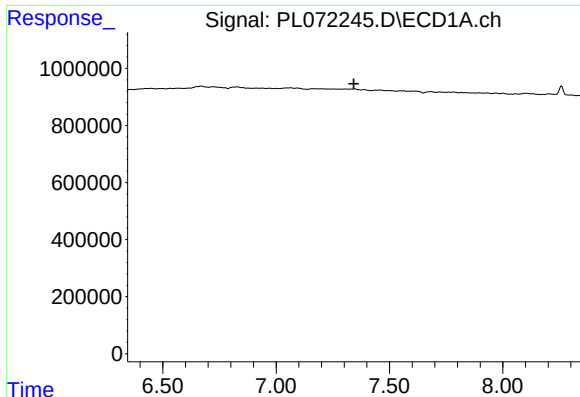

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142255BL

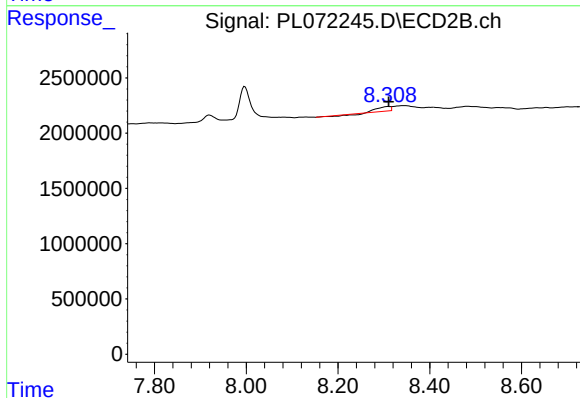


#26 Chlordane-4

R.T.: 8.309 min
Delta R.T.: -0.001 min
Response: 558748
Conc: 1.68 ng/ml

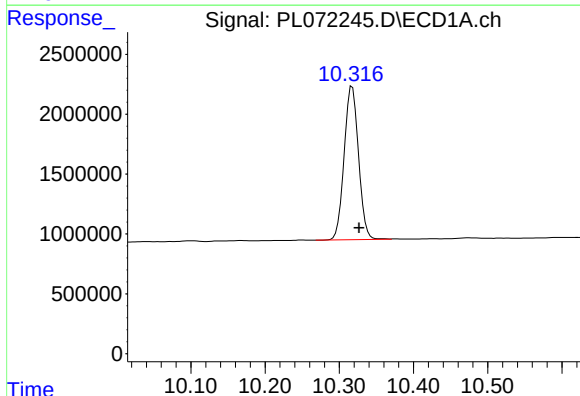

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.009 min
Response: 17259748
Conc: 19.43 ng/ml

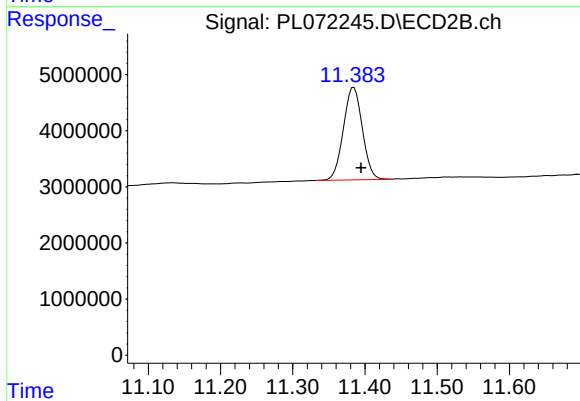

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 29903244
Conc: 18.53 ng/ml