

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 19:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:41:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	10225489	30101375	18.418	18.534
28)	SA Decachlor...	10.318	11.385	17218067	30519822	19.380	18.915
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	1152329	N.D.	0.468 #
8)	B Heptachlo...	0.000	7.962	0	213599	N.D.	0.107 #
9)	A Endosulfan I	0.000	8.382f	0	286592	N.D.	0.158 #
10)	B gamma-Chl...	0.000	8.223	0	530660	N.D.	0.263 #
15)	B Endosulfa...	0.000	9.143	0	312707	N.D.	0.182 #
20)	A Methoxychlor	0.000	9.850	0	131276	N.D.	0.158 #
21)	B Endrin ke...	0.000	10.004	0	126888	N.D.	0.077 #
25)	Chlordane-3	0.000	8.223	0	530660	N.D.	1.910 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 19:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:41:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

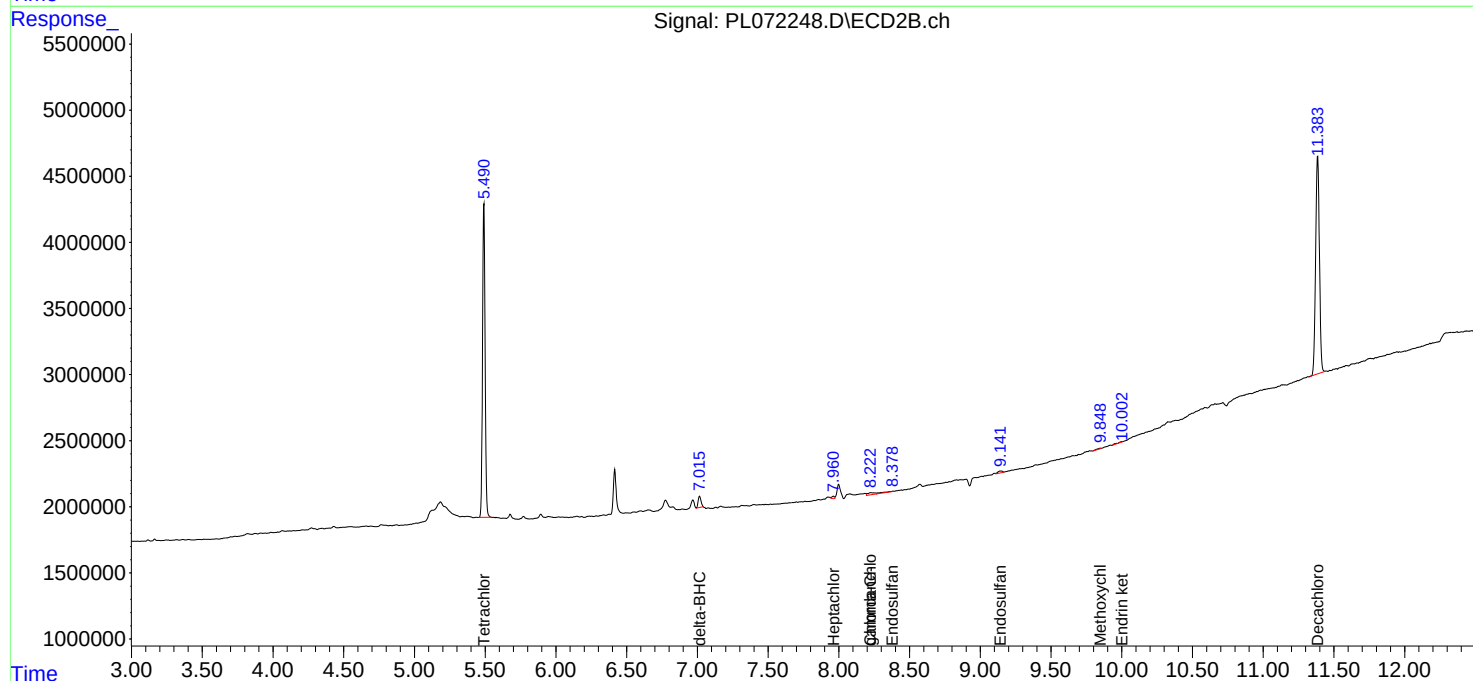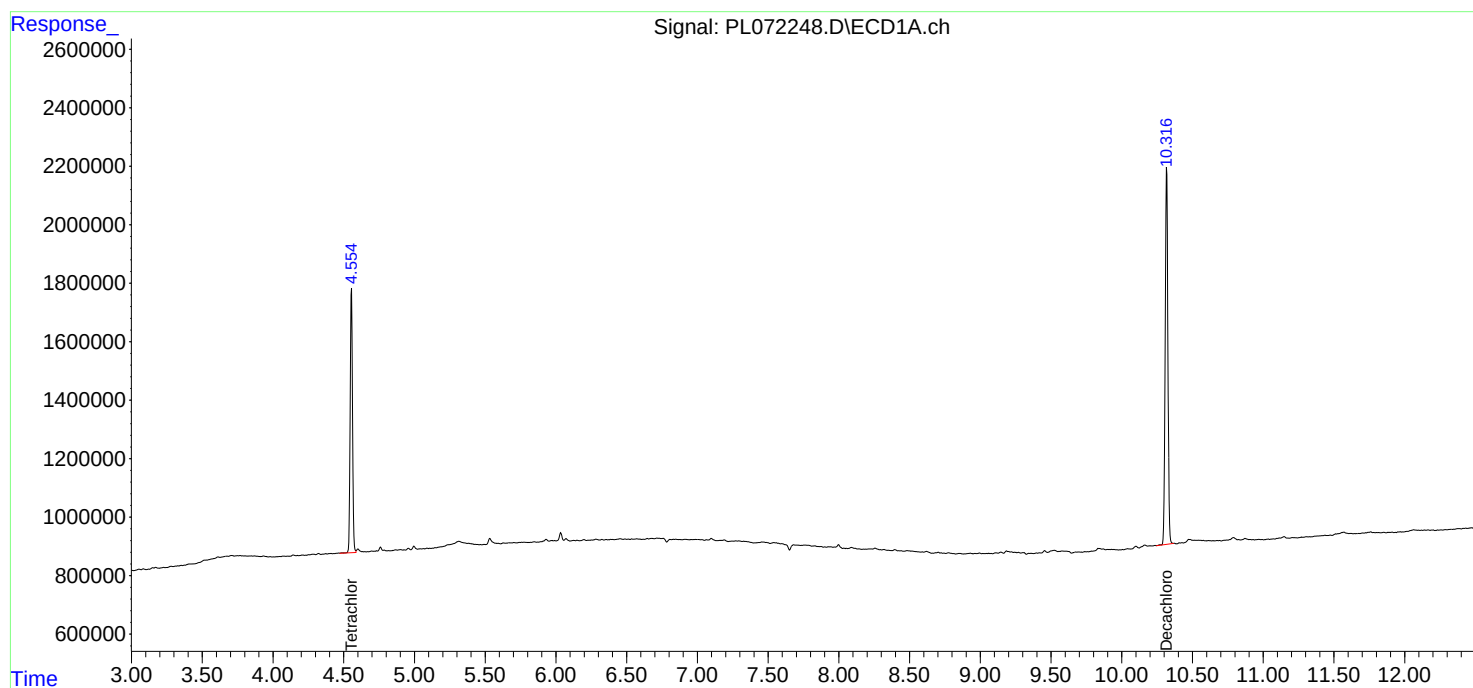


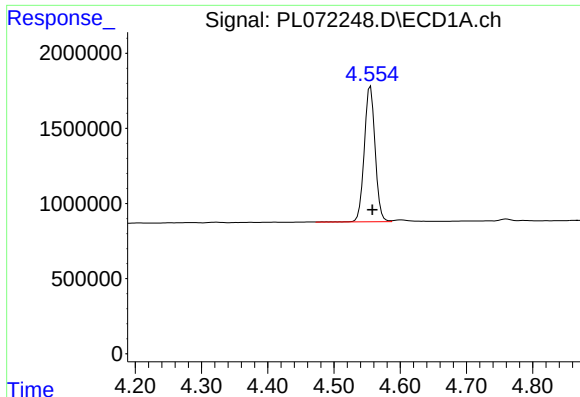

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 10225489
Conc: 18.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

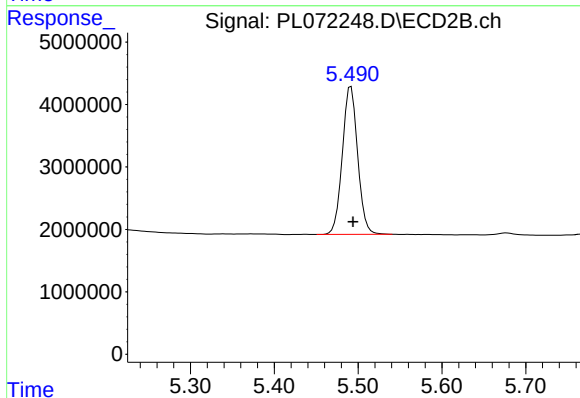


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 30101375
Conc: 18.53 ng/ml

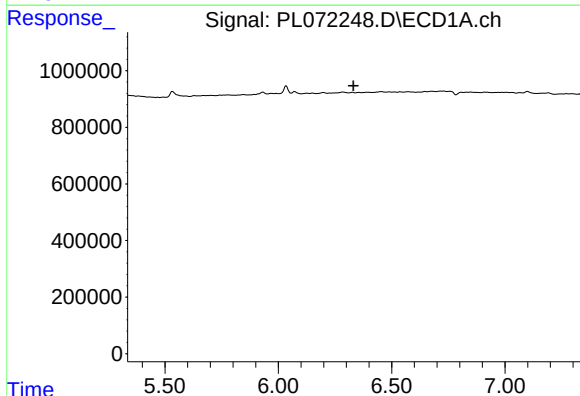


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

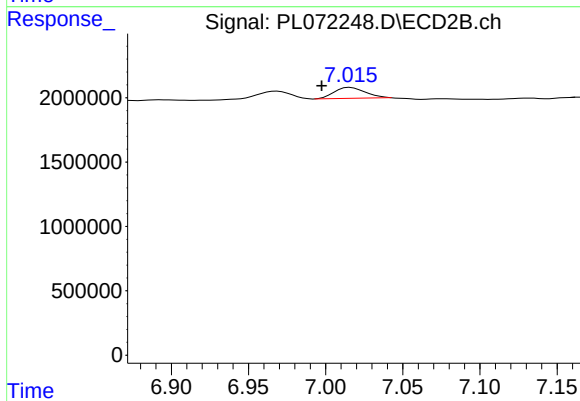

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.018 min
Response: 1152329
Conc: 0.47 ng/ml

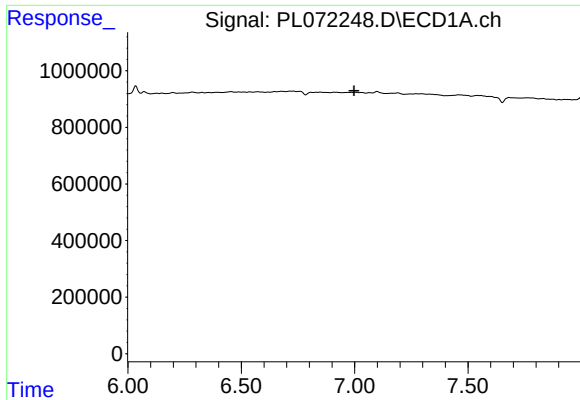

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

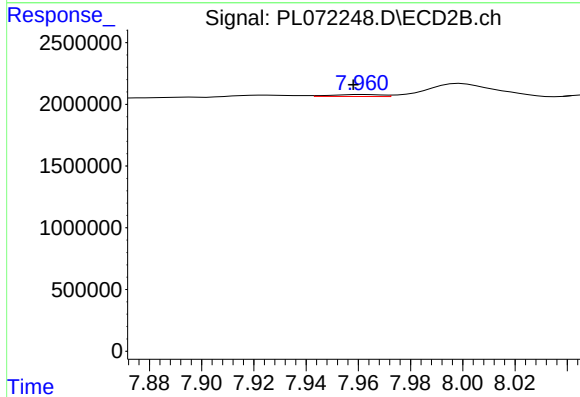


#8 Heptachlor epoxide

R.T.: 7.962 min
Delta R.T.: 0.004 min
Response: 213599
Conc: 0.11 ng/ml

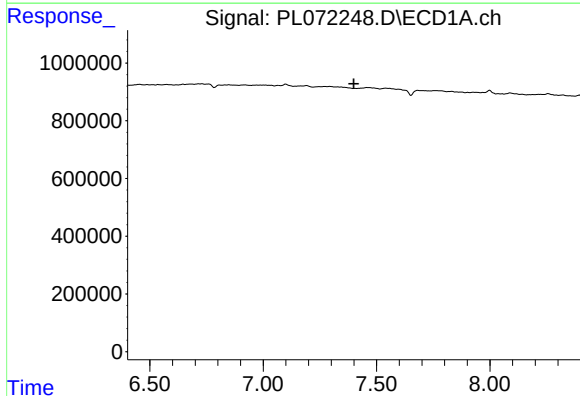


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

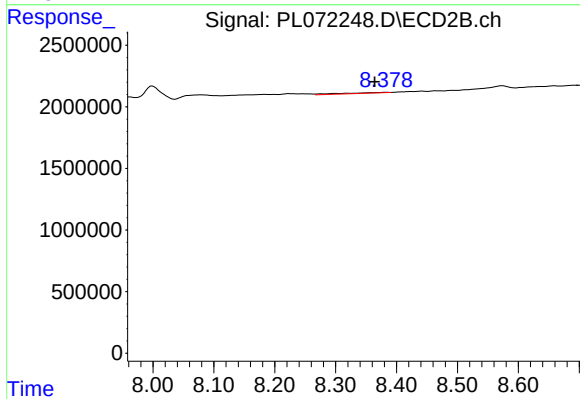

#9 Endosulfan I


R.T.: 8.382 min
Delta R.T.: 0.018 min
Response: 286592
Conc: 0.16 ng/ml

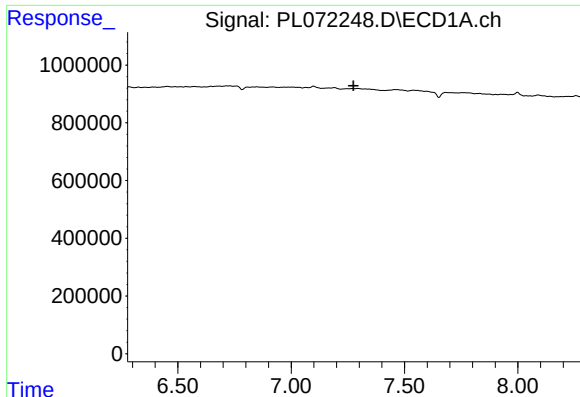

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

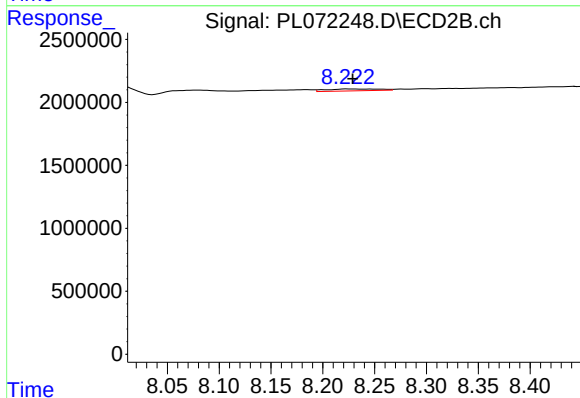


#10 gamma-Chlordane

R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 530660
Conc: 0.26 ng/ml

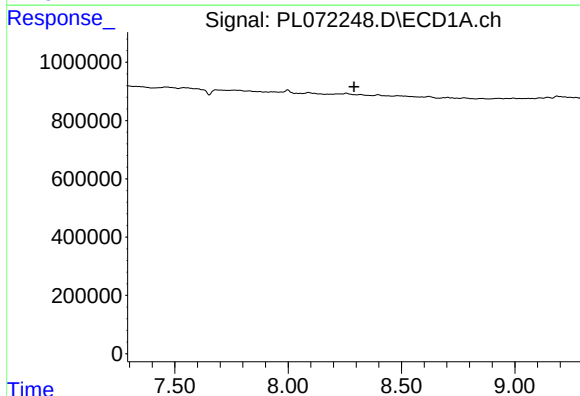


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

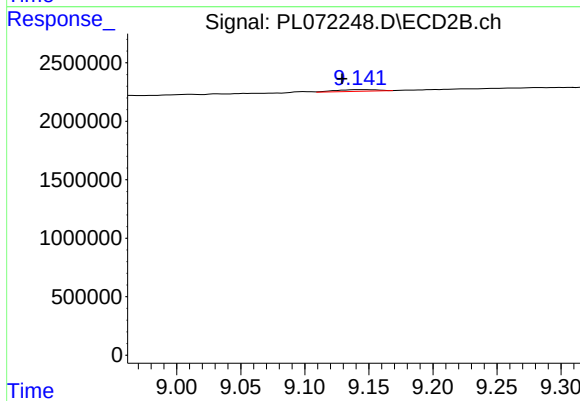

#15 Endosulfan II


R.T.: 9.143 min
Delta R.T.: 0.014 min
Response: 312707
Conc: 0.18 ng/ml

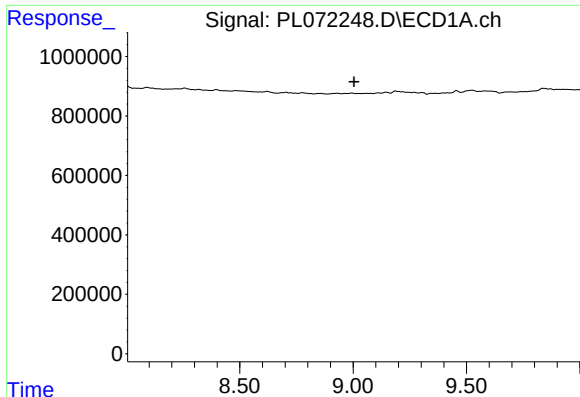

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

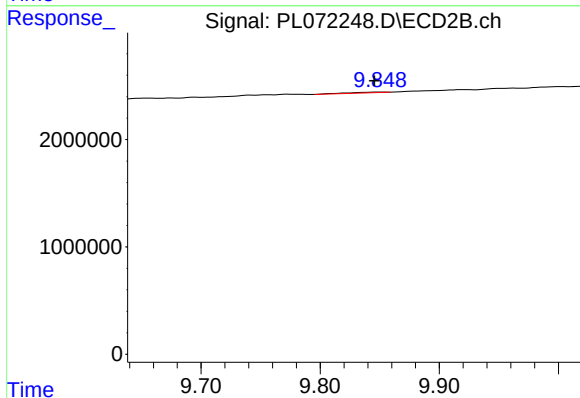


#20 Methoxychlor

R.T.: 9.850 min
Delta R.T.: 0.004 min
Response: 131276
Conc: 0.16 ng/ml

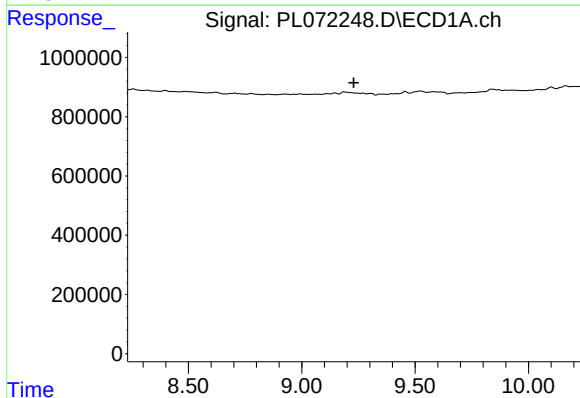


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

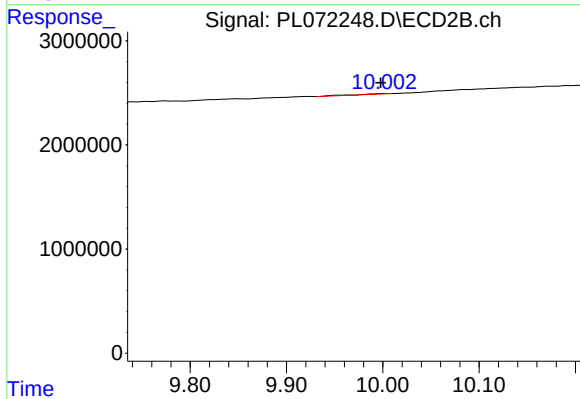

#21 Endrin ketone


R.T.: 10.004 min
Delta R.T.: 0.006 min
Response: 126888
Conc: 0.08 ng/ml

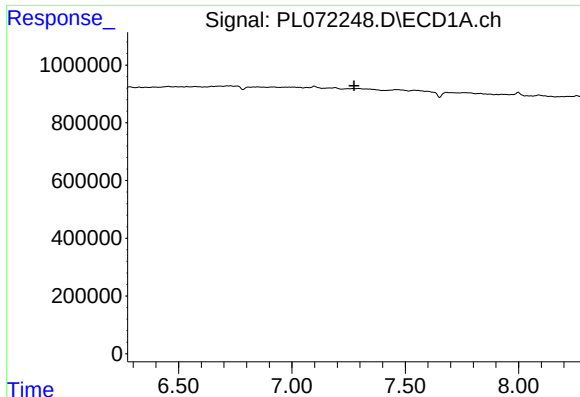

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

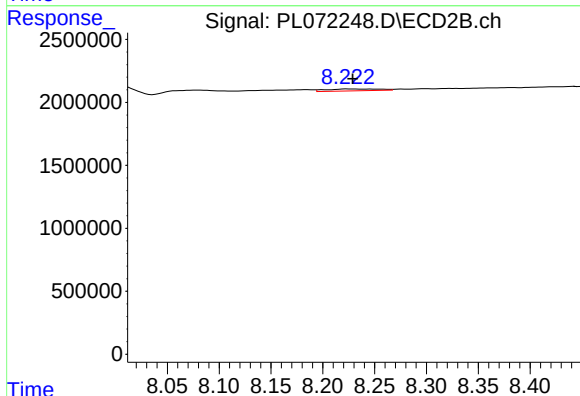


#25 Chlordane-3

R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 530660
Conc: 1.91 ng/ml

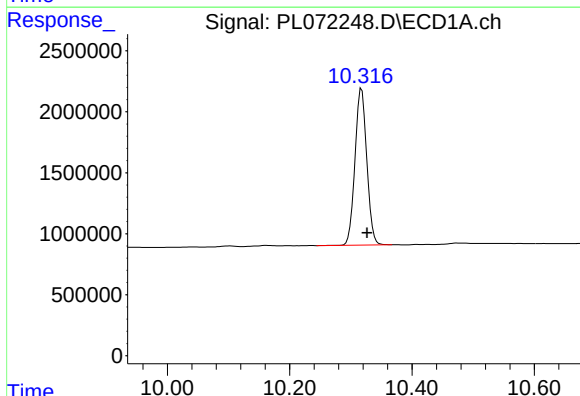

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 17218067
Conc: 19.38 ng/ml

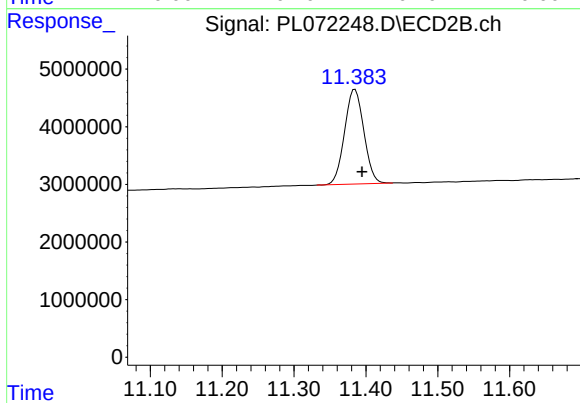

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 30519822
Conc: 18.92 ng/ml