

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 20:58
 Operator : AR\AJ
 Sample : PB142250BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB142250BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:42:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.493	9965134	31283842	17.949	19.262
28)	SA Decachlor...	10.318	11.387	17349785	30508333	19.528	18.908
Target Compounds							
7)	B delta-BHC	0.000	7.015f	0	5218974	N.D.	2.121 #
9)	A Endosulfan I	0.000	8.376	0	89933	N.D.	0.050 #
10)	B gamma-Chl...	0.000	8.233	0	267136	N.D.	0.132 #
15)	B Endosulfa...	0.000	9.150f	0	441417	N.D.	0.257 #
18)	B Endrin al...	0.000	9.290f	0	73632	N.D.	0.059 #
21)	B Endrin ke...	0.000	9.992	0	83875	N.D.	0.051 #
25)	Chlordane-3	0.000	8.233	0	267136	N.D.	0.962 #
27)	Chlordane-5	0.000	9.201	0	25478	N.D.	0.418 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 20:58
Operator : AR\AJ
Sample : PB142250BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB142250BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:42:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

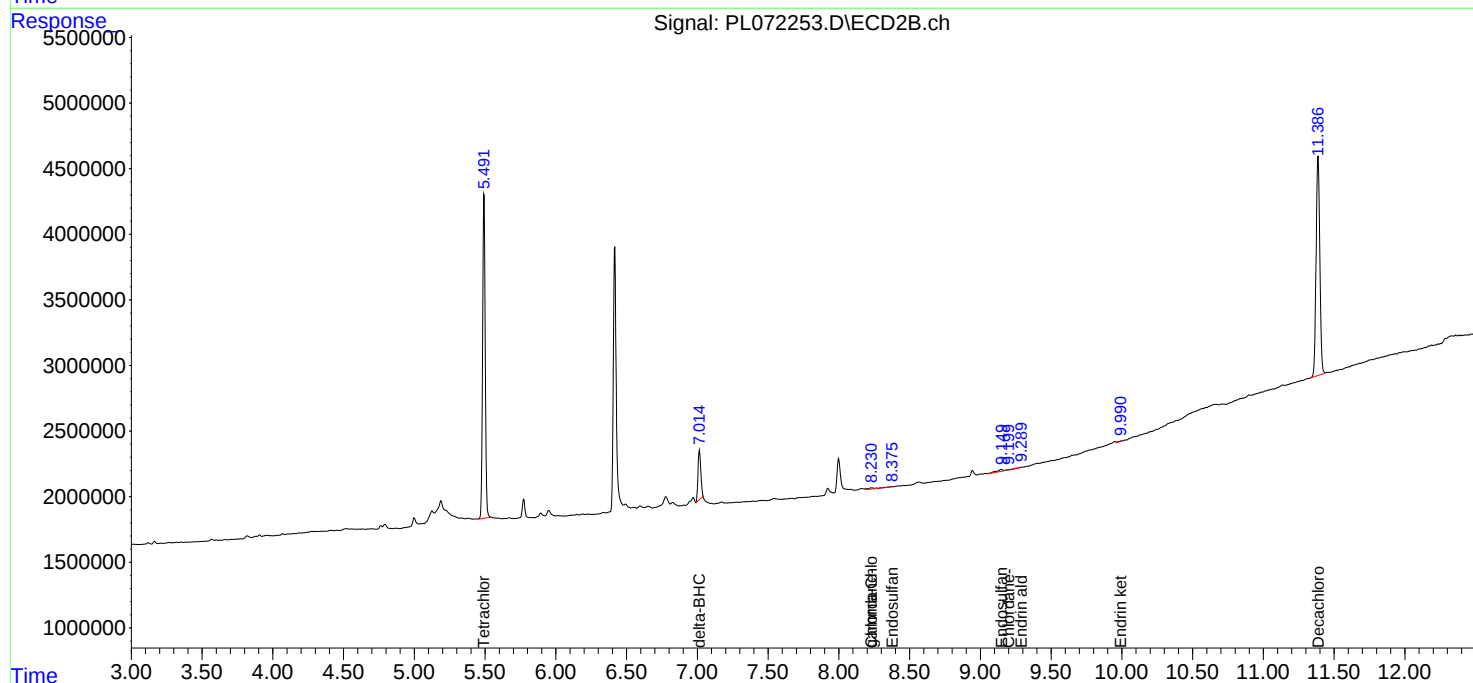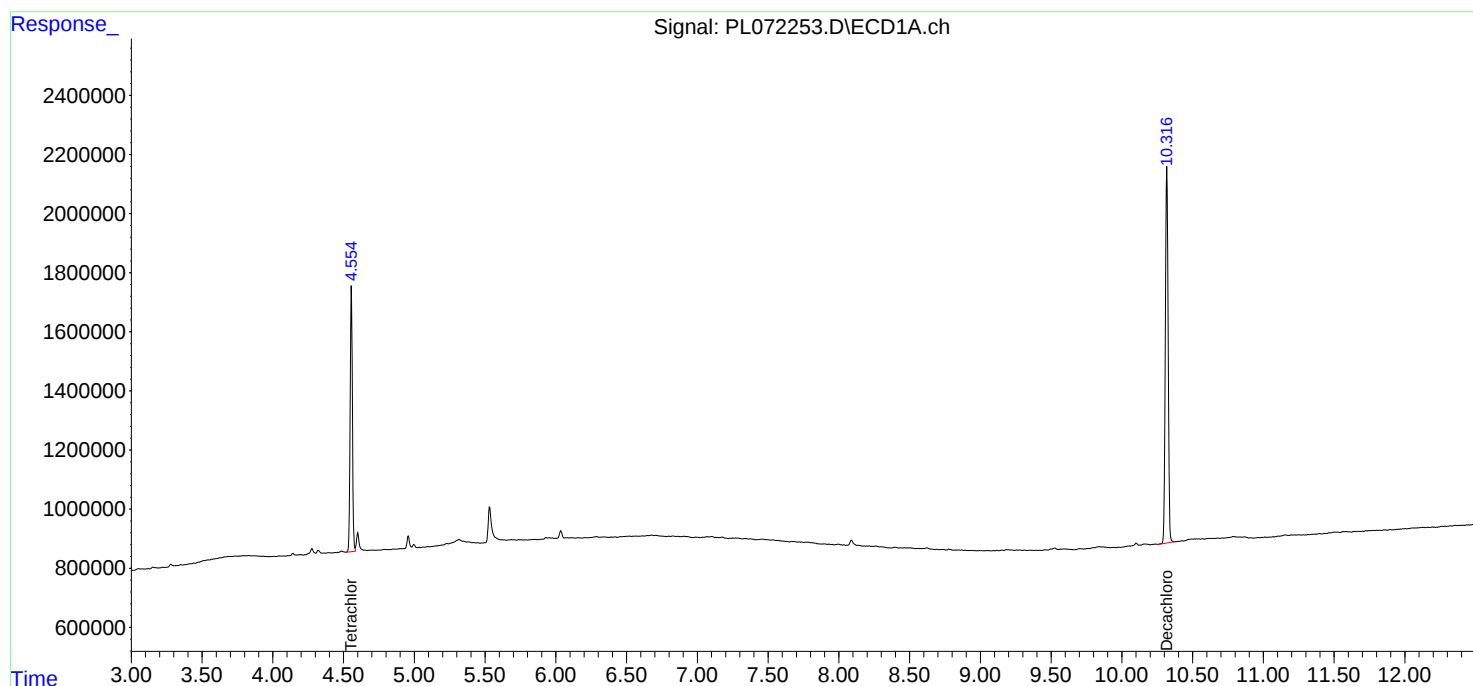


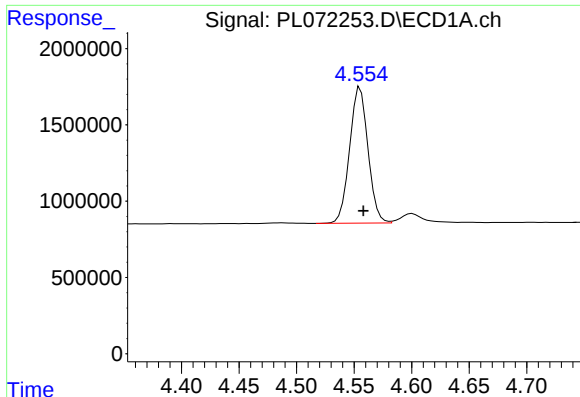

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 9965134
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB142250BL

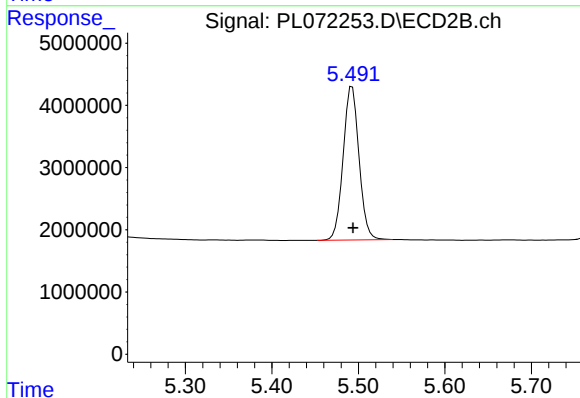


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: -0.001 min
Response: 31283842
Conc: 19.26 ng/ml

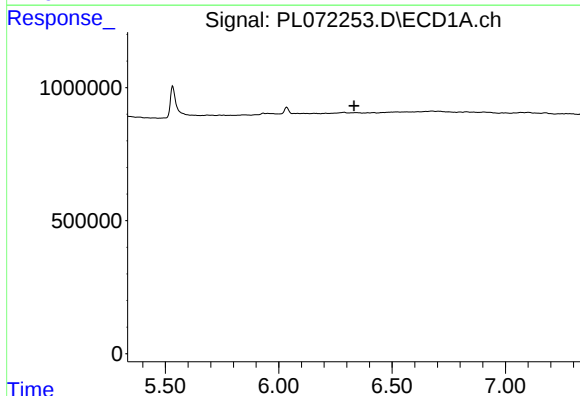


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

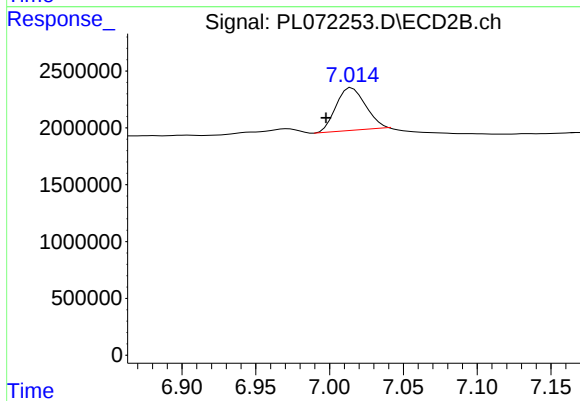

#7 delta-BHC


R.T.: 7.015 min
Delta R.T.: 0.017 min
Response: 5218974
Conc: 2.12 ng/ml

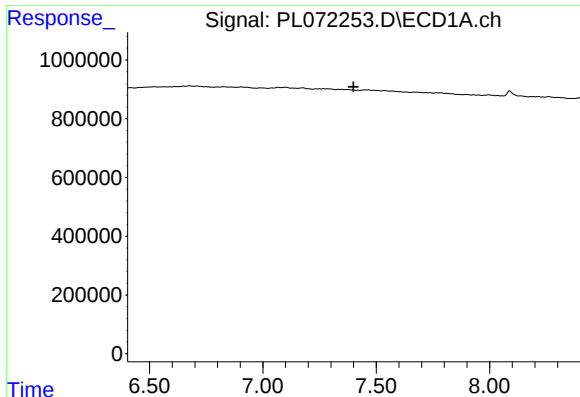

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142250BL

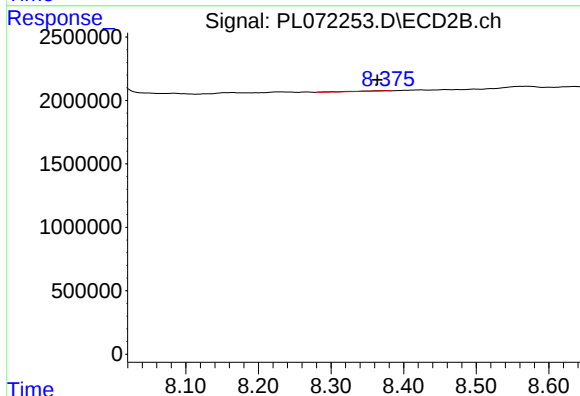


#9 Endosulfan I

R.T.: 8.376 min
Delta R.T.: 0.012 min
Response: 89933
Conc: 0.05 ng/ml

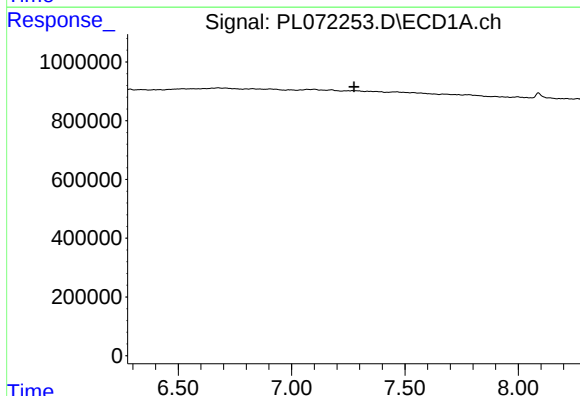


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

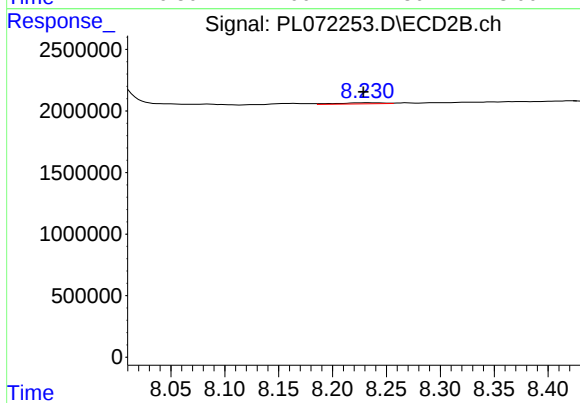

#10 gamma-Chlordane


R.T.: 8.233 min
Delta R.T.: 0.004 min
Response: 267136
Conc: 0.13 ng/ml

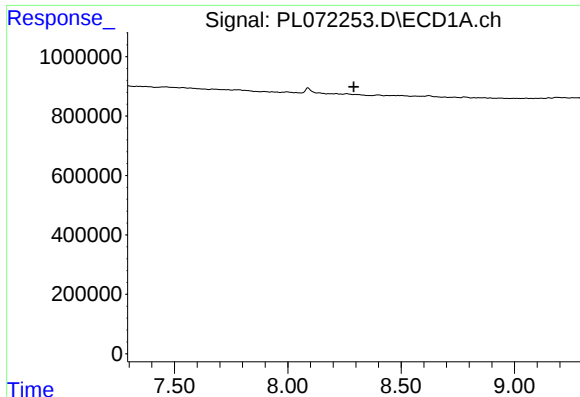

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142250BL

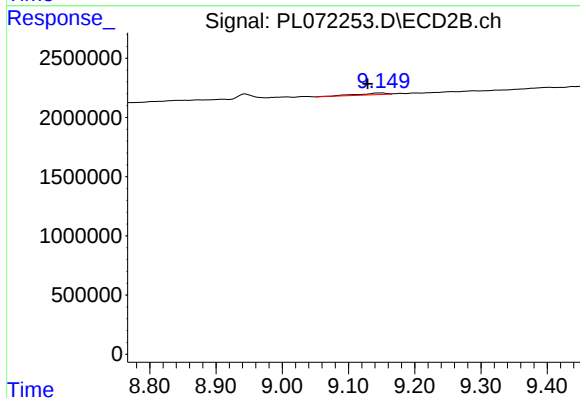


#15 Endosulfan II

R.T.: 9.150 min
Delta R.T.: 0.021 min
Response: 441417
Conc: 0.26 ng/ml

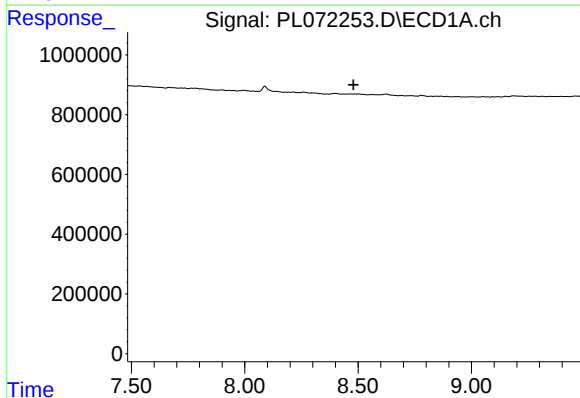


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

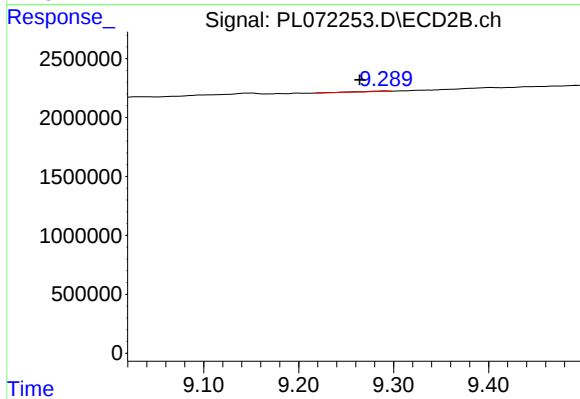

#18 Endrin aldehyde


R.T.: 9.290 min
Delta R.T.: 0.026 min
Response: 73632
Conc: 0.06 ng/ml

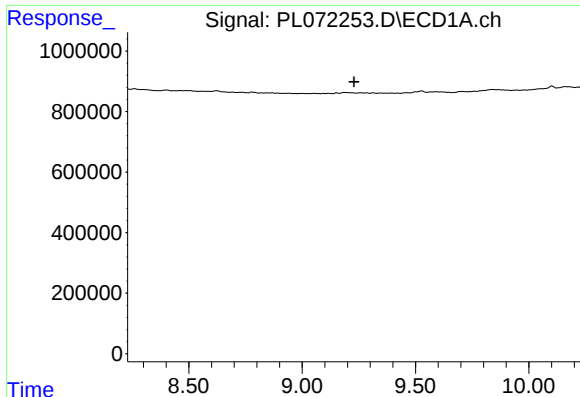

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142250BL

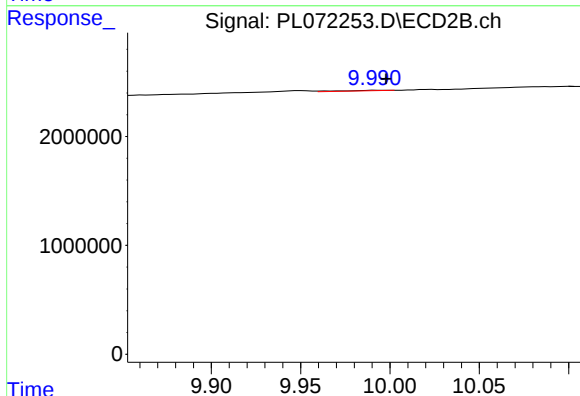


#21 Endrin ketone

R.T.: 9.992 min
Delta R.T.: -0.006 min
Response: 83875
Conc: 0.05 ng/ml

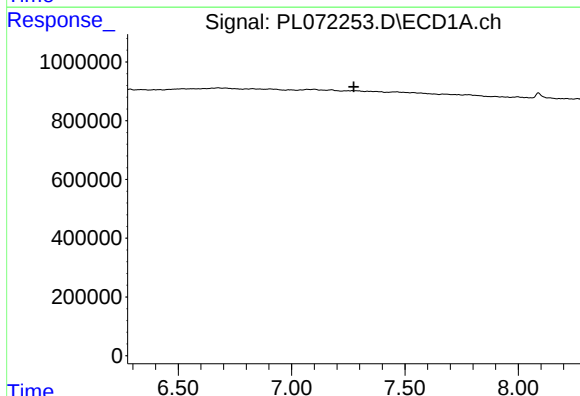


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

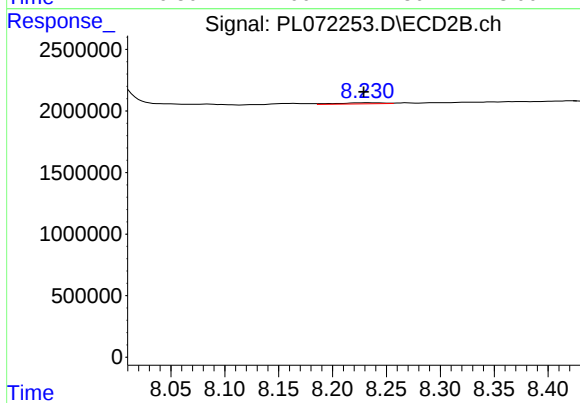

#25 Chlordane-3


R.T.: 8.233 min
Delta R.T.: 0.004 min
Response: 267136
Conc: 0.96 ng/ml

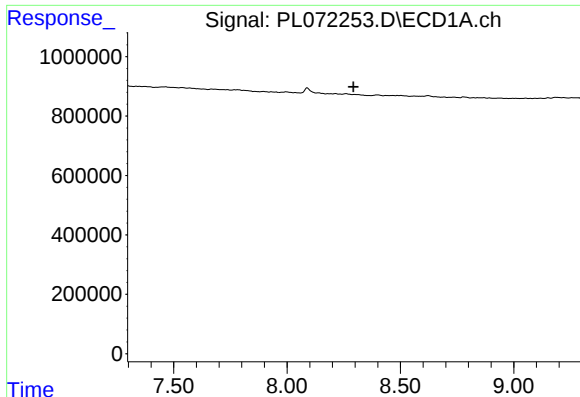

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB142250BL

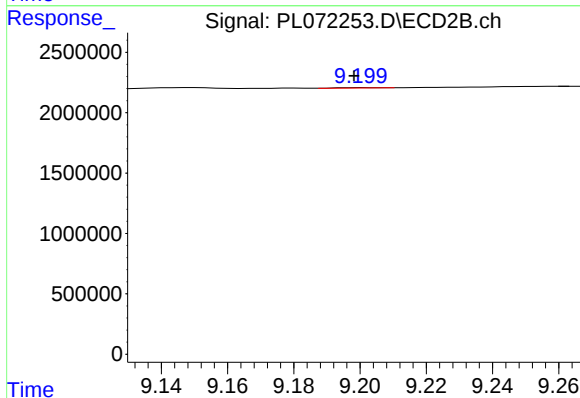


#27 Chlordane-5

R.T.: 9.201 min
Delta R.T.: 0.003 min
Response: 25478
Conc: 0.42 ng/ml

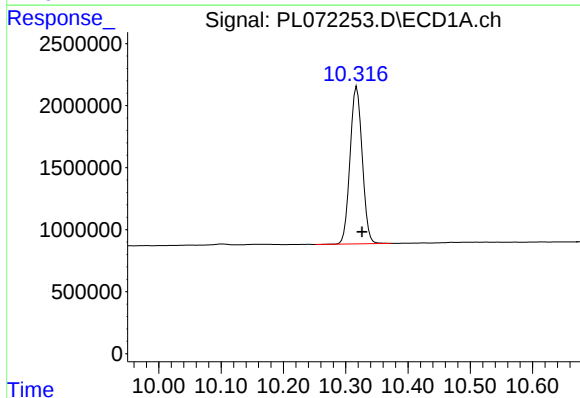

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 17349785
Conc: 19.53 ng/ml

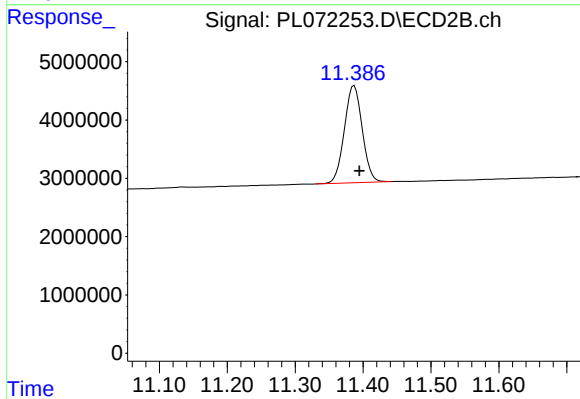

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 30508333
Conc: 18.91 ng/ml