

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 23:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:43:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	10396051	30599757	18.725	18.841
2)	SA Decachlor...	10.318	11.386	16356289	28973021	18.410	17.957
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	977691	N.D.	0.397 #
8)	B Heptachlo...	0.000	7.963	0	589368	N.D.	0.294 #
9)	A Endosulfan I	0.000	8.363	0	284857	N.D.	0.157 #
10)	B gamma-Chl...	0.000	8.232	0	666456	N.D.	0.330 #
11)	B alpha-Chl...	0.000	8.319	0	353112	N.D.	0.178 #
13)	MA Dieldrin	7.682	0.000	117122	0	0.155	N.D. #
14)	MA Endrin	7.999f	0.000	219227	0	0.313	N.D. #
15)	B Endosulfa...	0.000	9.146f	0	1643389	N.D.	0.958 #
16)	A 4,4'-DDD	0.000	9.068f	0	584543	N.D.	0.409 #
21)	B Endrin ke...	0.000	10.007	0	140799	N.D.	0.085 #
25)	Chlordane-3	0.000	8.232	0	666456	N.D.	2.399 #
26)	Chlordane-4	0.000	8.319	0	353112	N.D.	1.063 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 23:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:43:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

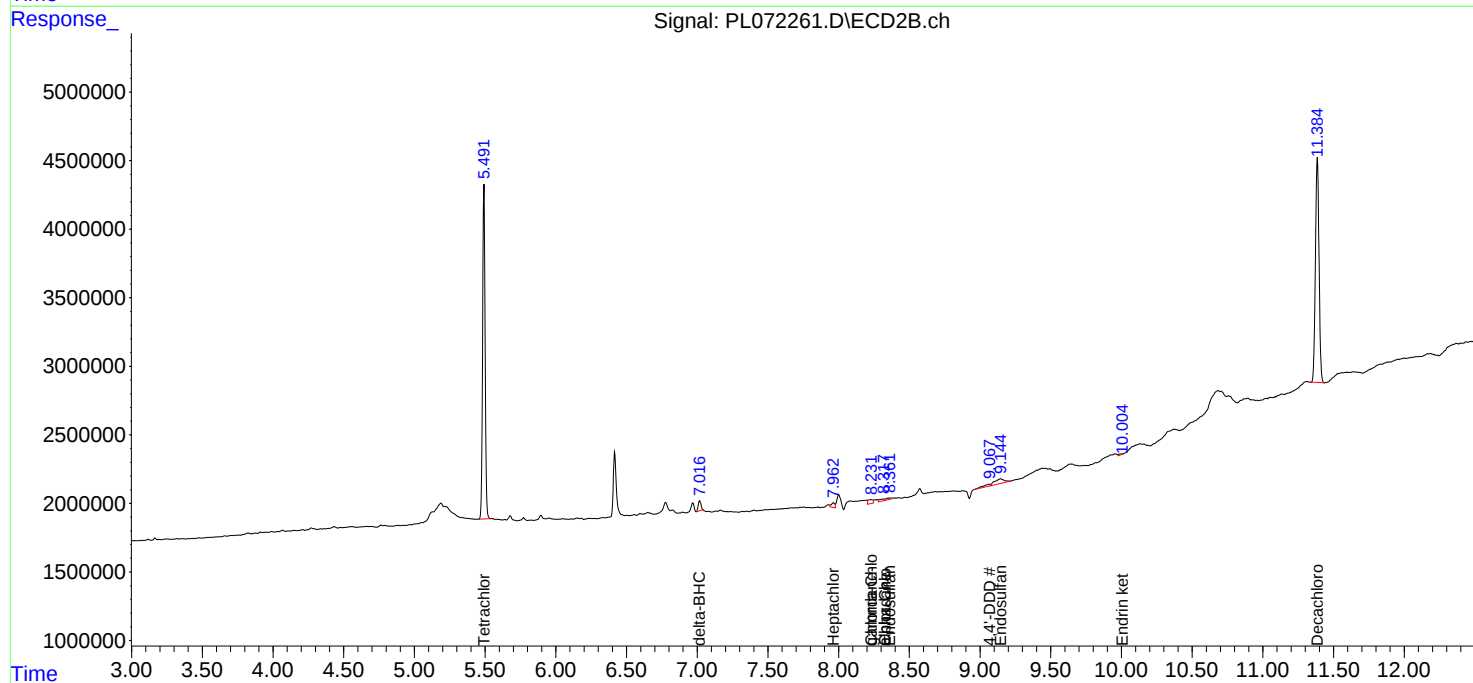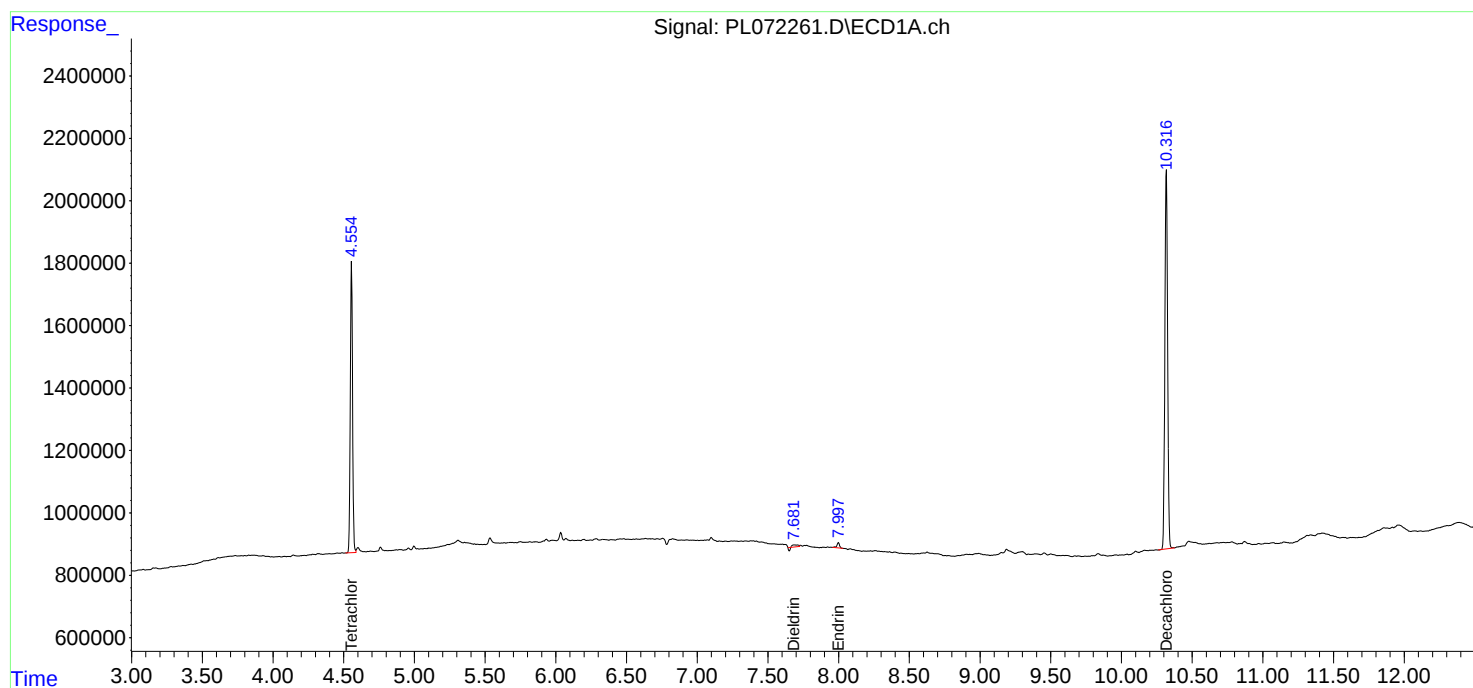


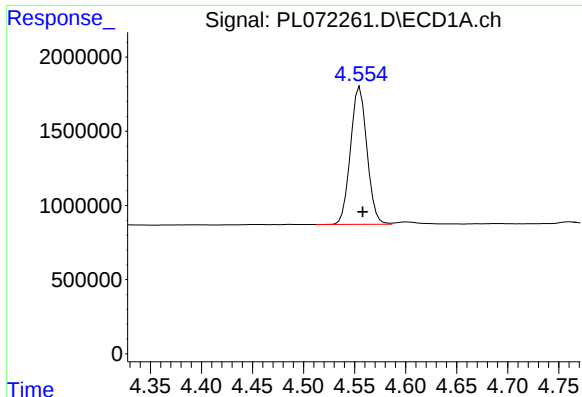

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 10396051
Conc: 18.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

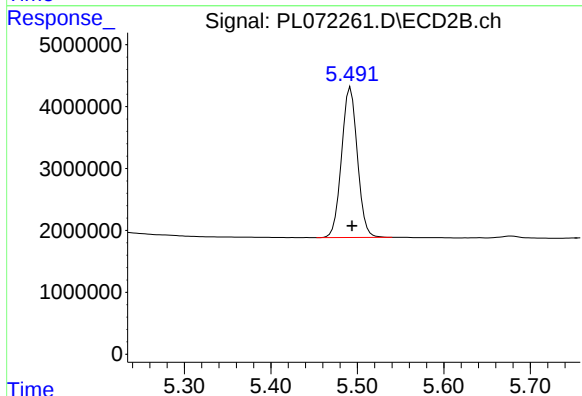


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 30599757
Conc: 18.84 ng/ml

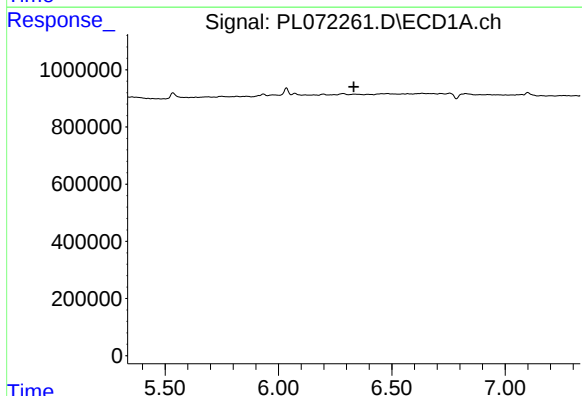


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

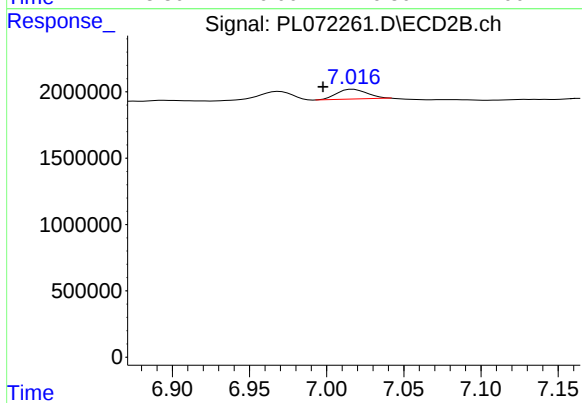

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.020 min
Response: 977691
Conc: 0.40 ng/ml

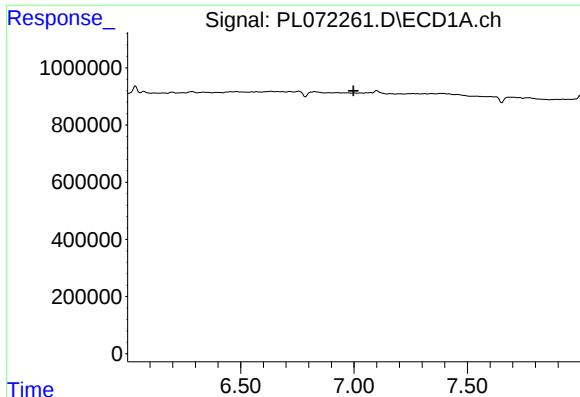

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

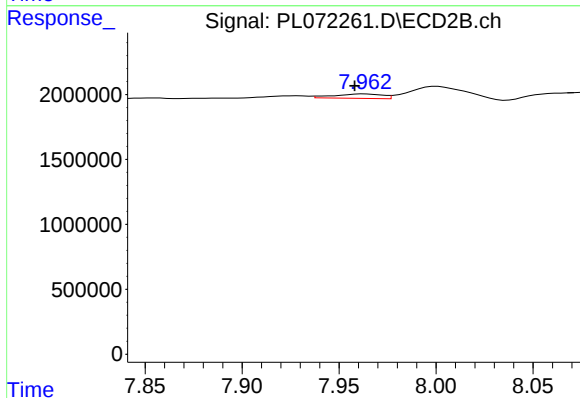


#8 Heptachlor epoxide

R.T.: 7.963 min
Delta R.T.: 0.005 min
Response: 589368
Conc: 0.29 ng/ml

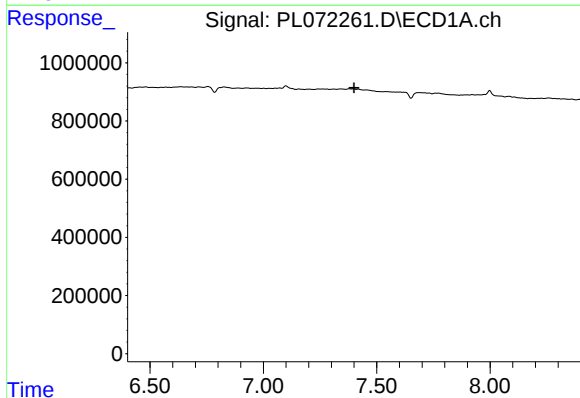


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

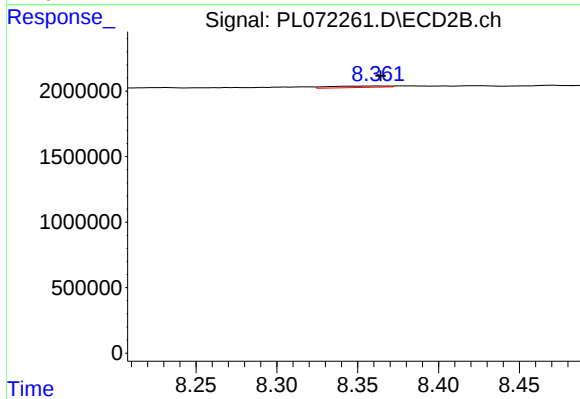

#9 Endosulfan I


R.T.: 8.363 min
Delta R.T.: -0.001 min
Response: 284857
Conc: 0.16 ng/ml

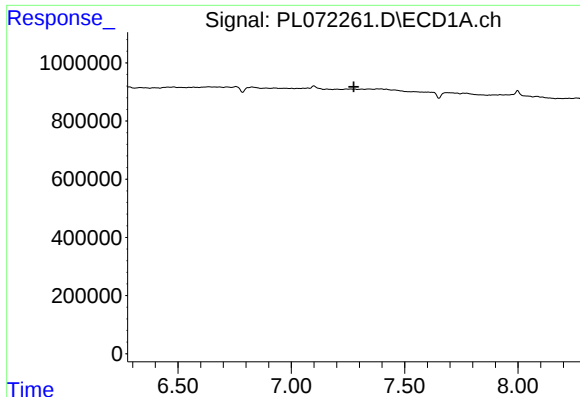

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

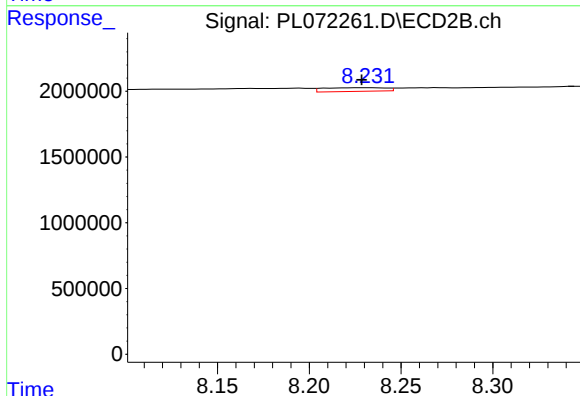


#10 gamma-Chlordane

R.T.: 8.232 min
Delta R.T.: 0.003 min
Response: 666456
Conc: 0.33 ng/ml

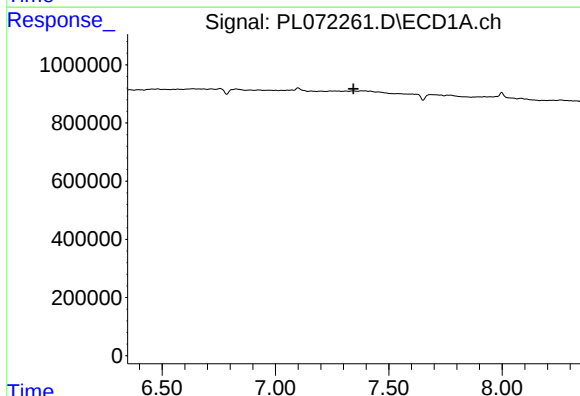


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

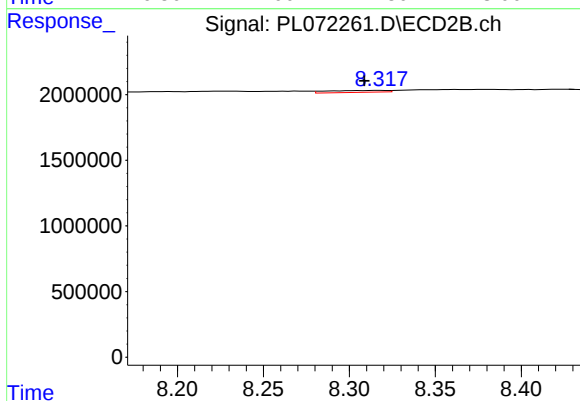

#11 alpha-Chlordane


R.T.: 8.319 min
Delta R.T.: 0.010 min
Response: 353112
Conc: 0.18 ng/ml

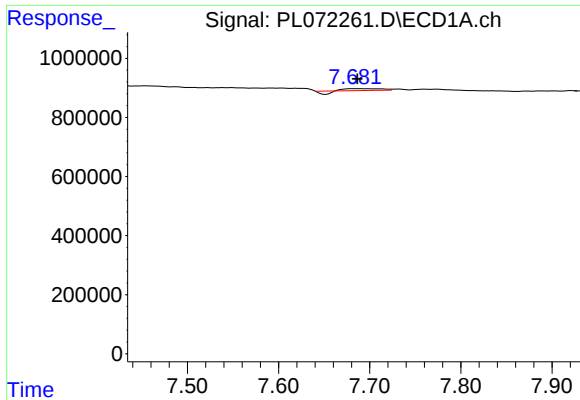

#13 Dieldrin


R.T.: 7.682 min
Delta R.T.: -0.004 min
Response: 117122
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

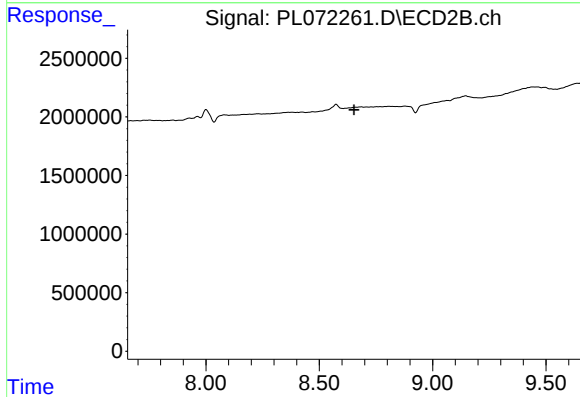


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.653 min
Response: 0
Conc: N.D.

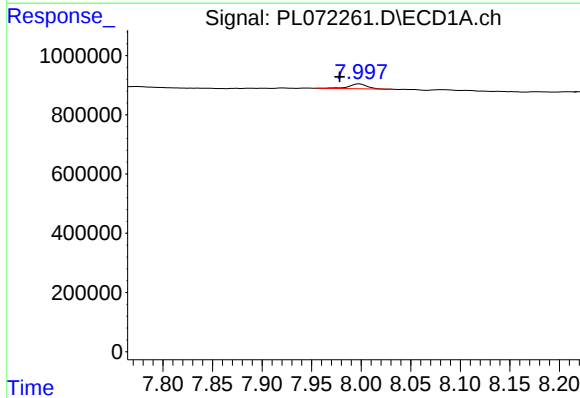


#14 Endrin

R.T.: 7.999 min
Delta R.T.: 0.020 min
Response: 219227
Conc: 0.31 ng/ml

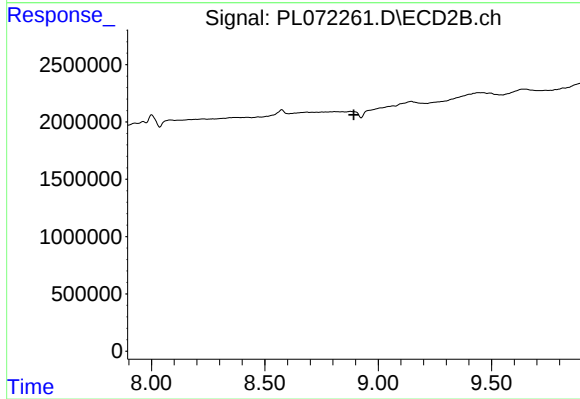

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

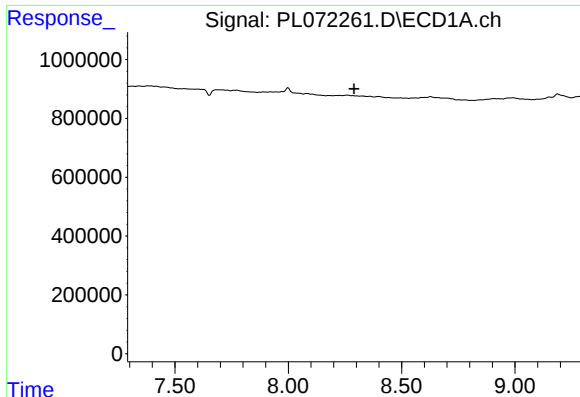

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

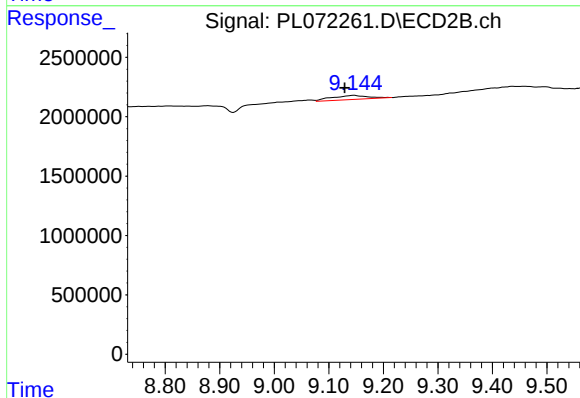


#15 Endosulfan II

R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 1643389
Conc: 0.96 ng/ml

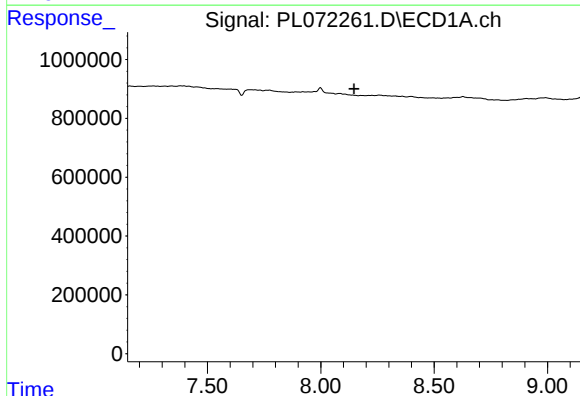


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

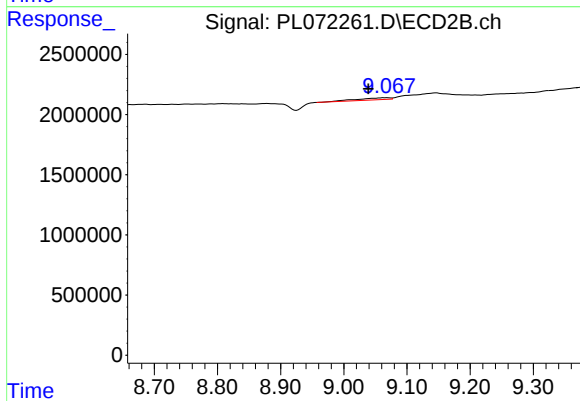

#16 4,4'-DDD


R.T.: 9.068 min
Delta R.T.: 0.030 min
Response: 584543
Conc: 0.41 ng/ml

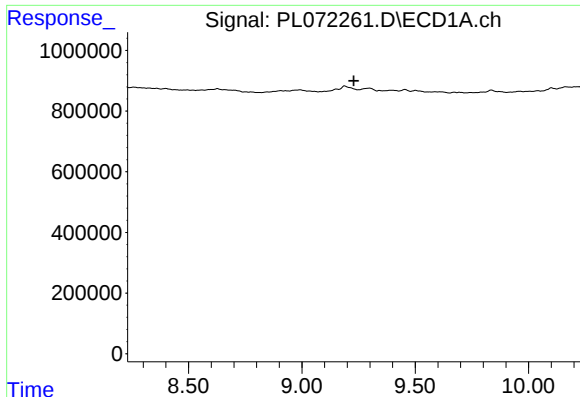

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

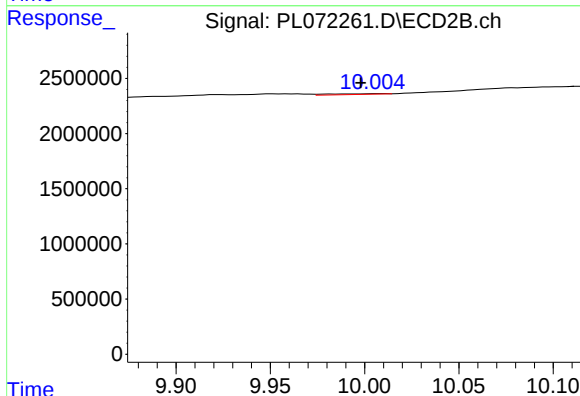


#21 Endrin ketone

R.T.: 10.007 min
Delta R.T.: 0.009 min
Response: 140799
Conc: 0.09 ng/ml

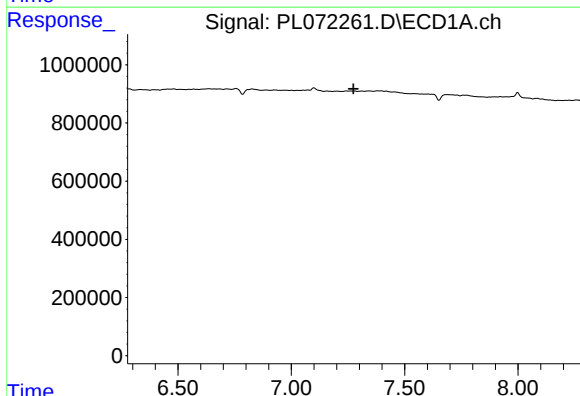


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

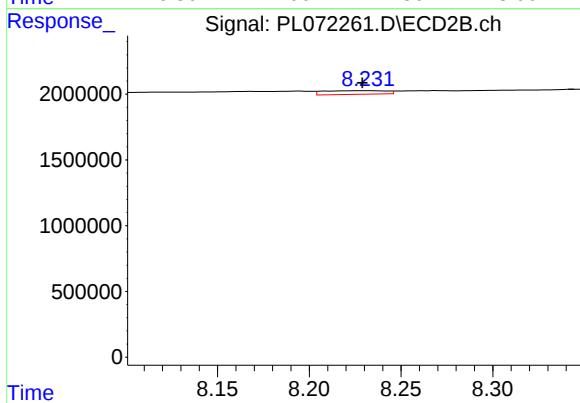

#25 Chlordane-3


R.T.: 8.232 min
Delta R.T.: 0.003 min
Response: 666456
Conc: 2.40 ng/ml

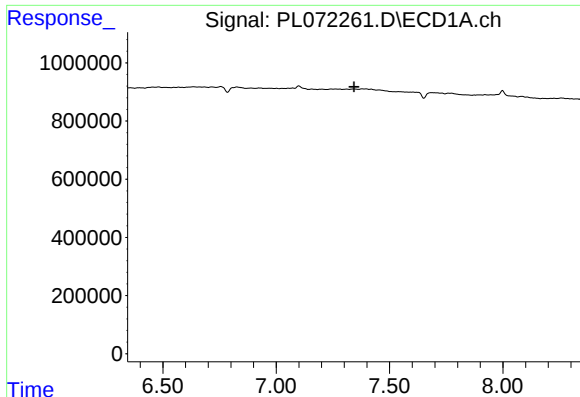

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

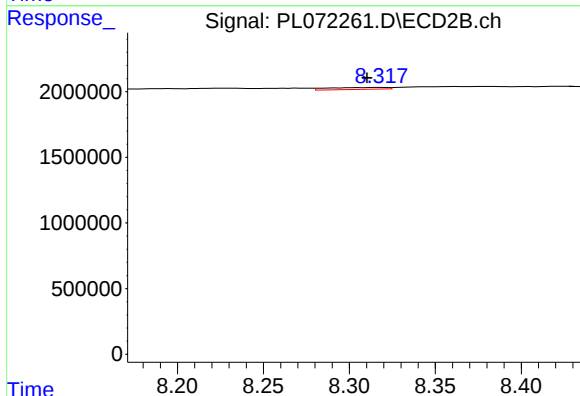


#26 Chlorodane-4

R.T.: 8.319 min
Delta R.T.: 0.008 min
Response: 353112
Conc: 1.06 ng/ml

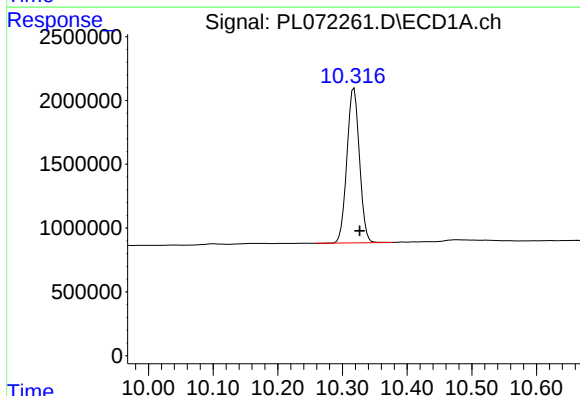

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 16356289
Conc: 18.41 ng/ml

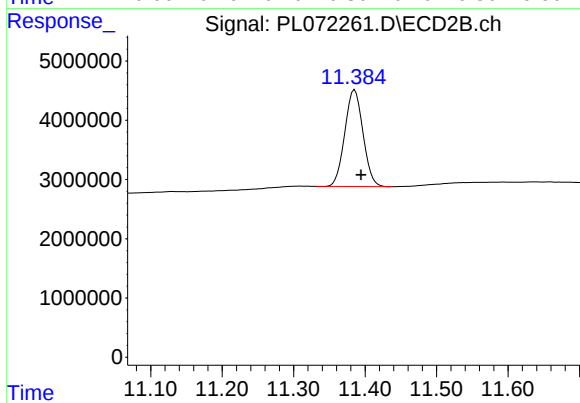

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 28973021
Conc: 17.96 ng/ml