

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
 Data File : PL072239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 17:10
 Operator : AR\AJ
 Sample : N1099-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VACLOT-BACKFILL-TILCON-06

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/26/2022
 Supervised By : Ankita Jodhani 01/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 00:40:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	6600517	18804557	11.889	11.578
2)	SA Decachlor...	10.318	11.385	12121586	20739196	13.644m	12.854

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012522\
Data File : PL072239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 17:10
Operator : AR\AJ
Sample : N1099-06
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/26/2022
Supervised By : Ankita Jodhani 01/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 00:40:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

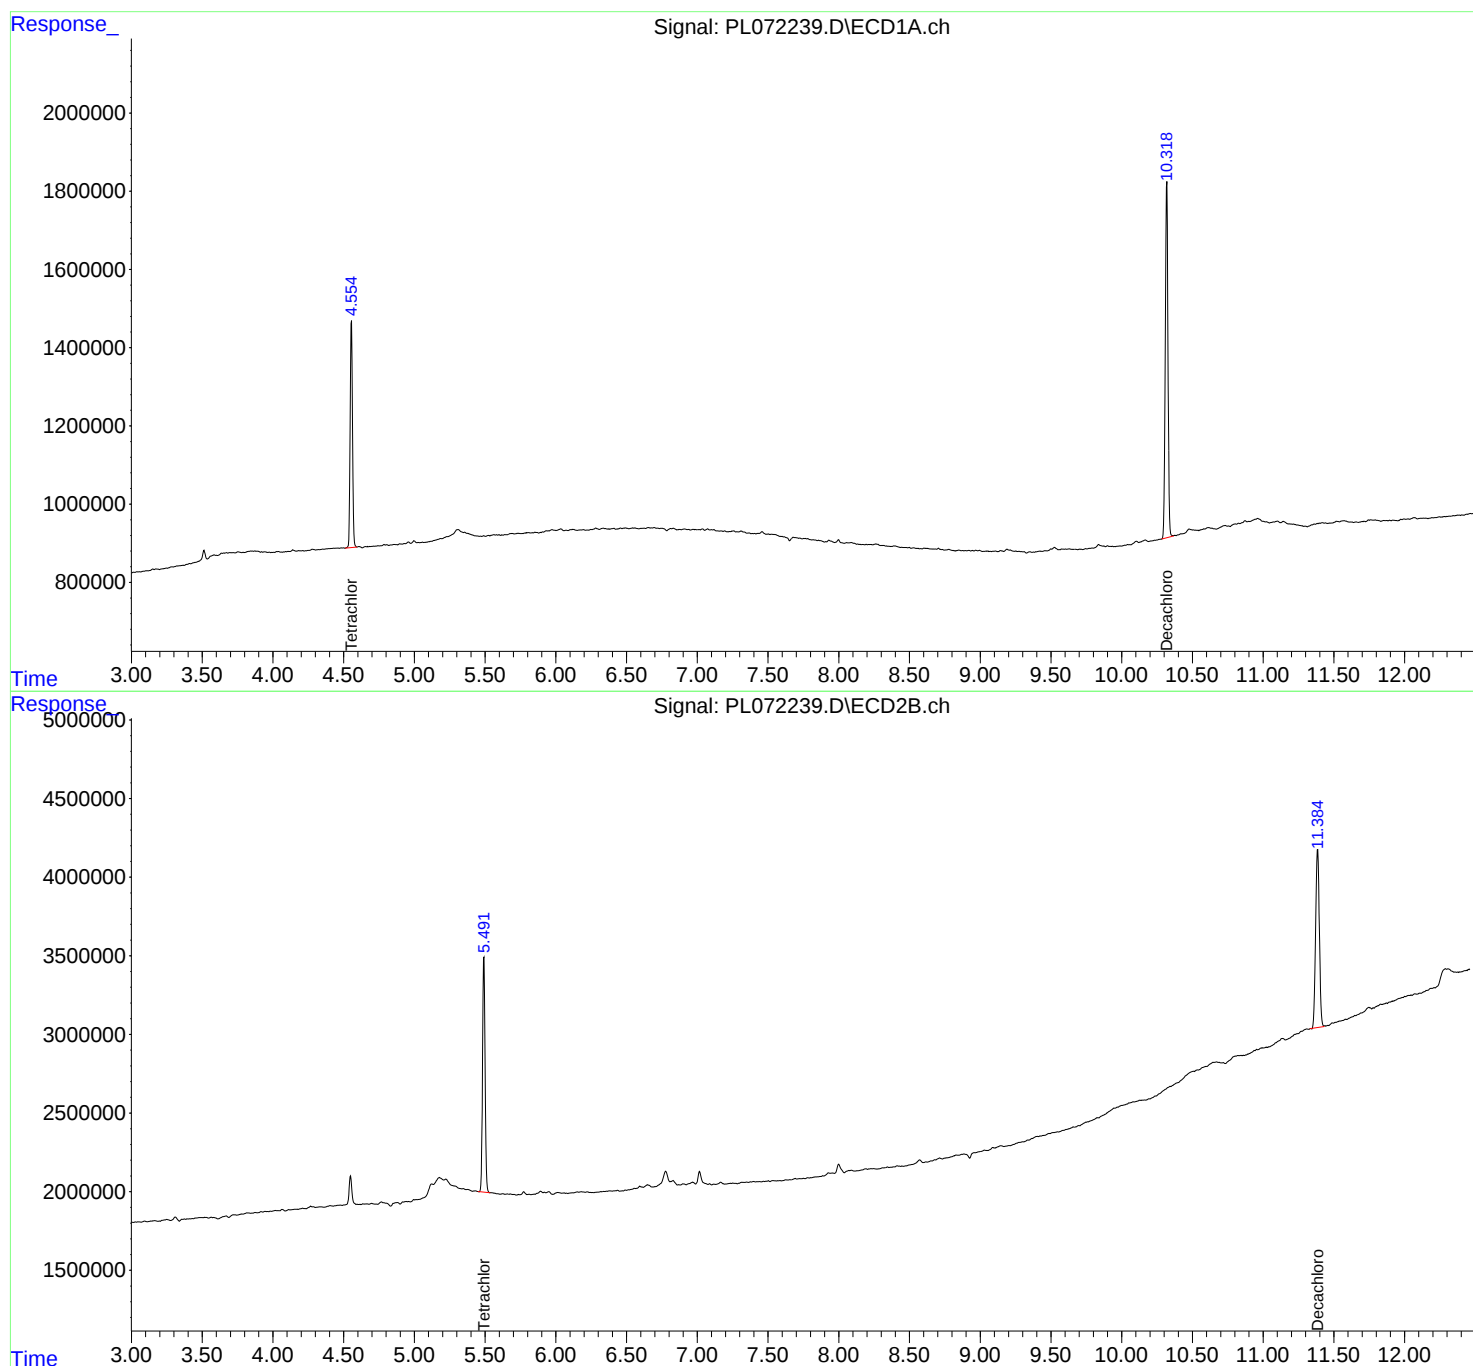

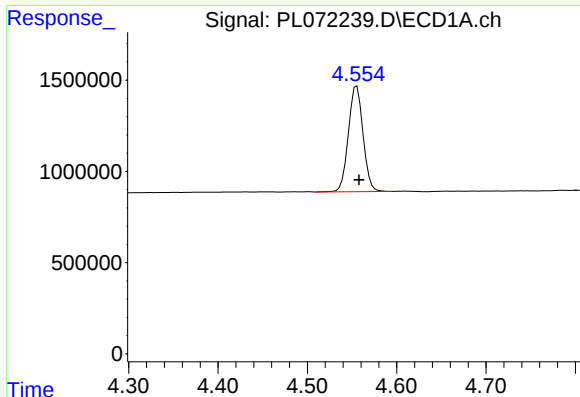


#1 Tetrachloro-m-xylene

R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 6600517
Conc: 11.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
VACLOT-BACKFILL-TILCON-06


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/26/2022
Supervised By :Ankita Jodhani 01/26/2022

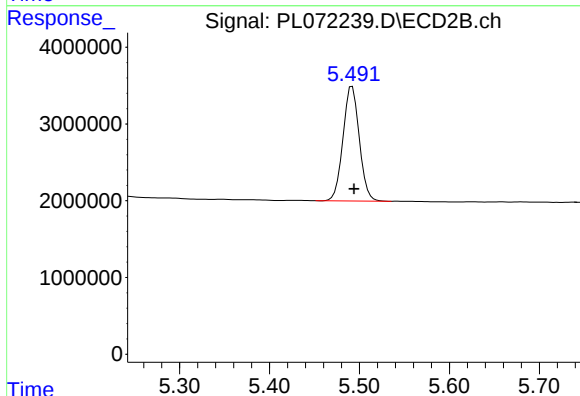


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 18804557
Conc: 11.58 ng/ml

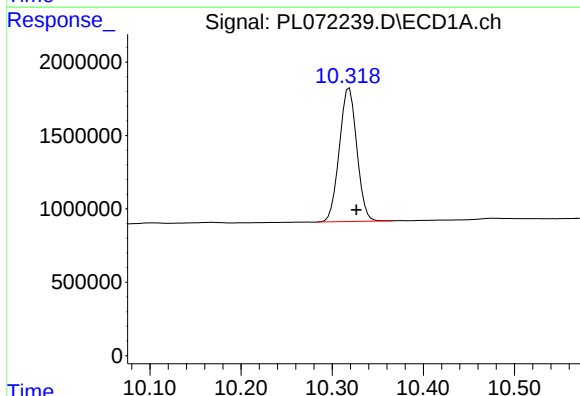

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 12121586
Conc: 13.64 ng/ml m

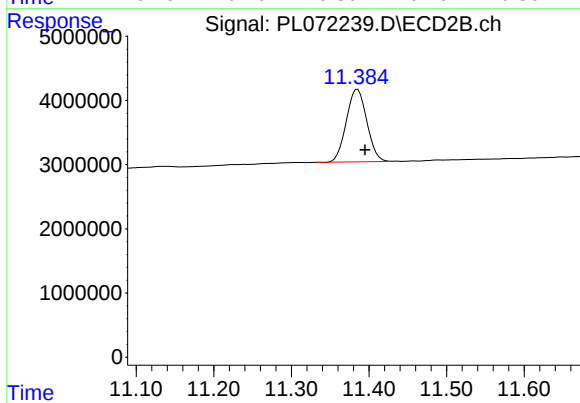

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.009 min
Response: 20739196
Conc: 12.85 ng/ml