

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
 Data File : PL056072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 09:55
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 15:50:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

9) A	Endosulfan I	5.546	0.000	3229480	0	0.249	N.D.	#
11) B	alpha-Chl...	5.488	0.000	11567870	0	0.837	N.D.	#
14) MA	Endrin	6.054	0.000	3620781	0	0.287	N.D.	#
15) B	Endosulfa...	6.303	6.843	4569912	1793762	0.409	0.669	#
23)	Chlordane-1	4.352	0.000	4220465	0	11.511	N.D.	#
24)	Chlordane-2	4.842f	0.000	10211109	0	23.596	N.D.	#
26)	Chlordane-4	5.488	0.000	11567870	0	11.218	N.D.	#
27)	Chlordane-5	6.303f	0.000	4569912	0	11.684	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
Data File : PL056072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 09:55
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 15:50:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

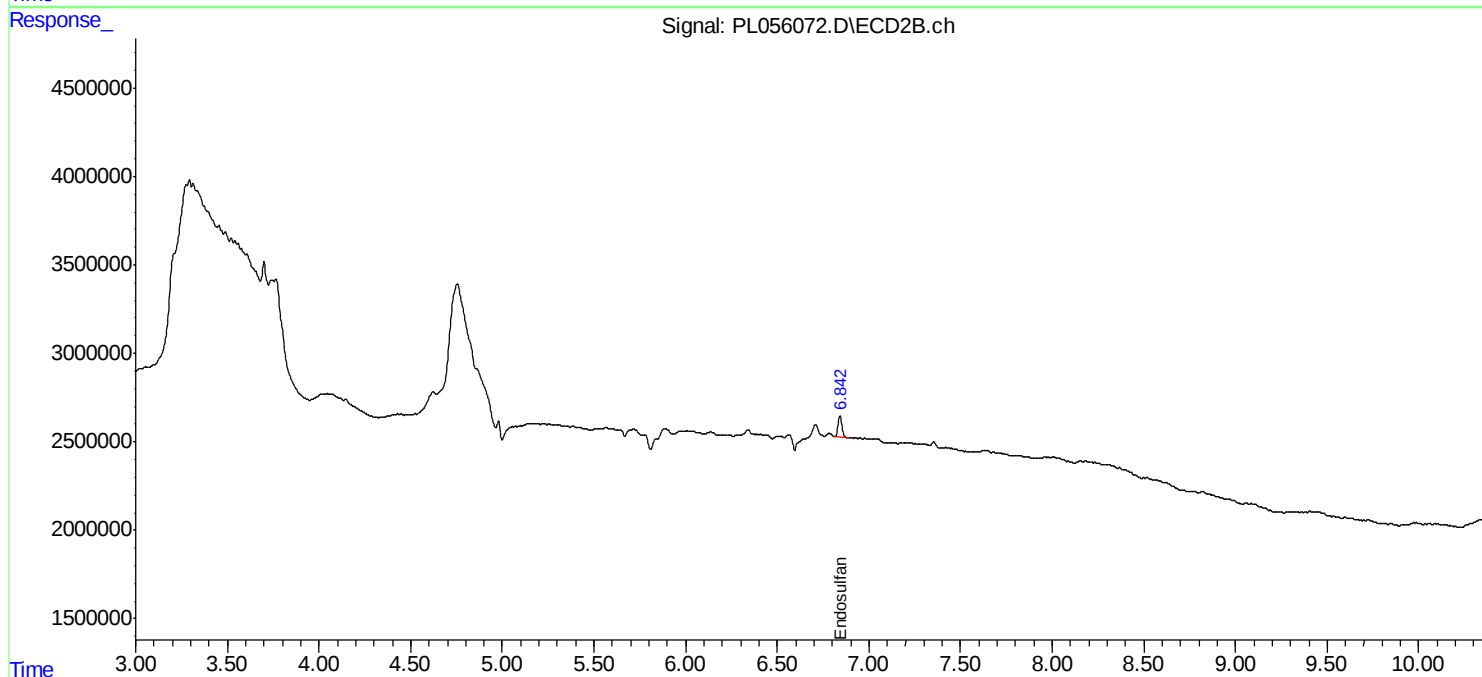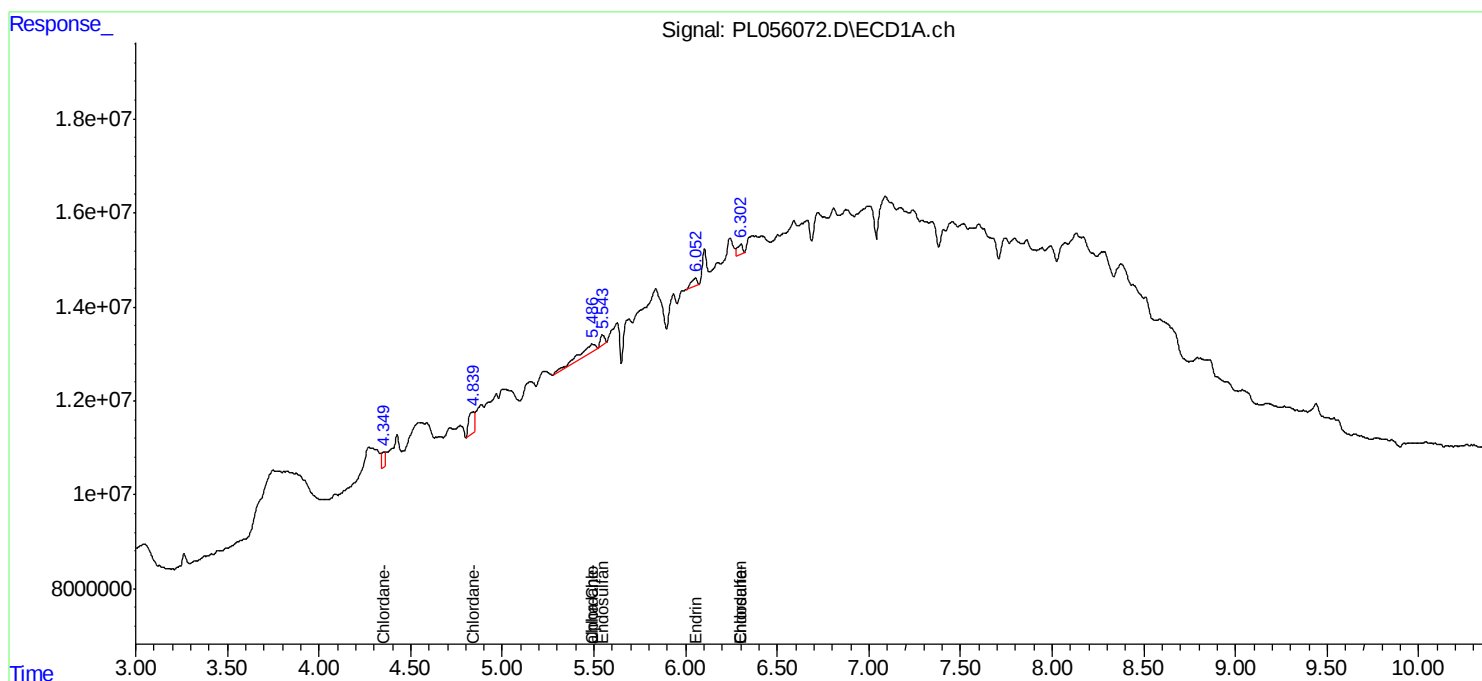


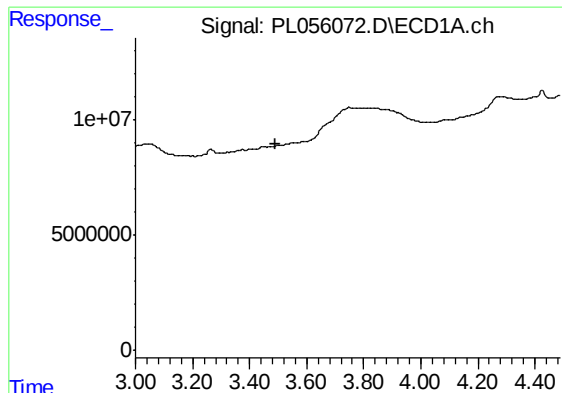

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

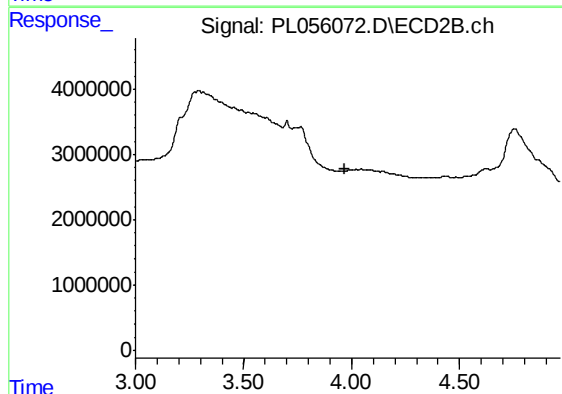


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.967 min
Response: 0
Conc: N.D.

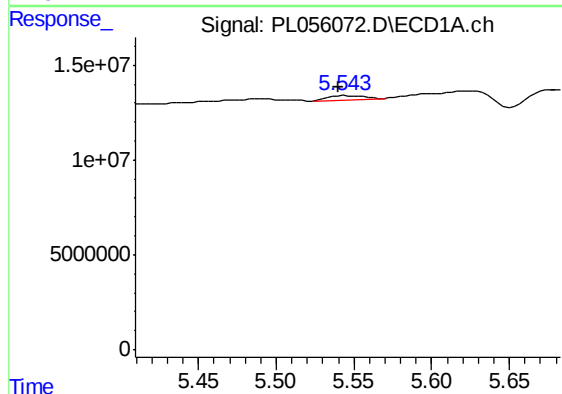


#9 Endosulfan I

R.T.: 5.546 min
Delta R.T.: 0.006 min
Response: 3229480
Conc: 0.25 ng/ml

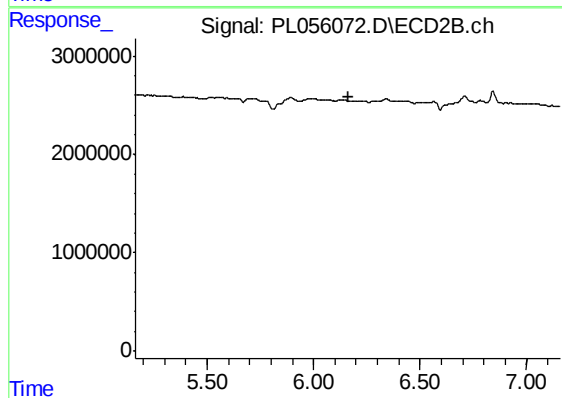

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

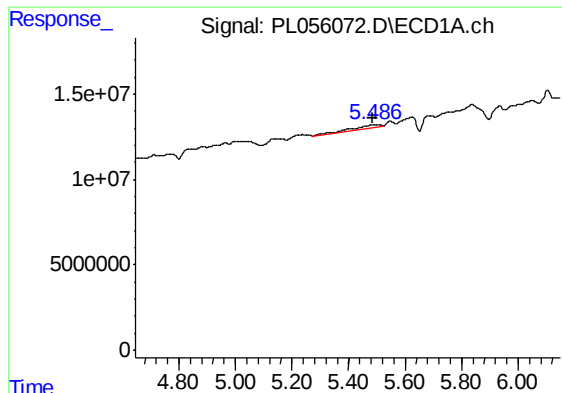

#11 alpha-Chlordane


R.T.: 5.488 min
Delta R.T.: 0.002 min
Response: 11567870
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

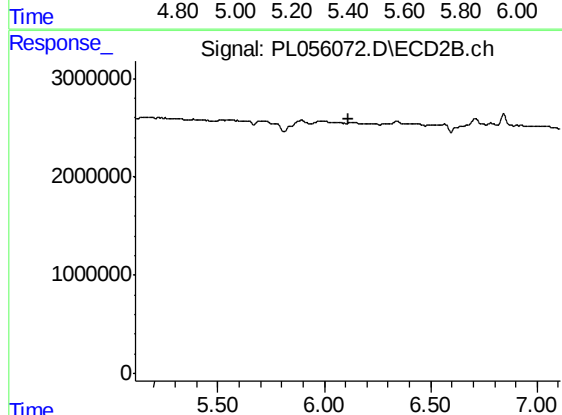


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

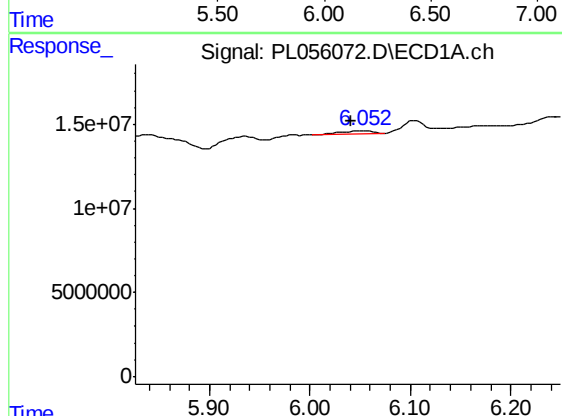


#14 Endrin

R.T.: 6.054 min
Delta R.T.: 0.013 min
Response: 3620781
Conc: 0.29 ng/ml

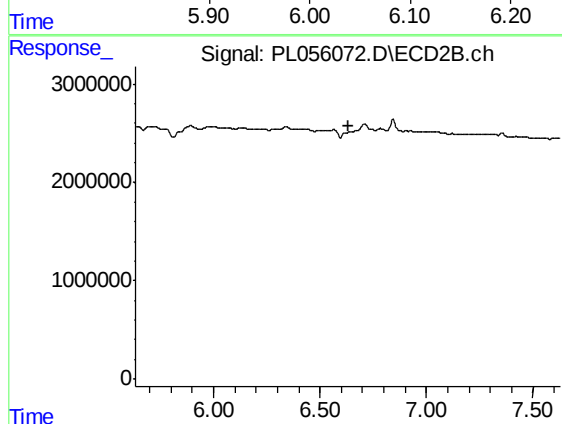

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

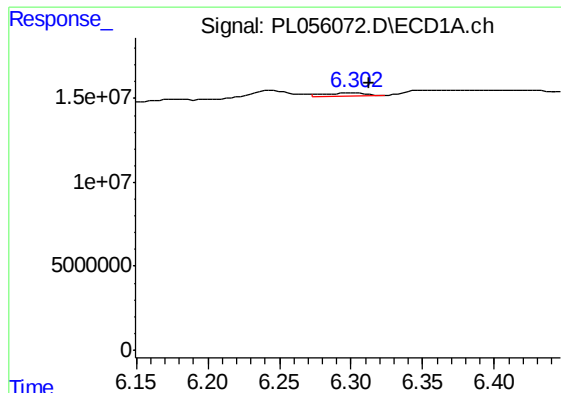

#15 Endosulfan II


R.T.: 6.303 min
Delta R.T.: -0.010 min
Response: 4569912
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

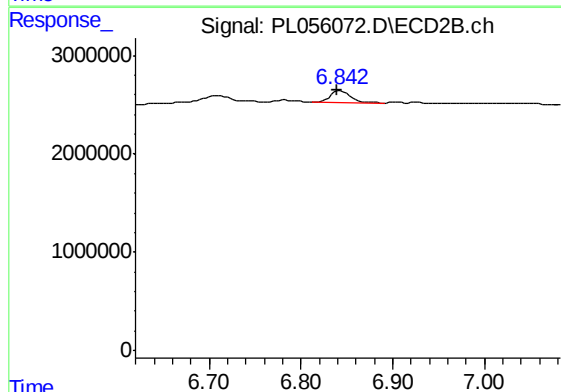


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.004 min
Response: 1793762
Conc: 0.67 ng/ml

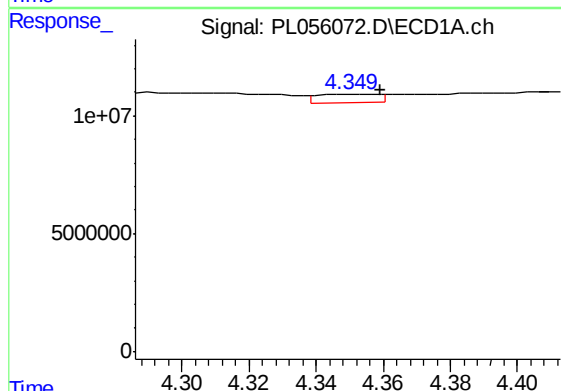


#23 Chlordane-1

R.T.: 4.352 min
Delta R.T.: -0.007 min
Response: 4220465
Conc: 11.51 ng/ml

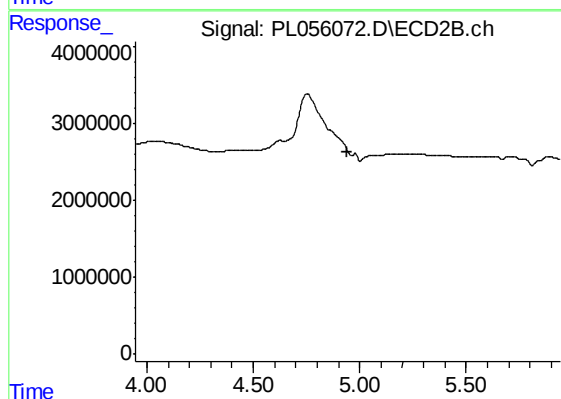

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

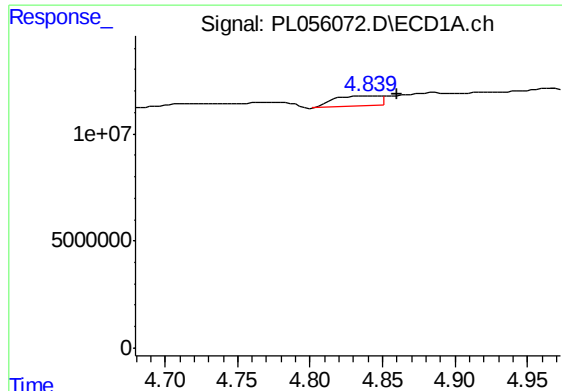

#24 Chlordane-2


R.T.: 4.842 min
Delta R.T.: -0.018 min
Response: 10211109
Conc: 23.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

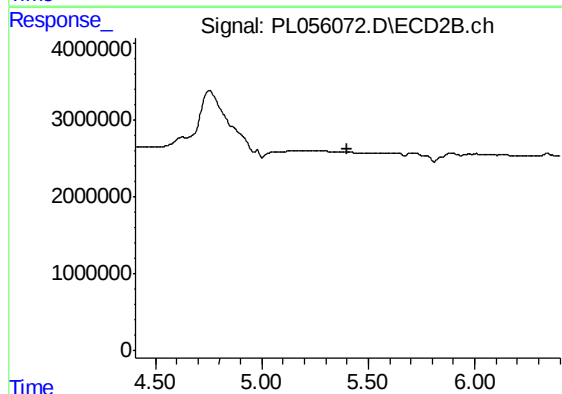


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

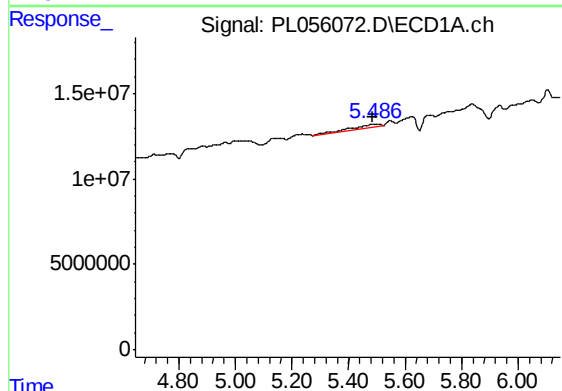


#26 Chlordane-4

R.T.: 5.488 min
Delta R.T.: 0.002 min
Response: 11567870
Conc: 11.22 ng/ml

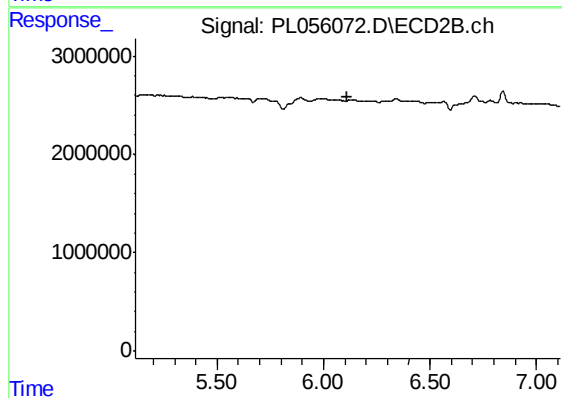

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

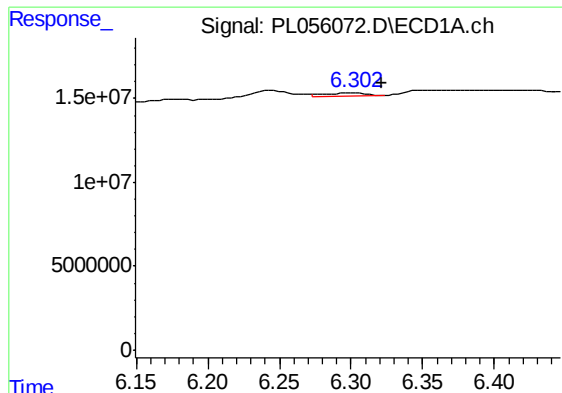

#27 Chlordane-5


R.T.: 6.303 min
Delta R.T.: -0.019 min
Response: 4569912
Conc: 11.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

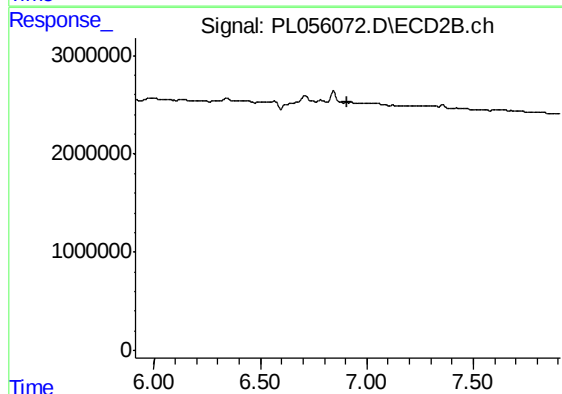


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.910 min
Response: 0
Conc: N.D.

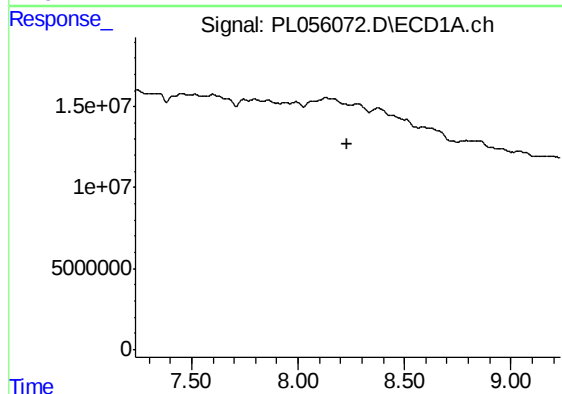

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.233 min
Response: 0
Conc: N.D.

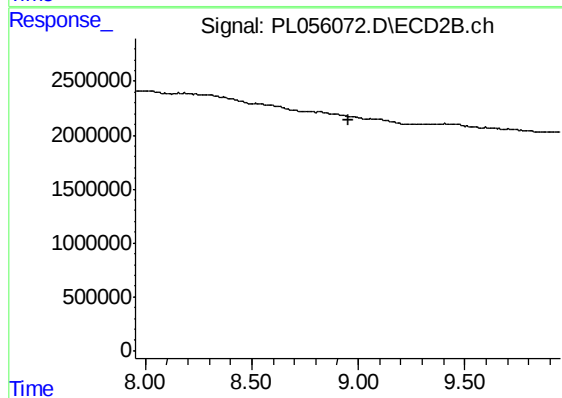

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.952 min
Response: 0
Conc: N.D.