

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
 Data File : PL056077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 13:20
 Operator : AJ\MA
 Sample : PB126343BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB126343BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 15:52:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.490	3.966	219.2E6	68470170	22.865	24.227
28) SA	Decachlor...	8.237	8.954	219.8E6	49820614	21.021	21.747
Target Compounds							
2) A	alpha-BHC	3.925	0.000	7653490	0	0.461	N.D. #
6) B	beta-BHC	4.480f	0.000	790800	0	0.123	N.D. #
9) A	Endosulfan I	5.543	0.000	2249615	0	0.173	N.D. #
11) B	alpha-Chl...	5.481	0.000	10945401	0	0.792	N.D. #
24)	Chlordane-2	4.881f	0.000	3539375	0	8.179	N.D. #
26)	Chlordane-4	5.481	0.000	10945401	0	10.615	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
Data File : PL056077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 13:20
Operator : AJ\MA
Sample : PB126343BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB126343BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 15:52:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

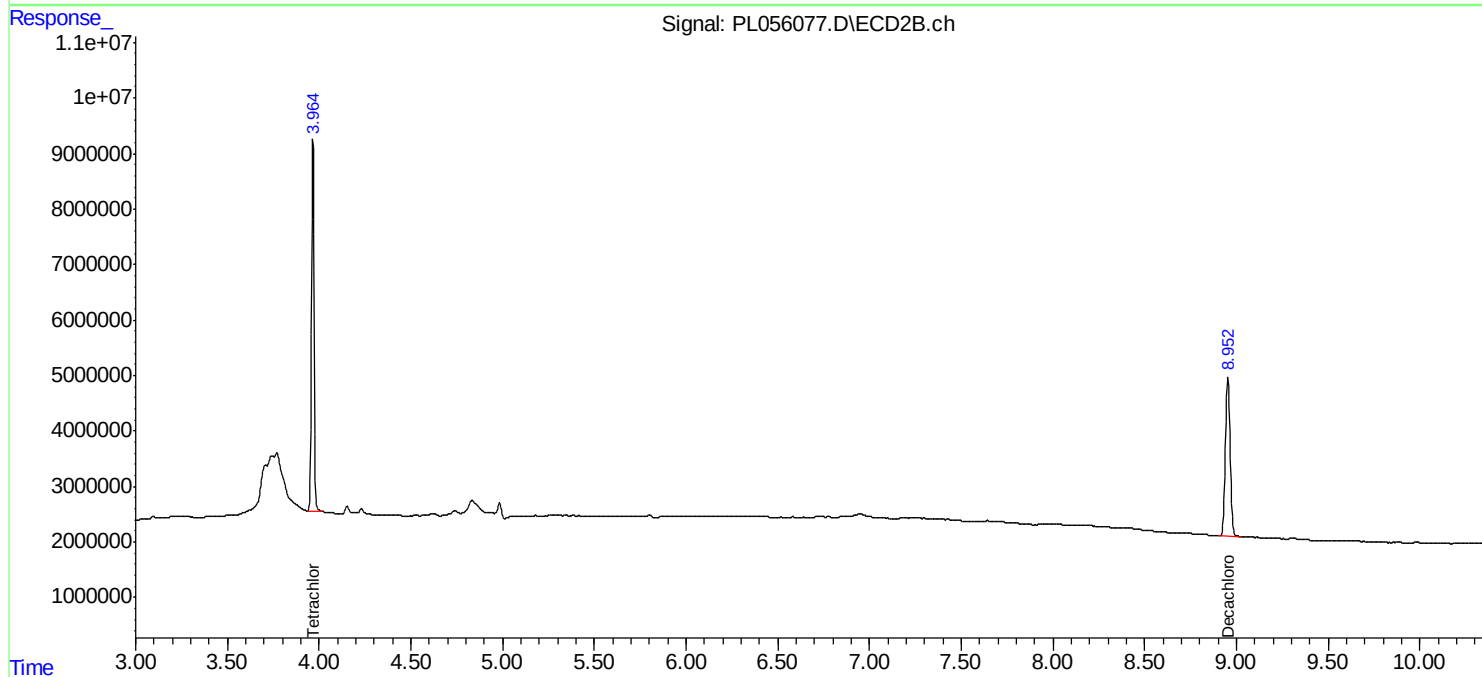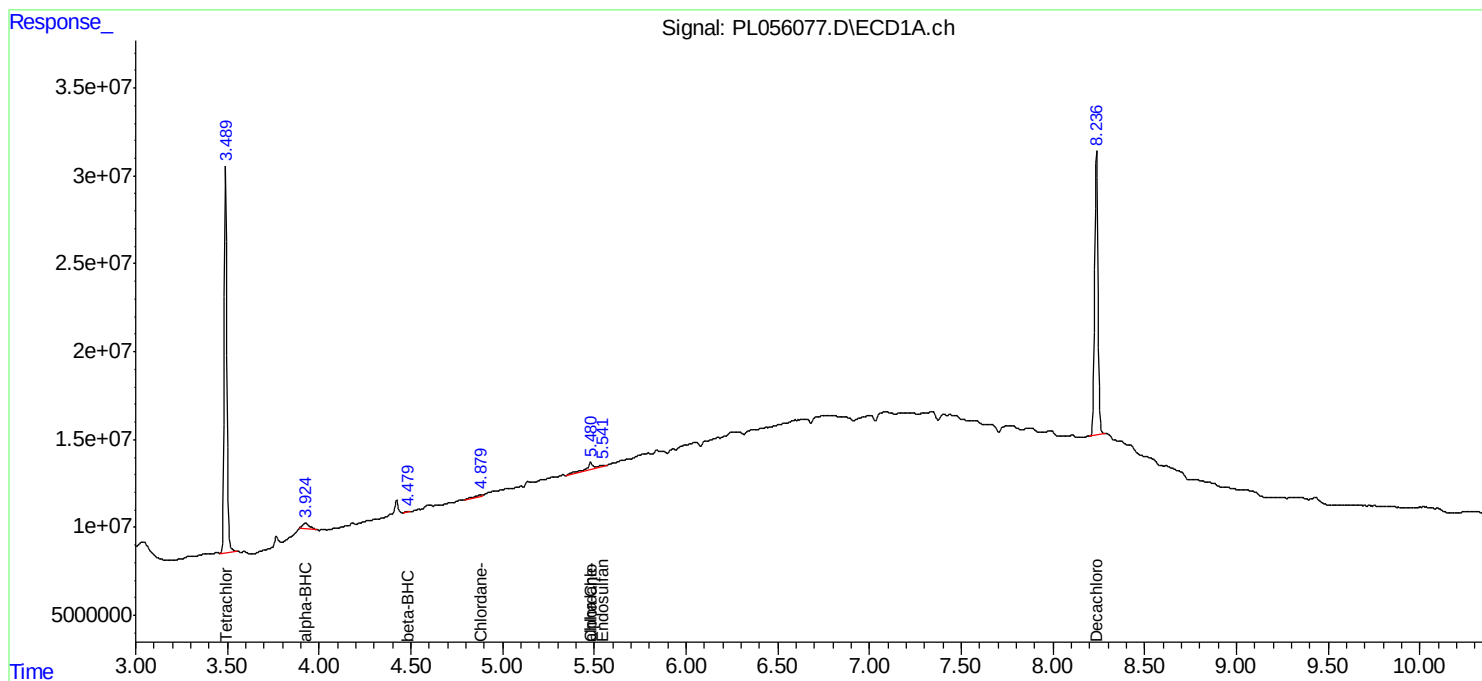


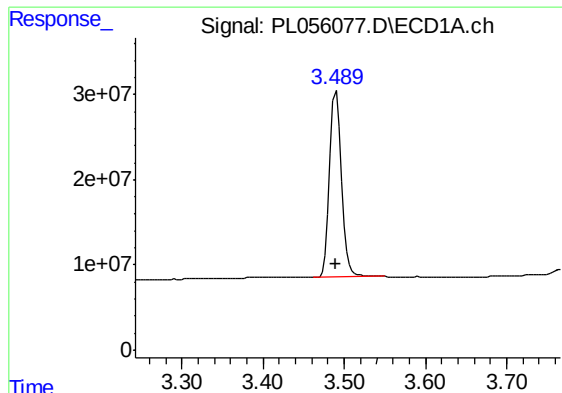

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 219152735
Conc: 22.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126343BL

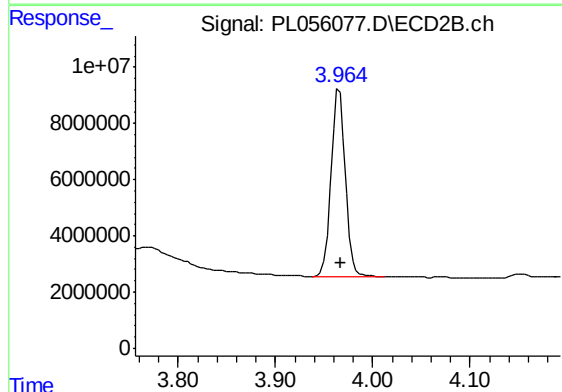


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: -0.001 min
Response: 68470170
Conc: 24.23 ng/ml

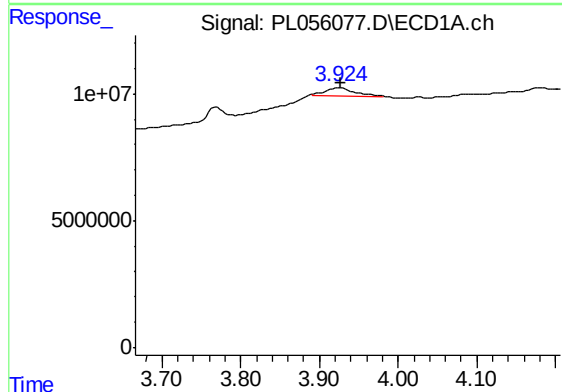


#2 alpha-BHC

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 7653490
Conc: 0.46 ng/ml

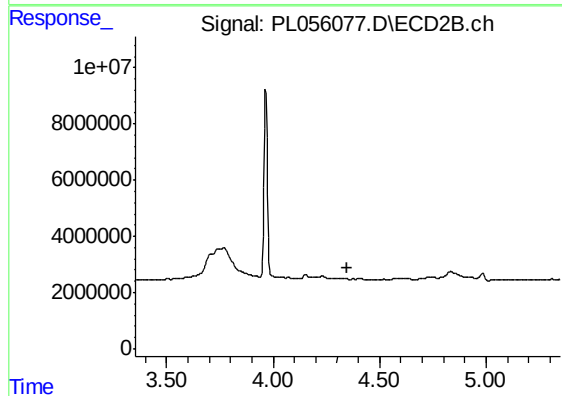

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

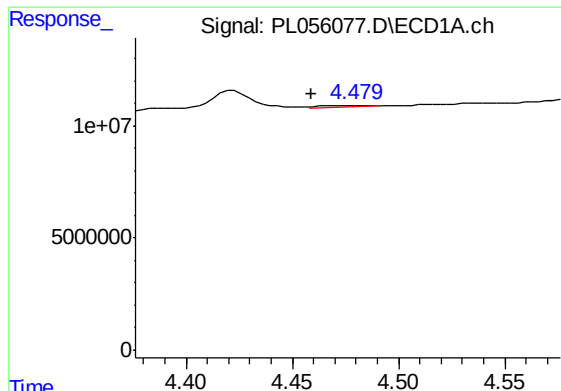

#6 beta-BHC


R.T.: 4.480 min
Delta R.T.: 0.021 min
Response: 790800
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126343BL

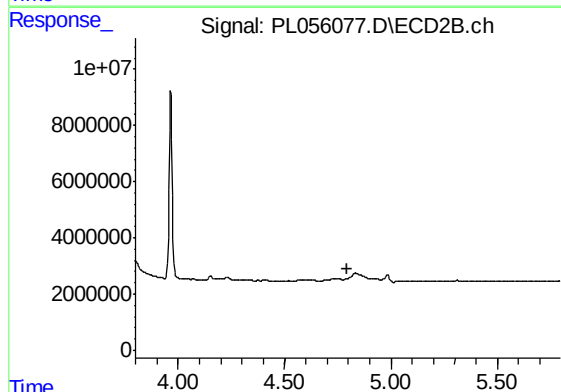


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

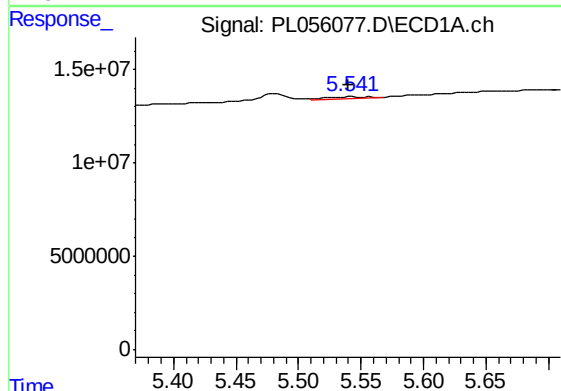


#9 Endosulfan I

R.T.: 5.543 min
Delta R.T.: 0.003 min
Response: 2249615
Conc: 0.17 ng/ml

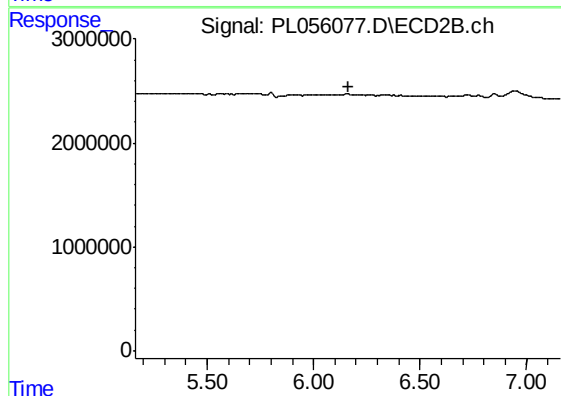

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

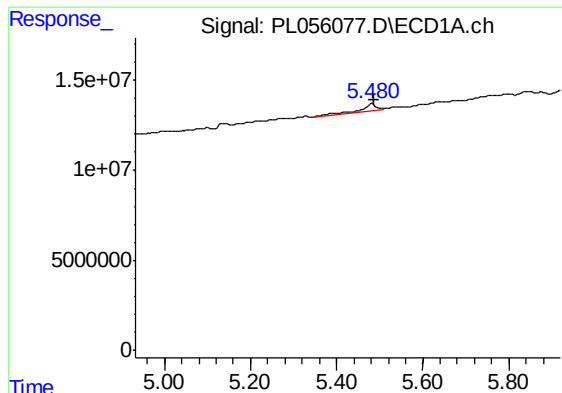

#11 alpha-Chlordane


R.T.: 5.481 min
Delta R.T.: -0.005 min
Response: 10945401
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126343BL

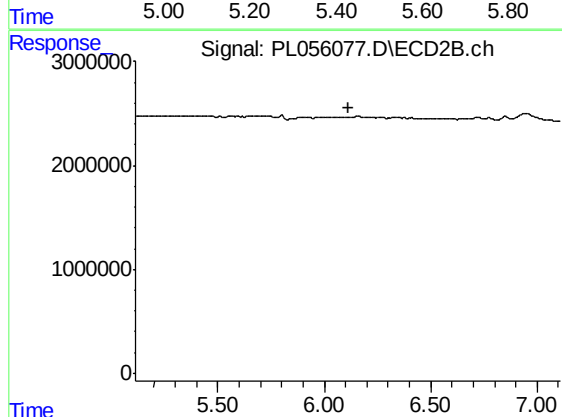


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

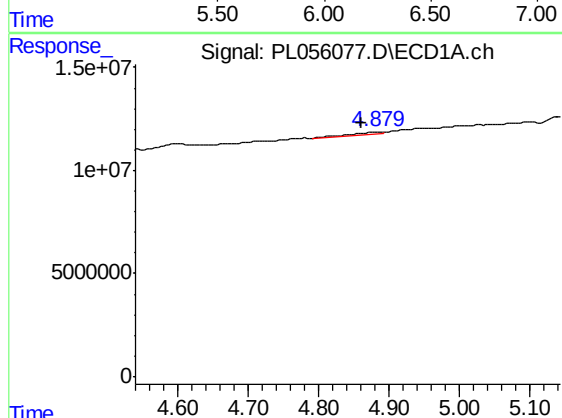


#24 Chlordane-2

R.T.: 4.881 min
Delta R.T.: 0.021 min
Response: 3539375
Conc: 8.18 ng/ml

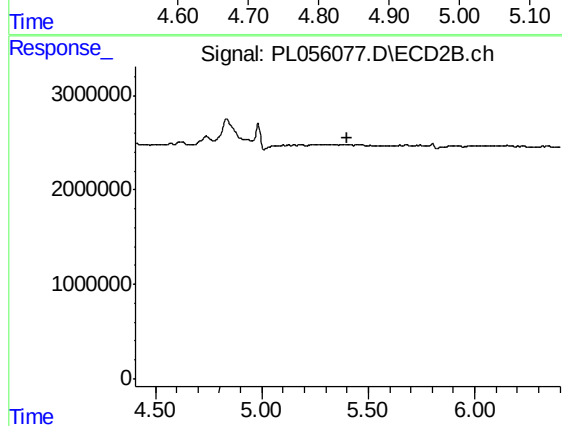

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

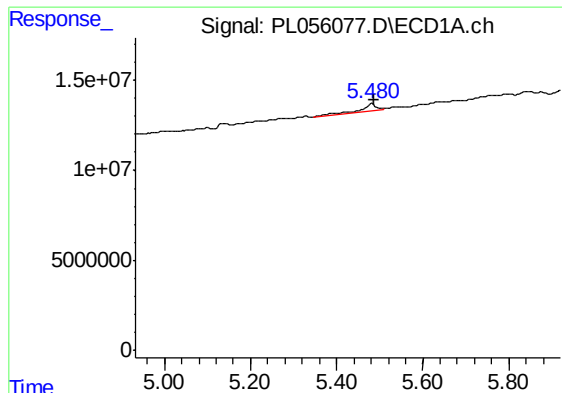

#26 Chlordane-4


R.T.: 5.481 min
Delta R.T.: -0.005 min
Response: 10945401
Conc: 10.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126343BL

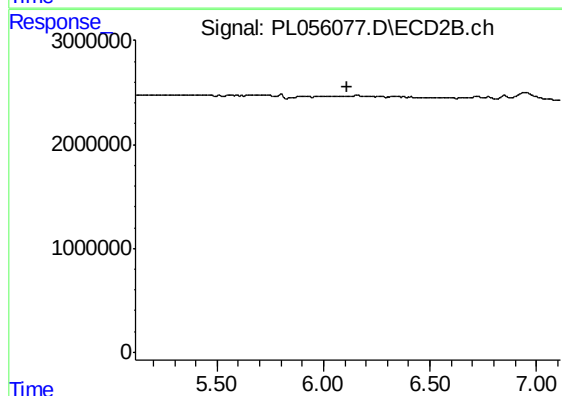


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

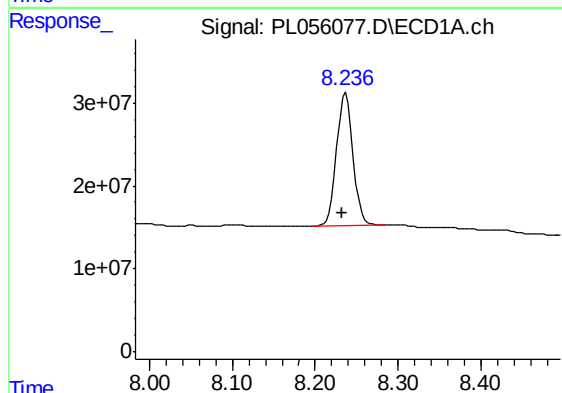

#28 Decachlorobiphenyl

R.T.: 8.237 min
Delta R.T.: 0.004 min
Response: 219784337
Conc: 21.02 ng/ml

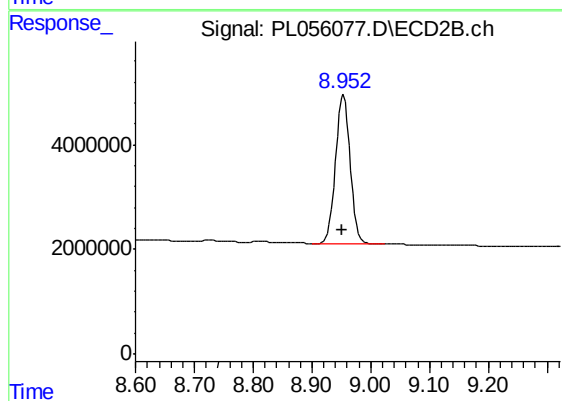

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: 0.001 min
Response: 49820614
Conc: 21.75 ng/ml