

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
 Data File : PL056087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 16:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 17:02:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.963	219.6E6	68342723	22.911	24.181
28)	SA Decachlor...	8.229	8.942	217.9E6	48585601	20.836	21.207
Target Compounds							
2)	A alpha-BHC	3.924	0.000	9783741	0	0.590	N.D. #
4)	MA Heptachlor	4.536f	0.000	2340651	0	0.157	N.D. #
6)	B beta-BHC	0.000	4.827f	0	10755208	N.D.	6.777 #
11)	B alpha-Chl...	5.476	0.000	6589959	0	0.477	N.D. #
23)	Chlordane-1	4.339f	0.000	654804	0	1.786	N.D. #
24)	Chlordane-2	4.877f	0.000	6040093	0	13.958	N.D. #
26)	Chlordane-4	5.476	0.000	6589959	0	6.391	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
Data File : PL056087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 16:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 17:02:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

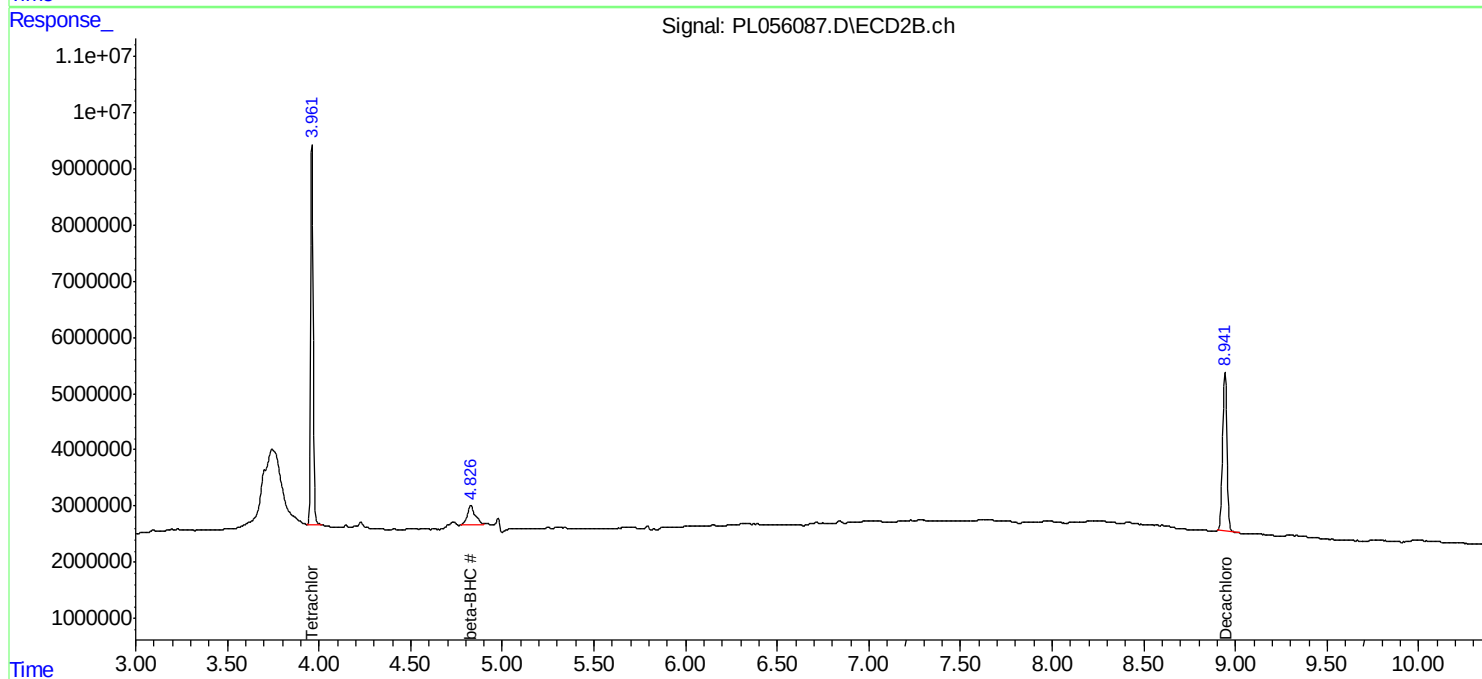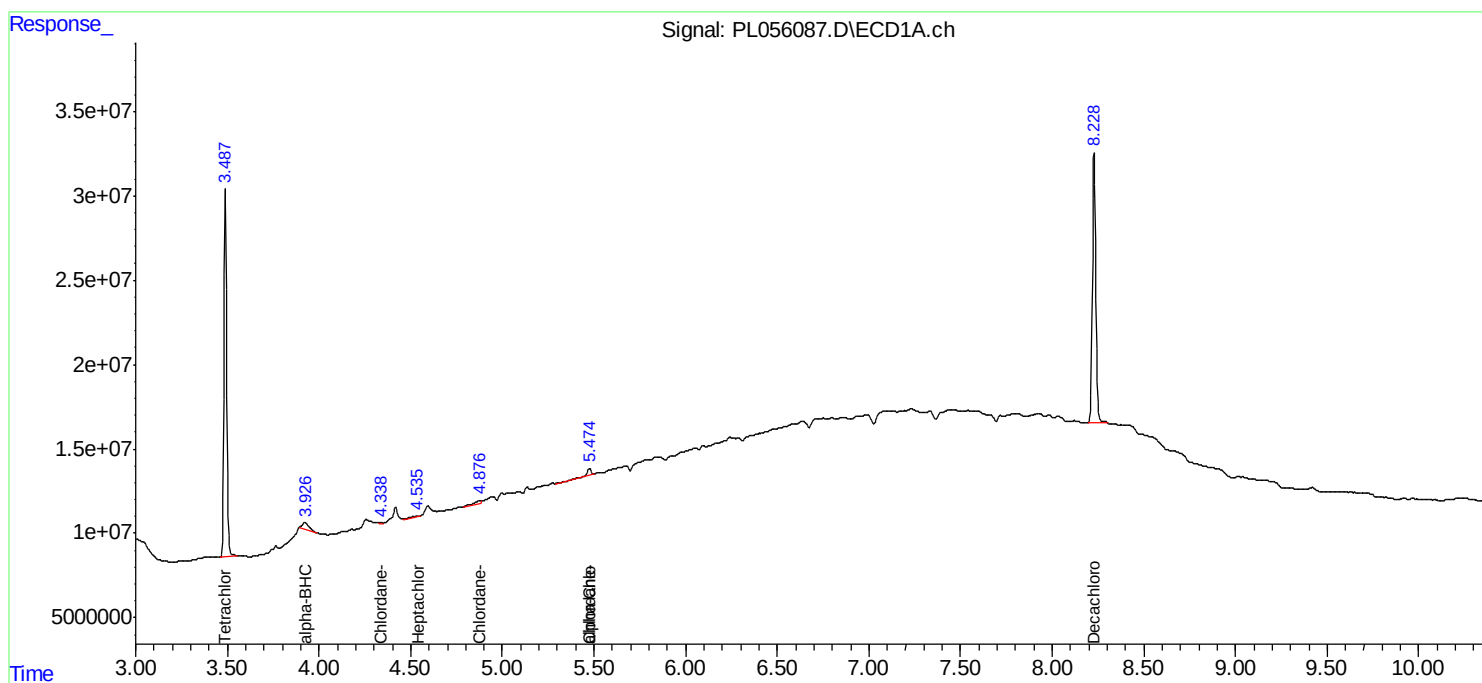


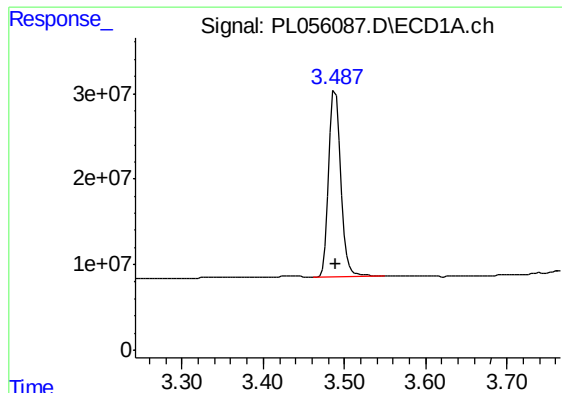

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: -0.001 min
Response: 219591555
Conc: 22.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

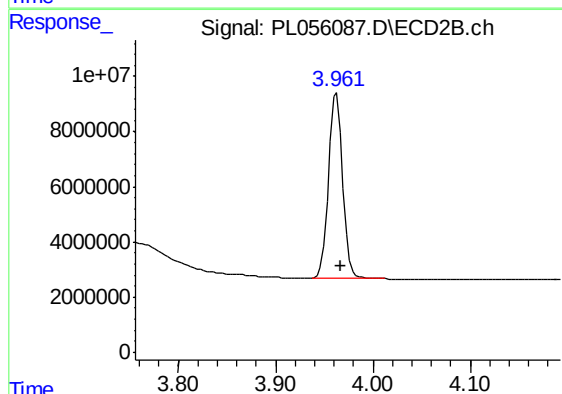


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.004 min
Response: 68342723
Conc: 24.18 ng/ml

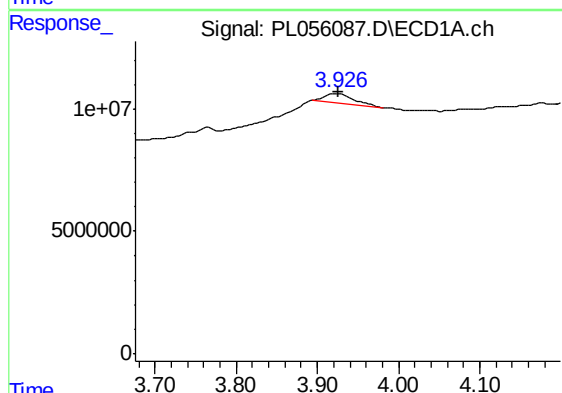


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 9783741
Conc: 0.59 ng/ml

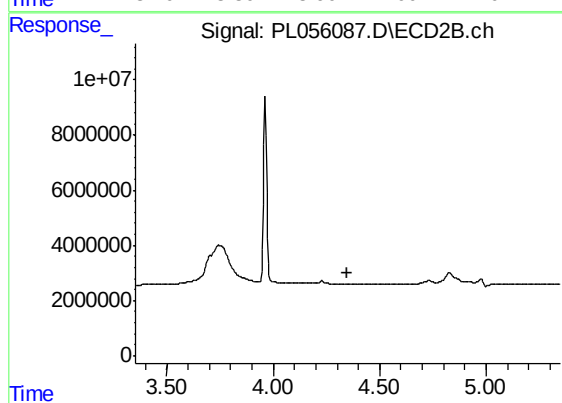

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

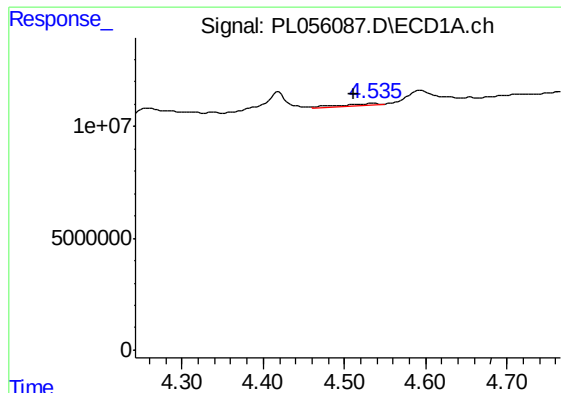

#4 Heptachlor


R.T.: 4.536 min
Delta R.T.: 0.026 min
Response: 2340651
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

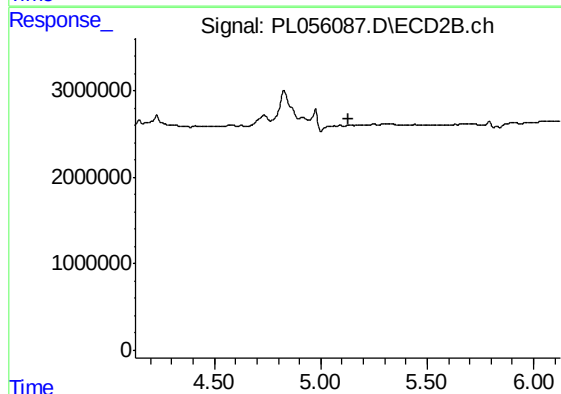


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

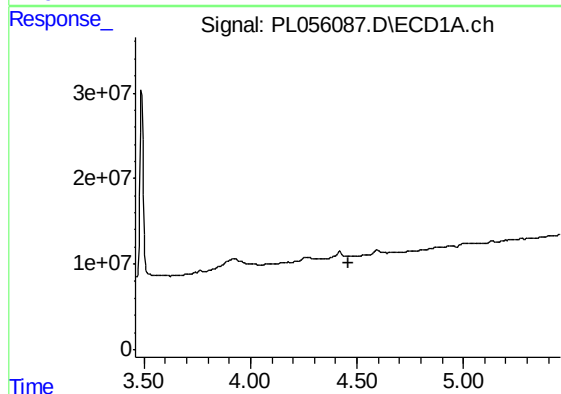


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

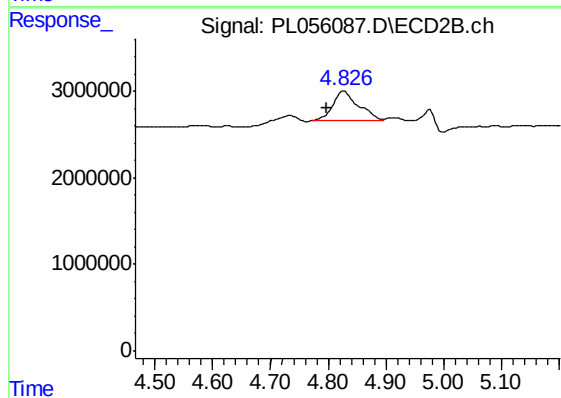

#6 beta-BHC


R.T.: 4.827 min
Delta R.T.: 0.029 min
Response: 10755208
Conc: 6.78 ng/ml

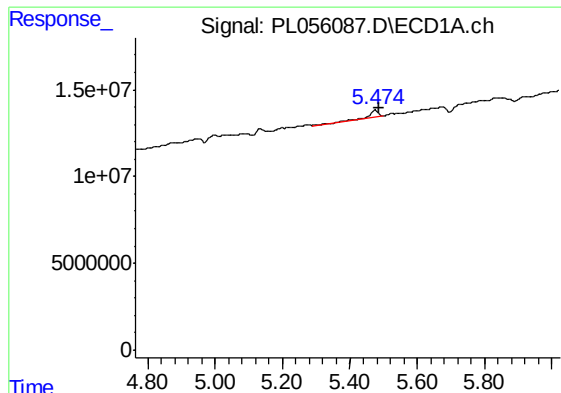

#11 alpha-Chlordane


R.T.: 5.476 min
Delta R.T.: -0.011 min
Response: 6589959
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

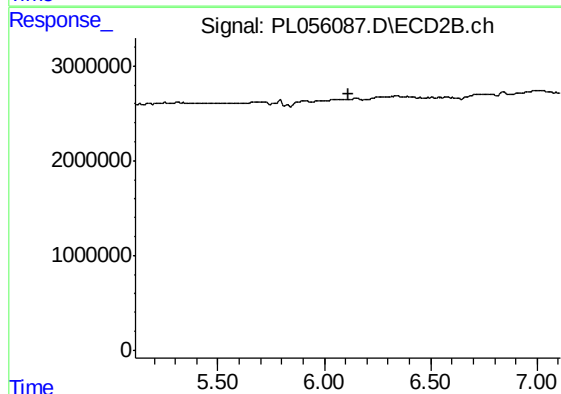


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

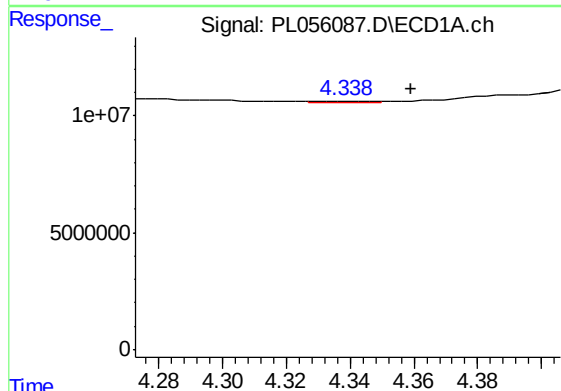


#23 Chlordane-1

R.T.: 4.339 min
Delta R.T.: -0.020 min
Response: 654804
Conc: 1.79 ng/ml

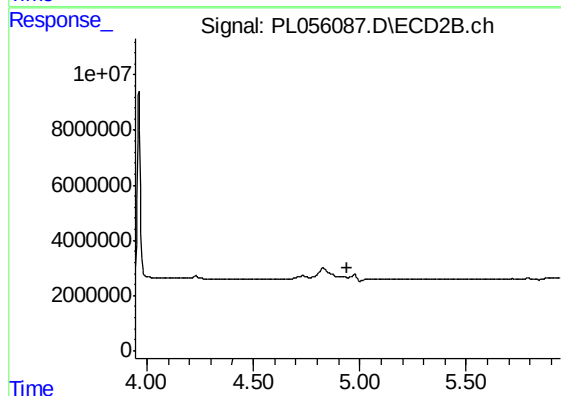

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

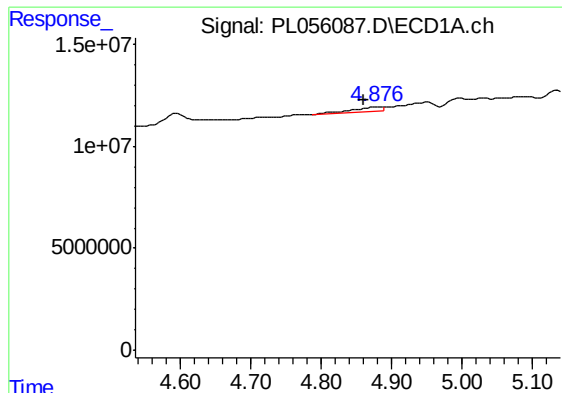

#24 Chlordane-2


R.T.: 4.877 min
Delta R.T.: 0.017 min
Response: 6040093
Conc: 13.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

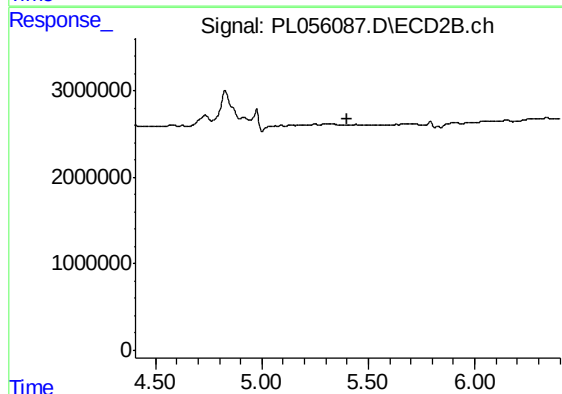


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

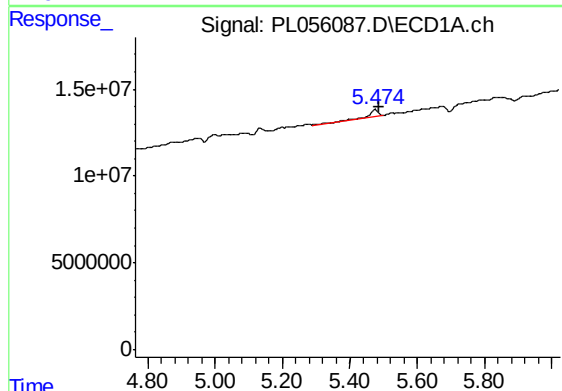


#26 Chlordane-4

R.T.: 5.476 min
Delta R.T.: -0.010 min
Response: 6589959
Conc: 6.39 ng/ml

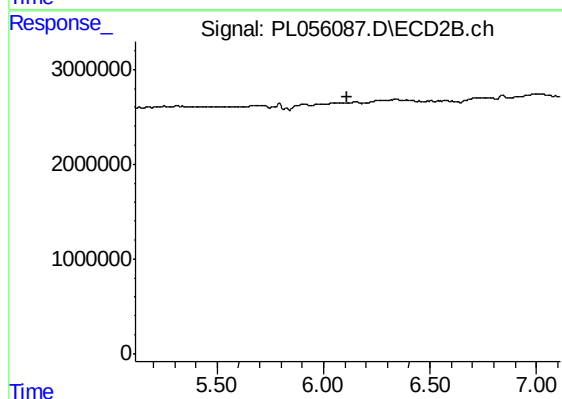

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

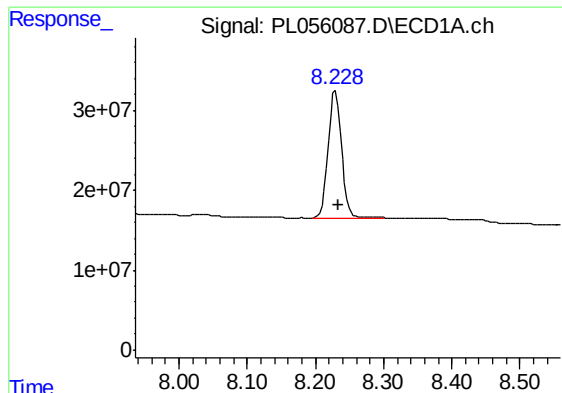

#28 Decachlorobiphenyl

R.T.: 8.229 min
Delta R.T.: -0.004 min
Response: 217857505
Conc: 20.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

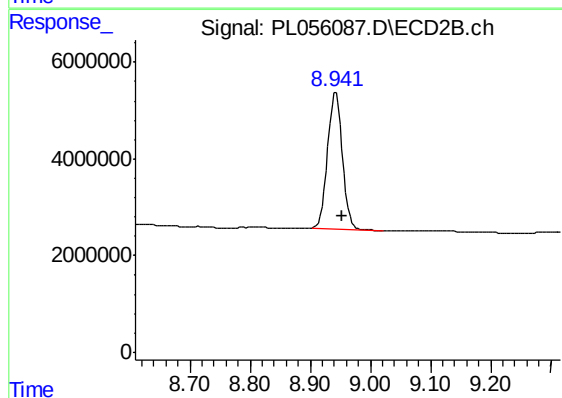

#28 Decachlorobiphenyl

R.T.: 8.942 min
Delta R.T.: -0.010 min
Response: 48585601
Conc: 21.21 ng/ml