

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
 Data File : PL056090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 17:31
 Operator : AJ\MA
 Sample : PB126357BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 01:05:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.493	3.962	202.1E6	64196411	21.087	22.714
28)	SA Decachlor...	8.240	8.951	222.8E6	48198233	21.308	21.038
Target Compounds							
6)	B beta-BHC	4.474f	4.803	765786	11641999	0.119	7.336 #
9)	A Endosulfan I	5.533	0.000	3143138	0	0.242	N.D. #
10)	B gamma-Chl...	5.422	0.000	6599459	0	0.470	N.D. #
11)	B alpha-Chl...	5.489	0.000	6887716	0	0.498	N.D. #
13)	MA Dieldrin	5.790	0.000	7211924	0	0.521	N.D. #
15)	B Endosulfa...	0.000	6.843	0	1591615	N.D.	0.593 #
18)	B Endrin al...	6.490	0.000	5000114	0	0.481	N.D. #
25)	Chlordane-3	5.422	0.000	6599459	0	5.300	N.D. #
26)	Chlordane-4	5.489	0.000	6887716	0	6.680	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
Data File : PL056090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 17:31
Operator : AJ\MA
Sample : PB126357BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 01:05:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

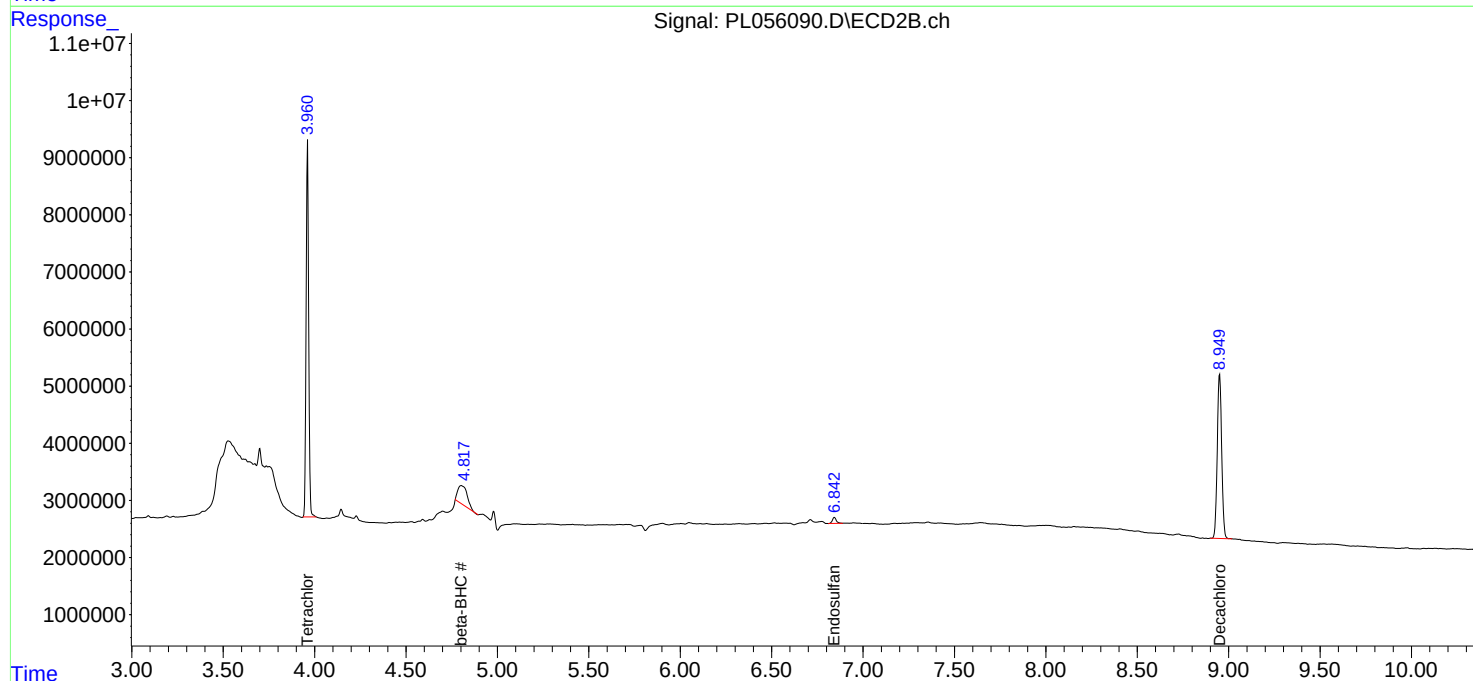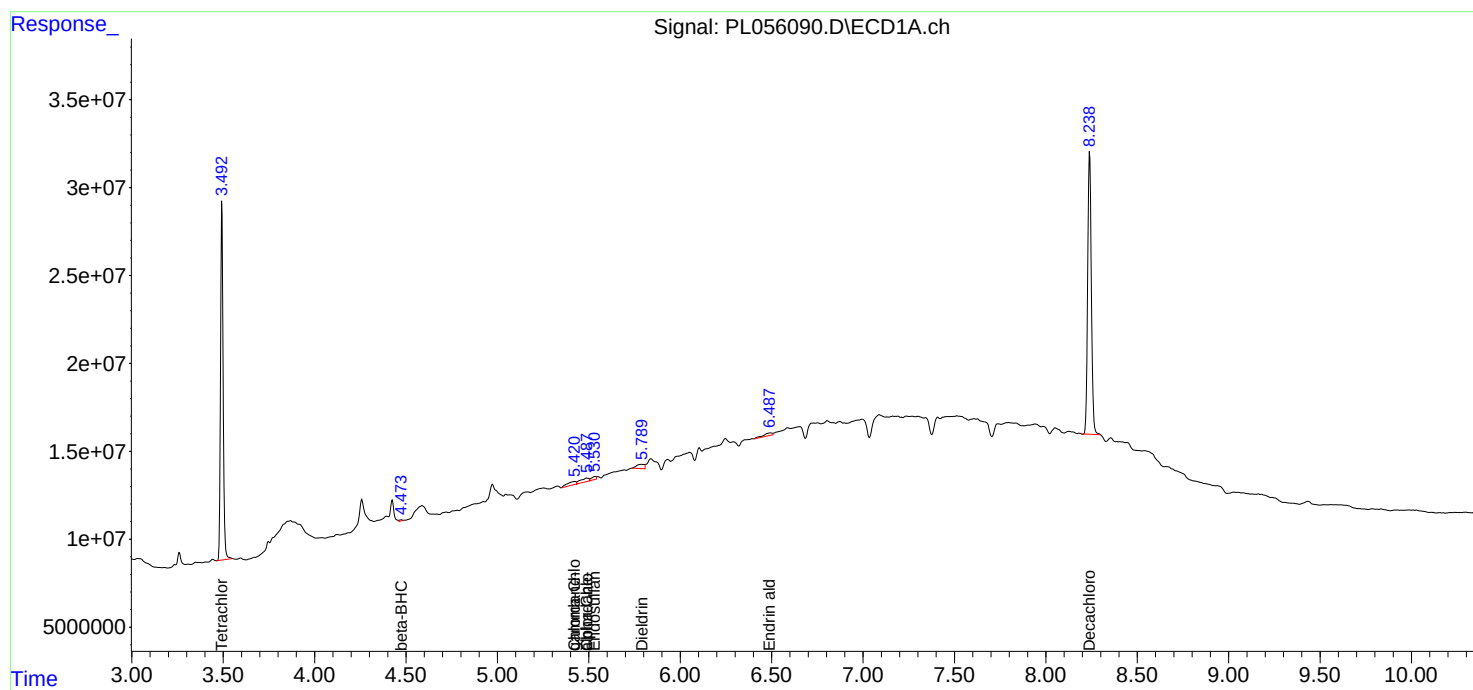


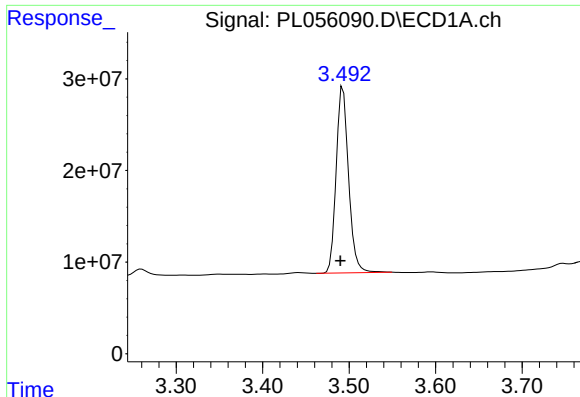

#1 Tetrachloro-m-xylene


R.T.: 3.493 min
Delta R.T.: 0.003 min
Response: 202112240
Conc: 21.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

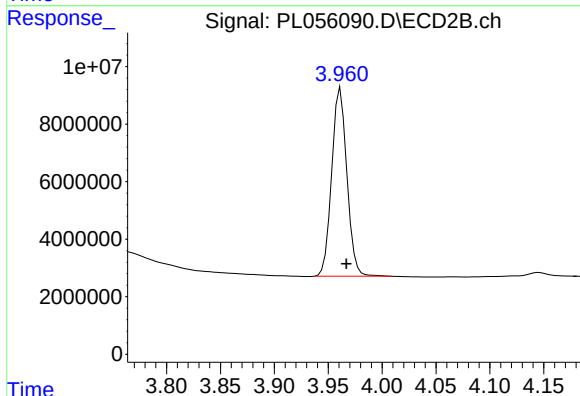


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.005 min
Response: 64196411
Conc: 22.71 ng/ml

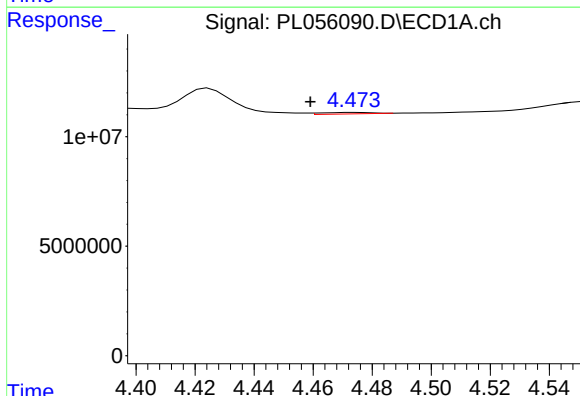


#6 beta-BHC

R.T.: 4.474 min
Delta R.T.: 0.015 min
Response: 765786
Conc: 0.12 ng/ml

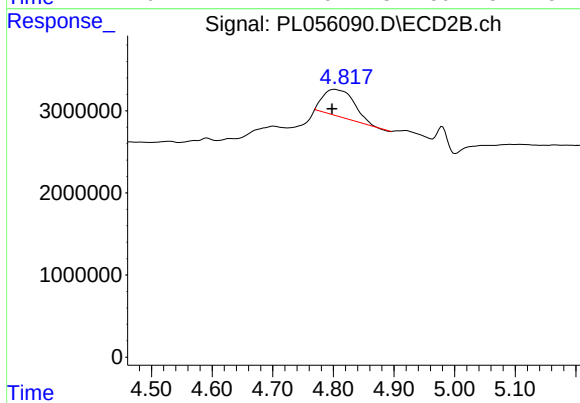

#6 beta-BHC


R.T.: 4.803 min
Delta R.T.: 0.005 min
Response: 11641999
Conc: 7.34 ng/ml

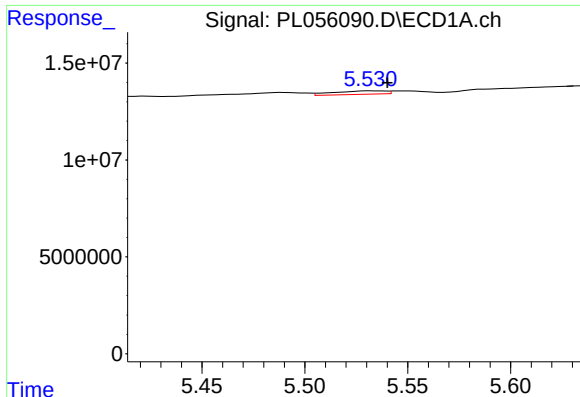

#9 Endosulfan I


R.T.: 5.533 min
Delta R.T.: -0.007 min
Response: 3143138
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

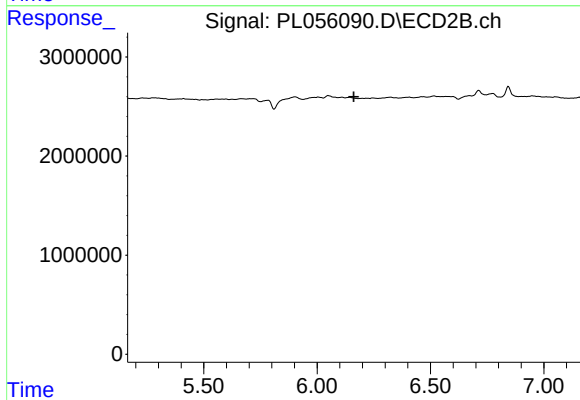


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

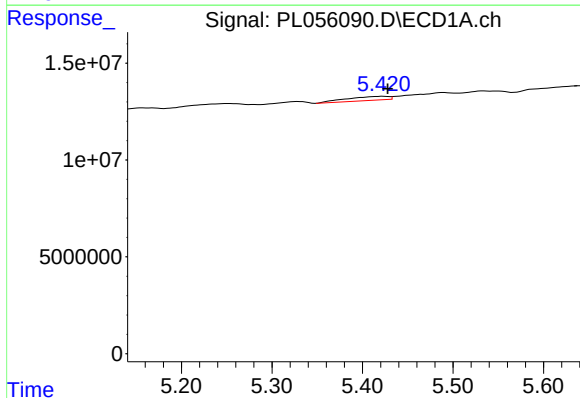


#10 gamma-Chlordane

R.T.: 5.422 min
Delta R.T.: -0.006 min
Response: 6599459
Conc: 0.47 ng/ml

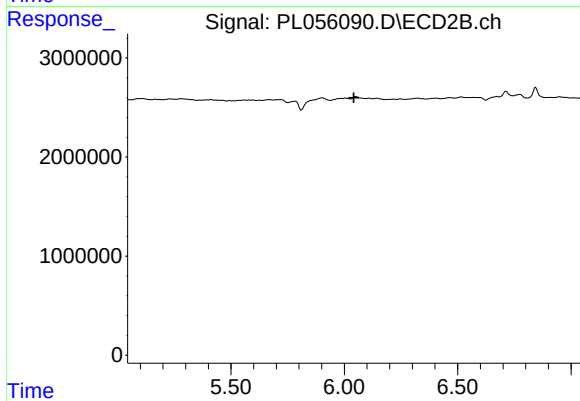

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

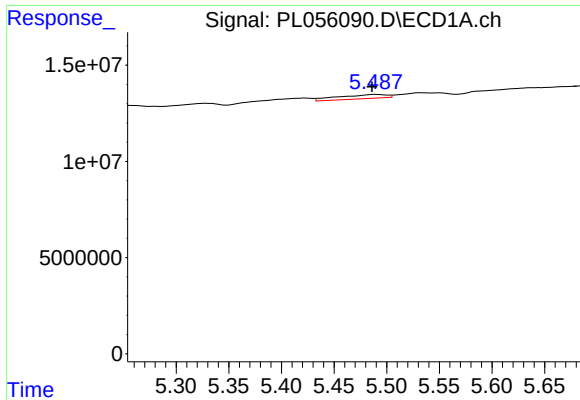

#11 alpha-Chlordane


R.T.: 5.489 min
Delta R.T.: 0.003 min
Response: 6887716
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

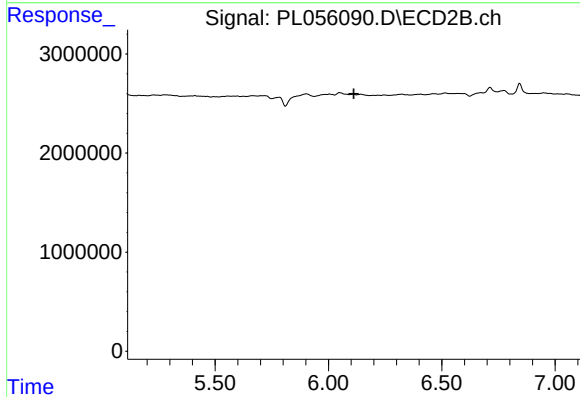


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

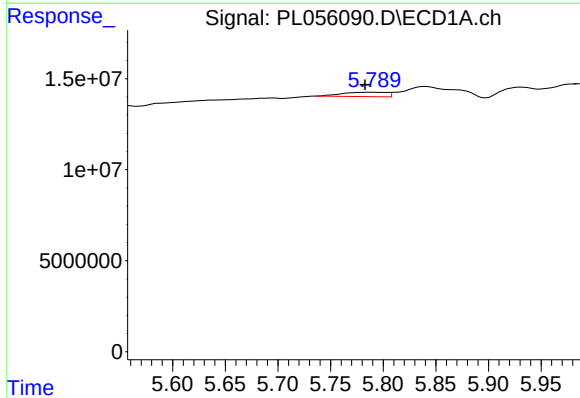


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: 0.007 min
Response: 7211924
Conc: 0.52 ng/ml

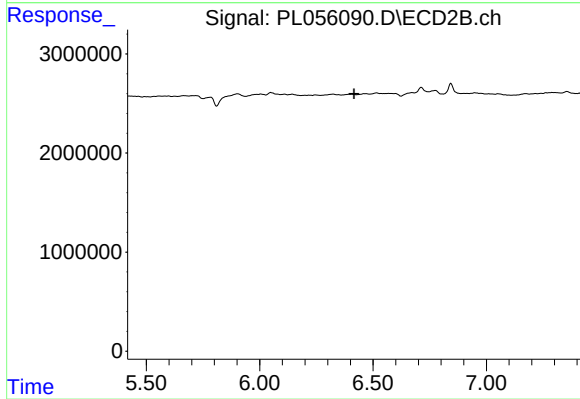

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

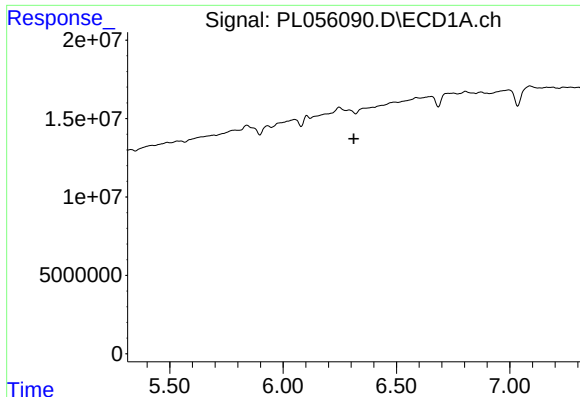

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.312 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

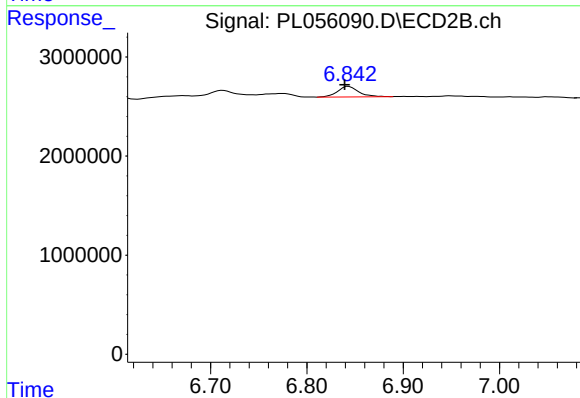


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.004 min
Response: 1591615
Conc: 0.59 ng/ml

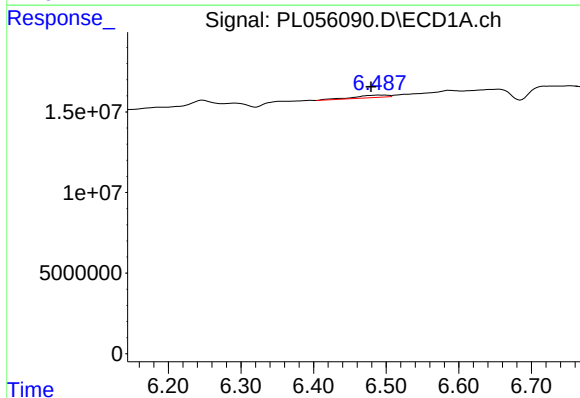


#18 Endrin aldehyde

R.T.: 6.490 min
Delta R.T.: 0.010 min
Response: 5000114
Conc: 0.48 ng/ml

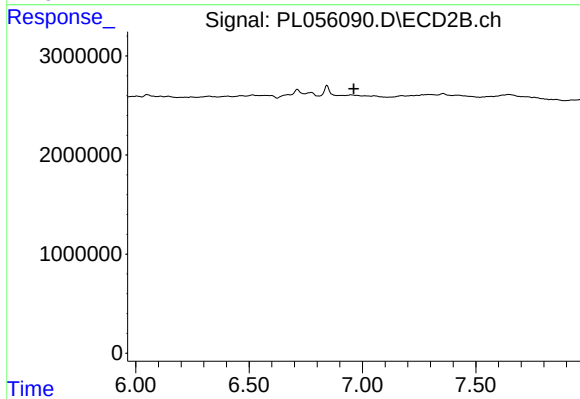

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.962 min
Response: 0
Conc: N.D.

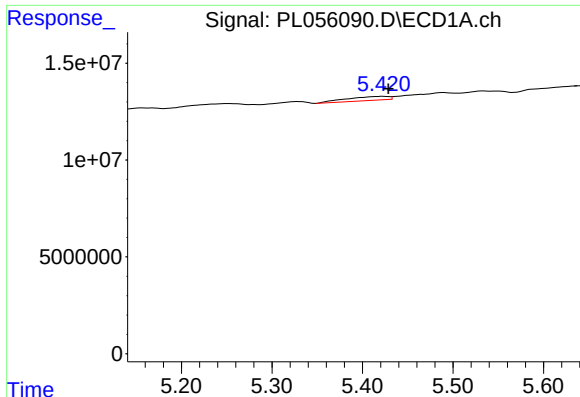

#25 Chlordane-3


R.T.: 5.422 min
Delta R.T.: -0.006 min
Response: 6599459
Conc: 5.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

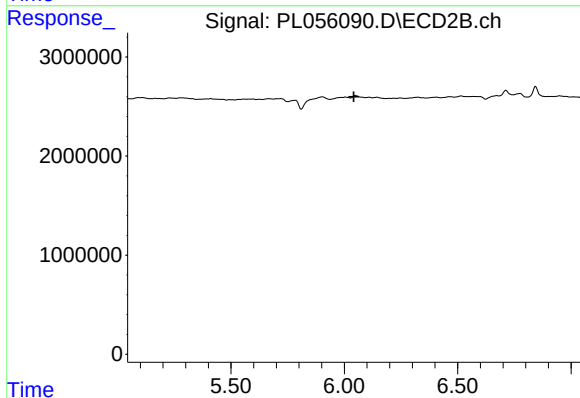


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

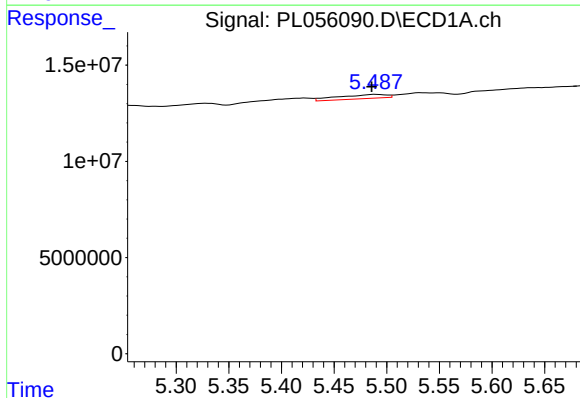


#26 Chlordane-4

R.T.: 5.489 min
Delta R.T.: 0.003 min
Response: 6887716
Conc: 6.68 ng/ml

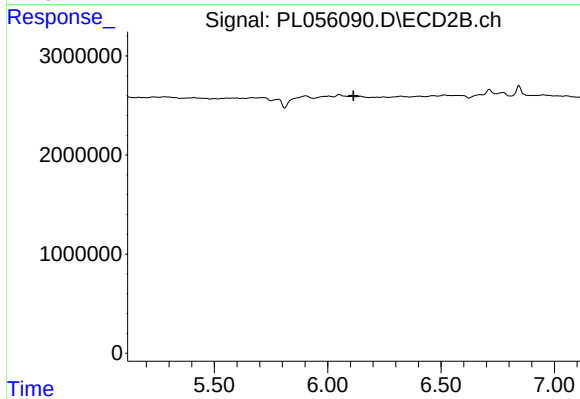

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

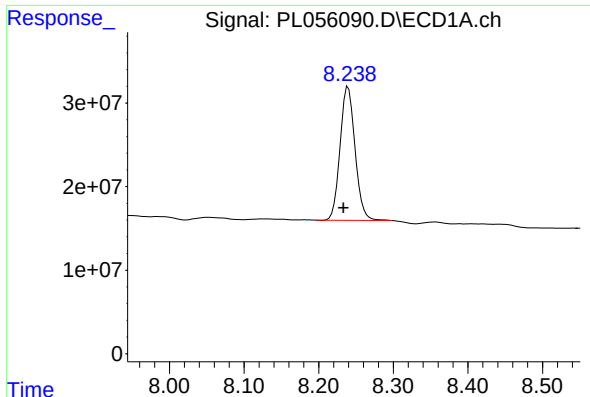

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.006 min
Response: 222787571
Conc: 21.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

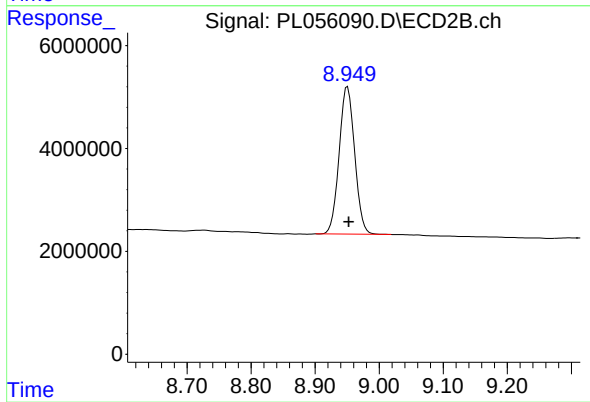

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.002 min
Response: 48198233
Conc: 21.04 ng/ml