

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
 Data File : PL056105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 21:02
 Operator : AJ\MA
 Sample : L1258-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 01:08:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.965	120.4E6	38638448	12.565	13.671
28)	SA Decachlor...	8.235	8.953	149.9E6	34082526	14.339	14.877
Target Compounds							
2)	A alpha-BHC	0.000	4.373f	0	6905711	N.D.	1.628 #
4)	MA Heptachlor	4.486f	0.000	2439009	0	0.163	N.D. #
6)	B beta-BHC	4.486f	0.000	2439009	0	0.380	N.D. #
9)	A Endosulfan I	5.524f	0.000	3051203	0	0.235	N.D. #
11)	B alpha-Chl...	5.480	0.000	10502711	0	0.760	N.D. #
12)	B 4,4'-DDE	5.649	6.266	9093376	2000282	0.696	0.683
18)	B Endrin al...	6.497f	0.000	4114778	0	0.396	N.D. #
26)	Chlordane-4	5.480	0.000	10502711	0	10.185	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
Data File : PL056105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 21:02
Operator : AJ\MA
Sample : L1258-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 01:08:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

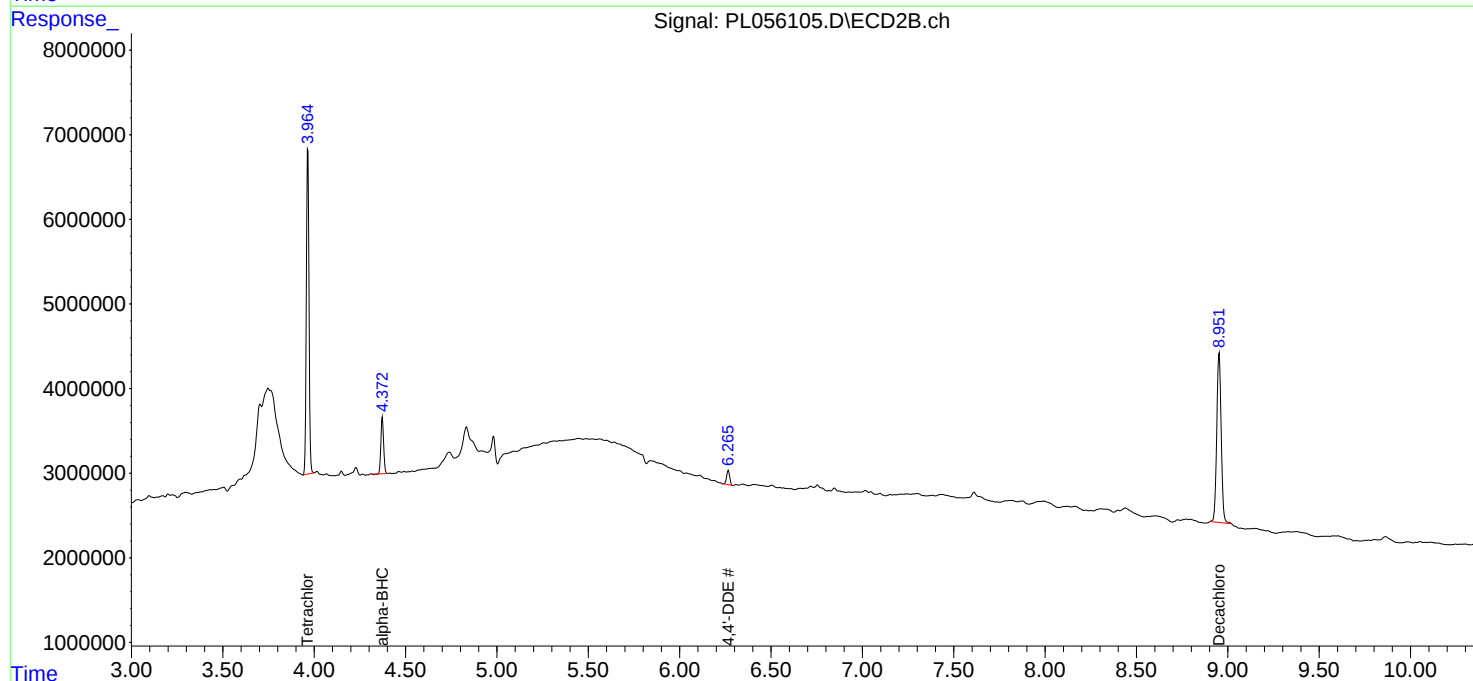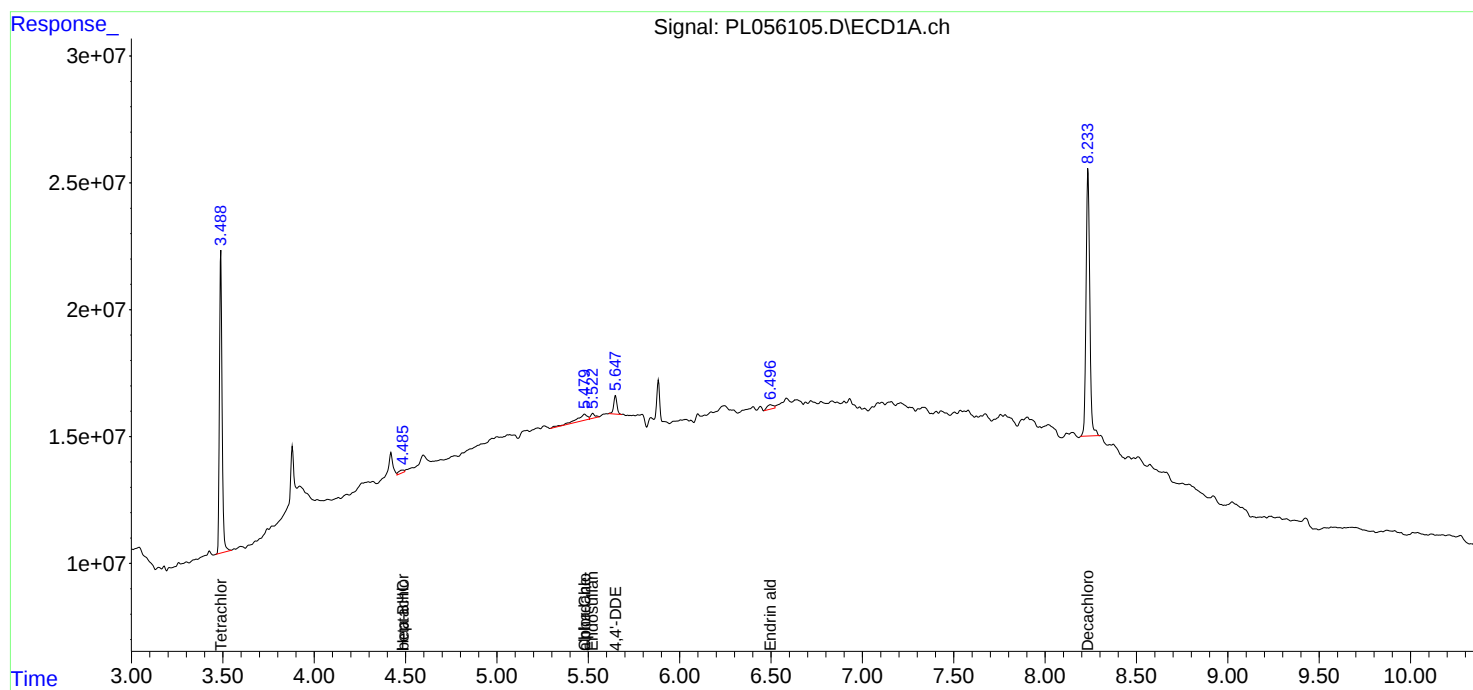


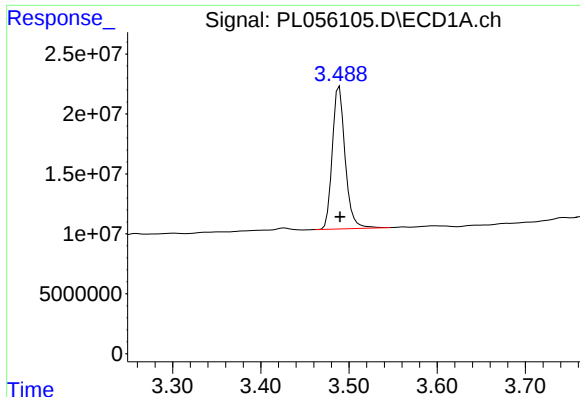

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.000 min
Response: 120432106
Conc: 12.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

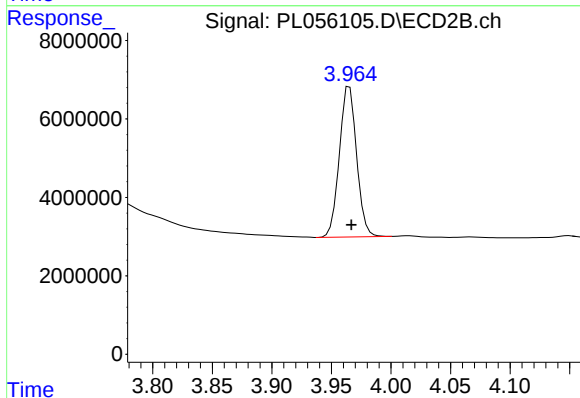


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.002 min
Response: 38638448
Conc: 13.67 ng/ml

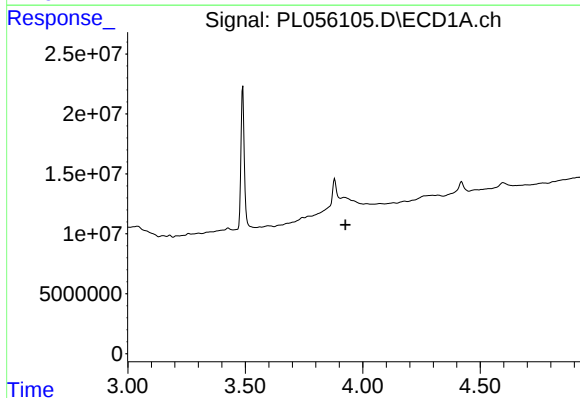


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.927 min
Response: 0
Conc: N.D.

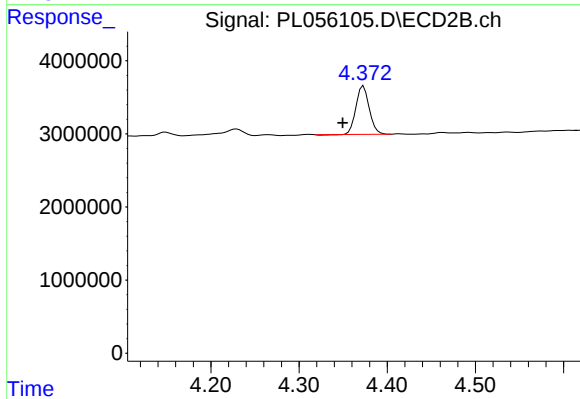

#2 alpha-BHC


R.T.: 4.373 min
Delta R.T.: 0.024 min
Response: 6905711
Conc: 1.63 ng/ml

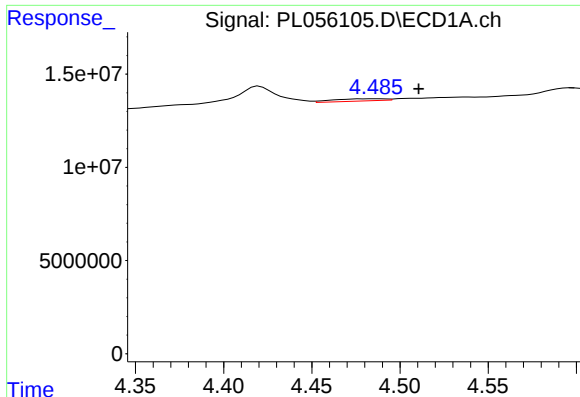

#4 Heptachlor


R.T.: 4.486 min
Delta R.T.: -0.024 min
Response: 2439009
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

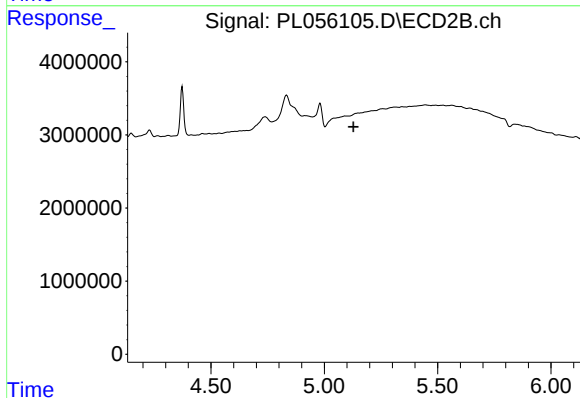


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

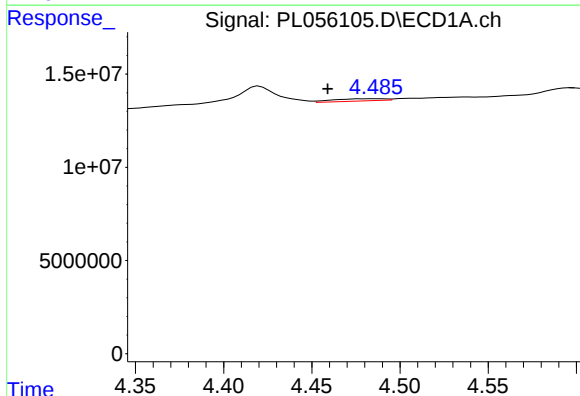


#6 beta-BHC

R.T.: 4.486 min
Delta R.T.: 0.027 min
Response: 2439009
Conc: 0.38 ng/ml

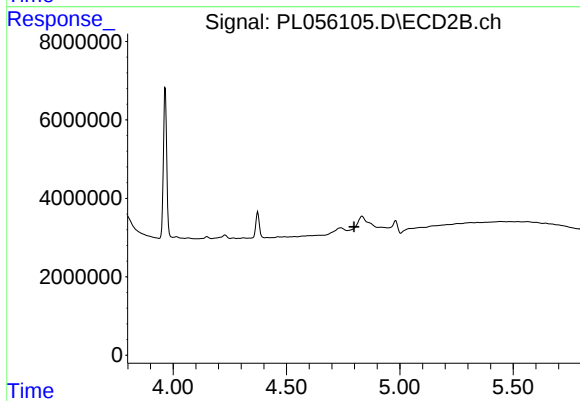

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

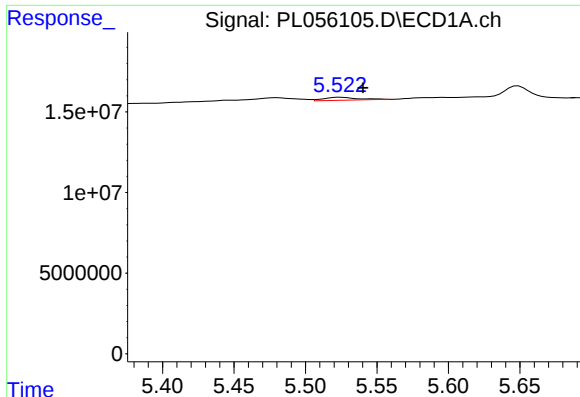

#9 Endosulfan I


R.T.: 5.524 min
Delta R.T.: -0.016 min
Response: 3051203
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

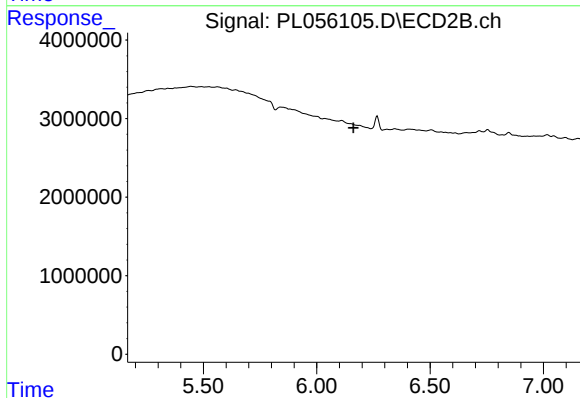


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

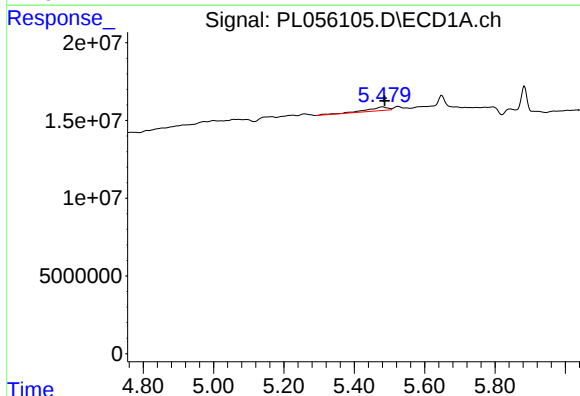


#11 alpha-Chlordane

R.T.: 5.480 min
Delta R.T.: -0.006 min
Response: 10502711
Conc: 0.76 ng/ml

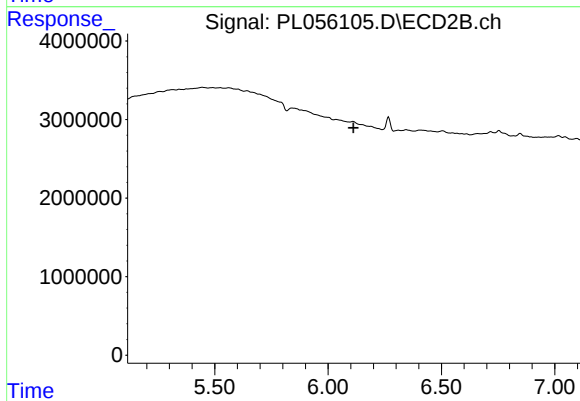

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

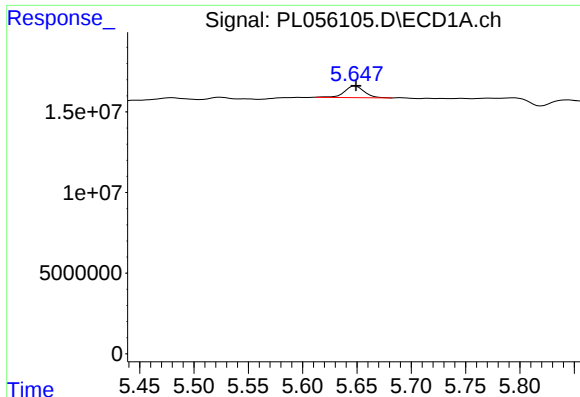

#12 4,4'-DDE


R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 9093376
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

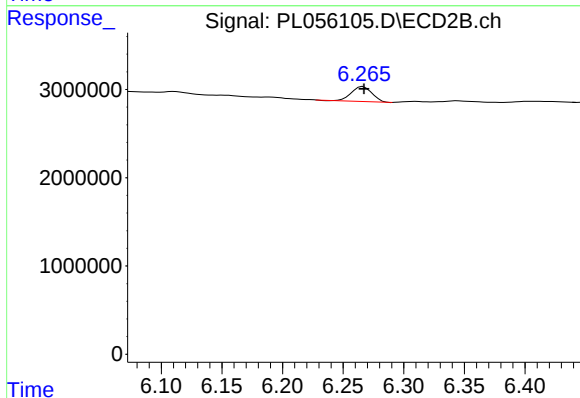


#12 4,4'-DDE

R.T.: 6.266 min
Delta R.T.: -0.001 min
Response: 2000282
Conc: 0.68 ng/ml

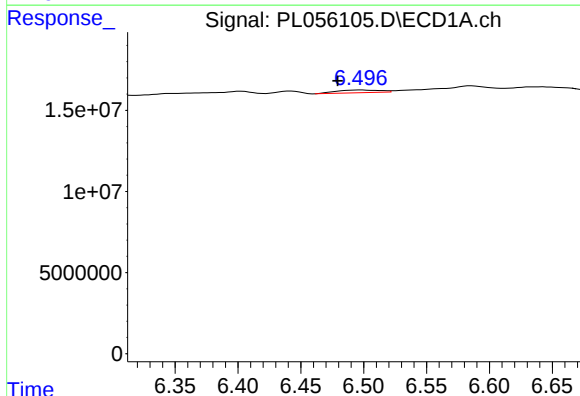


#18 Endrin aldehyde

R.T.: 6.497 min
Delta R.T.: 0.018 min
Response: 4114778
Conc: 0.40 ng/ml

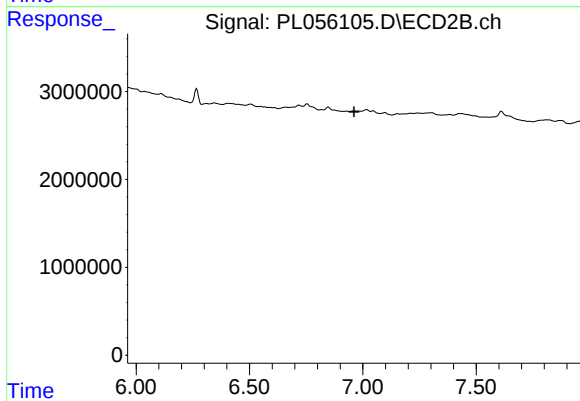

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.962 min
Response: 0
Conc: N.D.

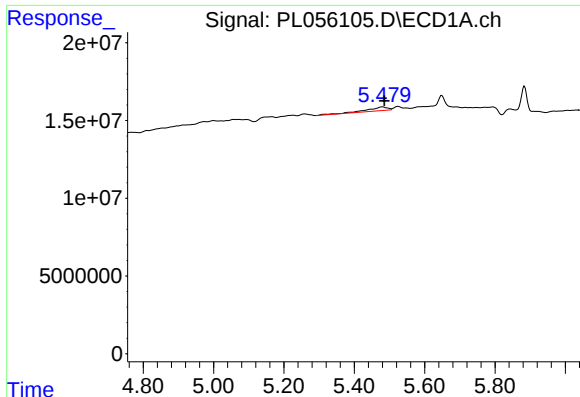

#26 Chlordane-4


R.T.: 5.480 min
Delta R.T.: -0.006 min
Response: 10502711
Conc: 10.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

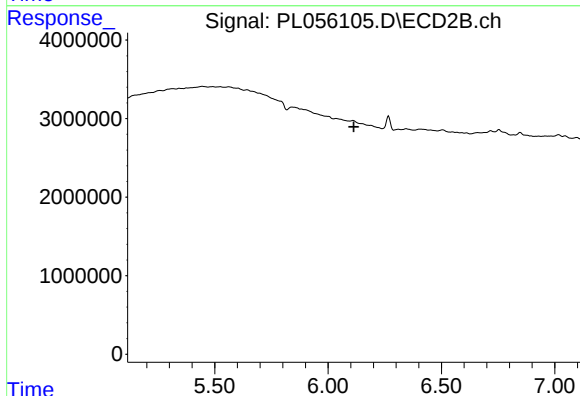


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

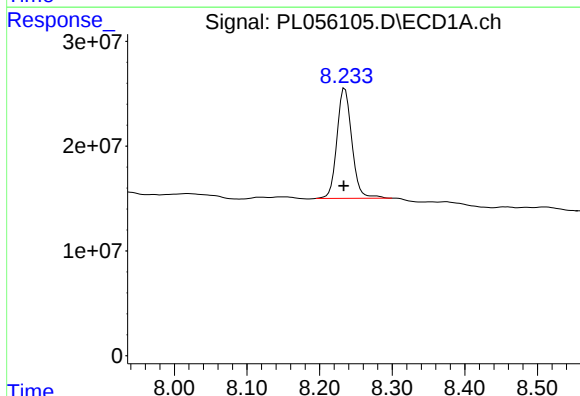

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.002 min
Response: 149923196
Conc: 14.34 ng/ml

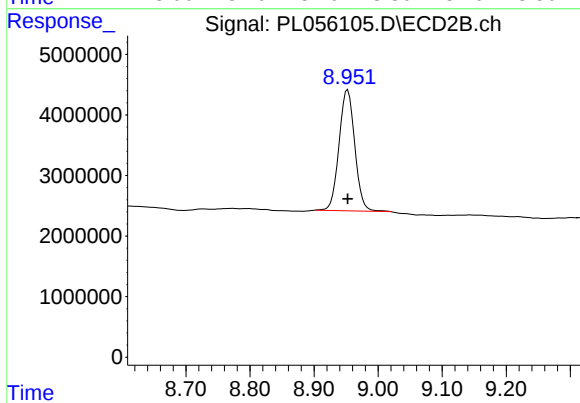

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.000 min
Response: 34082526
Conc: 14.88 ng/ml