

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
 Data File : PL056110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 22:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 01:10:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.966	215.5E6	67351641	22.486	23.831
28)	SA Decachlor...	8.235	8.952	221.1E6	49042532	21.146	21.407
Target Compounds							
2)	A alpha-BHC	3.925	0.000	11097696	0	0.669	N.D. #
4)	MA Heptachlor	4.539f	0.000	2788841	0	0.187	N.D. #
9)	A Endosulfan I	5.533	0.000	2487922	0	0.192	N.D. #
11)	B alpha-Chl...	5.479	0.000	14957057	0	1.082	N.D. #
18)	B Endrin al...	6.489	0.000	589379	0	0.057	N.D. #
23)	Chlordane-1	4.337f	0.000	1372856	0	3.744	N.D. #
24)	Chlordane-2	4.879f	0.000	14285128	0	33.010	N.D. #
26)	Chlordane-4	5.479	0.000	14957057	0	14.505	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012720\
Data File : PL056110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 22:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 01:10:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

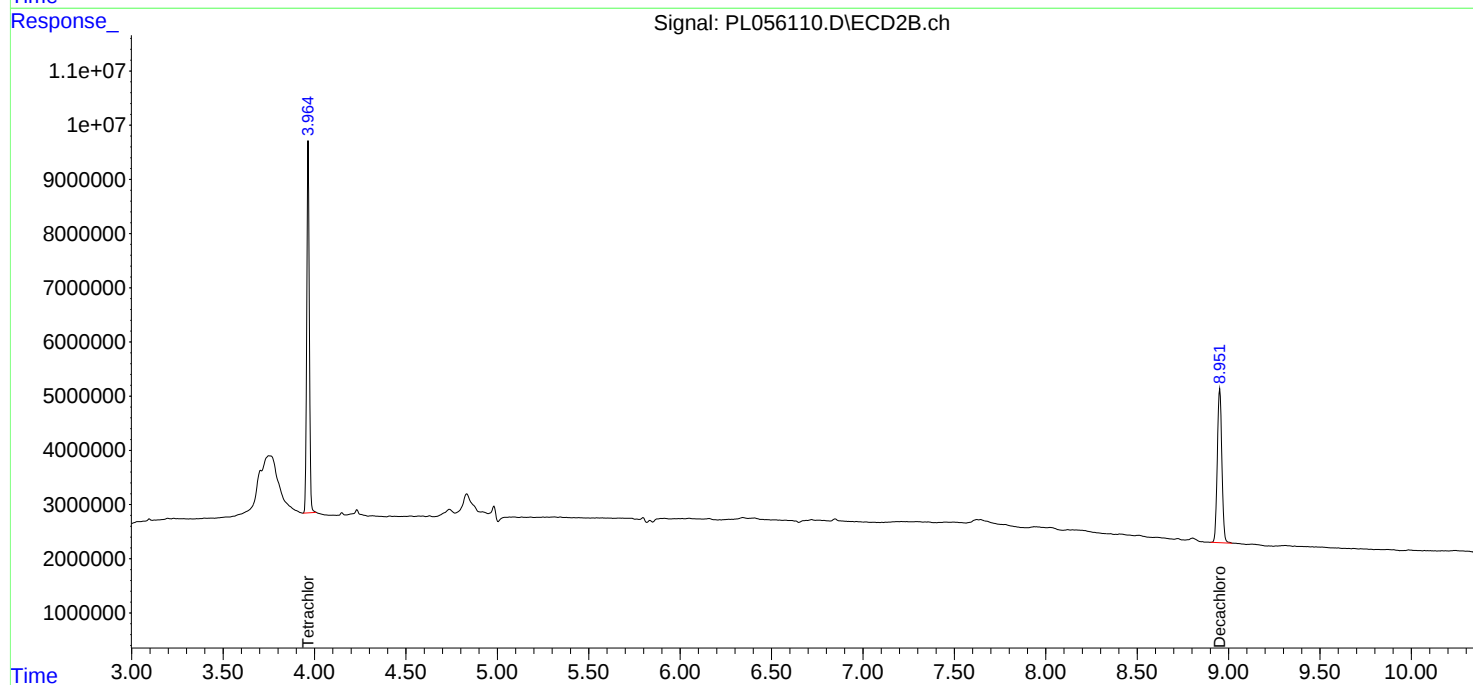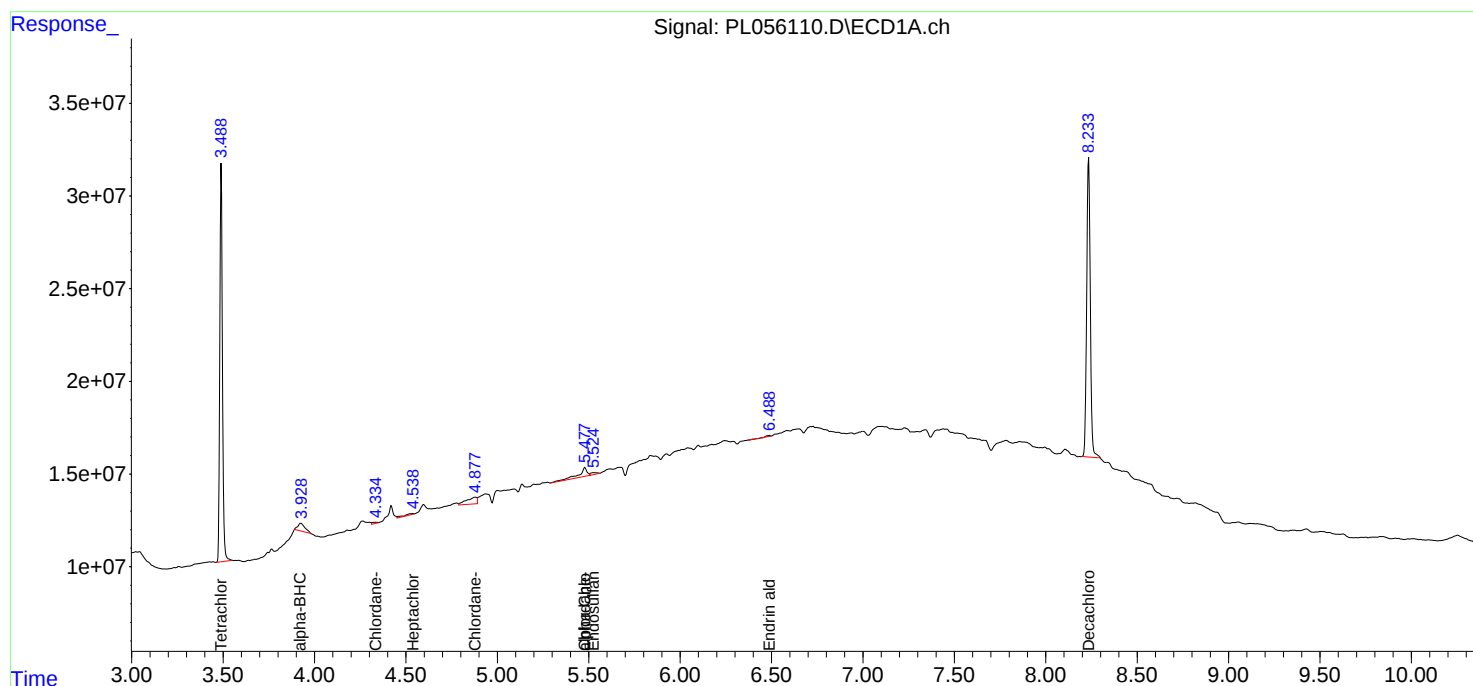


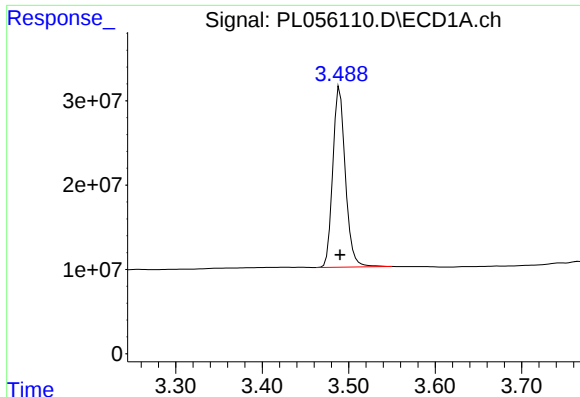

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 215516130
Conc: 22.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

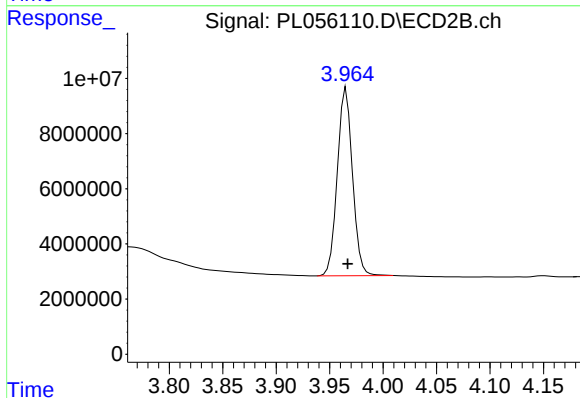


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: -0.001 min
Response: 67351641
Conc: 23.83 ng/ml

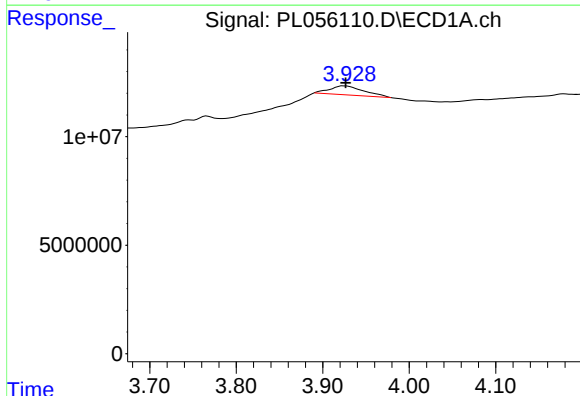


#2 alpha-BHC

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 11097696
Conc: 0.67 ng/ml

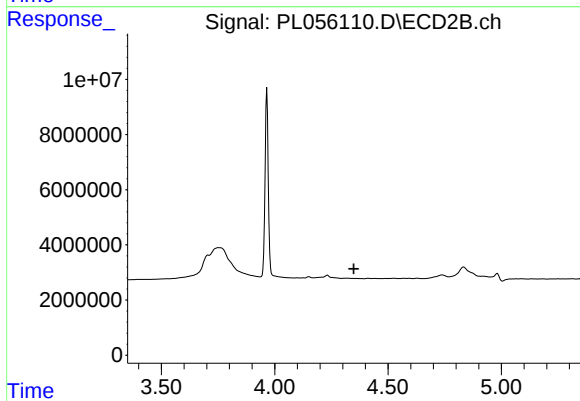

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

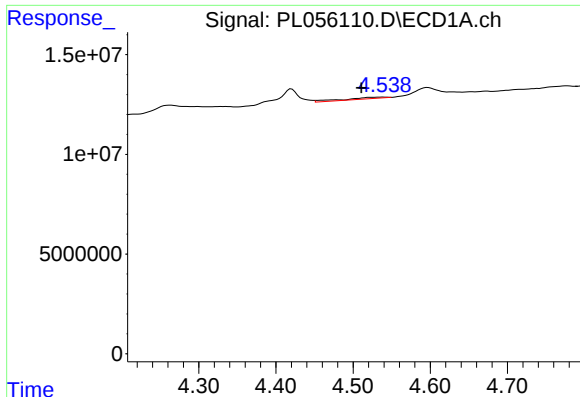

#4 Heptachlor


R.T.: 4.539 min
Delta R.T.: 0.028 min
Response: 2788841
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

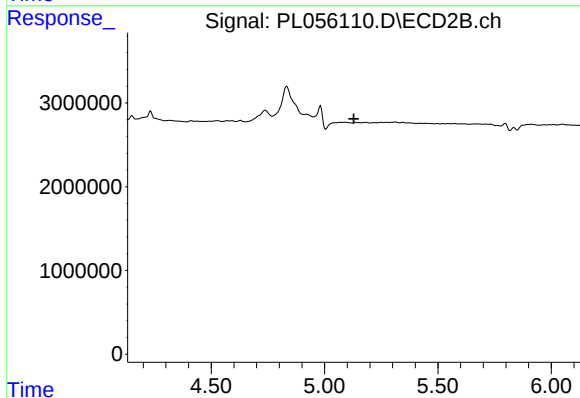


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

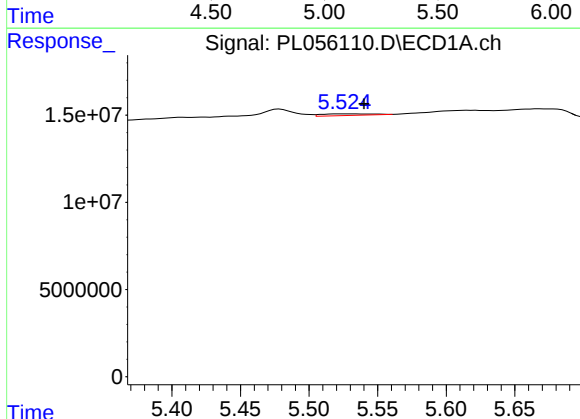


#9 Endosulfan I

R.T.: 5.533 min
Delta R.T.: -0.007 min
Response: 2487922
Conc: 0.19 ng/ml

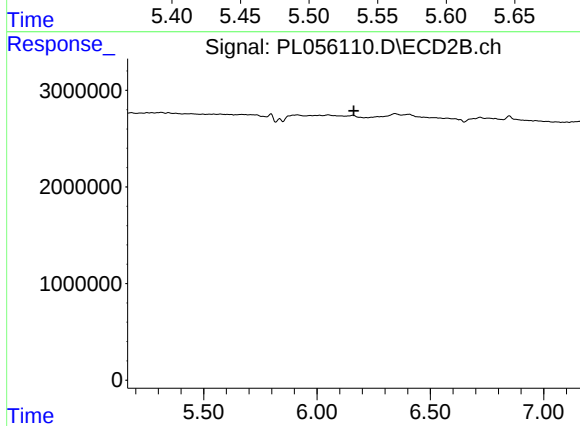

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

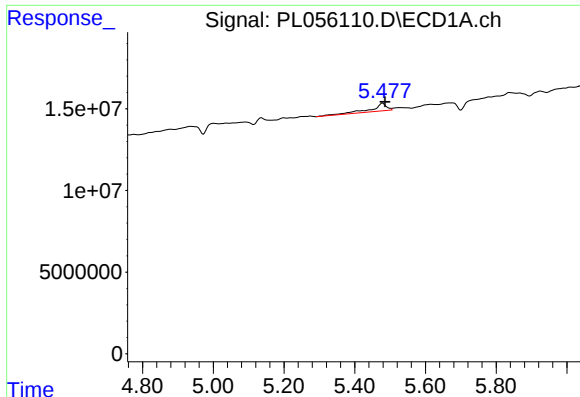

#11 alpha-Chlordane


R.T.: 5.479 min
Delta R.T.: -0.008 min
Response: 14957057
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

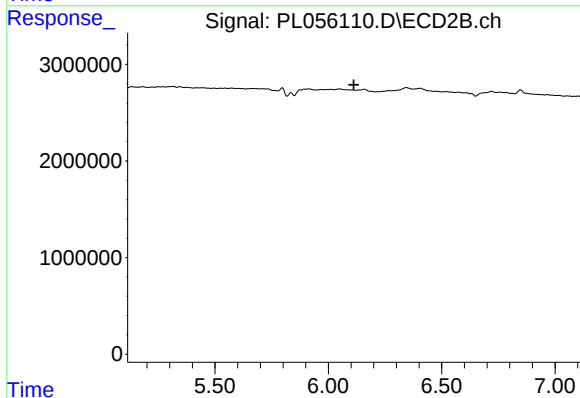


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

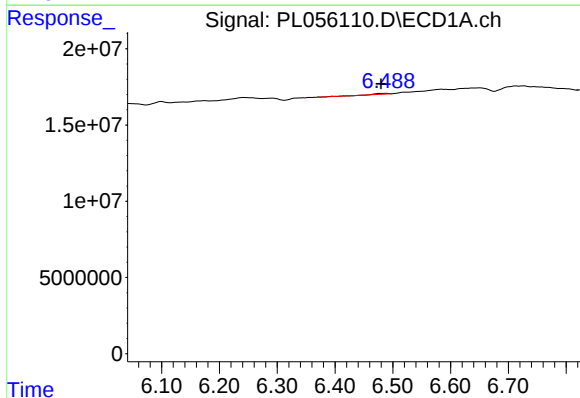


#18 Endrin aldehyde

R.T.: 6.489 min
Delta R.T.: 0.010 min
Response: 589379
Conc: 0.06 ng/ml

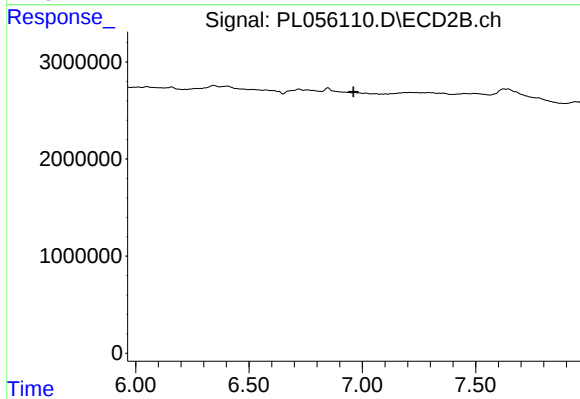

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

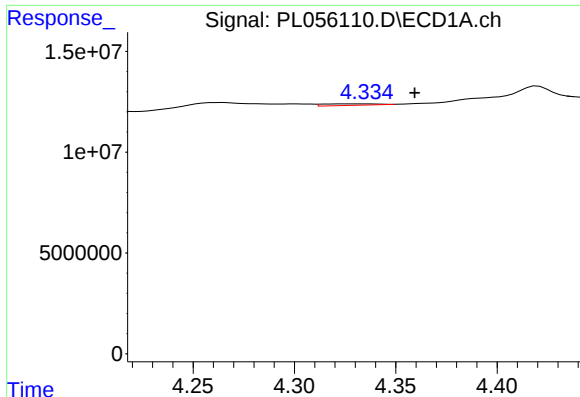

#23 Chlordane-1


R.T.: 4.337 min
Delta R.T.: -0.023 min
Response: 1372856
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

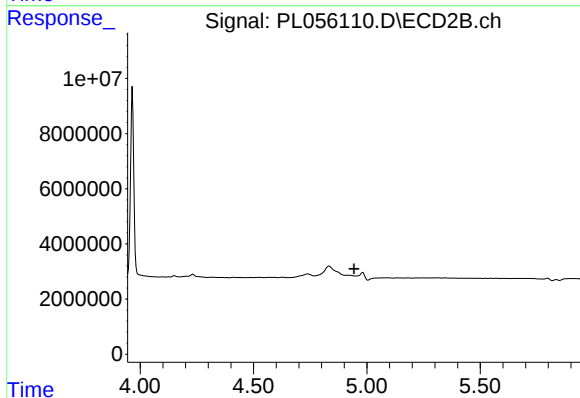


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

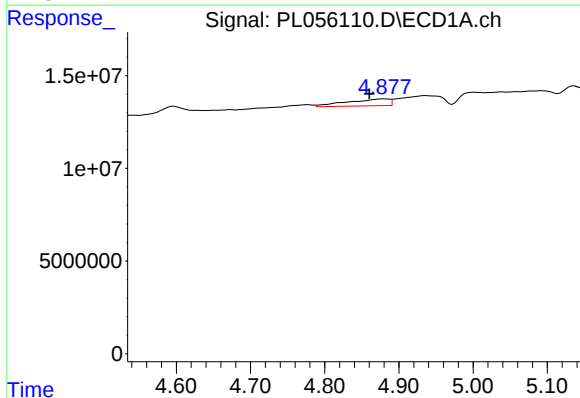


#24 Chlordane-2

R.T.: 4.879 min
Delta R.T.: 0.019 min
Response: 14285128
Conc: 33.01 ng/ml

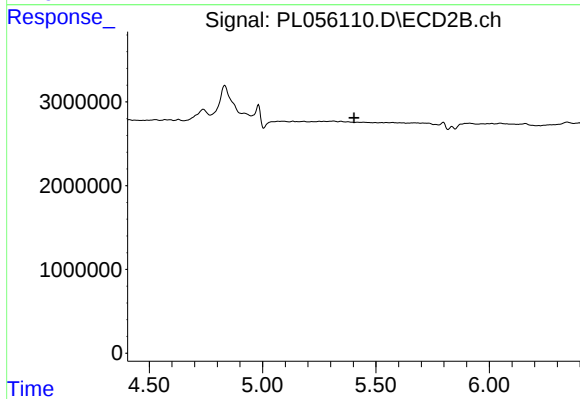

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

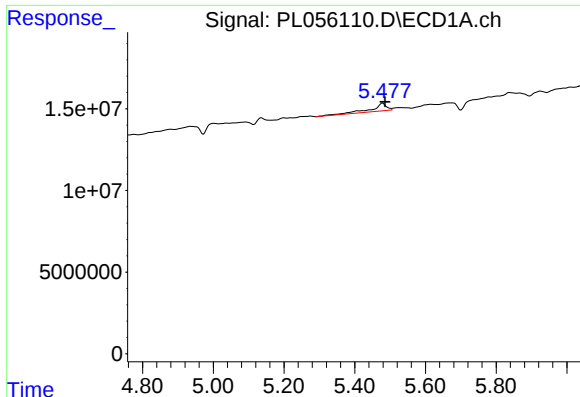

#26 Chlordane-4


R.T.: 5.479 min
Delta R.T.: -0.007 min
Response: 14957057
Conc: 14.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

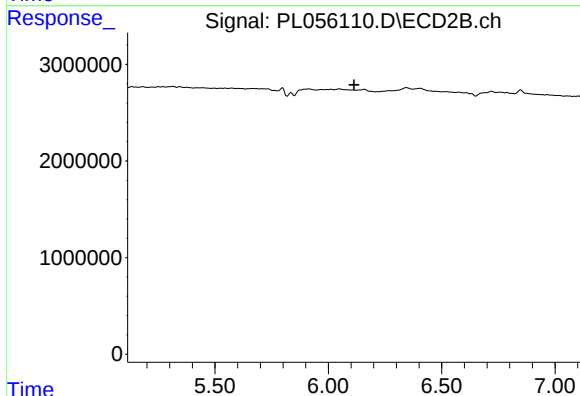


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

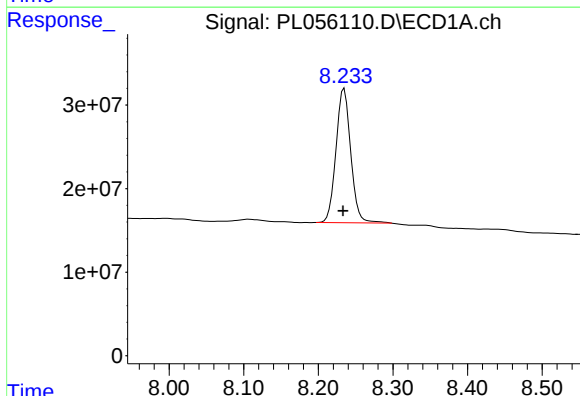

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.001 min
Response: 221097133
Conc: 21.15 ng/ml

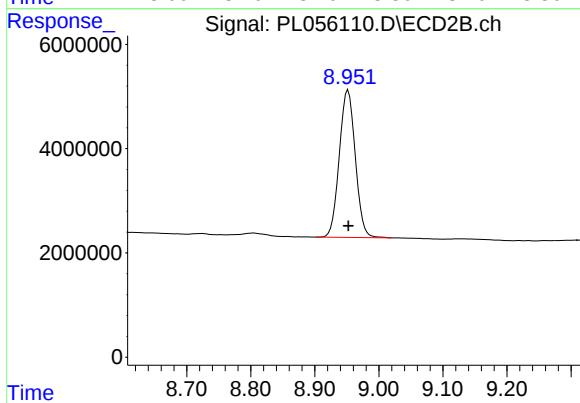

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 49042532
Conc: 21.41 ng/ml