

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012722\
 Data File : PL072287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2022 14:44
 Operator : AR\AJ
 Sample : N1280-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:10:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	6370217	18992029	11.474	11.694
28)	SA Decachlor...	10.316	11.384	11455601	23629480	12.894	14.645
Target Compounds							
2)	A alpha-BHC	0.000	6.106f	0	259534	N.D.	0.108 #
5)	MB Aldrin	0.000	7.487	0	114217	N.D.	0.052 #
7)	B delta-BHC	0.000	7.016f	0	355342	N.D.	0.144 #
15)	B Endosulfa...	0.000	9.126	0	455938	N.D.	0.266 #
16)	A 4,4'-DDD	0.000	9.037	0	168507	N.D.	0.118 #
18)	B Endrin al...	0.000	9.271	0	49996	N.D.	0.040 #
21)	B Endrin ke...	0.000	9.988	0	27071	N.D.	0.016 #
24)	Chlordane-2	0.000	7.487f	0	114217	N.D.	1.634 #
27)	Chlordane-5	0.000	9.177f	0	30354	N.D.	0.497 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012722\
Data File : PL072287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2022 14:44
Operator : AR\AJ
Sample : N1280-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:10:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

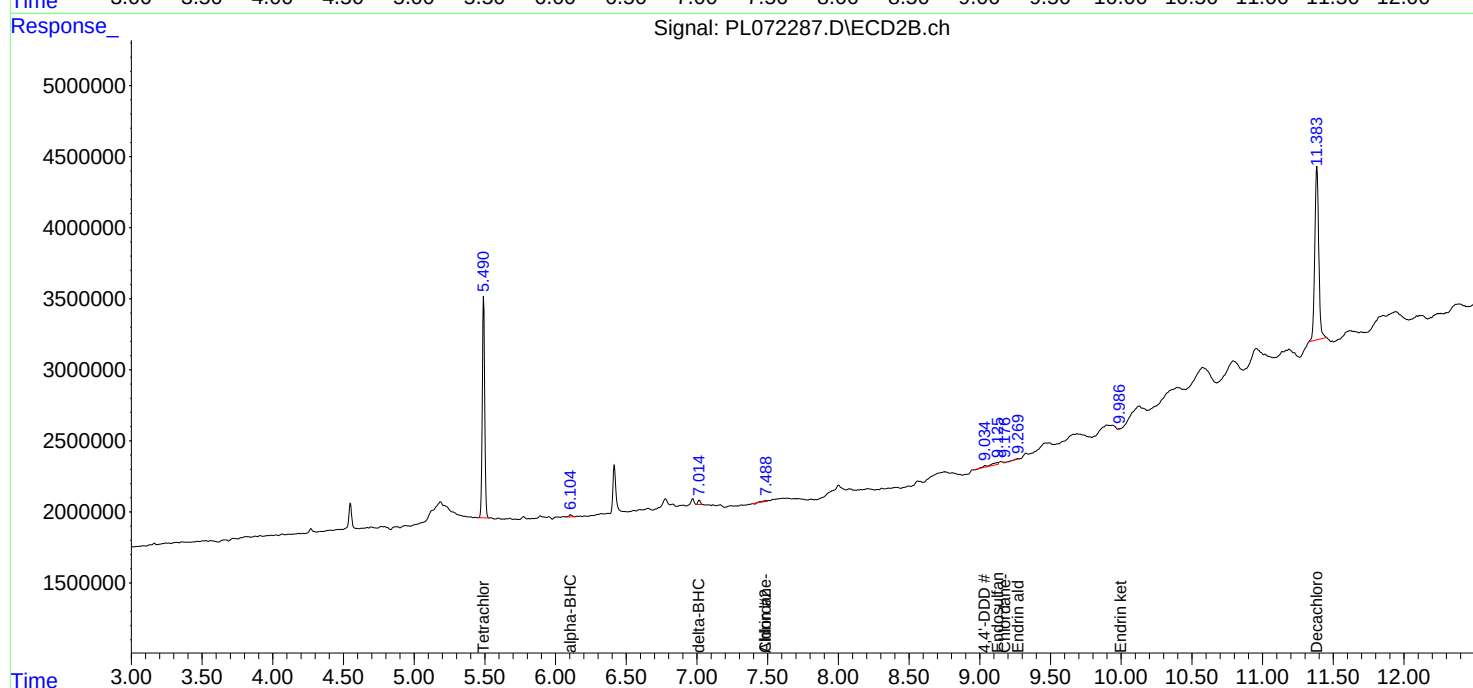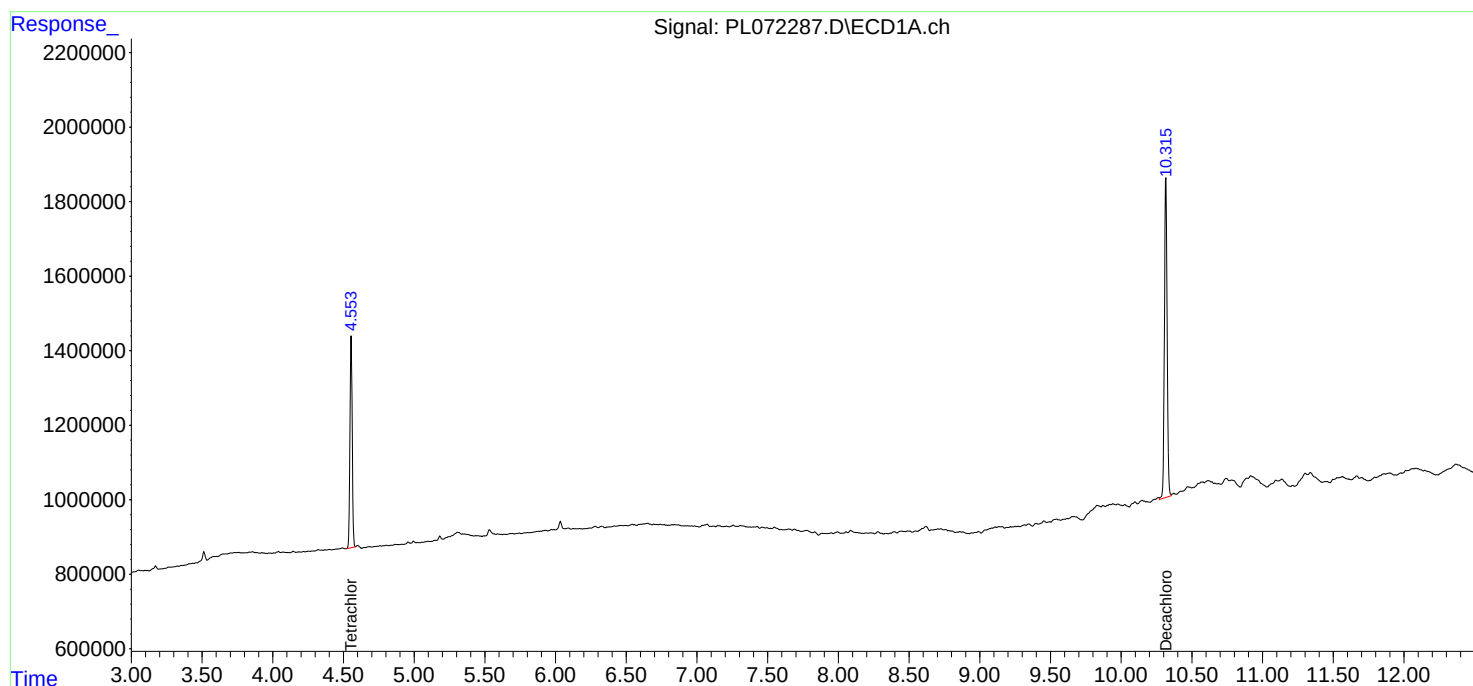


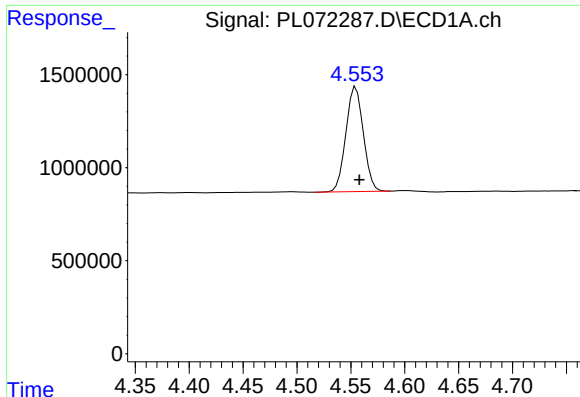

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 6370217
Conc: 11.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

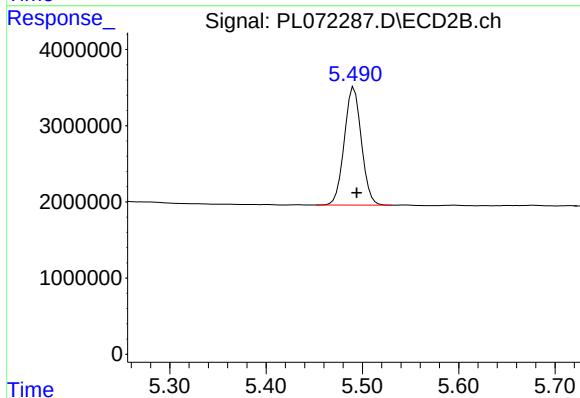


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 18992029
Conc: 11.69 ng/ml

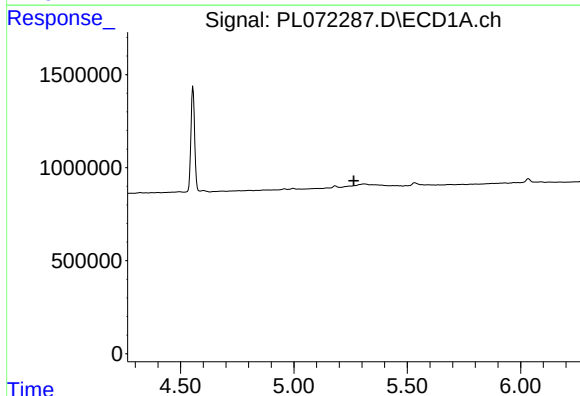


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

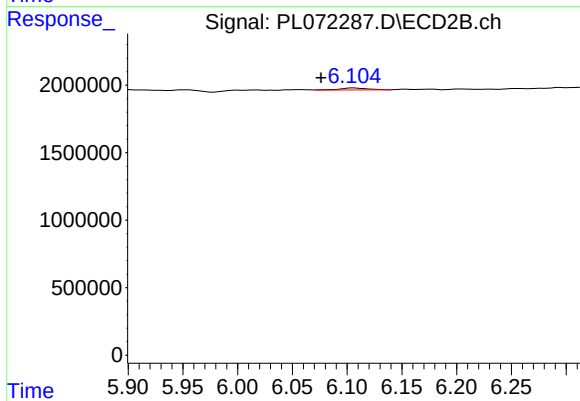

#2 alpha-BHC


R.T.: 6.106 min
Delta R.T.: 0.030 min
Response: 259534
Conc: 0.11 ng/ml

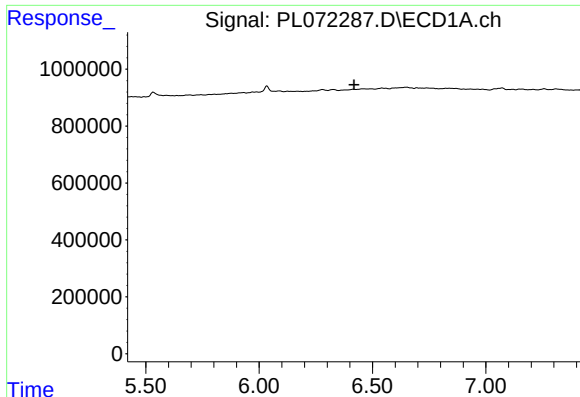

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

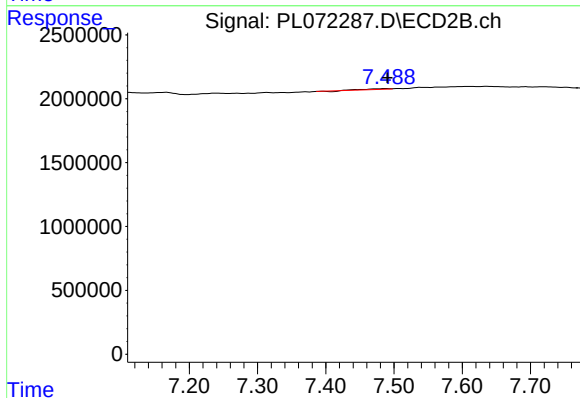


#5 Aldrin

R.T.: 7.487 min
Delta R.T.: -0.003 min
Response: 114217
Conc: 0.05 ng/ml

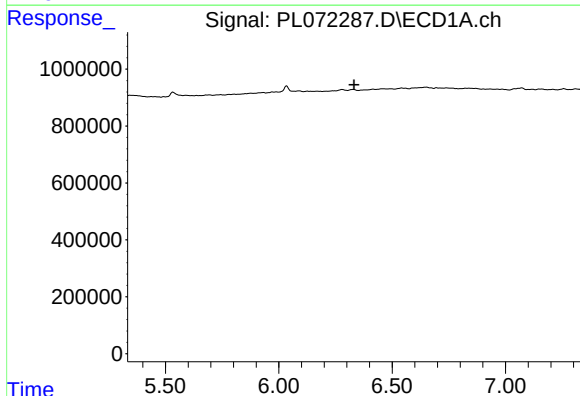


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

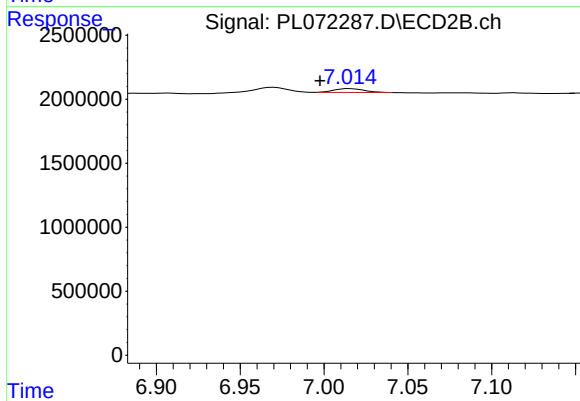

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.018 min
Response: 355342
Conc: 0.14 ng/ml

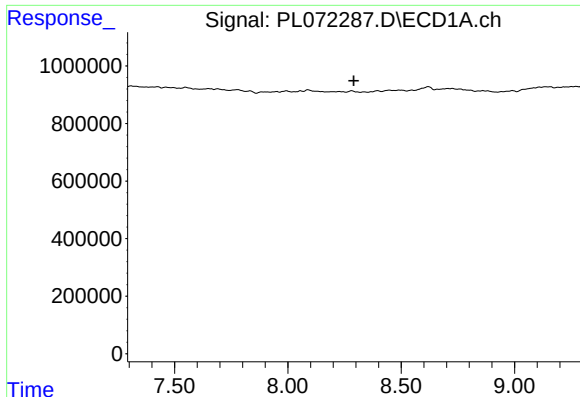

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

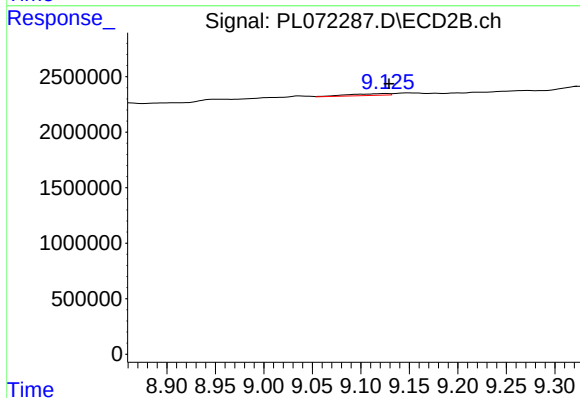


#15 Endosulfan II

R.T.: 9.126 min
Delta R.T.: -0.003 min
Response: 455938
Conc: 0.27 ng/ml

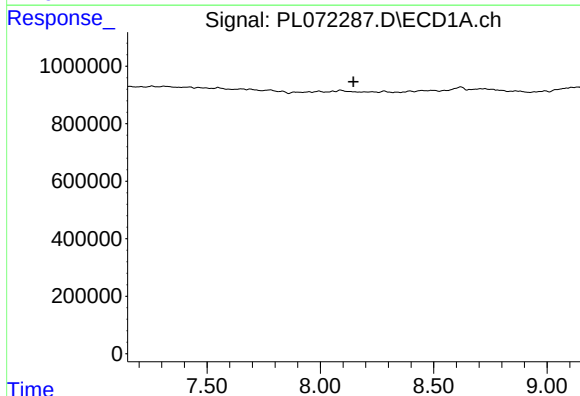


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

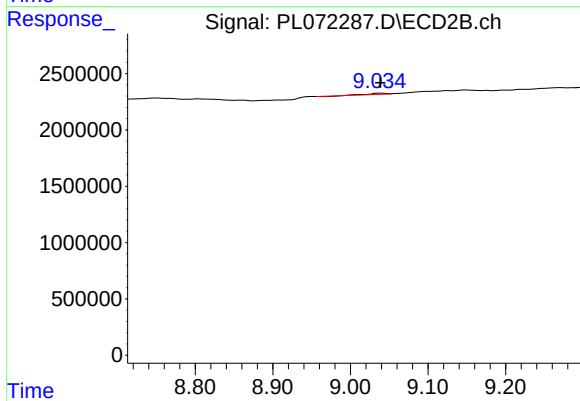

#16 4,4'-DDD


R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 168507
Conc: 0.12 ng/ml

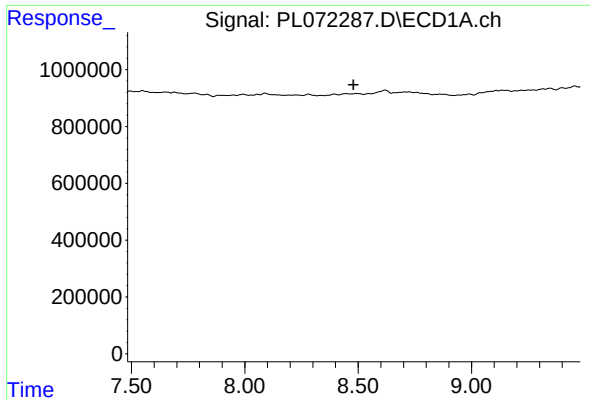

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

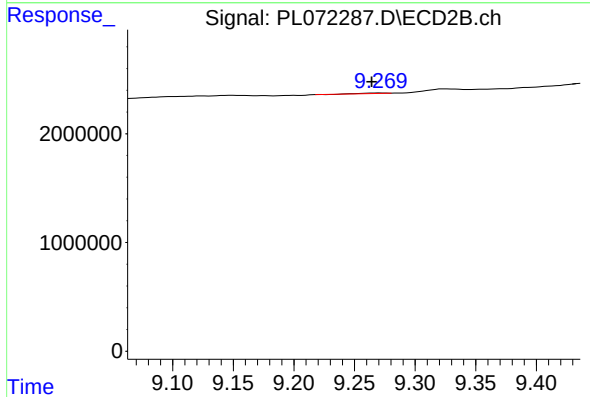


#18 Endrin aldehyde

R.T.: 9.271 min
Delta R.T.: 0.007 min
Response: 49996
Conc: 0.04 ng/ml

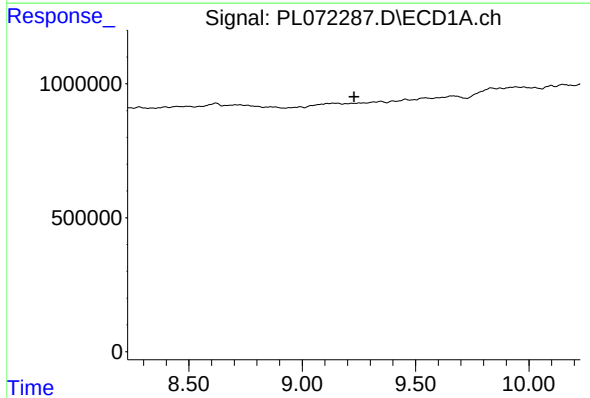


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.229 min
Response: 0
Conc: N.D.

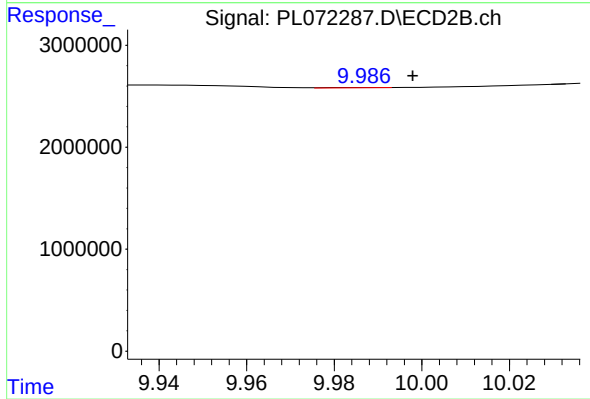

#21 Endrin ketone


R.T.: 9.988 min
Delta R.T.: -0.010 min
Response: 27071
Conc: 0.02 ng/ml

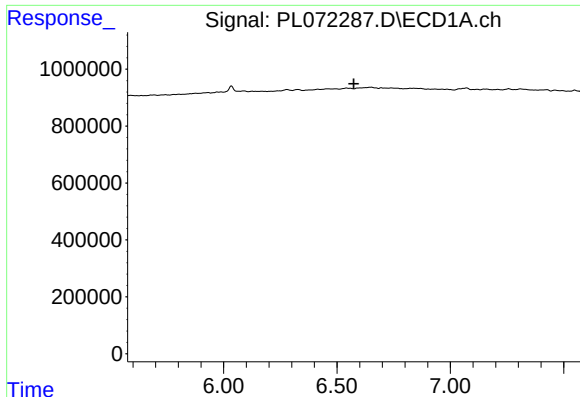

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

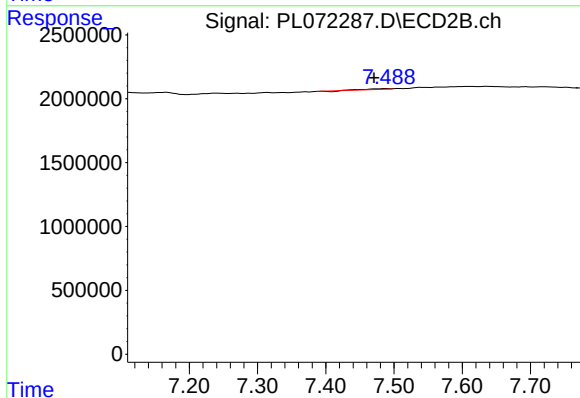


#24 Chlordane-2

R.T.: 7.487 min
Delta R.T.: 0.017 min
Response: 114217
Conc: 1.63 ng/ml

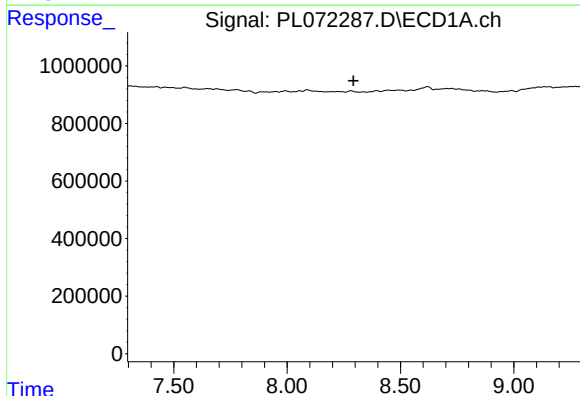


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

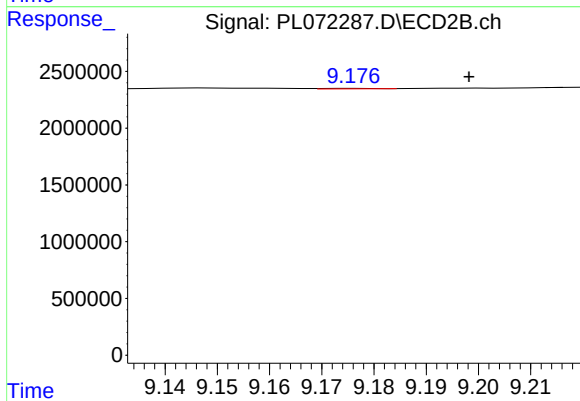

#27 Chlordane-5

R.T.: 9.177 min
Delta R.T.: -0.021 min
Response: 30354
Conc: 0.50 ng/ml

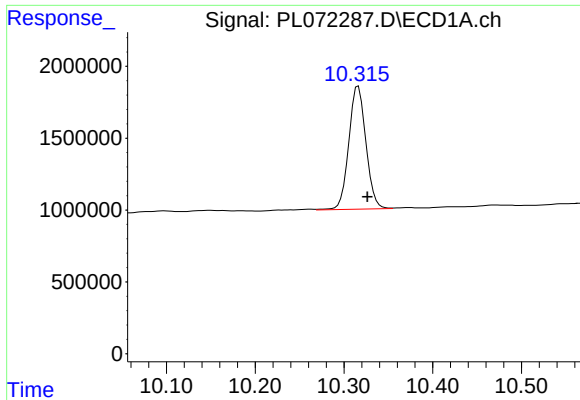

#28 Decachlorobiphenyl


R.T.: 10.316 min

Delta R.T.: -0.010 min

Response: 11455601

Conc: 12.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

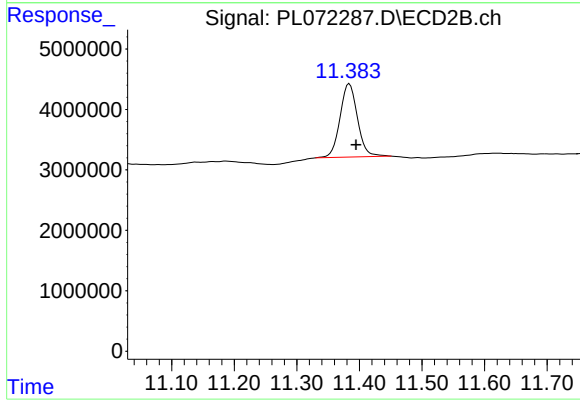

#28 Decachlorobiphenyl

R.T.: 11.384 min

Delta R.T.: -0.011 min

Response: 23629480

Conc: 14.64 ng/ml