

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012722\
 Data File : PL072290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2022 15:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:11:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.491	10810345	32264317	19.472	19.866
28)	SA Decachlor...	10.316	11.384	16894180	30789541	19.016	19.082
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	645286	N.D.	0.262 #
8)	B Heptachlo...	0.000	7.962	0	1496683	N.D.	0.747 #
9)	A Endosulfan I	0.000	8.354	0	1293448	N.D.	0.715 #
10)	B gamma-Chl...	0.000	8.224	0	1772842	N.D.	0.877 #
14)	MA Endrin	7.998f	0.000	410541	0	0.586	N.D. #
15)	B Endosulfa...	0.000	9.147f	0	437693	N.D.	0.255 #
16)	A 4,4'-DDD	0.000	9.062f	0	215836	N.D.	0.151 #
18)	B Endrin al...	0.000	9.287f	0	73523	N.D.	0.059 #
19)	B Endosulfa...	0.000	9.497	0	42725	N.D.	0.027 #
22)	Mirex	0.000	10.450	0	93144	N.D.	0.075 #
25)	Chlordane-3	0.000	8.224	0	1772842	N.D.	6.381 #
27)	Chlordane-5	0.000	9.195	0	21662	N.D.	0.355 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012722\
Data File : PL072290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2022 15:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:11:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

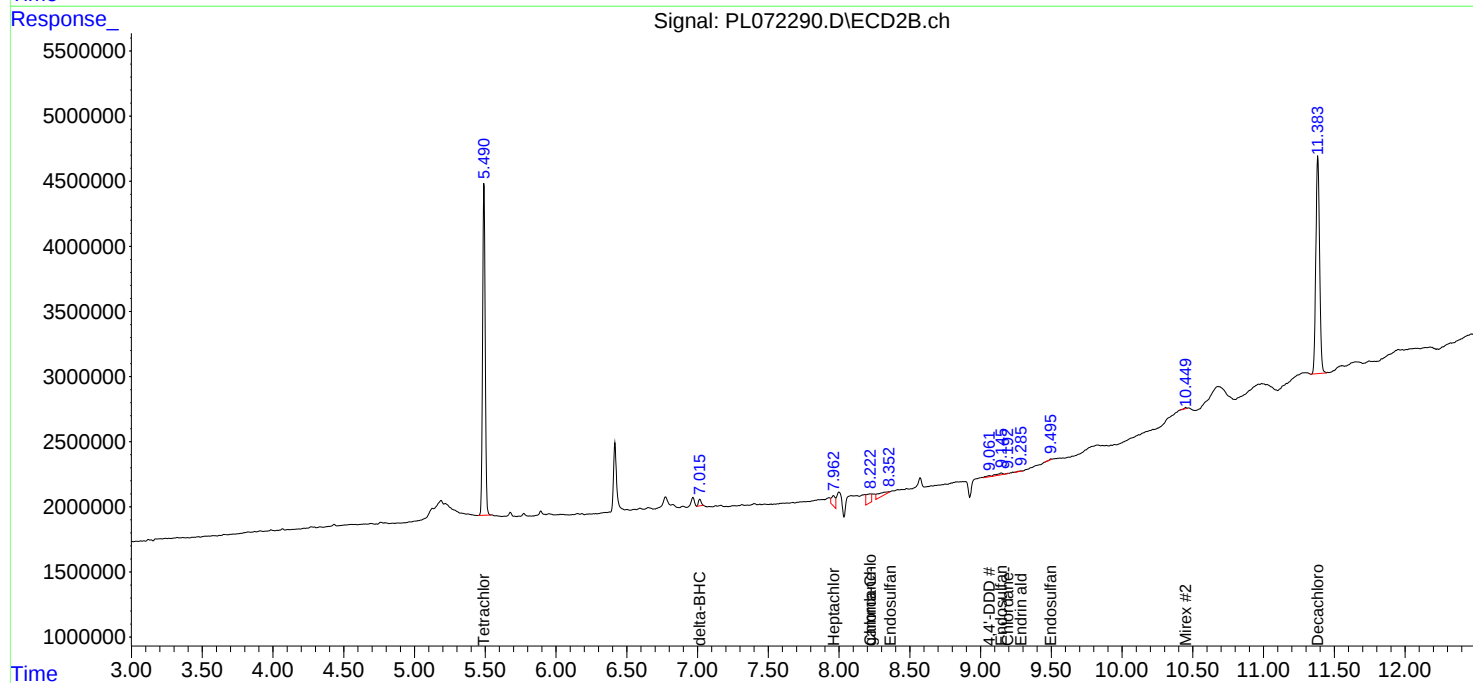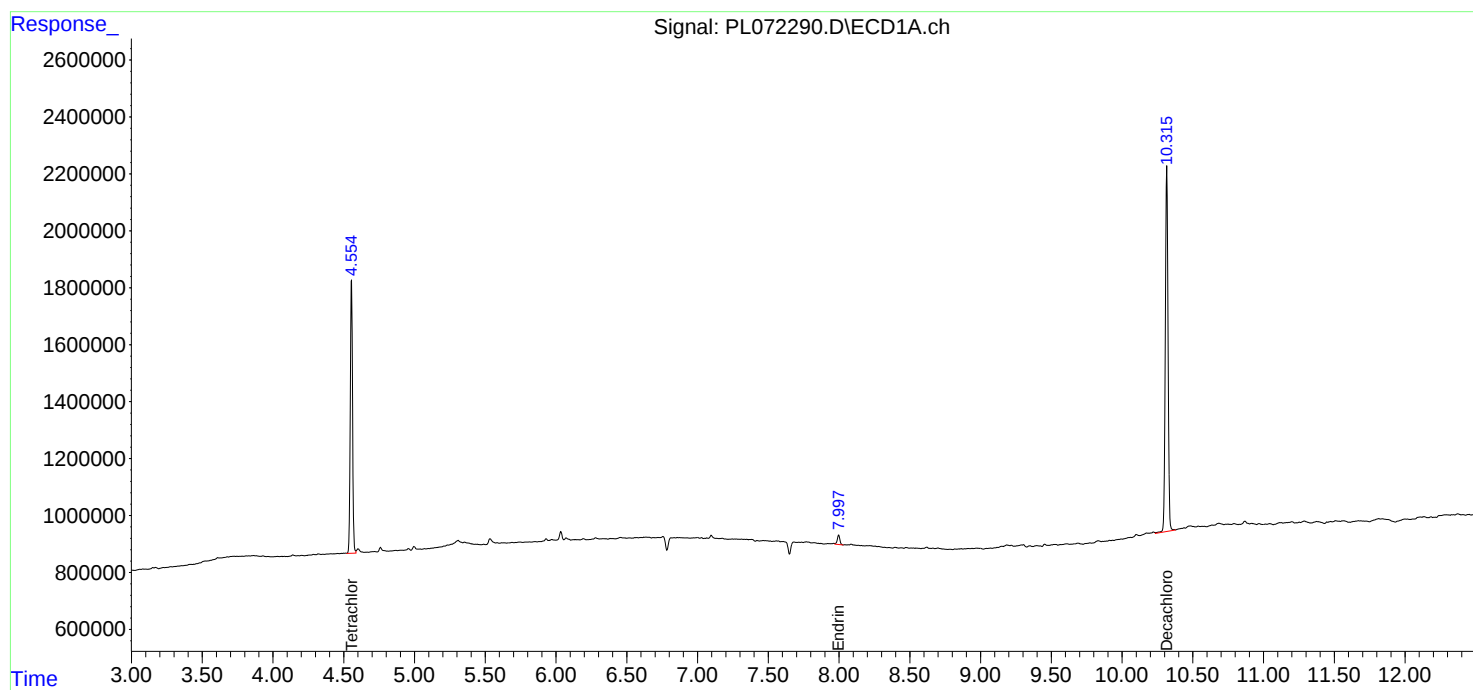


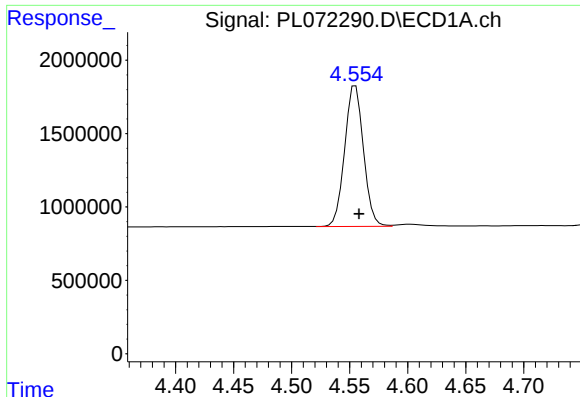

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 10810345
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

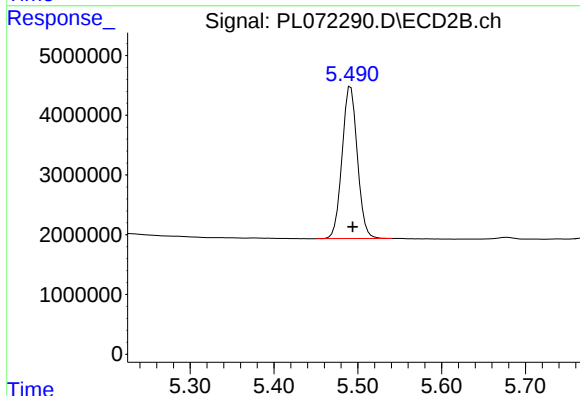


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 32264317
Conc: 19.87 ng/ml

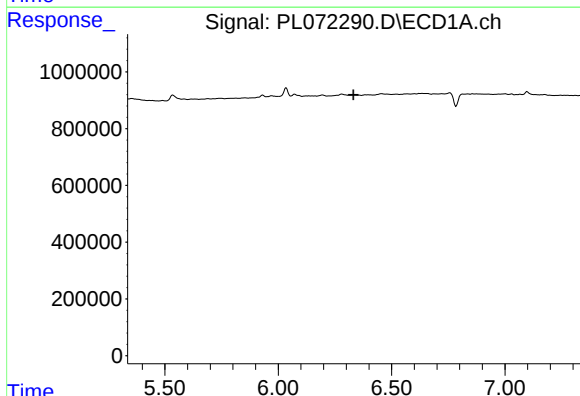


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

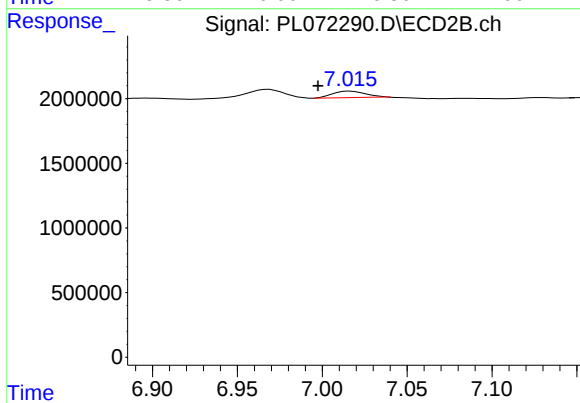

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.019 min
Response: 645286
Conc: 0.26 ng/ml

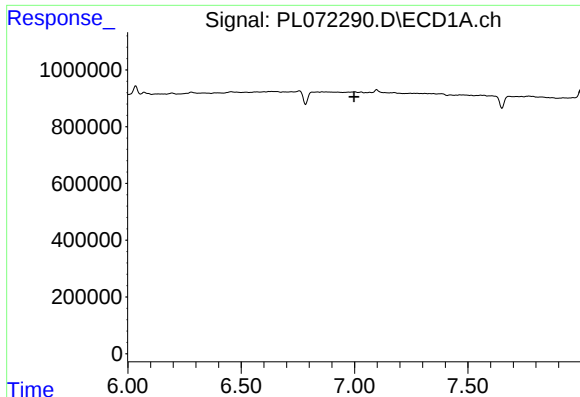

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

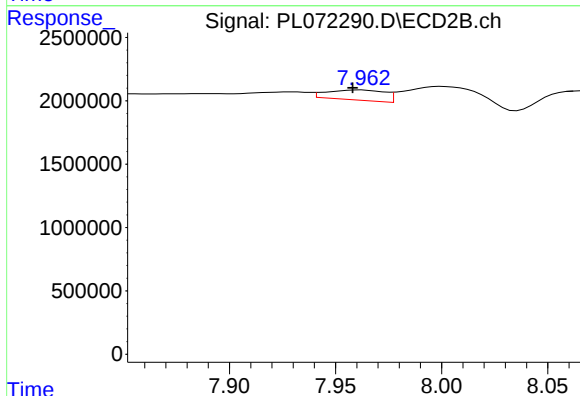


#8 Heptachlor epoxide

R.T.: 7.962 min
Delta R.T.: 0.004 min
Response: 1496683
Conc: 0.75 ng/ml

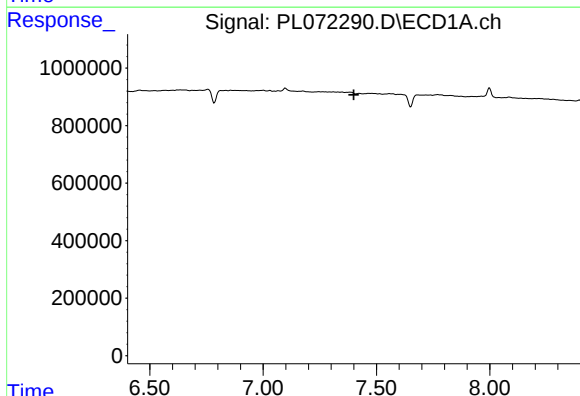


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

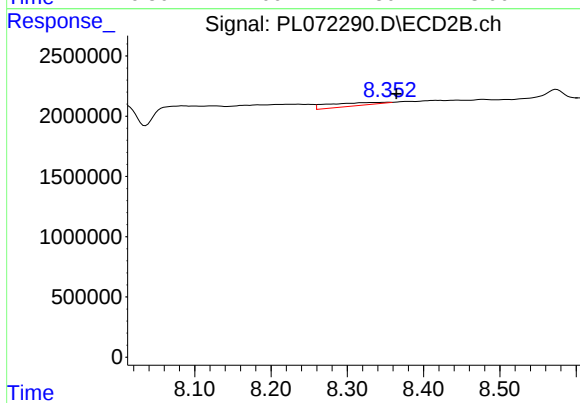

#9 Endosulfan I


R.T.: 8.354 min
Delta R.T.: -0.010 min
Response: 1293448
Conc: 0.71 ng/ml

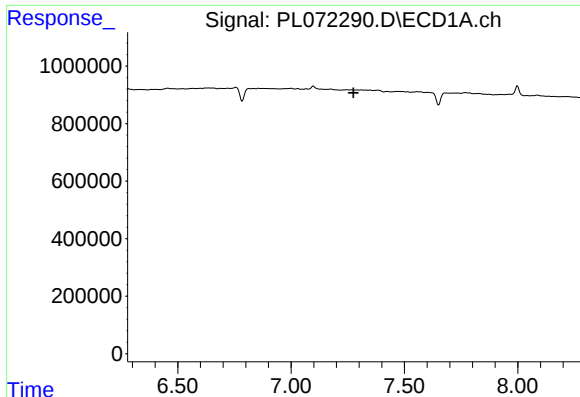

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

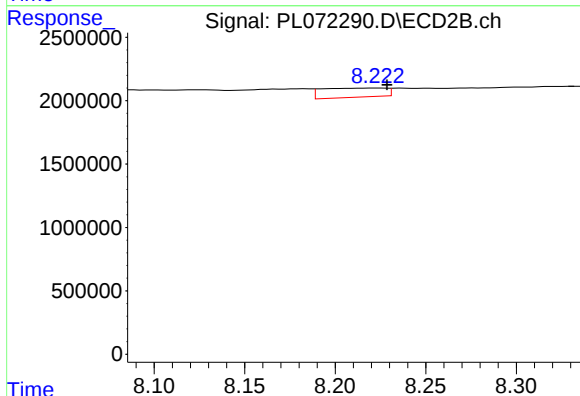


#10 gamma-Chlordane

R.T.: 8.224 min
Delta R.T.: -0.005 min
Response: 1772842
Conc: 0.88 ng/ml

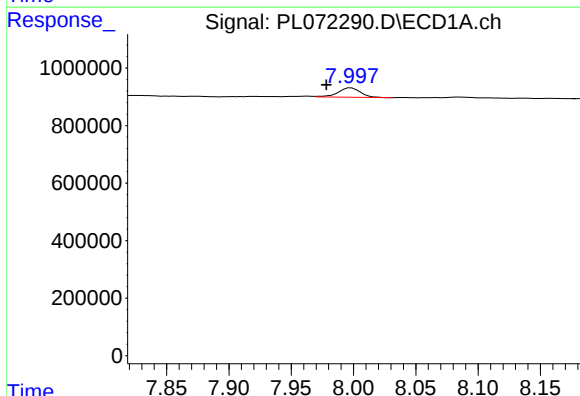


#14 Endrin

R.T.: 7.998 min
Delta R.T.: 0.020 min
Response: 410541
Conc: 0.59 ng/ml

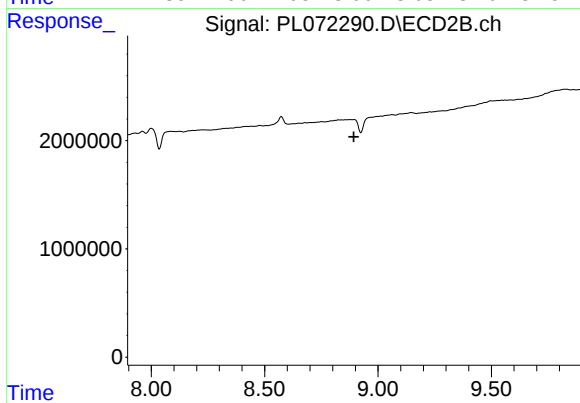

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

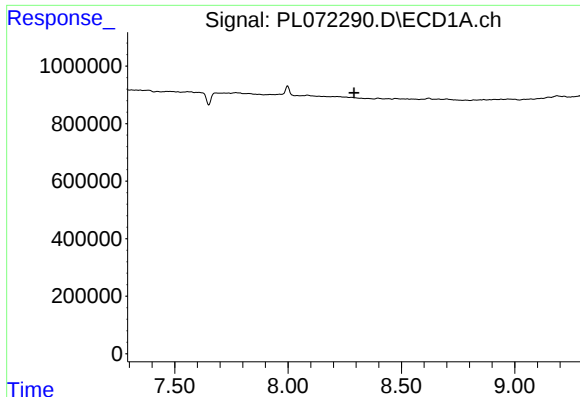

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

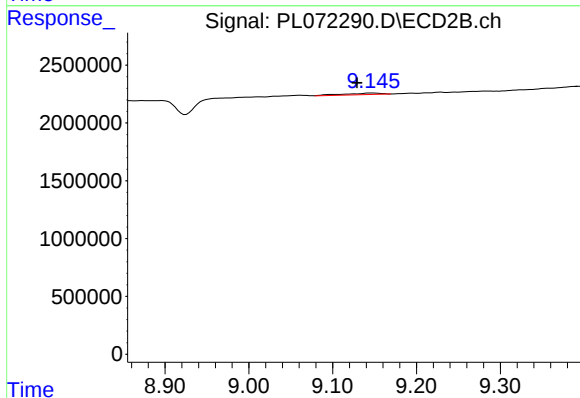


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.018 min
Response: 437693
Conc: 0.26 ng/ml

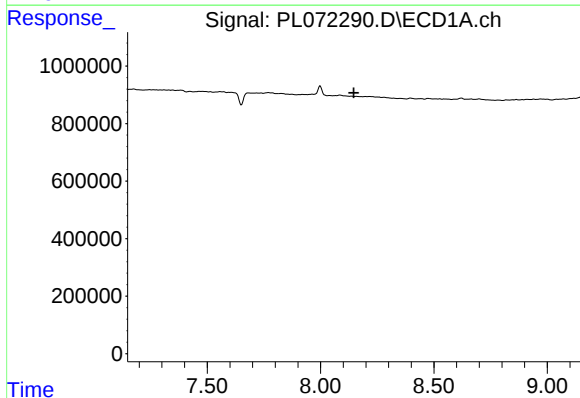


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

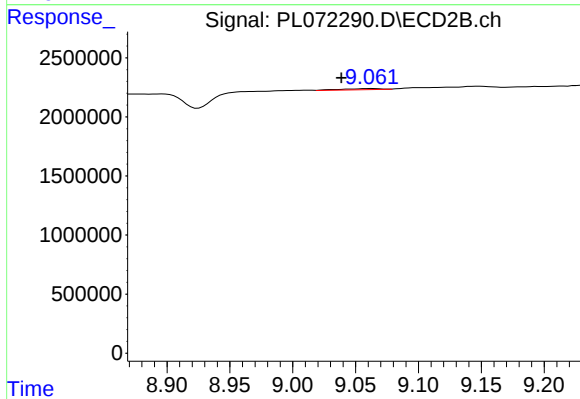

#16 4,4'-DDD


R.T.: 9.062 min
Delta R.T.: 0.024 min
Response: 215836
Conc: 0.15 ng/ml

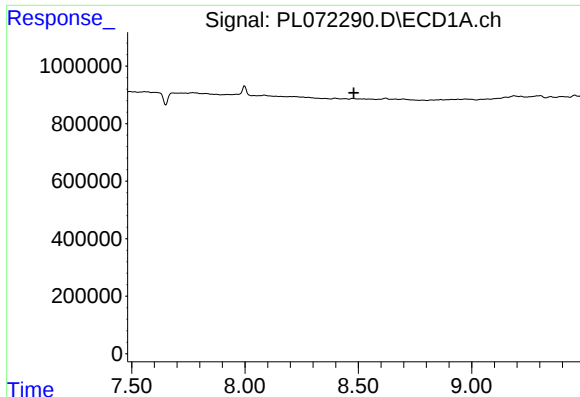

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

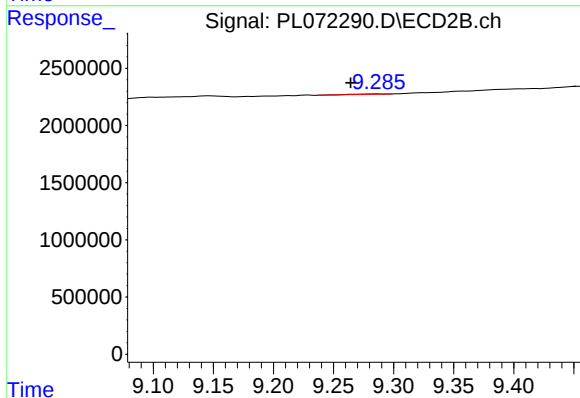


#18 Endrin aldehyde

R.T.: 9.287 min
Delta R.T.: 0.022 min
Response: 73523
Conc: 0.06 ng/ml

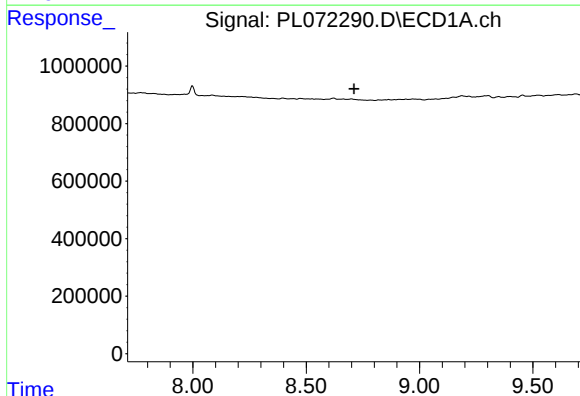


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

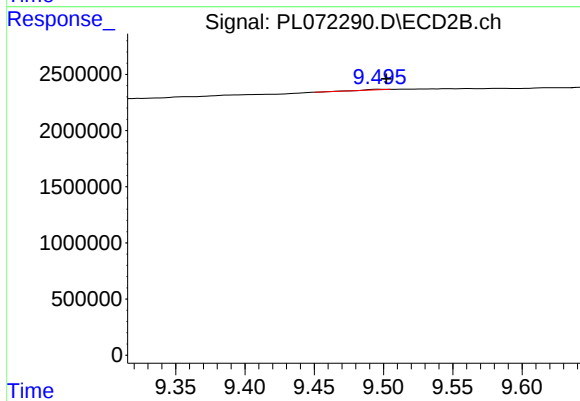

#19 Endosulfan Sulfate


R.T.: 9.497 min
Delta R.T.: -0.005 min
Response: 42725
Conc: 0.03 ng/ml

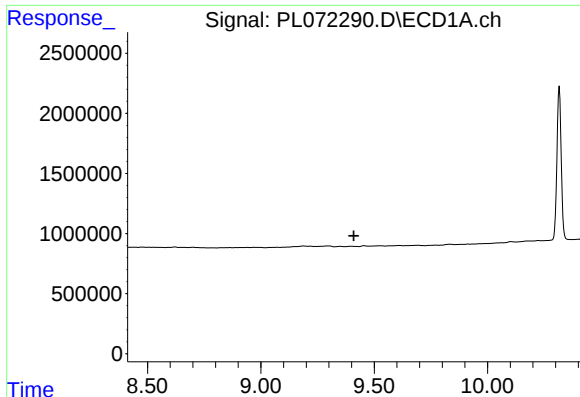

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

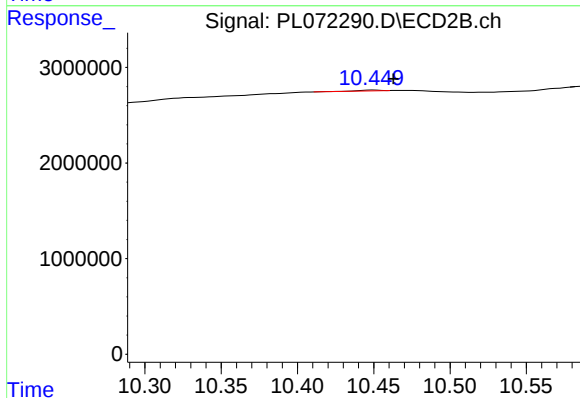


#22 Mirex

R.T.: 10.450 min
Delta R.T.: -0.013 min
Response: 93144
Conc: 0.07 ng/ml

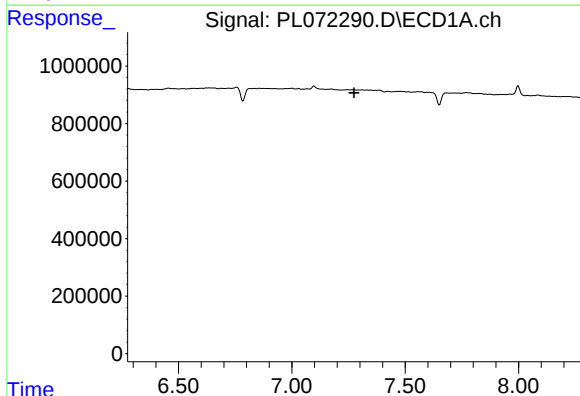


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

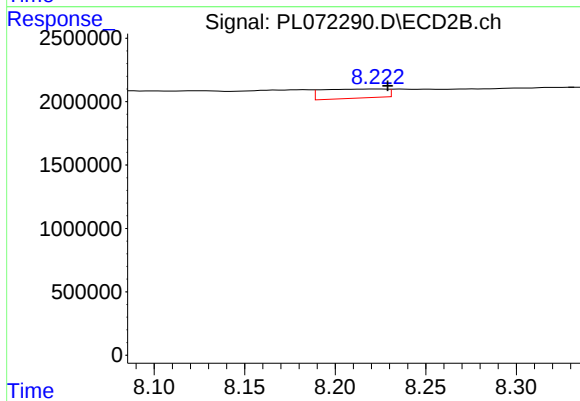

#25 Chlordane-3


R.T.: 8.224 min
Delta R.T.: -0.005 min
Response: 1772842
Conc: 6.38 ng/ml

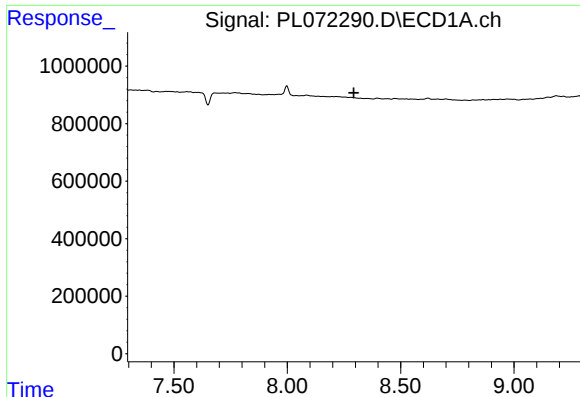

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

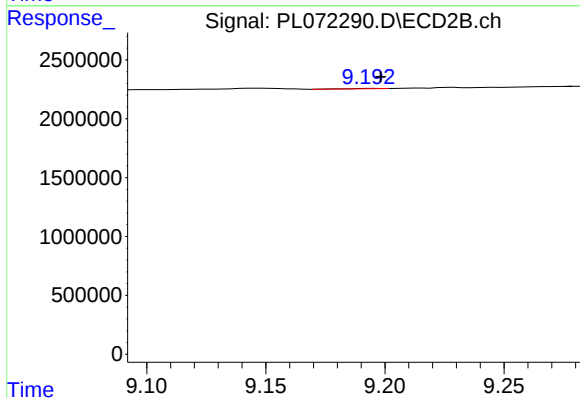


#27 Chlorine-5

R.T.: 9.195 min
Delta R.T.: -0.003 min
Response: 21662
Conc: 0.36 ng/ml

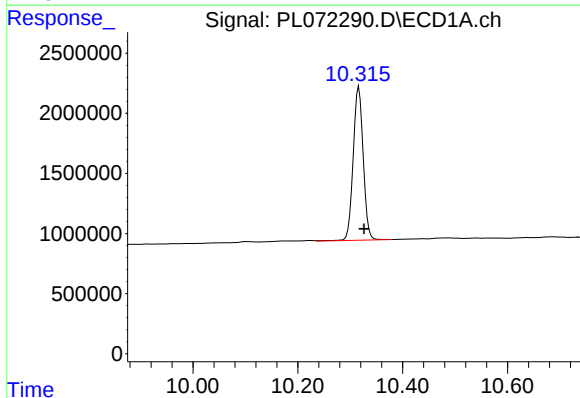

#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: -0.010 min
Response: 16894180
Conc: 19.02 ng/ml

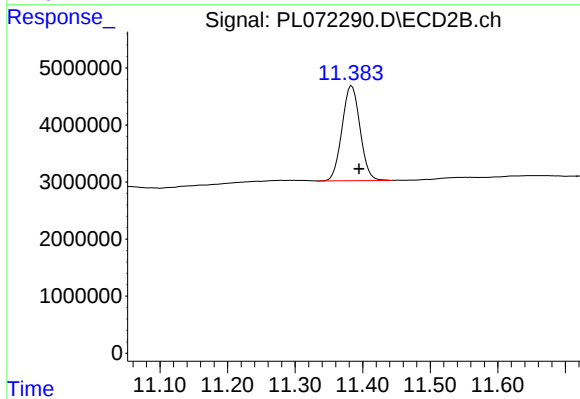

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.011 min
Response: 30789541
Conc: 19.08 ng/ml