

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
 Data File : PL080554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2023 14:57
 Operator : AR\AJ
 Sample : 01318-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DR-1-012523

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2023
 Supervised By : Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:28:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.689	20229732	19406582	9.432	8.835
28)	SA Decachlor...	8.790	7.837	41216813	45029318	23.542	18.900
Target Compounds							
12)	B 4,4'-DDE	5.987	5.149	4114508	3979889	1.847m	1.687

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
Data File : PL080554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2023 14:57
Operator : AR\AJ
Sample : 01318-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DR-1-012523


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/30/2023
Supervised By : Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:28:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

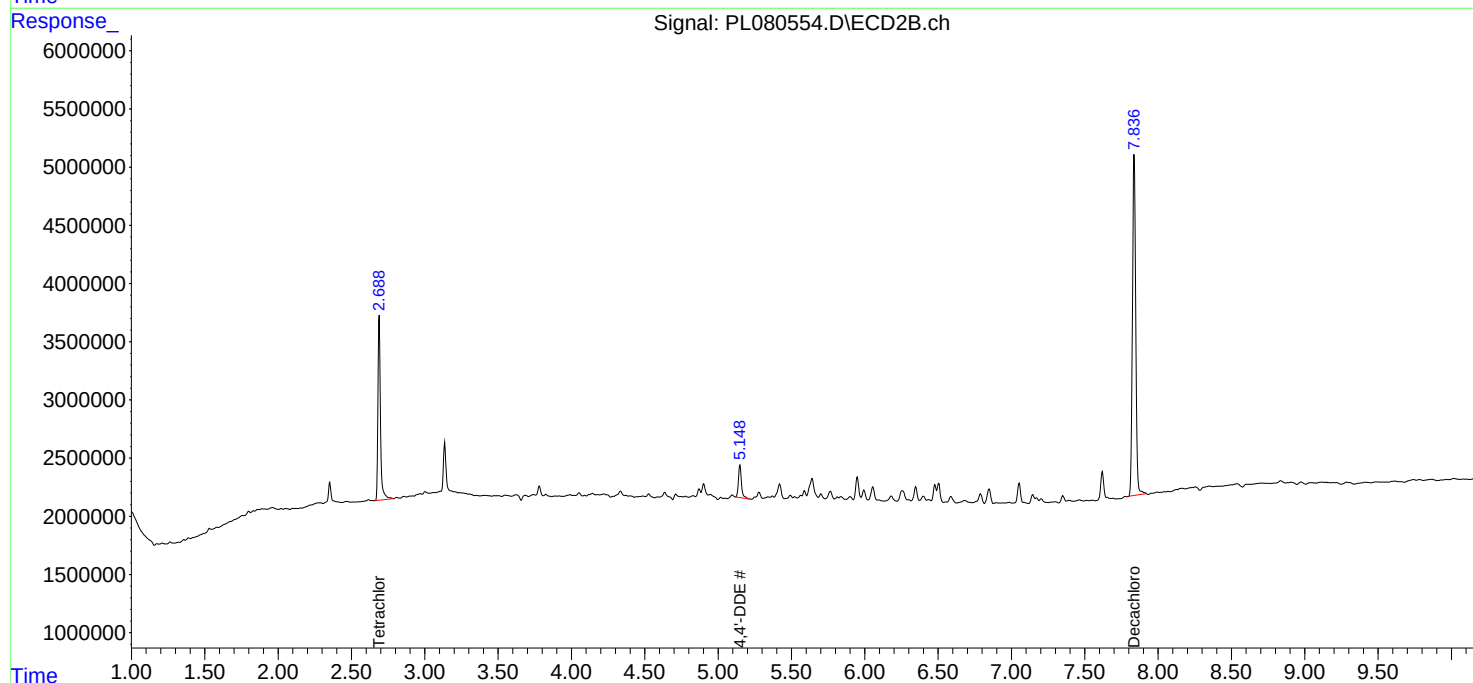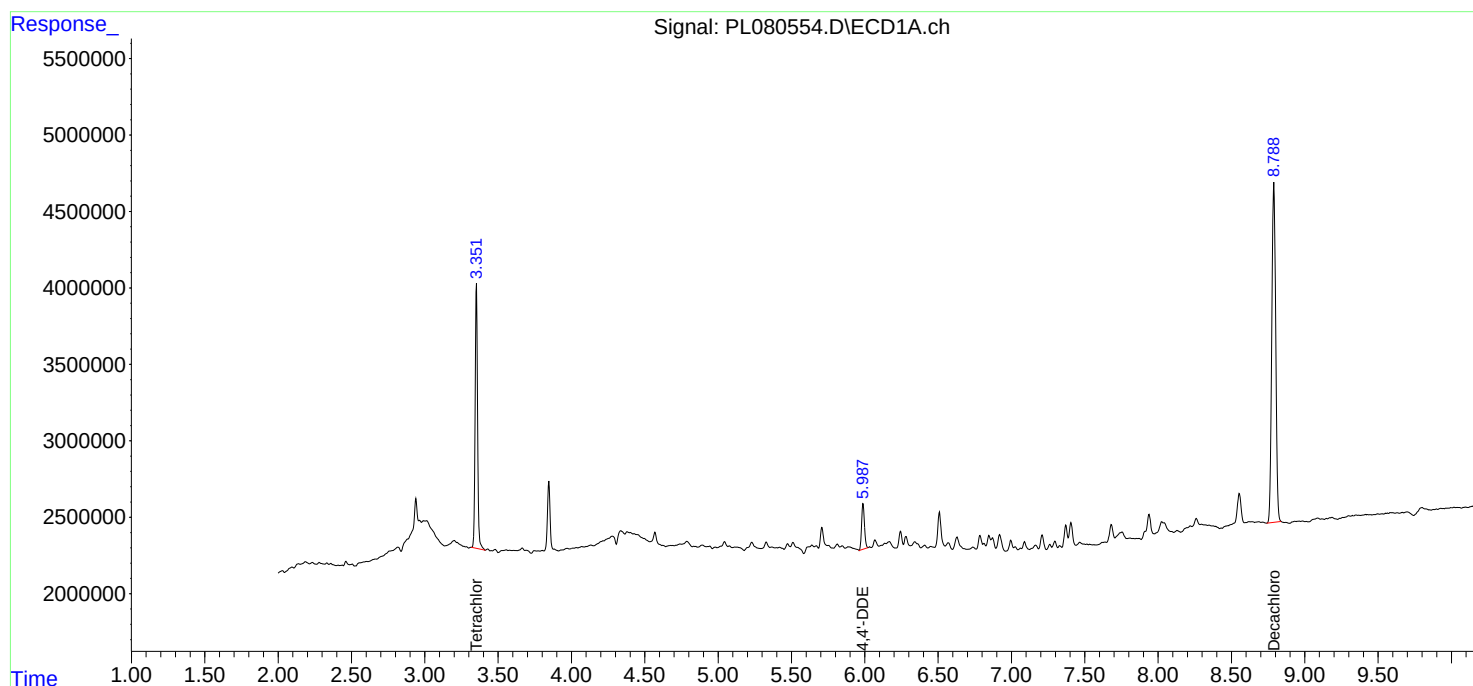

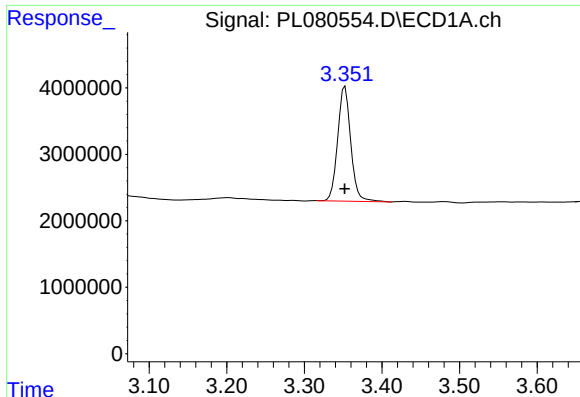


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 20229732
Conc: 9.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
DR-1-012523


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

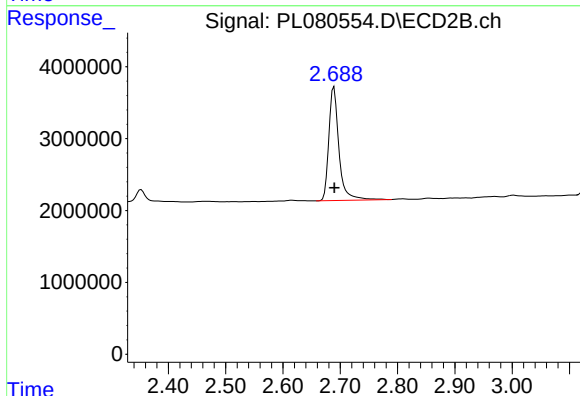


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 19406582
Conc: 8.84 ng/ml

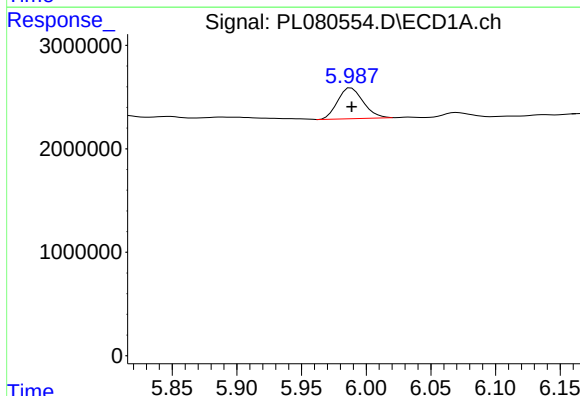


#12 4,4'-DDE

R.T.: 5.987 min
Delta R.T.: -0.002 min
Response: 4114508
Conc: 1.85 ng/ml m

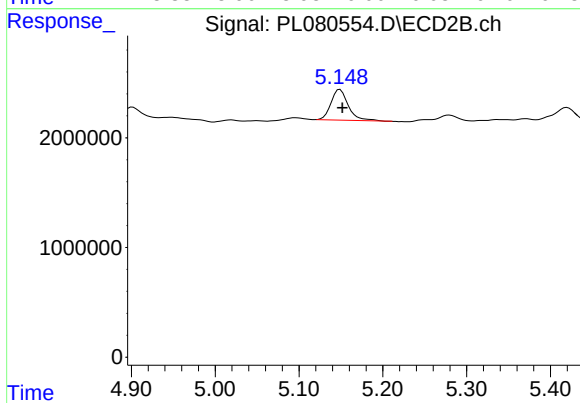

#12 4,4'-DDE

R.T.: 5.149 min
Delta R.T.: -0.003 min
Response: 3979889
Conc: 1.69 ng/ml

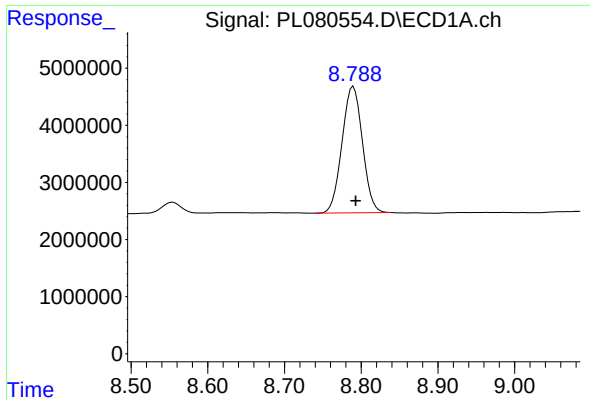


#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 41216813
Conc: 23.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
DR-1-012523

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

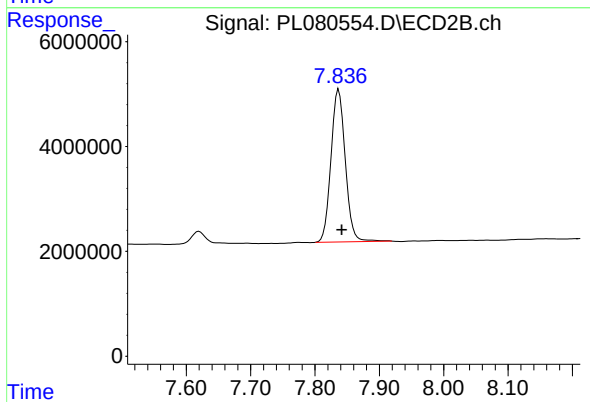

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: -0.005 min
Response: 45029318
Conc: 18.90 ng/ml