

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
 Data File : PL080572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2023 19:06
 Operator : AR\AJ
 Sample : 01329-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-6-BORING-2-7-14

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/30/2023
 Supervised By :Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:55:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.688	19037454	18851405	8.876	8.583
28) SA Decachlor...	8.786	7.835	18485846	22847042	10.559	9.589
Target Compounds						
11) B alpha-Chl...	5.812	4.954	1967200	1012733	0.779	0.354 #
12) B 4,4'-DDE	5.985	5.147	2347686	2268879	1.054	0.962
17) MA 4,4'-DDT	6.811	5.951	1512814	1445750	0.728m	0.688m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
Data File : PL080572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2023 19:06
Operator : AR\AJ
Sample : 01329-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-6-BORING-2-7-14


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/30/2023
Supervised By : Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:55:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

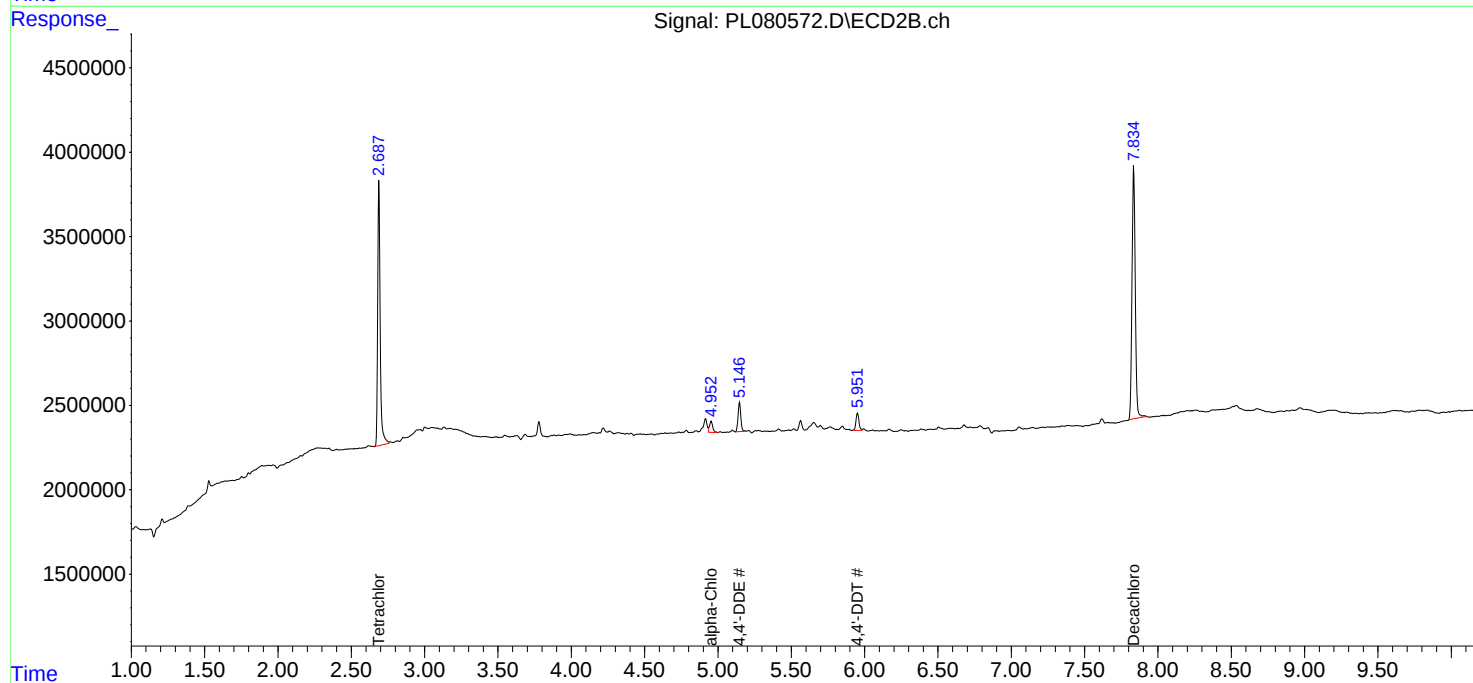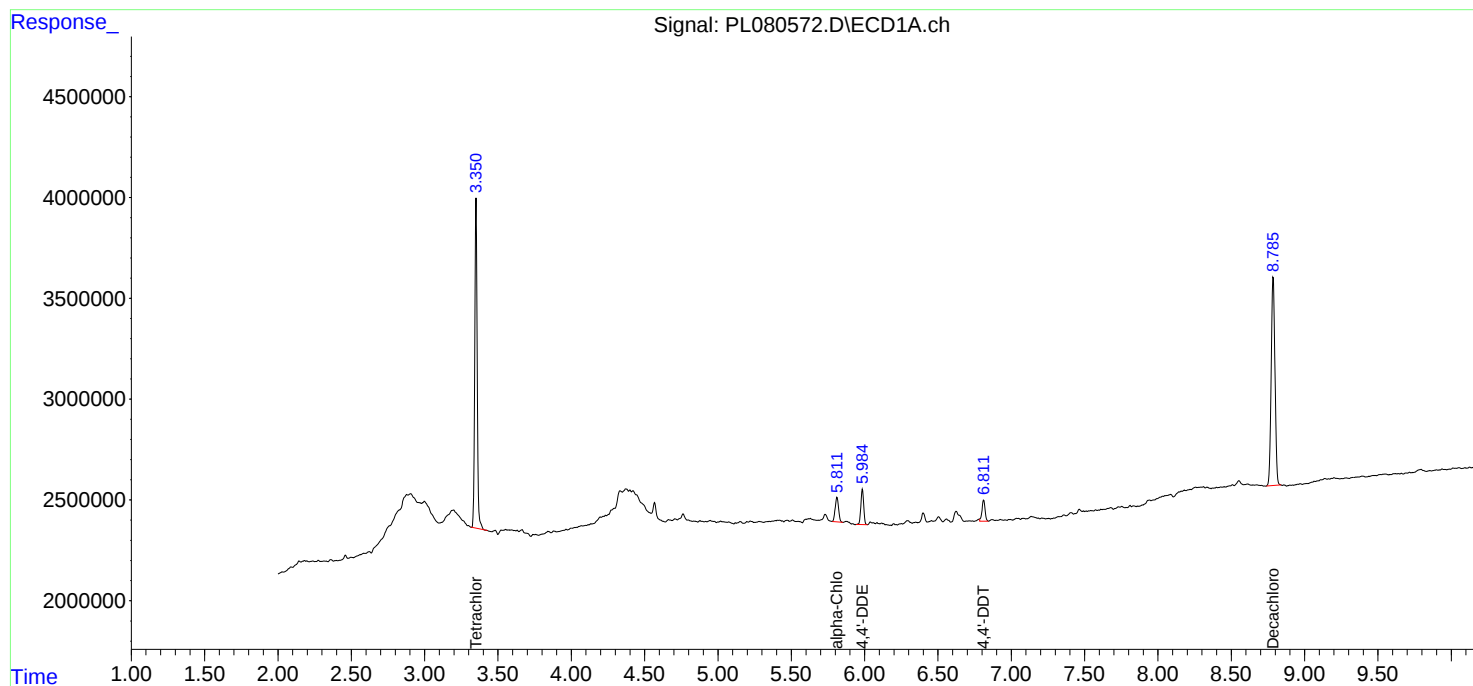

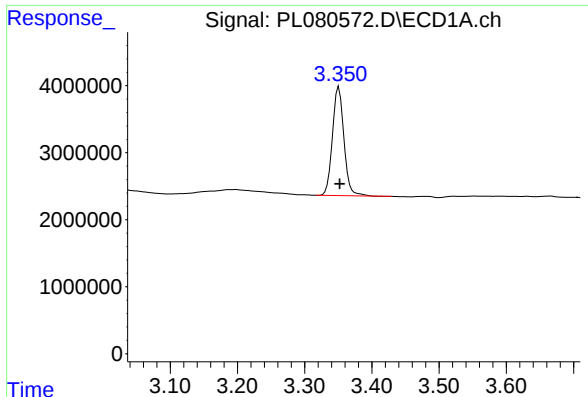


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: -0.001 min
Response: 19037454
Conc: 8.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-6-BORING-2-7-14


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

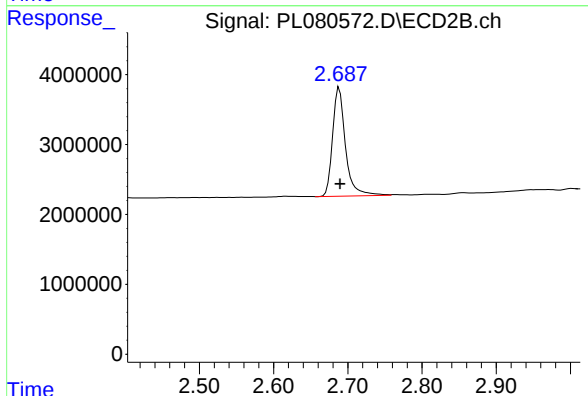


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.001 min
Response: 18851405
Conc: 8.58 ng/ml

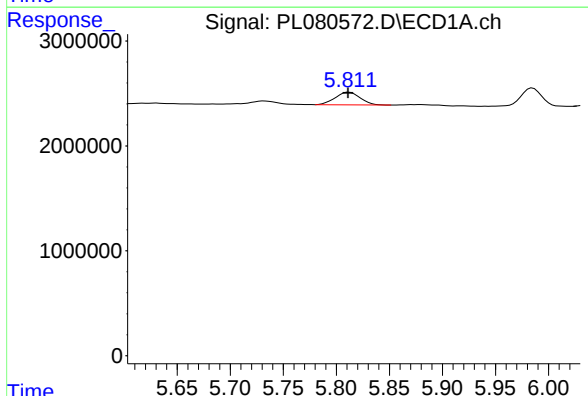


#11 alpha-Chlordane

R.T.: 5.812 min
Delta R.T.: 0.001 min
Response: 1967200
Conc: 0.78 ng/ml

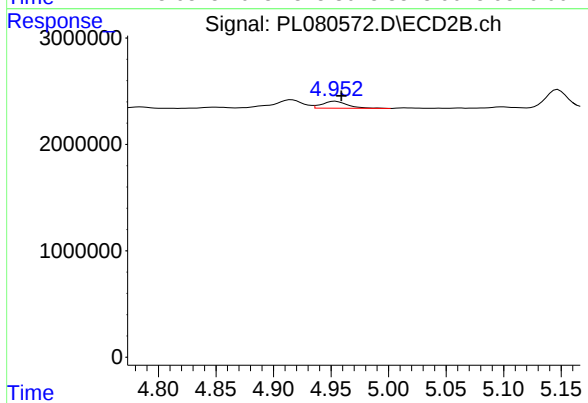

#11 alpha-Chlordane

R.T.: 4.954 min
Delta R.T.: -0.005 min
Response: 1012733
Conc: 0.35 ng/ml

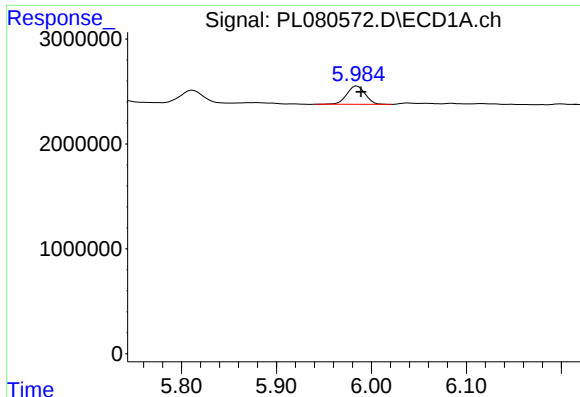


#12 4,4'-DDE

R.T.: 5.985 min
Delta R.T.: -0.004 min
Response: 2347686
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-6-BORING-2-7-14


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

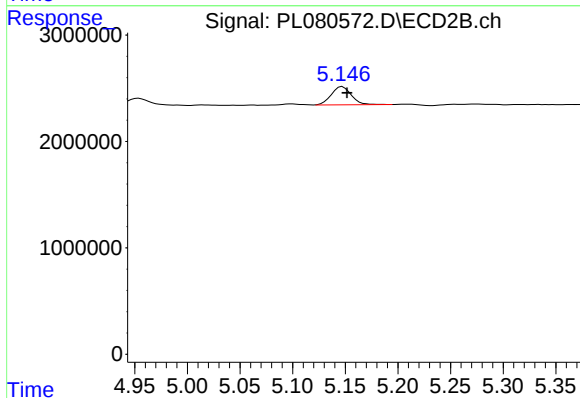


#12 4,4'-DDE

R.T.: 5.147 min
Delta R.T.: -0.005 min
Response: 2268879
Conc: 0.96 ng/ml

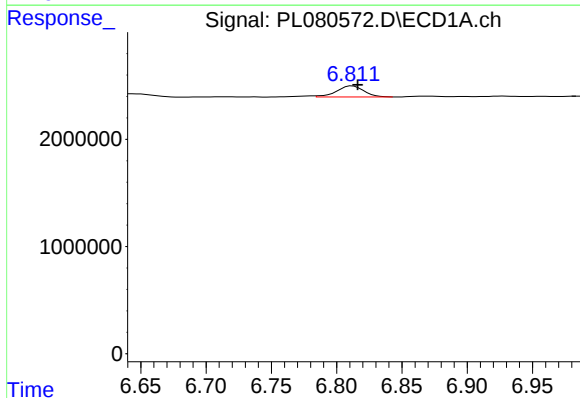


#17 4,4'-DDT

R.T.: 6.811 min
Delta R.T.: -0.006 min
Response: 1512814
Conc: 0.73 ng/ml m

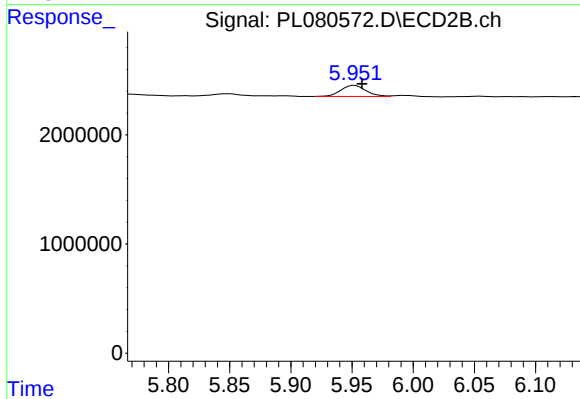

#17 4,4'-DDT

R.T.: 5.951 min
Delta R.T.: -0.008 min
Response: 1445750
Conc: 0.69 ng/ml m

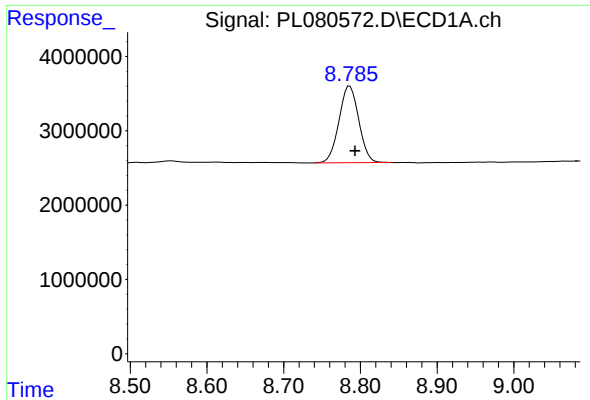


#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 18485846
Conc: 10.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-6-BORING-2-7-14

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

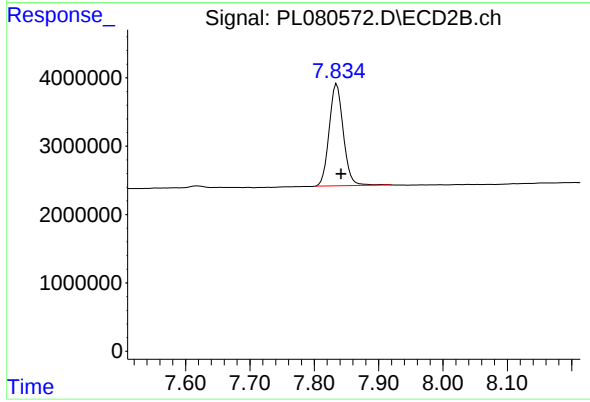

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.007 min
Response: 22847042
Conc: 9.59 ng/ml