

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
 Data File : PL080573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2023 19:20
 Operator : AR\AJ
 Sample : 01329-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-7-BORING-2-14-21

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/30/2023
 Supervised By :Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:57:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.349	2.689	37839019	38076195	17.642m	17.335
28) SA Decachlor...	8.787	7.835	26400700	32084758	15.080	13.467

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
Data File : PL080573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2023 19:20
Operator : AR\AJ
Sample : 01329-06
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
COMP-7-BORING-2-14-21


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/30/2023
Supervised By : Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:57:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

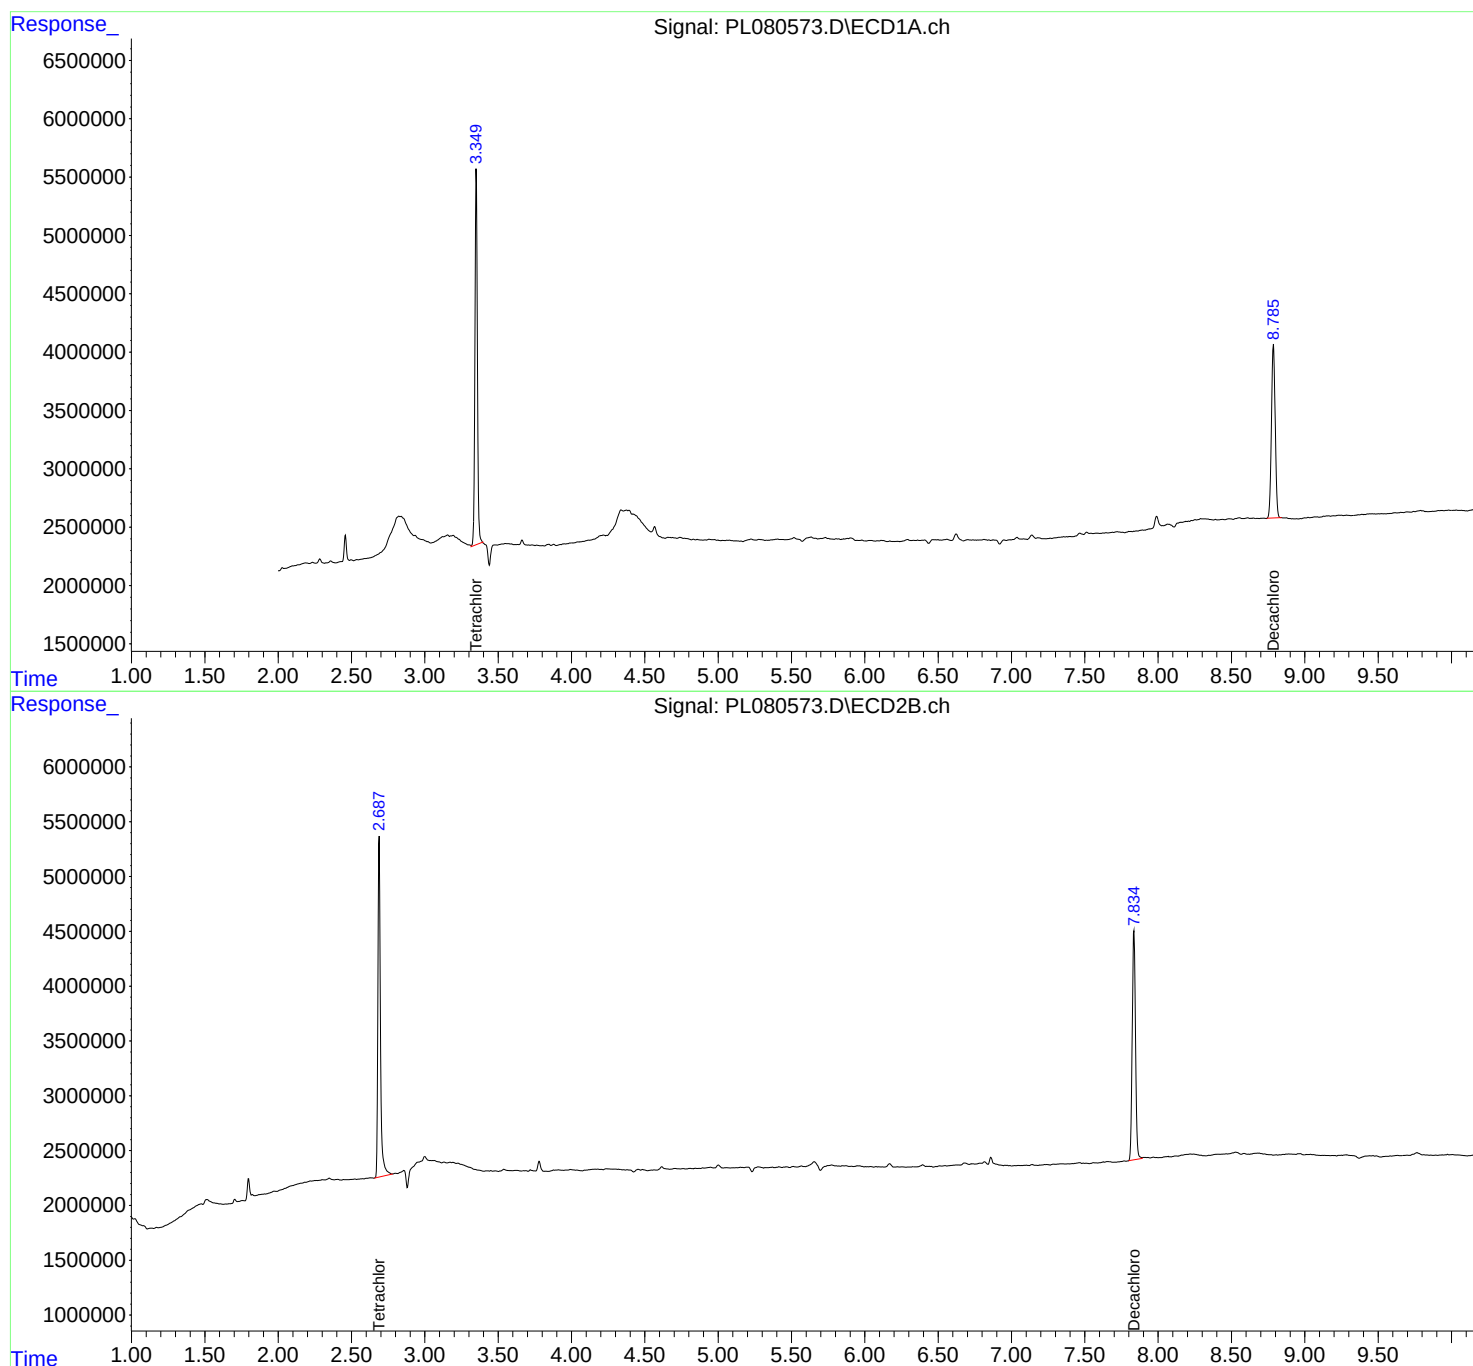

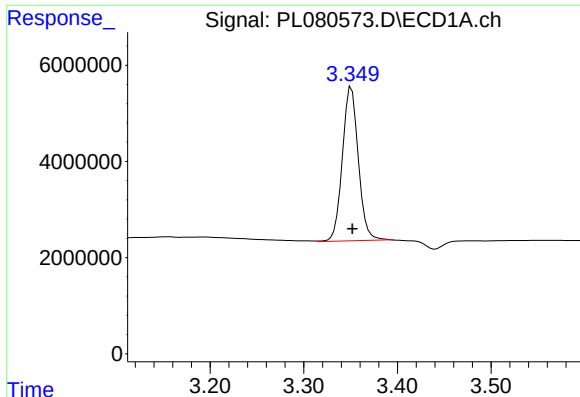


#1 Tetrachloro-m-xylene

R.T.: 3.349 min
Delta R.T.: -0.003 min
Response: 37839019
Conc: 17.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-7-BORING-2-14-21


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

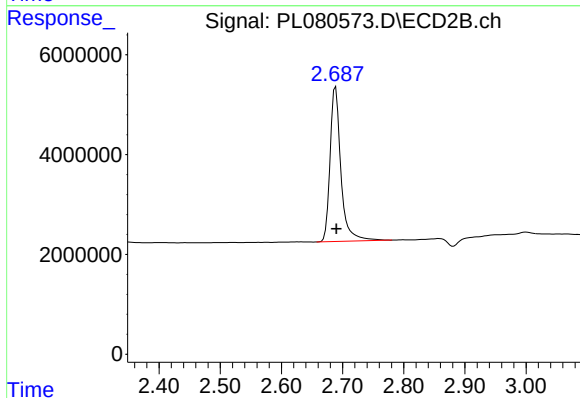


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: -0.001 min
Response: 38076195
Conc: 17.34 ng/ml

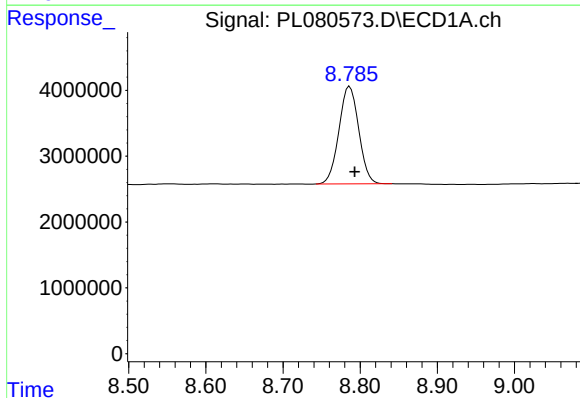

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.007 min
Response: 26400700
Conc: 15.08 ng/ml

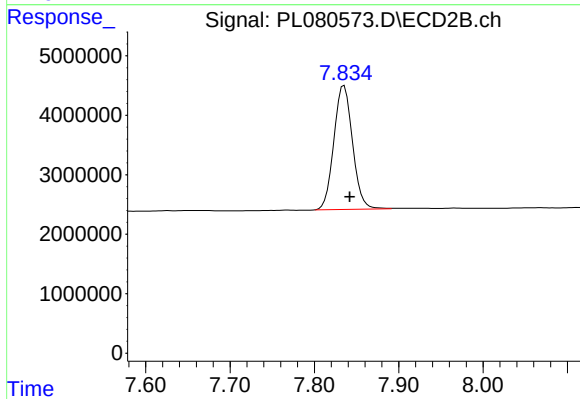

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.007 min
Response: 32084758
Conc: 13.47 ng/ml