

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
 Data File : PL080575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2023 19:48
 Operator : AR\AJ
 Sample : 01329-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-9-BORING-2-28-35

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/30/2023
 Supervised By :Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 23:59:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.689	36209362	36697973	16.882m	16.708
2) SA Decachlor...	8.786	7.835	25129276	30887311	14.353	12.964

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012723\
Data File : PL080575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2023 19:48
Operator : AR\AJ
Sample : 01329-16
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
COMP-9-BORING-2-28-35


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/30/2023
Supervised By : Ankita Jodhani 01/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 23:59:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

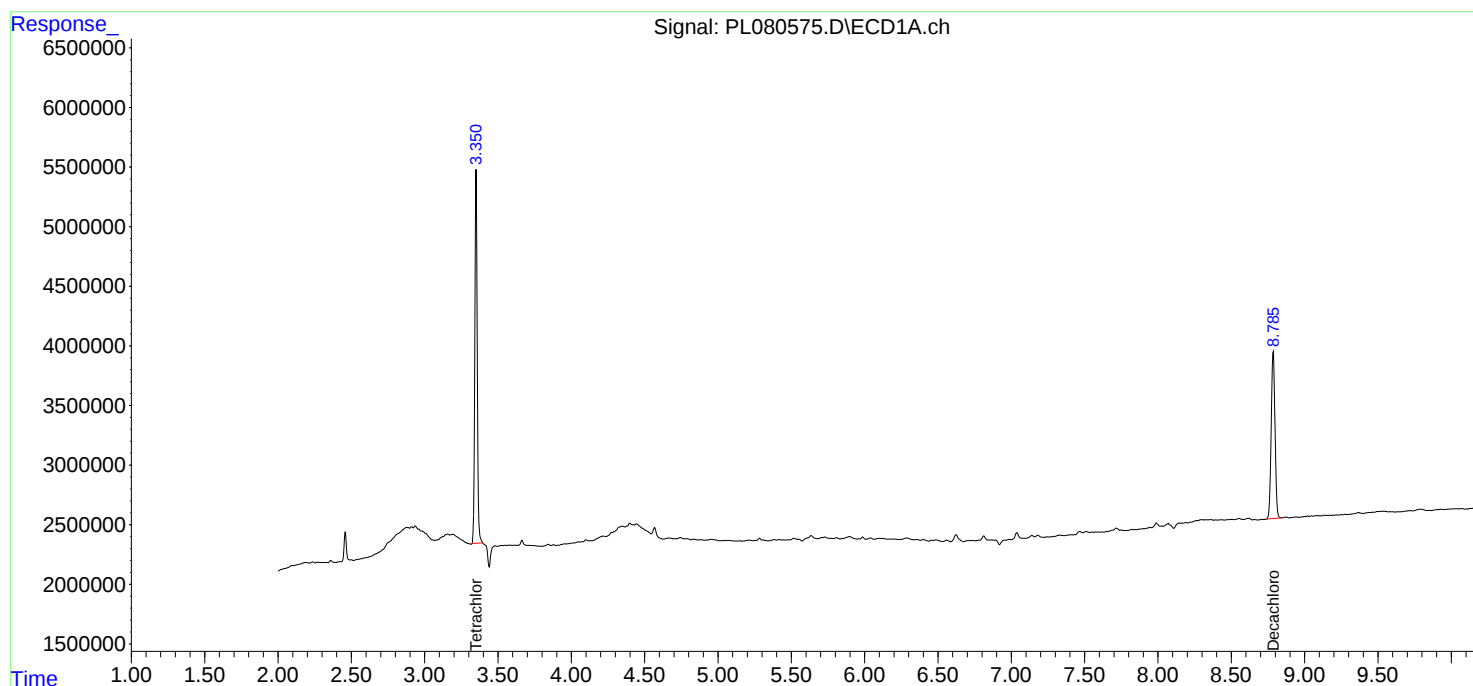

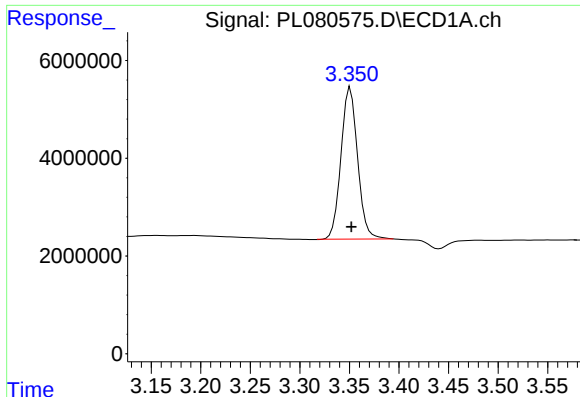


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 36209362
Conc: 16.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-9-BORING-2-28-35


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/30/2023
Supervised By :Ankita Jodhani 01/30/2023

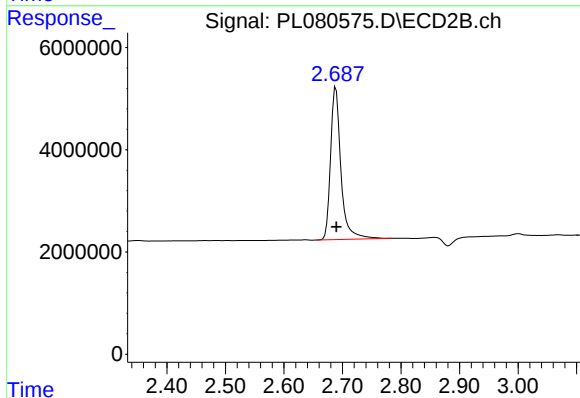


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 36697973
Conc: 16.71 ng/ml

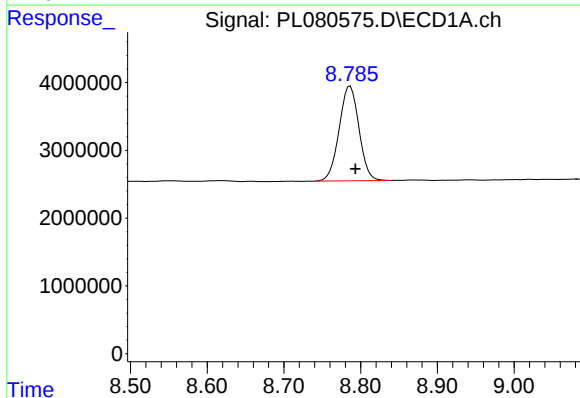

#28 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 25129276
Conc: 14.35 ng/ml

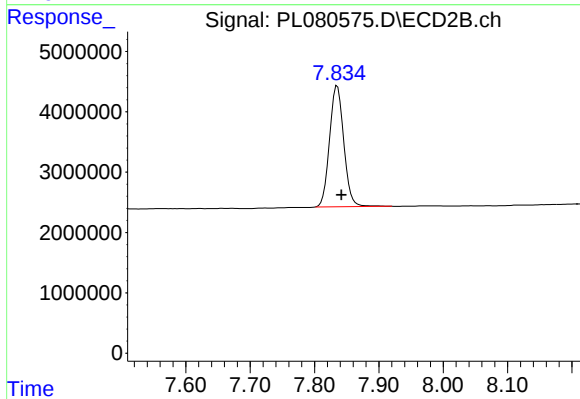

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.006 min
Response: 30887311
Conc: 12.96 ng/ml