

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
 Data File : PL087986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 20:16
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 03:35:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 03:25:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.671	58876117	24525194	20.298	19.759
28)	SA Decachlor...	8.977	7.857	56416511	25583449	21.051	21.035
Target Compounds							
9)	A Endosulfan I	5.960	5.005	32923622	13246717	9.689	9.363
10)	B gamma-Chl...	5.833	4.887	36838181	15028715	9.950	9.736
12)	B 4,4'-DDE	6.094	5.150	58024150	24173848	19.292	18.923
13)	MA Dieldrin	6.239	5.272	67281889	28370691	18.938	18.507
19)	B Endosulfa...	7.059	6.253	57346063	24775582	19.816	19.512
20)	A Methoxychlor	7.417	6.547	146.6E6	68157973	94.368	96.028
21)	B Endrin ke...	7.545	6.759	59004910	28375002	19.272	19.111



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
Data File : PL087986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 20:16
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 03:35:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 03:25:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

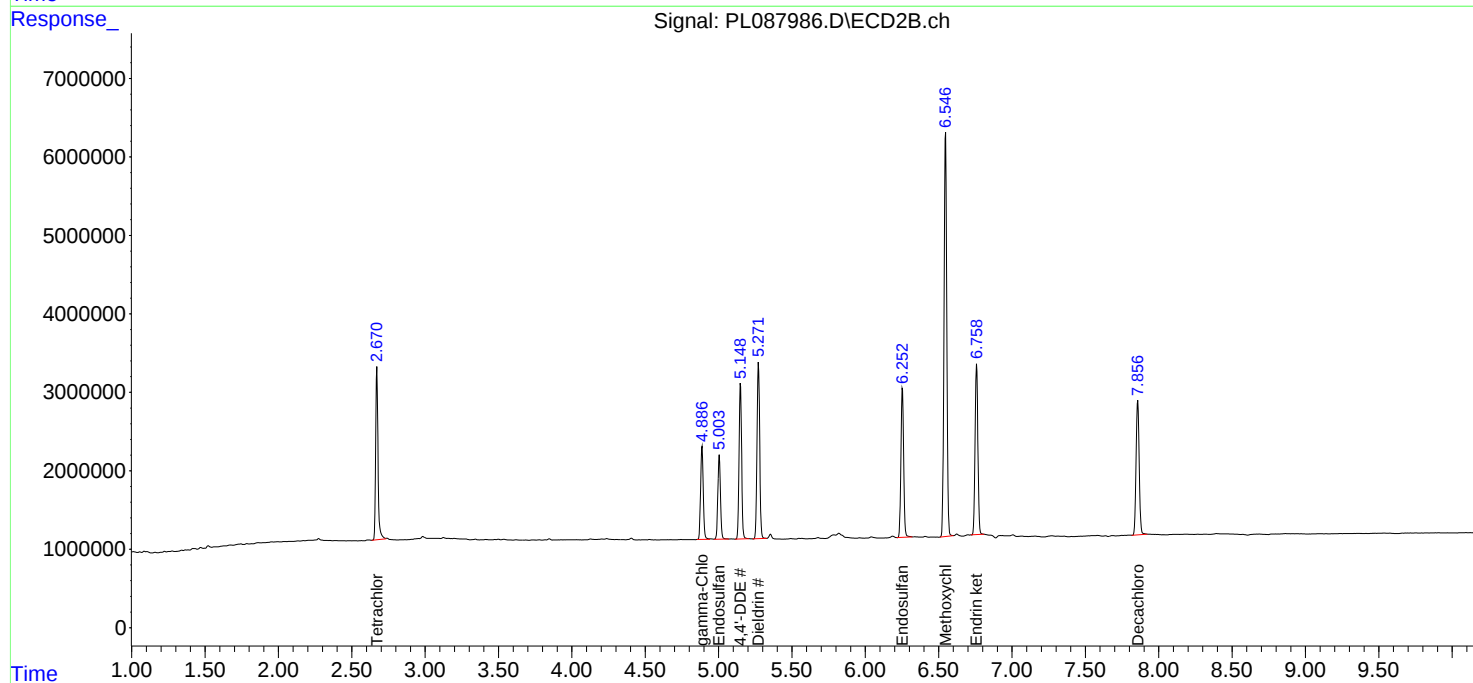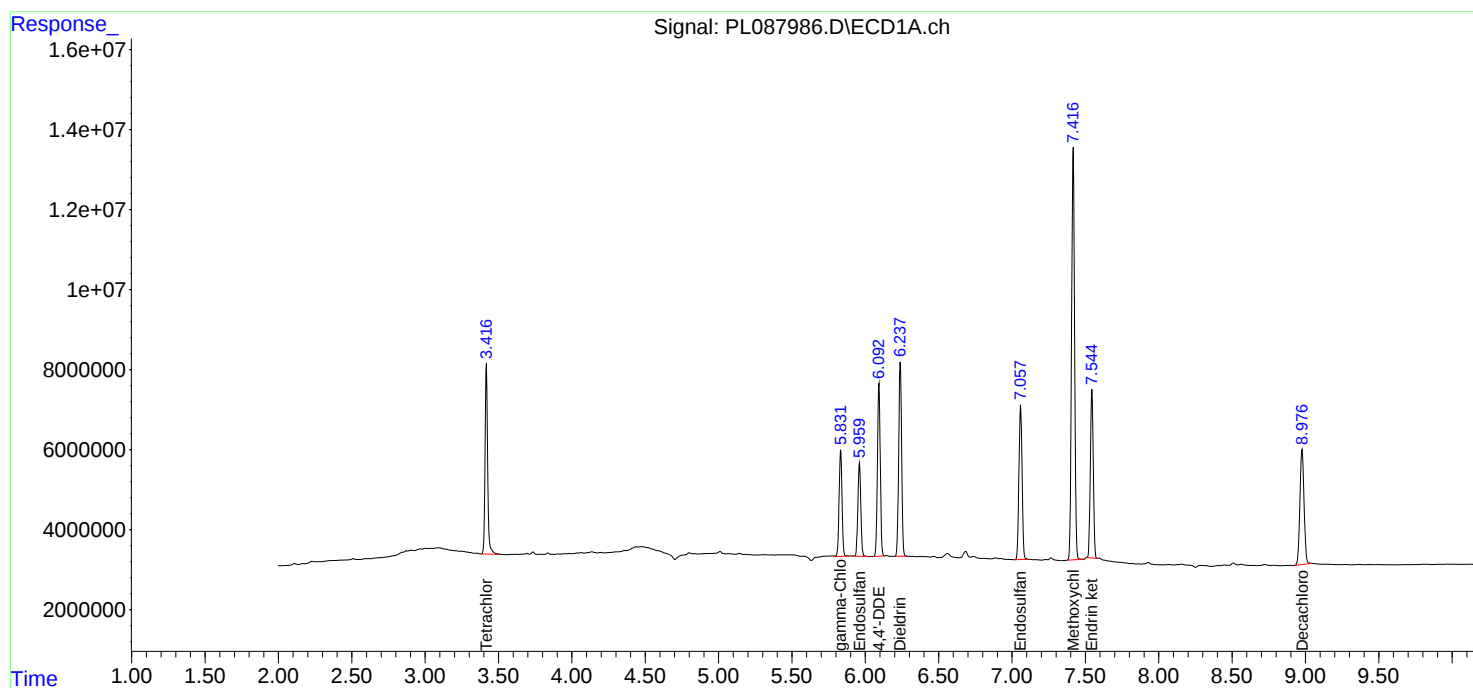


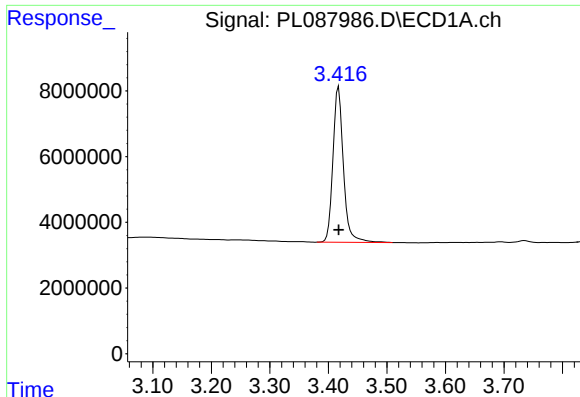

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 58876117
Conc: 20.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

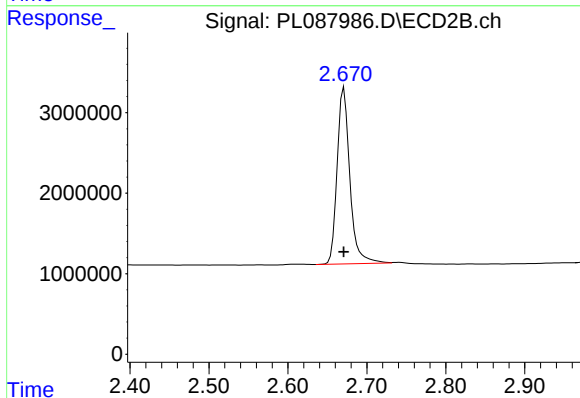


#1 Tetrachloro-m-xylene

R.T.: 2.671 min
Delta R.T.: 0.000 min
Response: 24525194
Conc: 19.76 ng/ml

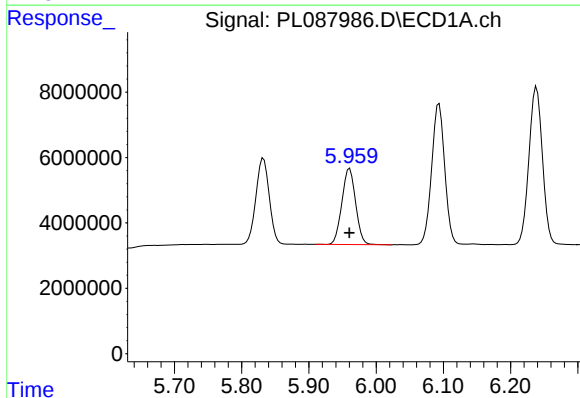


#9 Endosulfan I

R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 32923622
Conc: 9.69 ng/ml

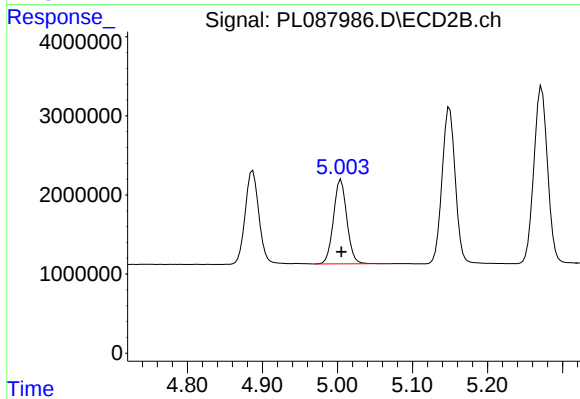

#9 Endosulfan I


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 13246717
Conc: 9.36 ng/ml

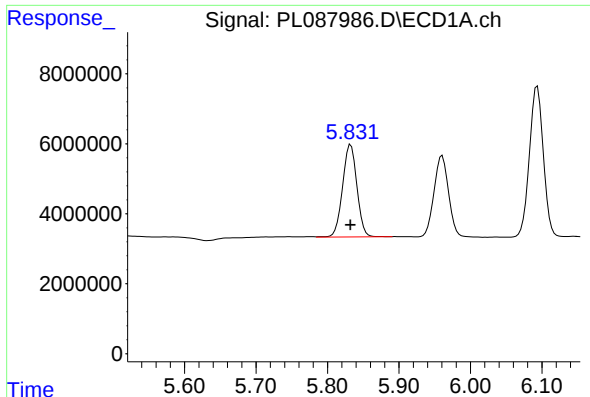

#10 gamma-Chlordane


R.T.: 5.833 min
Delta R.T.: 0.000 min
Response: 36838181
Conc: 9.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

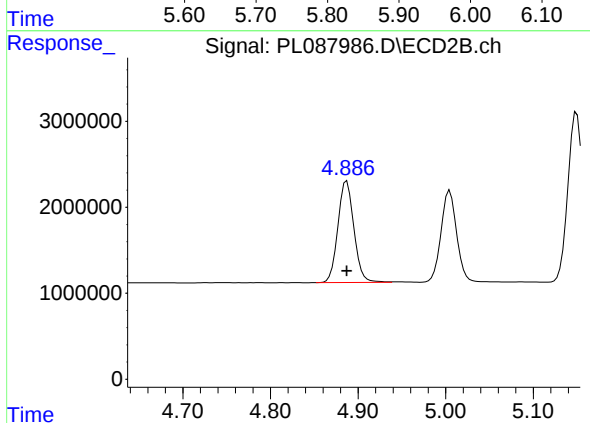


#10 gamma-Chlordane

R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 15028715
Conc: 9.74 ng/ml

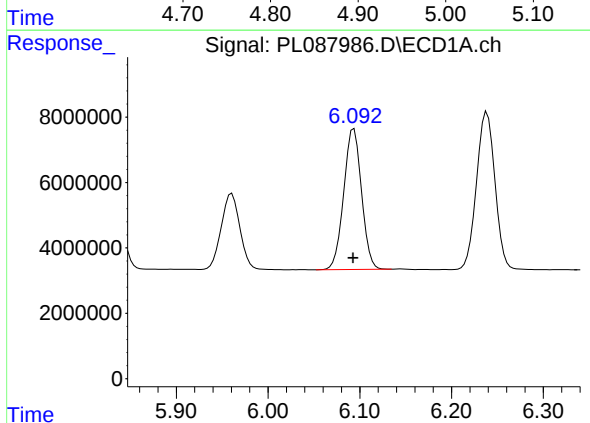


#12 4,4'-DDE

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 58024150
Conc: 19.29 ng/ml

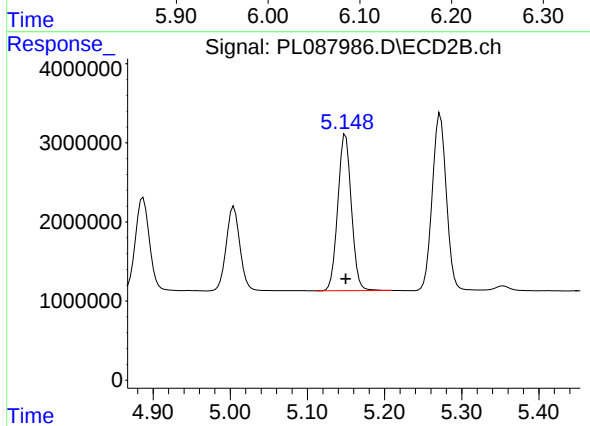

#12 4,4'-DDE


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 24173848
Conc: 18.92 ng/ml

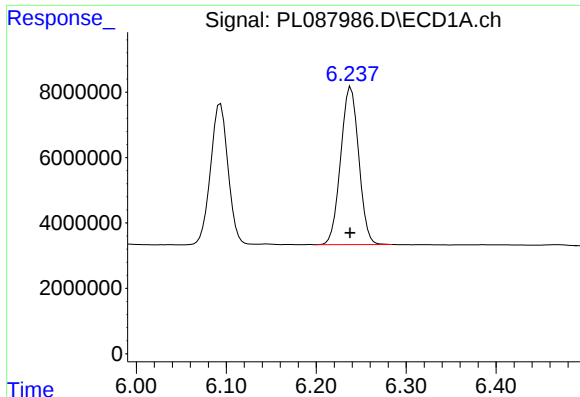

#13 Dieldrin


R.T.: 6.239 min
Delta R.T.: 0.000 min
Response: 67281889
Conc: 18.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

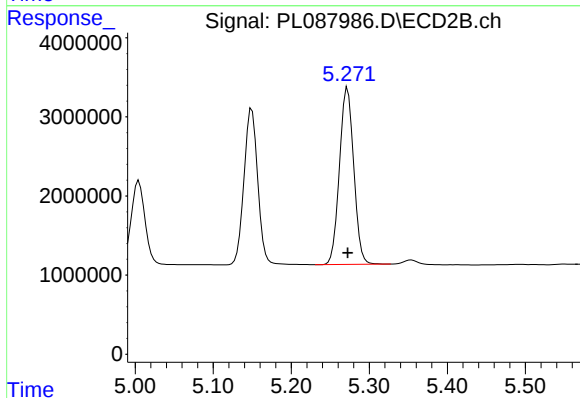


#13 Dieldrin

R.T.: 5.272 min
Delta R.T.: 0.000 min
Response: 28370691
Conc: 18.51 ng/ml

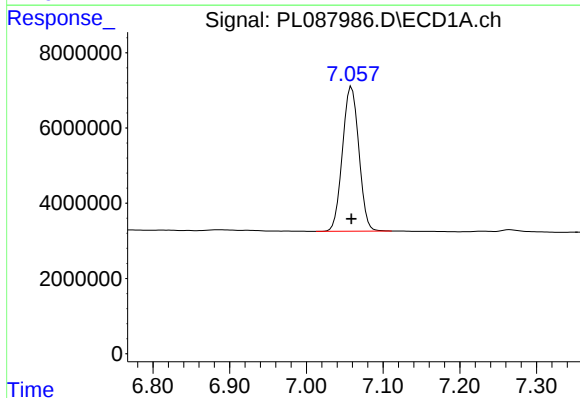


#19 Endosulfan Sulfate

R.T.: 7.059 min
Delta R.T.: 0.000 min
Response: 57346063
Conc: 19.82 ng/ml

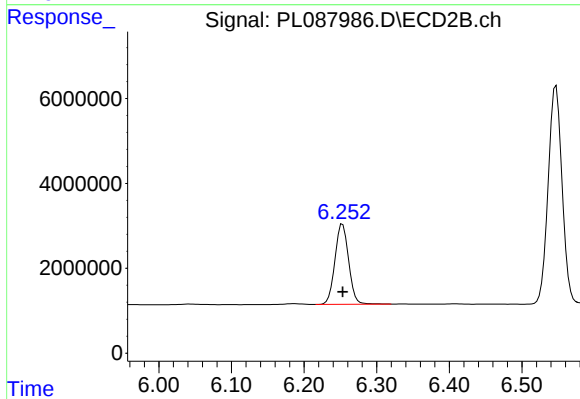

#19 Endosulfan Sulfate


R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 24775582
Conc: 19.51 ng/ml

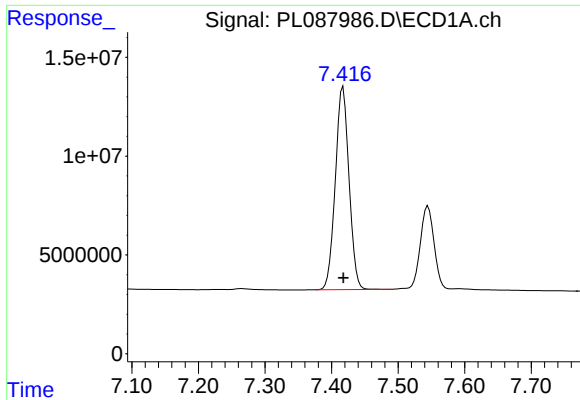

#20 Methoxychlor


R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 146632591
Conc: 94.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

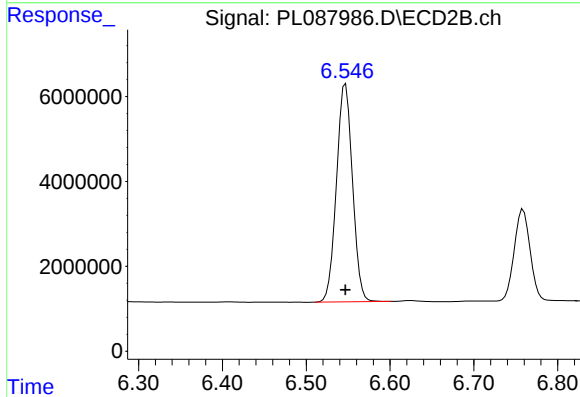


#20 Methoxychlor

R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 68157973
Conc: 96.03 ng/ml

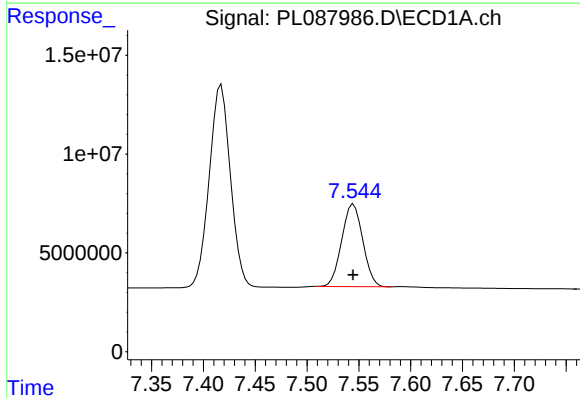


#21 Endrin ketone

R.T.: 7.545 min
Delta R.T.: 0.000 min
Response: 59004910
Conc: 19.27 ng/ml

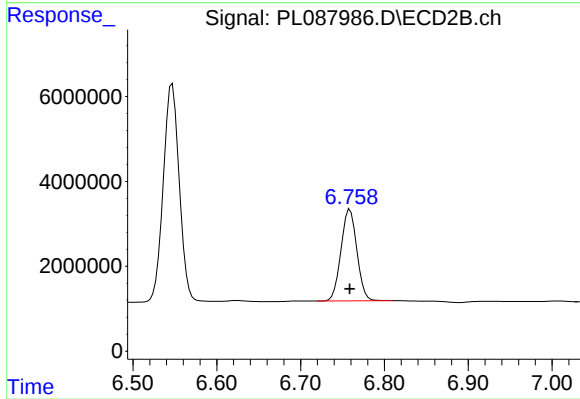

#21 Endrin ketone


R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 28375002
Conc: 19.11 ng/ml

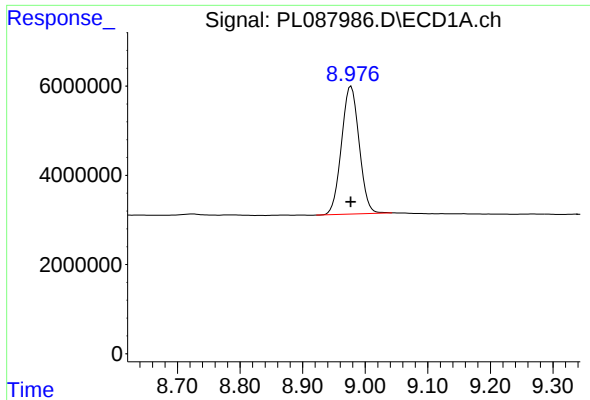

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.000 min
Response: 56416511
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

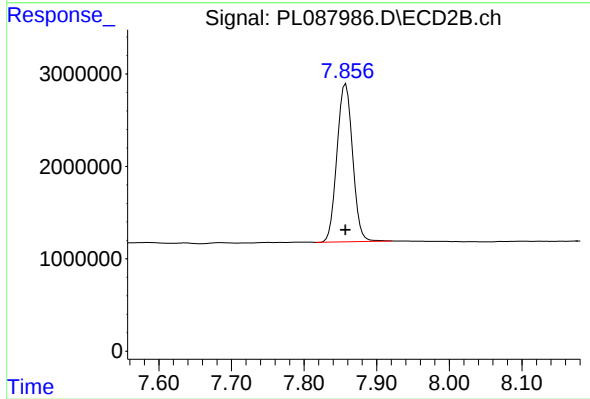

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.000 min
Response: 25583449
Conc: 21.04 ng/ml