

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
 Data File : PL087992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 21:40
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:33:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 00:33:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.670	302.2E6	166.6E6	101.806	102.269
28)	SA Decachlor...	8.977	7.857	252.8E6	119.0E6	97.578	97.802
Target Compounds							
23)	Chlordane-1	4.584	3.671	131.6E6	47465843	1015.850	1019.240
24)	Chlordane-2	5.118	4.253	136.6E6	57281629	992.046	993.071
25)	Chlordane-3	5.834	4.888	552.8E6	166.8E6	1023.373	1028.947
26)	Chlordane-4	5.917	4.950	668.7E6	176.8E6	1014.739	1030.770
27)	Chlordane-5	6.769	5.624	108.5E6	46083419	1006.334	1010.012



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
Data File : PL087992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 21:40
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:33:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 00:33:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

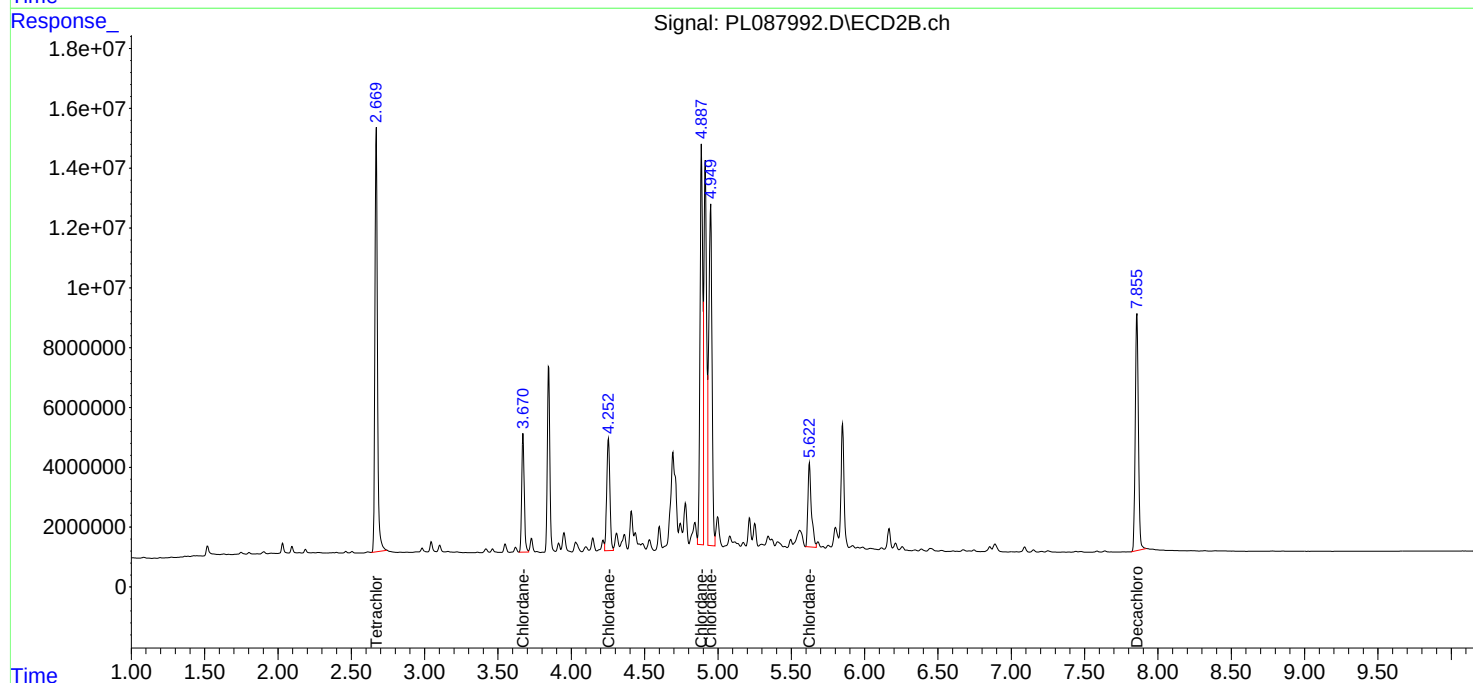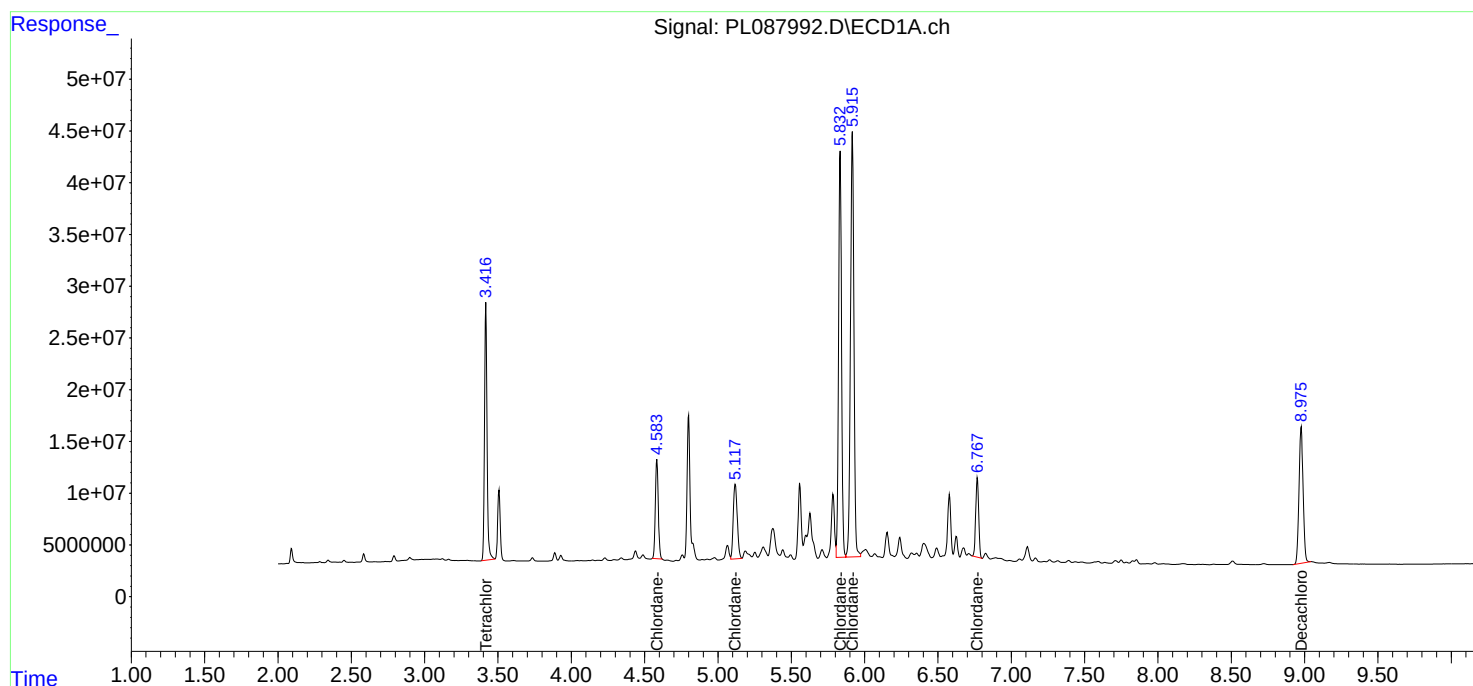


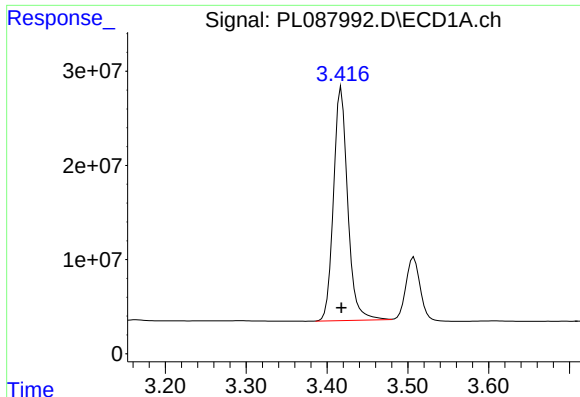

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.000 min
Response: 302194987
Conc: 101.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

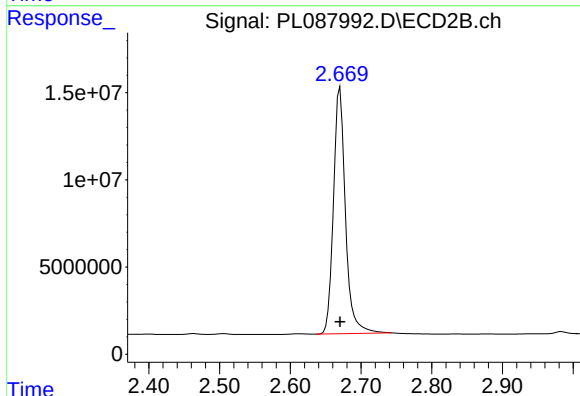


#1 Tetrachloro-m-xylene

R.T.: 2.670 min
Delta R.T.: 0.000 min
Response: 166639384
Conc: 102.27 ng/ml

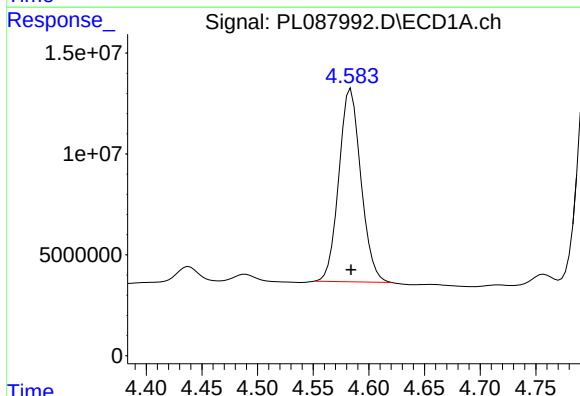


#23 Chlordane-1

R.T.: 4.584 min
Delta R.T.: 0.000 min
Response: 131571298
Conc: 1015.85 ng/ml

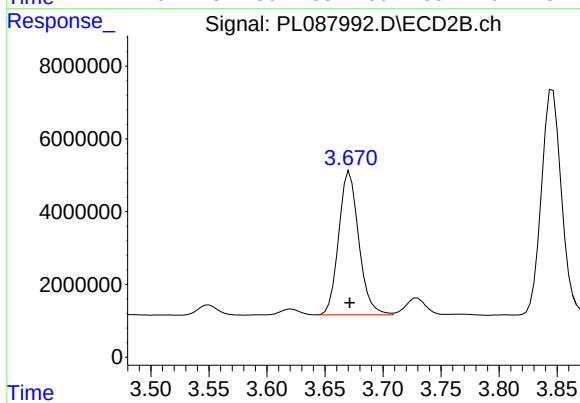

#23 Chlordane-1


R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 47465843
Conc: 1019.24 ng/ml

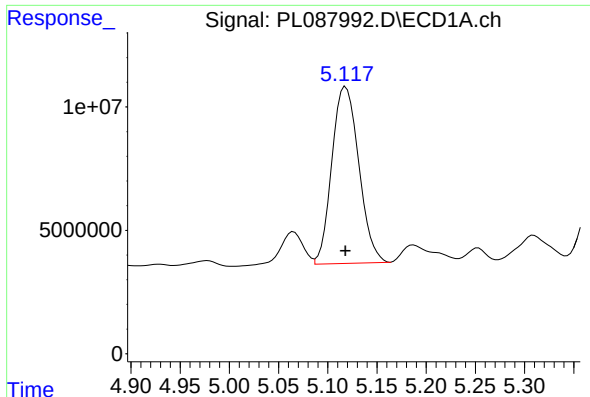

#24 Chlordane-2


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 136550843
Conc: 992.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

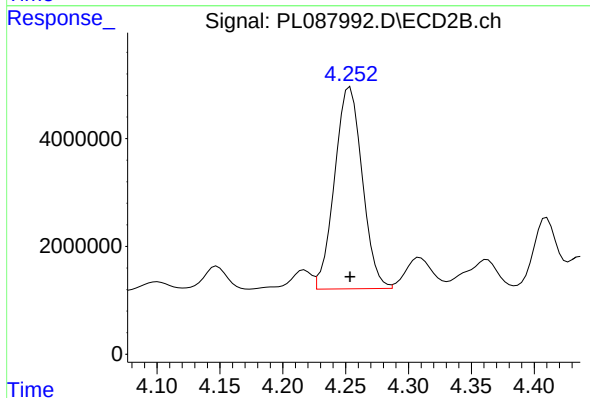


#24 Chlordane-2

R.T.: 4.253 min
Delta R.T.: 0.000 min
Response: 57281629
Conc: 993.07 ng/ml

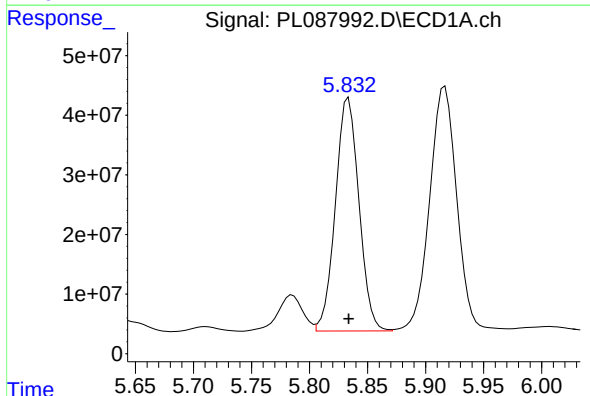


#25 Chlordane-3

R.T.: 5.834 min
Delta R.T.: 0.000 min
Response: 552827780
Conc: 1023.37 ng/ml

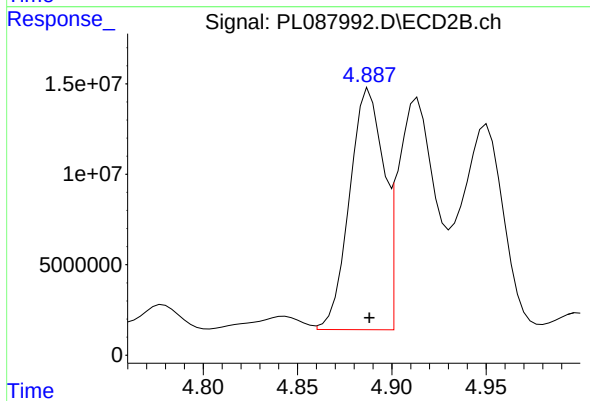

#25 Chlordane-3


R.T.: 4.888 min
Delta R.T.: 0.000 min
Response: 166840222
Conc: 1028.95 ng/ml

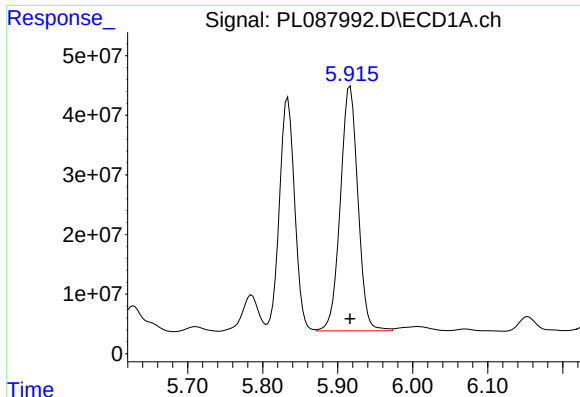

#26 Chlordane-4


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 668686952
Conc: 1014.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

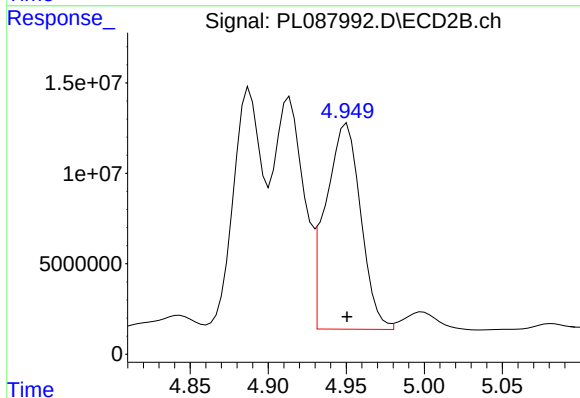


#26 Chlordane-4

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 176811887
Conc: 1030.77 ng/ml

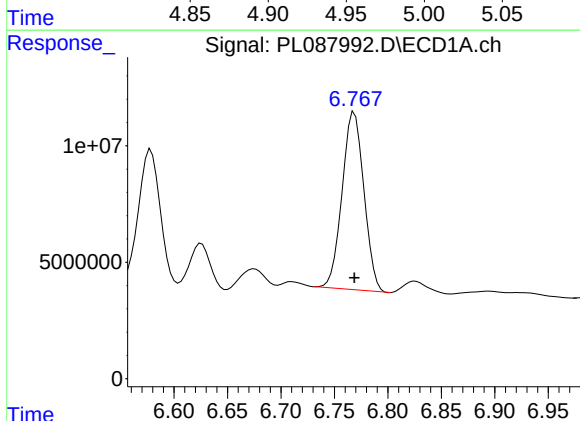


#27 Chlordane-5

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 108502282
Conc: 1006.33 ng/ml

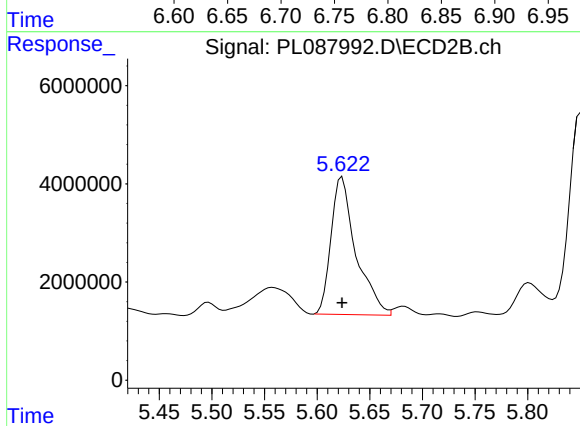

#27 Chlordane-5

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 46083419
Conc: 1010.01 ng/ml

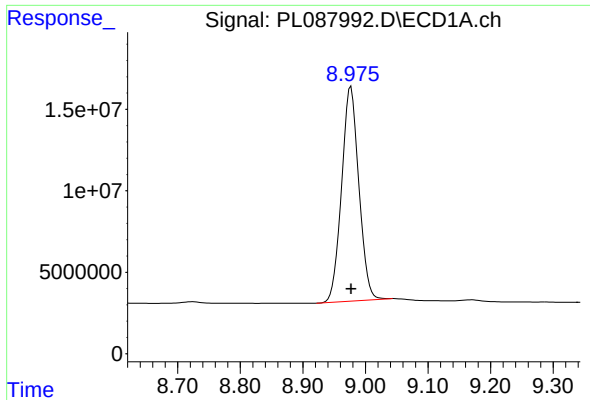

#28 Decachlorobiphenyl


R.T.: 8.977 min

Delta R.T.: 0.000 min

Response: 252821712

Conc: 97.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

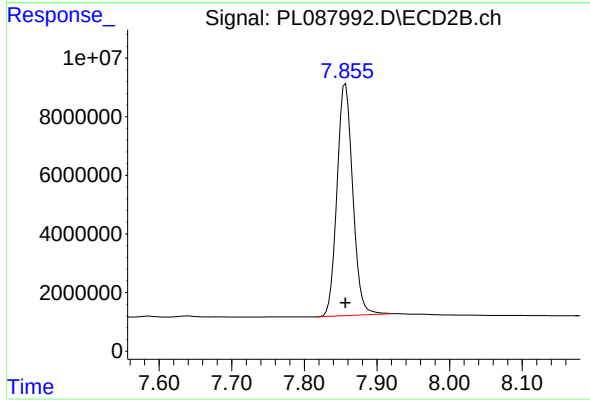

#28 Decachlorobiphenyl

R.T.: 7.857 min

Delta R.T.: 0.000 min

Response: 119021956

Conc: 97.80 ng/ml