

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
 Data File : PL087993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 21:54
 Operator : AR\AJ
 Sample : PCHLORICC750 (Sig #1); CHLORICC750 (Sig #2)
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:35:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 00:34:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.670	222.6E6	122.0E6	74.988	74.923
28)	SA Decachlor...	8.977	7.857	192.0E6	90156894	74.387	74.386
Target Compounds							
23)	Chlordane-1	4.583	3.671	96400811	34734276	746.192	747.230
24)	Chlordane-2	5.118	4.254	102.4E6	43005072	746.025	747.037
25)	Chlordane-3	5.833	4.888	402.5E6	121.3E6	746.748	748.742
26)	Chlordane-4	5.916	4.950	490.5E6	127.4E6	746.253	744.979
27)	Chlordane-5	6.769	5.624	80265962	33987980	746.290	746.603



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
Data File : PL087993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 21:54
Operator : AR\AJ
Sample : PCHLORICC750 (Sig #1); CHLORICC750 (Sig #2)
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:35:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 00:34:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

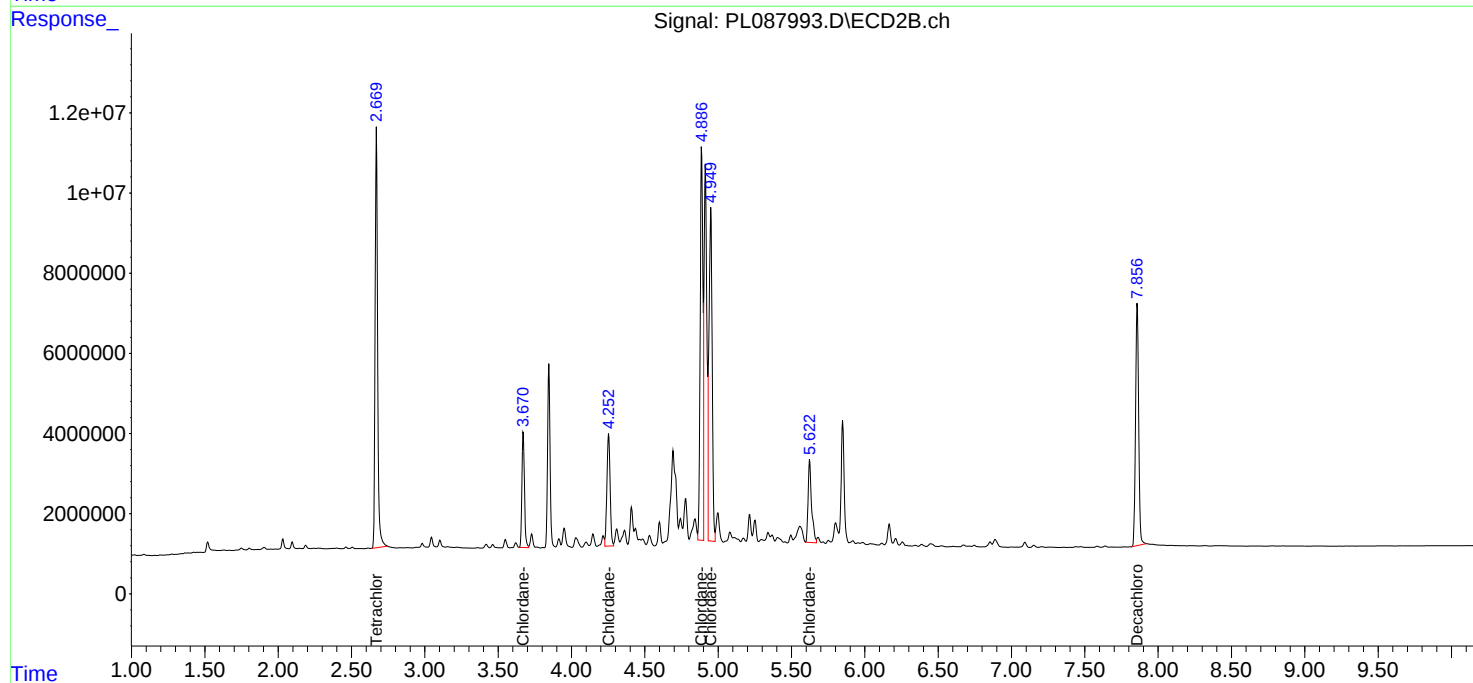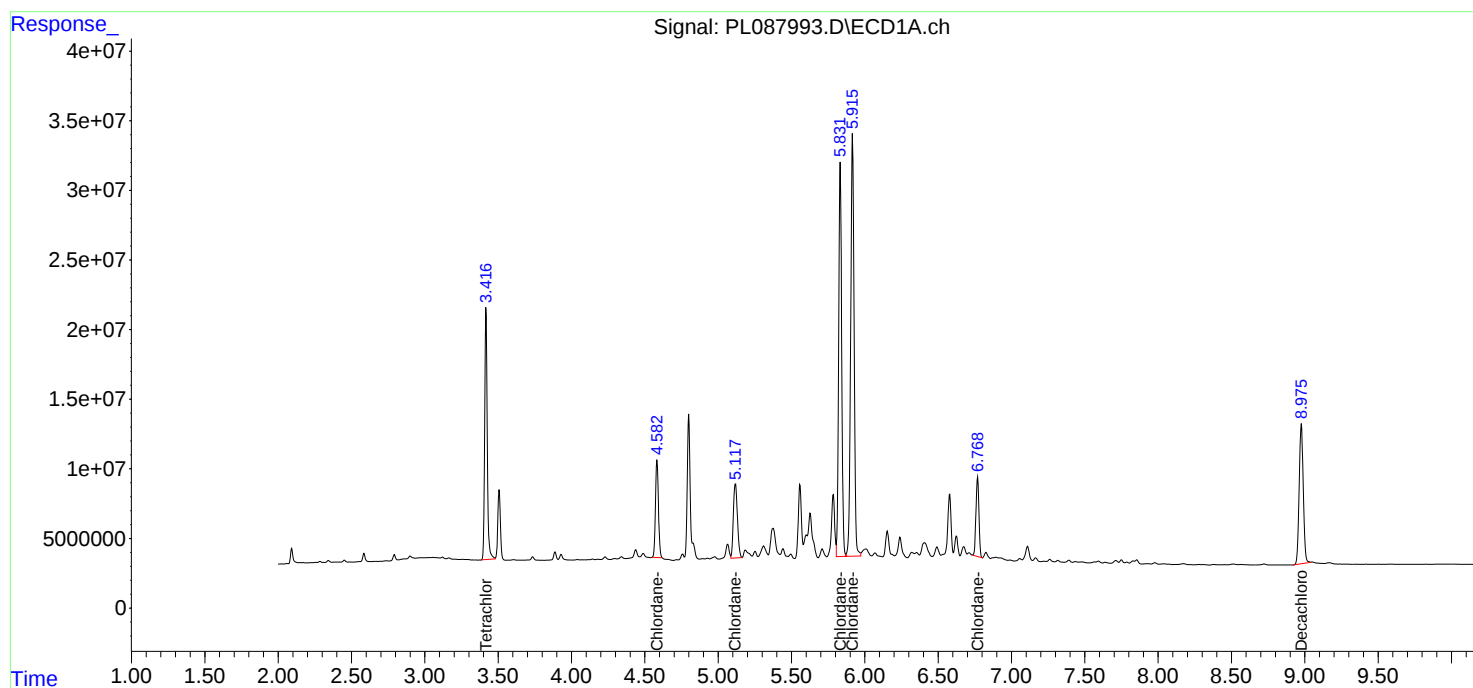


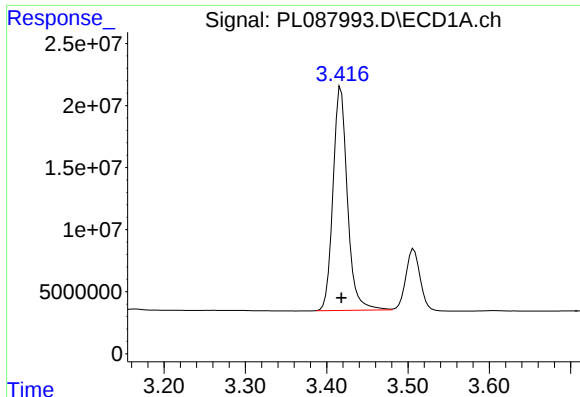

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.000 min
Response: 222571941
Conc: 74.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

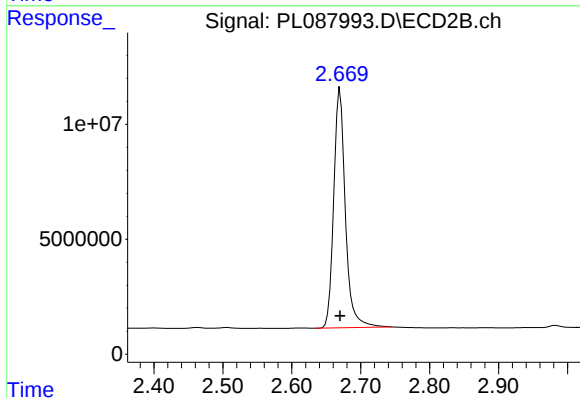


#1 Tetrachloro-m-xylene

R.T.: 2.670 min
Delta R.T.: 0.000 min
Response: 122019059
Conc: 74.92 ng/ml

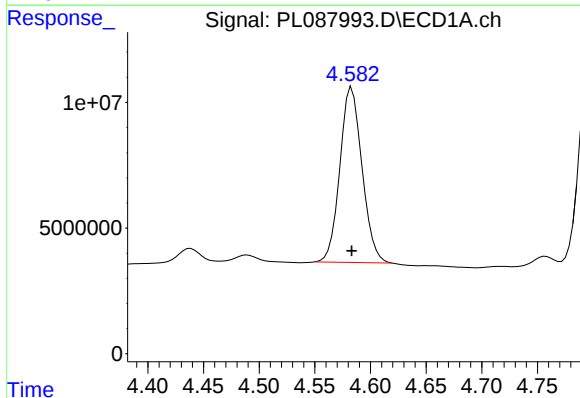


#23 Chlordane-1

R.T.: 4.583 min
Delta R.T.: 0.000 min
Response: 96400811
Conc: 746.19 ng/ml

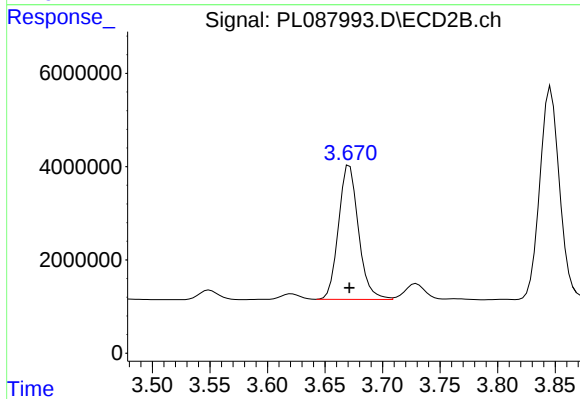

#23 Chlordane-1


R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 34734276
Conc: 747.23 ng/ml

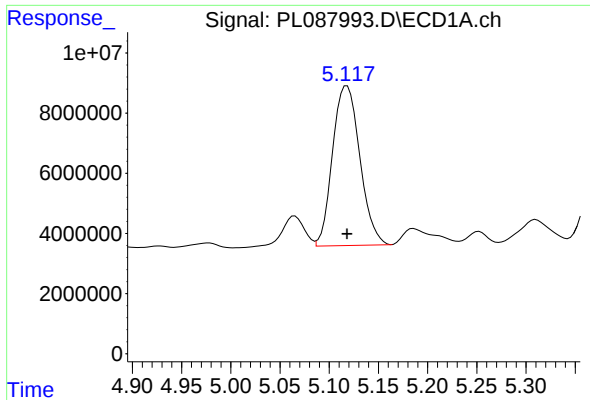

#24 Chlordane-2


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 102415640
Conc: 746.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

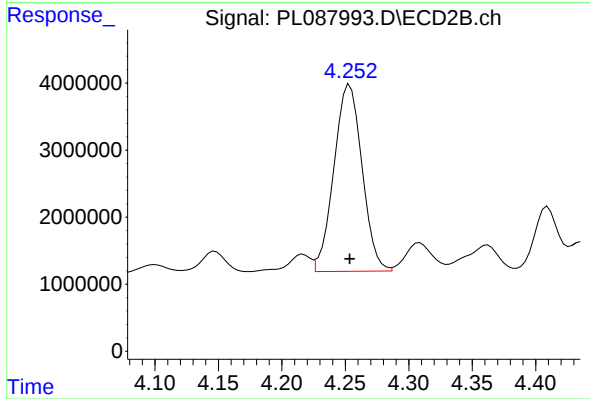


#24 Chlordane-2

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 43005072
Conc: 747.04 ng/ml

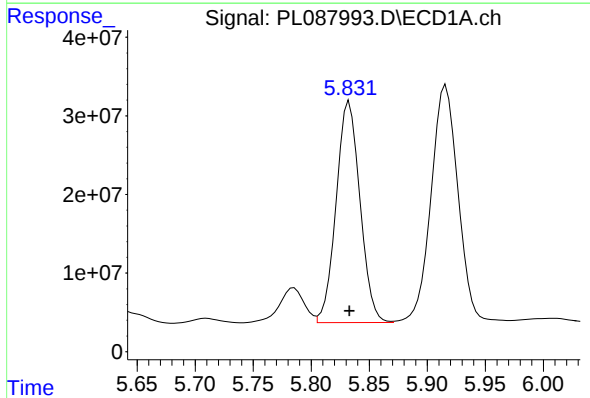


#25 Chlordane-3

R.T.: 5.833 min
Delta R.T.: 0.000 min
Response: 402522128
Conc: 746.75 ng/ml

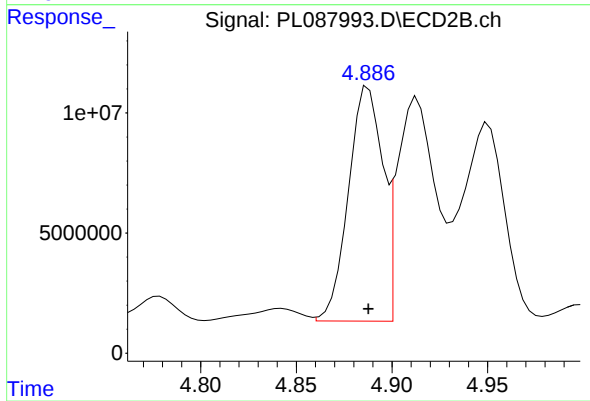

#25 Chlordane-3


R.T.: 4.888 min
Delta R.T.: 0.000 min
Response: 121304194
Conc: 748.74 ng/ml

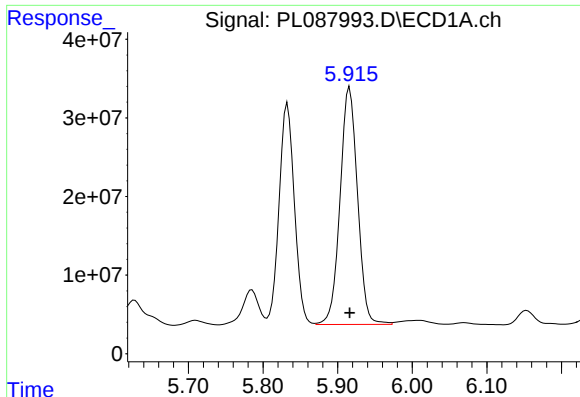

#26 Chlordane-4


R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 490536515
Conc: 746.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

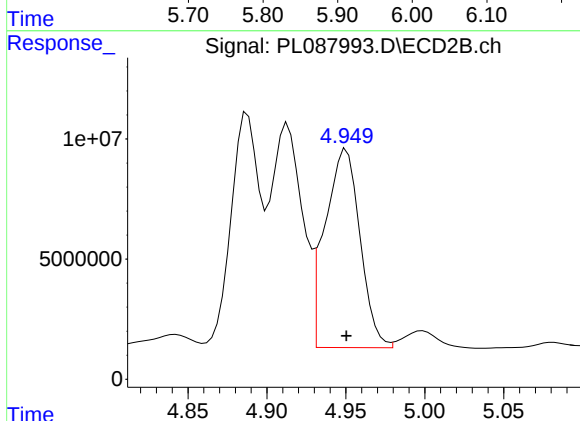


#26 Chlordane-4

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 127362718
Conc: 744.98 ng/ml

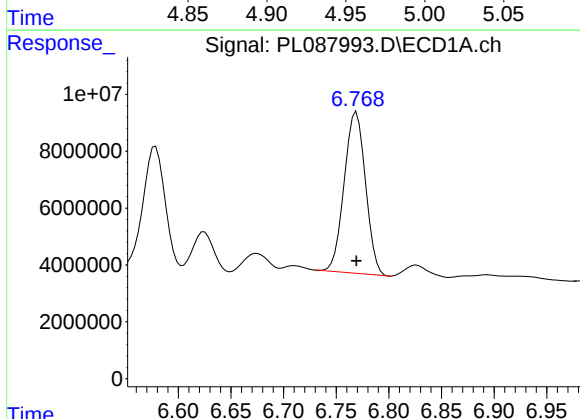


#27 Chlordane-5

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 80265962
Conc: 746.29 ng/ml

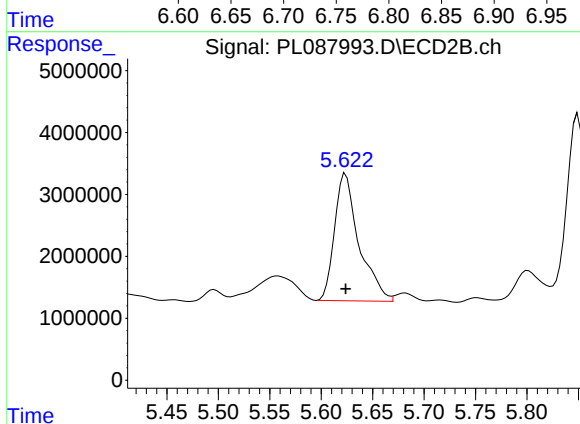

#27 Chlordane-5


R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 33987980
Conc: 746.60 ng/ml

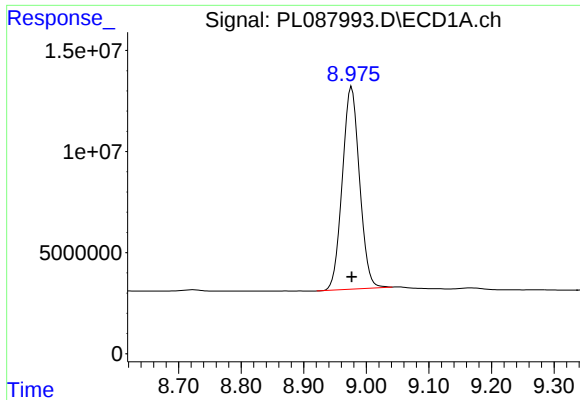

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.000 min
Response: 191951538
Conc: 74.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

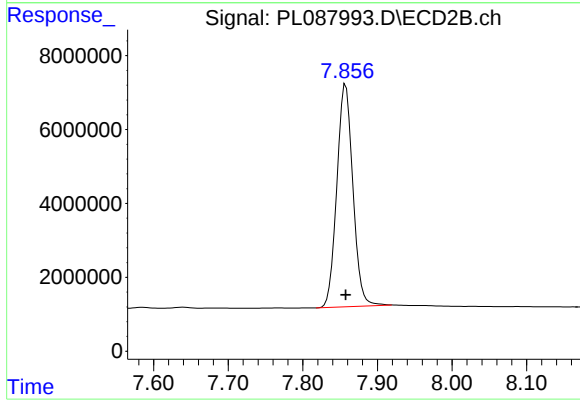

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.000 min
Response: 90156894
Conc: 74.39 ng/ml