

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
 Data File : PL087995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 22:22
 Operator : AR\AJ
 Sample : PCHLORICC250 (Sig #1); CHLORICC250 (Sig #2)
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:36:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 00:36:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.671	73232817	39615391	24.754	24.490
28)	SA Decachlor...	8.978	7.857	71518673	33414813	26.983	26.879
Target Compounds							
23)	Chlordane-1	4.584	3.672	32364395	11340824	250.388	245.452
24)	Chlordane-2	5.118	4.254	36277058	15300458	260.539	261.653
25)	Chlordane-3	5.833	4.888	130.4E6	38485286	243.931	240.543
26)	Chlordane-4	5.917	4.951	162.8E6	40572022	248.227	240.365
27)	Chlordane-5	6.769	5.624	27445696	11350279	253.867	249.496



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
Data File : PL087995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 22:22
Operator : AR\AJ
Sample : PCHLORICC250 (Sig #1); CHLORICC250 (Sig #2)
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:36:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 00:36:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

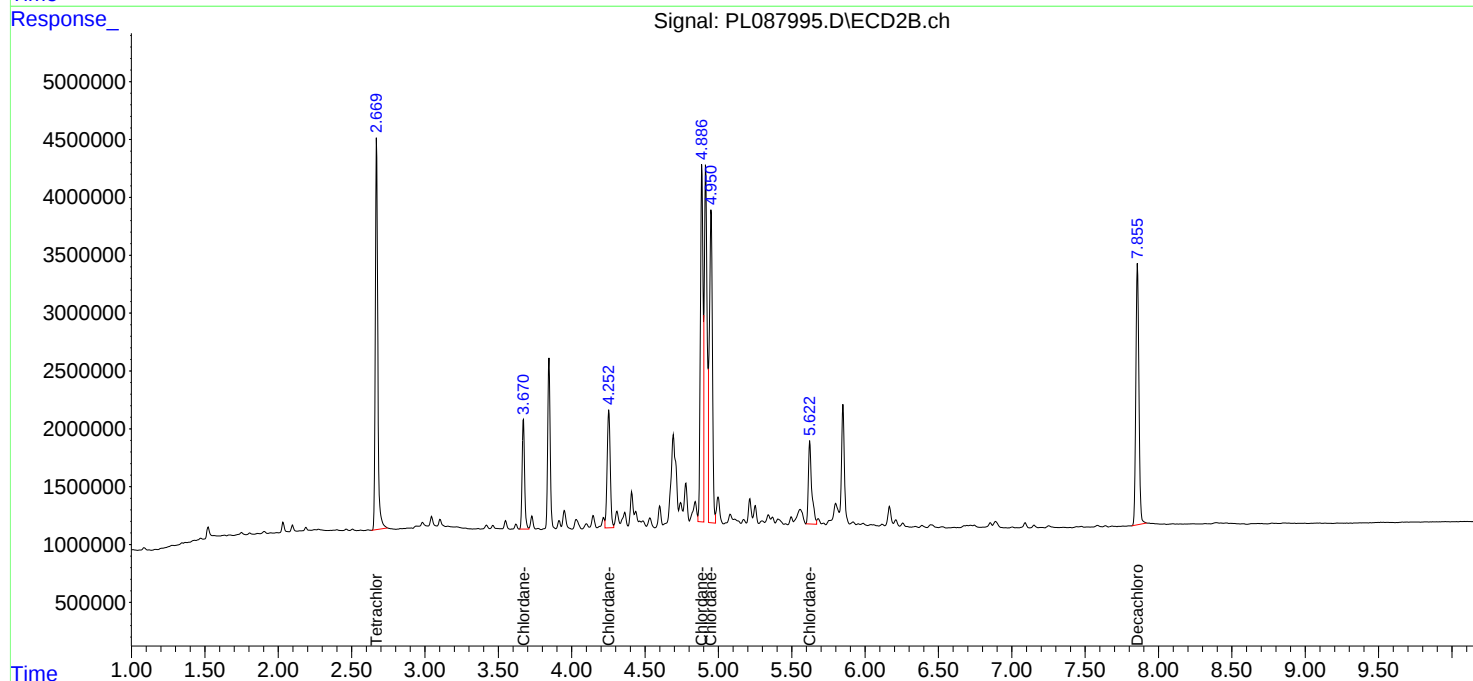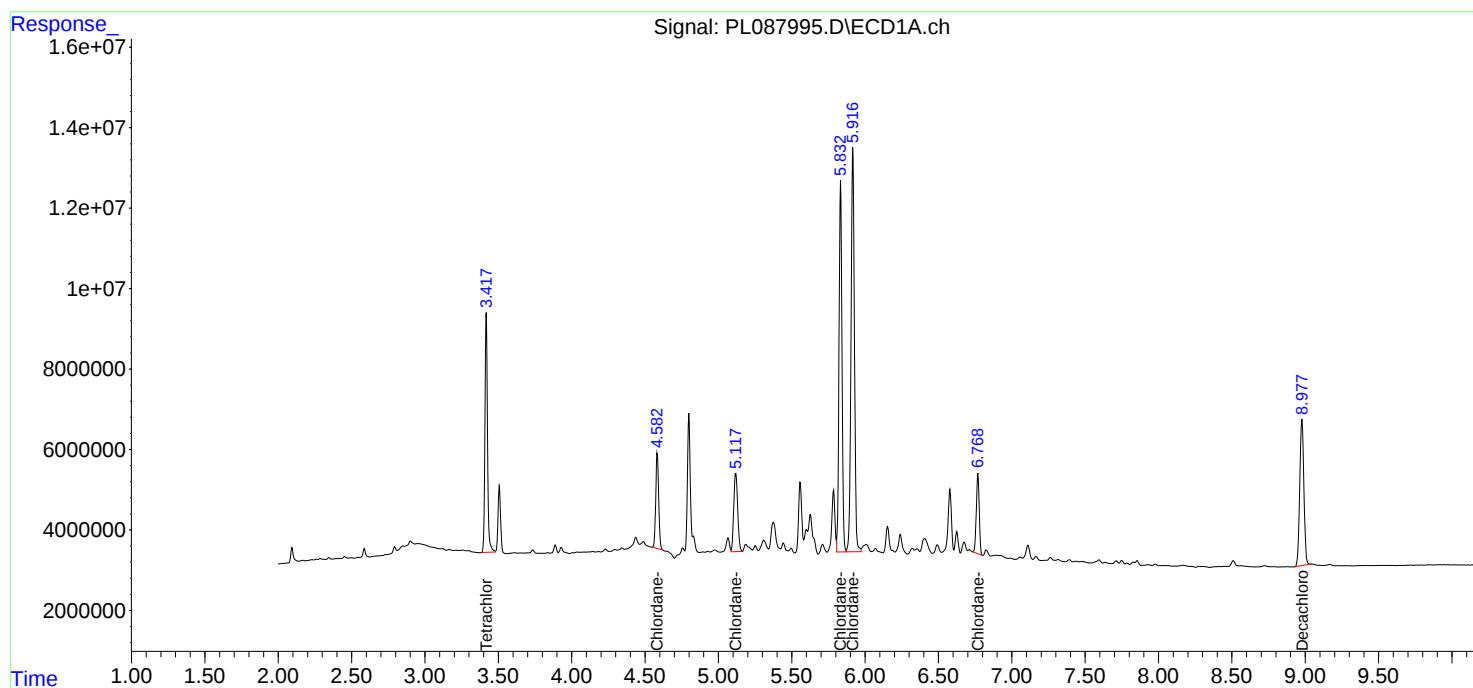


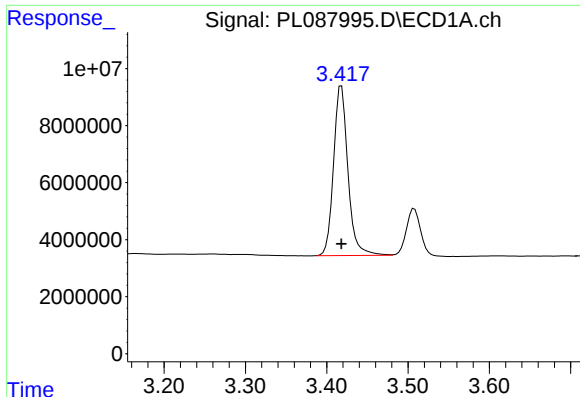

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.000 min
Response: 73232817
Conc: 24.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

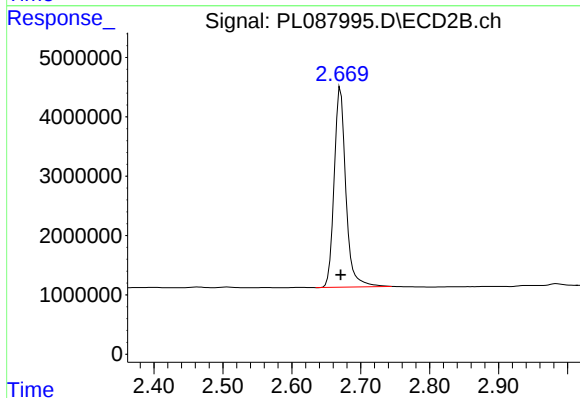


#1 Tetrachloro-m-xylene

R.T.: 2.671 min
Delta R.T.: 0.000 min
Response: 39615391
Conc: 24.49 ng/ml

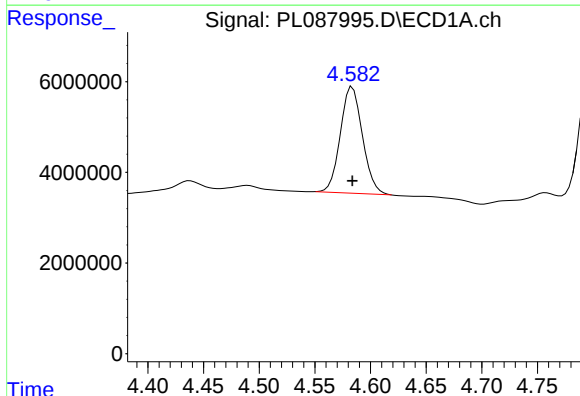


#23 Chlordane-1

R.T.: 4.584 min
Delta R.T.: 0.000 min
Response: 32364395
Conc: 250.39 ng/ml

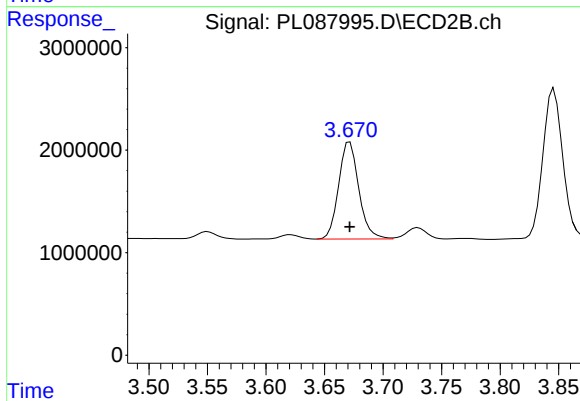

#23 Chlordane-1


R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 11340824
Conc: 245.45 ng/ml

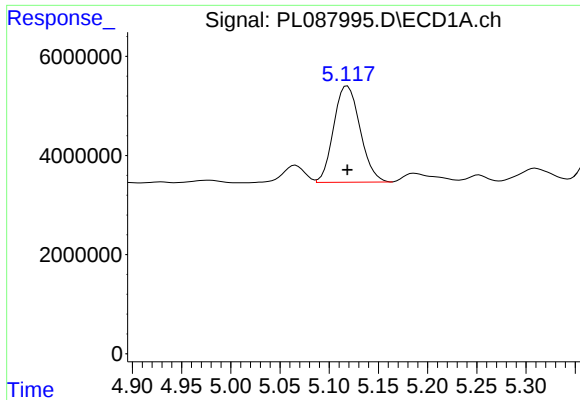

#24 Chlordane-2


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 36277058
Conc: 260.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

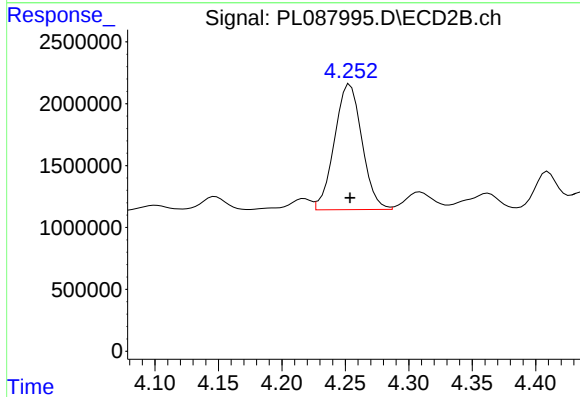


#24 Chlordane-2

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 15300458
Conc: 261.65 ng/ml

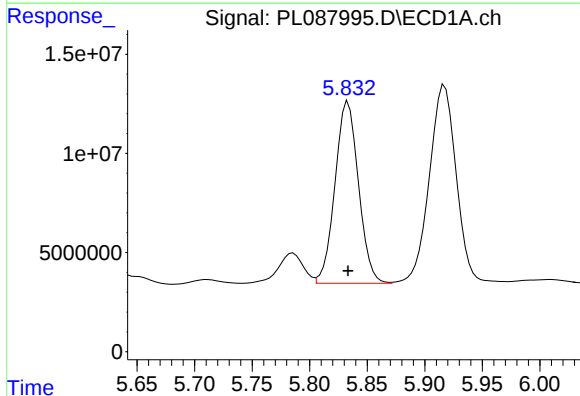


#25 Chlordane-3

R.T.: 5.833 min
Delta R.T.: 0.000 min
Response: 130431647
Conc: 243.93 ng/ml

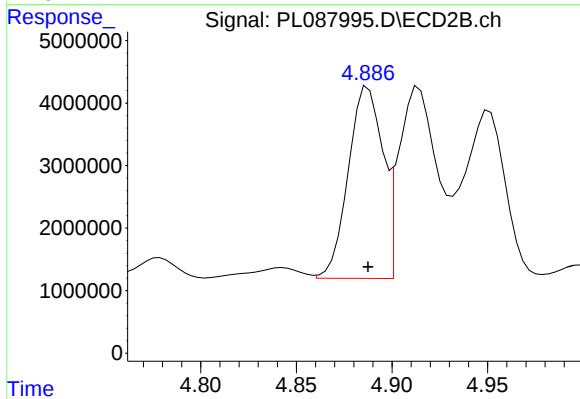

#25 Chlordane-3


R.T.: 4.888 min
Delta R.T.: 0.000 min
Response: 38485286
Conc: 240.54 ng/ml

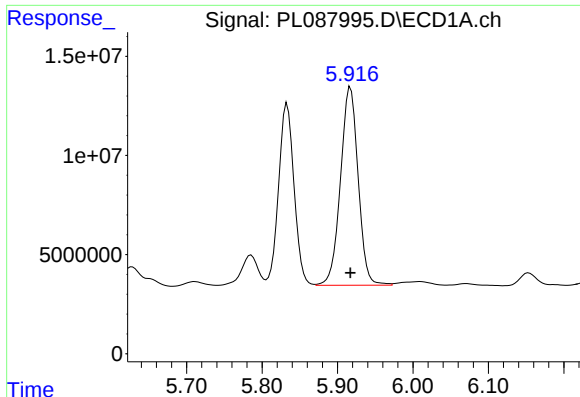

#26 Chlordane-4


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 162782832
Conc: 248.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

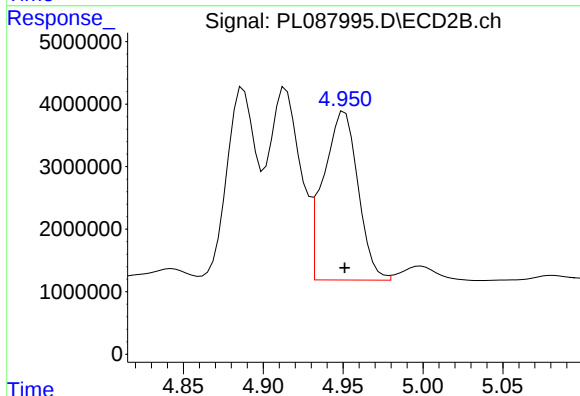


#26 Chlordane-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 40572022
Conc: 240.37 ng/ml

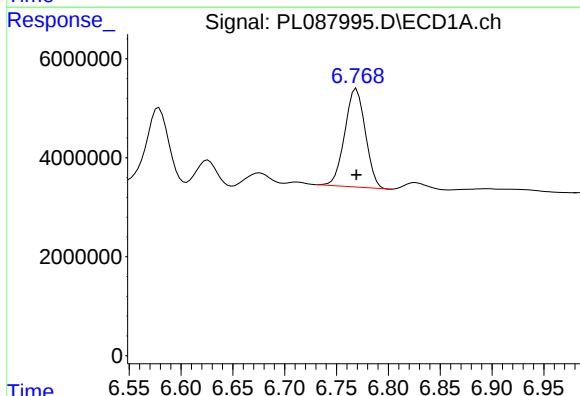


#27 Chlordane-5

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 27445696
Conc: 253.87 ng/ml

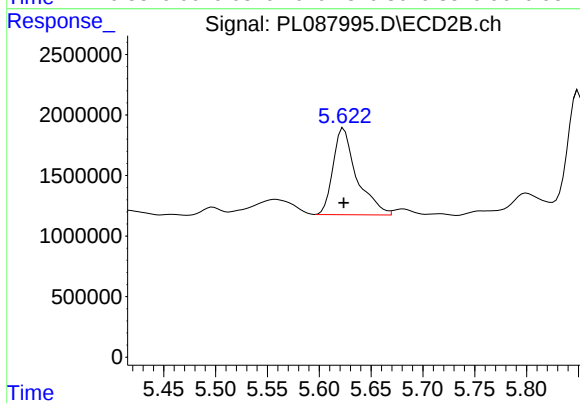

#27 Chlordane-5


R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 11350279
Conc: 249.50 ng/ml

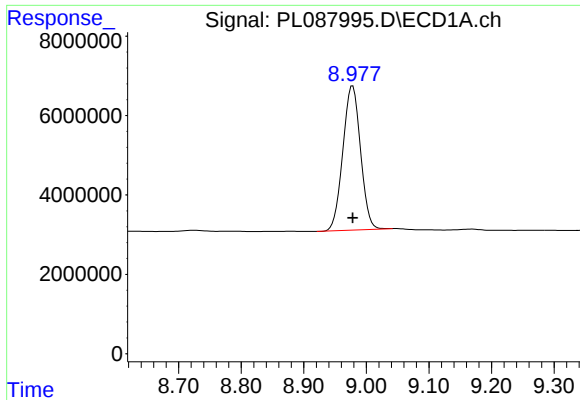

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.000 min
Response: 71518673
Conc: 26.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

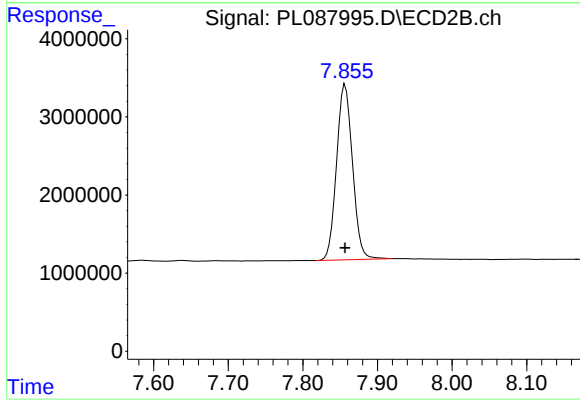

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.000 min
Response: 33414813
Conc: 26.88 ng/ml