

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
 Data File : PL087996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 22:36
 Operator : AR\AJ
 Sample : PCHLORICC050 (Sig #1); CHLORICC050 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:38:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 00:37:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.670	15371285	7953950	5.155	4.933
28)	SA Decachlor...	8.978	7.857	16204115	7387290	5.853	5.727
Target Compounds							
23)	Chlordane-1	4.583	3.671	6820795	2297076	52.191	49.773
24)	Chlordane-2	5.118	4.253	7896895	3329607	55.231	55.402
25)	Chlordane-3	5.833	4.887	26613397	7501001	49.817	47.475
26)	Chlordane-4	5.917	4.950	33259480	8002109	50.572	47.905
27)	Chlordane-5	6.769	5.623	5783707	2304451	52.760	50.523



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012724\
Data File : PL087996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 22:36
Operator : AR\AJ
Sample : PCHLORICC050 (Sig #1); CHLORICC050 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:38:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 00:37:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

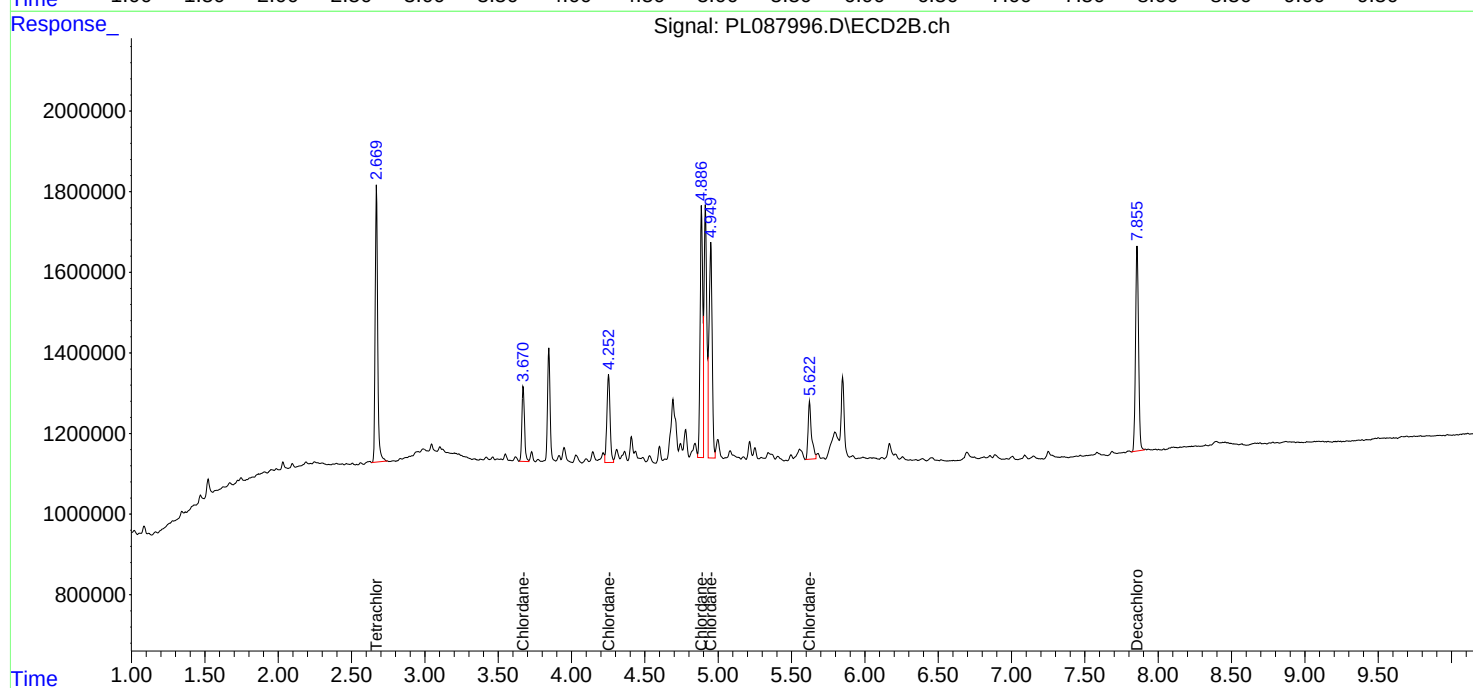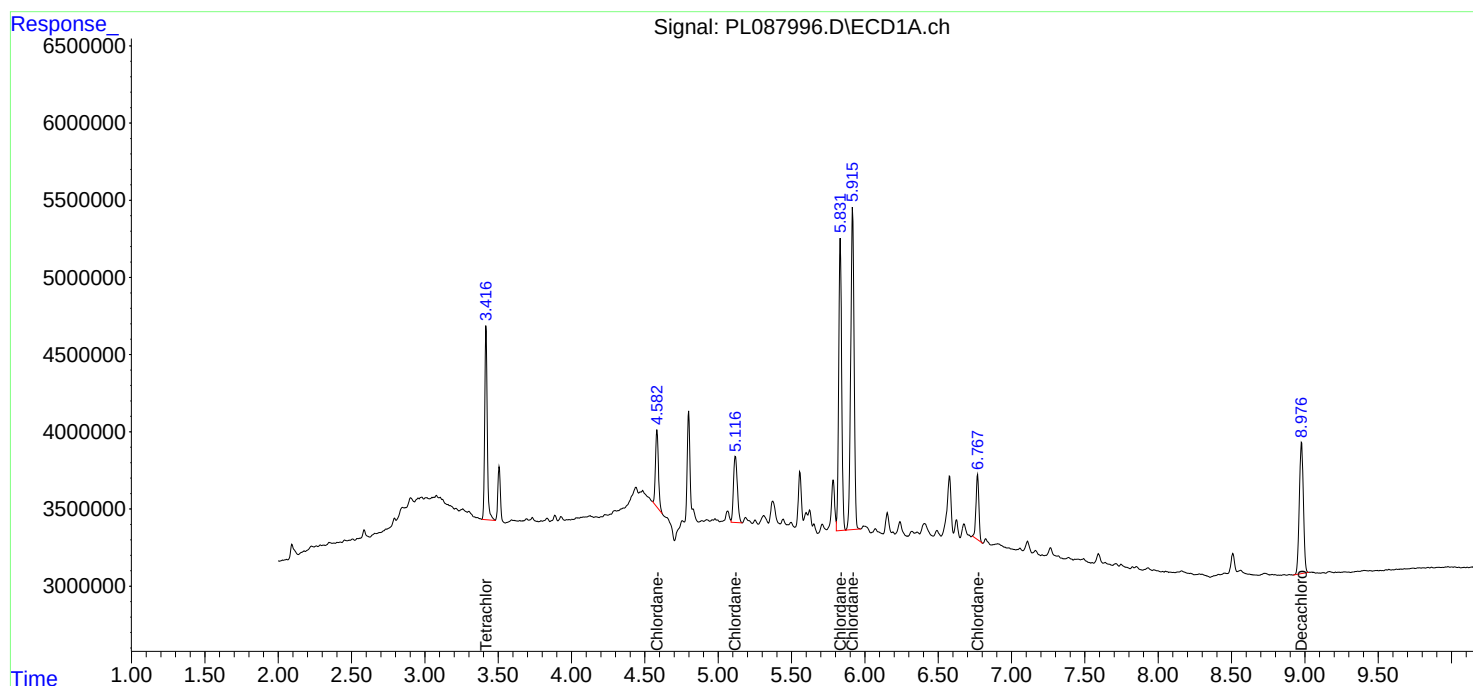


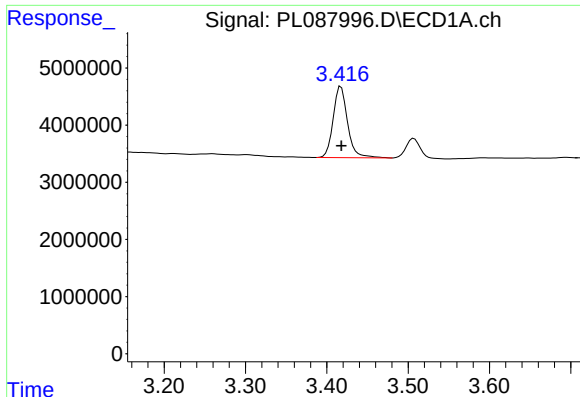

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: 0.000 min
Response: 15371285
Conc: 5.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

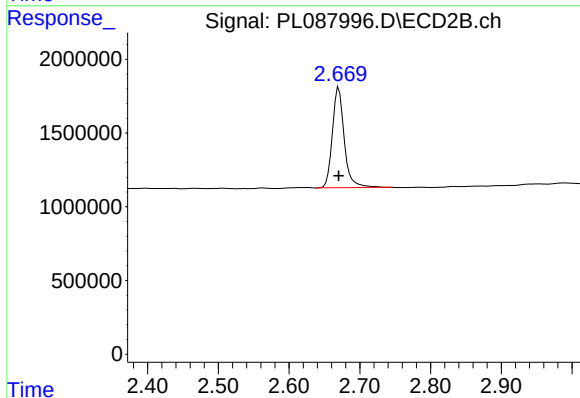


#1 Tetrachloro-m-xylene

R.T.: 2.670 min
Delta R.T.: 0.000 min
Response: 7953950
Conc: 4.93 ng/ml

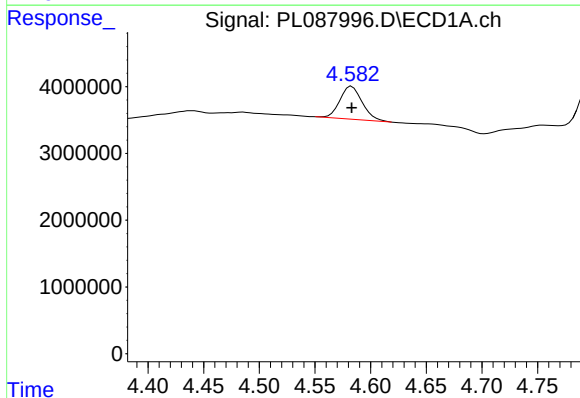


#23 Chlordane-1

R.T.: 4.583 min
Delta R.T.: 0.000 min
Response: 6820795
Conc: 52.19 ng/ml

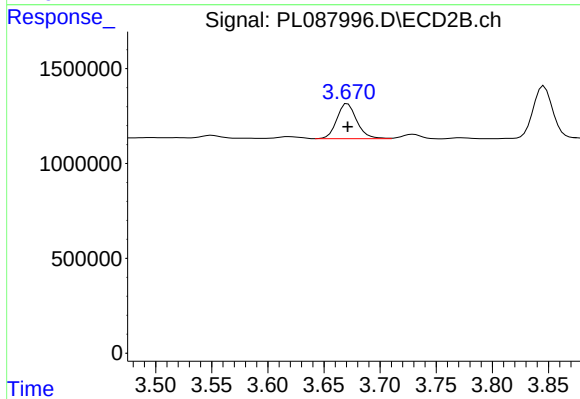

#23 Chlordane-1


R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 2297076
Conc: 49.77 ng/ml

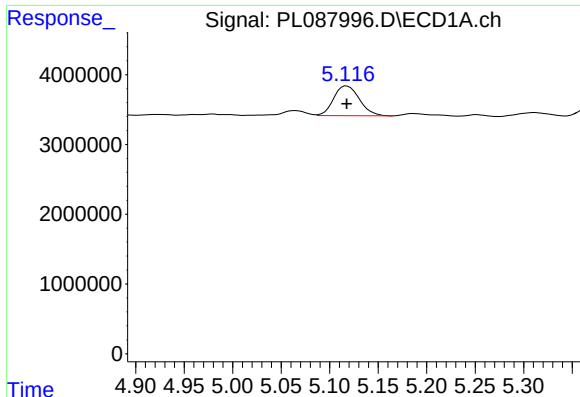

#24 Chlordane-2


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 7896895
Conc: 55.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

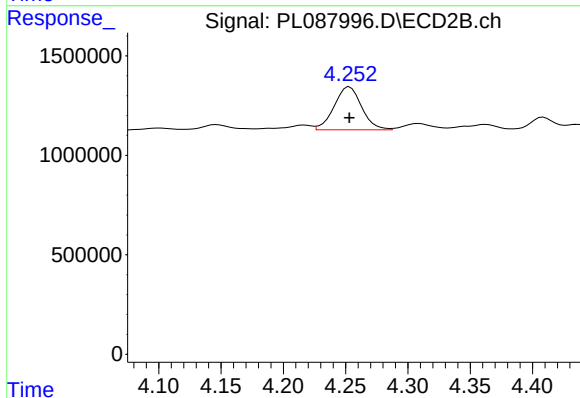


#24 Chlordane-2

R.T.: 4.253 min
Delta R.T.: 0.000 min
Response: 3329607
Conc: 55.40 ng/ml

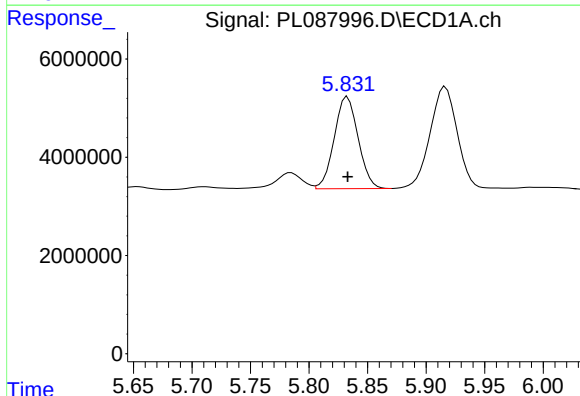


#25 Chlordane-3

R.T.: 5.833 min
Delta R.T.: 0.000 min
Response: 26613397
Conc: 49.82 ng/ml

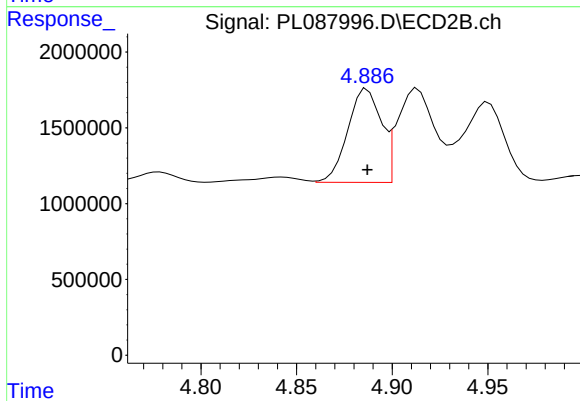

#25 Chlordane-3


R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 7501001
Conc: 47.48 ng/ml

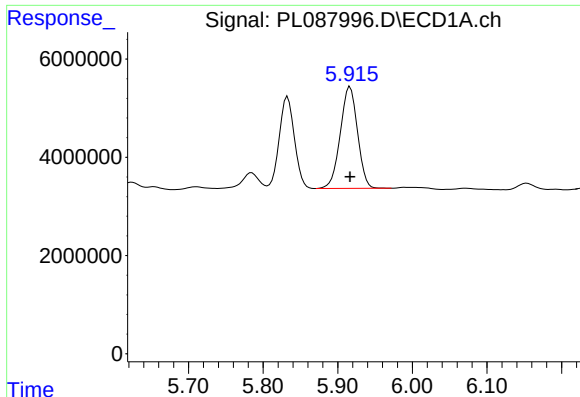

#26 Chlordane-4


R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 33259480
Conc: 50.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

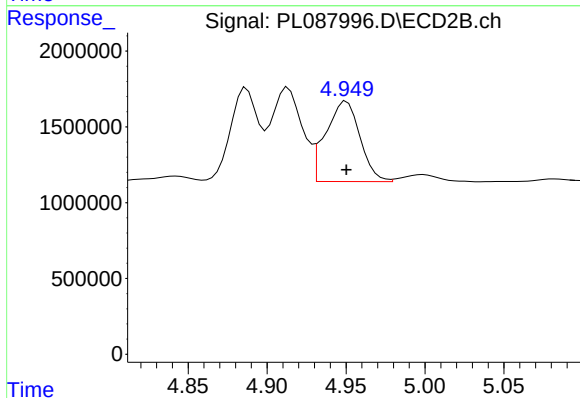


#26 Chlordane-4

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 8002109
Conc: 47.90 ng/ml

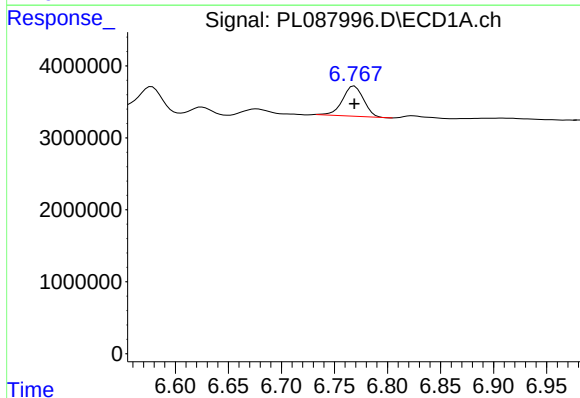


#27 Chlordane-5

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 5783707
Conc: 52.76 ng/ml

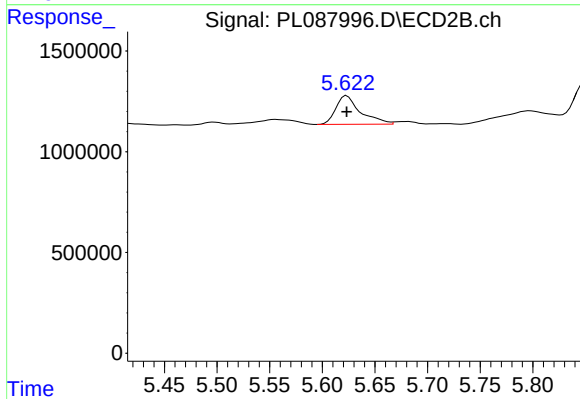

#27 Chlordane-5


R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 2304451
Conc: 50.52 ng/ml

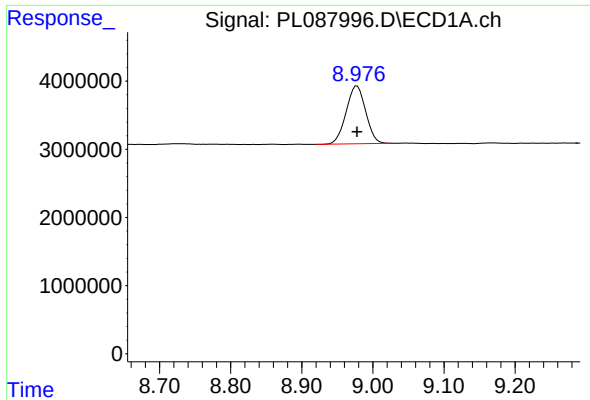

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.000 min
Response: 16204115
Conc: 5.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

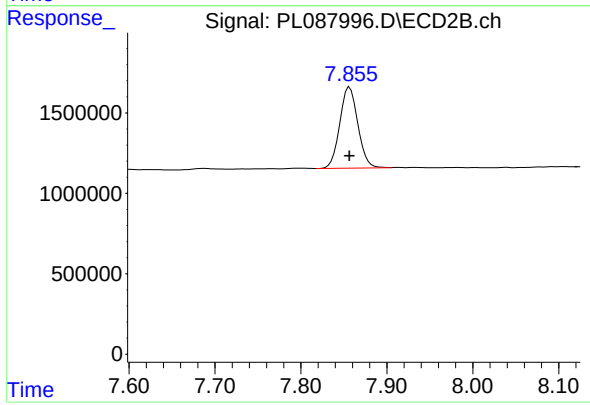

#28 Decachlorobiphenyl

R.T.: 7.857 min
Delta R.T.: 0.000 min
Response: 7387290
Conc: 5.73 ng/ml