

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012819\
 Data File : PL044268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2019 15:52
 Operator : AJ\SJ
 Sample : K1259-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-01-A01-B01-A01A-A01B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 23:59:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 28 01:20:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.366	3.986	120.4E6	42708586	19.872	19.579
28)	SA Decachlor...	8.052	9.046	116.7E6	39171756	16.832	17.658
Target Compounds							
6)	B beta-BHC	4.285f	0.000	7524676	0	2.170	N.D. #
8)	B Heptachlo...	0.000	5.842	0	4155150	N.D.	1.797 #
15)	B Endosulfa...	6.092f	0.000	22938978	0	3.400	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012819\
Data File : PL044268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2019 15:52
Operator : AJ\SJ
Sample : K1259-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-A01-B01-A01A-A01B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 23:59:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Mon Jan 28 01:20:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

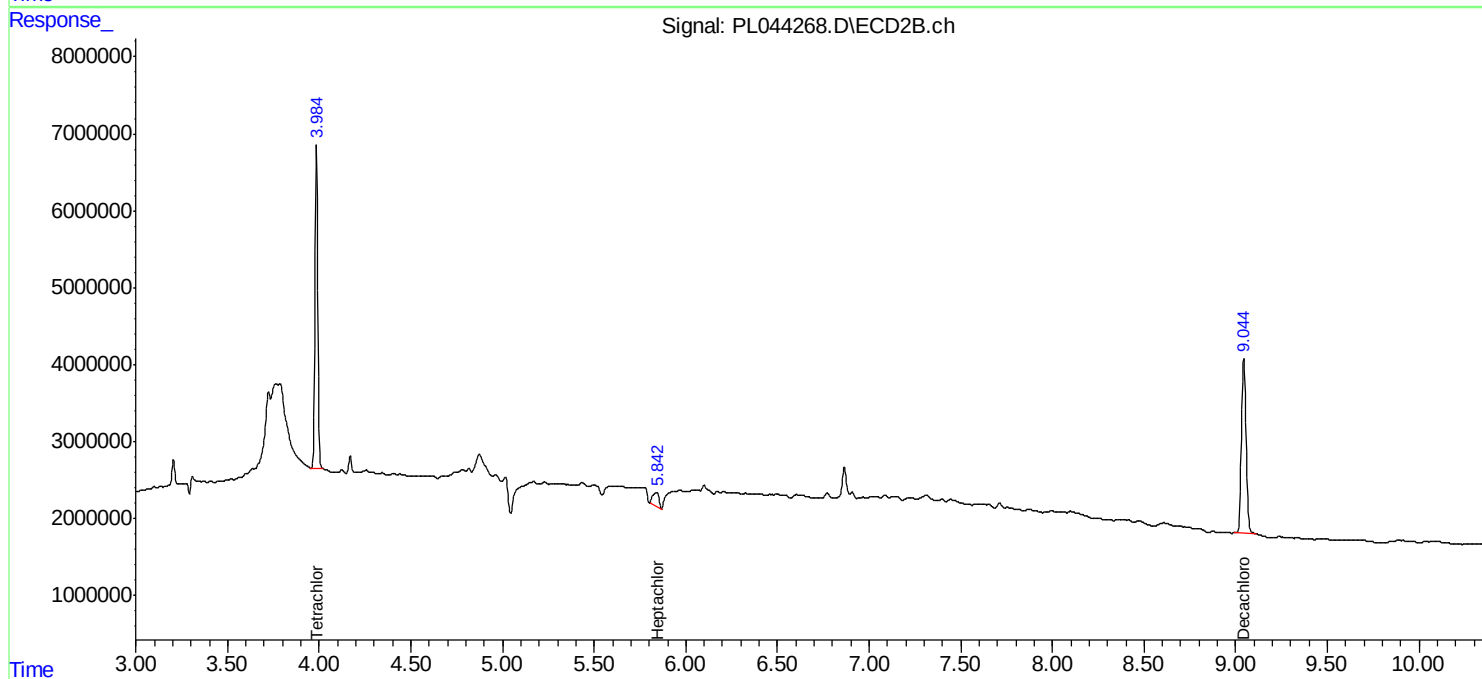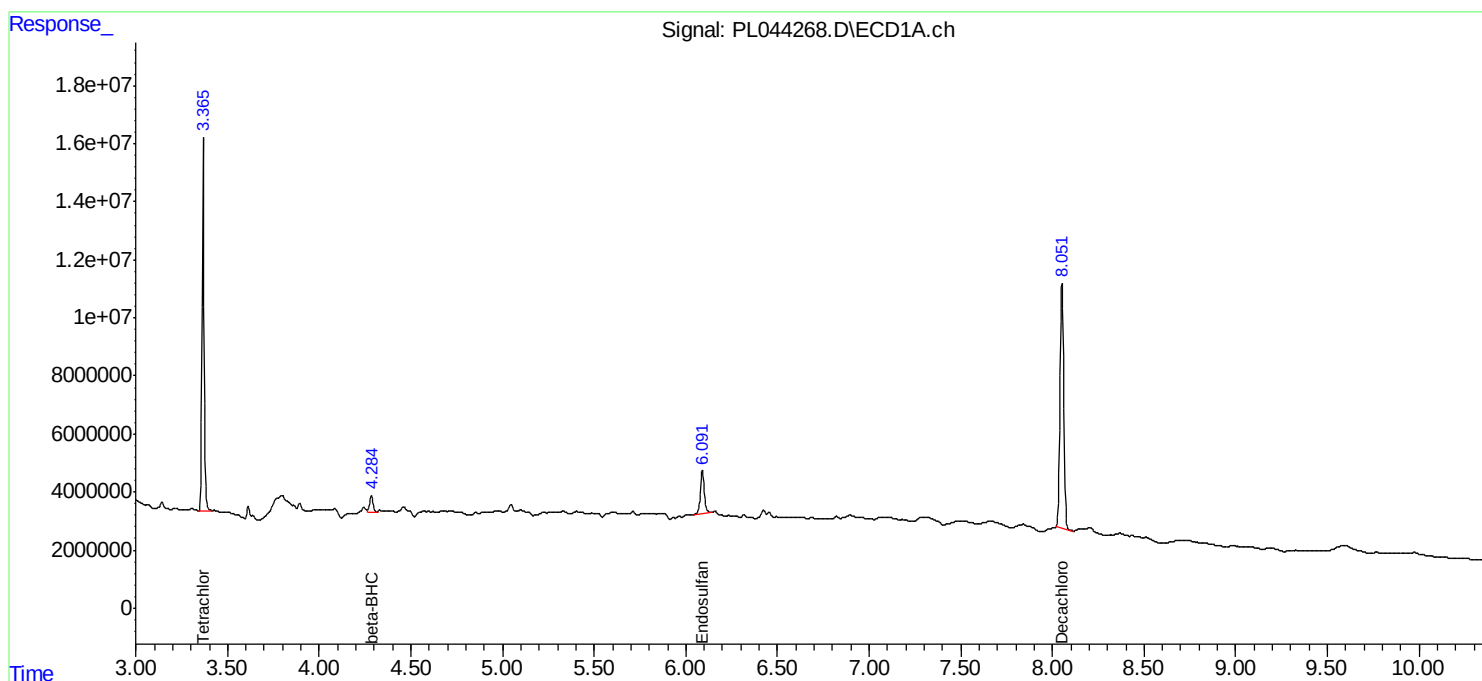


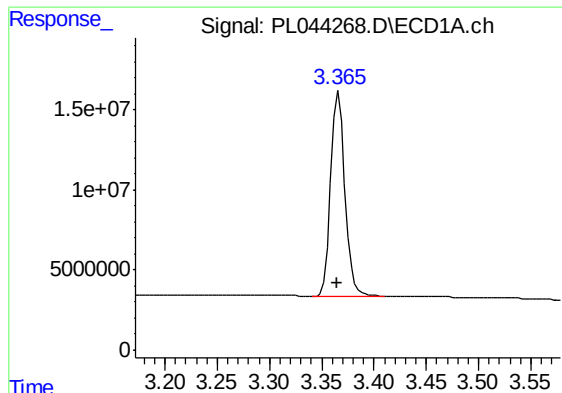

#1 Tetrachloro-m-xylene


R.T.: 3.366 min
Delta R.T.: 0.001 min
Response: 120430532
Conc: 19.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-A01-B01-A01A-A01B

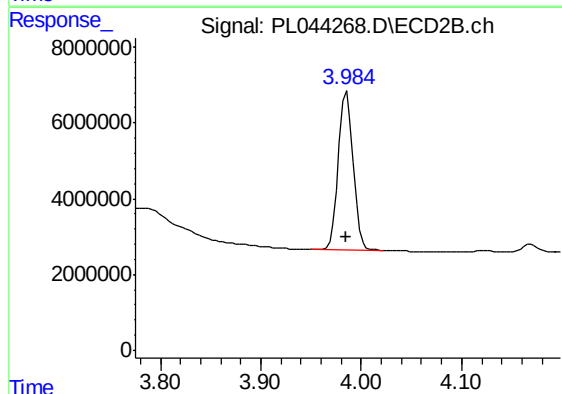


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.001 min
Response: 42708586
Conc: 19.58 ng/ml

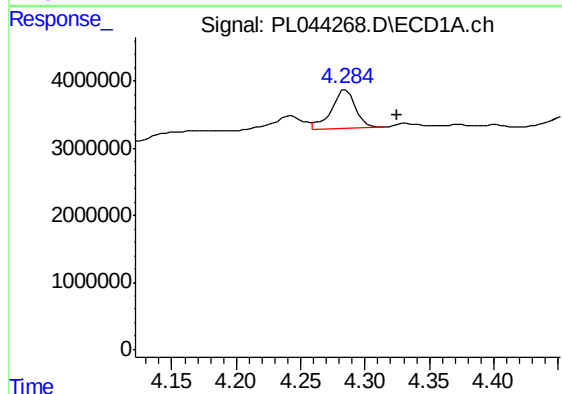


#6 beta-BHC

R.T.: 4.285 min
Delta R.T.: -0.040 min
Response: 7524676
Conc: 2.17 ng/ml

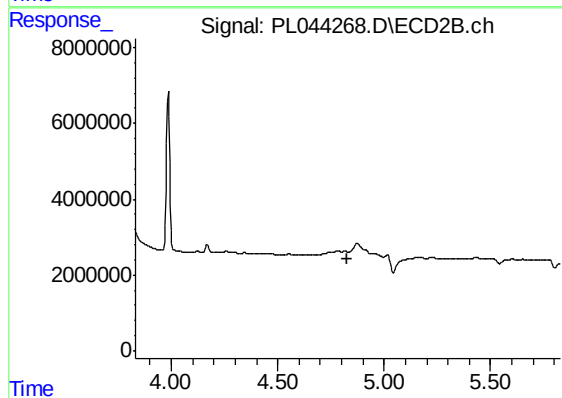

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.830 min
Response: 0
Conc: N.D.

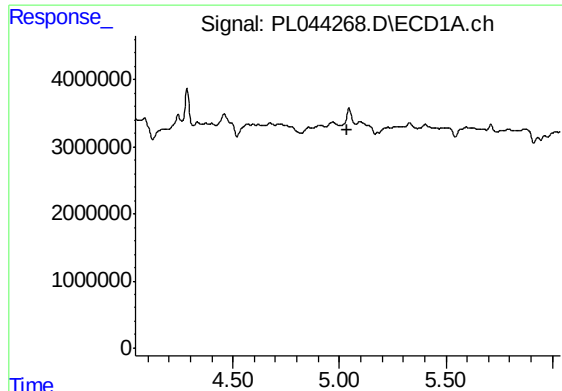

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-A01-B01-A01A-A01B

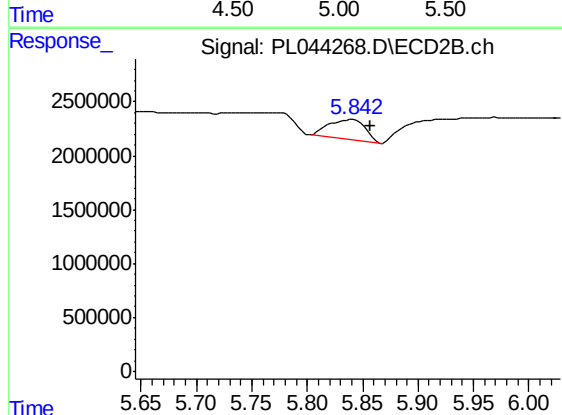


#8 Heptachlor epoxide

R.T.: 5.842 min
Delta R.T.: -0.015 min
Response: 4155150
Conc: 1.80 ng/ml

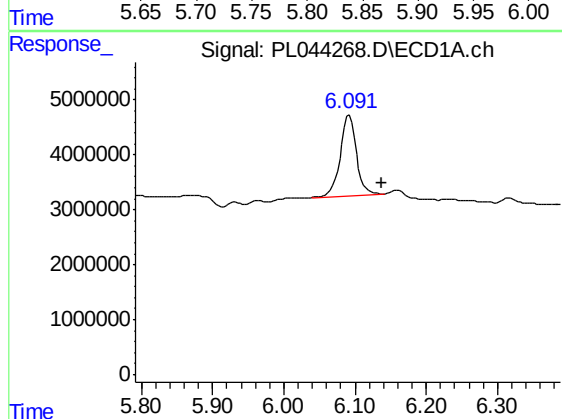


#15 Endosulfan II

R.T.: 6.092 min
Delta R.T.: -0.046 min
Response: 22938978
Conc: 3.40 ng/ml

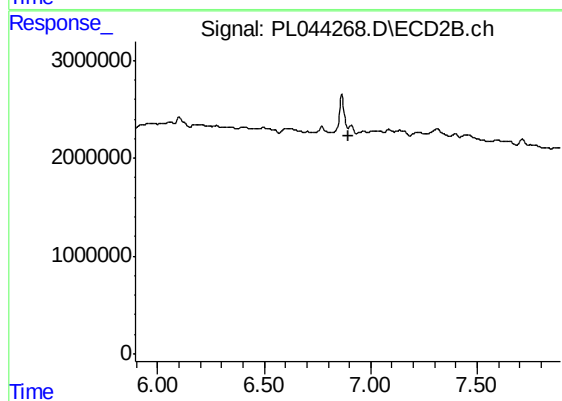

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

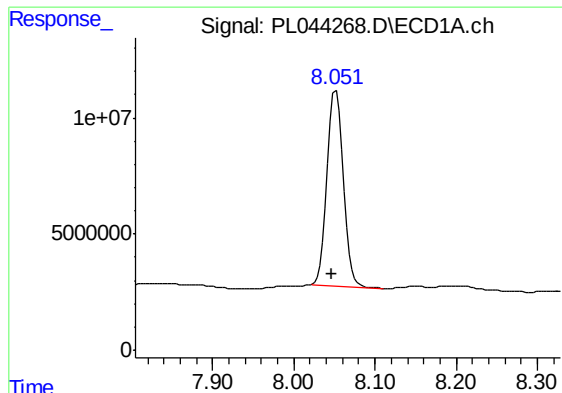

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.004 min
Response: 116728563
Conc: 16.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-A01-B01-A01A-A01B

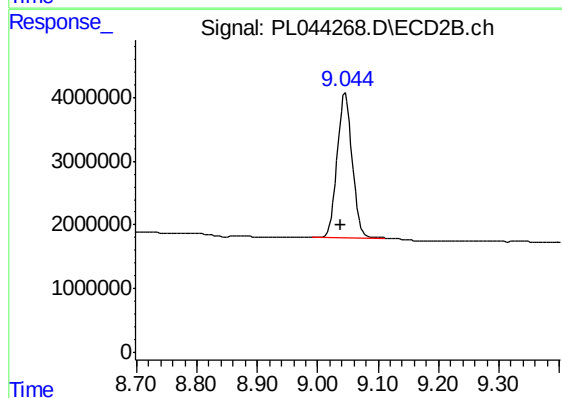

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: 0.006 min
Response: 39171756
Conc: 17.66 ng/ml