

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012819\
 Data File : PL044274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2019 17:16
 Operator : AJ\SJ
 Sample : K1261-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-C05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 00:01:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 28 01:20:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.986	119.8E6	43075540	19.765	19.748
28)	SA Decachlor...	8.052	9.047	113.6E6	34536012	16.381	15.568
Target Compounds							
3)	MA gamma-BHC...	0.000	4.641	0	1380308	N.D.	0.522 #
8)	B Heptachlo...	0.000	5.840	0	6381503	N.D.	2.759 #
9)	A Endosulfan I	5.402	6.252f	22848326	783410	3.243	0.338 #
10)	B gamma-Chl...	5.257	6.081	11184788	5628122	1.444	2.230 #
11)	B alpha-Chl...	5.257f	0.000	11184788	0	1.468	N.D. #
12)	B 4,4'-DDE	5.504	6.252f	7854876	783410	1.160	0.365 #
13)	MA Dieldrin	5.605	0.000	28191164	0	3.751	N.D. #
15)	B Endosulfa...	6.093f	0.000	16176398	0	2.398	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012819\
Data File : PL044274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2019 17:16
Operator : AJ\SJ
Sample : K1261-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
MH-C05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 00:01:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Mon Jan 28 01:20:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

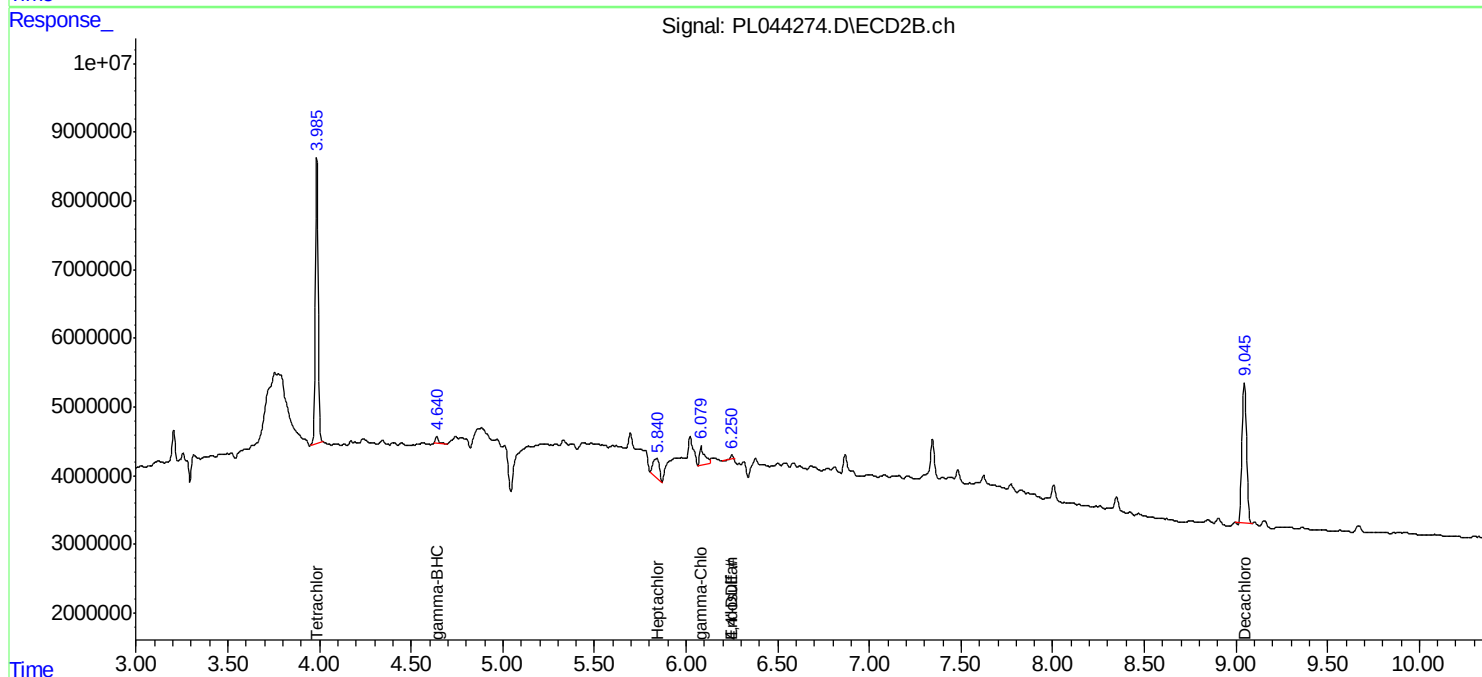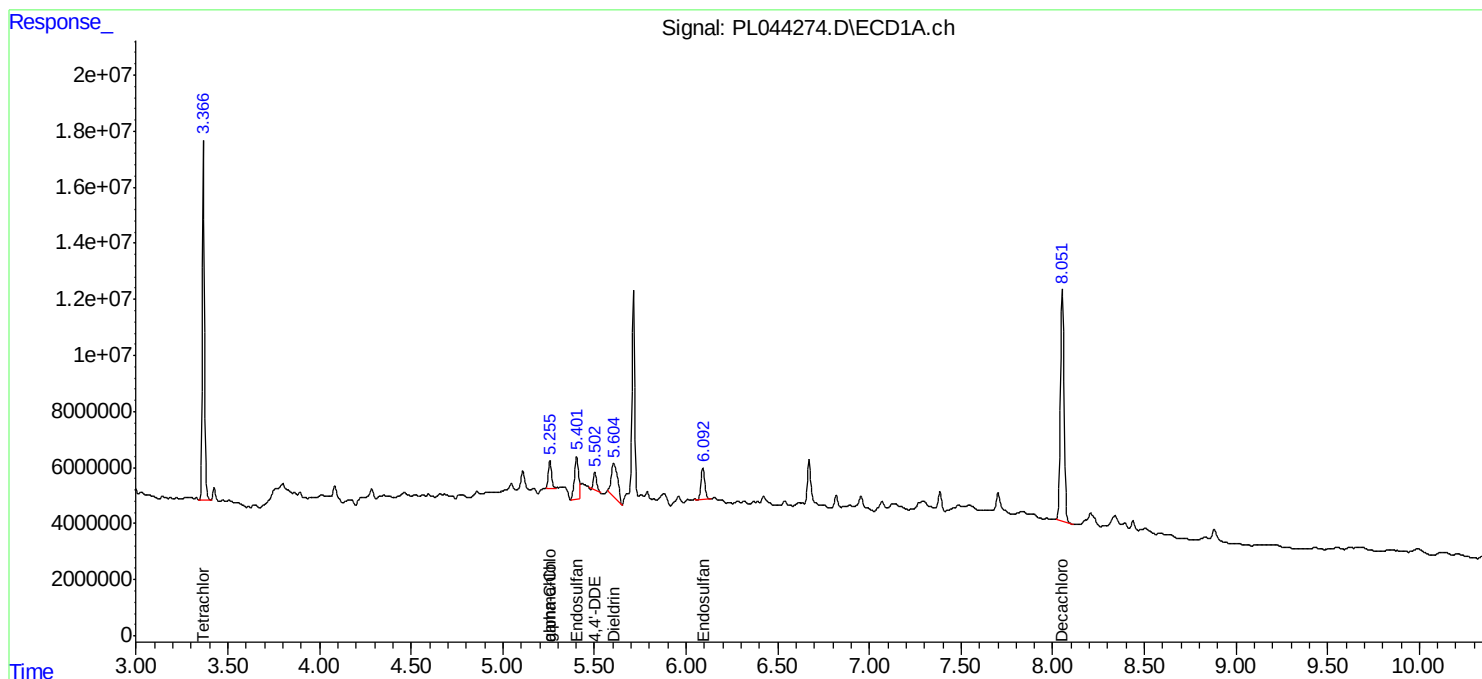


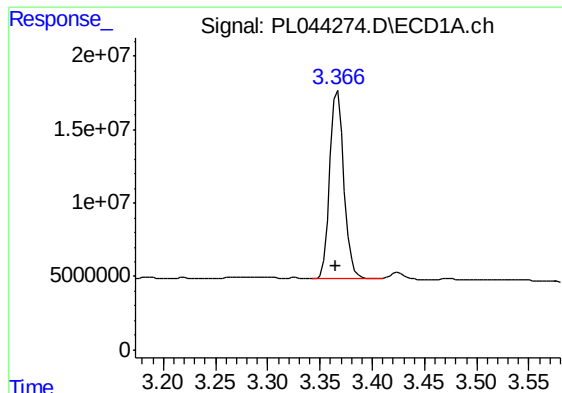

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.002 min
Response: 119783899
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-C05

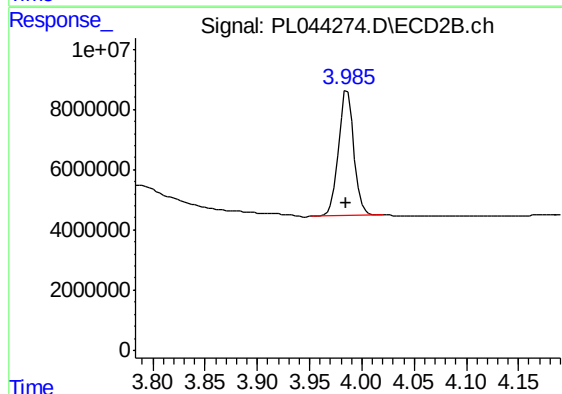


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.001 min
Response: 43075540
Conc: 19.75 ng/ml

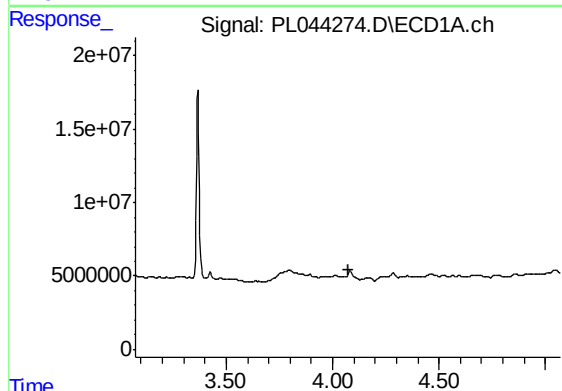


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.073 min
Response: 0
Conc: N.D.

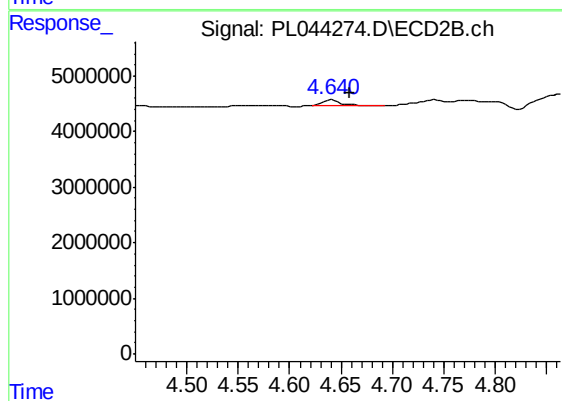

#3 gamma-BHC (Lindane)


R.T.: 4.641 min
Delta R.T.: -0.018 min
Response: 1380308
Conc: 0.52 ng/ml

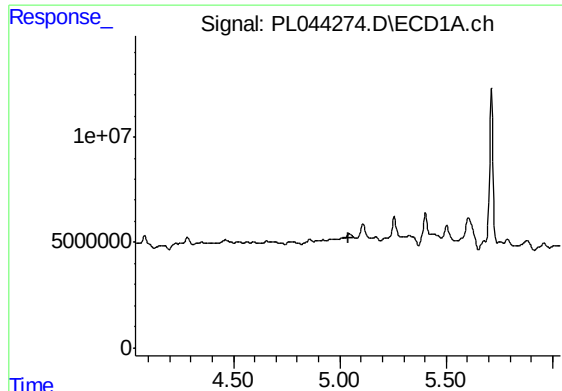

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.039 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MH-C05

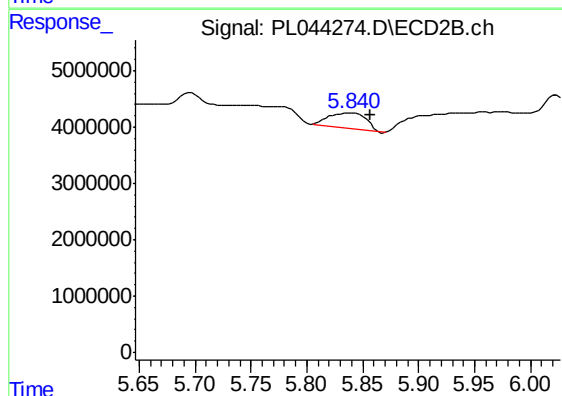


#8 Heptachlor epoxide

R.T.: 5.840 min
Delta R.T.: -0.017 min
Response: 6381503
Conc: 2.76 ng/ml

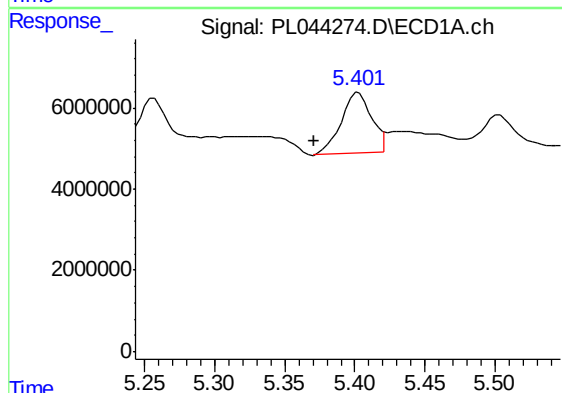


#9 Endosulfan I

R.T.: 5.402 min
Delta R.T.: 0.032 min
Response: 22848326
Conc: 3.24 ng/ml

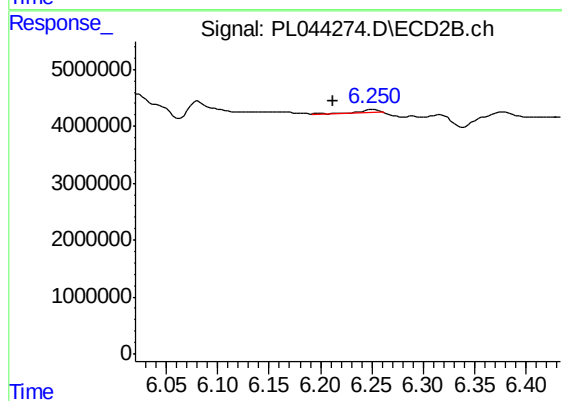

#9 Endosulfan I


R.T.: 6.252 min
Delta R.T.: 0.040 min
Response: 783410
Conc: 0.34 ng/ml

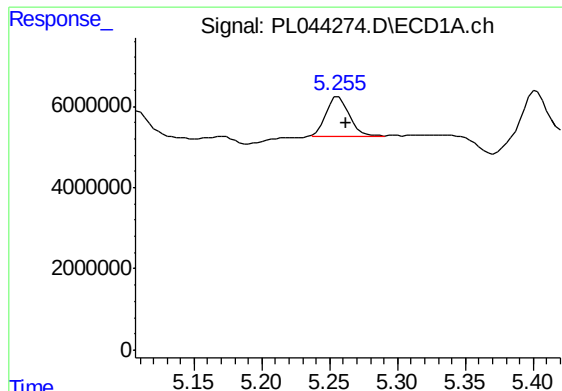

#10 gamma-Chlordane


R.T.: 5.257 min
Delta R.T.: -0.005 min
Response: 11184788
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-C05

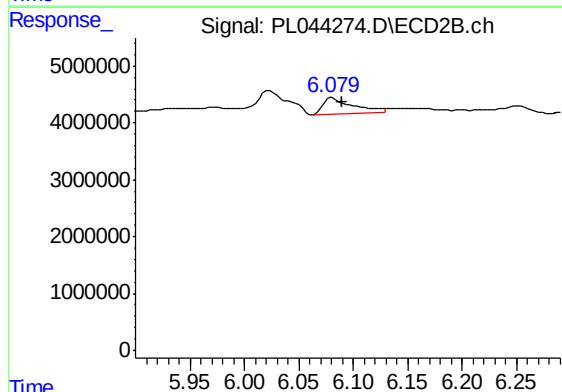


#10 gamma-Chlordane

R.T.: 6.081 min
Delta R.T.: -0.009 min
Response: 5628122
Conc: 2.23 ng/ml

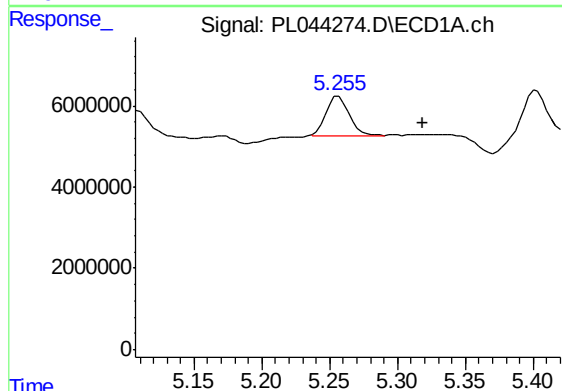


#11 alpha-Chlordane

R.T.: 5.257 min
Delta R.T.: -0.062 min
Response: 11184788
Conc: 1.47 ng/ml

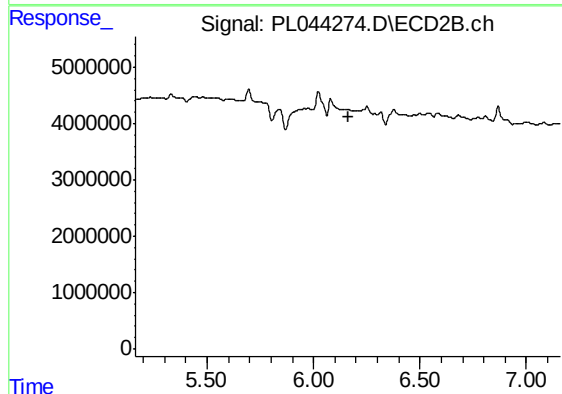

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

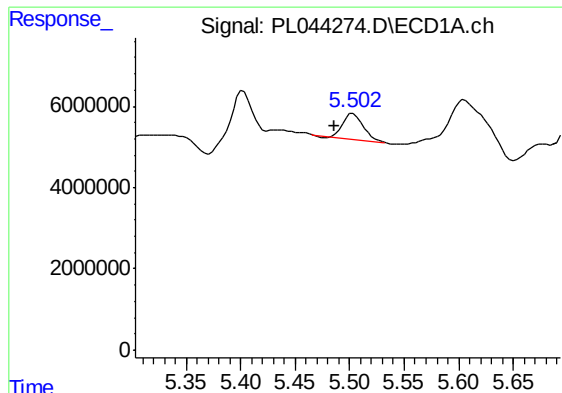

#12 4,4'-DDE


R.T.: 5.504 min
Delta R.T.: 0.018 min
Response: 7854876
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-C05

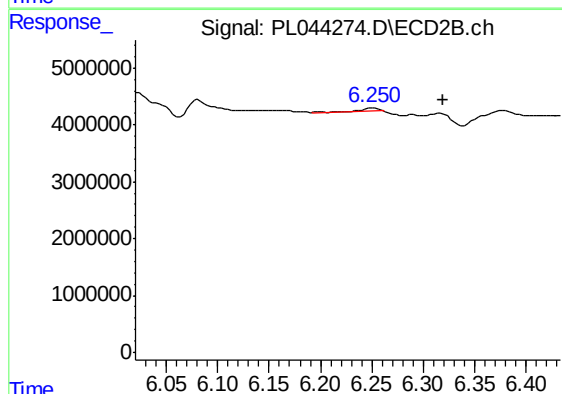


#12 4,4'-DDE

R.T.: 6.252 min
Delta R.T.: -0.068 min
Response: 783410
Conc: 0.37 ng/ml

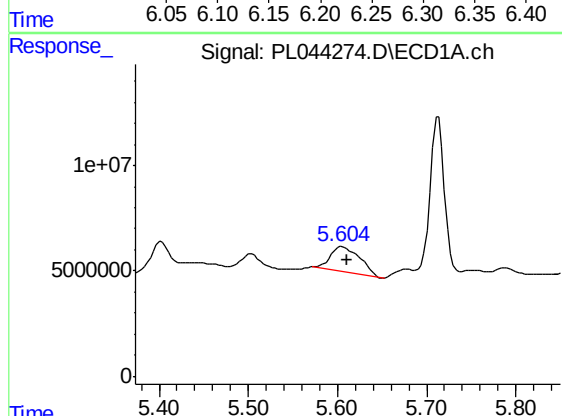


#13 Dieldrin

R.T.: 5.605 min
Delta R.T.: -0.006 min
Response: 28191164
Conc: 3.75 ng/ml

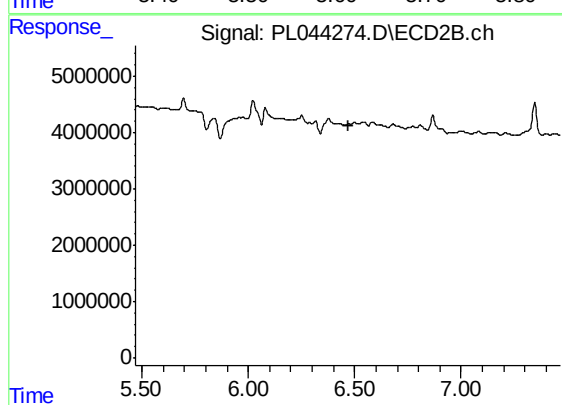

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.469 min
Response: 0
Conc: N.D.

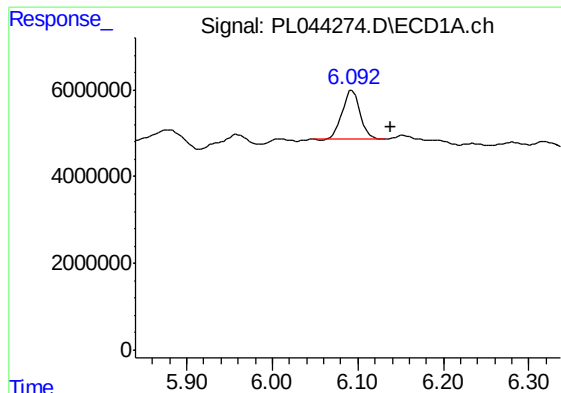

#15 Endosulfan II


R.T.: 6.093 min
Delta R.T.: -0.045 min
Response: 16176398
Conc: 2.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-C05

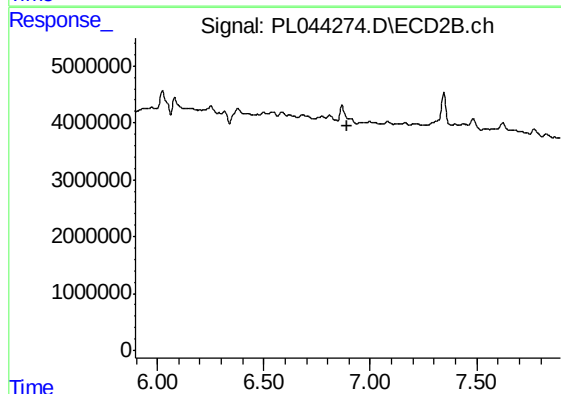


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

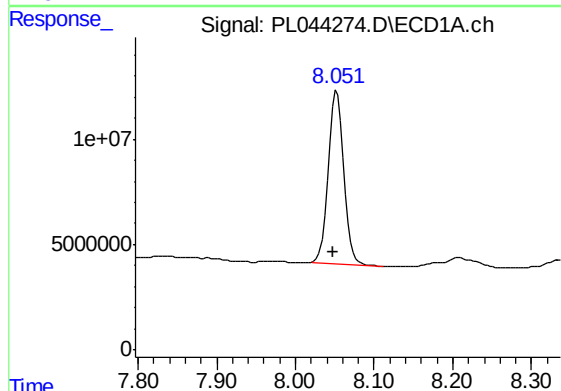

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.005 min
Response: 113601386
Conc: 16.38 ng/ml

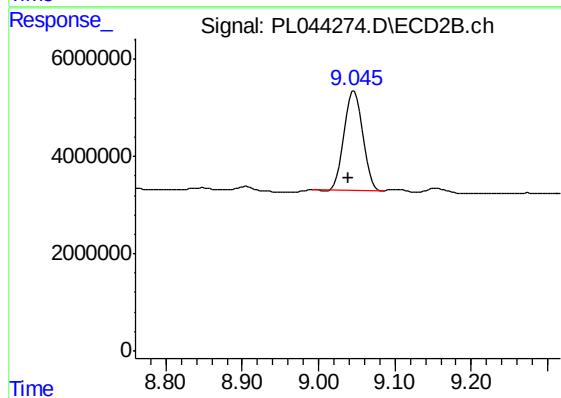

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: 0.007 min
Response: 34536012
Conc: 15.57 ng/ml