

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012820\
 Data File : PL056116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2020 10:31
 Operator : AJ\MA
 Sample : RSCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 13:16:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.016	218.6E6	62848485	20.872	21.493
28)	SA Decachlor...	8.254	9.095	221.6E6	48709730	21.048	21.534
Target Compounds							
9)	A Endosulfan I	5.554	6.247	147.0E6	30981571	10.132	10.352
10)	B gamma-Chl...	5.442	6.123	150.0E6	31900272	9.567	10.031
12)	B 4,4'-DDE	5.663	6.354	293.8E6	60387910	20.272	20.160
13)	MA Dieldrin	5.797	6.504	309.4E6	62898406	20.114	20.264
19)	B Endosulfa...	6.708	7.281	235.1E6	49527721	19.340	19.570
20)	A Methoxychlor	6.964	7.606	552.0E6	119.0E6	103.902	97.038
21)	B Endrin ke...	7.200	7.754	254.1E6	52944476	19.416	19.853
25)	Chlordane-3	5.442	6.123	150.0E6	31900272	118.842	84.878 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012820\
Data File : PL056116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2020 10:31
Operator : AJ\MA
Sample : RSCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 13:16:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

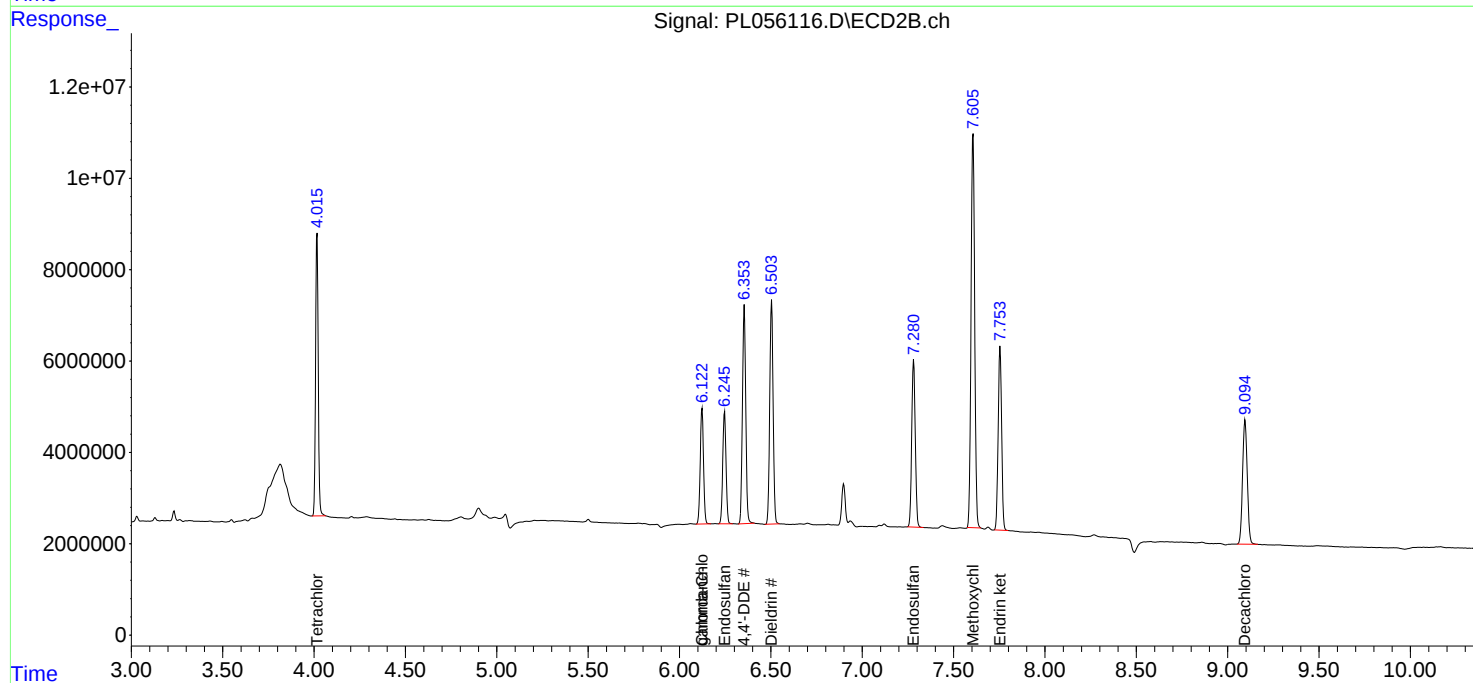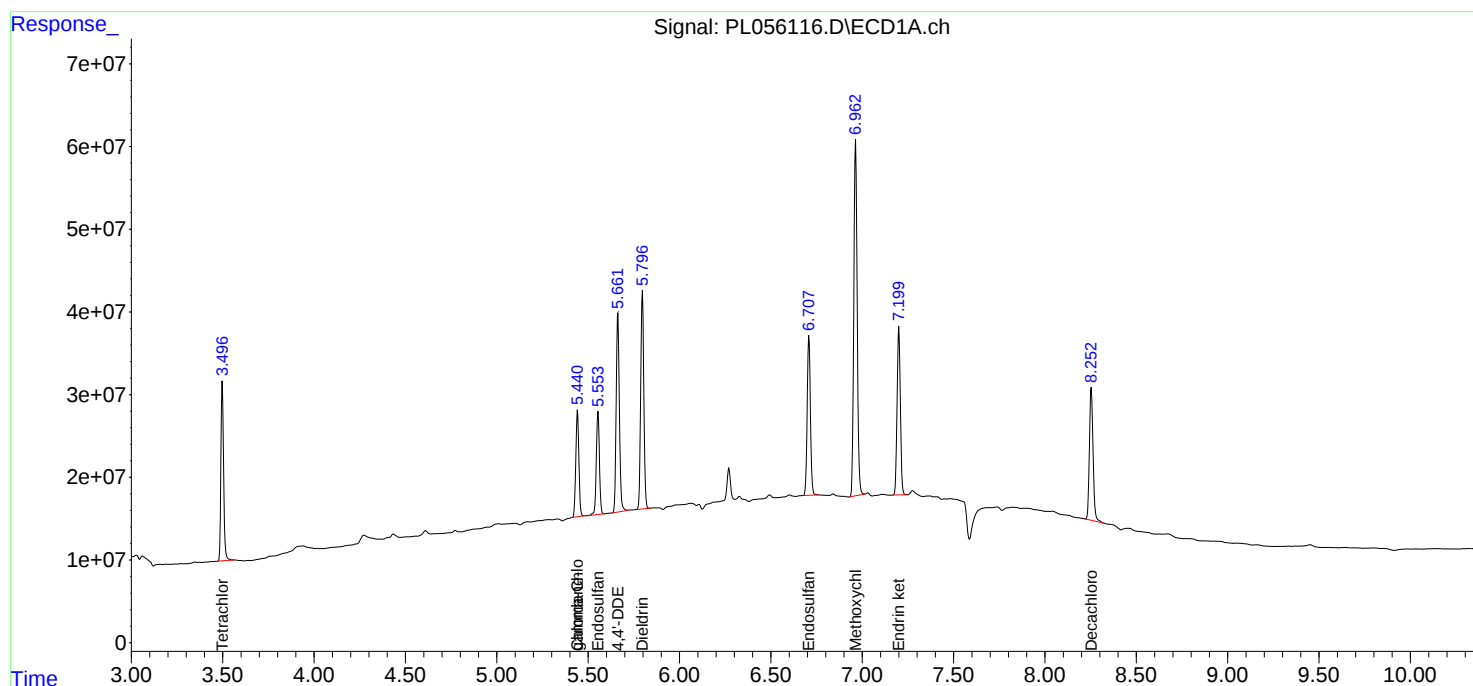


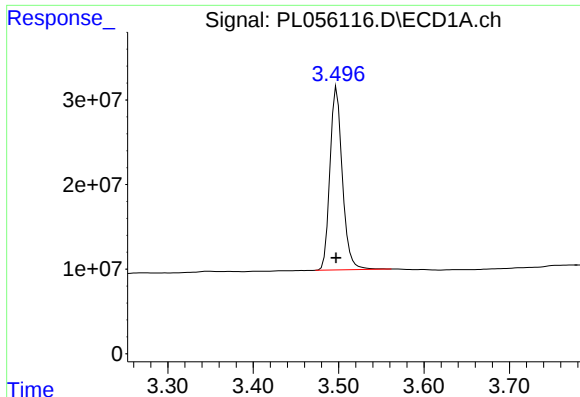

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 218595781
Conc: 20.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

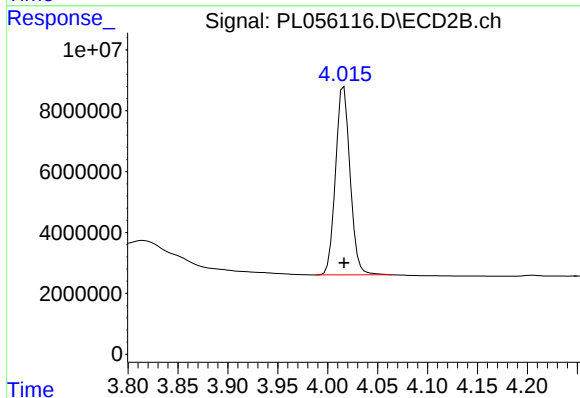


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 62848485
Conc: 21.49 ng/ml

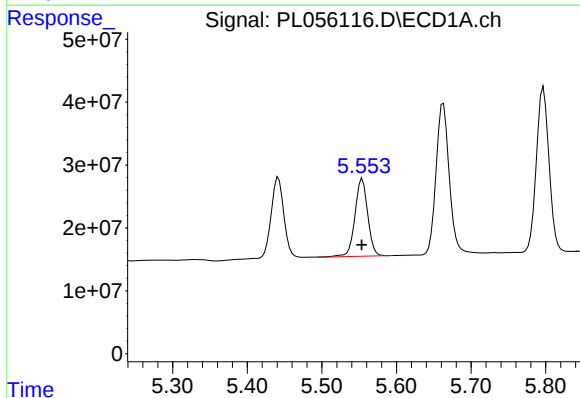


#9 Endosulfan I

R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 147034041
Conc: 10.13 ng/ml

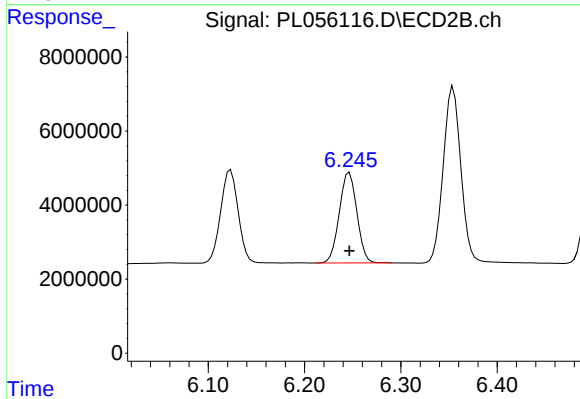

#9 Endosulfan I


R.T.: 6.247 min
Delta R.T.: 0.000 min
Response: 30981571
Conc: 10.35 ng/ml

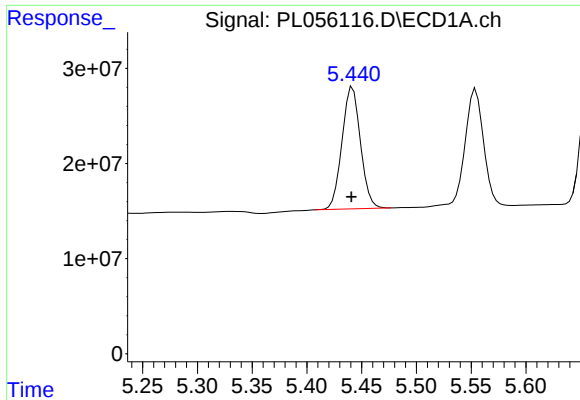

#10 gamma-Chlordane


R.T.: 5.442 min
Delta R.T.: 0.001 min
Response: 150042988
Conc: 9.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

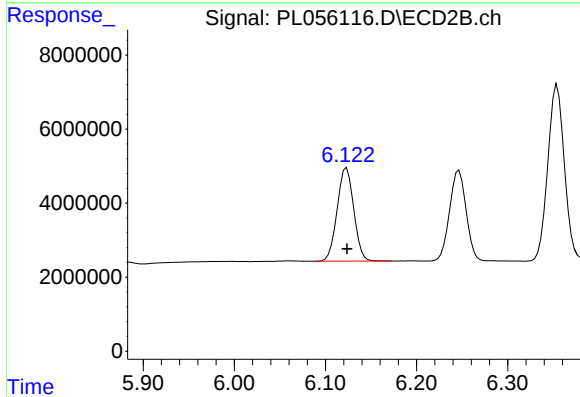


#10 gamma-Chlordane

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 31900272
Conc: 10.03 ng/ml

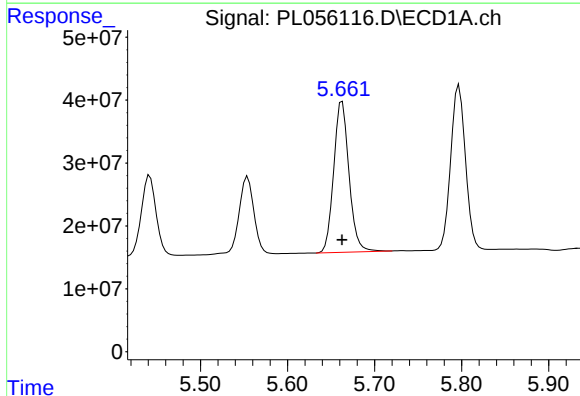


#12 4,4'-DDE

R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 293820005
Conc: 20.27 ng/ml

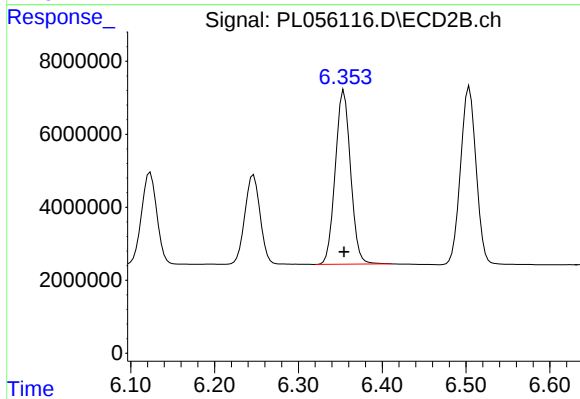

#12 4,4'-DDE


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 60387910
Conc: 20.16 ng/ml

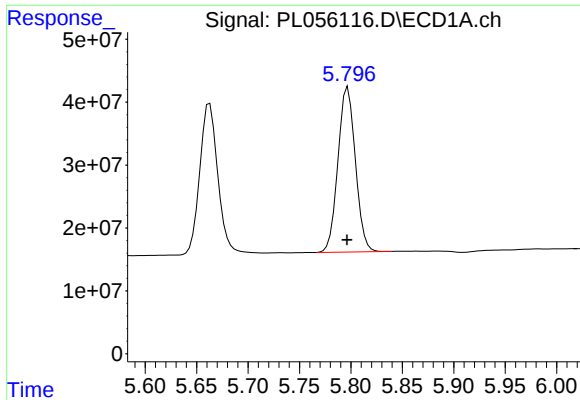

#13 Dieldrin


R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 309356393
Conc: 20.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

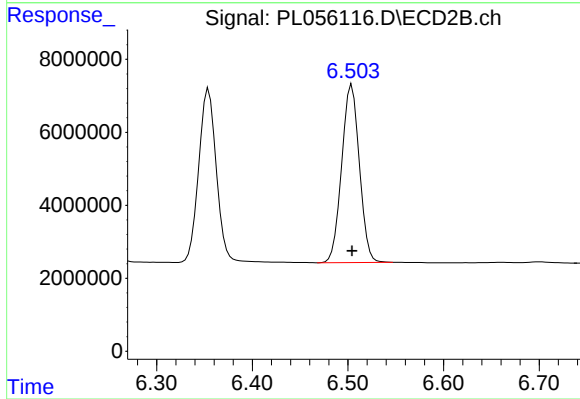


#13 Dieldrin

R.T.: 6.504 min
Delta R.T.: 0.000 min
Response: 62898406
Conc: 20.26 ng/ml

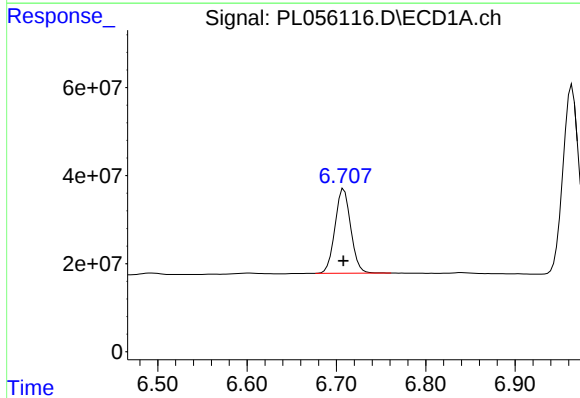


#19 Endosulfan Sulfate

R.T.: 6.708 min
Delta R.T.: 0.000 min
Response: 235128181
Conc: 19.34 ng/ml

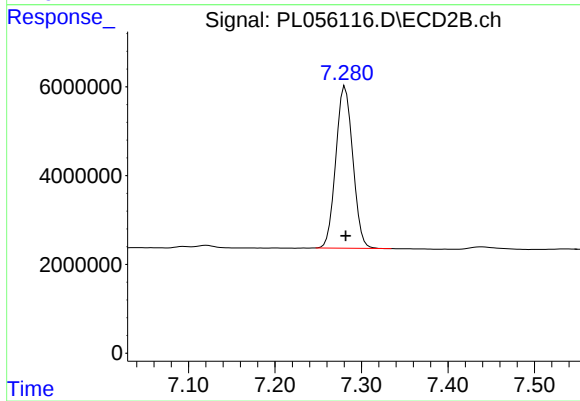

#19 Endosulfan Sulfate


R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 49527721
Conc: 19.57 ng/ml

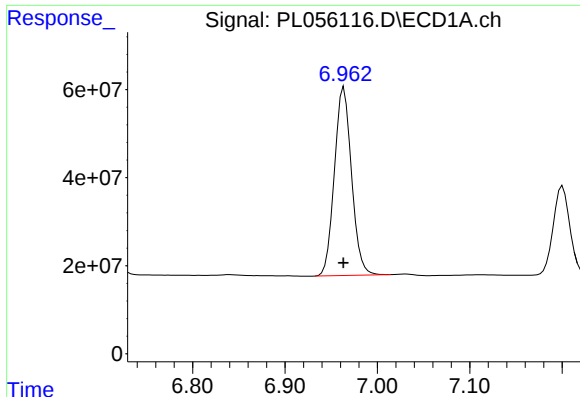

#20 Methoxychlor


R.T.: 6.964 min
Delta R.T.: 0.000 min
Response: 551950559
Conc: 103.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

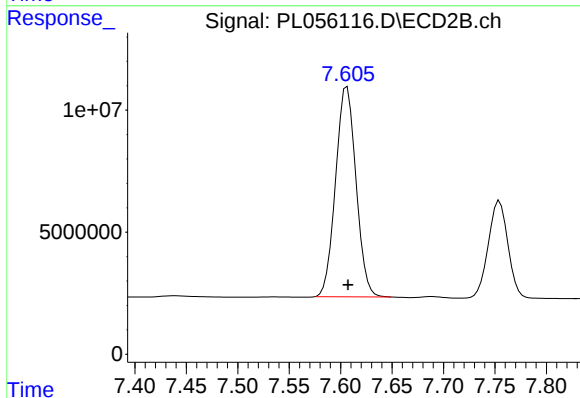


#20 Methoxychlor

R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 118978383
Conc: 97.04 ng/ml

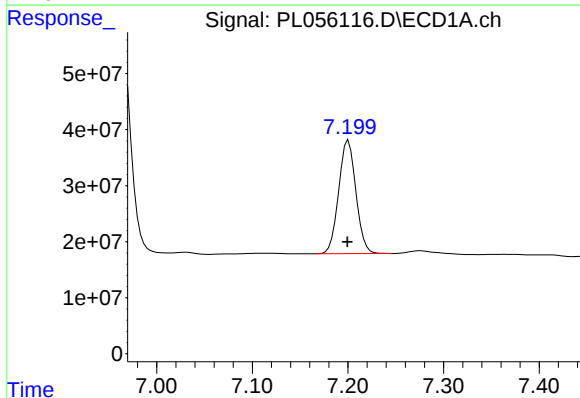


#21 Endrin ketone

R.T.: 7.200 min
Delta R.T.: 0.000 min
Response: 254059522
Conc: 19.42 ng/ml

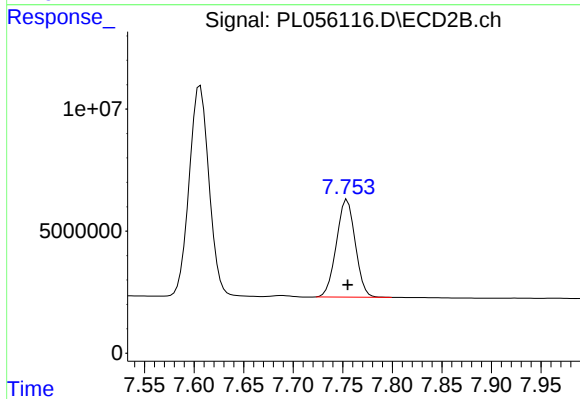

#21 Endrin ketone


R.T.: 7.754 min
Delta R.T.: 0.000 min
Response: 52944476
Conc: 19.85 ng/ml

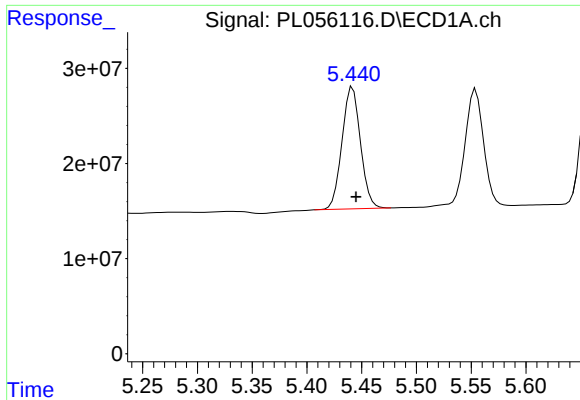

#25 Chlordane-3


R.T.: 5.442 min
Delta R.T.: -0.003 min
Response: 150042988
Conc: 118.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

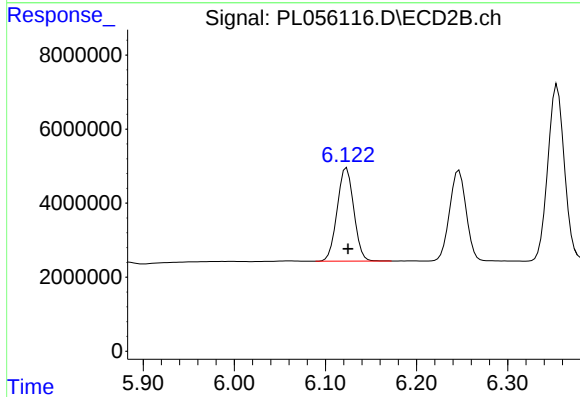


#25 Chlordane-3

R.T.: 6.123 min
Delta R.T.: -0.002 min
Response: 31900272
Conc: 84.88 ng/ml

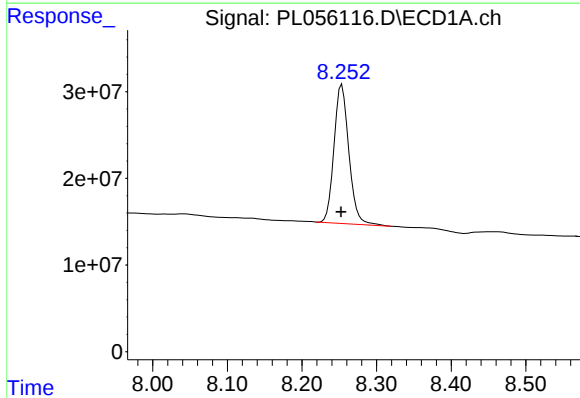

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.001 min
Response: 221595668
Conc: 21.05 ng/ml

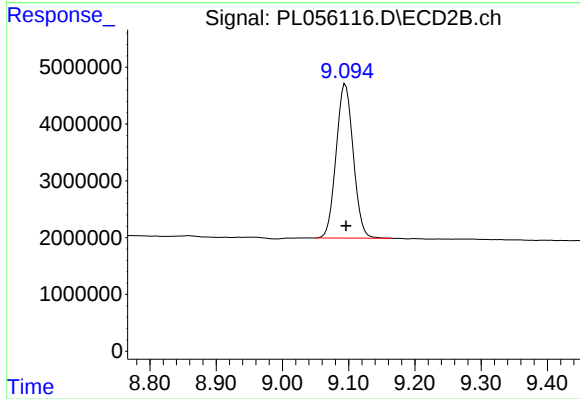

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 48709730
Conc: 21.53 ng/ml