

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012820\
 Data File : PL056141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2020 16:27
 Operator : AJ\MA
 Sample : L1245-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 17:53:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.016	194.9E6	55537154	18.606	18.993
28)	SA Decachlor...	8.254	9.094	172.5E6	40401296	16.383	17.861
Target Compounds							
2)	A alpha-BHC	3.948	0.000	20243475	0	1.136	N.D. #
4)	MA Heptachlor	4.549f	0.000	34874801	0	2.172	N.D. #
5)	MB Aldrin	4.759	0.000	8826832	0	0.543	N.D. #
9)	A Endosulfan I	5.567	0.000	8762666	0	0.604	N.D. #
10)	B gamma-Chl...	5.460f	6.133	177.4E6	61589290	11.311	19.367 #
12)	B 4,4'-DDE	5.692f	0.000	11055443	0	0.763	N.D. #
23)	Chlordane-1	4.365	0.000	72347561	0	191.121	N.D. #
25)	Chlordane-3	5.460f	6.133	177.4E6	61589290	140.503	163.873



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012820\
Data File : PL056141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2020 16:27
Operator : AJ\MA
Sample : L1245-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 17:53:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

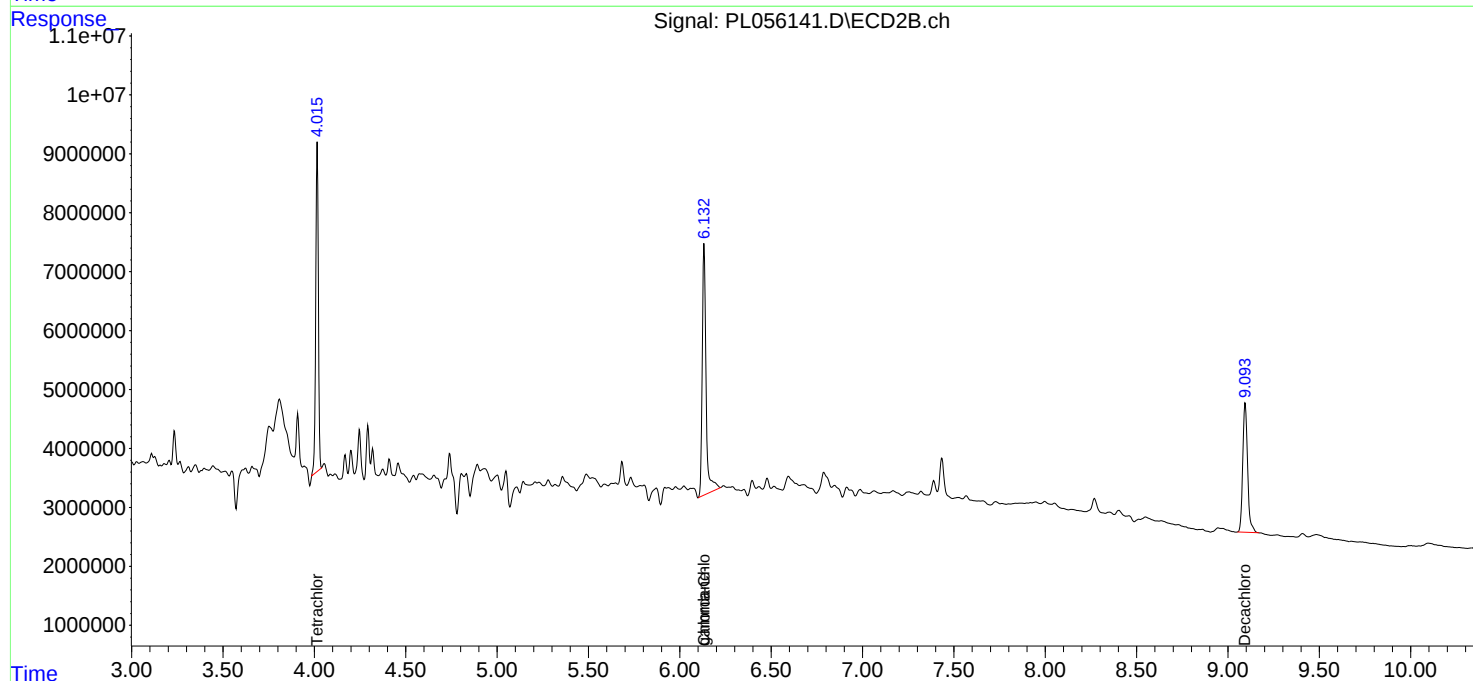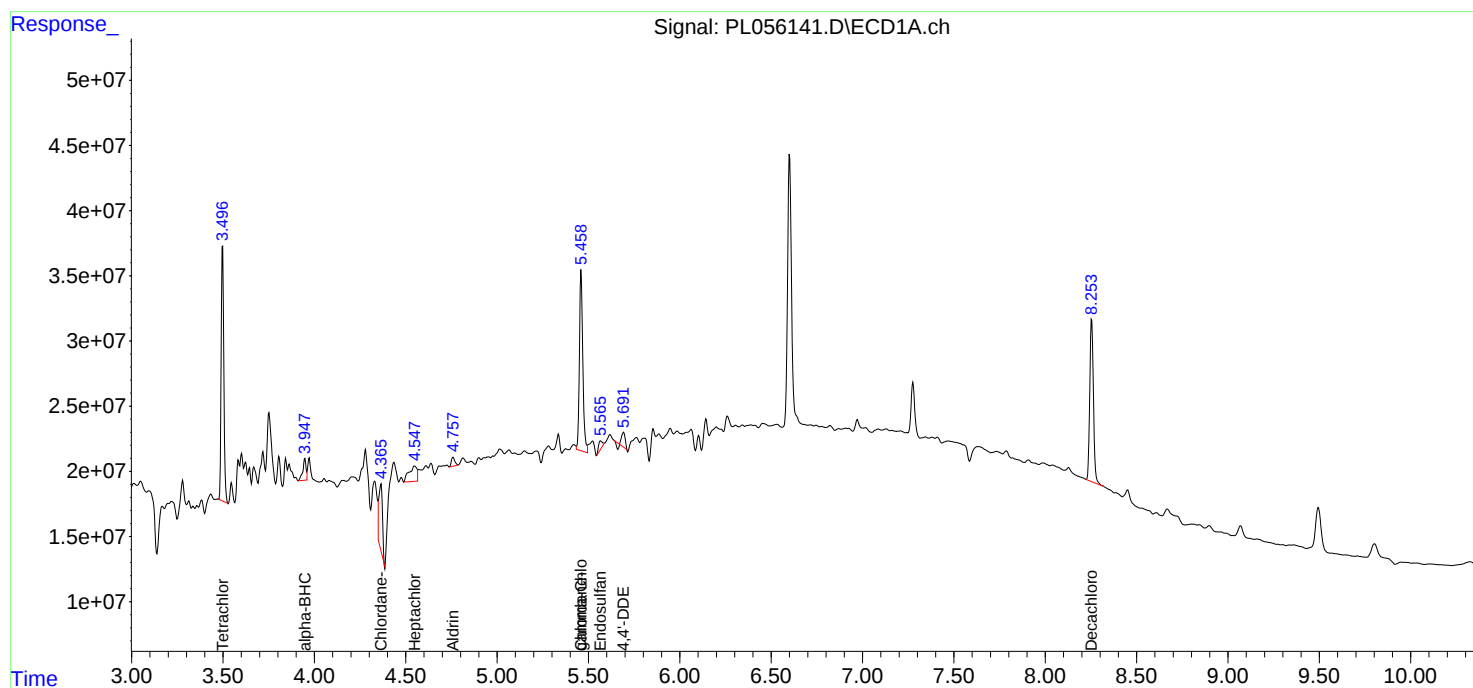


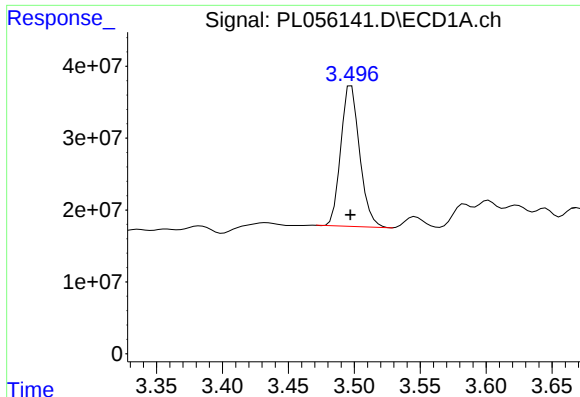

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 194856360
Conc: 18.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

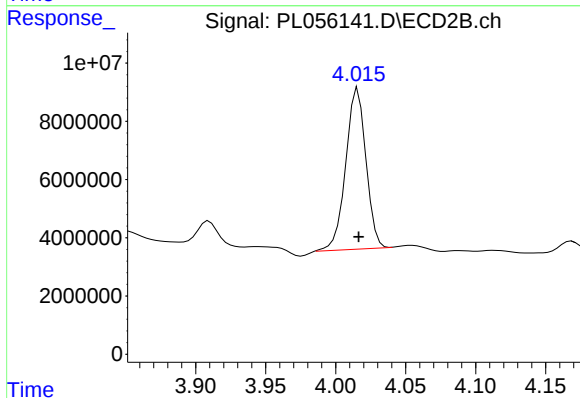


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 55537154
Conc: 18.99 ng/ml

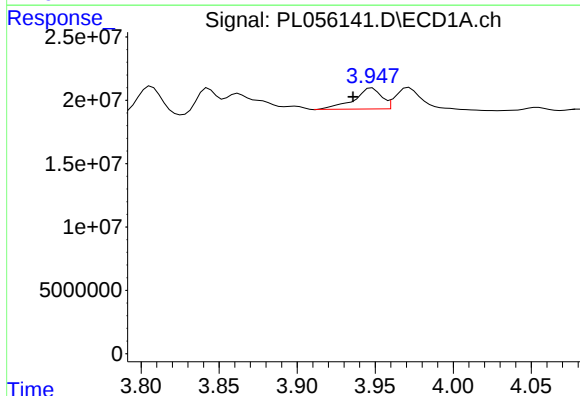


#2 alpha-BHC

R.T.: 3.948 min
Delta R.T.: 0.012 min
Response: 20243475
Conc: 1.14 ng/ml

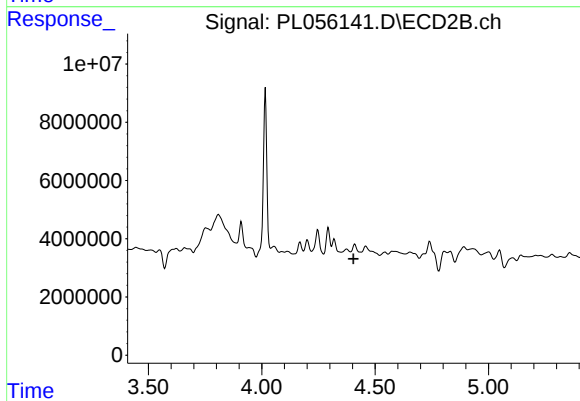

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.405 min
Response: 0
Conc: N.D.

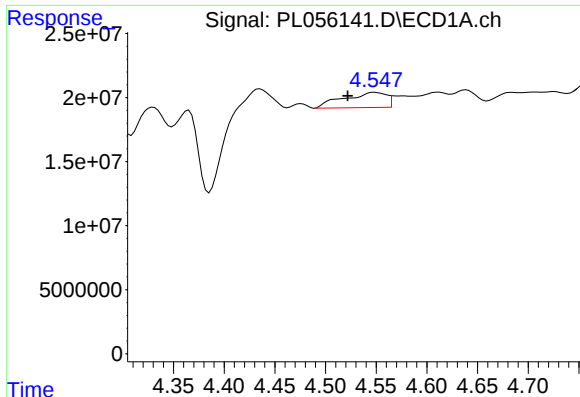

#4 Heptachlor


R.T.: 4.549 min
Delta R.T.: 0.026 min
Response: 34874801
Conc: 2.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

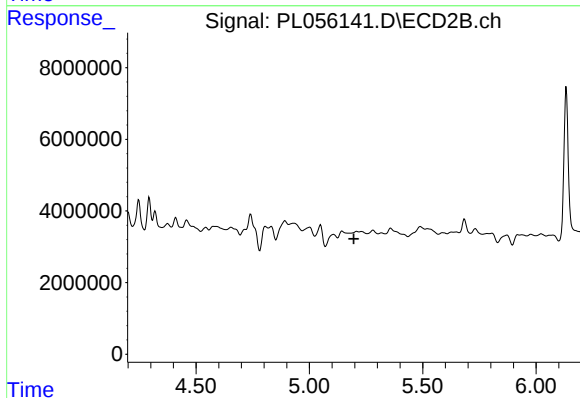


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

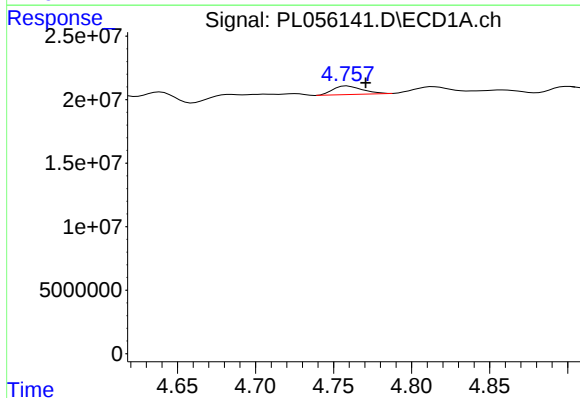


#5 Aldrin

R.T.: 4.759 min
Delta R.T.: -0.012 min
Response: 8826832
Conc: 0.54 ng/ml

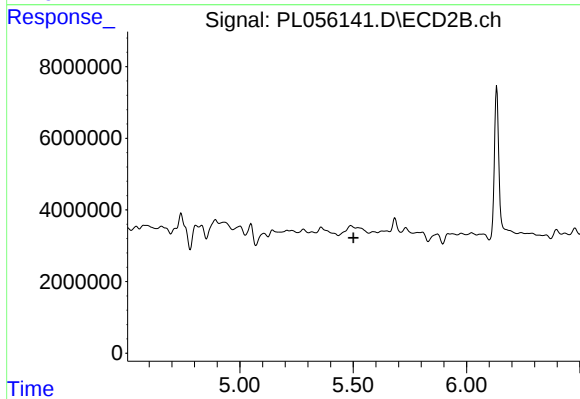

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

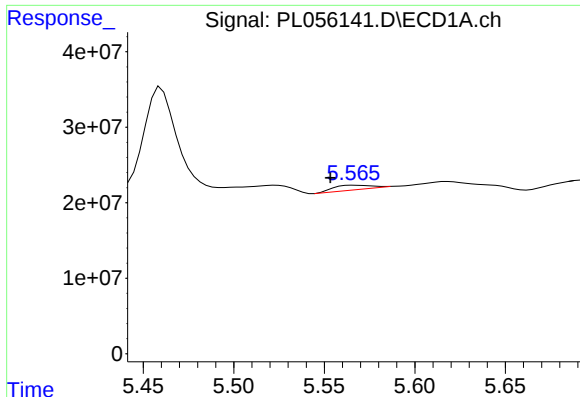

#9 Endosulfan I


R.T.: 5.567 min
Delta R.T.: 0.013 min
Response: 8762666
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

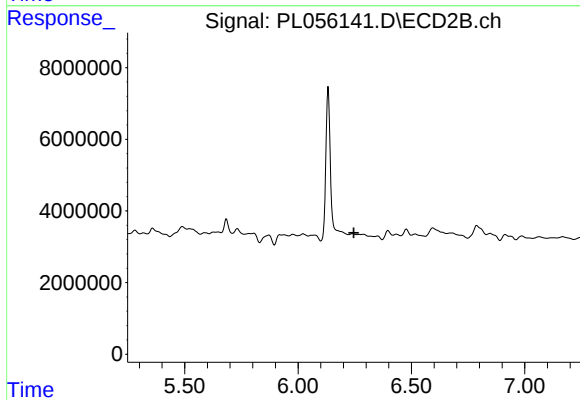


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

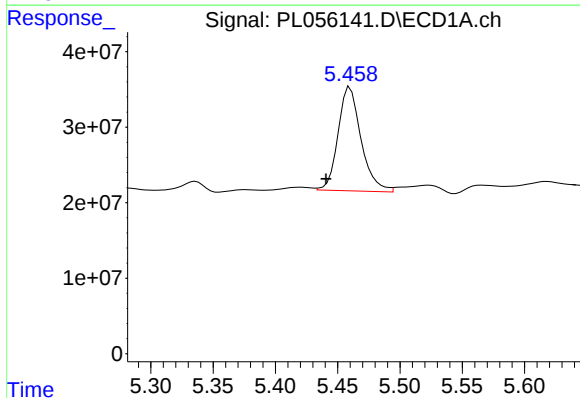


#10 gamma-Chlordane

R.T.: 5.460 min
Delta R.T.: 0.019 min
Response: 177390920
Conc: 11.31 ng/ml

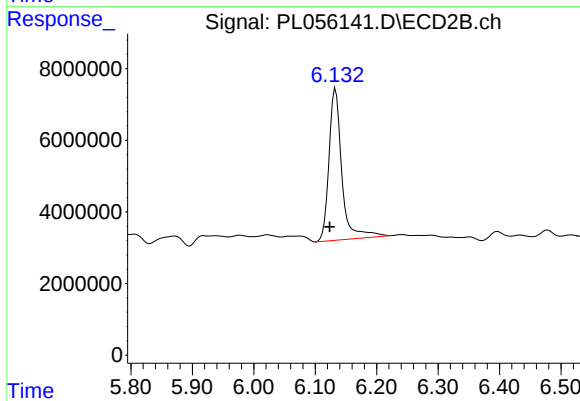

#10 gamma-Chlordane


R.T.: 6.133 min
Delta R.T.: 0.009 min
Response: 61589290
Conc: 19.37 ng/ml

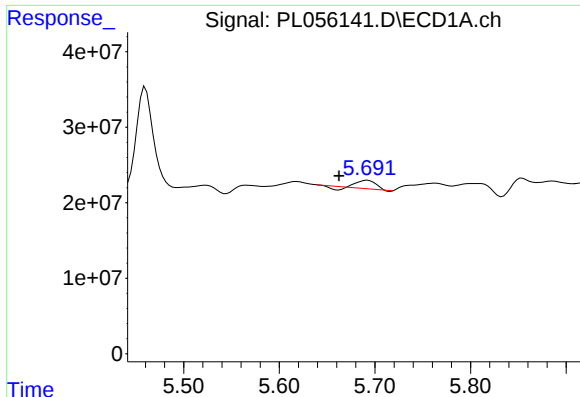

#12 4,4'-DDE


R.T.: 5.692 min
Delta R.T.: 0.030 min
Response: 11055443
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

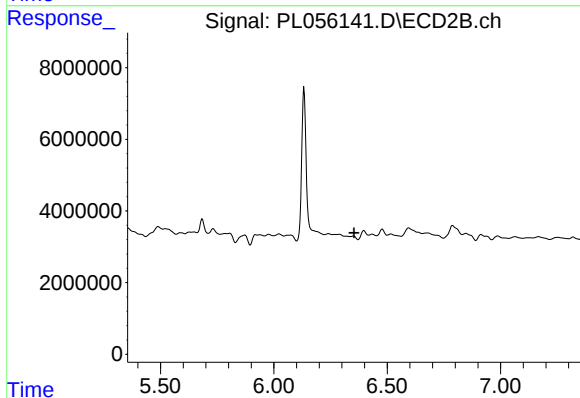


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

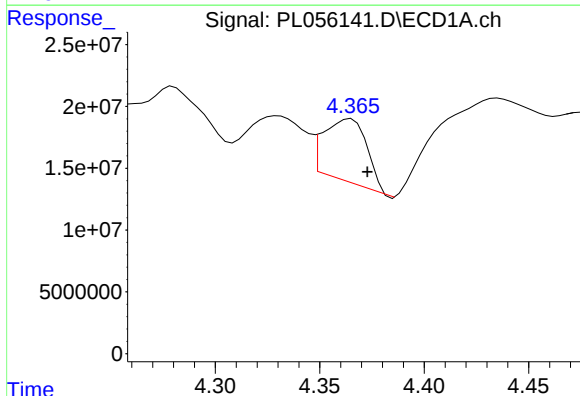


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: -0.008 min
Response: 72347561
Conc: 191.12 ng/ml

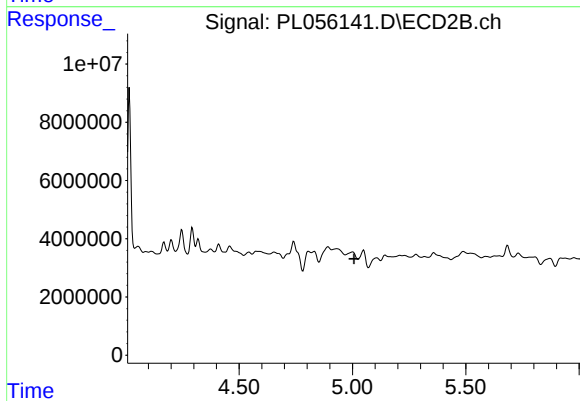

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

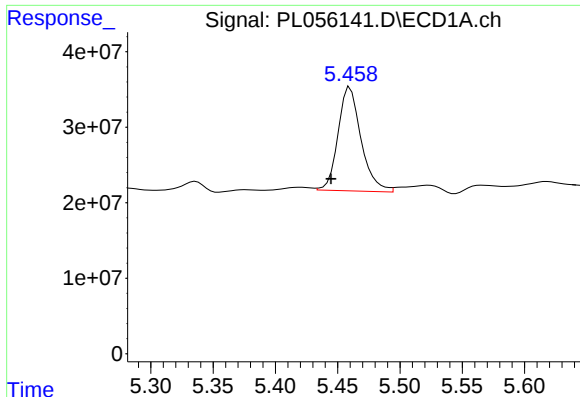

#25 Chlordane-3


R.T.: 5.460 min
Delta R.T.: 0.015 min
Response: 177390920
Conc: 140.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

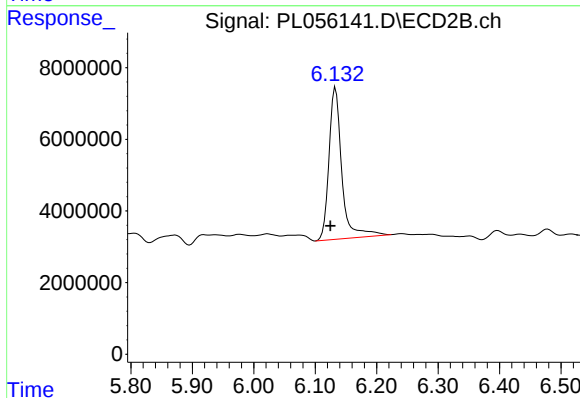


#25 Chlordane-3

R.T.: 6.133 min
Delta R.T.: 0.008 min
Response: 61589290
Conc: 163.87 ng/ml

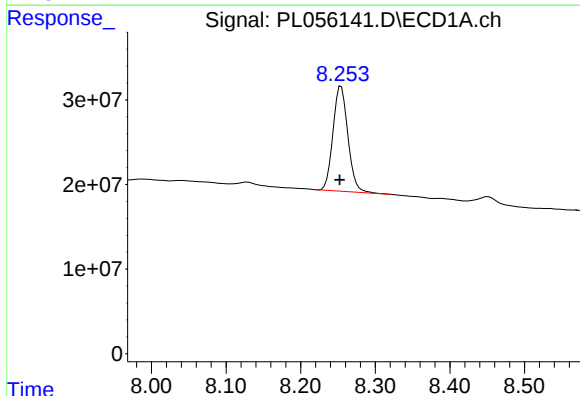

#28 Decachlorobiphenyl

R.T.: 8.254 min
Delta R.T.: 0.002 min
Response: 172481032
Conc: 16.38 ng/ml

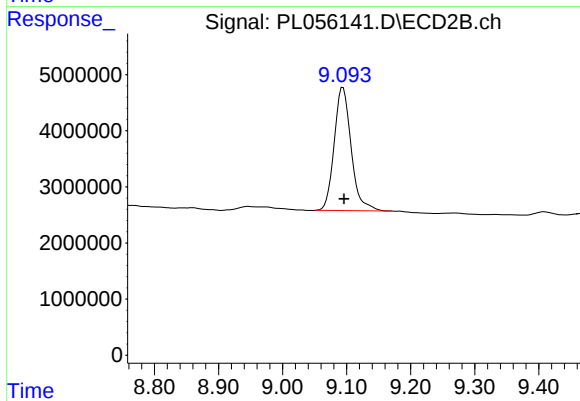

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.002 min
Response: 40401296
Conc: 17.86 ng/ml