

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
 Data File : PL064472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 13:35
 Operator : AR\AJ
 Sample : M1242-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 17:12:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	60423913	45154653	20.151	17.663
28)	SA Decachlor...	8.165	9.269	45682549	31211276	14.968	13.150
Target Compounds							
2)	A alpha-BHC	3.852f	0.000	2541061	0	0.511	N.D. #
4)	MA Heptachlor	0.000	5.305	0	6994520	N.D.	1.947 #
7)	B delta-BHC	0.000	5.221f	0	4298864	N.D.	1.354 #
10)	B gamma-Chl...	0.000	6.252	0	1049456	N.D.	0.349 #
23)	Chlordane-1	4.297	0.000	769354	0	6.606	N.D. #
25)	Chlordane-3	0.000	6.252	0	1049456	N.D.	2.596 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
Data File : PL064472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 13:35
Operator : AR\AJ
Sample : M1242-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 17:12:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

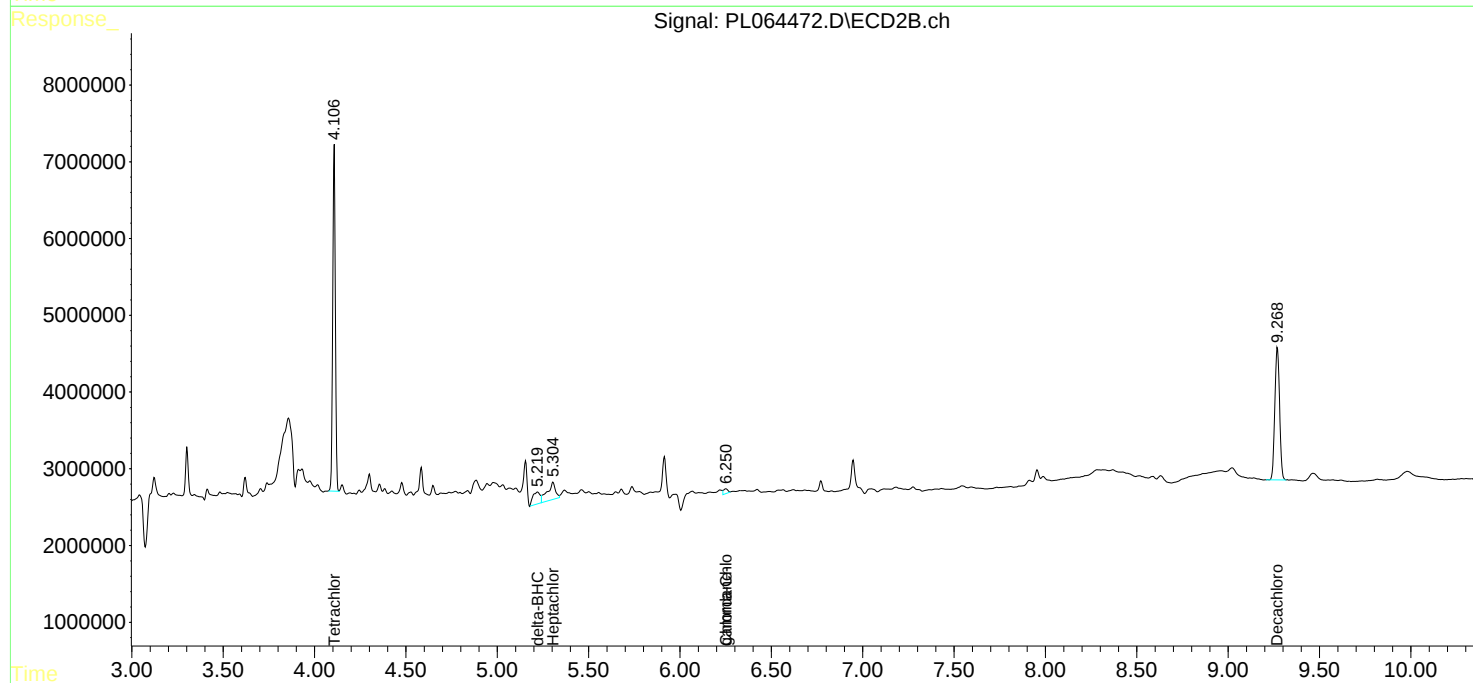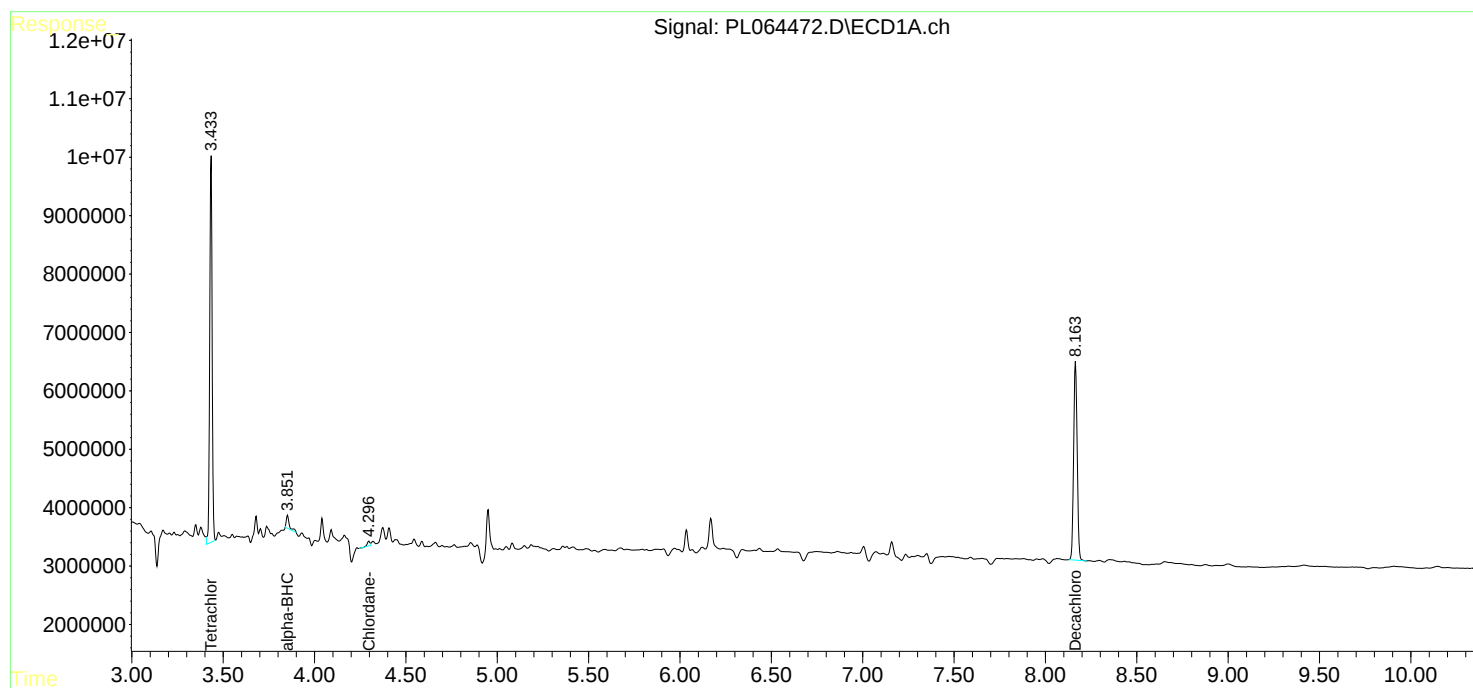


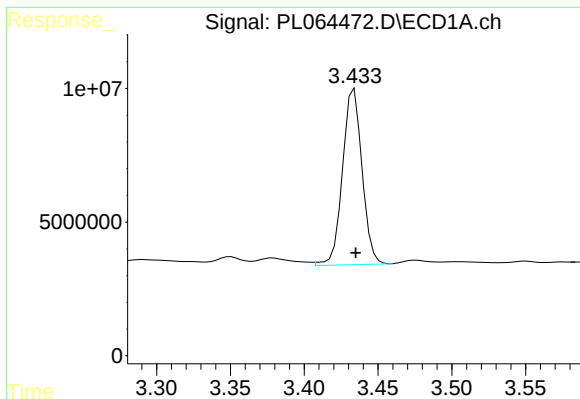

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: -0.001 min
Response: 60423913
Conc: 20.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

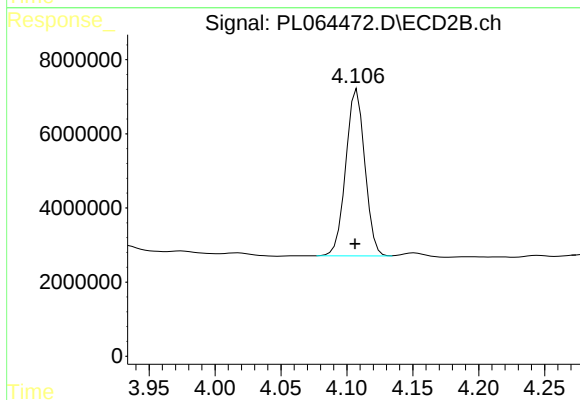


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 45154653
Conc: 17.66 ng/ml

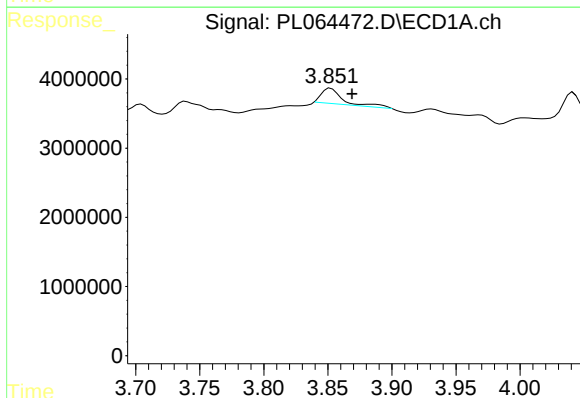


#2 alpha-BHC

R.T.: 3.852 min
Delta R.T.: -0.017 min
Response: 2541061
Conc: 0.51 ng/ml

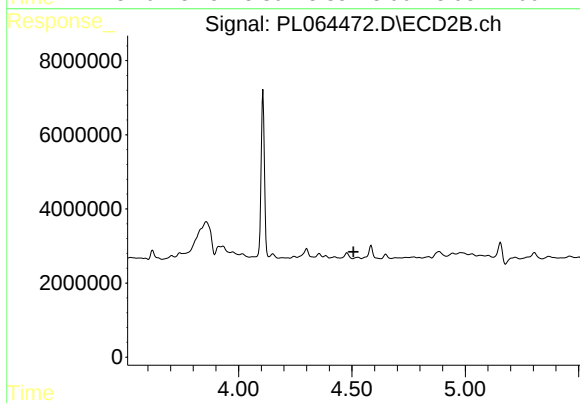

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.508 min
Response: 0
Conc: N.D.

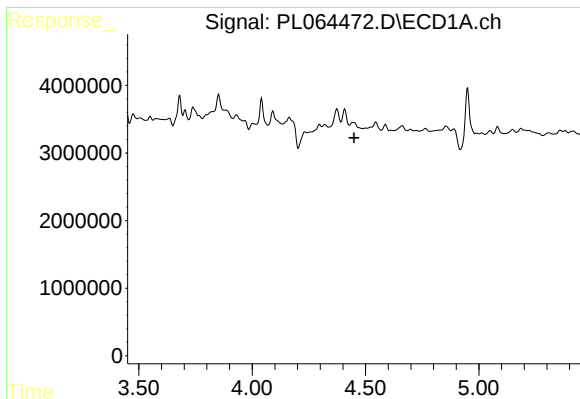

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

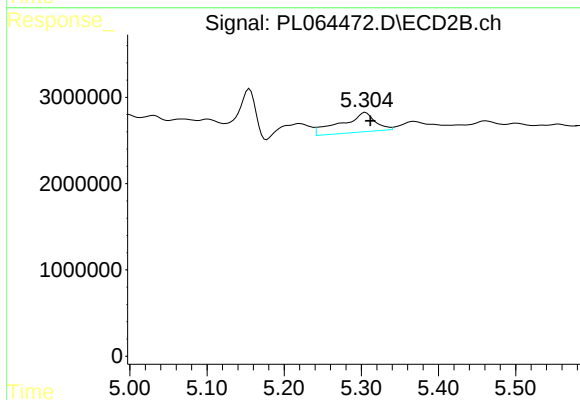


#4 Heptachlor

R.T.: 5.305 min
Delta R.T.: -0.007 min
Response: 6994520
Conc: 1.95 ng/ml

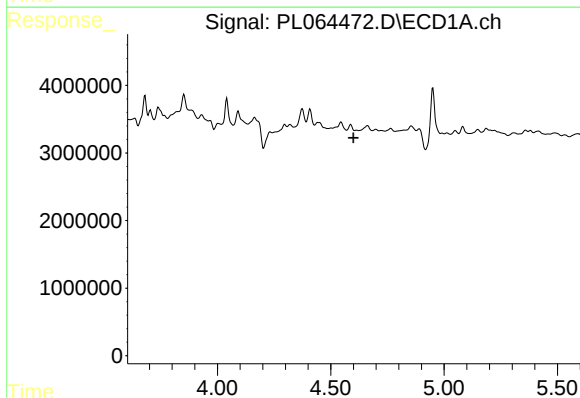


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.601 min
Response: 0
Conc: N.D.

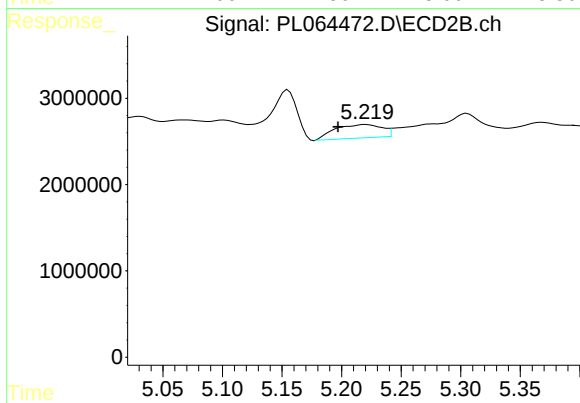

#7 delta-BHC


R.T.: 5.221 min
Delta R.T.: 0.023 min
Response: 4298864
Conc: 1.35 ng/ml

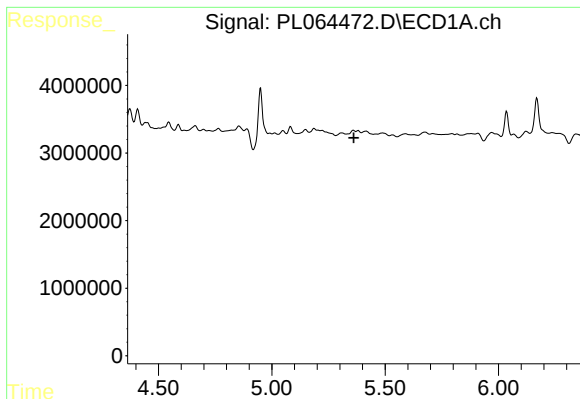

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

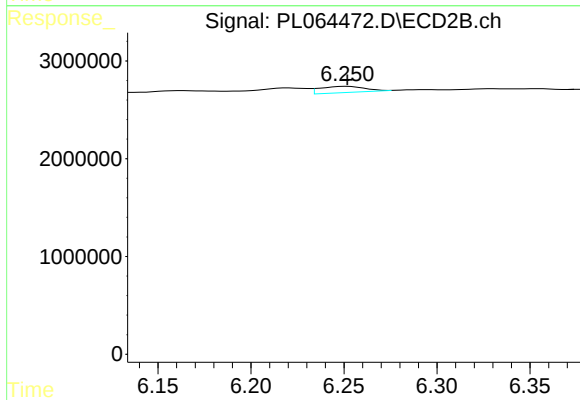


#10 gamma-Chlordane

R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 1049456
Conc: 0.35 ng/ml

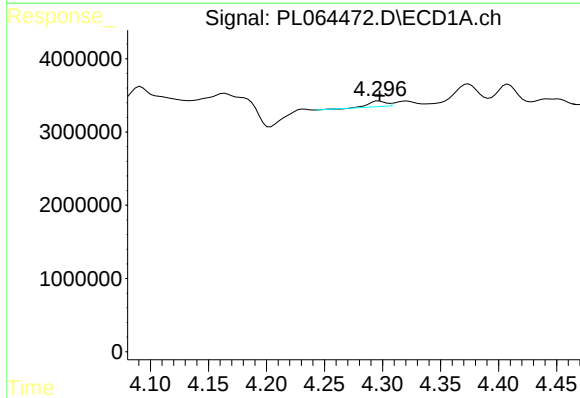


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 769354
Conc: 6.61 ng/ml

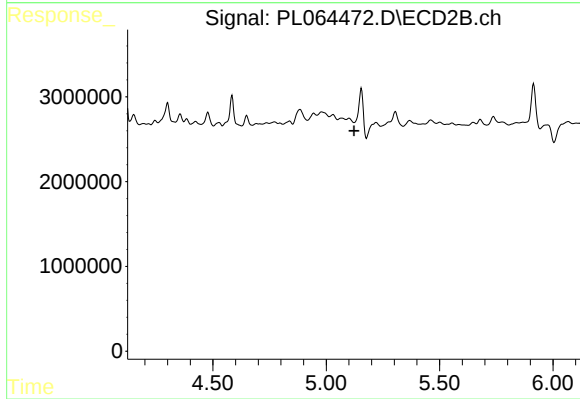

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

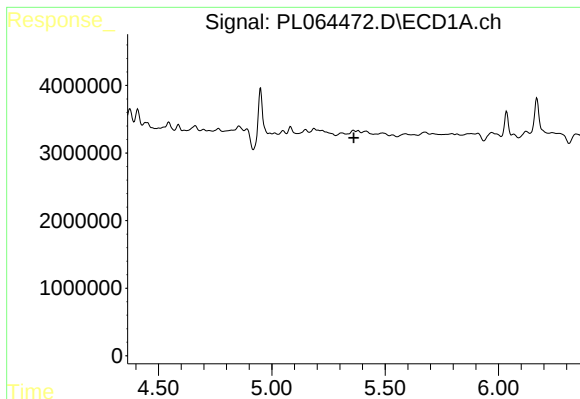

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

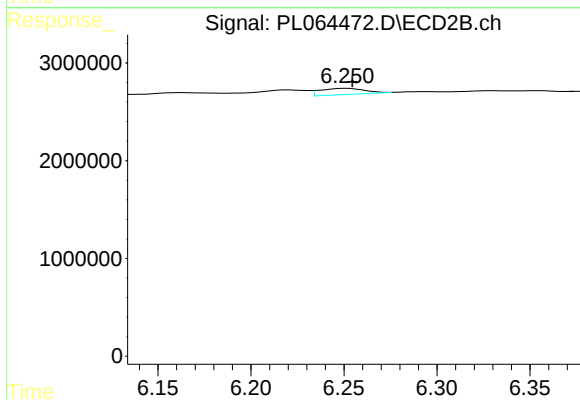


#25 Chlordane-3

R.T.: 6.252 min
Delta R.T.: -0.003 min
Response: 1049456
Conc: 2.60 ng/ml

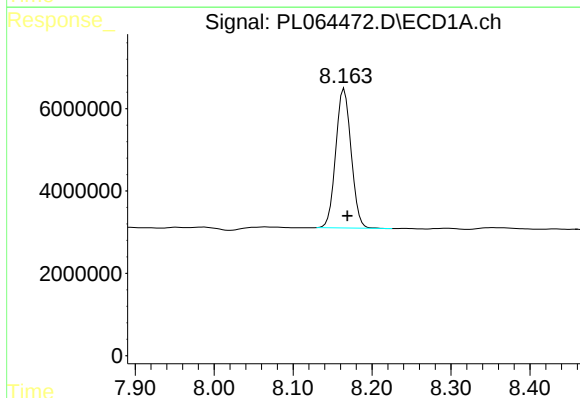

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 45682549
Conc: 14.97 ng/ml

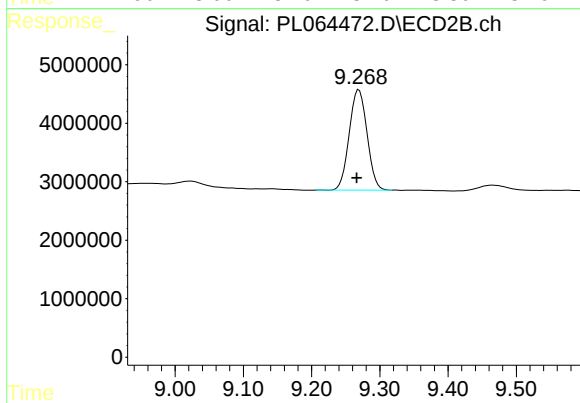

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.003 min
Response: 31211276
Conc: 13.15 ng/ml