

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
 Data File : PL064478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 15:28
 Operator : AR\AJ
 Sample : PB134358BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 17:14:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.108	50972807	38444476	16.999	15.038
28)	SA Decachlor...	8.168	9.271	63824301	44218912	20.912	18.631
Target Compounds							
6)	B beta-BHC	4.413	4.976	10137983	4432696	2.589	N.D. #
8)	B Heptachlo...	0.000	6.014	0	10576402	N.D.	4.060 #
10)	B gamma-Chl...	0.000	6.263	0	1066888	N.D.	0.355 #
14)	MA Endrin	5.974	0.000	10433435	0	3.005	N.D. #
15)	B Endosulfa...	0.000	7.068	0	1753389	N.D.	0.694 #
18)	B Endrin al...	6.405	0.000	1532205	0	0.534	N.D. #
21)	B Endrin ke...	0.000	7.917	0	699609	N.D.	0.280 #
23)	Chlordane-1	4.288	0.000	412321	0	3.541	N.D. #
25)	Chlordane-3	0.000	6.263	0	1066888	N.D.	2.639 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
Data File : PL064478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 15:28
Operator : AR\AJ
Sample : PB134358BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 17:14:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

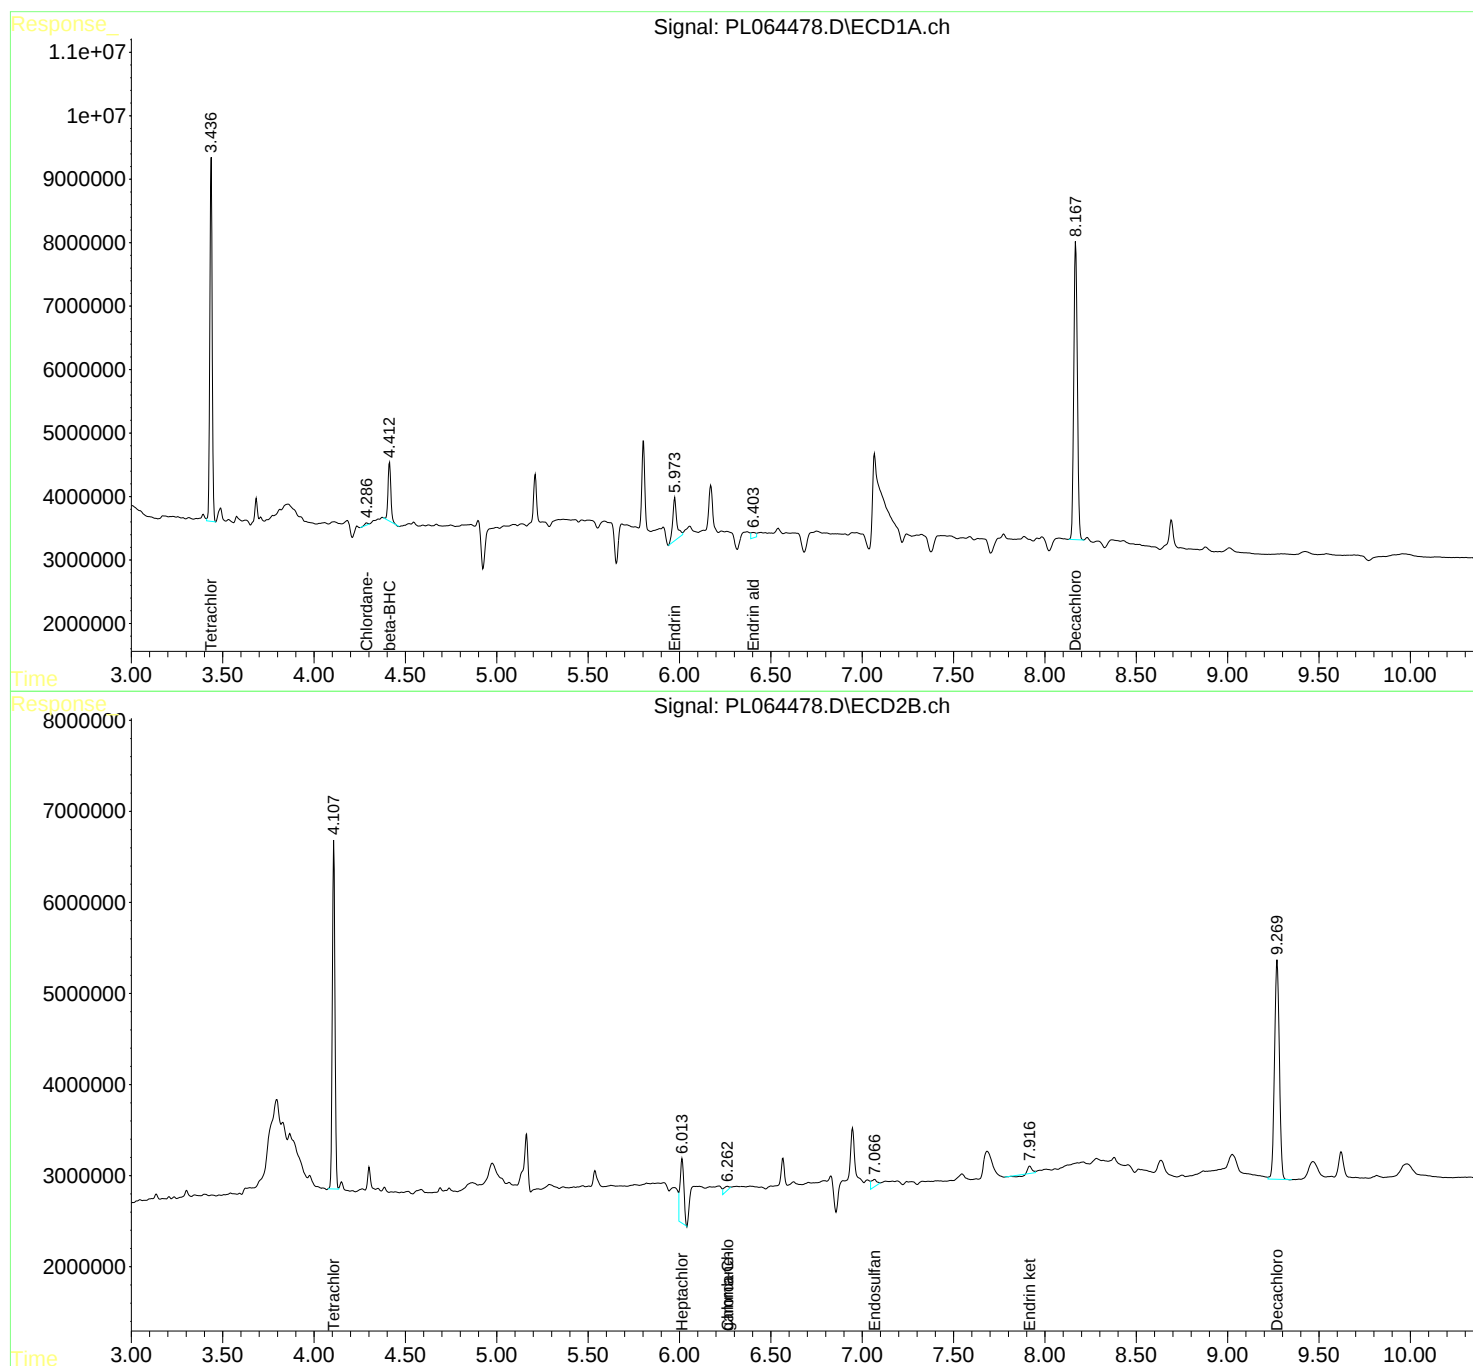


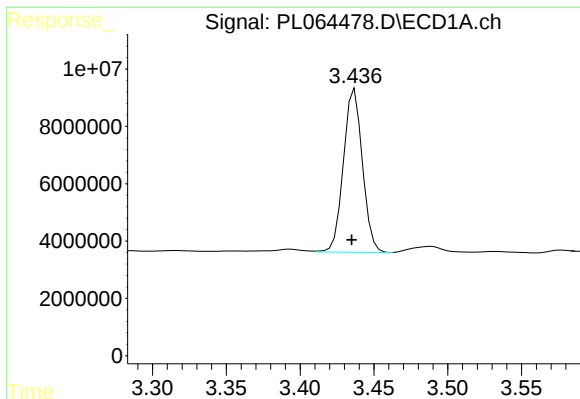

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: 0.002 min
Response: 50972807
Conc: 17.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

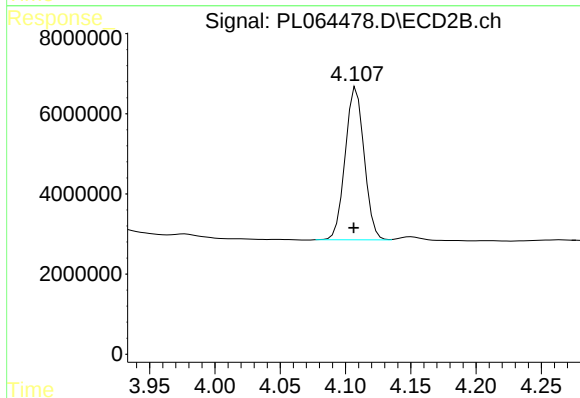


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 38444476
Conc: 15.04 ng/ml

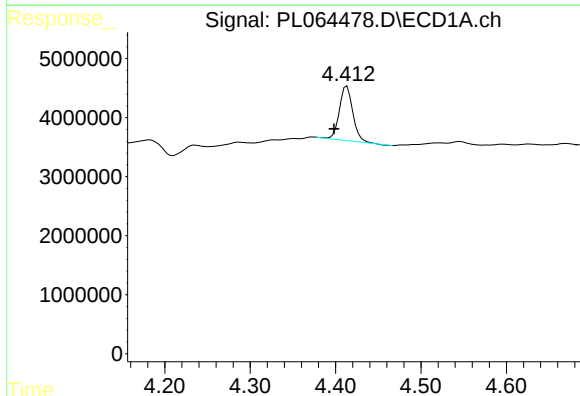


#6 beta-BHC

R.T.: 4.413 min
Delta R.T.: 0.015 min
Response: 10137983
Conc: 2.59 ng/ml

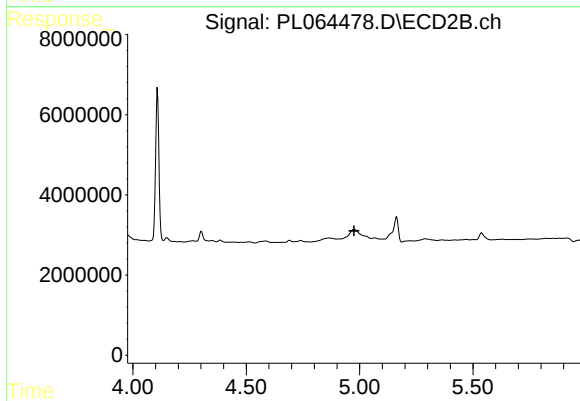

#6 beta-BHC


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 4432696
Conc: N.D.

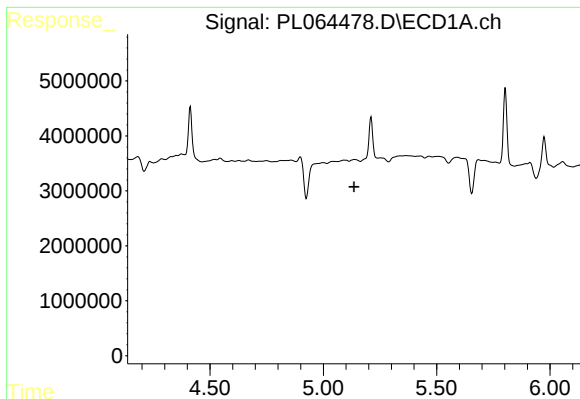

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

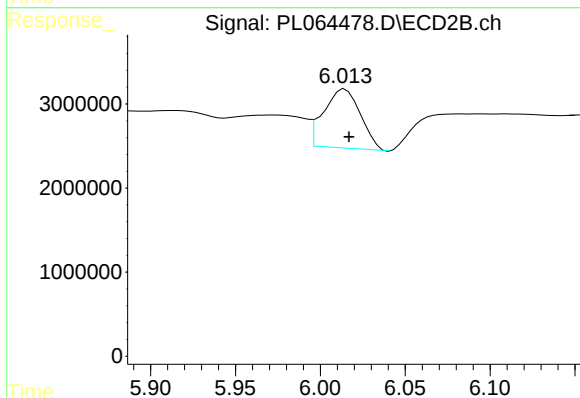


#8 Heptachlor epoxide

R.T.: 6.014 min
Delta R.T.: -0.003 min
Response: 10576402
Conc: 4.06 ng/ml

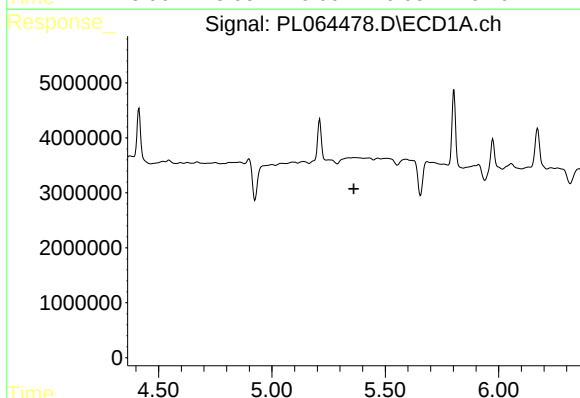


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

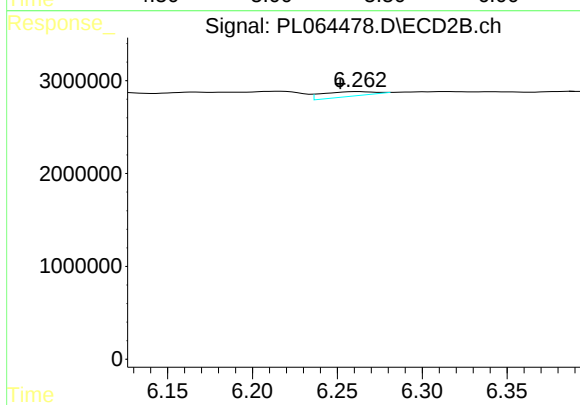

#10 gamma-Chlordane


R.T.: 6.263 min
Delta R.T.: 0.011 min
Response: 1066888
Conc: 0.36 ng/ml

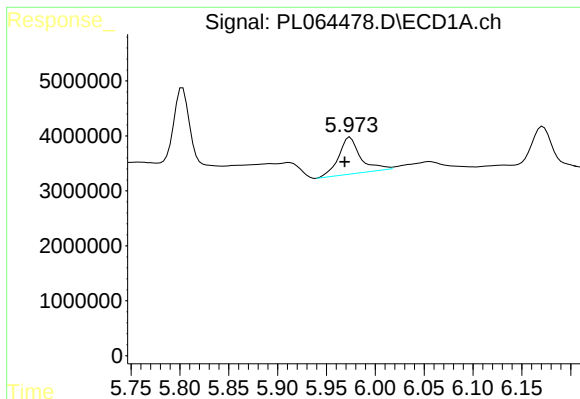

#14 Endrin


R.T.: 5.974 min
Delta R.T.: 0.006 min
Response: 10433435
Conc: 3.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

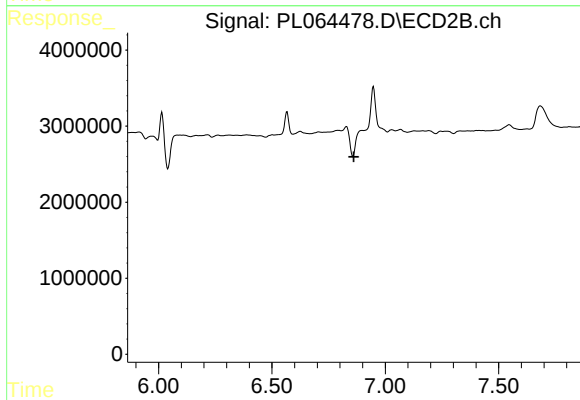


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.861 min
Response: 0
Conc: N.D.

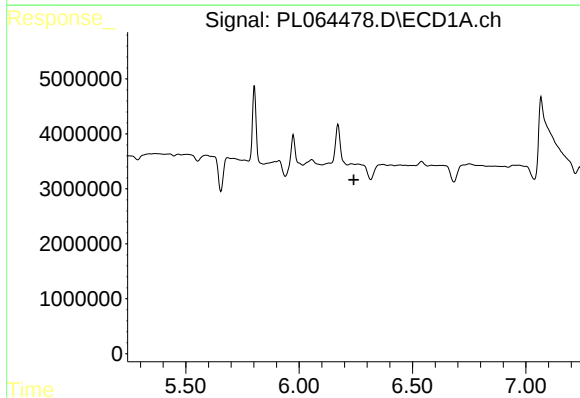


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

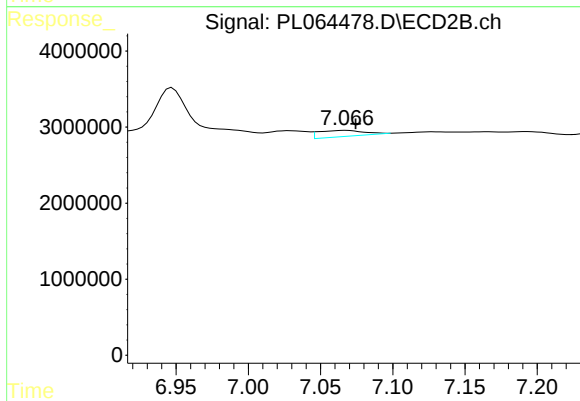

#15 Endosulfan II


R.T.: 7.068 min
Delta R.T.: -0.006 min
Response: 1753389
Conc: 0.69 ng/ml

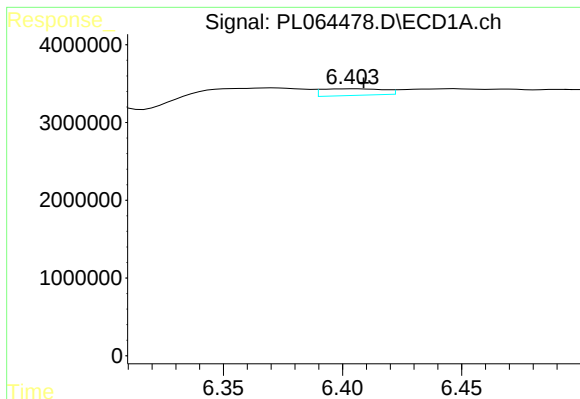

#18 Endrin aldehyde


R.T.: 6.405 min
Delta R.T.: -0.003 min
Response: 1532205
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

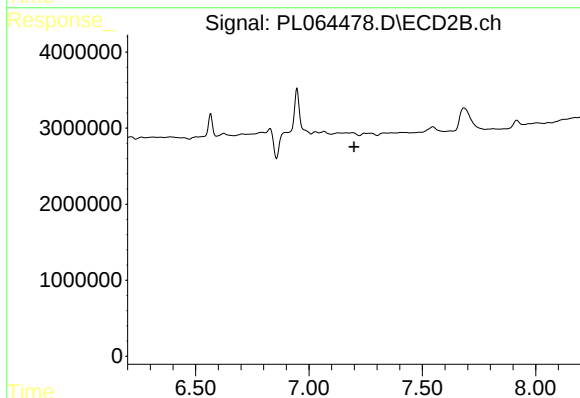


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

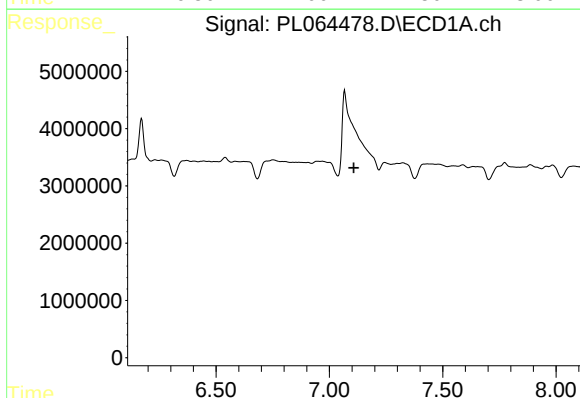


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.108 min
Response: 0
Conc: N.D.

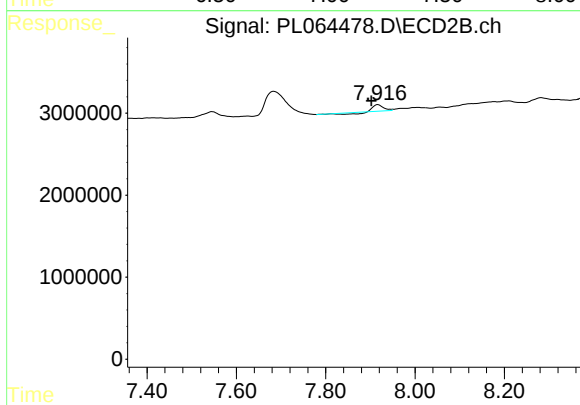

#21 Endrin ketone


R.T.: 7.917 min
Delta R.T.: 0.015 min
Response: 699609
Conc: 0.28 ng/ml

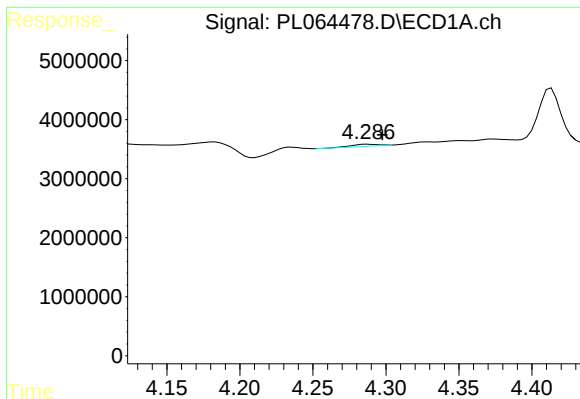

#23 Chlordane-1


R.T.: 4.288 min
Delta R.T.: -0.010 min
Response: 412321
Conc: 3.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

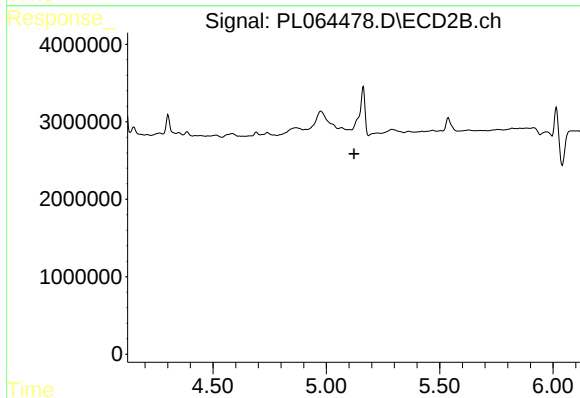


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

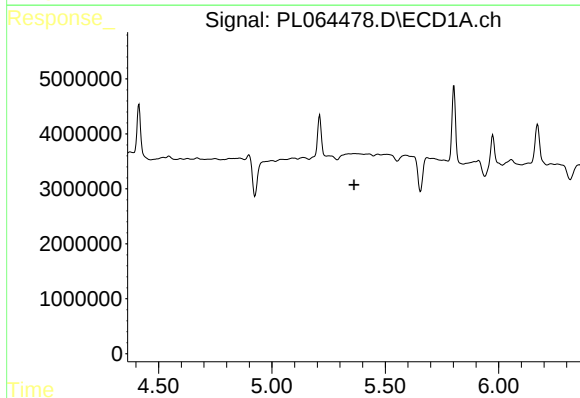


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

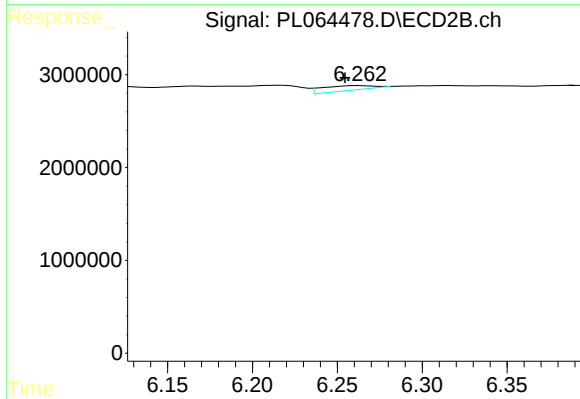

#25 Chlordane-3


R.T.: 6.263 min
Delta R.T.: 0.009 min
Response: 1066888
Conc: 2.64 ng/ml

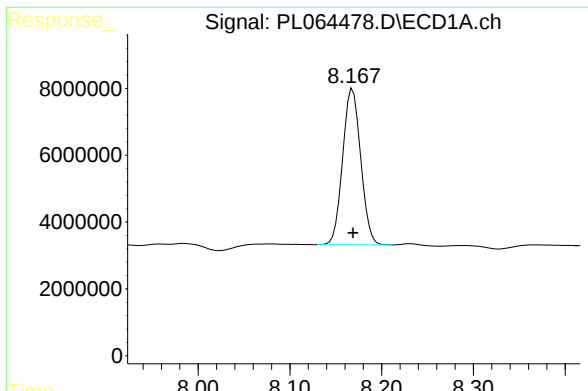

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 63824301
Conc: 20.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

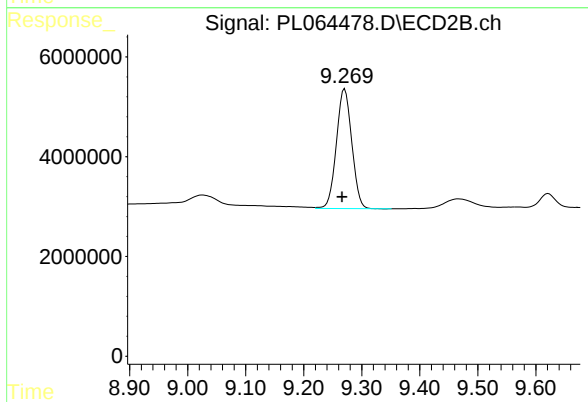

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.004 min
Response: 44218912
Conc: 18.63 ng/ml