

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
 Data File : PL064471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 13:20
 Operator : AR\AJ
 Sample : M1242-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0014-048-COMP-G

Manual Integrations
 APPROVED

Ankita
 1/29/2021 1:22:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 17:12:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.436	4.107	28570617	22756483	9.528m	8.902
28) SA Decachlor...	8.169	9.271	26476872	18722875	8.675	7.889

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
Data File : PL064471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 13:20
Operator : AR\AJ
Sample : M1242-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0014-048-COMP-G


Manual Integrations
APPROVED

Ankita
1/29/2021 1:22:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 17:12:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

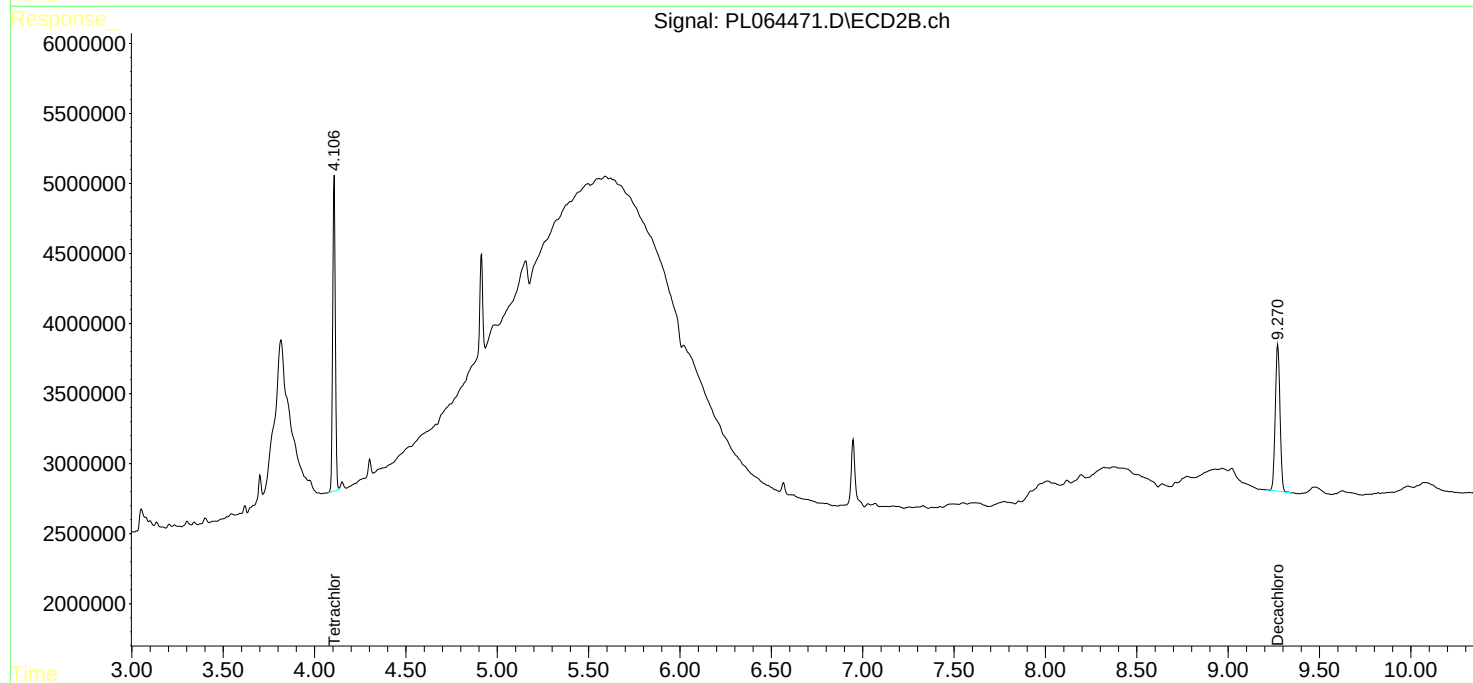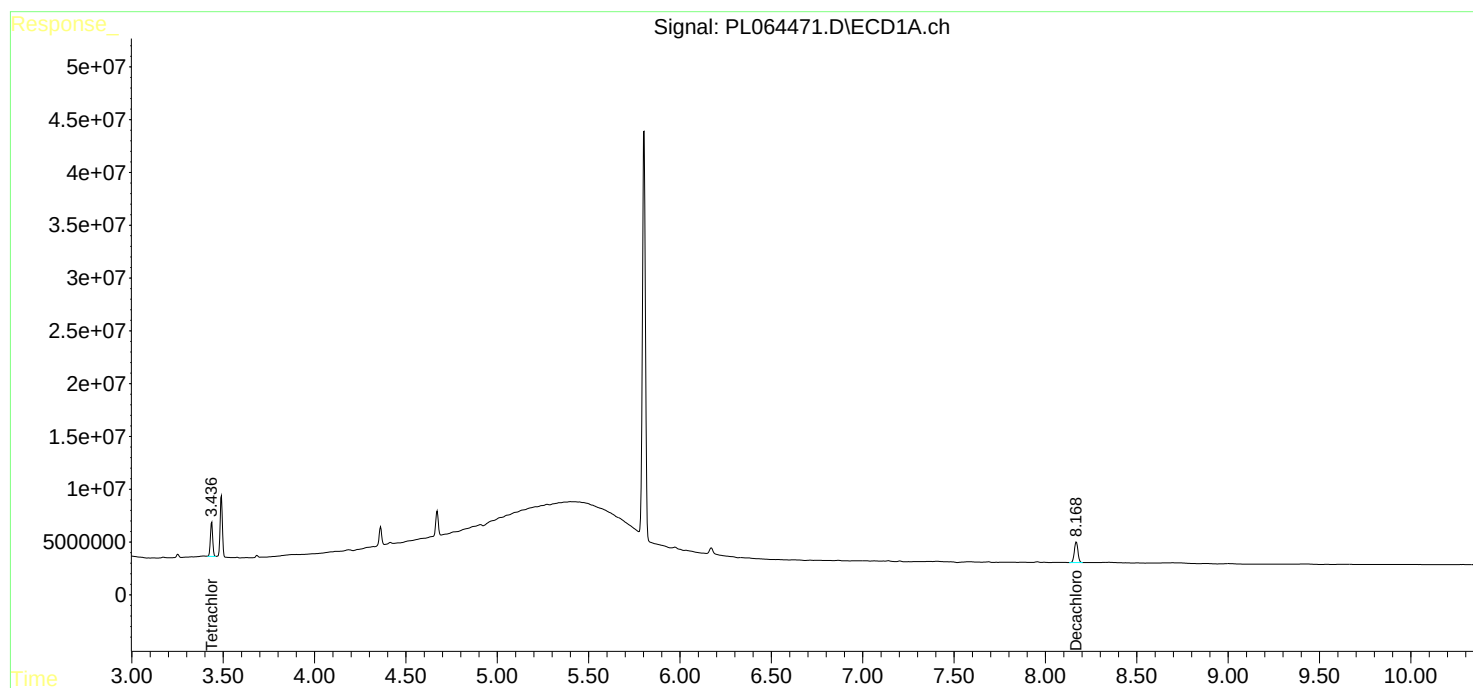

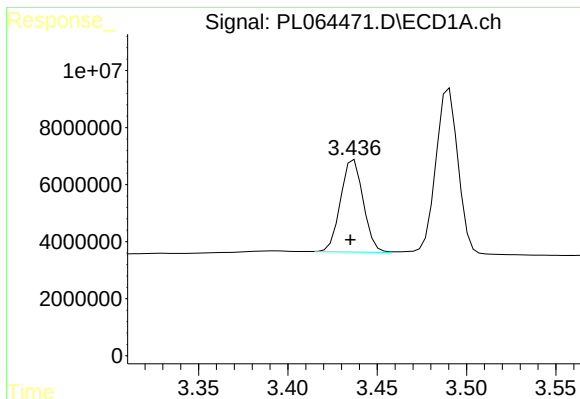

#1 Tetrachloro-m-xylene

R.T.: 3.436 min

Delta R.T.: 0.000 min


Response: 28570617

Conc: 9.53 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0014-048-COMP-G

Manual Integrations
APPROVED

Ankita
1/29/2021 1:22:34 PM

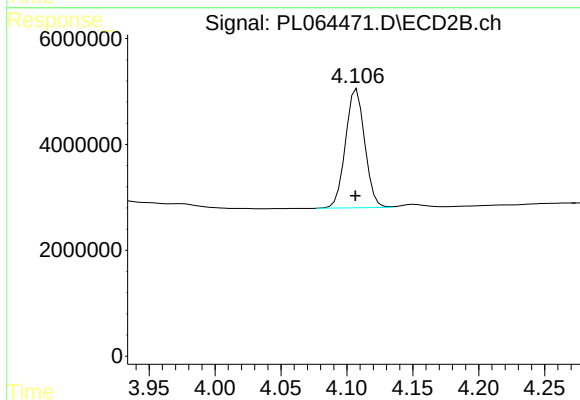


#1 Tetrachloro-m-xylene

R.T.: 4.107 min

Delta R.T.: 0.001 min

Response: 22756483

Conc: 8.90 ng/ml

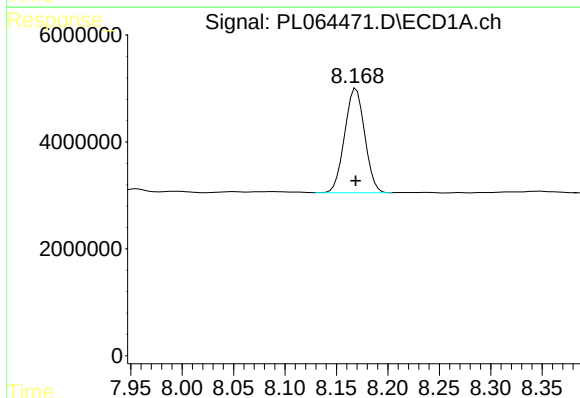


#28 Decachlorobiphenyl

R.T.: 8.169 min

Delta R.T.: 0.000 min

Response: 26476872

Conc: 8.68 ng/ml

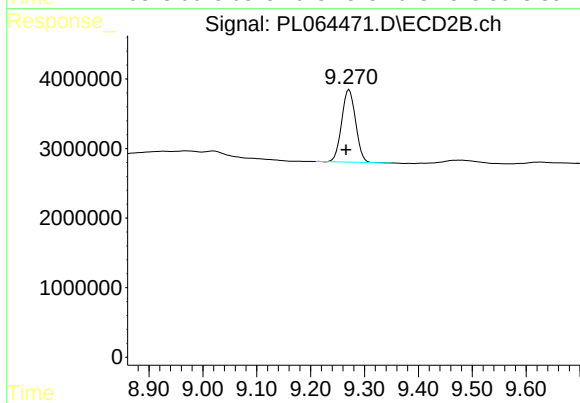

#28 Decachlorobiphenyl

R.T.: 9.271 min

Delta R.T.: 0.005 min

Response: 18722875

Conc: 7.89 ng/ml