

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
 Data File : PL064472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 13:35
 Operator : AR\AJ
 Sample : M1242-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0026-SITE-WATER-048-03-04

Manual Integrations
 APPROVED

Ankita
 1/29/2021 1:22:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 17:12:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.433	4.108	58450822	45154653	19.493m	17.663
28) SA Decachlor...	8.165	9.269	45682549	31211276	14.968	13.150

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012821\
Data File : PL064472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 13:35
Operator : AR\AJ
Sample : M1242-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0026-SITE-WATER-048-03-04


Manual Integrations
APPROVED

Ankita
1/29/2021 1:22:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 17:12:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

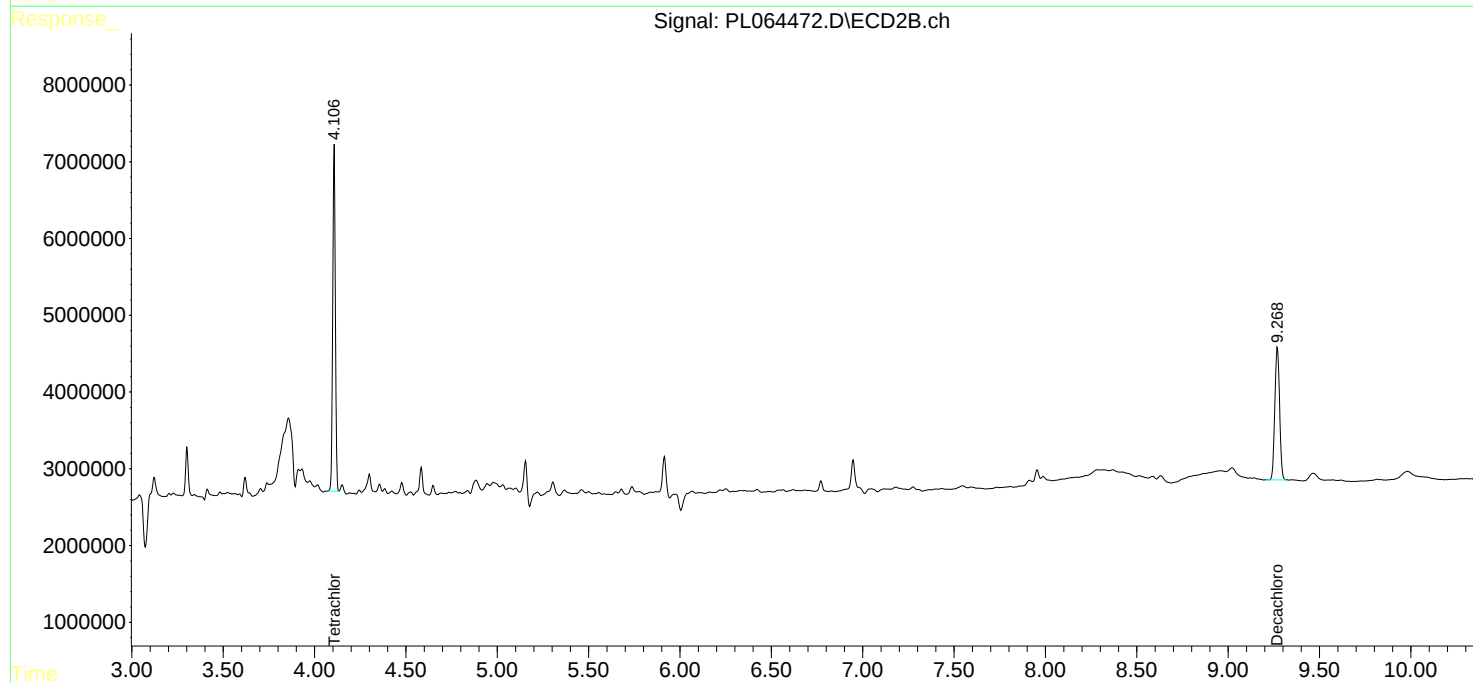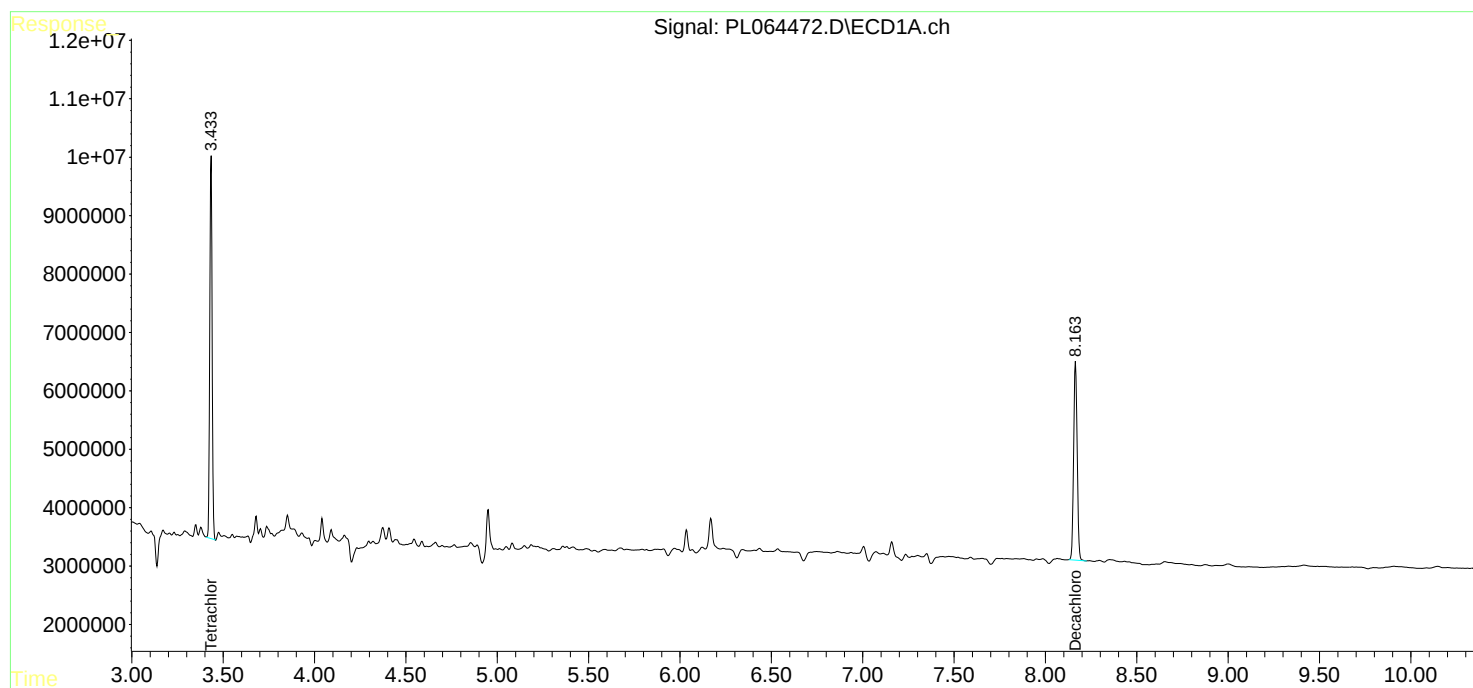

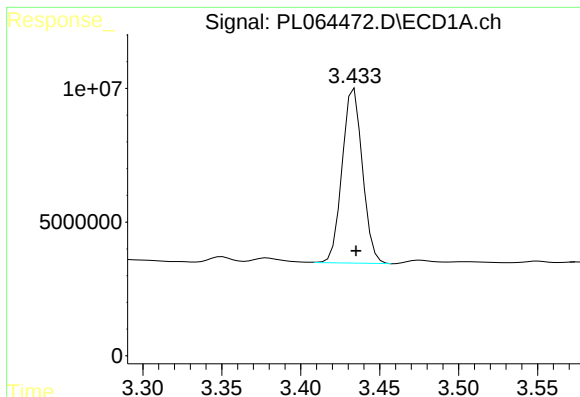


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: -0.002 min
Response: 58450822
Conc: 19.49 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0026-SITE-WATER-048-03-04


Manual Integrations
APPROVED

Ankita
1/29/2021 1:22:36 PM

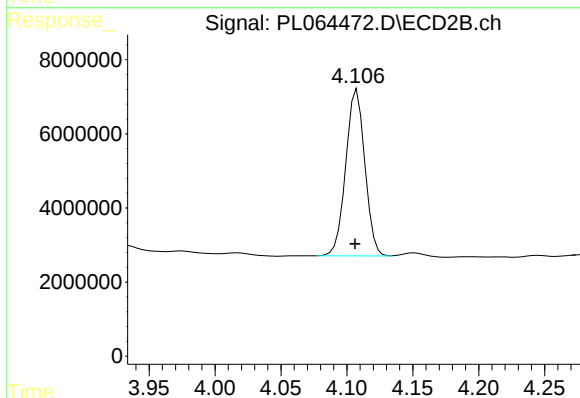


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 45154653
Conc: 17.66 ng/ml

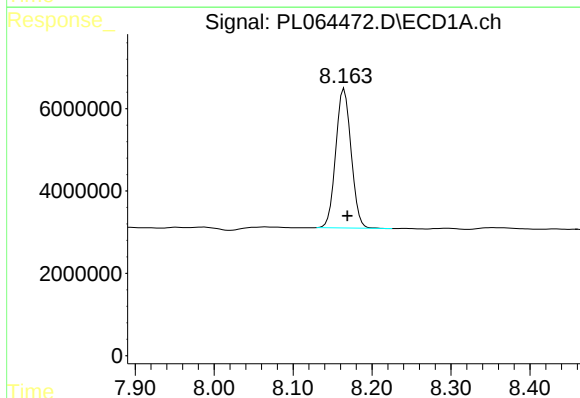

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 45682549
Conc: 14.97 ng/ml

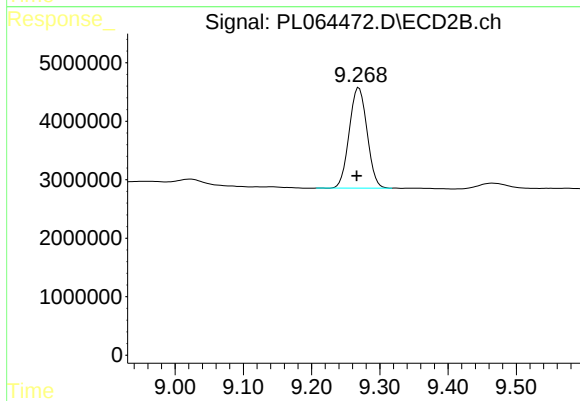

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.003 min
Response: 31211276
Conc: 13.15 ng/ml