

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 09:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:22:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.564	5.493	10009113	29731536	18.028	18.306
28)	SA Decachlor...	10.325	11.389	13637166	24228829	15.350	15.016
Target Compounds							
7)	B delta-BHC	0.000	7.019f	0	438839	N.D.	0.178 #
9)	A Endosulfan I	0.000	8.353	0	33514	N.D.	0.019 #
10)	B gamma-Chl...	0.000	8.241	0	76128	N.D.	0.038 #
11)	B alpha-Chl...	0.000	8.294	0	58155	N.D.	0.029 #
13)	MA Dieldrin	0.000	8.678f	0	179665	N.D.	0.091 #
15)	B Endosulfa...	0.000	9.149f	0	676053	N.D.	0.394 #
18)	B Endrin al...	0.000	9.251	0	35083	N.D.	0.028 #
19)	B Endosulfa...	0.000	9.500	0	56515	N.D.	0.036 #
25)	Chlordane-3	0.000	8.241	0	76128	N.D.	0.274 #
26)	Chlordane-4	0.000	8.294f	0	58155	N.D.	0.175 #
27)	Chlordane-5	0.000	9.202	0	223155	N.D.	3.657 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 09:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:22:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

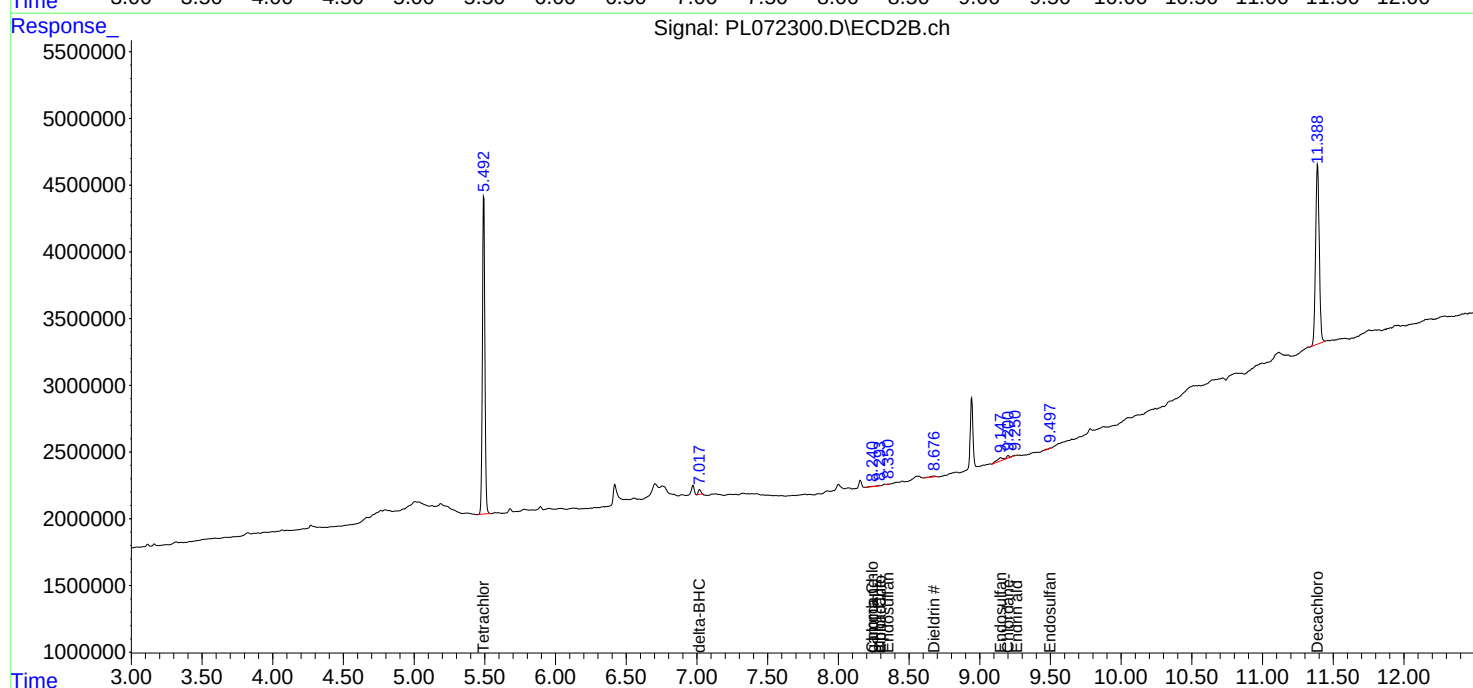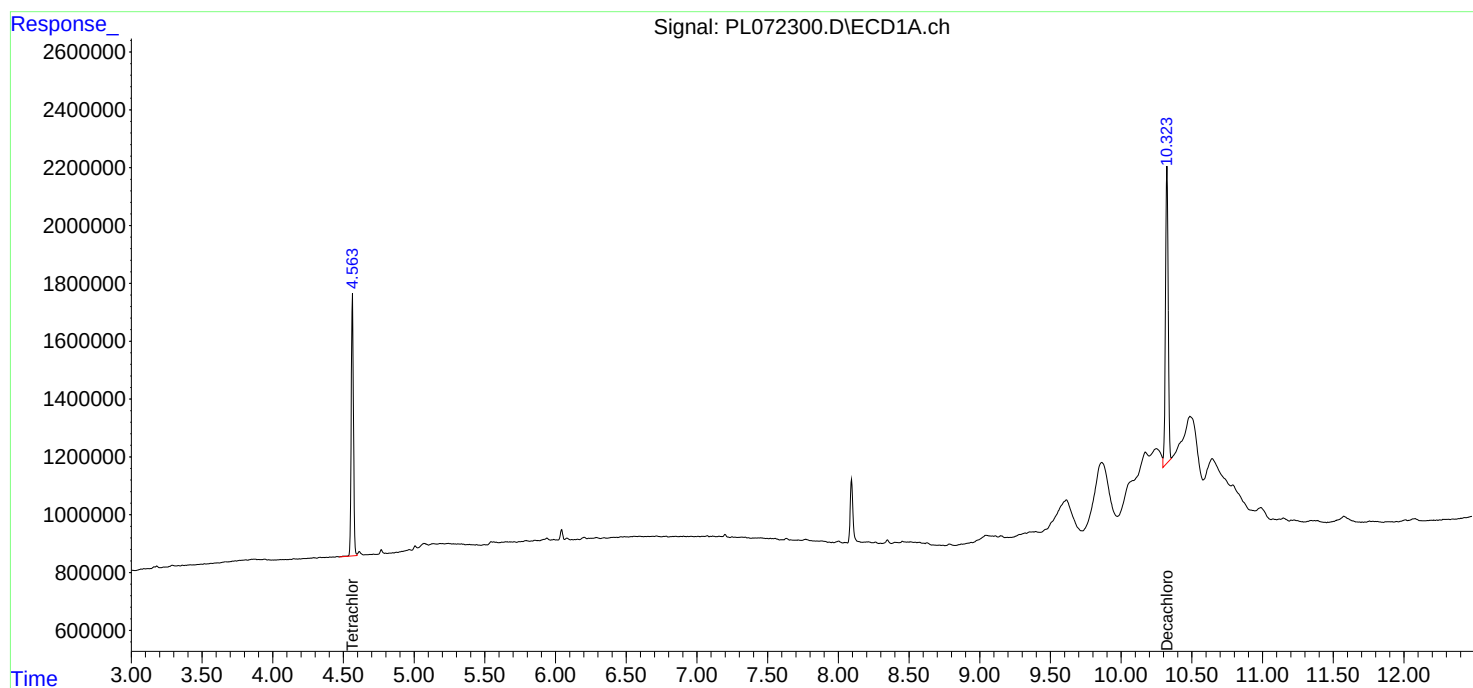


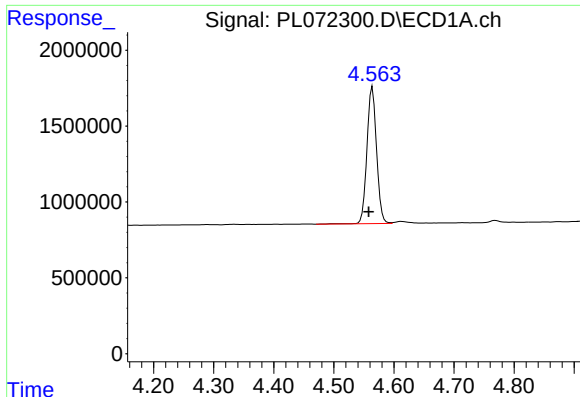

#1 Tetrachloro-m-xylene


R.T.: 4.564 min
Delta R.T.: 0.006 min
Response: 10009113
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

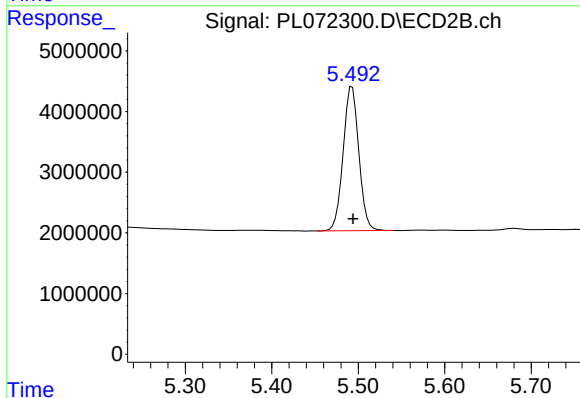


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: -0.001 min
Response: 29731536
Conc: 18.31 ng/ml

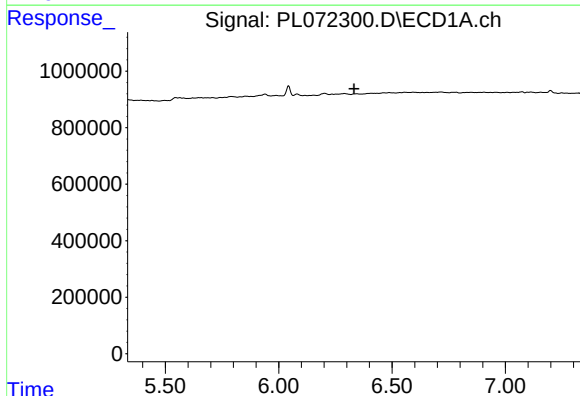


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

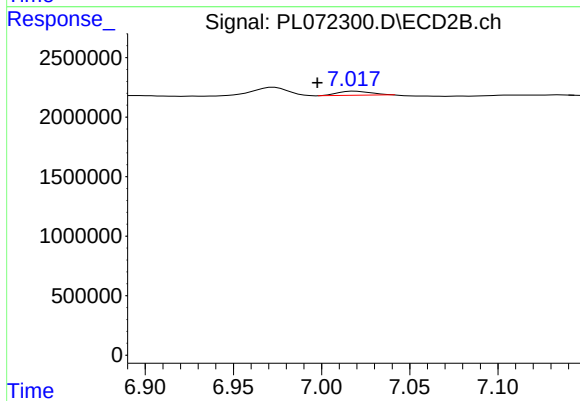

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.021 min
Response: 438839
Conc: 0.18 ng/ml

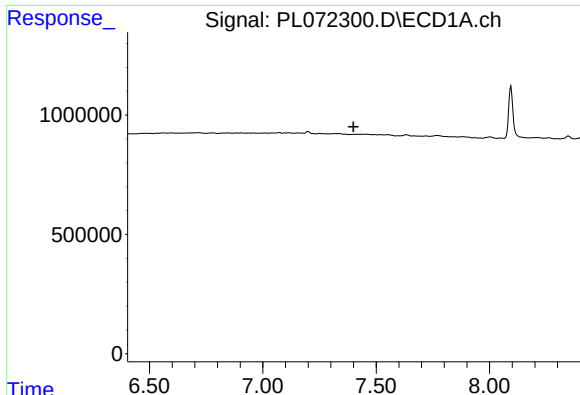

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

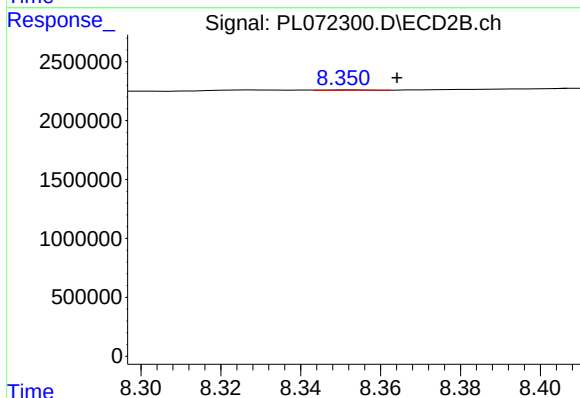


#9 Endosulfan I

R.T.: 8.353 min
Delta R.T.: -0.011 min
Response: 33514
Conc: 0.02 ng/ml

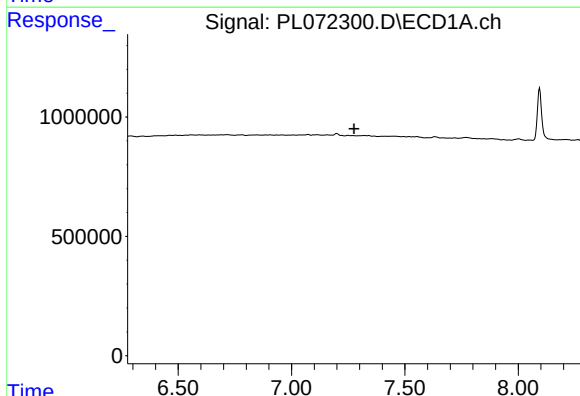


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

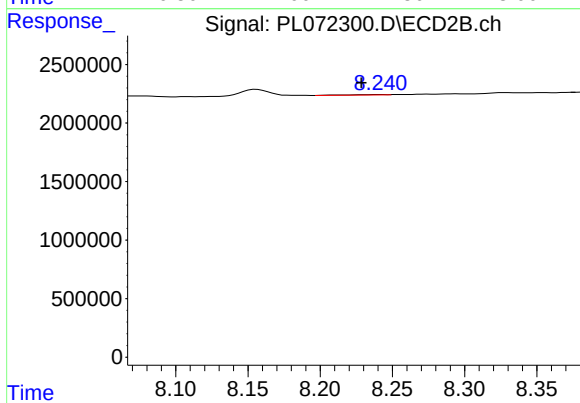

#10 gamma-Chlordane


R.T.: 8.241 min
Delta R.T.: 0.013 min
Response: 76128
Conc: 0.04 ng/ml

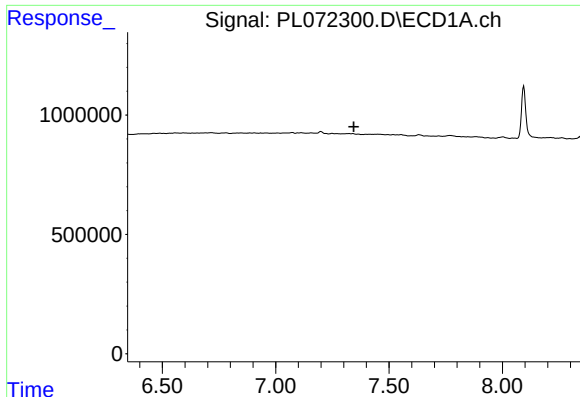

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

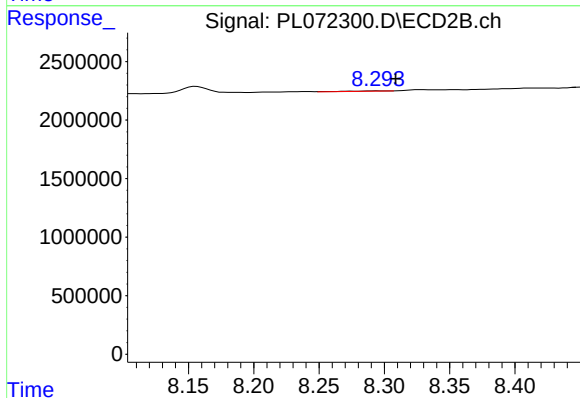


#11 alpha-Chlordane

R.T.: 8.294 min
Delta R.T.: -0.015 min
Response: 58155
Conc: 0.03 ng/ml

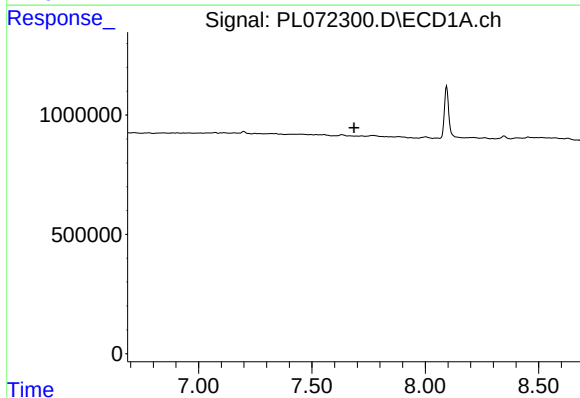


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

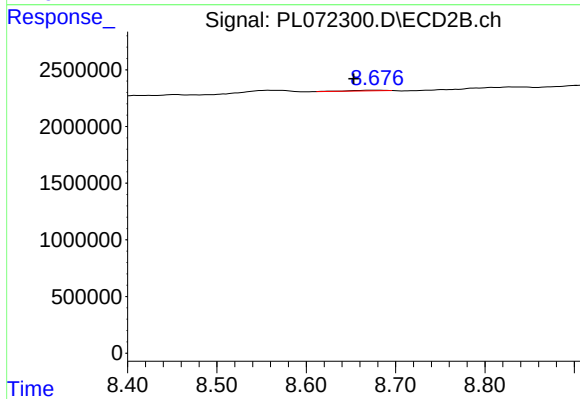

#13 Dieldrin


R.T.: 8.678 min
Delta R.T.: 0.024 min
Response: 179665
Conc: 0.09 ng/ml

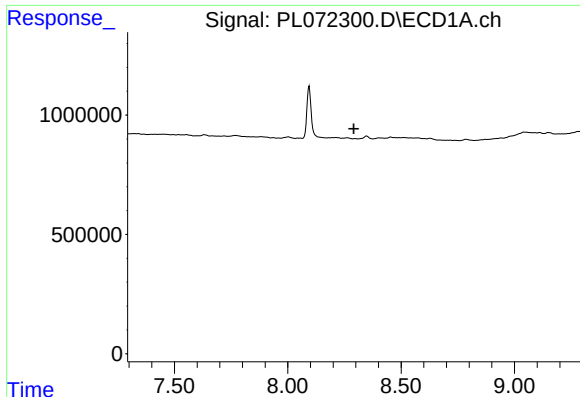

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

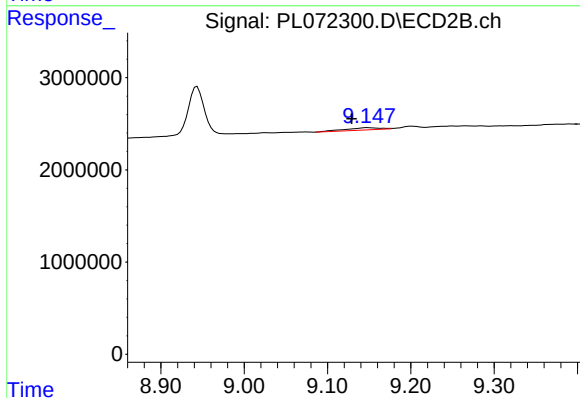


#15 Endosulfan II

R.T.: 9.149 min
Delta R.T.: 0.020 min
Response: 676053
Conc: 0.39 ng/ml

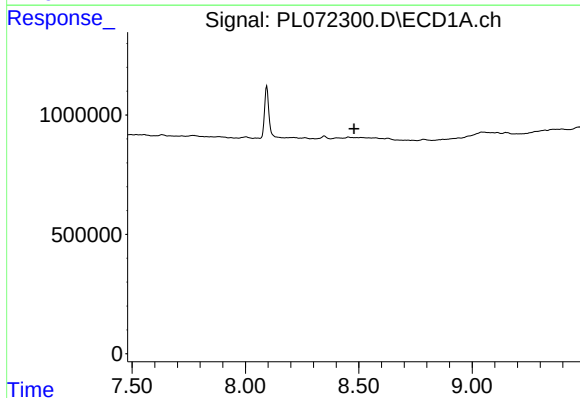


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

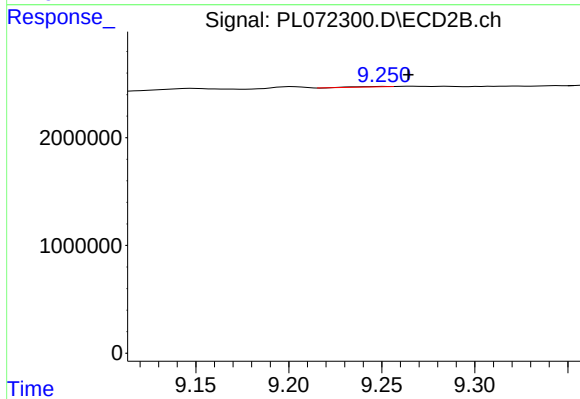

#18 Endrin aldehyde


R.T.: 9.251 min
Delta R.T.: -0.013 min
Response: 35083
Conc: 0.03 ng/ml

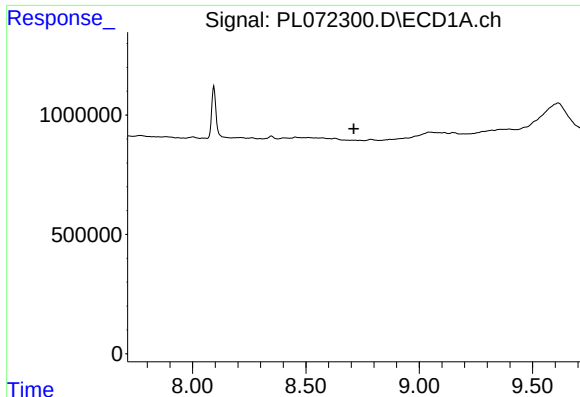

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

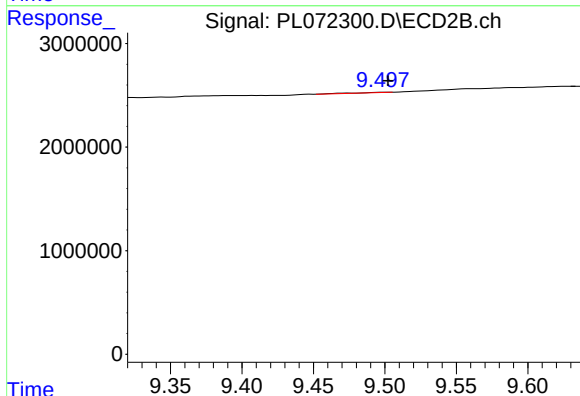


#19 Endosulfan Sulfate

R.T.: 9.500 min
Delta R.T.: -0.002 min
Response: 56515
Conc: 0.04 ng/ml

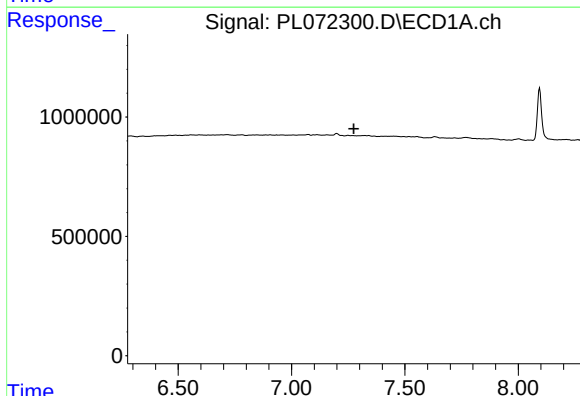


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

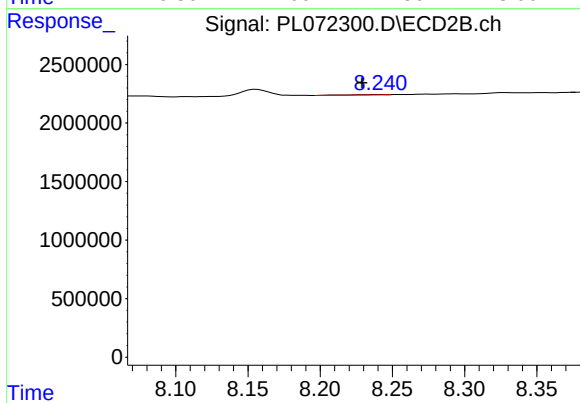

#25 Chlordane-3


R.T.: 8.241 min
Delta R.T.: 0.013 min
Response: 76128
Conc: 0.27 ng/ml

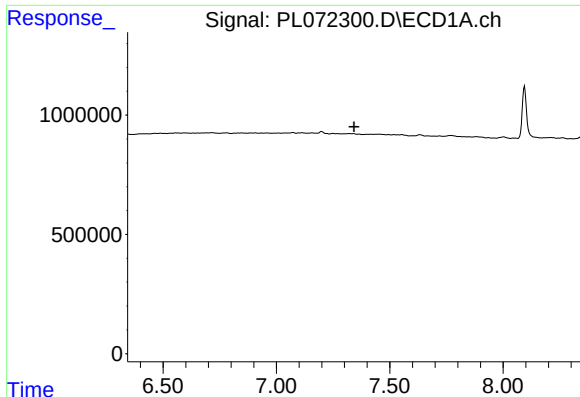

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

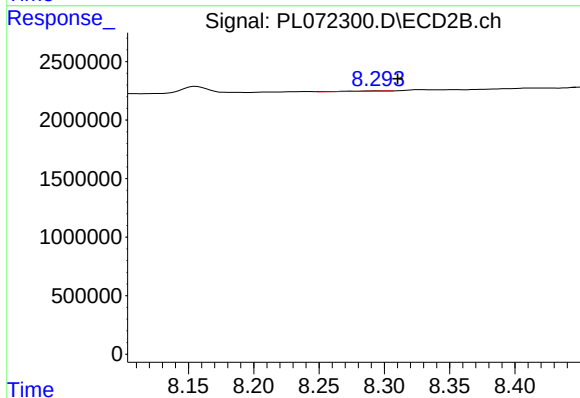


#26 Chlordane-4

R.T.: 8.294 min
Delta R.T.: -0.016 min
Response: 58155
Conc: 0.18 ng/ml

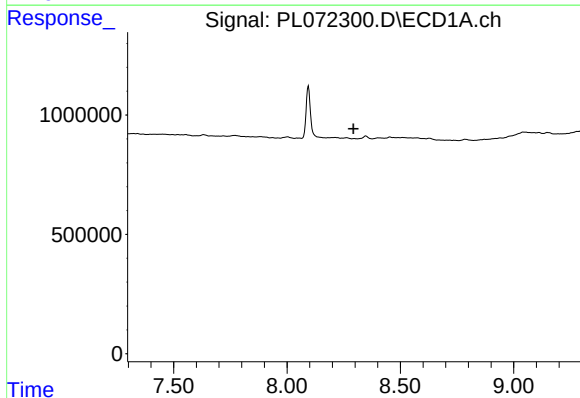


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

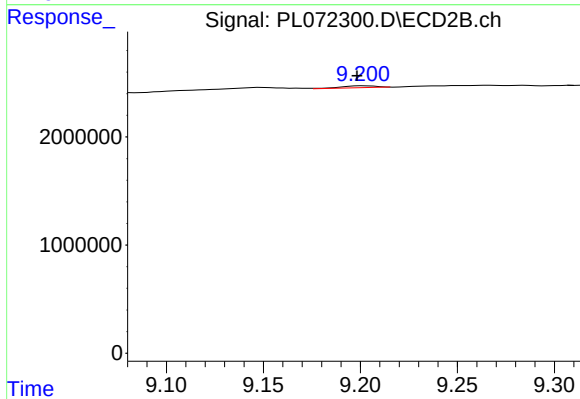

#27 Chlordane-5


R.T.: 9.202 min
Delta R.T.: 0.003 min
Response: 223155
Conc: 3.66 ng/ml

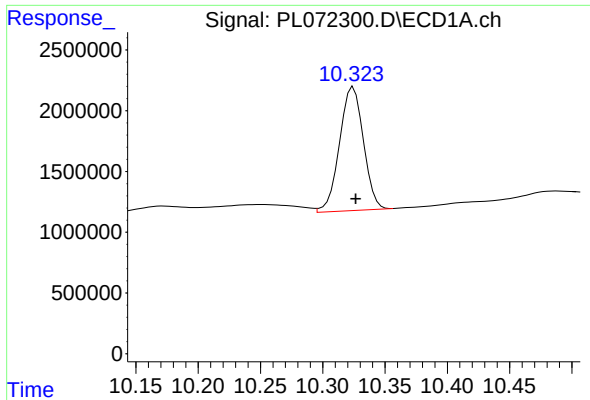

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: -0.002 min
Response: 13637166
Conc: 15.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

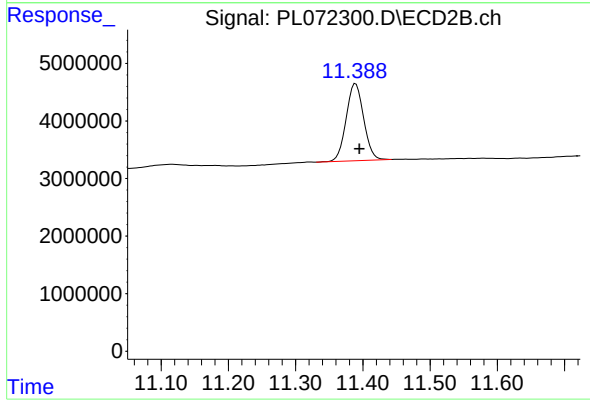

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.005 min
Response: 24228829
Conc: 15.02 ng/ml