

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 11:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:24:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10228653	30281116	18.424	18.645
28)	SA Decachlor...	10.318	11.385	14545810	24607288	16.372	15.251
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	1153462	N.D.	0.469 #
9)	A Endosulfan I	0.000	8.354	0	21252	N.D.	0.012 #
10)	B gamma-Chl...	0.000	8.227	0	143860	N.D.	0.071 #
11)	B alpha-Chl...	0.000	8.317	0	80593	N.D.	0.041 #
15)	B Endosulfa...	0.000	9.146f	0	334716	N.D.	0.195 #
20)	A Methoxychlor	0.000	9.867f	0	196536	N.D.	0.237 #
22)	Mirex	0.000	10.483f	0	131370	N.D.	0.105 #
23)	Chlordane-1	0.000	6.898f	0	61594	N.D.	0.944 #
25)	Chlordane-3	0.000	8.227	0	143860	N.D.	0.518 #
26)	Chlordane-4	0.000	8.317	0	80593	N.D.	0.243 #
27)	Chlordane-5	0.000	9.200	0	291627	N.D.	4.779 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 11:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:24:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

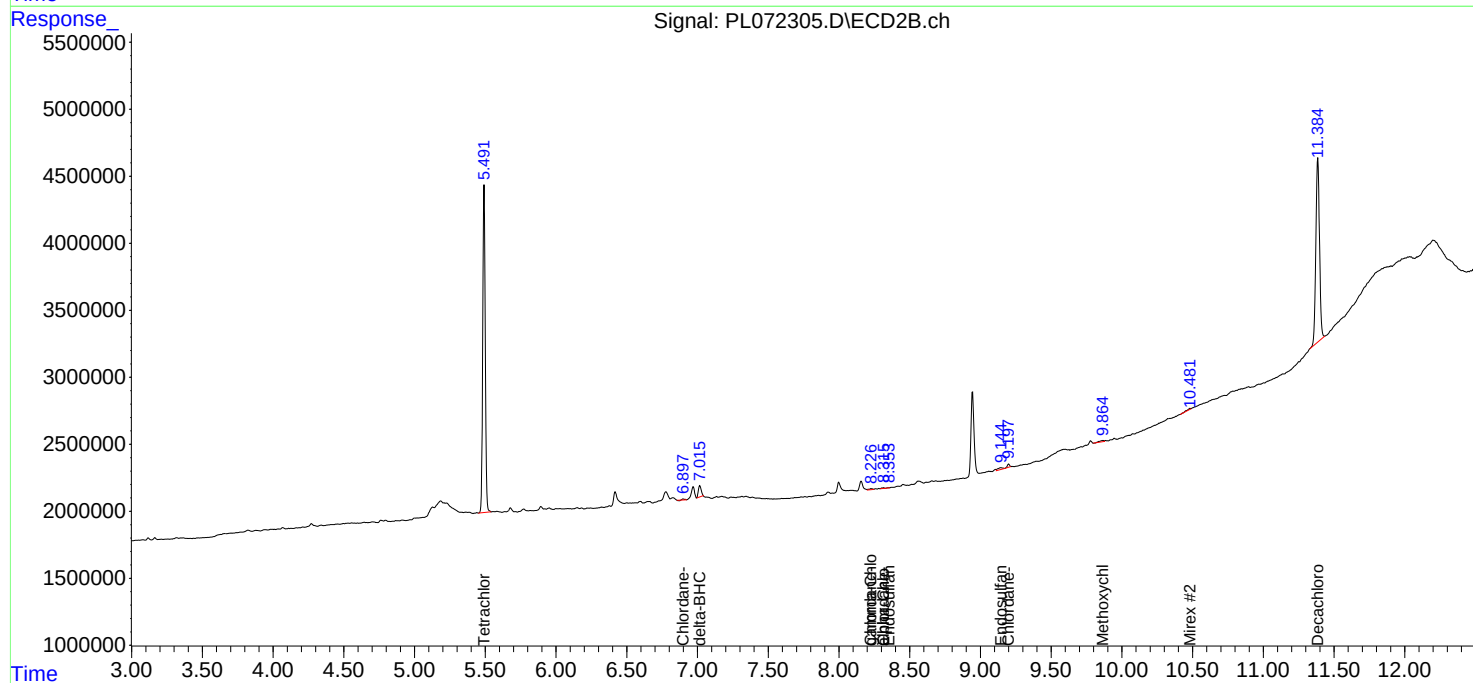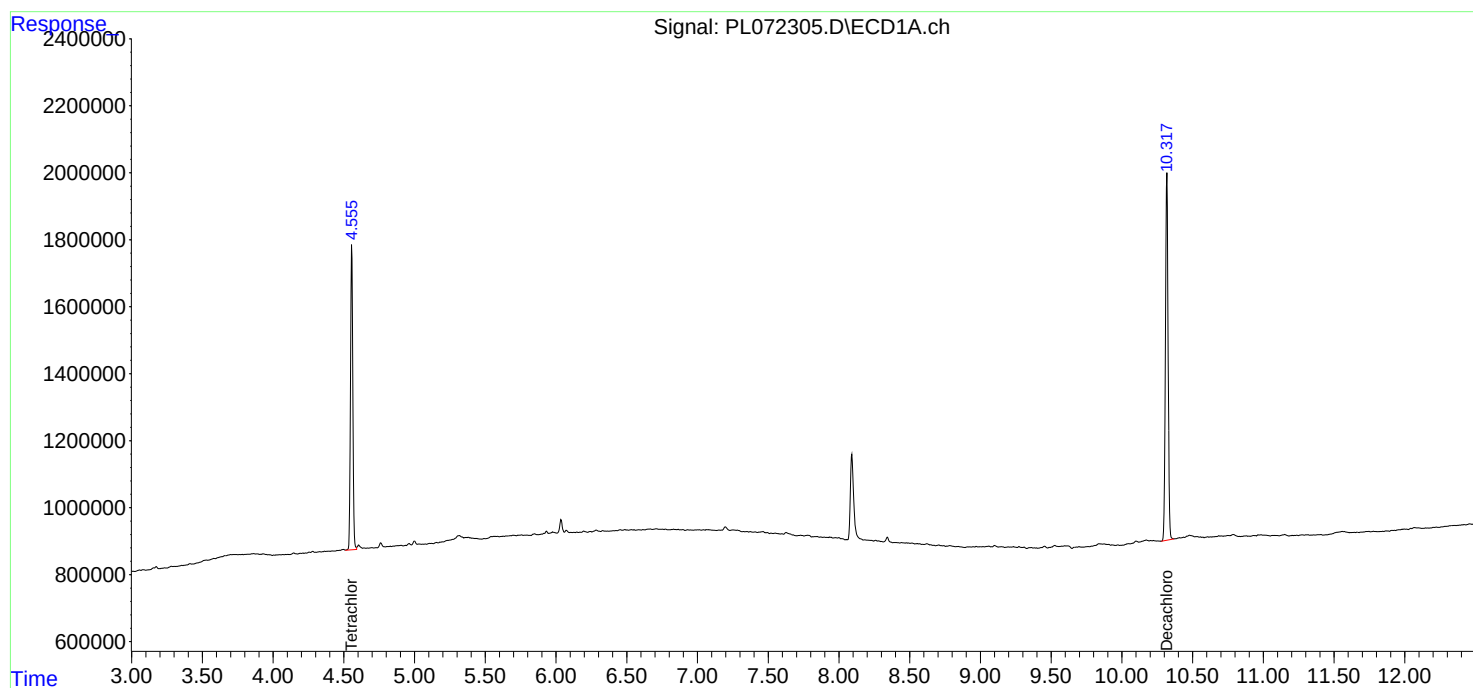


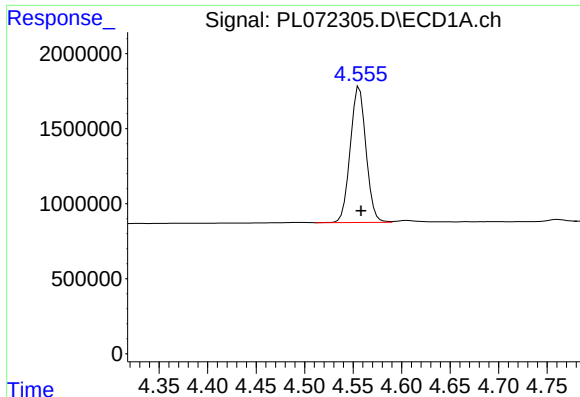

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10228653
Conc: 18.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

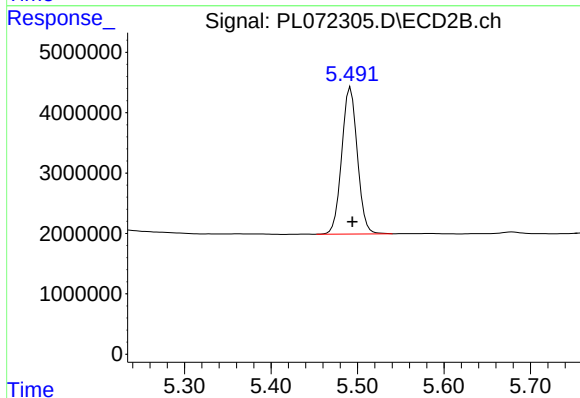


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 30281116
Conc: 18.64 ng/ml

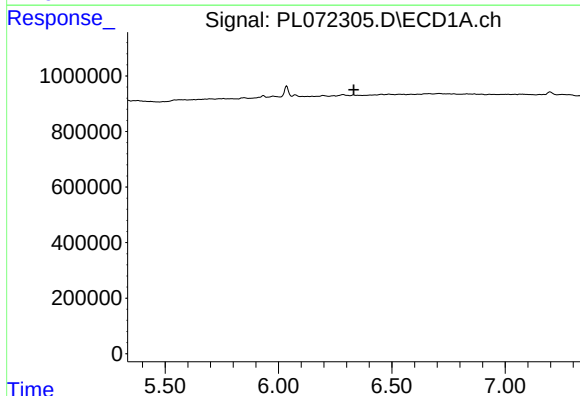


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

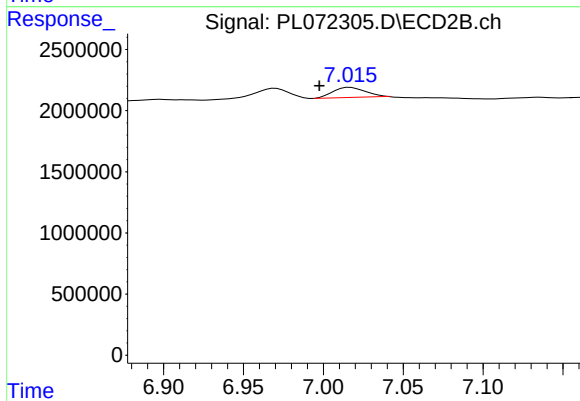

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 1153462
Conc: 0.47 ng/ml

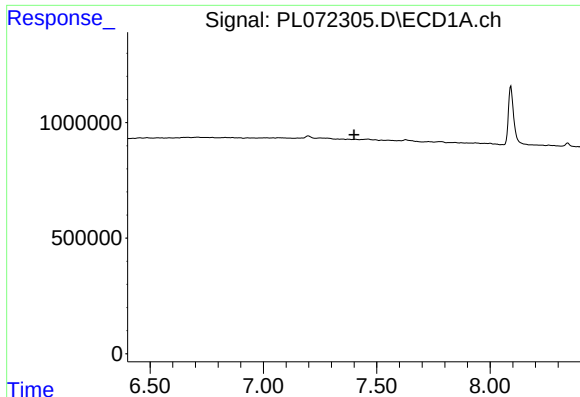

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

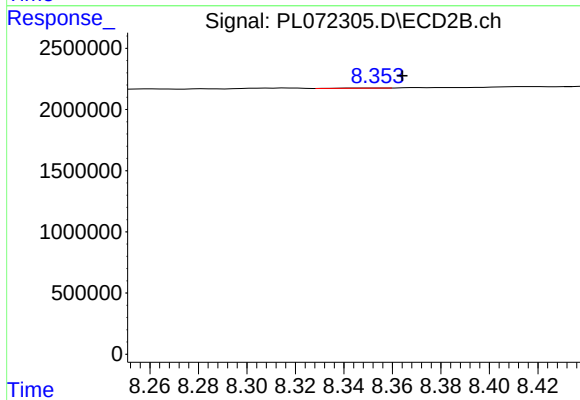


#9 Endosulfan I

R.T.: 8.354 min
Delta R.T.: -0.010 min
Response: 21252
Conc: 0.01 ng/ml

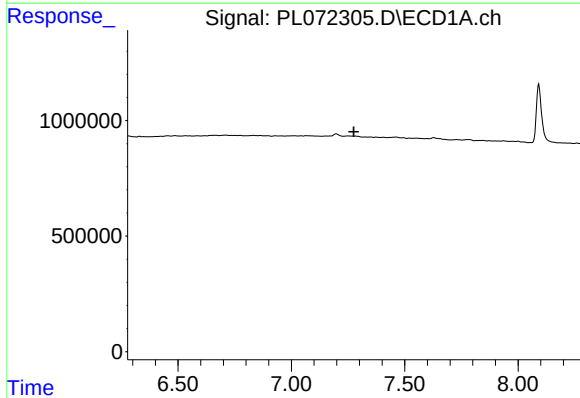


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

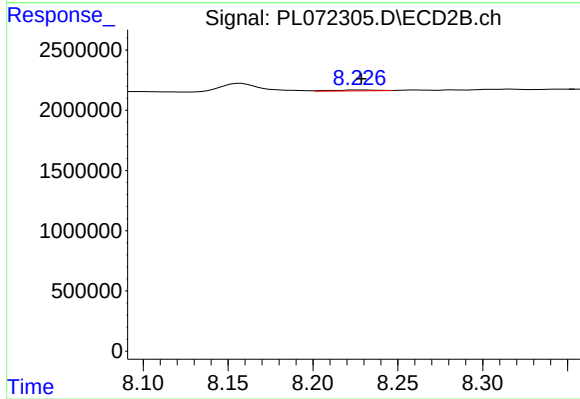

#10 gamma-Chlordane


R.T.: 8.227 min
Delta R.T.: -0.001 min
Response: 143860
Conc: 0.07 ng/ml

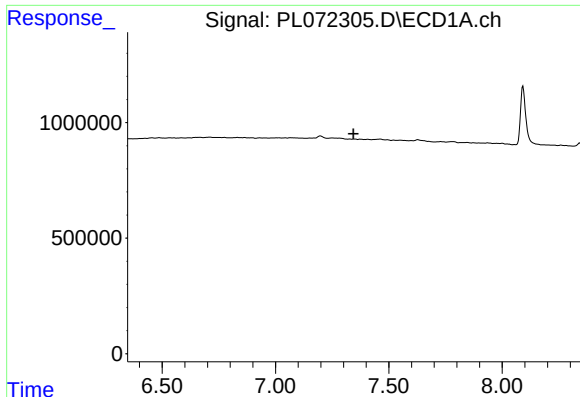

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

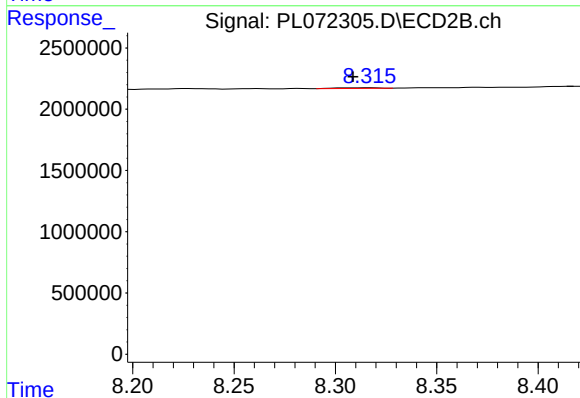


#11 alpha-Chlordane

R.T.: 8.317 min
Delta R.T.: 0.008 min
Response: 80593
Conc: 0.04 ng/ml

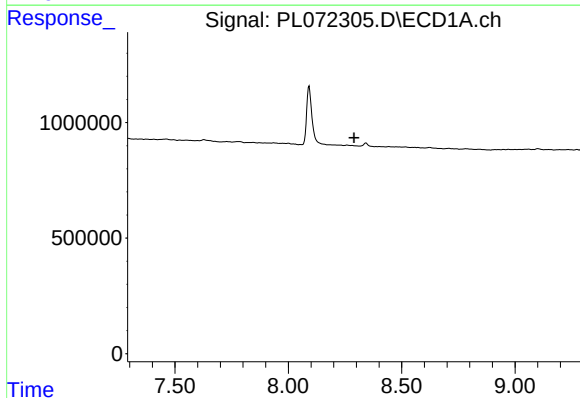


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

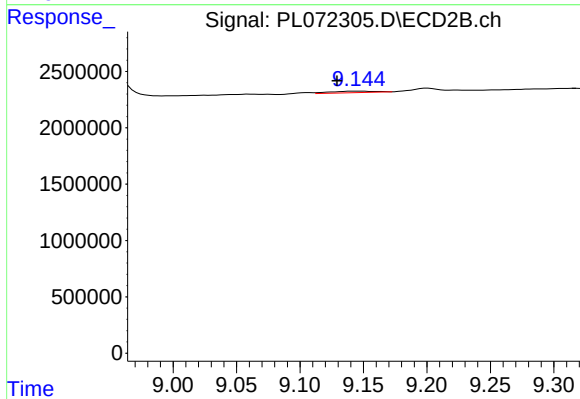

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 334716
Conc: 0.20 ng/ml

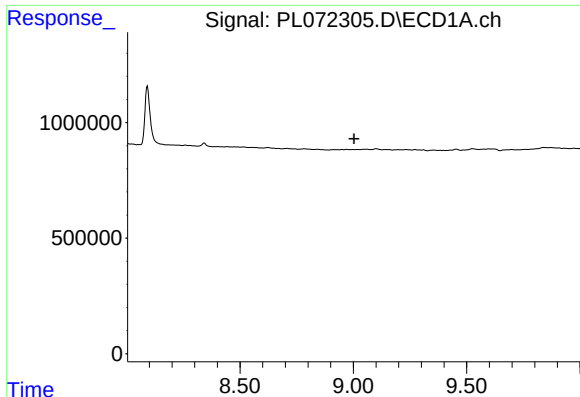

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

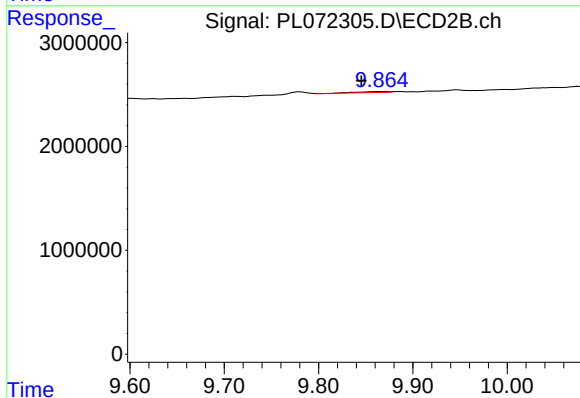


#20 Methoxychlor

R.T.: 9.867 min
Delta R.T.: 0.022 min
Response: 196536
Conc: 0.24 ng/ml

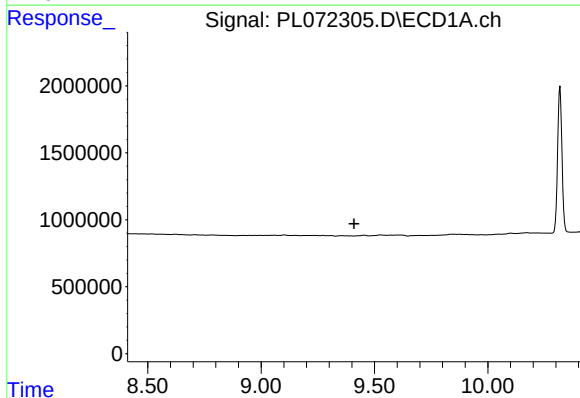


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

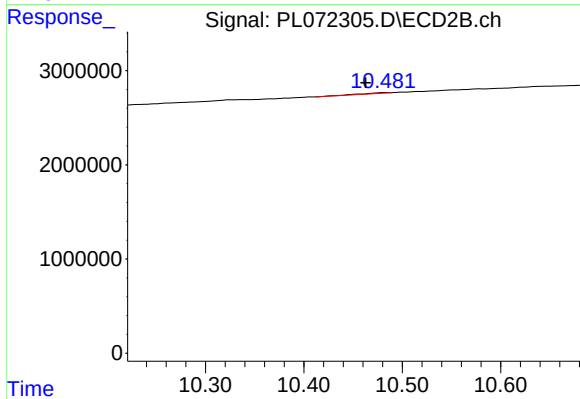

#22 Mirex


R.T.: 10.483 min
Delta R.T.: 0.020 min
Response: 131370
Conc: 0.11 ng/ml

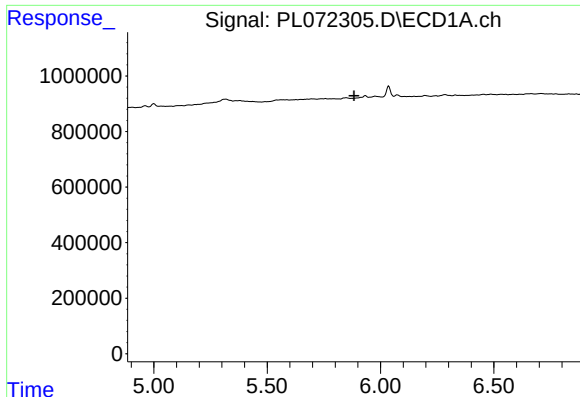

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

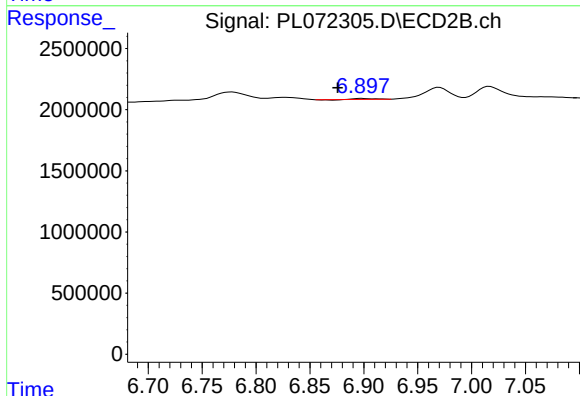


#23 Chlordane-1

R.T.: 6.898 min
Delta R.T.: 0.022 min
Response: 61594
Conc: 0.94 ng/ml

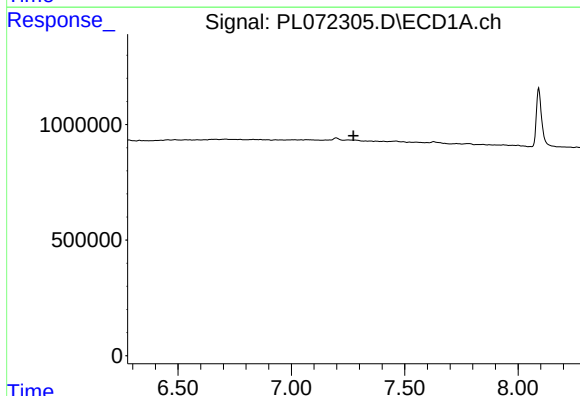


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.274 min
Response: 0
Conc: N.D.

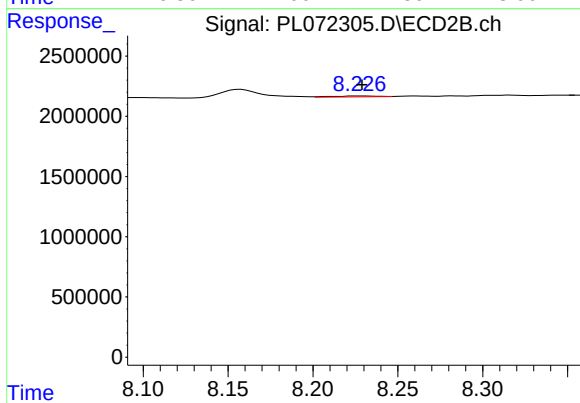

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: -0.002 min
Response: 143860
Conc: 0.52 ng/ml

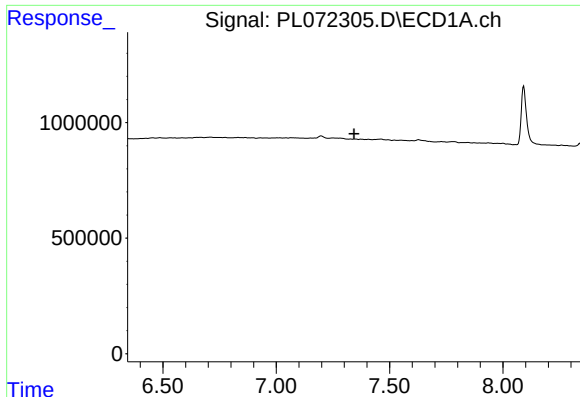

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

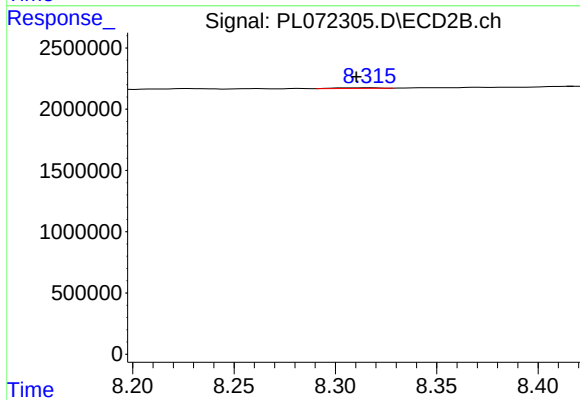


#26 Chlordane-4

R.T.: 8.317 min
Delta R.T.: 0.007 min
Response: 80593
Conc: 0.24 ng/ml

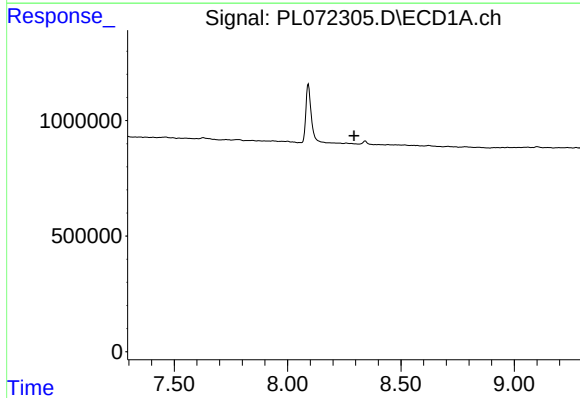


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

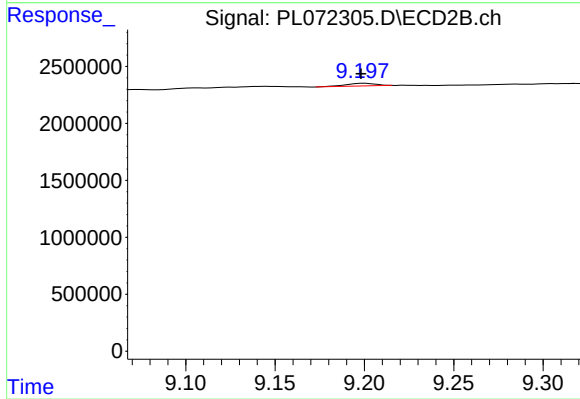

#27 Chlordane-5


R.T.: 9.200 min
Delta R.T.: 0.002 min
Response: 291627
Conc: 4.78 ng/ml

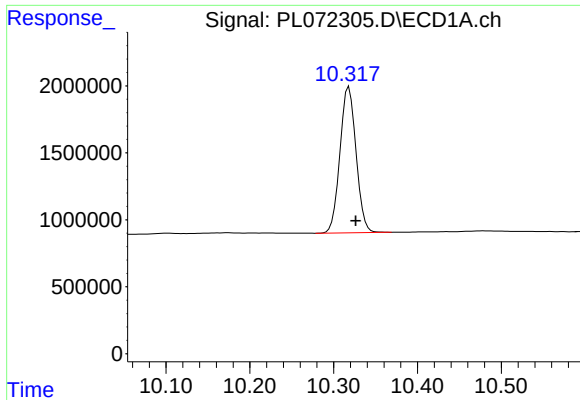

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 14545810
Conc: 16.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

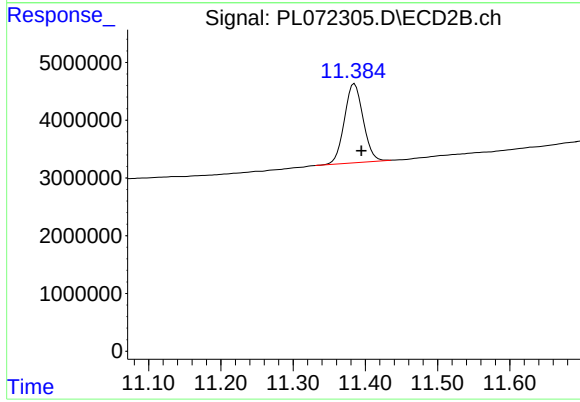

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 24607288
Conc: 15.25 ng/ml