

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 12:43
 Operator : AR\AJ
 Sample : PB142339BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:25:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.493	10090183	30003324	18.174	18.474
28)	SA Decachlor...	10.325	11.390	14713541	26092631	16.561	16.171
Target Compounds							
6)	B beta-BHC	6.045f	0.000	219614	0	0.664	N.D. #
7)	B delta-BHC	0.000	7.018f	0	2671237	N.D.	1.086 #
9)	A Endosulfan I	0.000	8.376	0	31260	N.D.	0.017 #
10)	B gamma-Chl...	0.000	8.225	0	68350	N.D.	0.034 #
14)	MA Endrin	0.000	8.917f	0	135908	N.D.	0.082 #
15)	B Endosulfa...	0.000	9.144f	0	1026516	N.D.	0.599 #
16)	A 4,4'-DDD	0.000	9.050	0	225167	N.D.	0.157 #
17)	MA 4,4'-DDT	0.000	9.381f	0	153154	N.D.	0.097 #
18)	B Endrin al...	0.000	9.268	0	194742	N.D.	0.157 #
20)	A Methoxychlor	0.000	9.839	0	191912	N.D.	0.232 #
25)	Chlordane-3	0.000	8.225	0	68350	N.D.	0.246 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 12:43
Operator : AR\AJ
Sample : PB142339BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:25:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

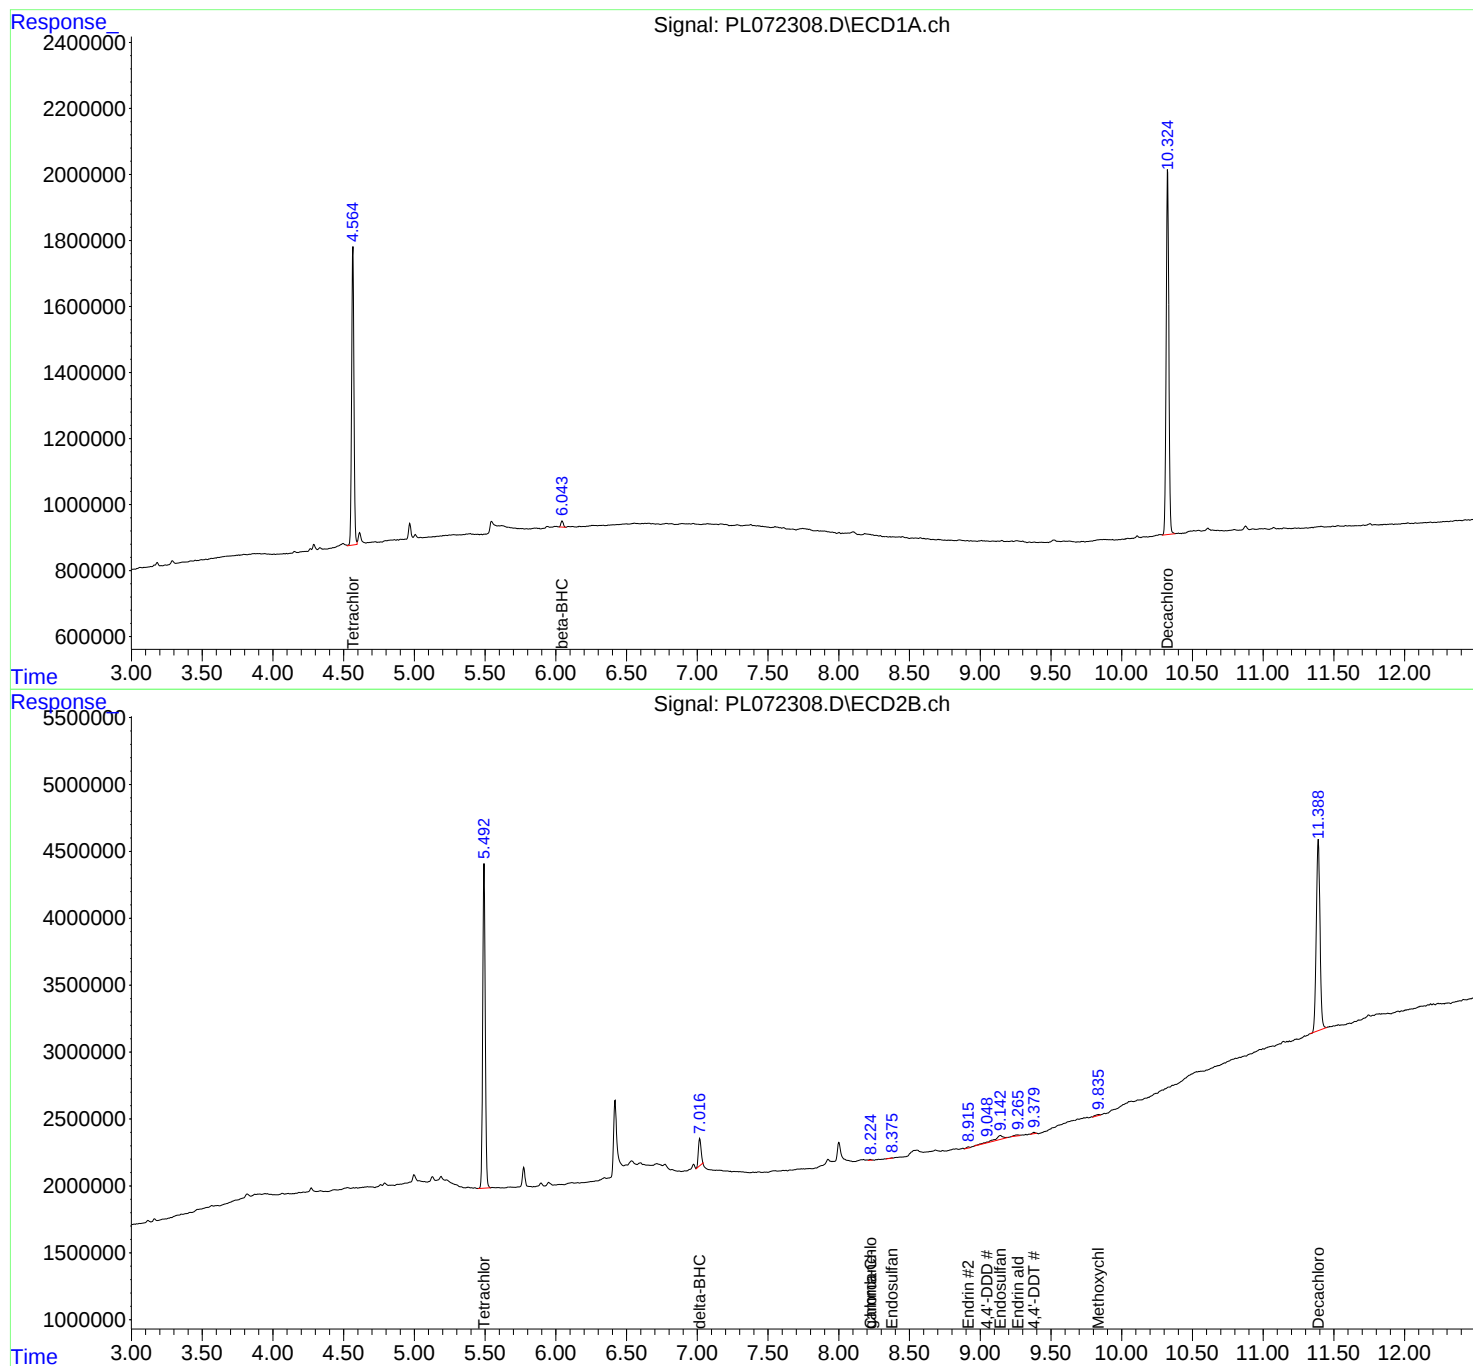


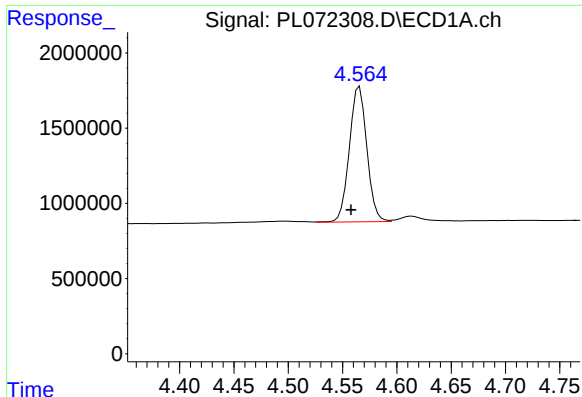

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: 0.008 min
Response: 10090183
Conc: 18.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

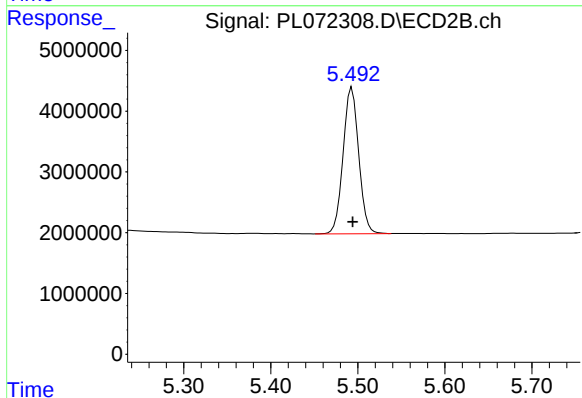


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 30003324
Conc: 18.47 ng/ml

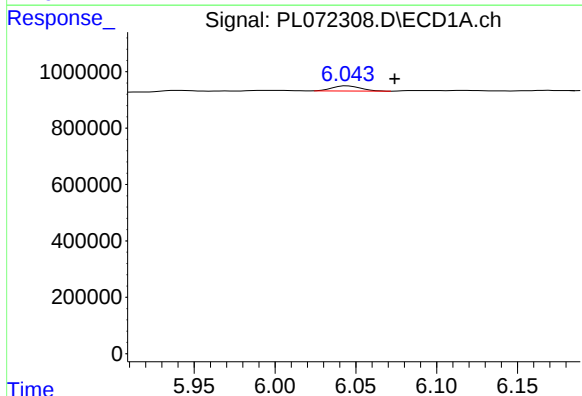


#6 beta-BHC

R.T.: 6.045 min
Delta R.T.: -0.029 min
Response: 219614
Conc: 0.66 ng/ml

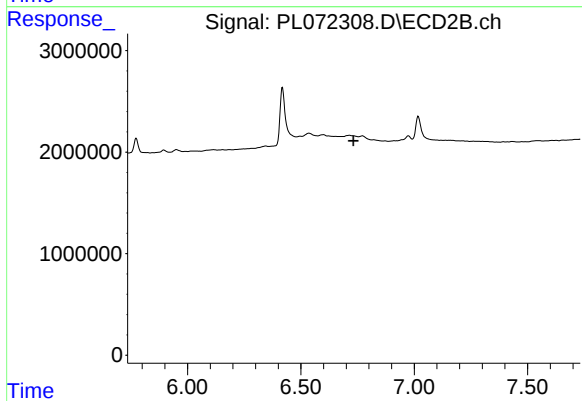

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.732 min
Response: 0
Conc: N.D.

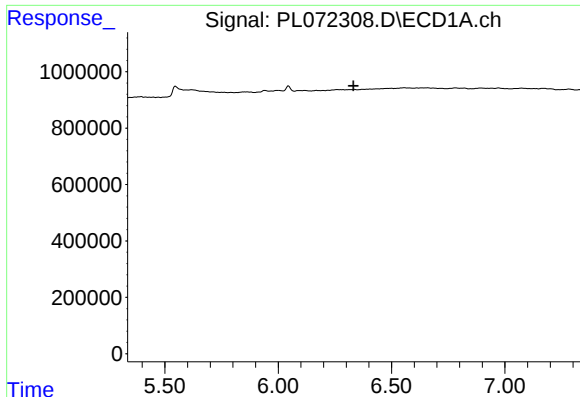

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

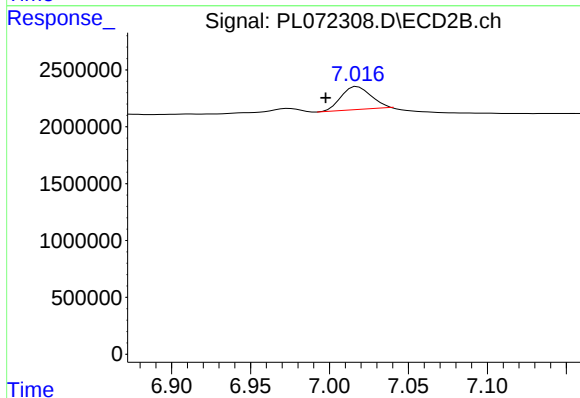


#7 delta-BHC

R.T.: 7.018 min
Delta R.T.: 0.020 min
Response: 2671237
Conc: 1.09 ng/ml

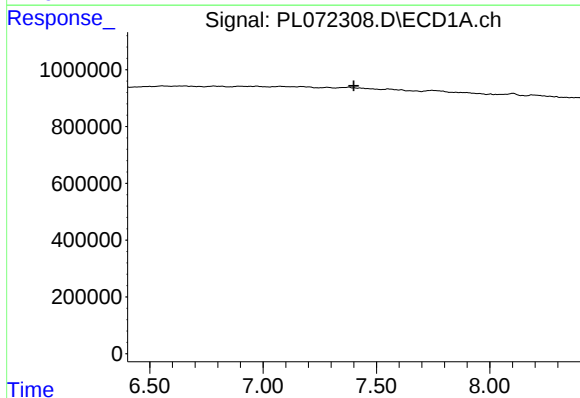


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

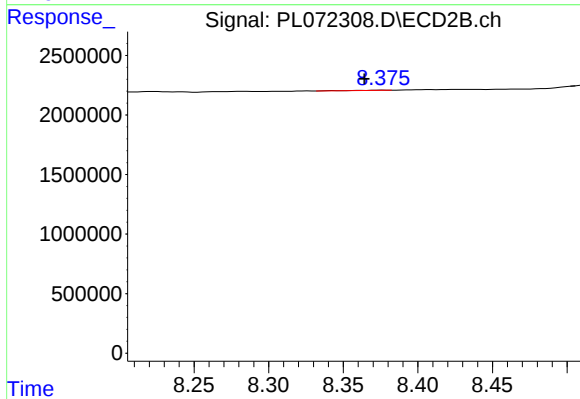

#9 Endosulfan I


R.T.: 8.376 min
Delta R.T.: 0.012 min
Response: 31260
Conc: 0.02 ng/ml

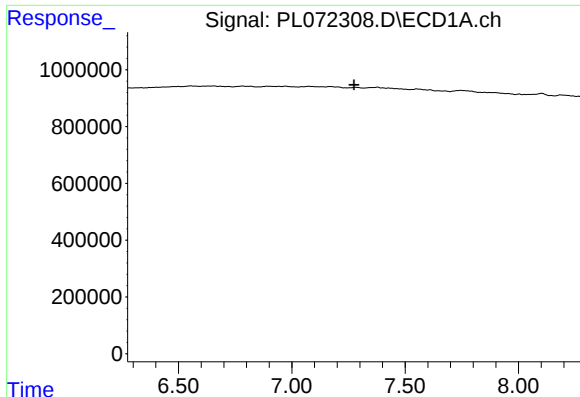

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

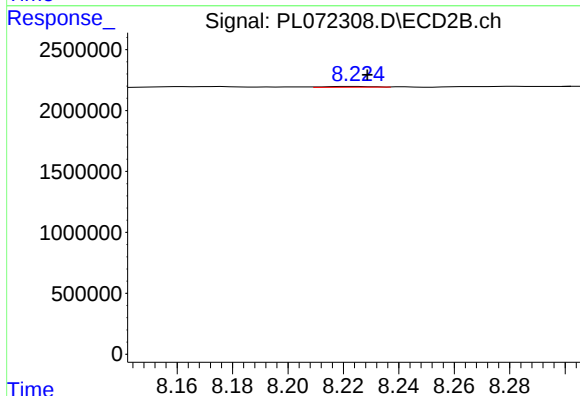


#10 gamma-Chlordane

R.T.: 8.225 min
Delta R.T.: -0.004 min
Response: 68350
Conc: 0.03 ng/ml

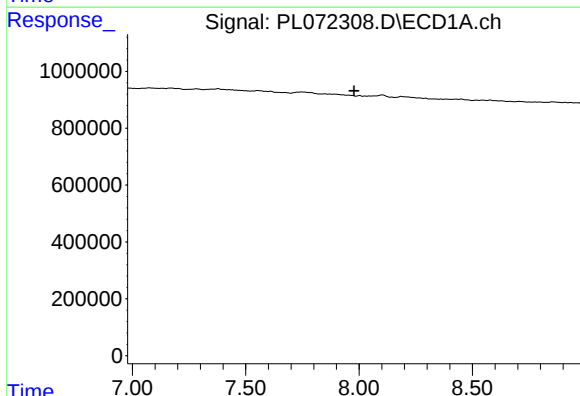


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.978 min
Response: 0
Conc: N.D.

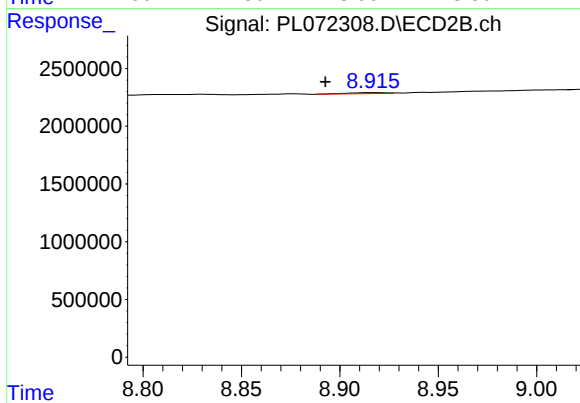

#14 Endrin


R.T.: 8.917 min
Delta R.T.: 0.025 min
Response: 135908
Conc: 0.08 ng/ml

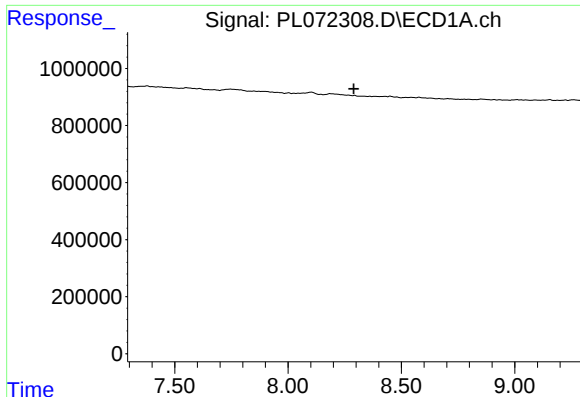

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

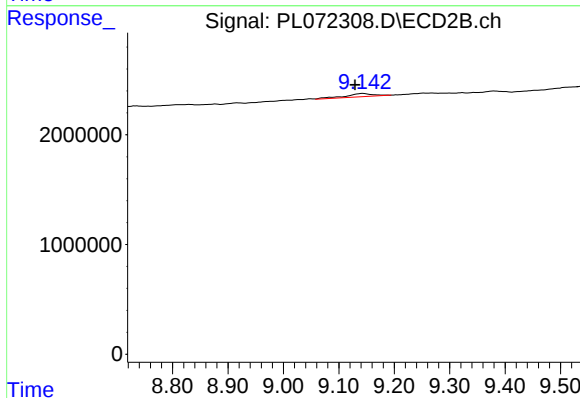


#15 Endosulfan II

R.T.: 9.144 min
Delta R.T.: 0.015 min
Response: 1026516
Conc: 0.60 ng/ml

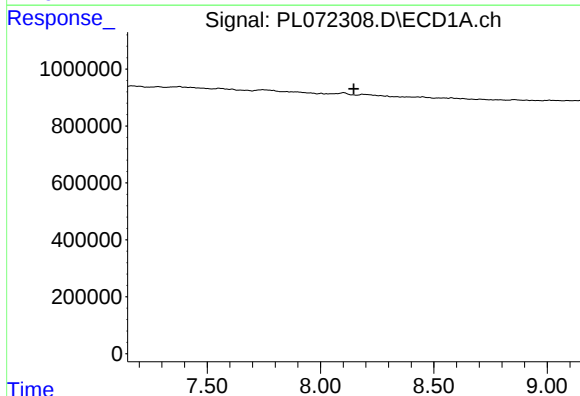


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

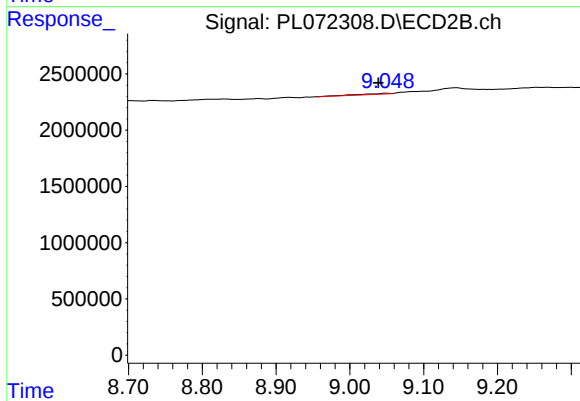

#16 4,4'-DDD


R.T.: 9.050 min
Delta R.T.: 0.011 min
Response: 225167
Conc: 0.16 ng/ml

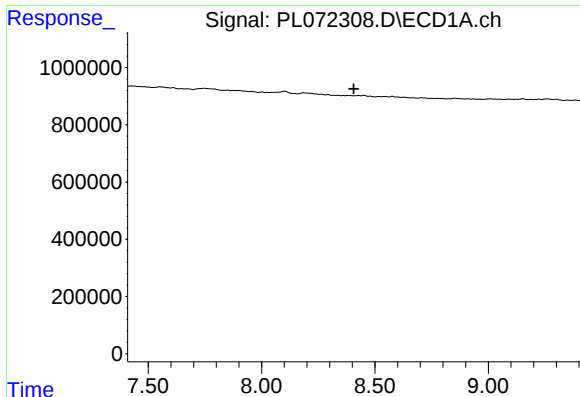

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

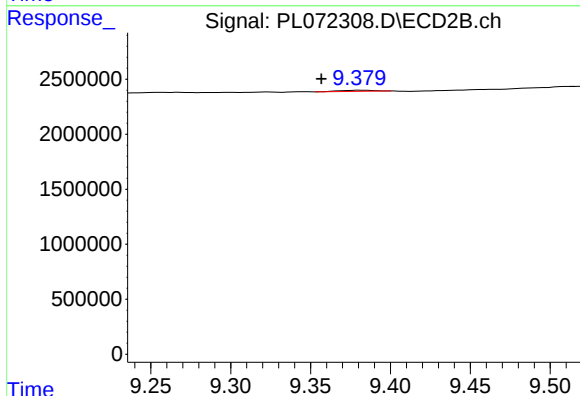


#17 4,4'-DDT

R.T.: 9.381 min
Delta R.T.: 0.024 min
Response: 153154
Conc: 0.10 ng/ml

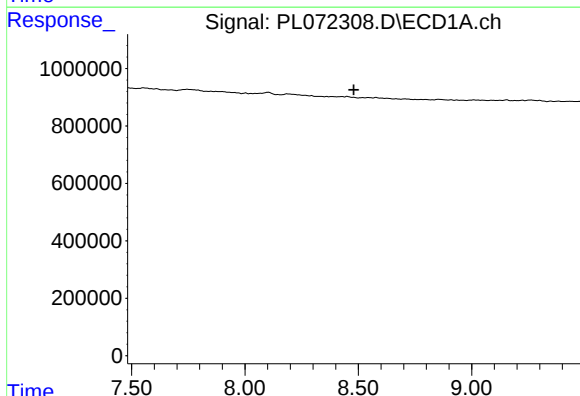


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

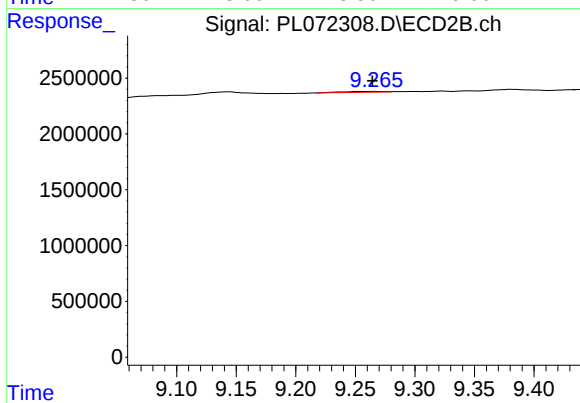

#18 Endrin aldehyde


R.T.: 9.268 min
Delta R.T.: 0.003 min
Response: 194742
Conc: 0.16 ng/ml

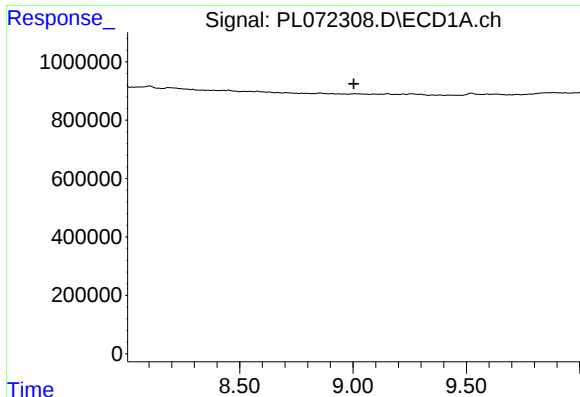

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

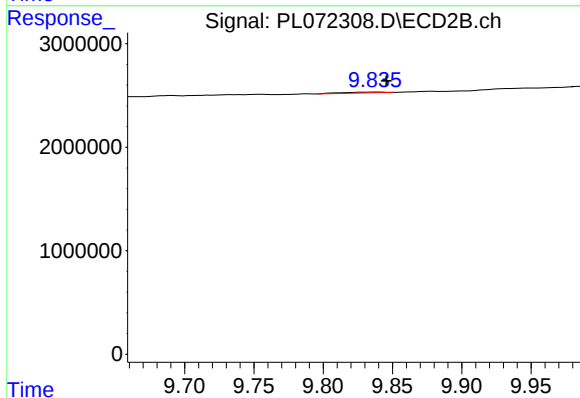


#20 Methoxychlor

R.T.: 9.839 min
Delta R.T.: -0.007 min
Response: 191912
Conc: 0.23 ng/ml

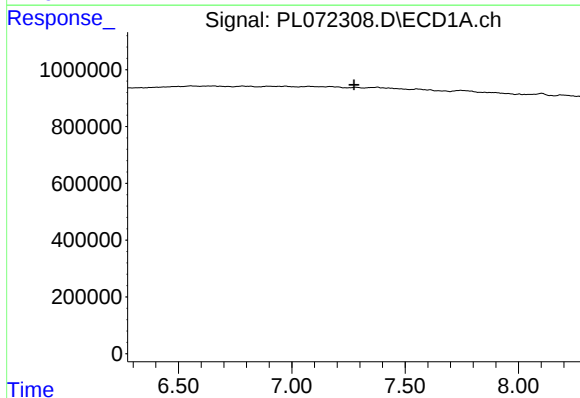


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

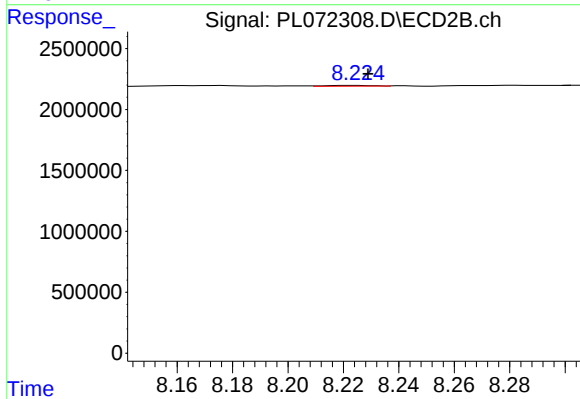

#25 Chlordane-3


R.T.: 8.225 min
Delta R.T.: -0.004 min
Response: 68350
Conc: 0.25 ng/ml

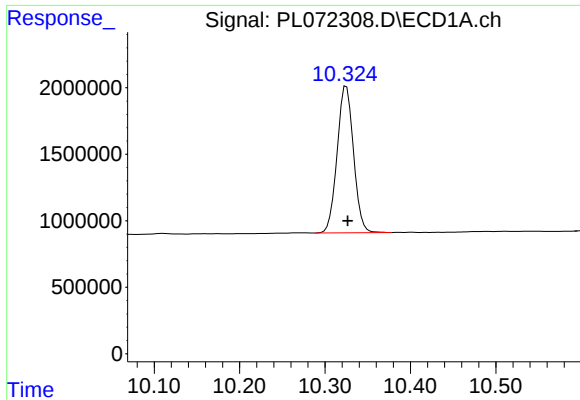

#28 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: -0.001 min
Response: 14713541
Conc: 16.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

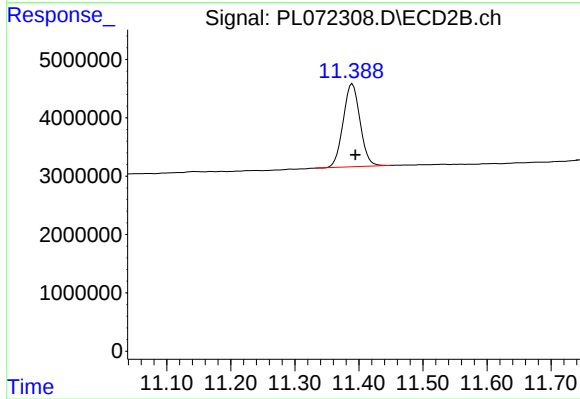

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: -0.005 min
Response: 26092631
Conc: 16.17 ng/ml