

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 13:25
 Operator : AR\AJ
 Sample : N1298-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:26:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.491	6118818	18348786	11.021	11.298
28)	SA Decachlor...	10.318	11.386	10057064	17449177	11.320	10.814
Target Compounds							
2)	A alpha-BHC	0.000	6.105f	0	224778	N.D.	0.093 #
6)	B beta-BHC	6.044f	0.000	596008	0	1.803	N.D. #
7)	B delta-BHC	0.000	7.017f	0	790417	N.D.	0.321 #
9)	A Endosulfan I	0.000	8.371	0	73983	N.D.	0.041 #
10)	B gamma-Chl...	0.000	8.218	0	76491	N.D.	0.038 #
11)	B alpha-Chl...	0.000	8.308	0	559498	N.D.	0.282 #
13)	MA Dieldrin	0.000	8.656	0	85445	N.D.	0.043 #
15)	B Endosulfa...	0.000	9.147f	0	462947	N.D.	0.270 #
17)	MA 4,4'-DDT	0.000	9.354	0	28840	N.D.	0.018 #
18)	B Endrin al...	0.000	9.281f	0	33992	N.D.	0.027 #
25)	Chlordane-3	0.000	8.218	0	76491	N.D.	0.275 #
26)	Chlordane-4	0.000	8.308	0	559498	N.D.	1.685 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 13:25
Operator : AR\AJ
Sample : N1298-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:26:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

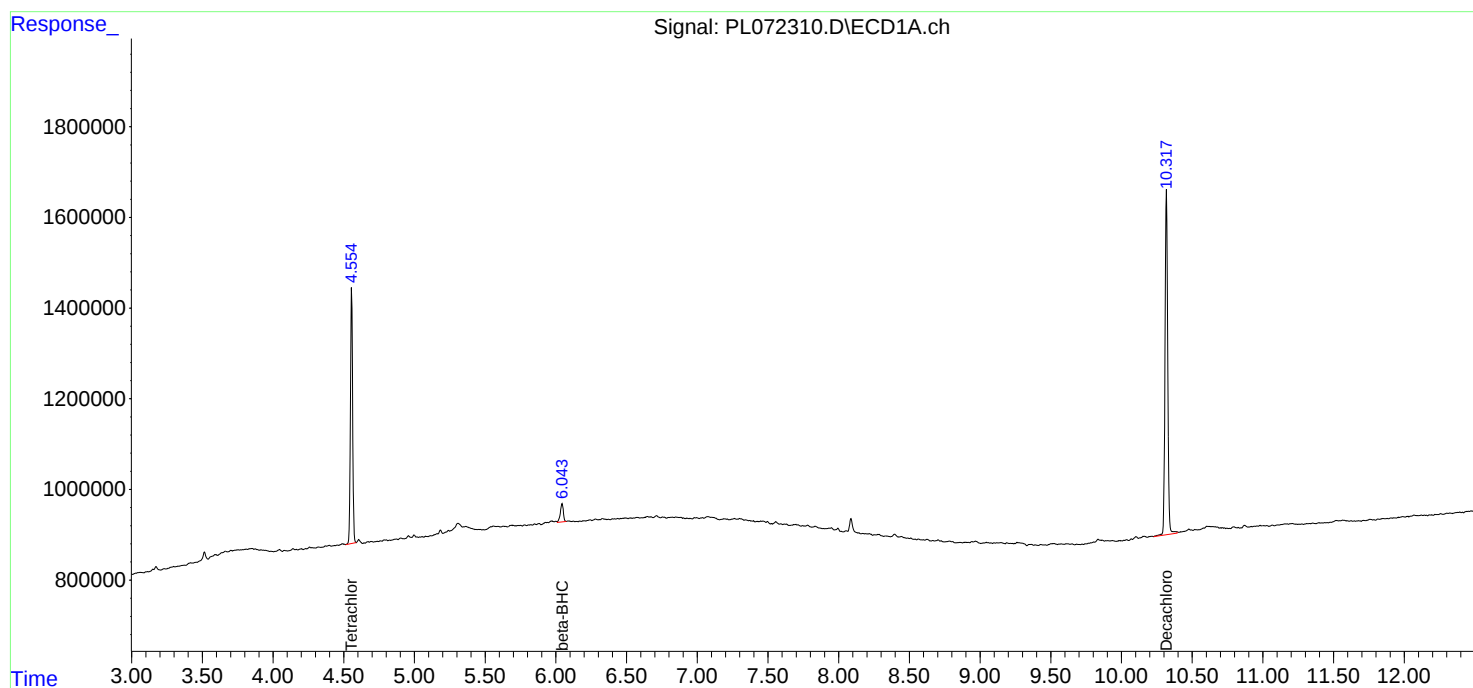


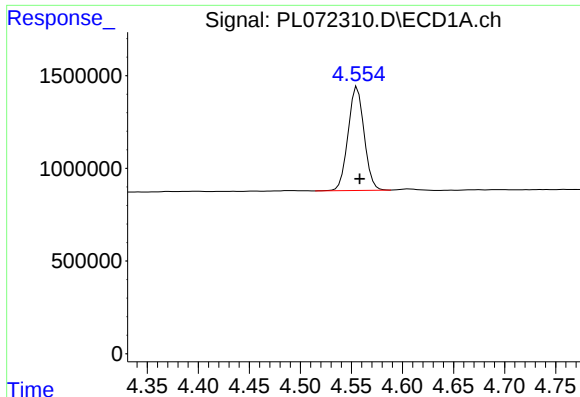

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 6118818
Conc: 11.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

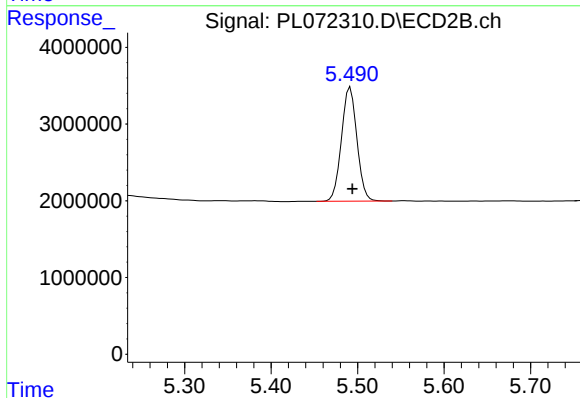


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 18348786
Conc: 11.30 ng/ml

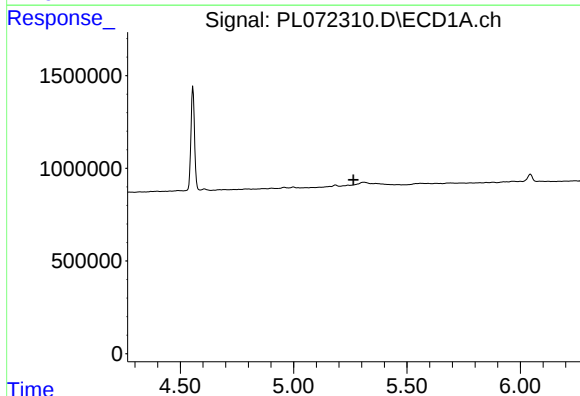


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

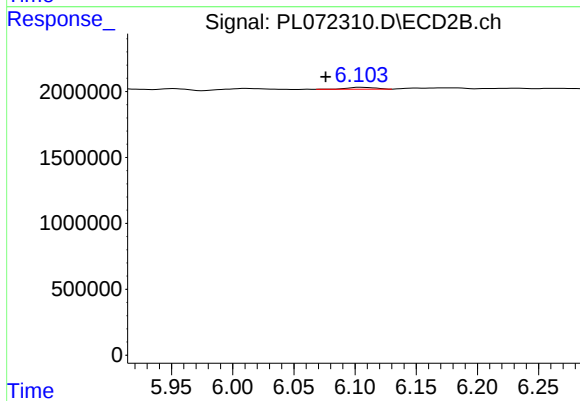

#2 alpha-BHC


R.T.: 6.105 min
Delta R.T.: 0.029 min
Response: 224778
Conc: 0.09 ng/ml

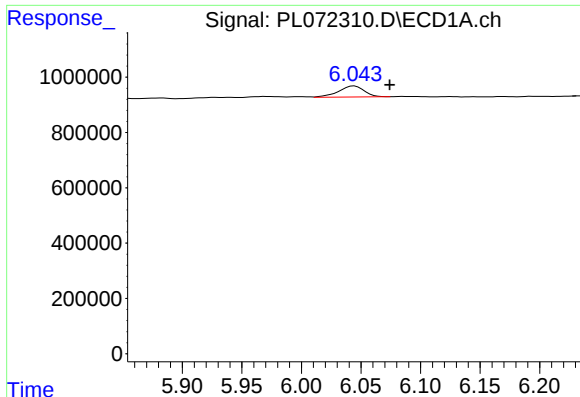

#6 beta-BHC


R.T.: 6.044 min
Delta R.T.: -0.030 min
Response: 596008
Conc: 1.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

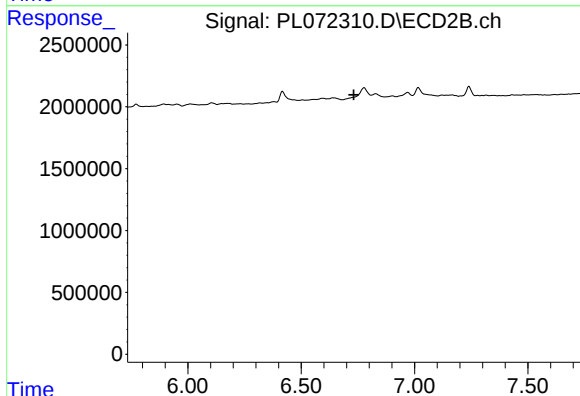


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.732 min
Response: 0
Conc: N.D.

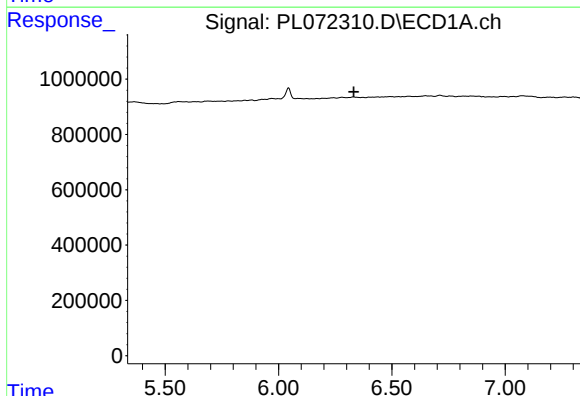


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

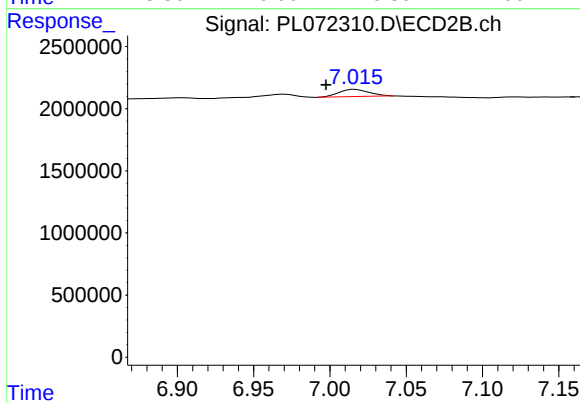

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 790417
Conc: 0.32 ng/ml

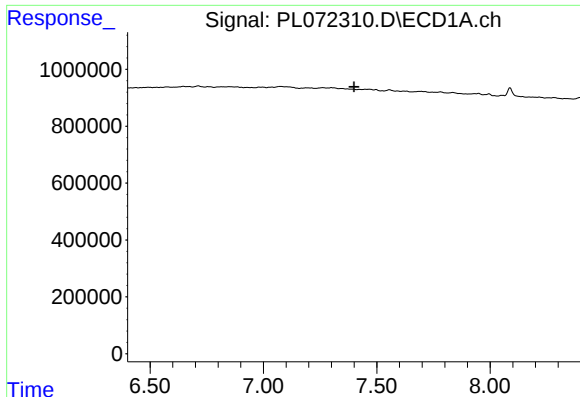

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

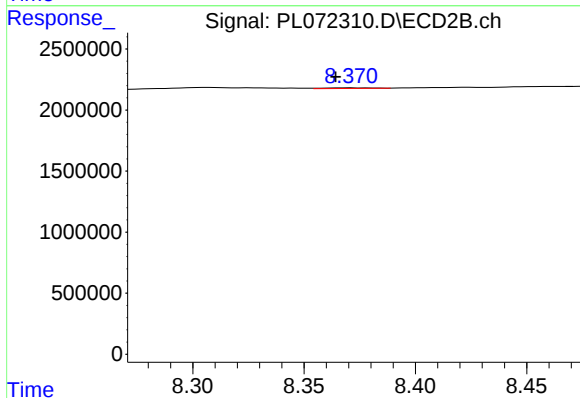


#9 Endosulfan I

R.T.: 8.371 min
Delta R.T.: 0.007 min
Response: 73983
Conc: 0.04 ng/ml

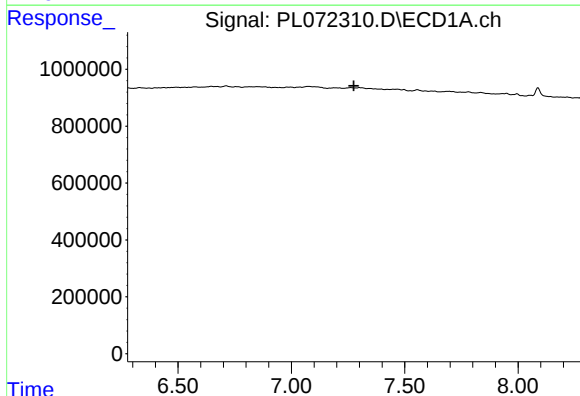


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

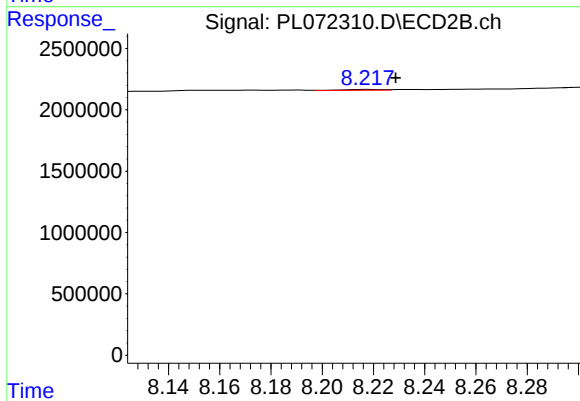

#10 gamma-Chlordane


R.T.: 8.218 min
Delta R.T.: -0.011 min
Response: 76491
Conc: 0.04 ng/ml

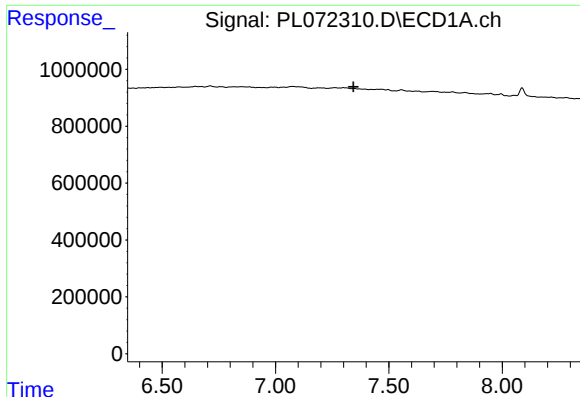

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

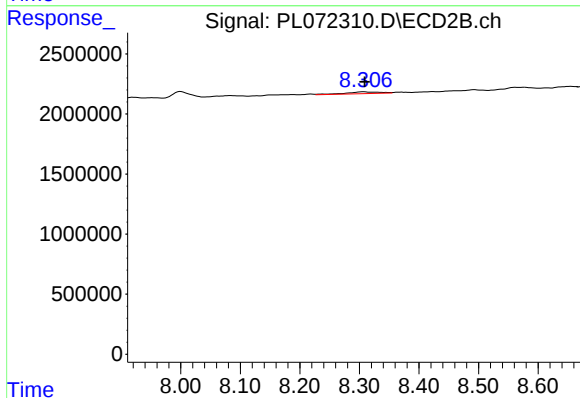


#11 alpha-Chlordane

R.T.: 8.308 min
Delta R.T.: -0.001 min
Response: 559498
Conc: 0.28 ng/ml

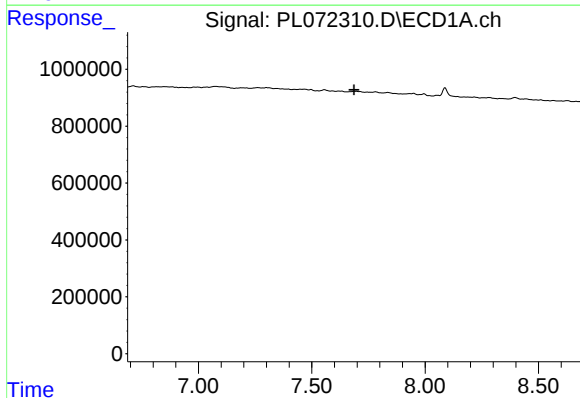


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

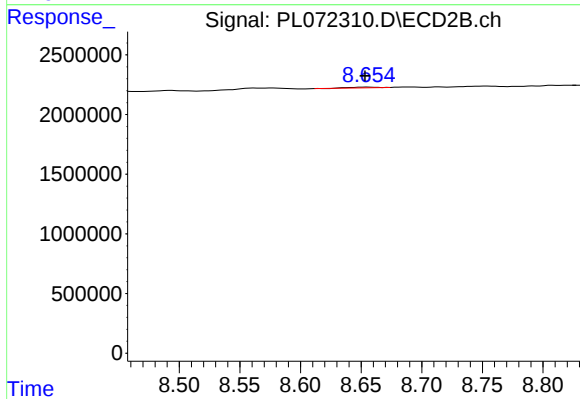

#13 Dieldrin


R.T.: 8.656 min
Delta R.T.: 0.002 min
Response: 85445
Conc: 0.04 ng/ml

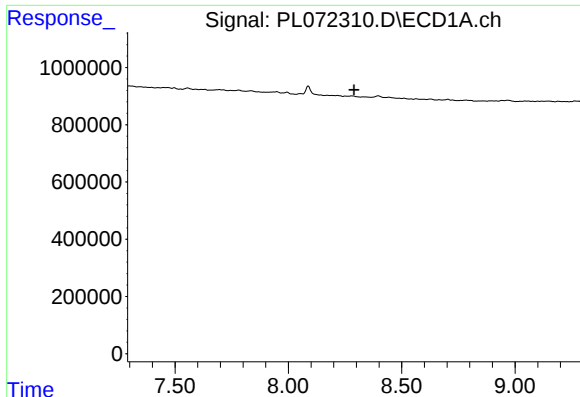

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

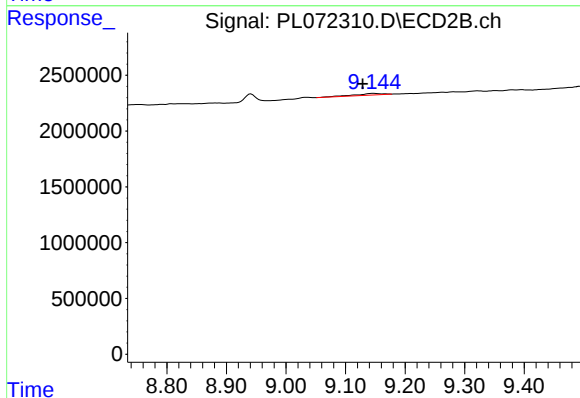


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.018 min
Response: 462947
Conc: 0.27 ng/ml

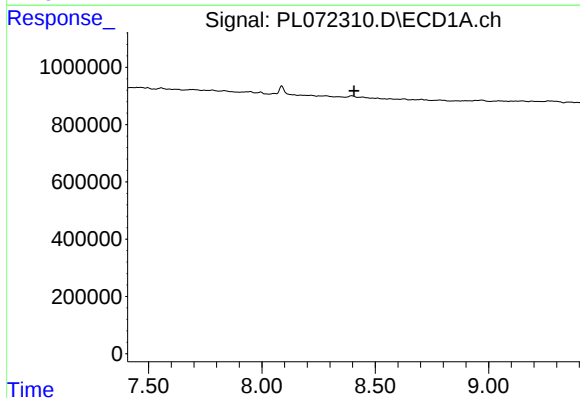


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

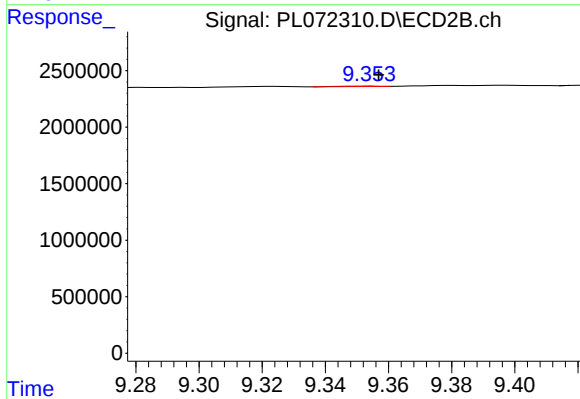

#17 4,4'-DDT


R.T.: 9.354 min
Delta R.T.: -0.003 min
Response: 28840
Conc: 0.02 ng/ml

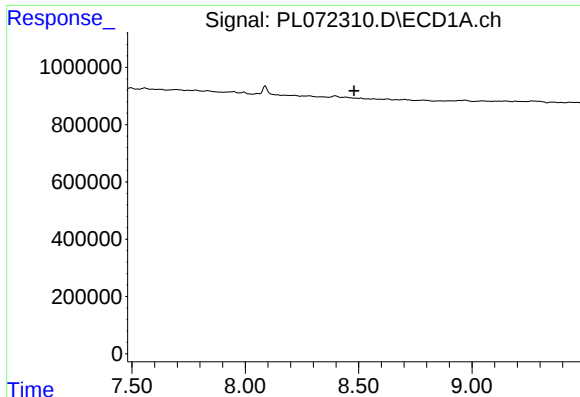

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

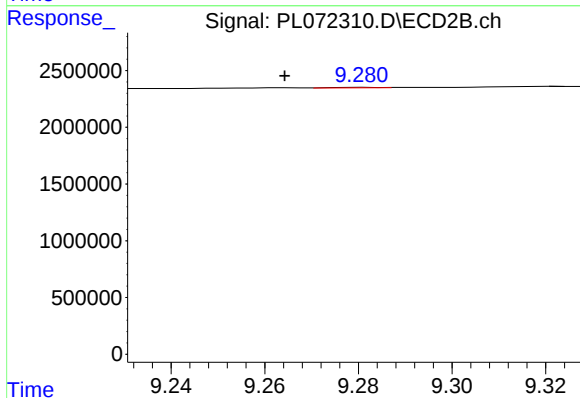


#18 Endrin aldehyde

R.T.: 9.281 min
Delta R.T.: 0.017 min
Response: 33992
Conc: 0.03 ng/ml

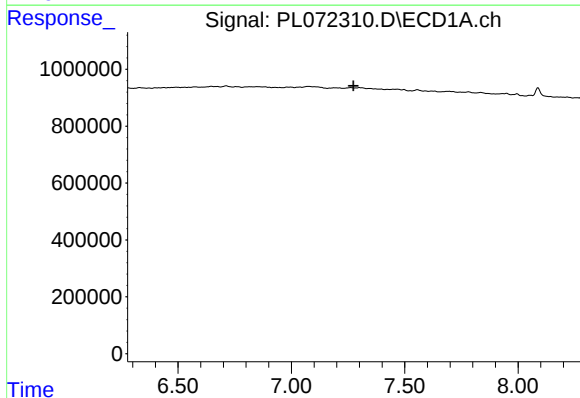


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

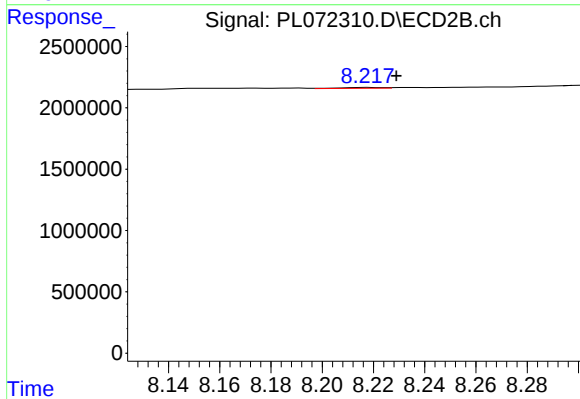

#25 Chlordane-3


R.T.: 8.218 min
Delta R.T.: -0.011 min
Response: 76491
Conc: 0.28 ng/ml

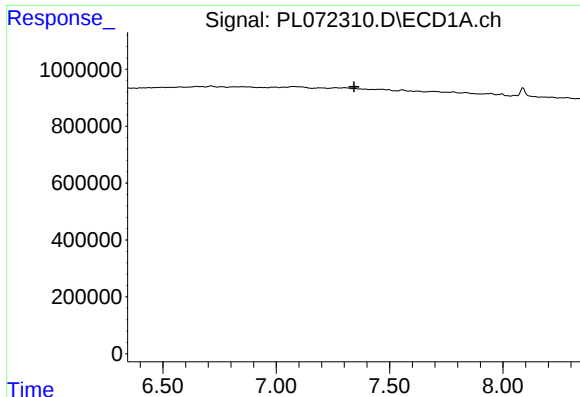

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

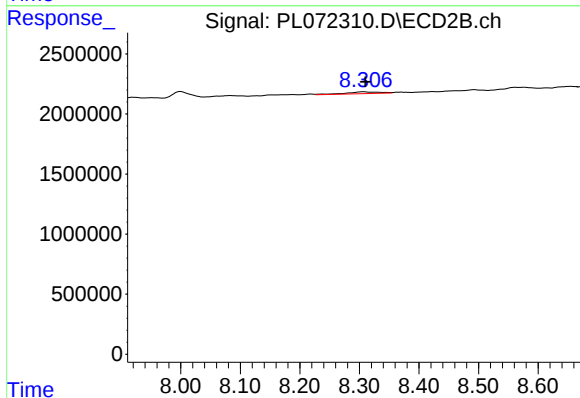


#26 Chlordane-4

R.T.: 8.308 min
Delta R.T.: -0.003 min
Response: 559498
Conc: 1.68 ng/ml

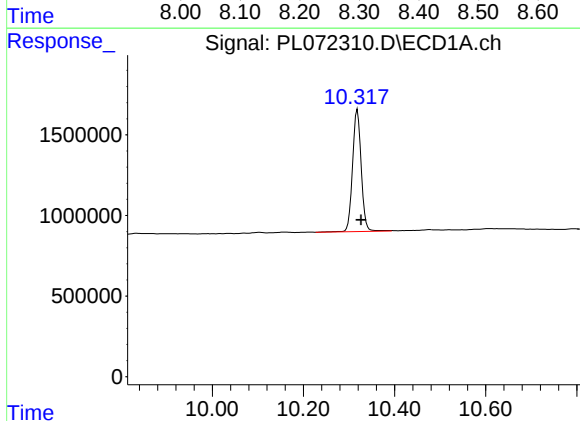

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 10057064
Conc: 11.32 ng/ml

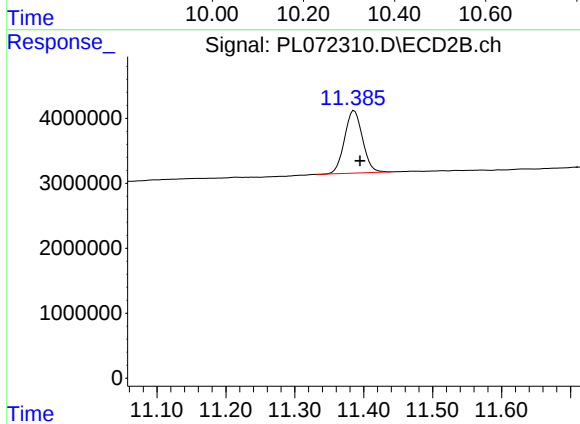

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.008 min
Response: 17449177
Conc: 10.81 ng/ml