

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 14:01
 Operator : AR\AJ
 Sample : N1309-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:26:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.493	6077032	18051323	10.946	11.115
28)	SA Decachlor...	10.319	11.387	10191839	16931567	11.472	10.494
Target Compounds							
2)	A alpha-BHC	5.279	0.000	149991	0	0.194	N.D. #
7)	B delta-BHC	0.000	7.017f	0	681511	N.D.	0.277 #
10)	B gamma-Chl...	0.000	8.227	0	283129	N.D.	0.140 #
13)	MA Dieldrin	0.000	8.654	0	58998	N.D.	0.030 #
15)	B Endosulfa...	0.000	9.145f	0	931555	N.D.	0.543 #
16)	A 4,4'-DDD	0.000	9.039	0	168634	N.D.	0.118 #
25)	Chlordane-3	0.000	8.227	0	283129	N.D.	1.019 #
27)	Chlordane-5	0.000	9.189	0	84972	N.D.	1.393 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 14:01
Operator : AR\AJ
Sample : N1309-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:26:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

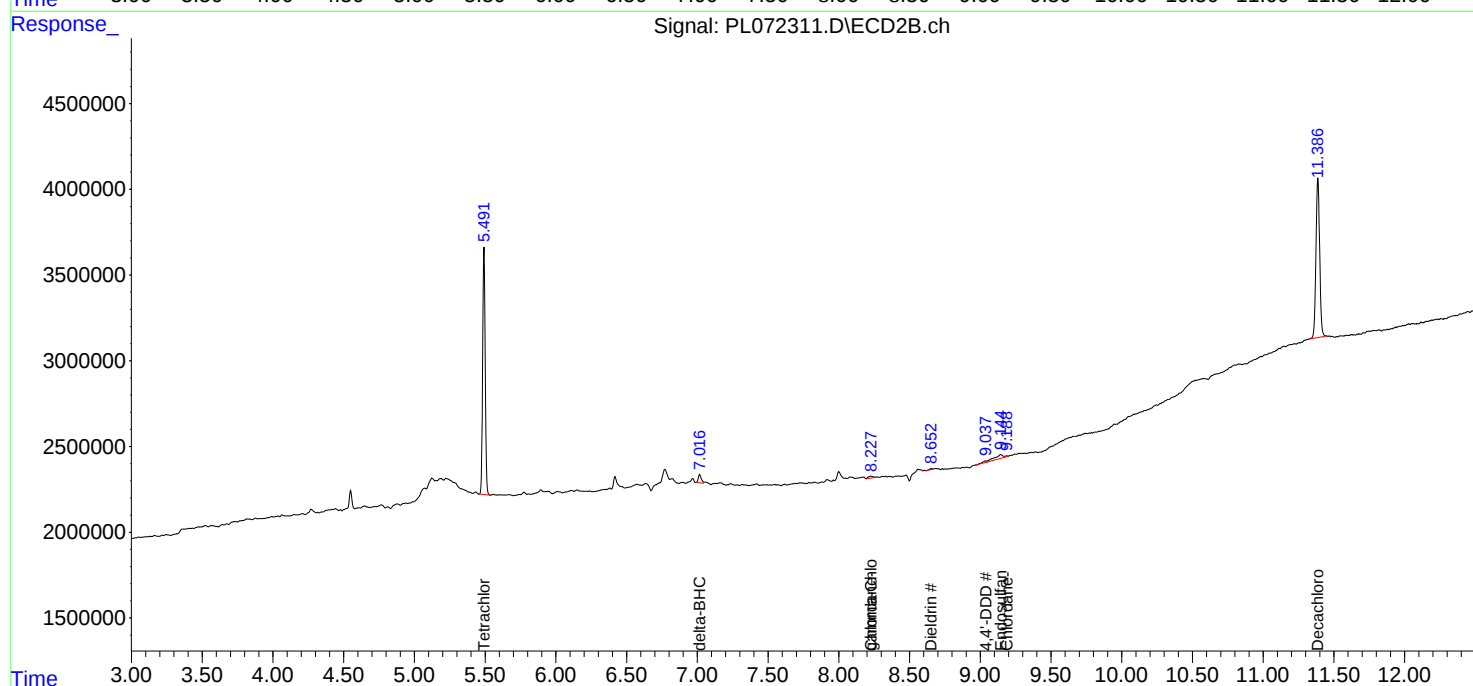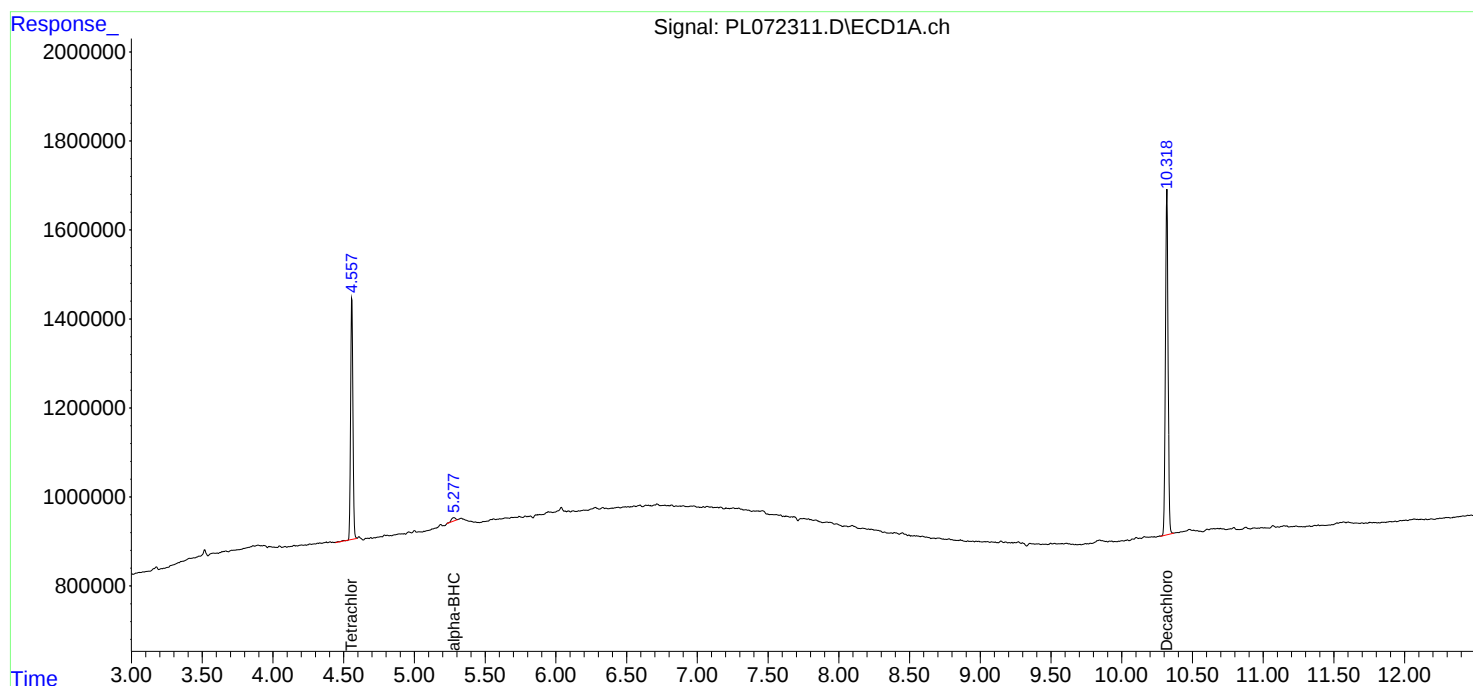


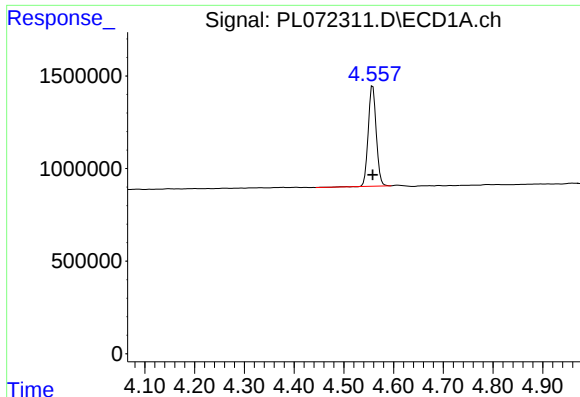

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.000 min
Response: 6077032
Conc: 10.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

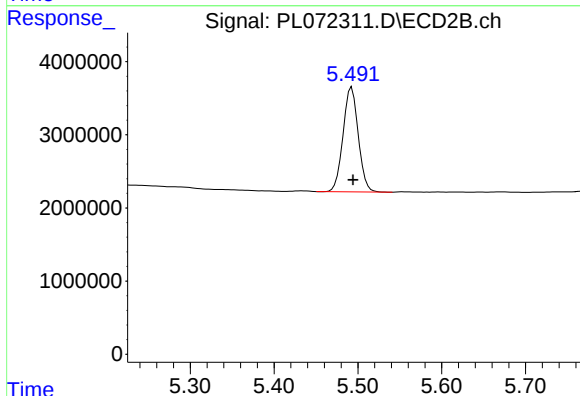


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: -0.001 min
Response: 18051323
Conc: 11.11 ng/ml

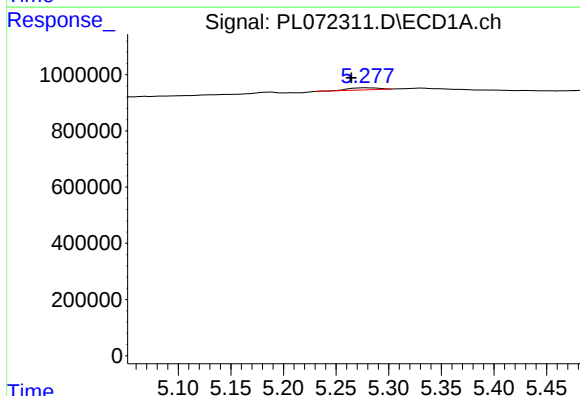


#2 alpha-BHC

R.T.: 5.279 min
Delta R.T.: 0.014 min
Response: 149991
Conc: 0.19 ng/ml

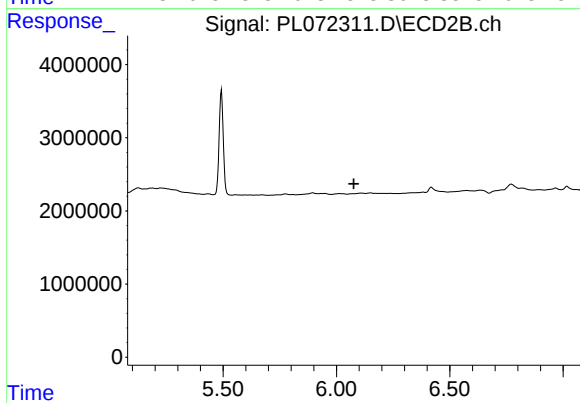

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

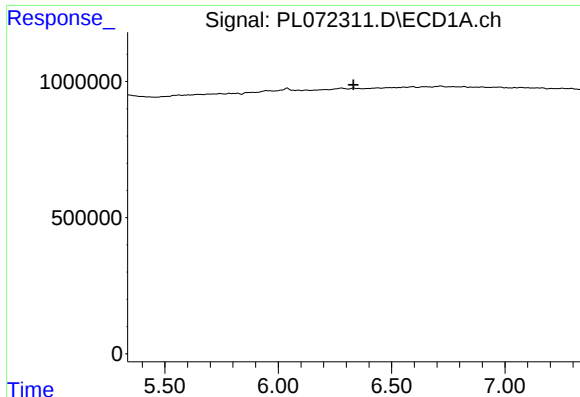

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

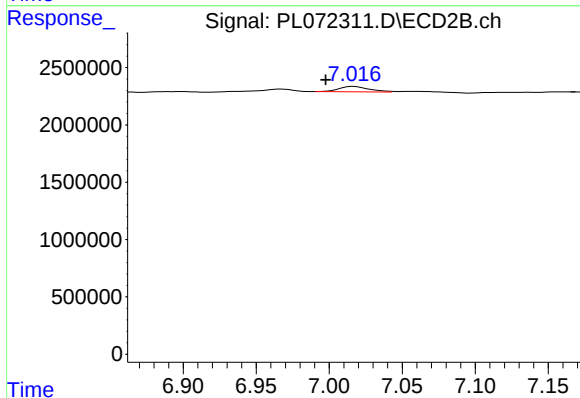


#7 delta-BHC

R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 681511
Conc: 0.28 ng/ml

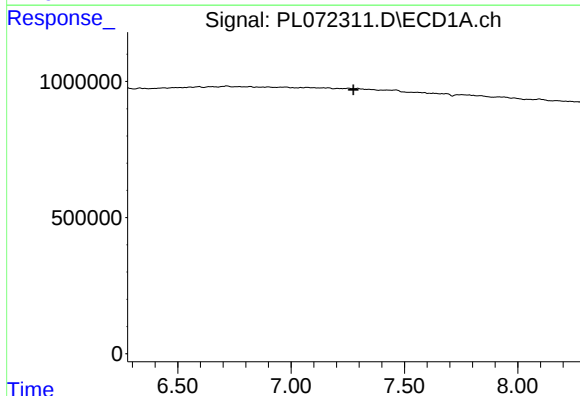


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

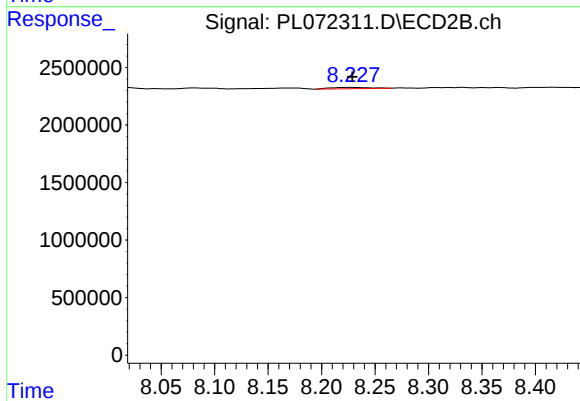

#10 gamma-Chlordane


R.T.: 8.227 min
Delta R.T.: -0.001 min
Response: 283129
Conc: 0.14 ng/ml

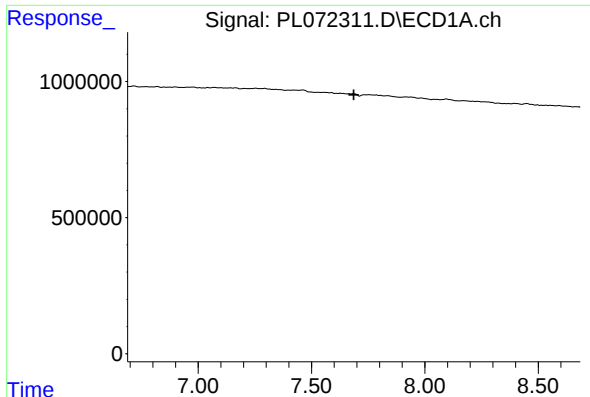

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

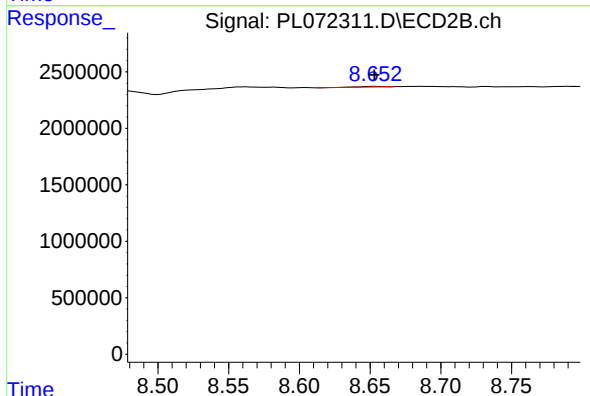


#13 Dieldrin

R.T.: 8.654 min
Delta R.T.: 0.001 min
Response: 58998
Conc: 0.03 ng/ml

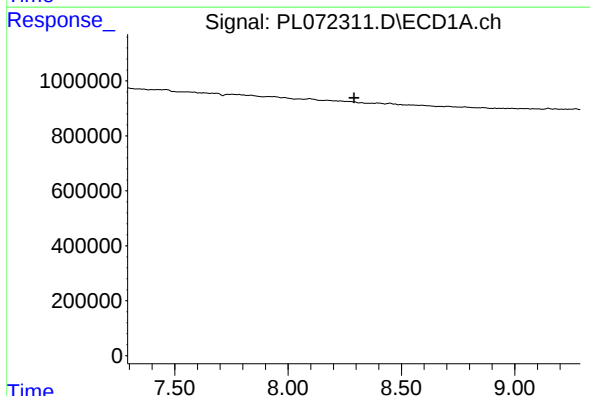


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

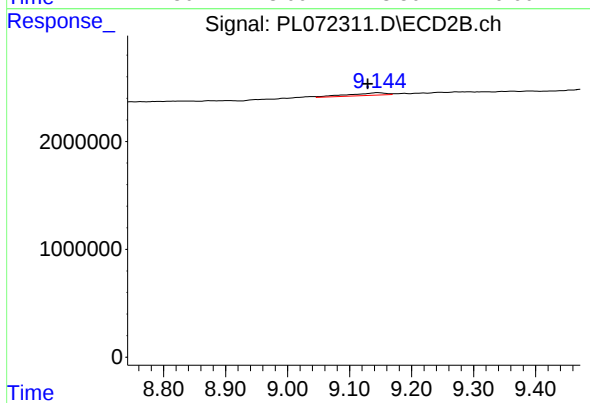

#15 Endosulfan II


R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 931555
Conc: 0.54 ng/ml

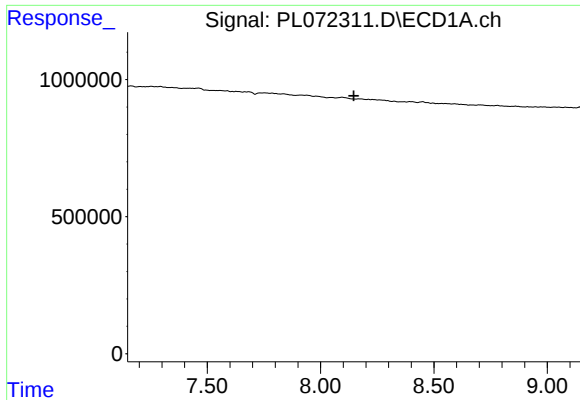

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

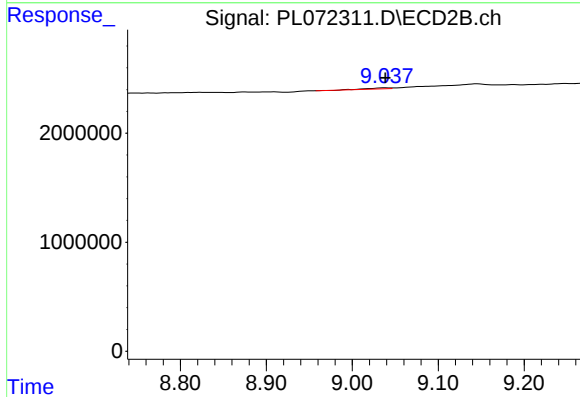


#16 4,4'-DDD

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 168634
Conc: 0.12 ng/ml

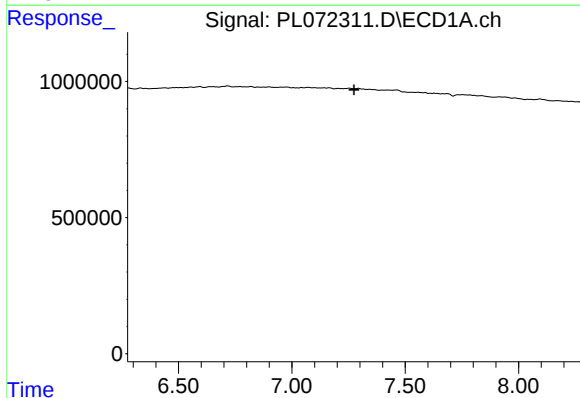


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

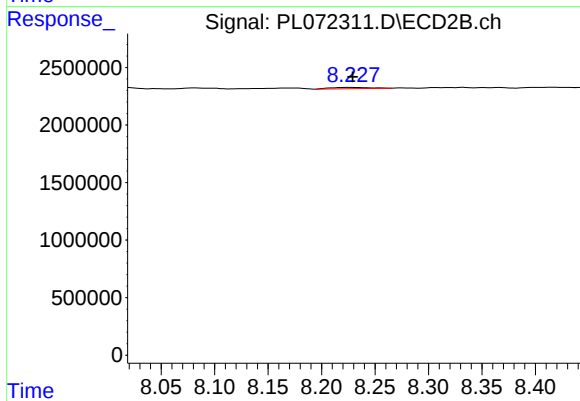

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: -0.002 min
Response: 283129
Conc: 1.02 ng/ml

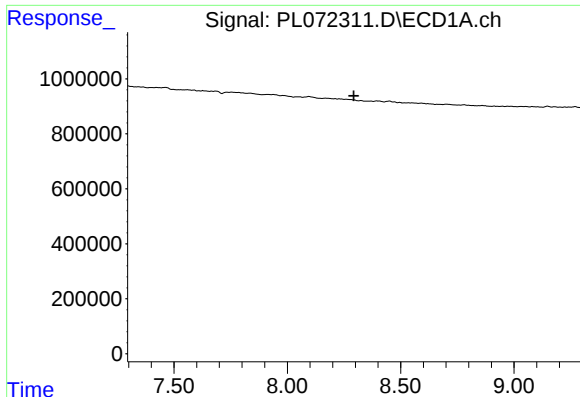

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

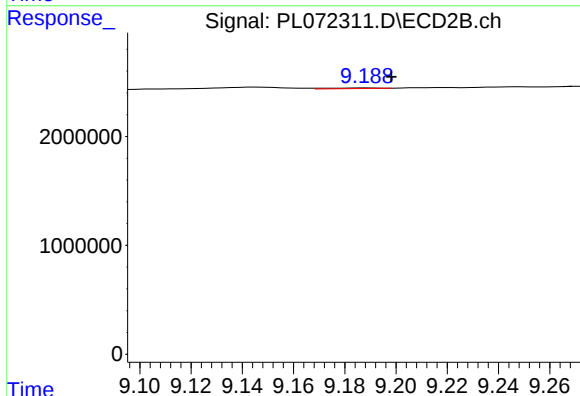


#27 Chlordane-5

R.T.: 9.189 min
Delta R.T.: -0.010 min
Response: 84972
Conc: 1.39 ng/ml

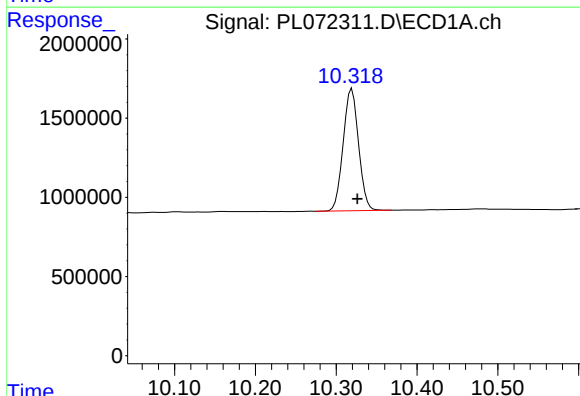

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.007 min
Response: 10191839
Conc: 11.47 ng/ml

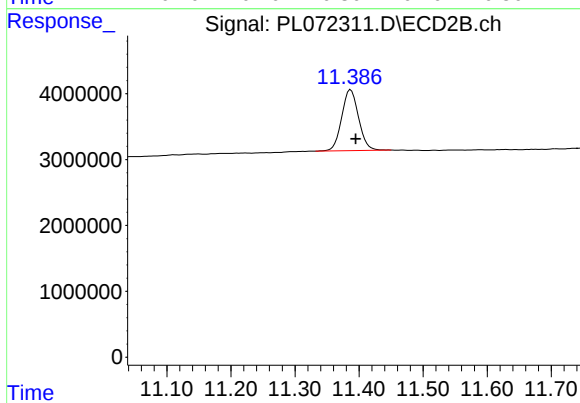

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 16931567
Conc: 10.49 ng/ml