

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 15:23
 Operator : AR\AJ
 Sample : N1319-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:28:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	10709576	32650732	19.290	20.104
28)	SA Decachlor...	10.318	11.385	14415866	25875535	16.226	16.037
Target Compounds							
2)	A alpha-BHC	0.000	6.101f	0	356514	N.D.	0.148 #
3)	MA gamma-BHC...	5.679	0.000	188851	0	0.250	N.D. #
7)	B delta-BHC	0.000	7.018f	0	914179	N.D.	0.372 #
10)	B gamma-Chl...	0.000	8.223	0	656174	N.D.	0.325 #
11)	B alpha-Chl...	0.000	8.307	0	270091	N.D.	0.136 #
13)	MA Dieldrin	0.000	8.657	0	125683	N.D.	0.064 #
15)	B Endosulfa...	0.000	9.144	0	269822	N.D.	0.157 #
17)	MA 4,4'-DDT	0.000	9.351	0	64263	N.D.	0.041 #
18)	B Endrin al...	0.000	9.282f	0	213887	N.D.	0.172 #
25)	Chlordane-3	0.000	8.223	0	656174	N.D.	2.362 #
26)	Chlordane-4	0.000	8.307	0	270091	N.D.	0.813 #
27)	Chlordane-5	0.000	9.194	0	114335	N.D.	1.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 15:23
Operator : AR\AJ
Sample : N1319-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:28:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

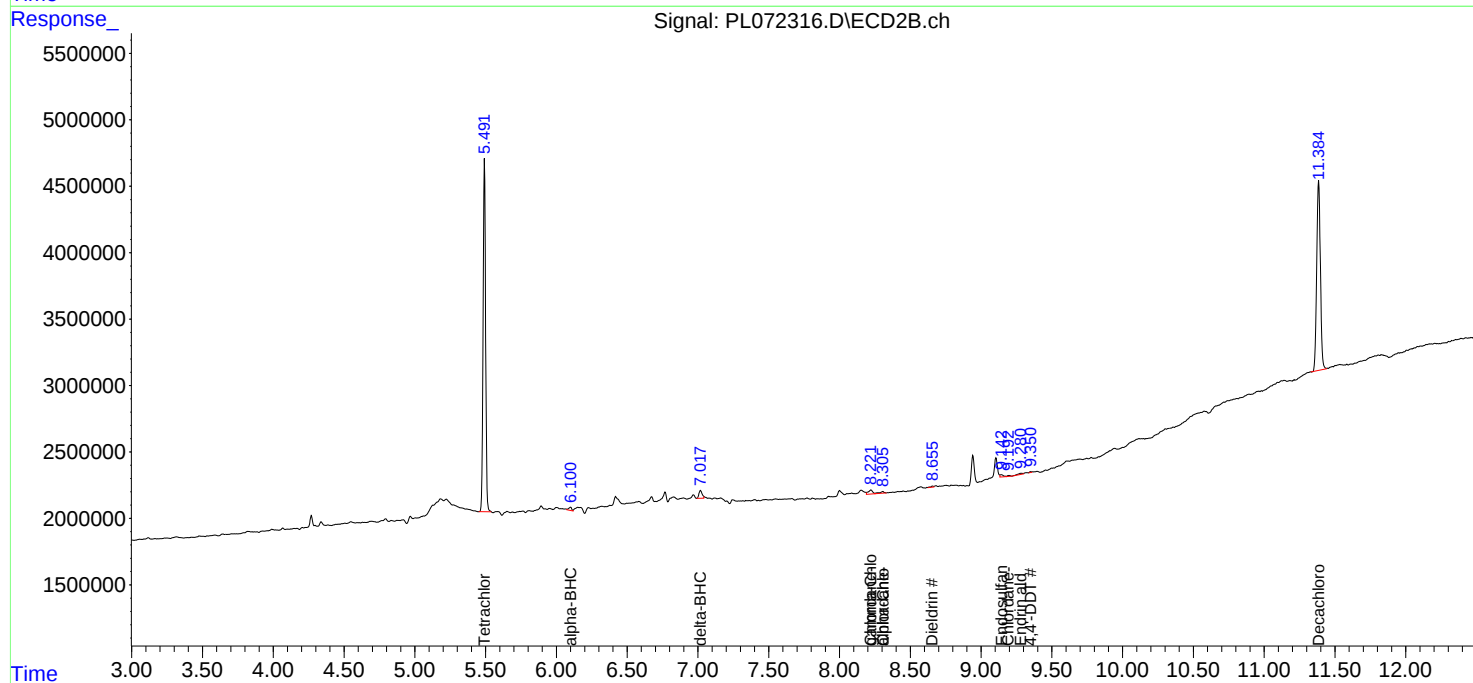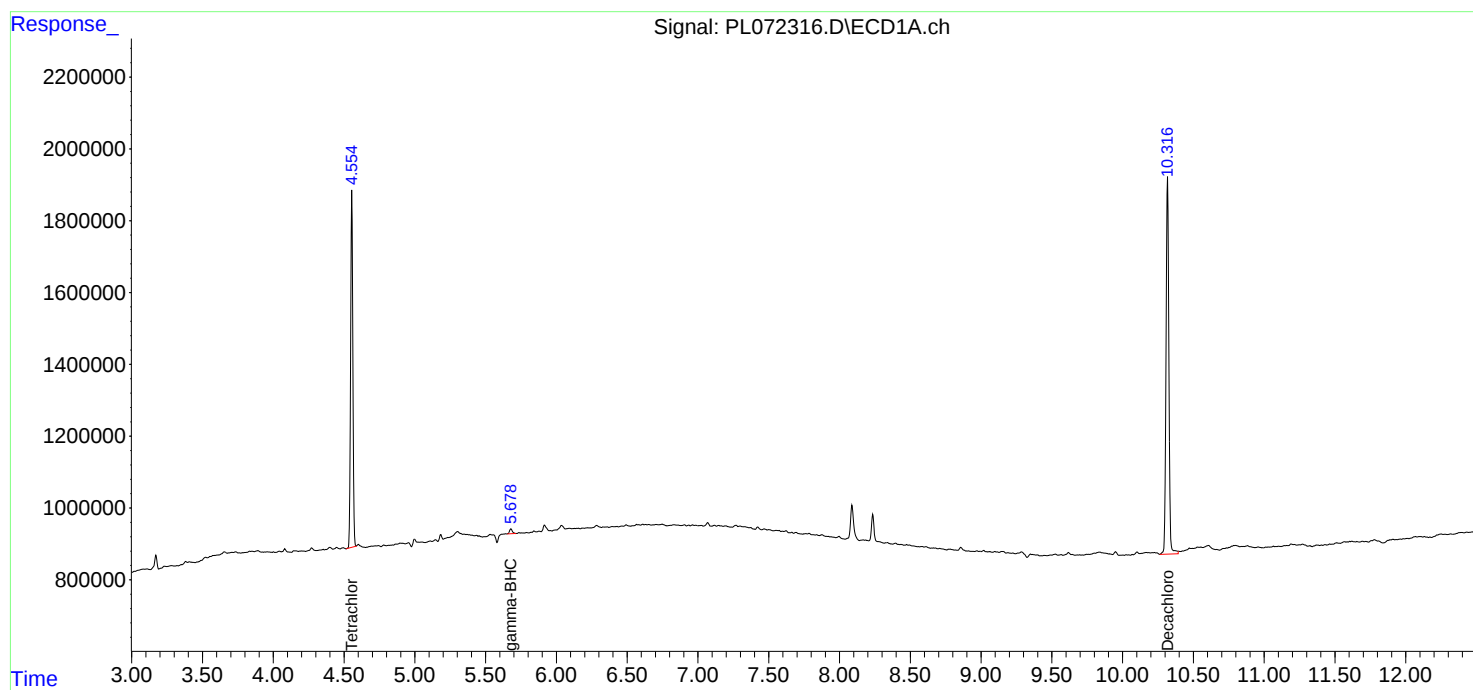


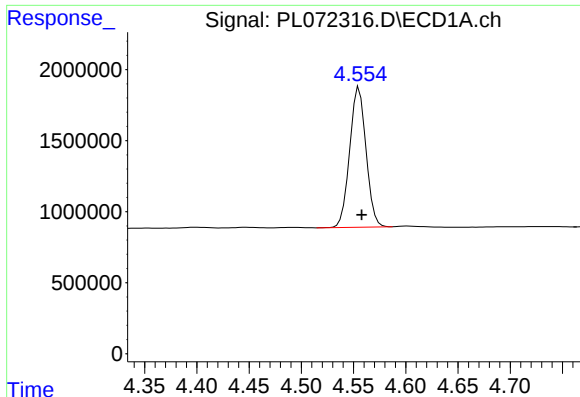

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 10709576
Conc: 19.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

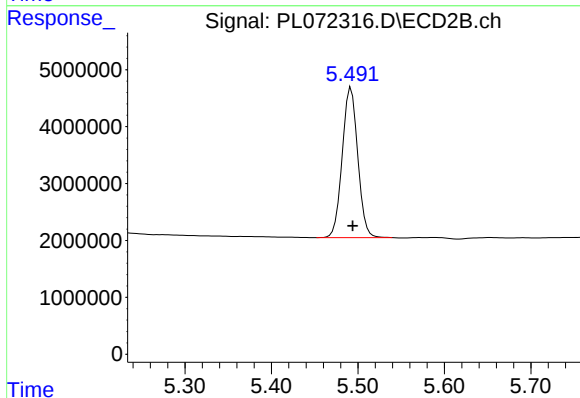


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 32650732
Conc: 20.10 ng/ml

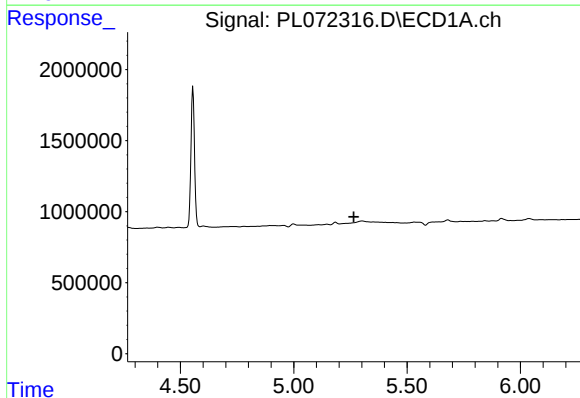


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

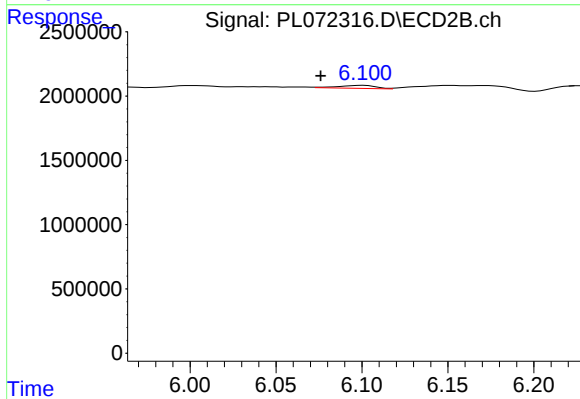

#2 alpha-BHC


R.T.: 6.101 min
Delta R.T.: 0.025 min
Response: 356514
Conc: 0.15 ng/ml

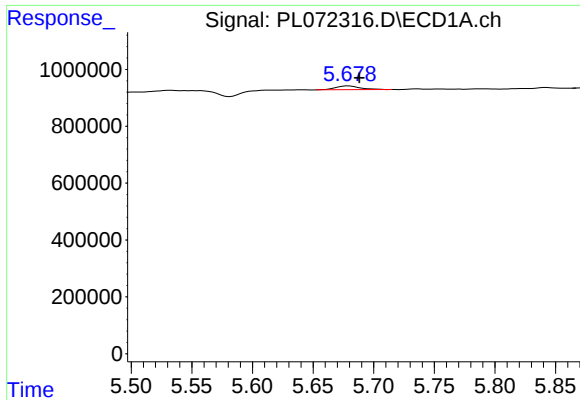

#3 gamma-BHC (Lindane)


R.T.: 5.679 min
Delta R.T.: -0.009 min
Response: 188851
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

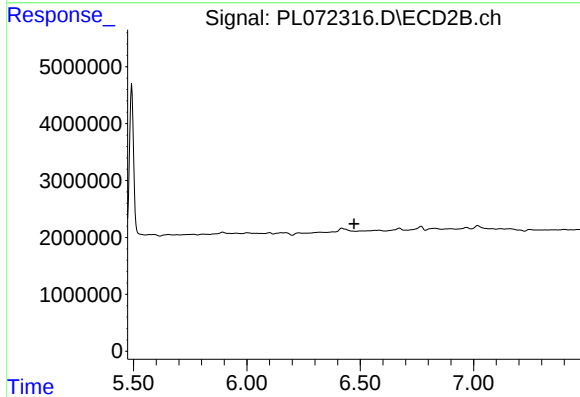


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.473 min
Response: 0
Conc: N.D.

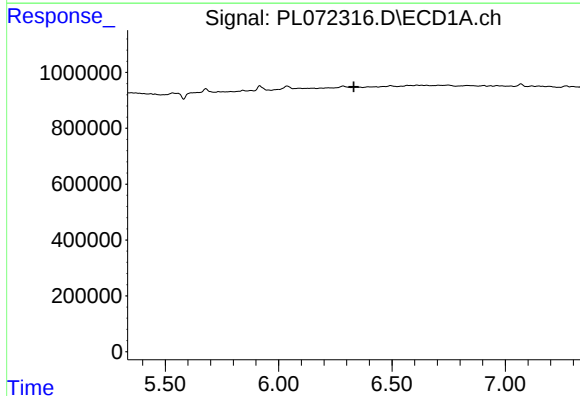


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

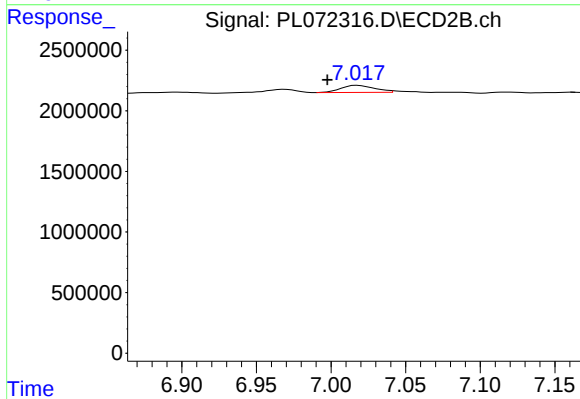

#7 delta-BHC


R.T.: 7.018 min
Delta R.T.: 0.020 min
Response: 914179
Conc: 0.37 ng/ml

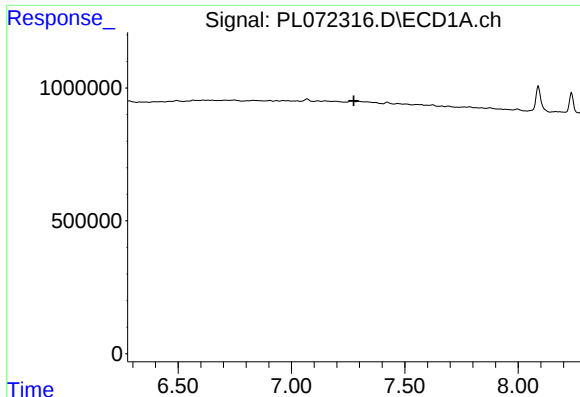

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

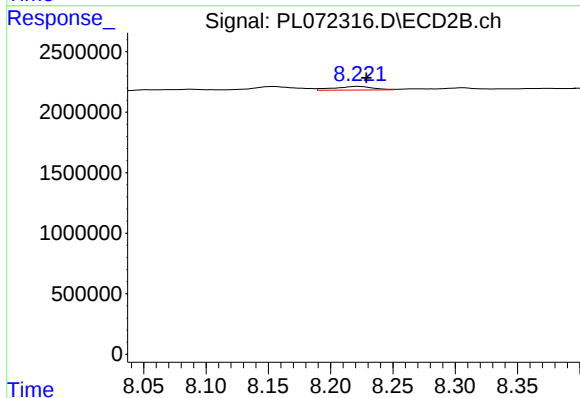


#10 gamma-Chlordane

R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 656174
Conc: 0.32 ng/ml

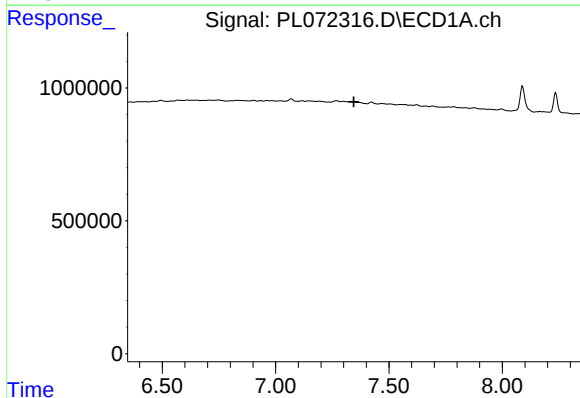


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

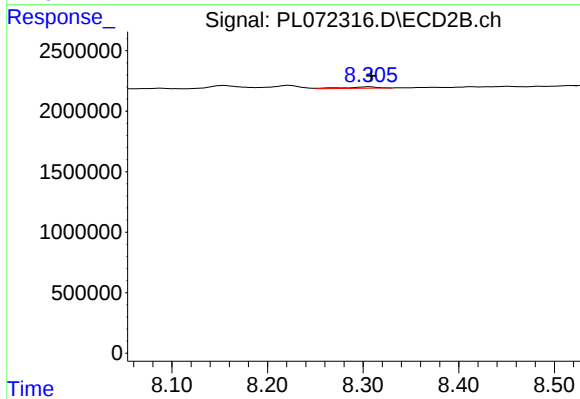

#11 alpha-Chlordane


R.T.: 8.307 min
Delta R.T.: -0.002 min
Response: 270091
Conc: 0.14 ng/ml

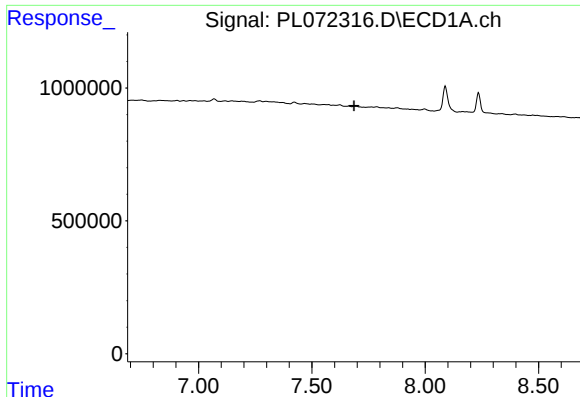

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

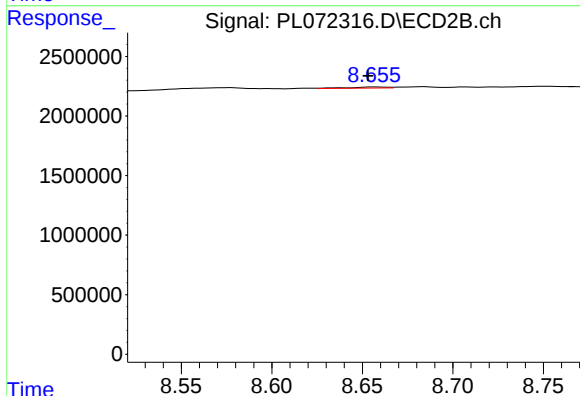


#13 Dieldrin

R.T.: 8.657 min
Delta R.T.: 0.003 min
Response: 125683
Conc: 0.06 ng/ml

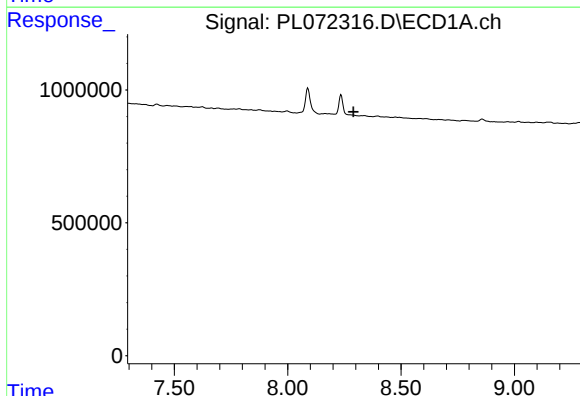


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

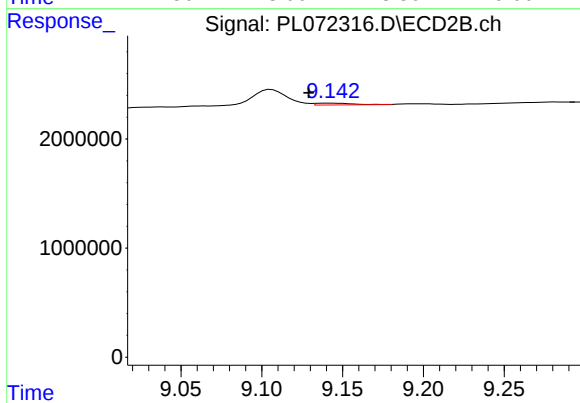

#15 Endosulfan II


R.T.: 9.144 min
Delta R.T.: 0.015 min
Response: 269822
Conc: 0.16 ng/ml

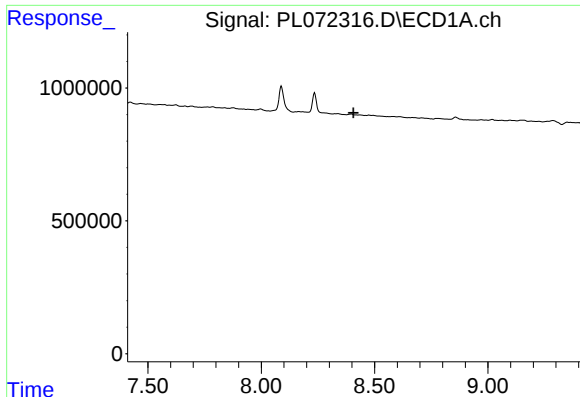

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

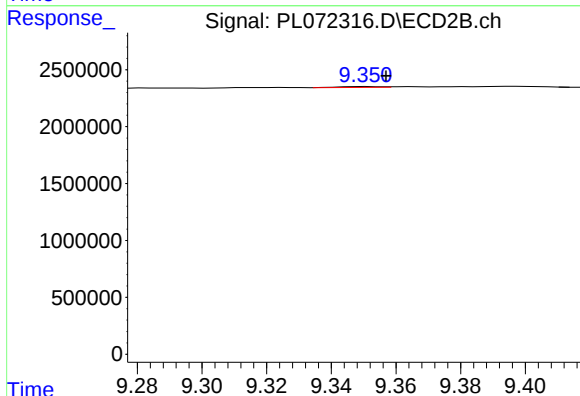


#17 4,4'-DDT

R.T.: 9.351 min
Delta R.T.: -0.006 min
Response: 64263
Conc: 0.04 ng/ml

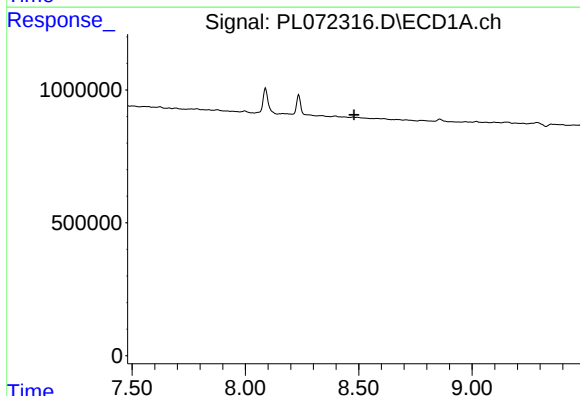


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

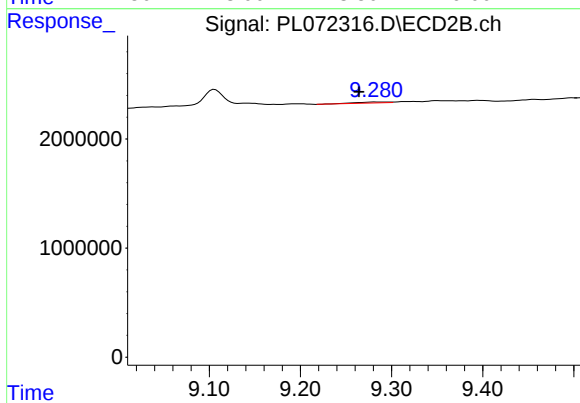

#18 Endrin aldehyde


R.T.: 9.282 min
Delta R.T.: 0.018 min
Response: 213887
Conc: 0.17 ng/ml

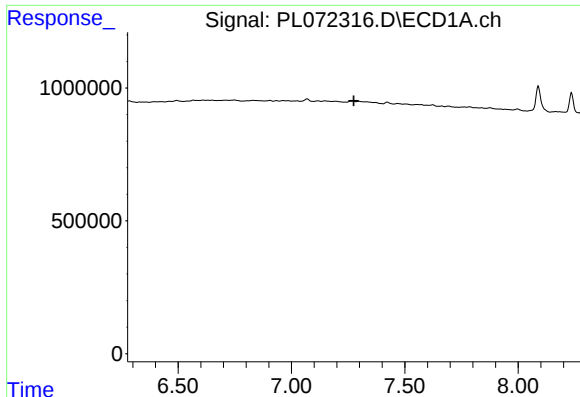

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

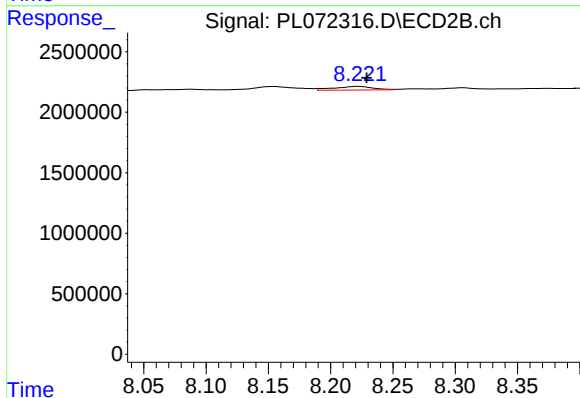


#25 Chlordane-3

R.T.: 8.223 min
Delta R.T.: -0.006 min
Response: 656174
Conc: 2.36 ng/ml

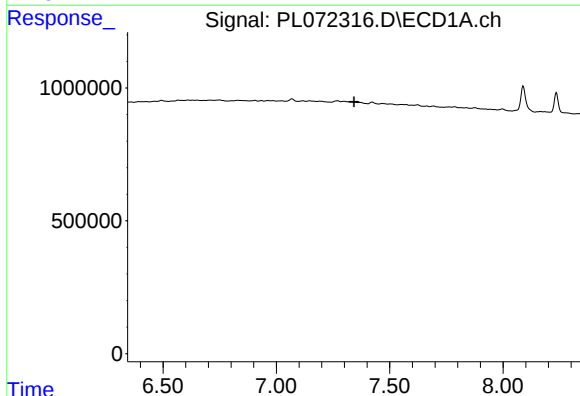


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

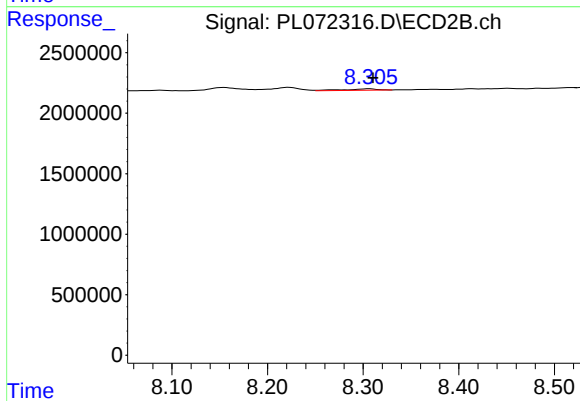

#26 Chlordane-4


R.T.: 8.307 min
Delta R.T.: -0.004 min
Response: 270091
Conc: 0.81 ng/ml

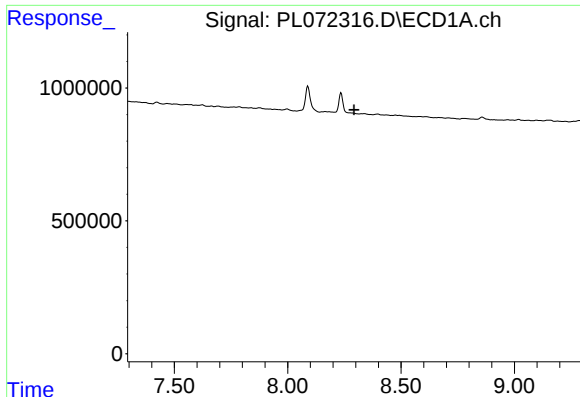

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

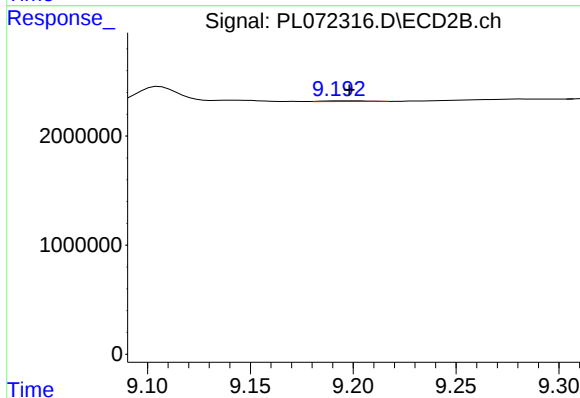


#27 Chlordane-5

R.T.: 9.194 min
Delta R.T.: -0.005 min
Response: 114335
Conc: 1.87 ng/ml

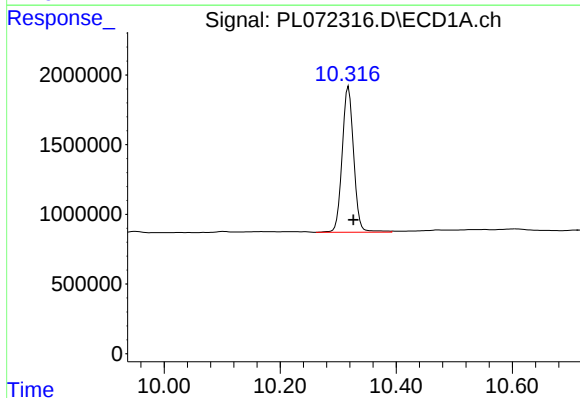

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 14415866
Conc: 16.23 ng/ml

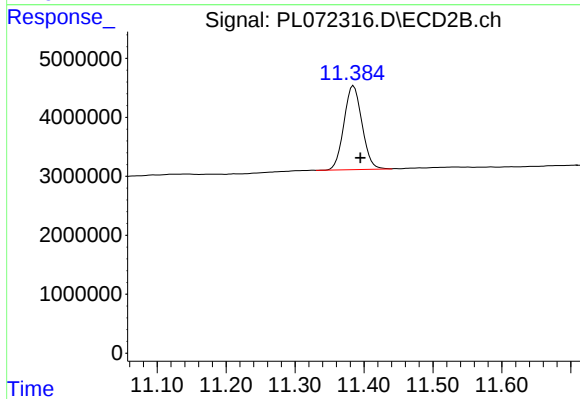

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 25875535
Conc: 16.04 ng/ml