

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 17:49
 Operator : AR\AJ
 Sample : PB142315TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:32:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	9557749	28671860	17.215	17.654
28)	SA Decachlor...	10.317	11.385	13787979	24491221	15.519	15.179
Target Compounds							
7)	B delta-BHC	0.000	7.015f	0	3533112	N.D.	1.436 #
10)	B gamma-Chl...	0.000	8.236	0	68556	N.D.	0.034 #
15)	B Endosulfa...	0.000	9.145f	0	1901808	N.D.	1.109 #
18)	B Endrin al...	0.000	9.283f	0	127845	N.D.	0.103 #
19)	B Endosulfa...	0.000	9.504	0	78311	N.D.	0.050 #
20)	A Methoxychlor	0.000	9.859	0	3790	N.D.	0.005 #
25)	Chlordane-3	0.000	8.236	0	68556	N.D.	0.247 #
27)	Chlordane-5	0.000	9.191	0	57303	N.D.	0.939 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 17:49
Operator : AR\AJ
Sample : PB142315TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:32:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

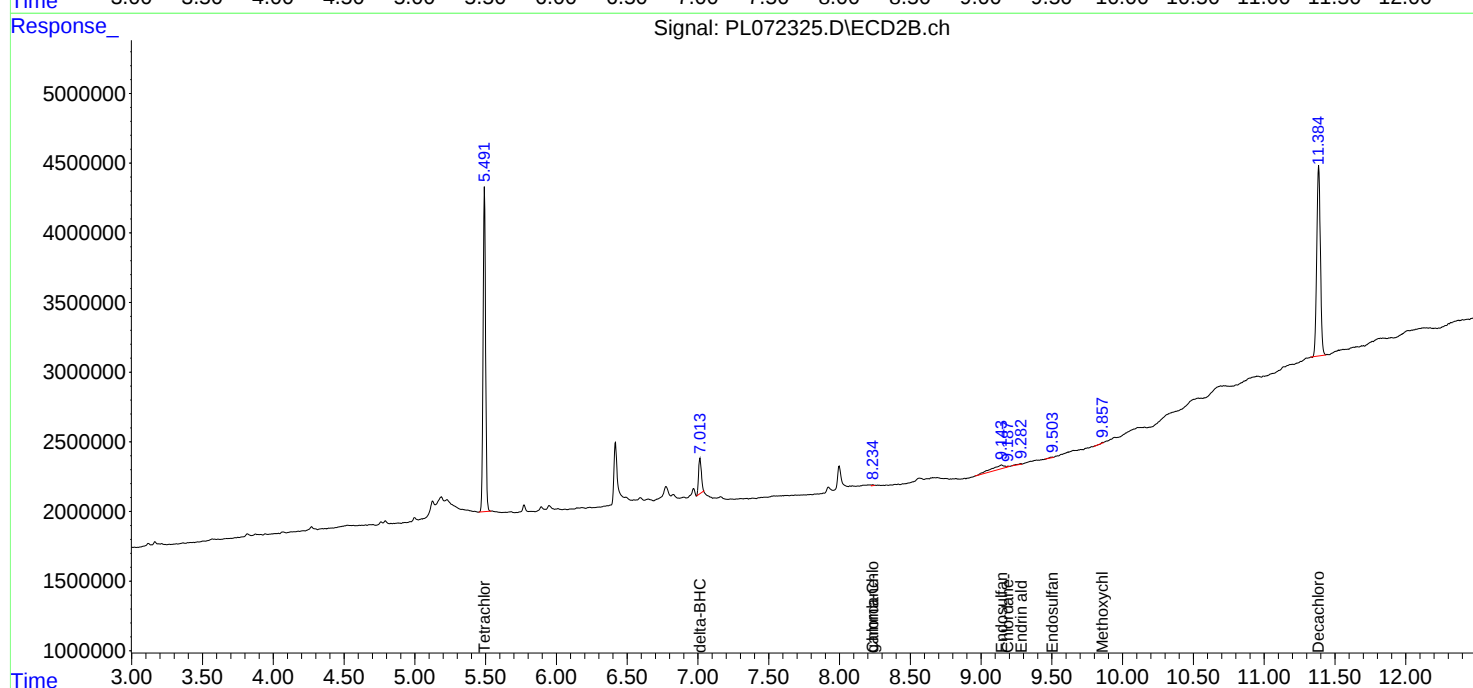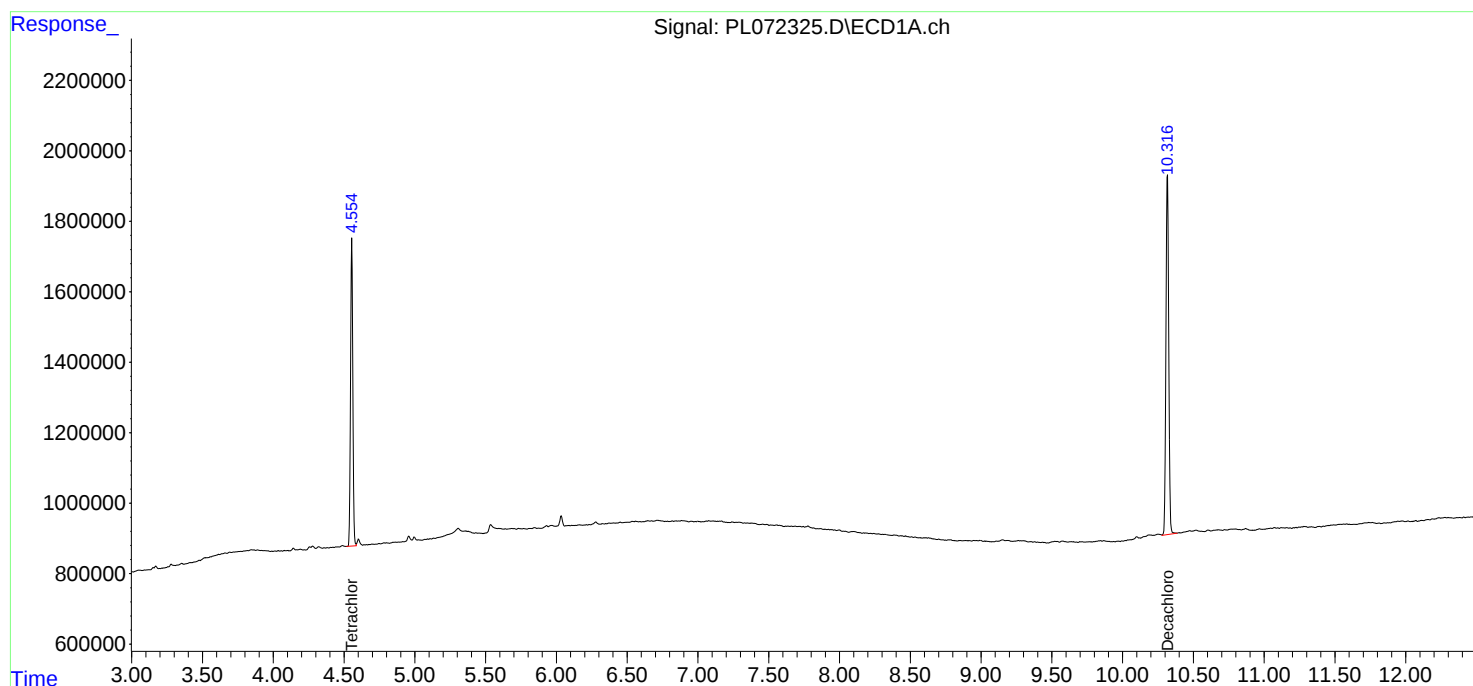


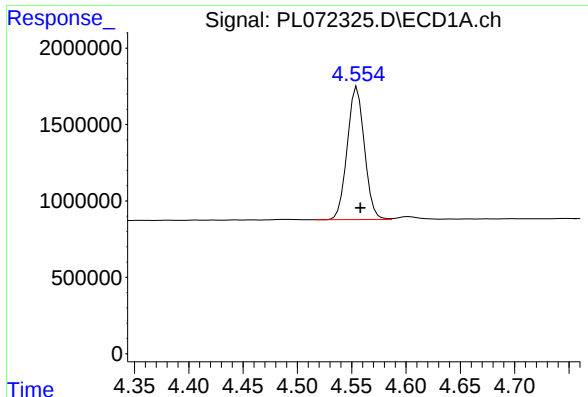

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 9557749
Conc: 17.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

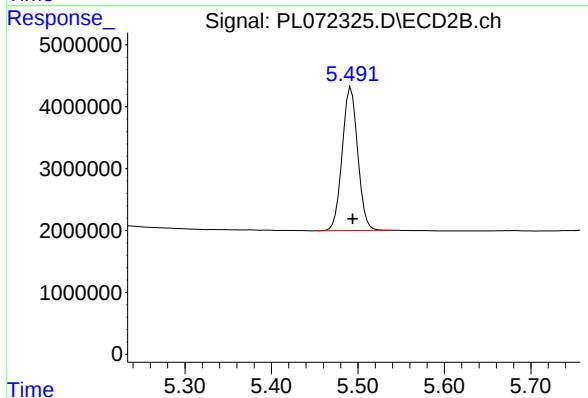


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 28671860
Conc: 17.65 ng/ml

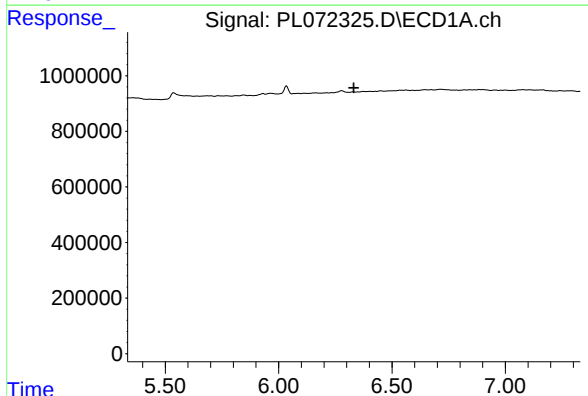


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

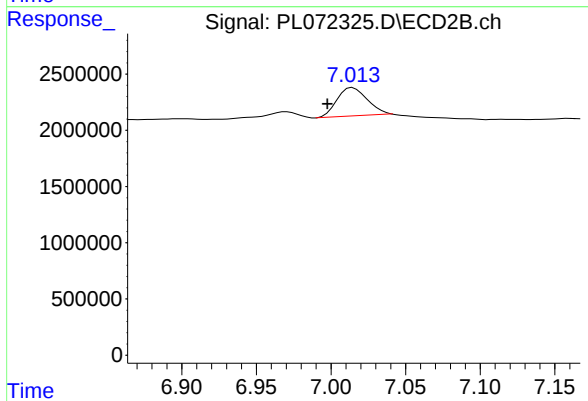

#7 delta-BHC


R.T.: 7.015 min
Delta R.T.: 0.017 min
Response: 3533112
Conc: 1.44 ng/ml

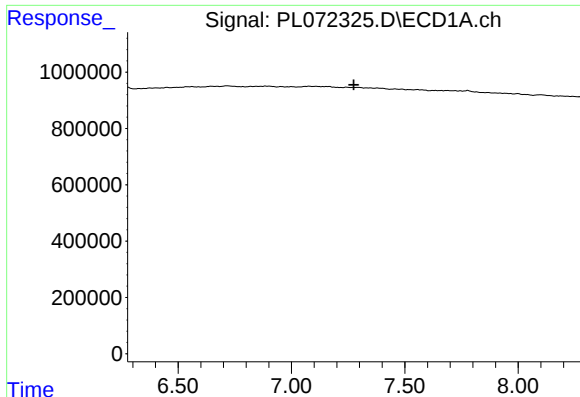

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

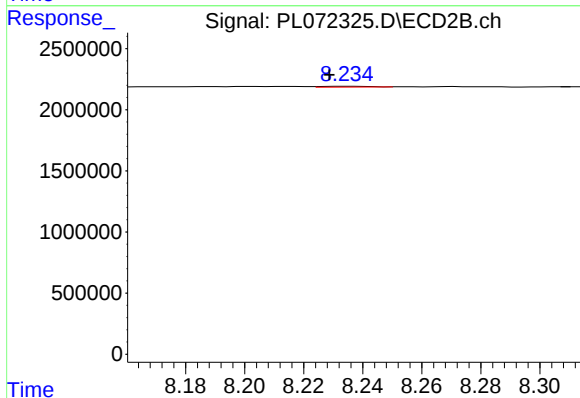


#10 gamma-Chlordane

R.T.: 8.236 min
Delta R.T.: 0.007 min
Response: 68556
Conc: 0.03 ng/ml

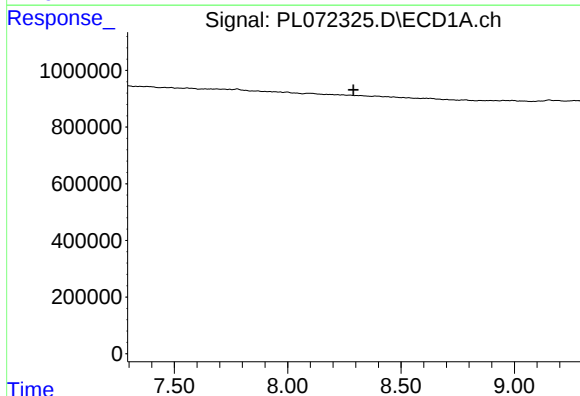


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

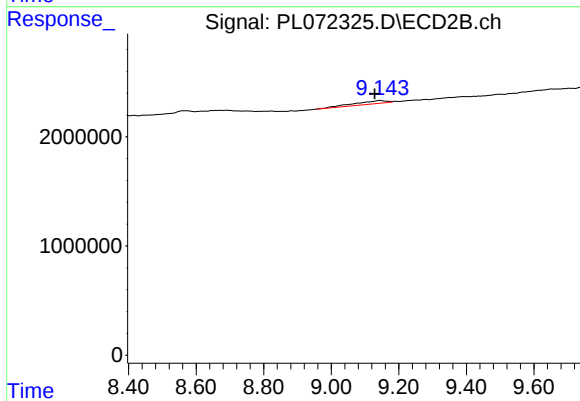

#15 Endosulfan II


R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 1901808
Conc: 1.11 ng/ml

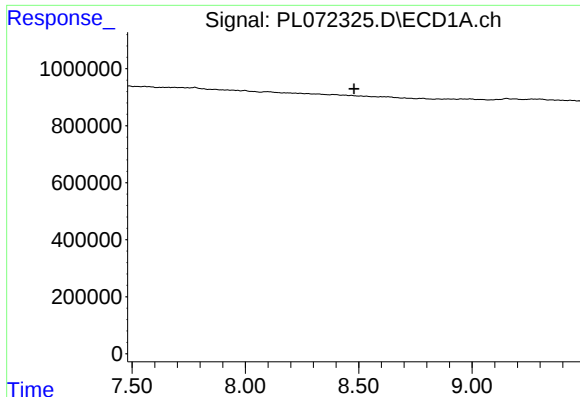

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

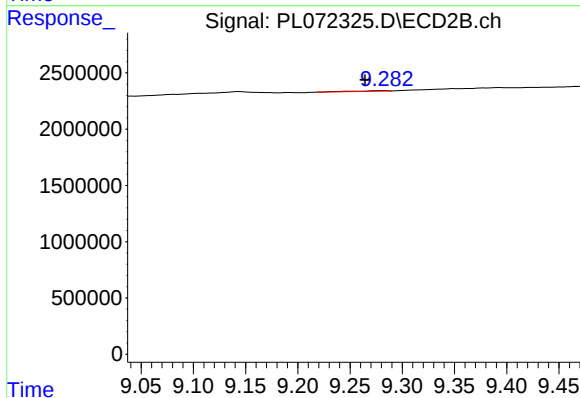


#18 Endrin aldehyde

R.T.: 9.283 min
Delta R.T.: 0.019 min
Response: 127845
Conc: 0.10 ng/ml

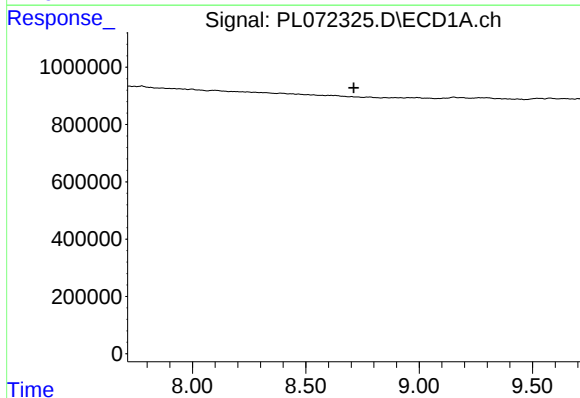


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

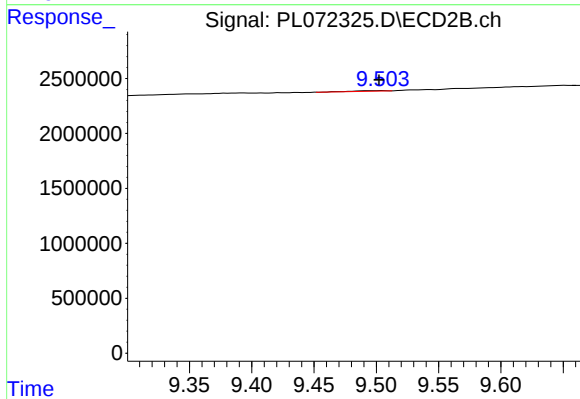

#19 Endosulfan Sulfate


R.T.: 9.504 min
Delta R.T.: 0.002 min
Response: 78311
Conc: 0.05 ng/ml

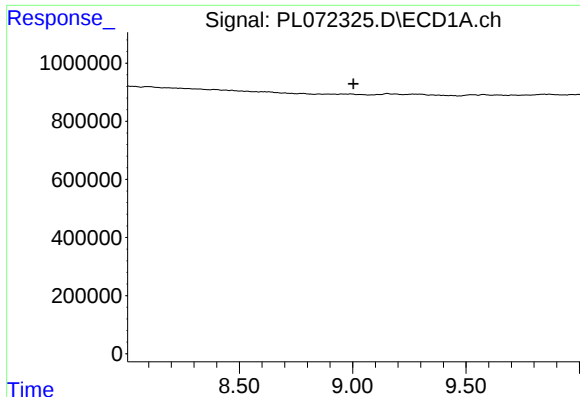

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

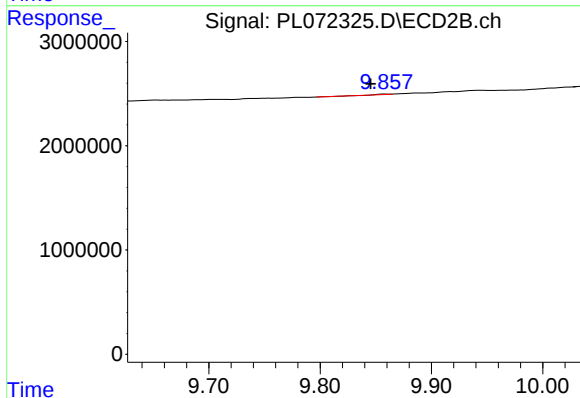


#20 Methoxychlor

R.T.: 9.859 min
Delta R.T.: 0.013 min
Response: 3790
Conc: 0.00 ng/ml

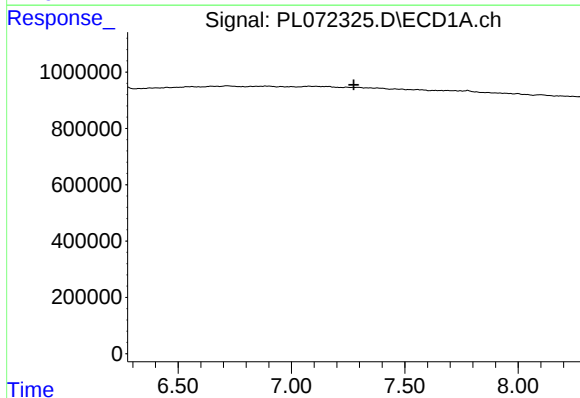


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

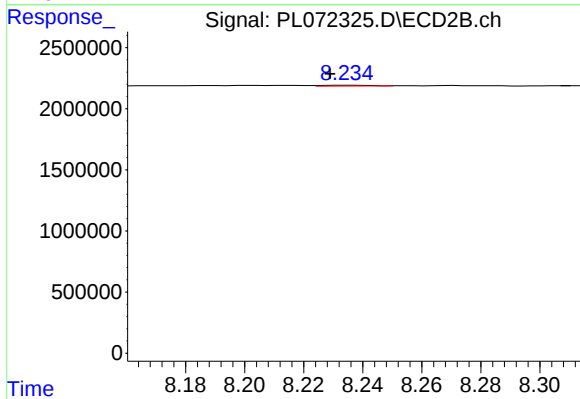

#25 Chlordane-3


R.T.: 8.236 min
Delta R.T.: 0.007 min
Response: 68556
Conc: 0.25 ng/ml

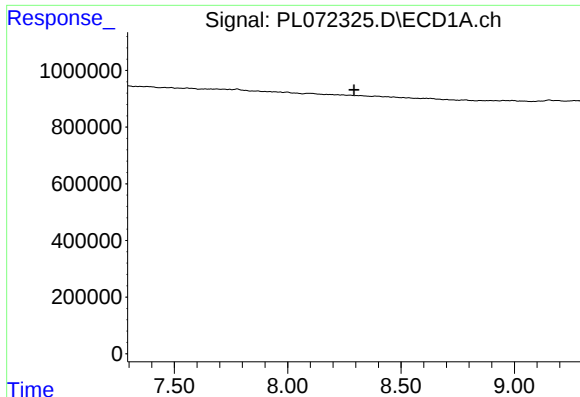

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

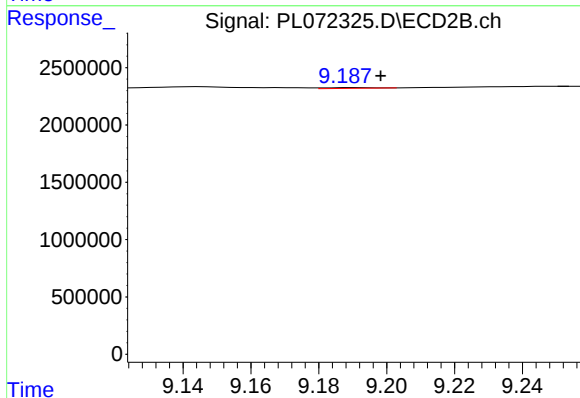


#27 Chlordane-5

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 57303
Conc: 0.94 ng/ml

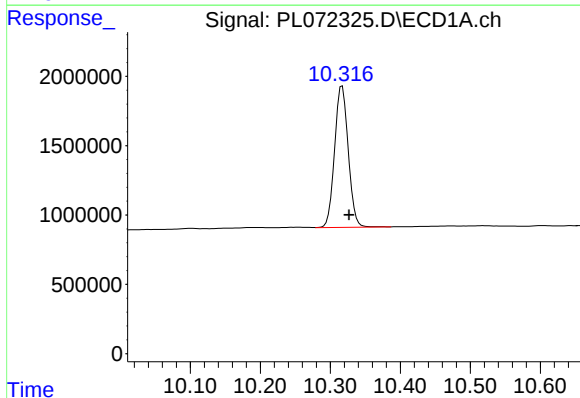

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 13787979
Conc: 15.52 ng/ml

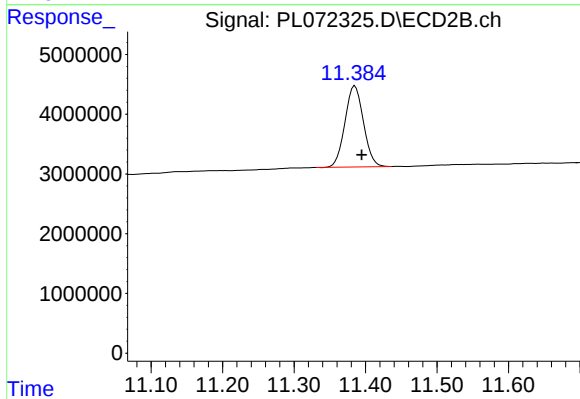

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.009 min
Response: 24491221
Conc: 15.18 ng/ml