

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 22:40
 Operator : AR\AJ
 Sample : N1313-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:36:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.492	11754234	35889854	21.172	22.098
28)	SA Decachlor...	10.320	11.387	17915374	32164433	20.165	19.935
Target Compounds							
2)	A alpha-BHC	0.000	6.053f	0	276104	N.D.	0.114 #
5)	MB Aldrin	0.000	7.511f	0	81612	N.D.	0.037 #
7)	B delta-BHC	0.000	7.015f	0	6768850	N.D.	2.751 #
9)	A Endosulfan I	0.000	8.345f	0	83233	N.D.	0.046 #
10)	B gamma-Chl...	0.000	8.220	0	881245	N.D.	0.436 #
11)	B alpha-Chl...	0.000	8.316	0	128658	N.D.	0.065 #
15)	B Endosulfa...	0.000	9.145f	0	2202284	N.D.	1.284 #
16)	A 4,4'-DDD	0.000	9.039	0	1387369	N.D.	0.970 #
17)	MA 4,4'-DDT	0.000	9.349	0	65972	N.D.	0.042 #
19)	B Endosulfa...	0.000	9.517	0	16897	N.D.	0.011 #
25)	Chlordane-3	0.000	8.220	0	881245	N.D.	3.172 #
26)	Chlordane-4	0.000	8.316	0	128658	N.D.	0.387 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 22:40
Operator : AR\AJ
Sample : N1313-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:36:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

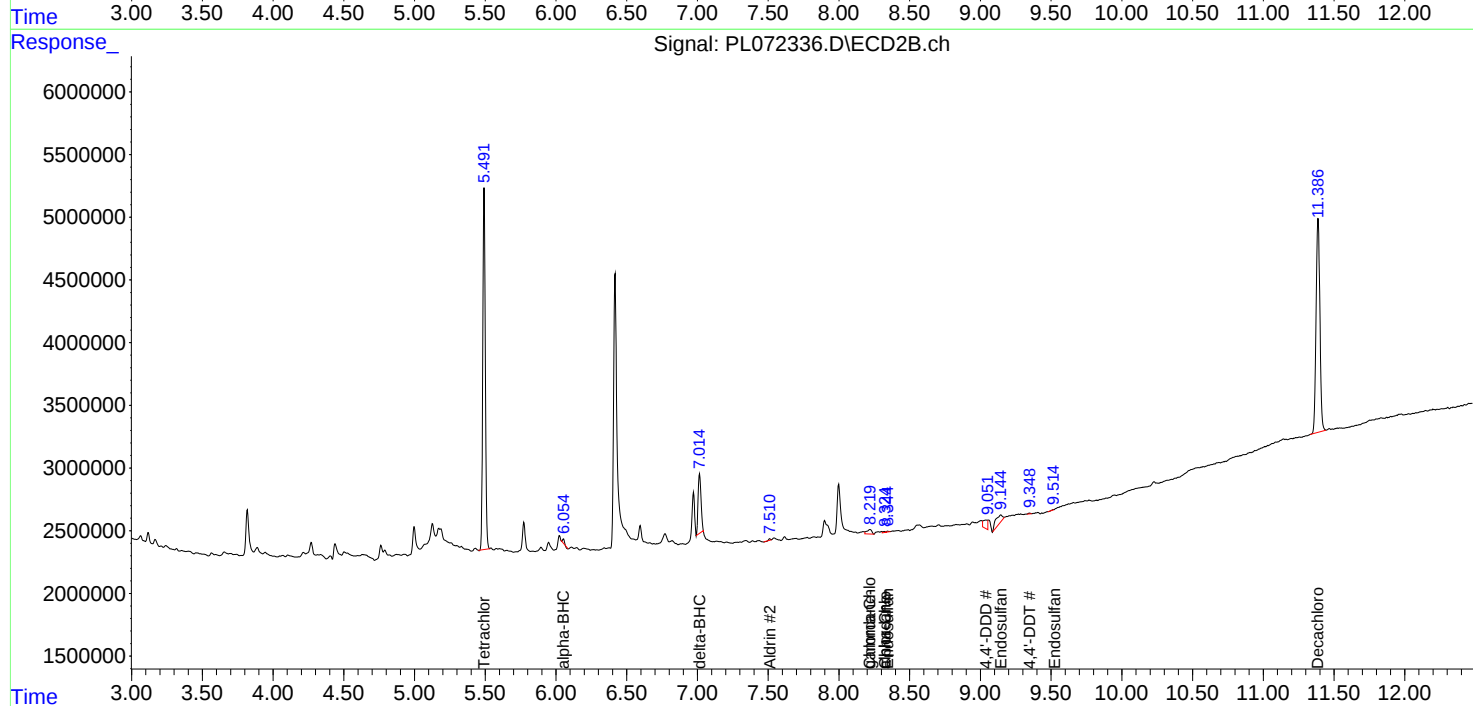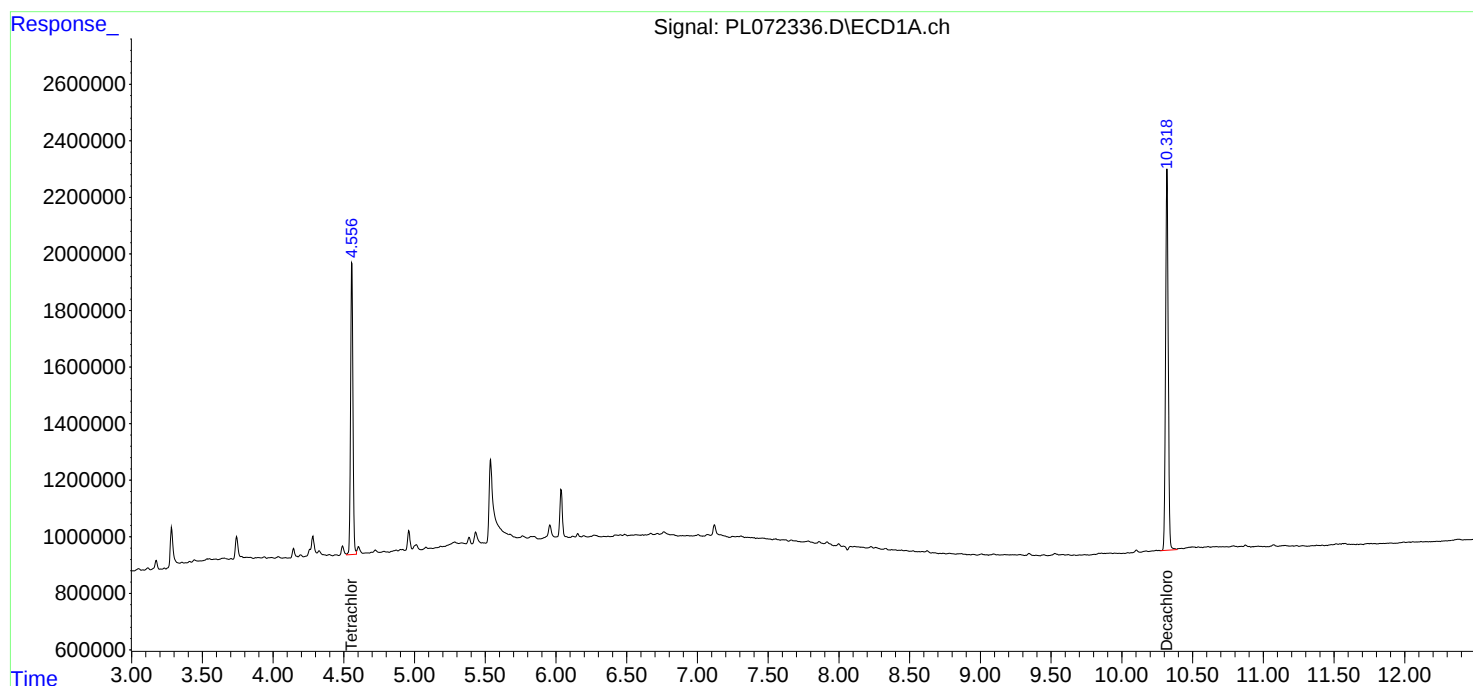


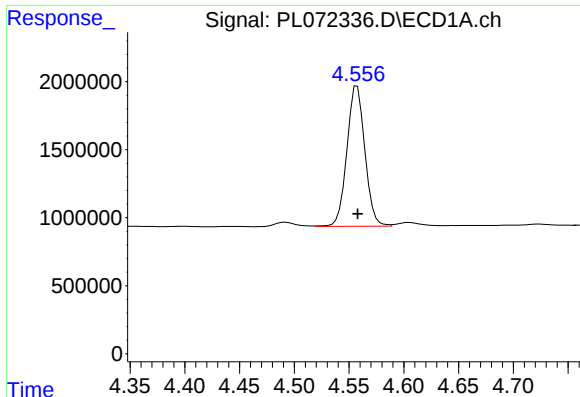

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 11754234
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

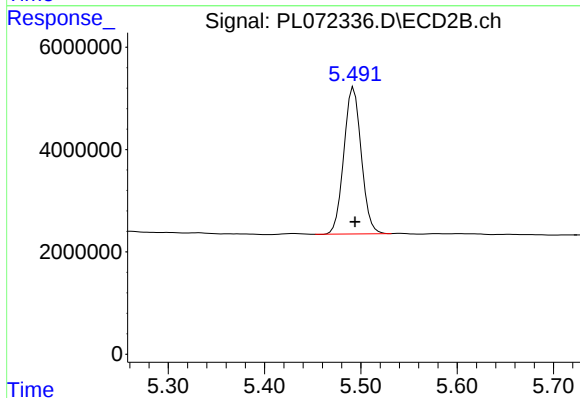


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 35889854
Conc: 22.10 ng/ml

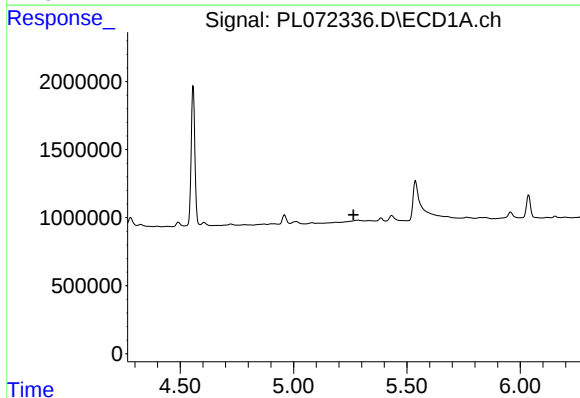


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

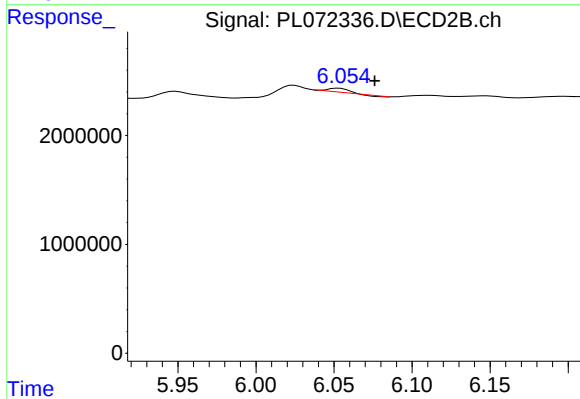

#2 alpha-BHC


R.T.: 6.053 min
Delta R.T.: -0.023 min
Response: 276104
Conc: 0.11 ng/ml

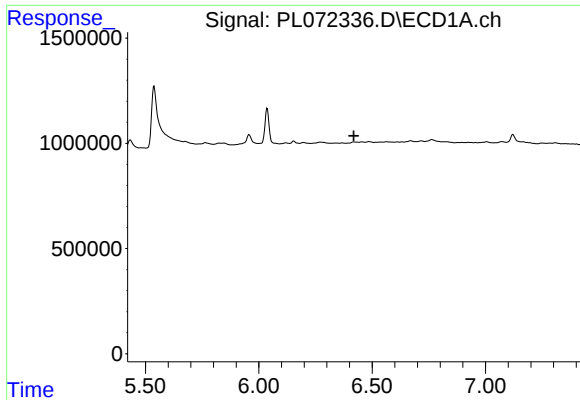

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

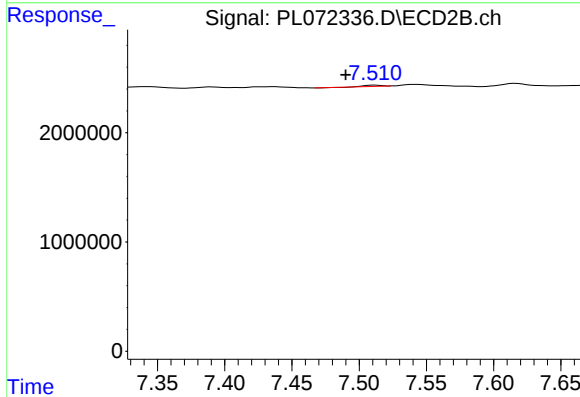


#5 Aldrin

R.T.: 7.511 min
Delta R.T.: 0.021 min
Response: 81612
Conc: 0.04 ng/ml

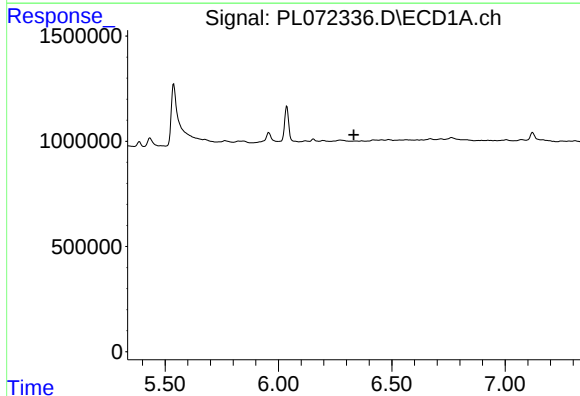


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

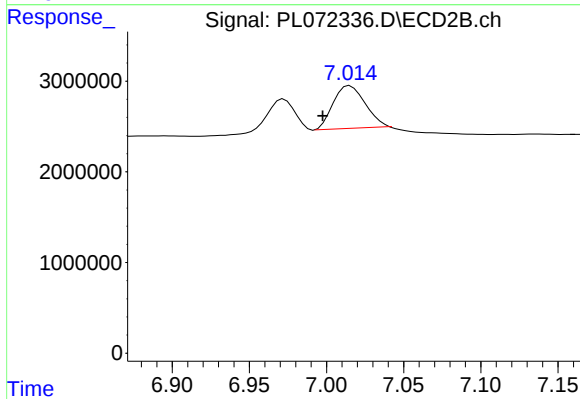

#7 delta-BHC


R.T.: 7.015 min
Delta R.T.: 0.018 min
Response: 6768850
Conc: 2.75 ng/ml

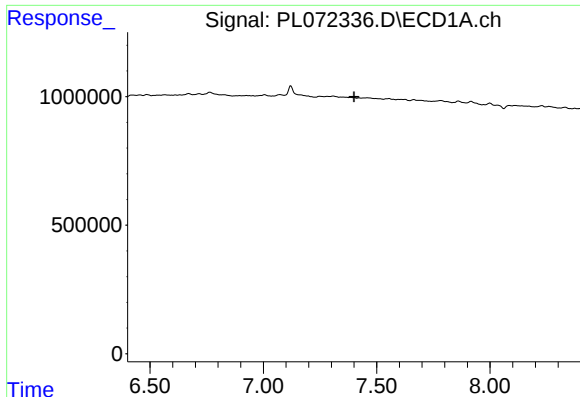

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

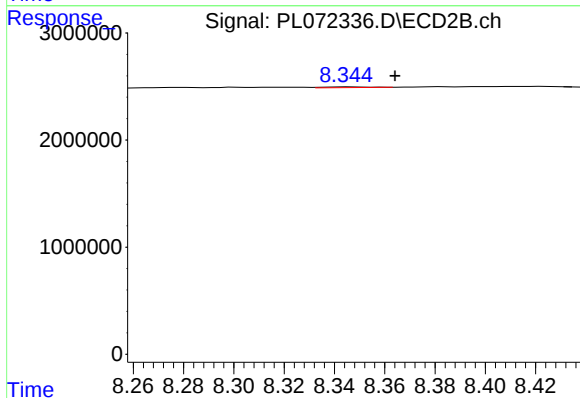


#9 Endosulfan I

R.T.: 8.345 min
Delta R.T.: -0.019 min
Response: 83233
Conc: 0.05 ng/ml

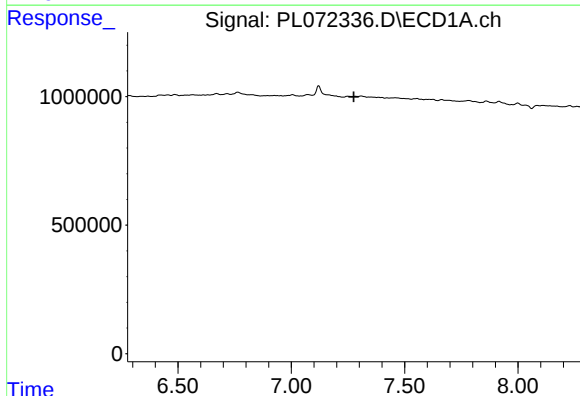


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

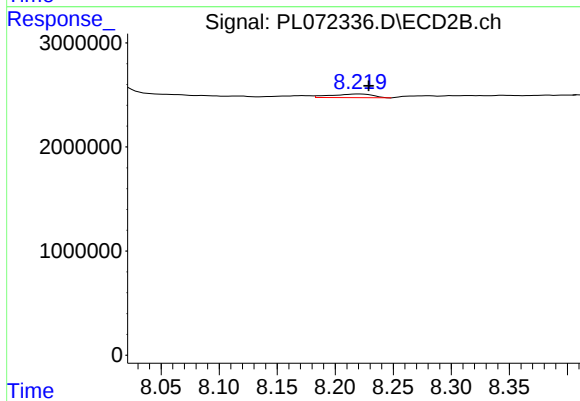

#10 gamma-Chlordane


R.T.: 8.220 min
Delta R.T.: -0.008 min
Response: 881245
Conc: 0.44 ng/ml

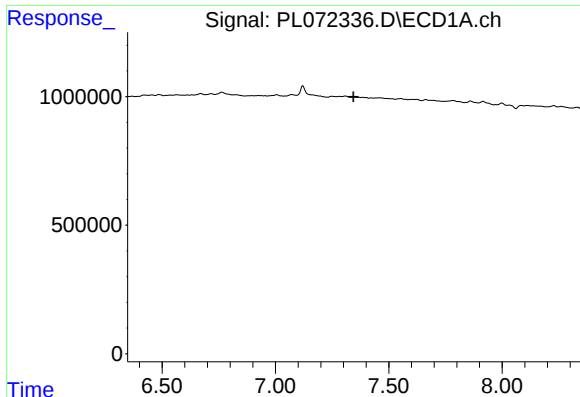

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

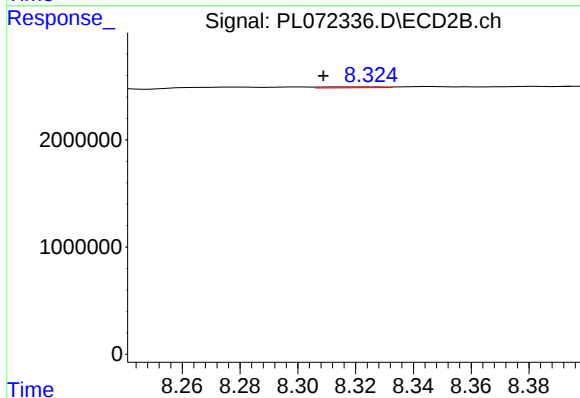


#11 alpha-Chlordane

R.T.: 8.316 min
Delta R.T.: 0.007 min
Response: 128658
Conc: 0.06 ng/ml

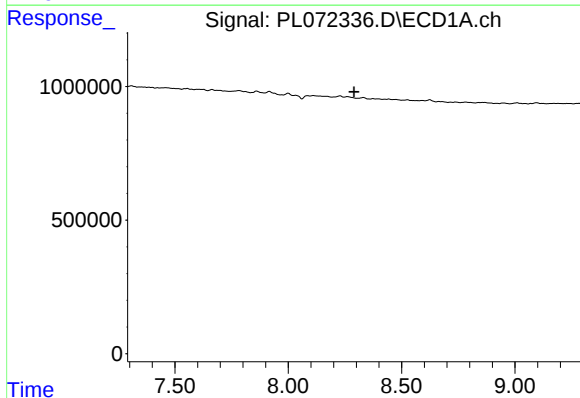


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

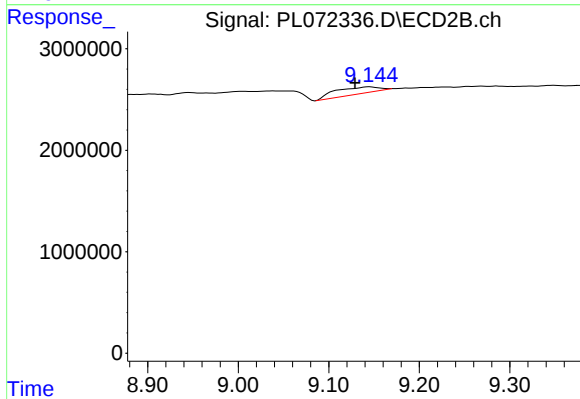

#15 Endosulfan II


R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 2202284
Conc: 1.28 ng/ml

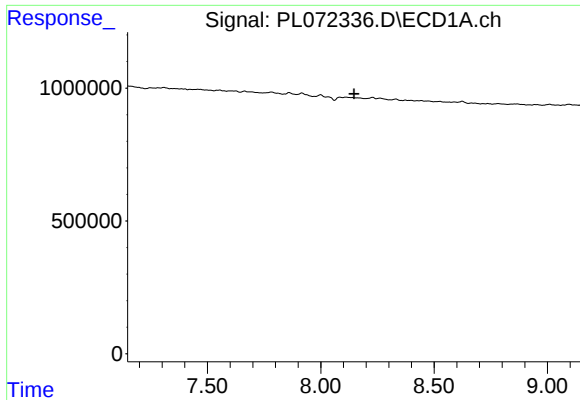

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

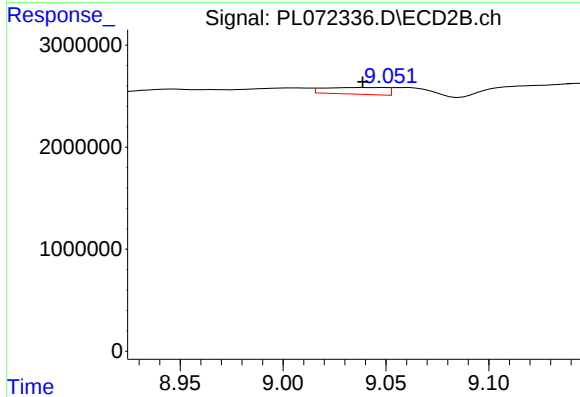


#16 4,4'-DDD

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 1387369
Conc: 0.97 ng/ml

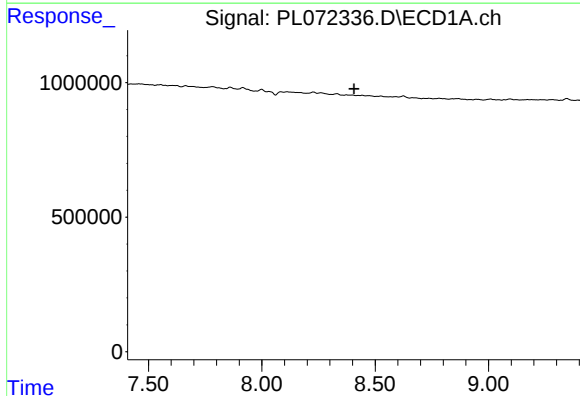


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

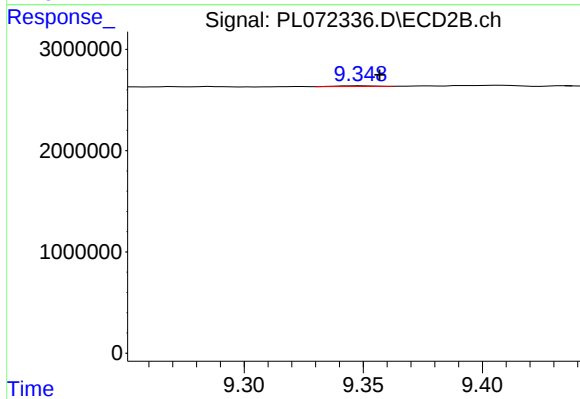

#17 4,4'-DDT


R.T.: 9.349 min
Delta R.T.: -0.008 min
Response: 65972
Conc: 0.04 ng/ml

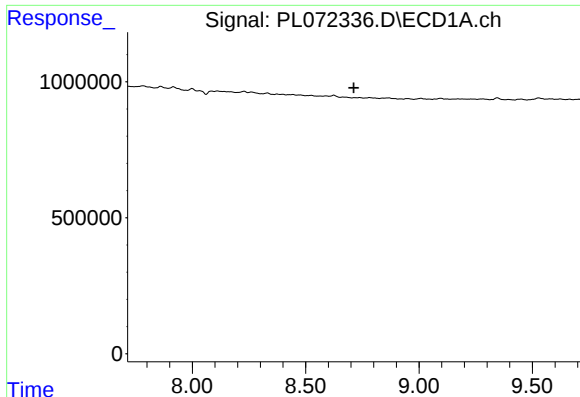

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

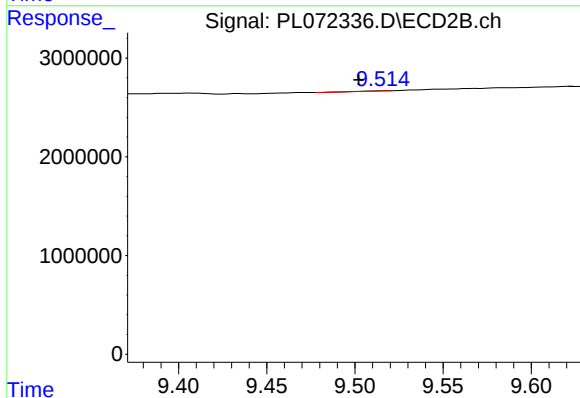


#19 Endosulfan Sulfate

R.T.: 9.517 min
Delta R.T.: 0.015 min
Response: 16897
Conc: 0.01 ng/ml

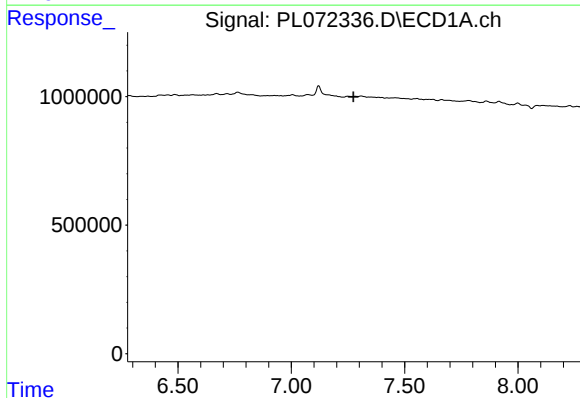


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

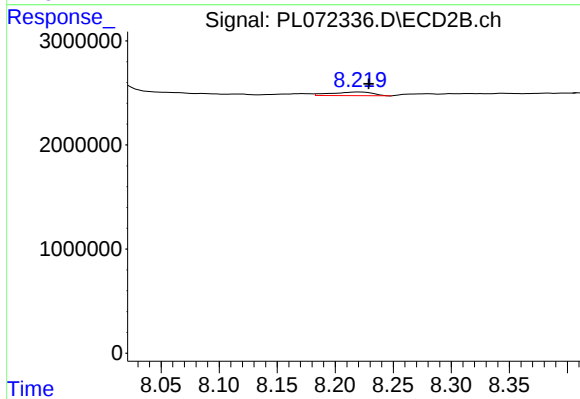

#25 Chlordane-3


R.T.: 8.220 min
Delta R.T.: -0.008 min
Response: 881245
Conc: 3.17 ng/ml

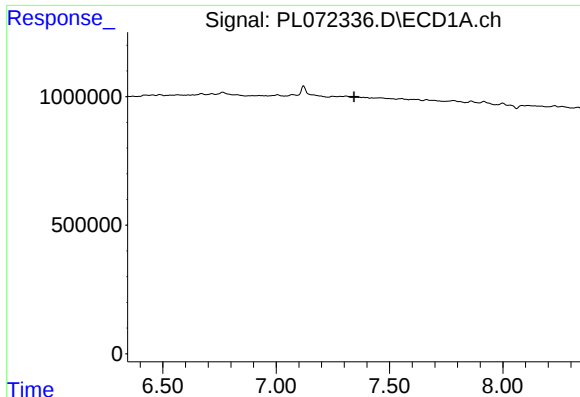

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

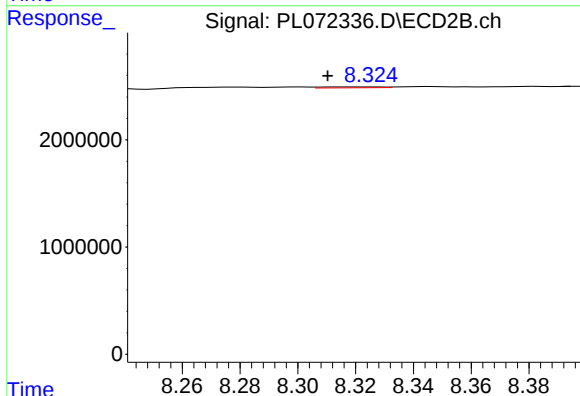


#26 Chlordane-4

R.T.: 8.316 min
Delta R.T.: 0.006 min
Response: 128658
Conc: 0.39 ng/ml

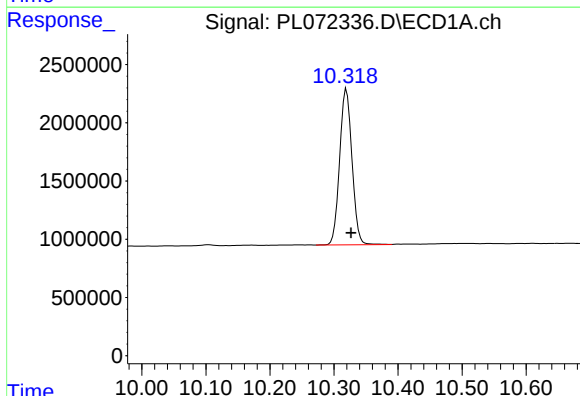

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.007 min
Response: 17915374
Conc: 20.17 ng/ml

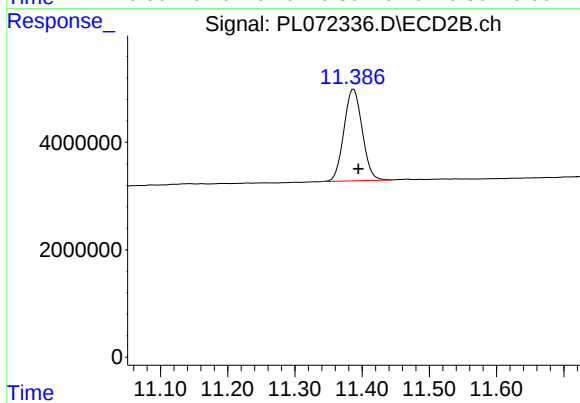

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.007 min
Response: 32164433
Conc: 19.93 ng/ml