

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
 Data File : PL072321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 16:44
 Operator : AR\AJ
 Sample : N1314-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-012722

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/31/2022
 Supervised By :Ankita Jodhani 01/31/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:30:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	839676	2058470	1.512	1.267
2)	SA Decachlor...	10.316	11.385	1278680	2458874	1.439m	1.524
Target Compounds							
10)	B gamma-Chl...	7.270	8.224	910989	3345734	1.159	1.656 #
11)	B alpha-Chl...	7.338	8.305	1510646	5903630	1.926	2.977 #
12)	B 4,4'-DDE	7.554	8.491	504439	707786	0.699	0.374 #
17)	MA 4,4'-DDT	8.399	9.348	315803	567069	0.476	0.359m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012822\
Data File : PL072321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 16:44
Operator : AR\AJ
Sample : N1314-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-01-012722


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/31/2022
Supervised By : Ankita Jodhani 01/31/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:30:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

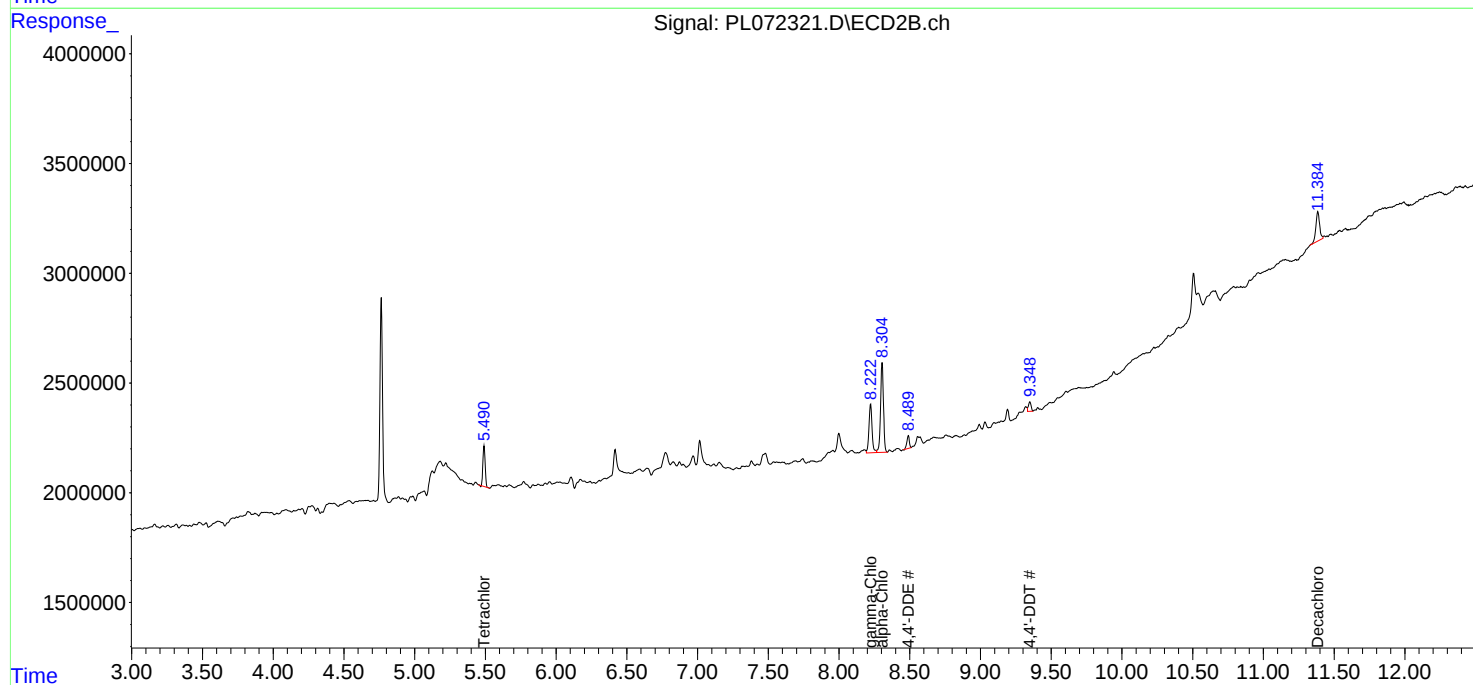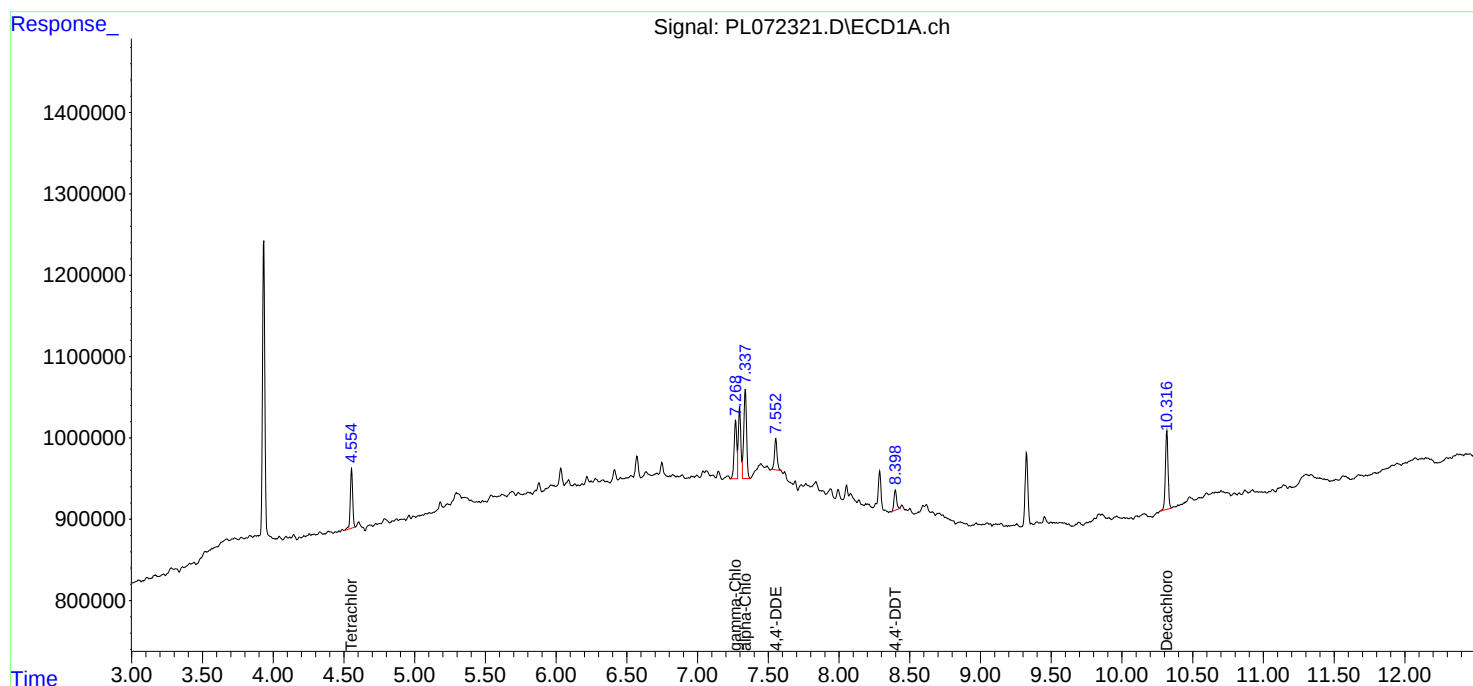

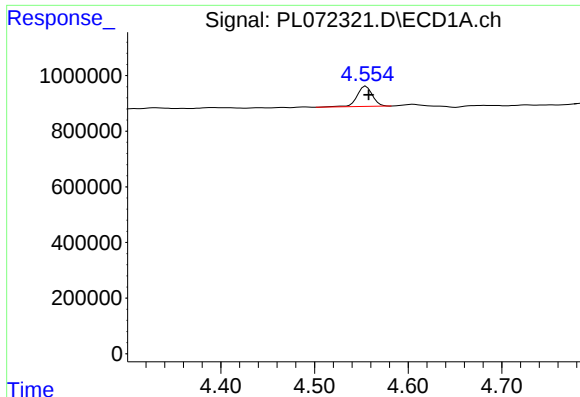


#1 Tetrachloro-m-xylene

R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 839676
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-012722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2022
Supervised By :Ankita Jodhani 01/31/2022

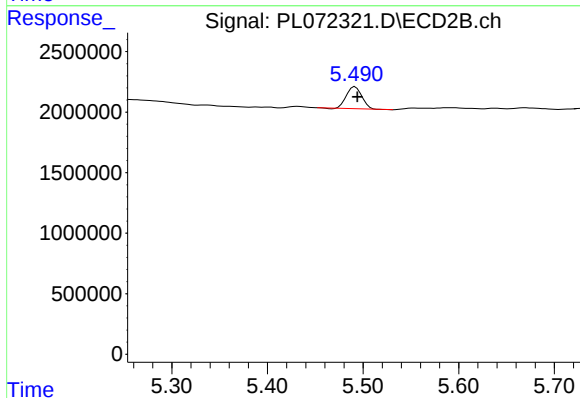


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 2058470
Conc: 1.27 ng/ml

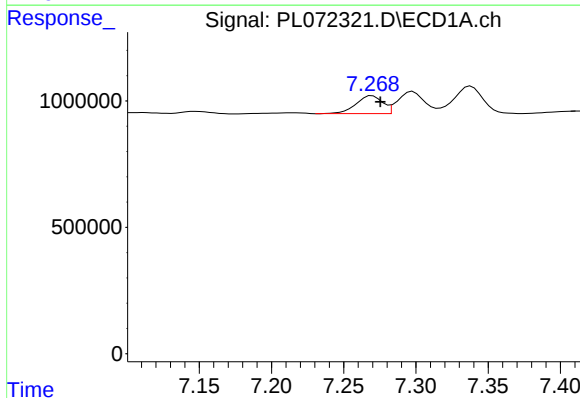


#10 gamma-Chlordane

R.T.: 7.270 min
Delta R.T.: -0.006 min
Response: 910989
Conc: 1.16 ng/ml

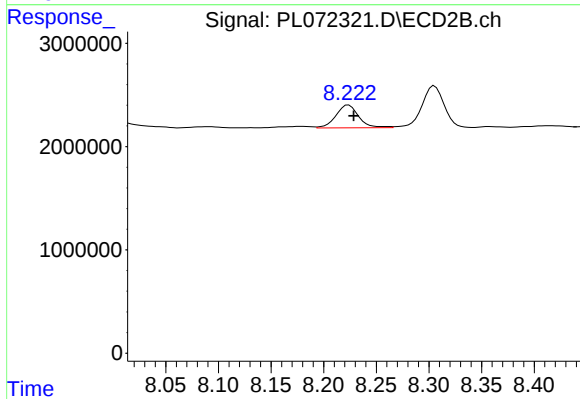

#10 gamma-Chlordane

R.T.: 8.224 min
Delta R.T.: -0.005 min
Response: 3345734
Conc: 1.66 ng/ml

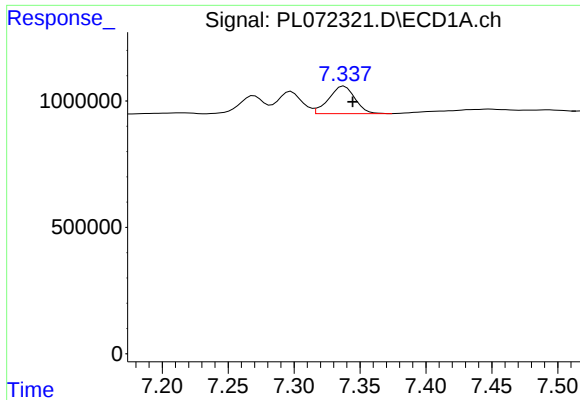


#11 alpha-Chlordane

R.T.: 7.338 min
Delta R.T.: -0.006 min
Response: 1510646
Conc: 1.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-012722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2022
Supervised By :Ankita Jodhani 01/31/2022

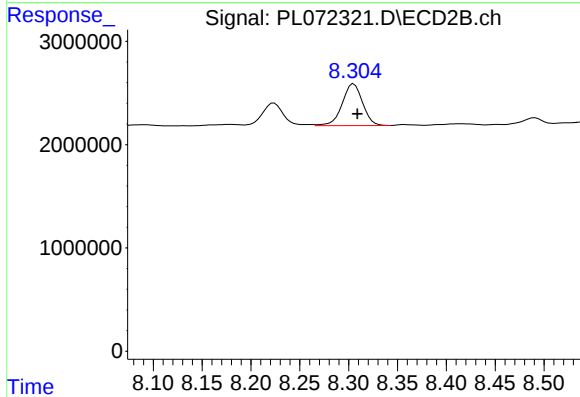


#11 alpha-Chlordane

R.T.: 8.305 min
Delta R.T.: -0.003 min
Response: 5903630
Conc: 2.98 ng/ml

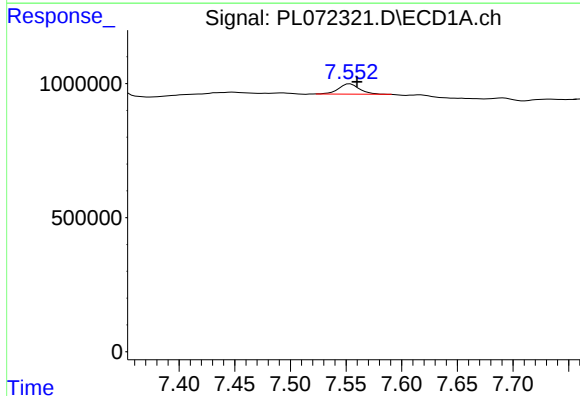


#12 4,4'-DDE

R.T.: 7.554 min
Delta R.T.: -0.006 min
Response: 504439
Conc: 0.70 ng/ml

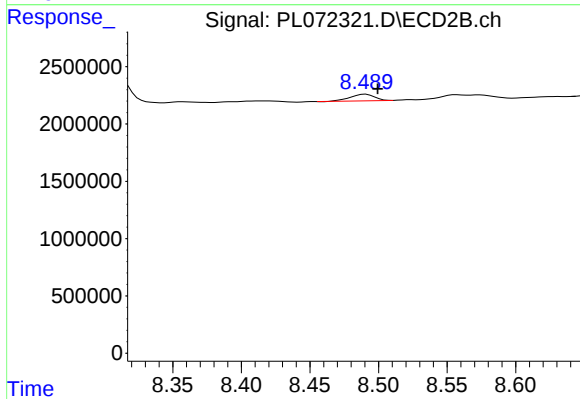

#12 4,4'-DDE

R.T.: 8.491 min
Delta R.T.: -0.009 min
Response: 707786
Conc: 0.37 ng/ml

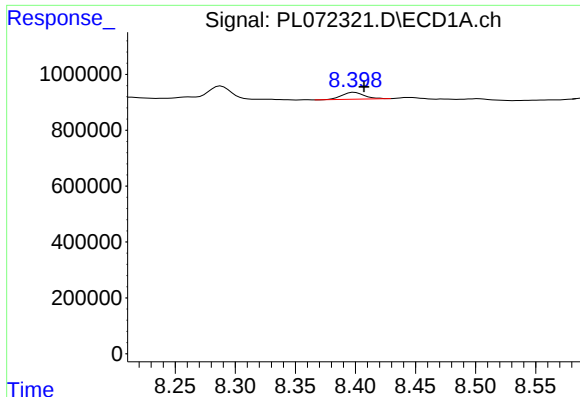


#17 4,4'-DDT

R.T.: 8.399 min
Delta R.T.: -0.008 min
Response: 315803
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-012722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2022
Supervised By :Ankita Jodhani 01/31/2022

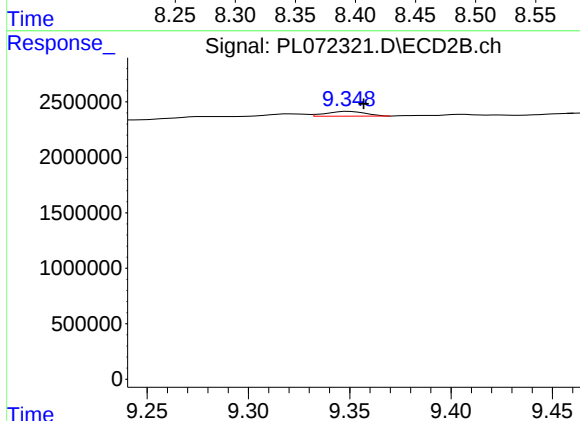


#17 4,4'-DDT

R.T.: 9.348 min
Delta R.T.: -0.009 min
Response: 567069
Conc: 0.36 ng/ml m

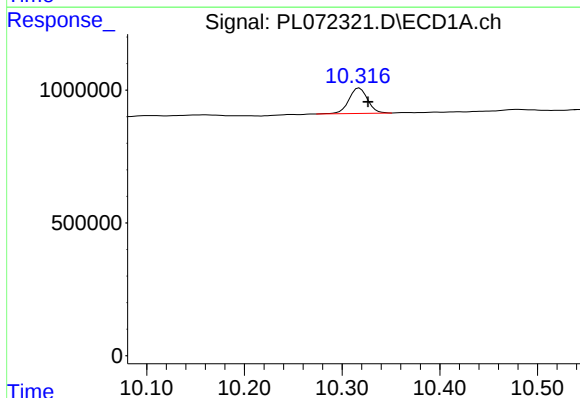

#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: -0.010 min
Response: 1278680
Conc: 1.44 ng/ml m

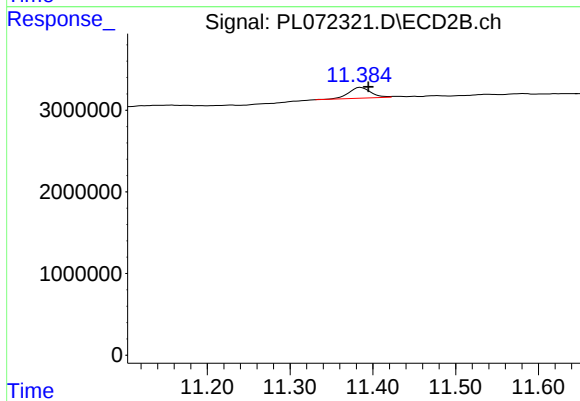

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 2458874
Conc: 1.52 ng/ml