

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012825\
 Data File : PL093831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2025 12:10
 Operator : AR\AJ
 Sample : Q1187-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/29/2025
 Supervised By :Ankita Jodhani 01/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 03:46:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.773	62811284	73336140	23.326m	22.467
28) SA Decachlor...	9.058	7.911	47679663	73981930	22.792	21.113
Target Compounds						
17) MA 4,4'-DDT	7.022	6.032	1982777	3830265	1.005m	1.177m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012825\
Data File : PL093831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2025 12:10
Operator : AR\AJ
Sample : Q1187-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/29/2025
Supervised By : Ankita Jodhani 01/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 03:46:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

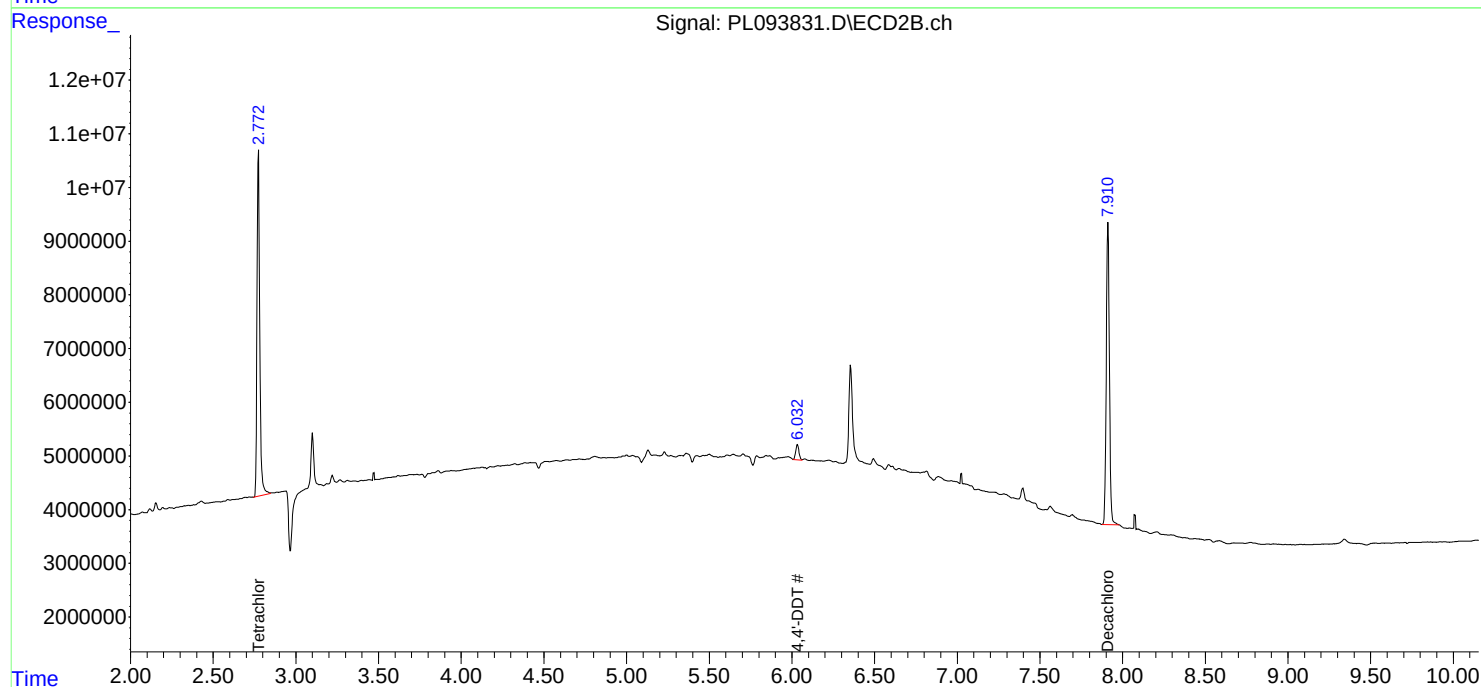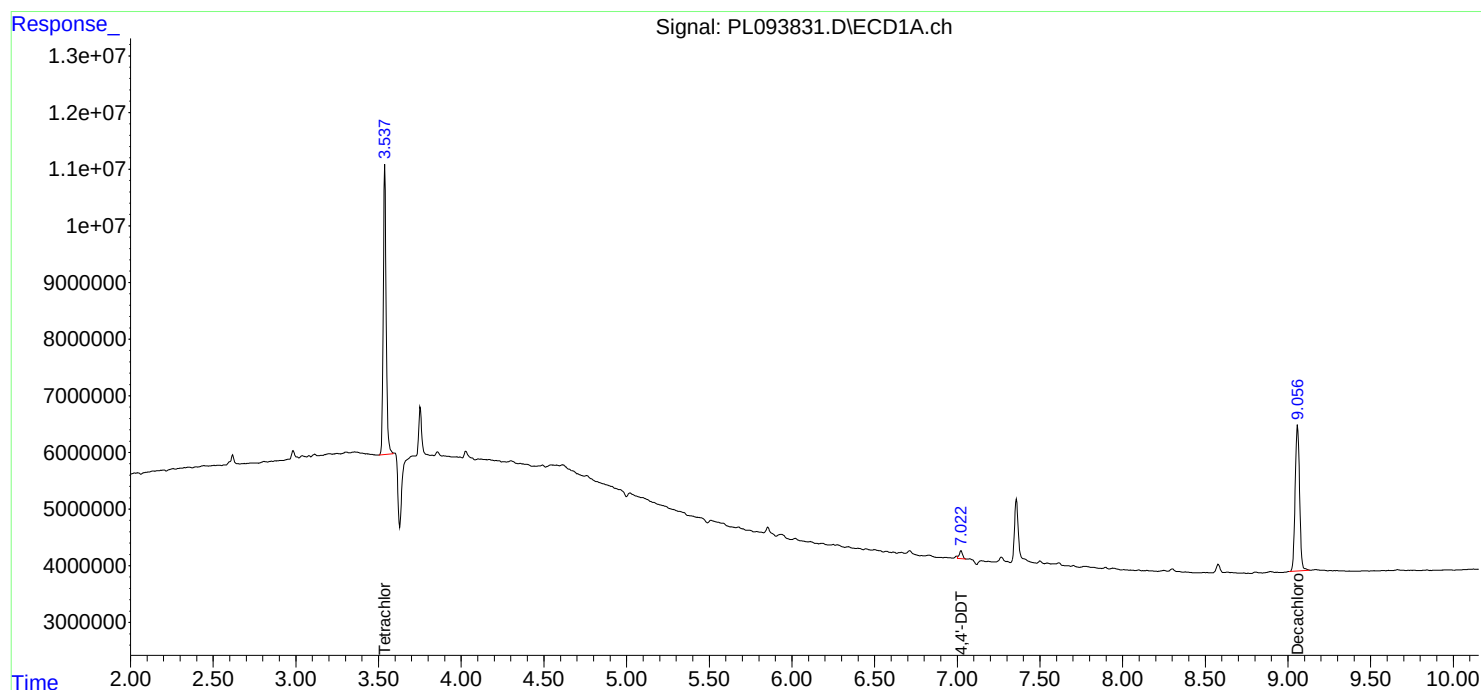

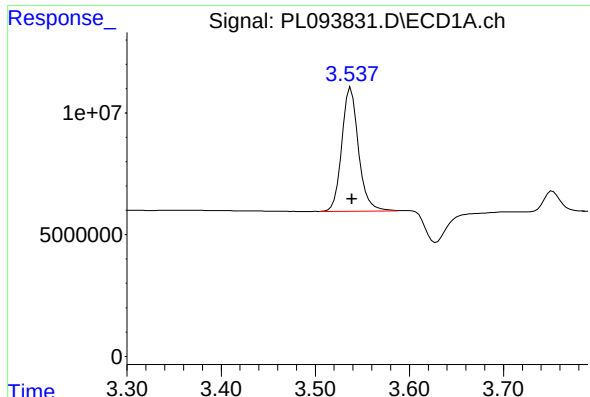


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.002 min
Response: 62811284
Conc: 23.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/29/2025
Supervised By :Ankita Jodhani 01/29/2025

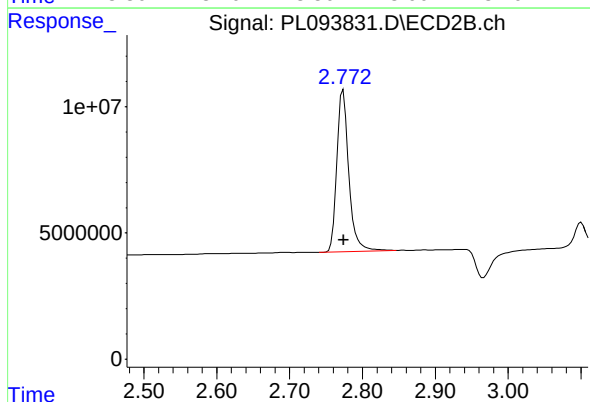


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 73336140
Conc: 22.47 ng/ml

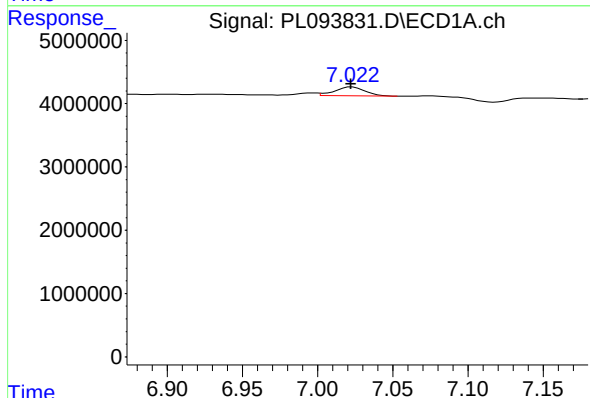


#17 4,4'-DDT

R.T.: 7.022 min
Delta R.T.: 0.000 min
Response: 1982777
Conc: 1.01 ng/ml m

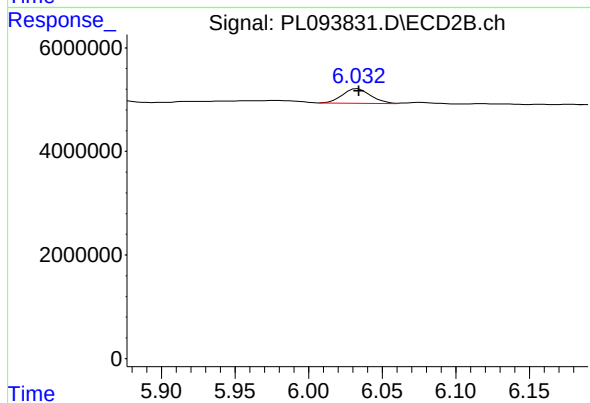

#17 4,4'-DDT

R.T.: 6.032 min
Delta R.T.: -0.002 min
Response: 3830265
Conc: 1.18 ng/ml m

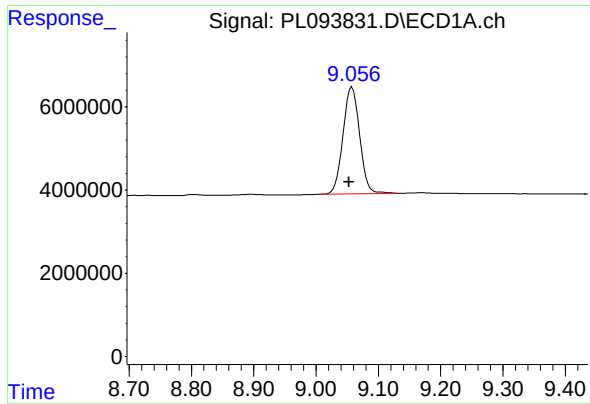


#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.005 min
Response: 47679663
Conc: 22.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-COMP

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/29/2025
Supervised By :Ankita Jodhani 01/29/2025

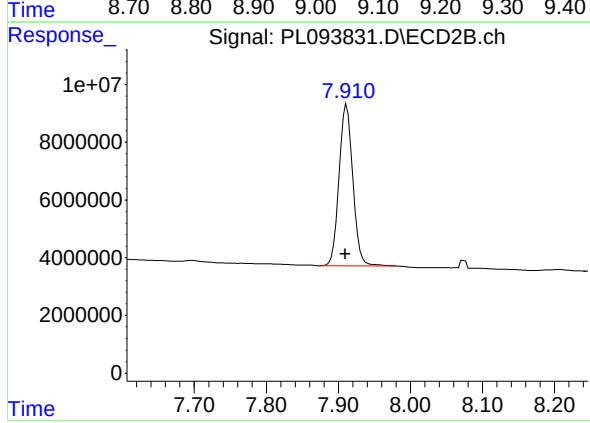

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: 0.002 min
Response: 73981930
Conc: 21.11 ng/ml