

Data Path : P:\HPCHEM1\ECD_L\Data\PL012918\
 Data File : PL032621.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2018 12:35
 Operator : UA\AJ
 Sample : J1288-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EPE-121-2(20-22)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 22:41:19 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 04:03:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.408	3.993	171.2E6	25410656	19.151	20.291
28)	SA Decachlor...	8.113	9.025	170.9E6	30188190	14.688	15.871
Target Compounds							
3)	MA gamma-BHC...	4.171f	0.000	12556957	0	0.973	N.D. #
6)	B beta-BHC	4.337f	0.000	12734679	0	2.230	N.D. #
7)	B delta-BHC	0.000	5.027	0	1667298	N.D.	0.750 #
15)	B Endosulfa...	6.138f	0.000	34665112	0	2.955	N.D. #
16)	A 4,4'-DDD	0.000	6.745f	0	7373026	N.D.	5.170 #
20)	A Methoxychlor	6.781f	0.000	33978673	0	5.848	N.D. #
23)	Chlordane-1	0.000	5.027	0	1667298	N.D.	21.562 #
27)	Chlordane-5	6.138	0.000	34665112	0	70.111	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_L\Data\PL012918\
Data File : PL032621.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2018 12:35
Operator : UA\AJ
Sample : J1288-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EPE-121-2(20-22)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 22:41:19 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 04:03:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

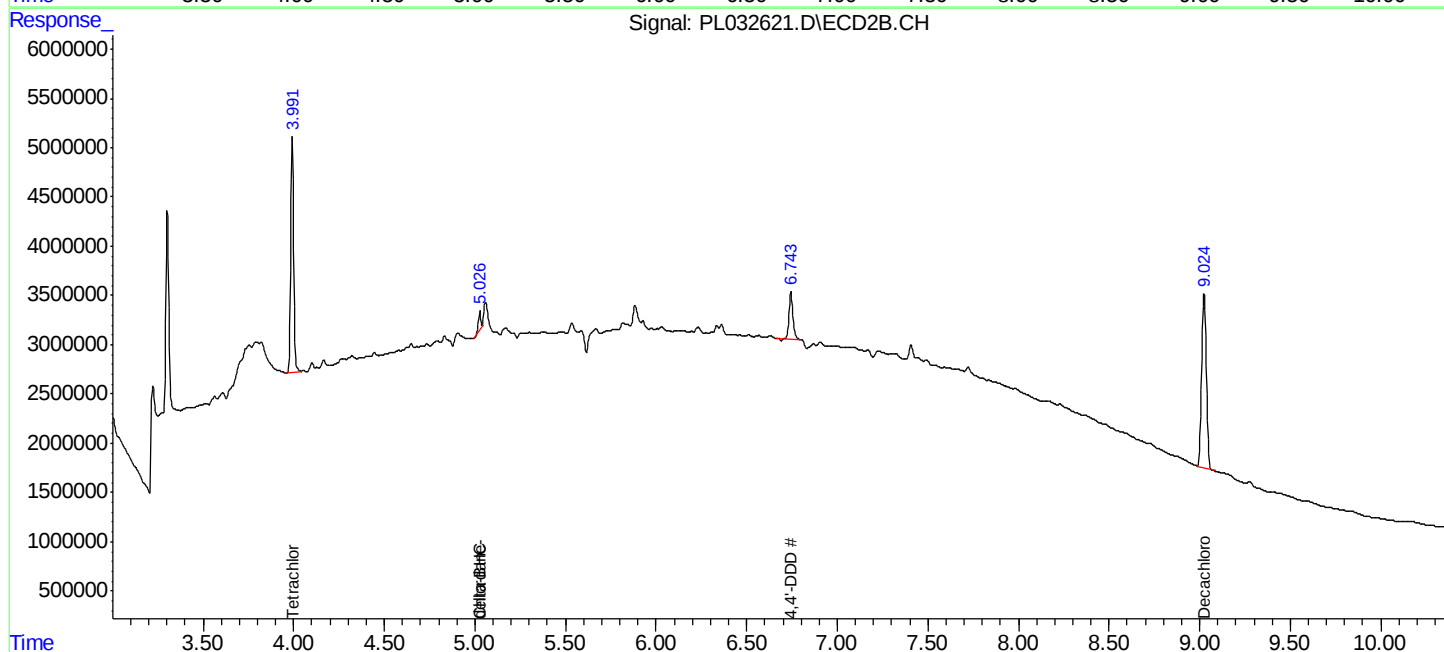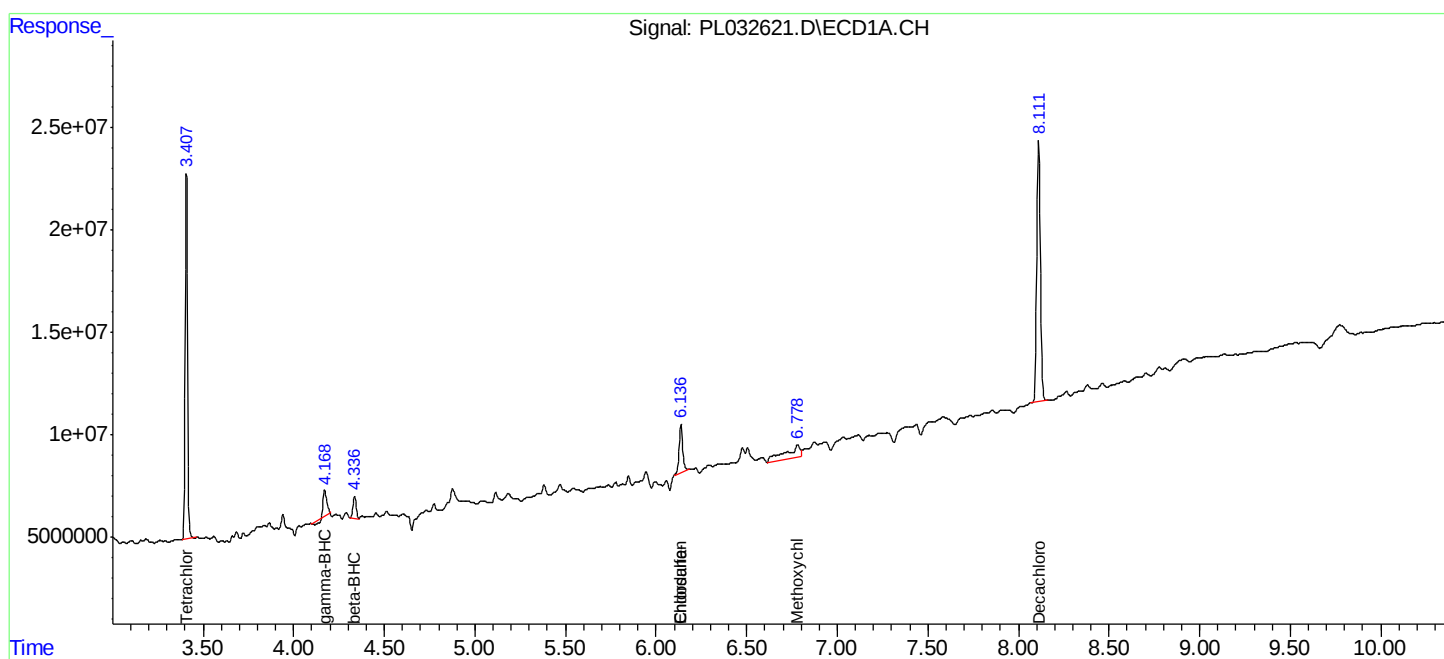


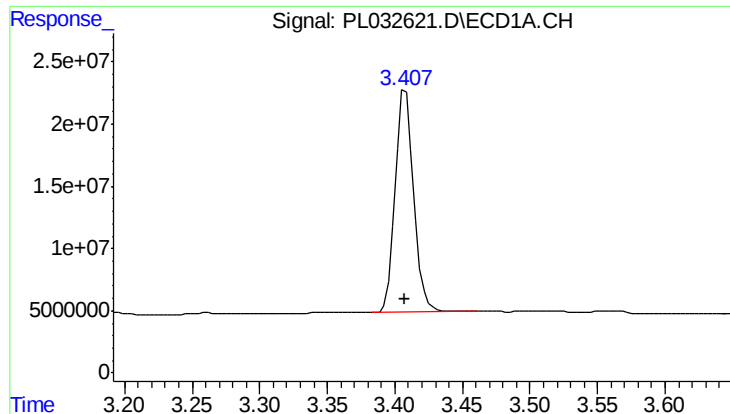

#1 Tetrachloro-m-xylene


R.T.: 3.408 min
Delta R.T.: 0.000 min
Response: 171210533
Conc: 19.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
EPE-121-2(20-22)

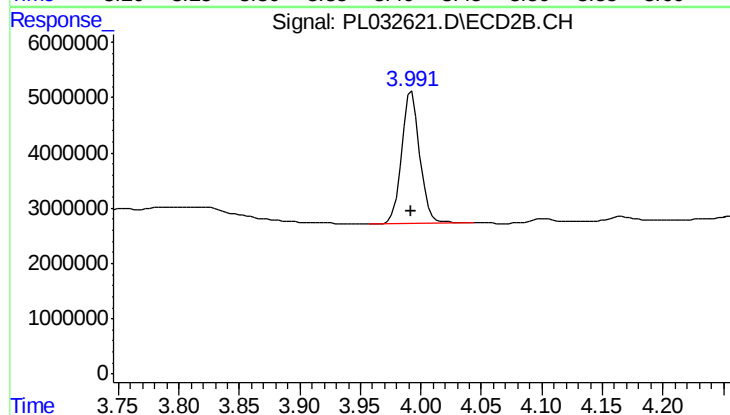


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: 0.001 min
Response: 25410656
Conc: 20.29 ng/ml

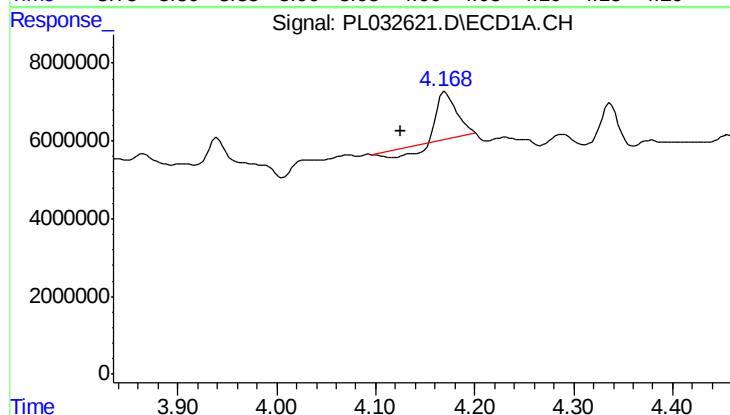


#3 gamma-BHC (Lindane)

R.T.: 4.171 min
Delta R.T.: 0.046 min
Response: 12556957
Conc: 0.97 ng/ml

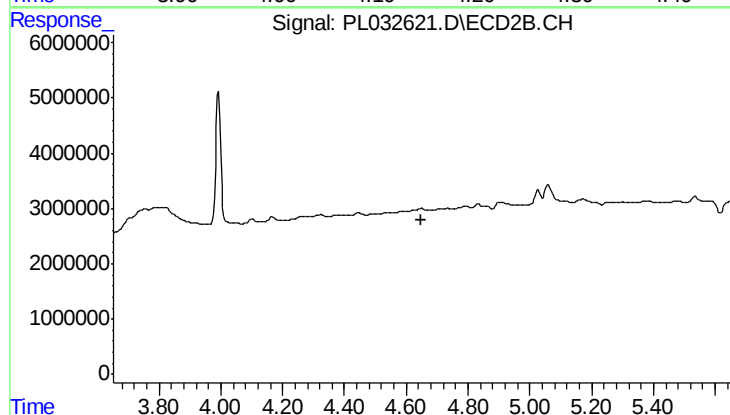

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.650 min
Response: 0
Conc: N.D.

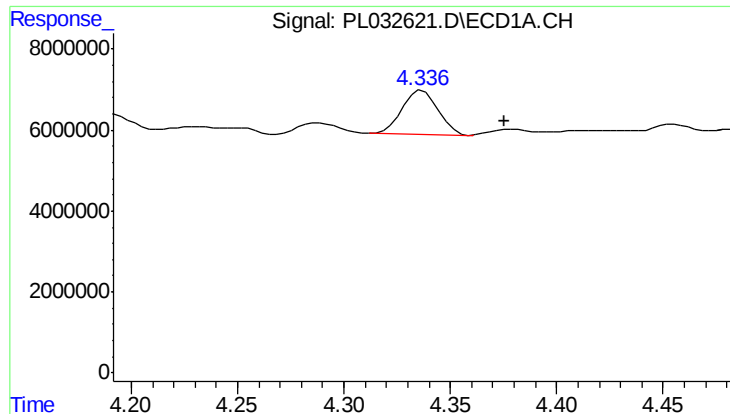

#6 beta-BHC


R.T.: 4.337 min
Delta R.T.: -0.039 min
Response: 12734679
Conc: 2.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
EPE-121-2(20-22)

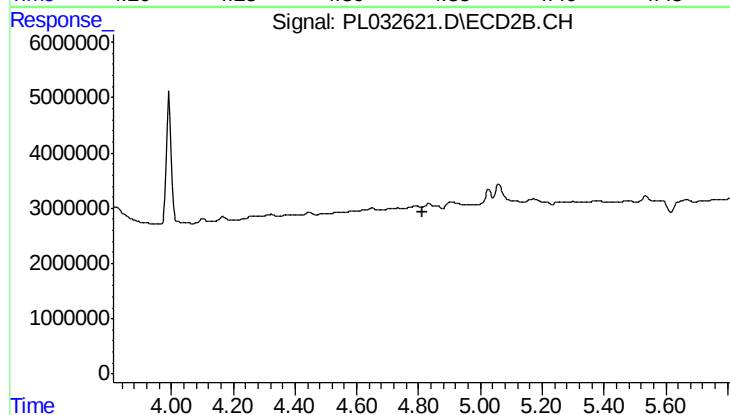


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.811 min
Response: 0
Conc: N.D.

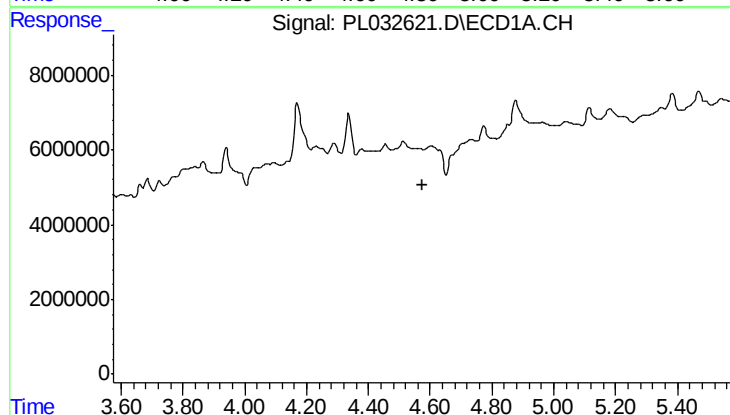


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.574 min
Response: 0
Conc: N.D.

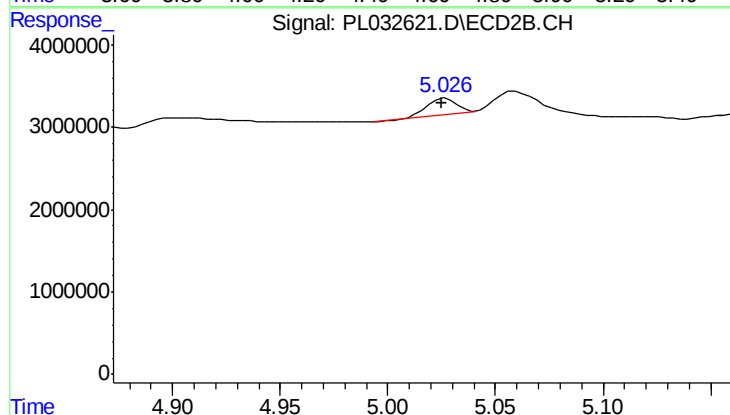

#7 delta-BHC


R.T.: 5.027 min
Delta R.T.: 0.002 min
Response: 1667298
Conc: 0.75 ng/ml

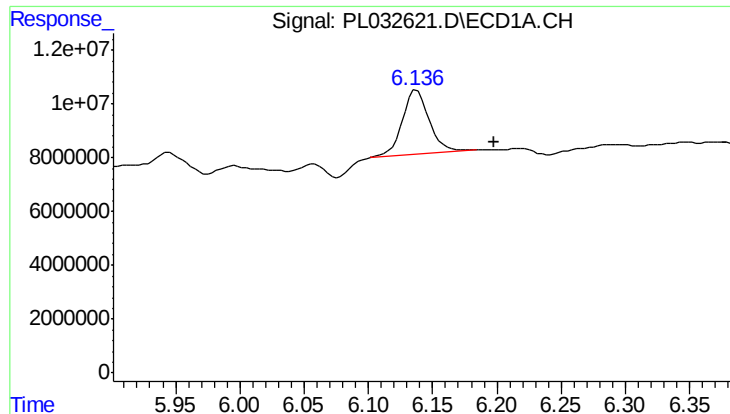

#15 Endosulfan II


R.T.: 6.138 min
Delta R.T.: -0.060 min
Response: 34665112
Conc: 2.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
EPE-121-2(20-22)

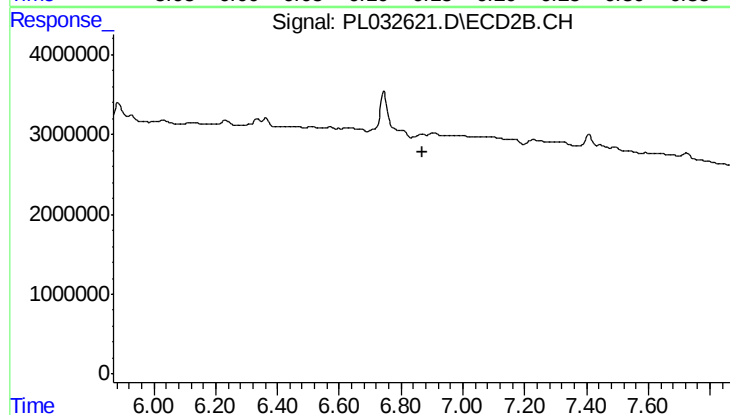


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.868 min
Response: 0
Conc: N.D.

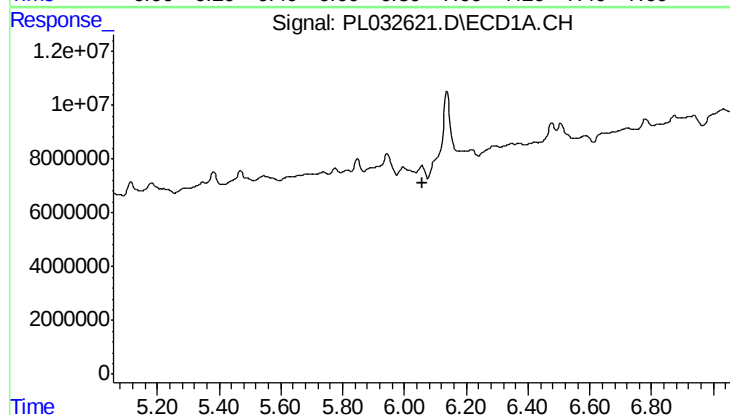


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.057 min
Response: 0
Conc: N.D.

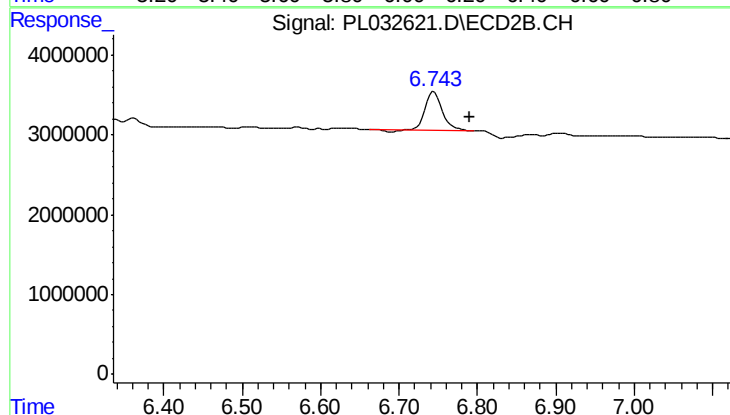

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: -0.045 min
Response: 7373026
Conc: 5.17 ng/ml

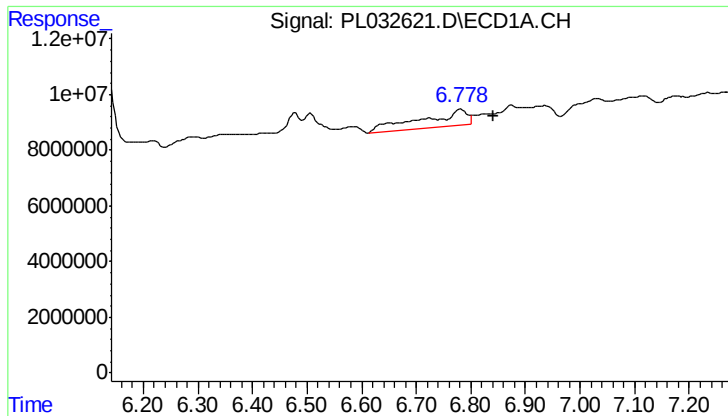

#20 Methoxychlor


R.T.: 6.781 min
Delta R.T.: -0.061 min
Response: 33978673
Conc: 5.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
EPE-121-2(20-22)

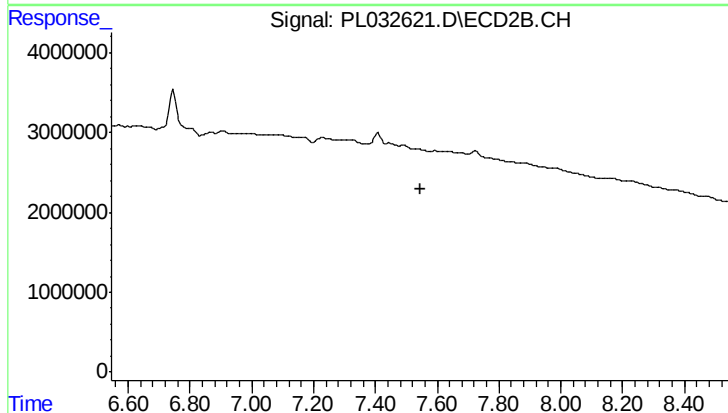


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.545 min
Response: 0
Conc: N.D.

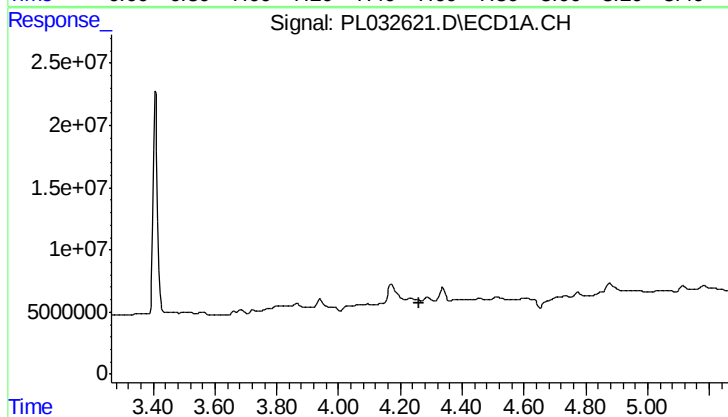


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.263 min
Response: 0
Conc: N.D.

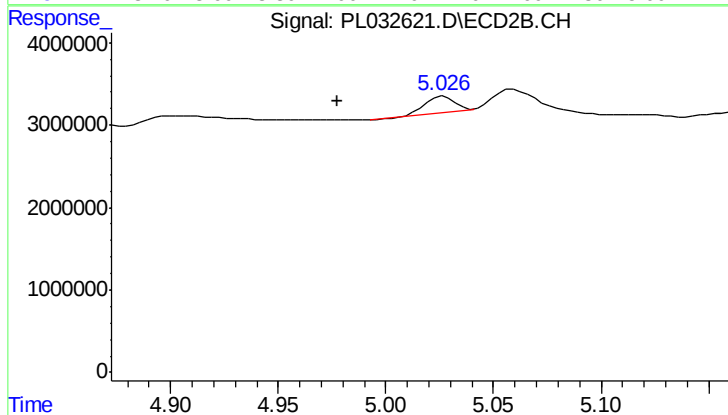

#23 Chlordane-1


R.T.: 5.027 min
Delta R.T.: 0.049 min
Response: 1667298
Conc: 21.56 ng/ml

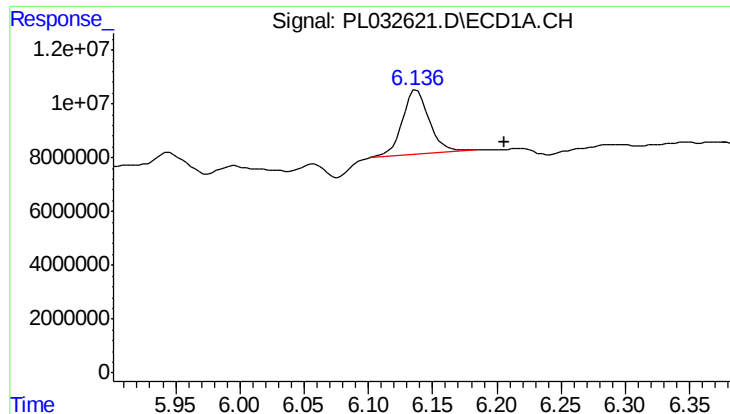

#27 Chlordane-5


R.T.: 6.138 min
Delta R.T.: -0.068 min
Response: 34665112
Conc: 70.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
EPE-121-2(20-22)

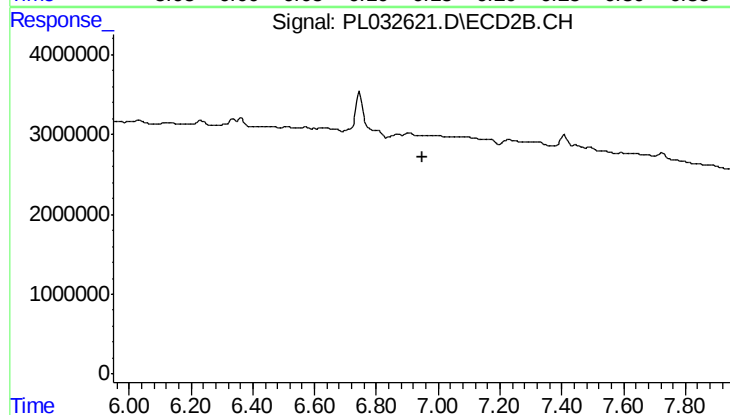


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.948 min
Response: 0
Conc: N.D.

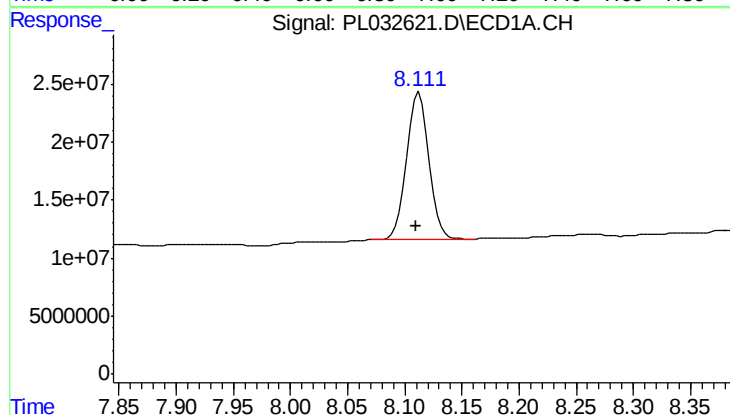

#28 Decachlorobiphenyl

R.T.: 8.113 min
Delta R.T.: 0.003 min
Response: 170907974
Conc: 14.69 ng/ml

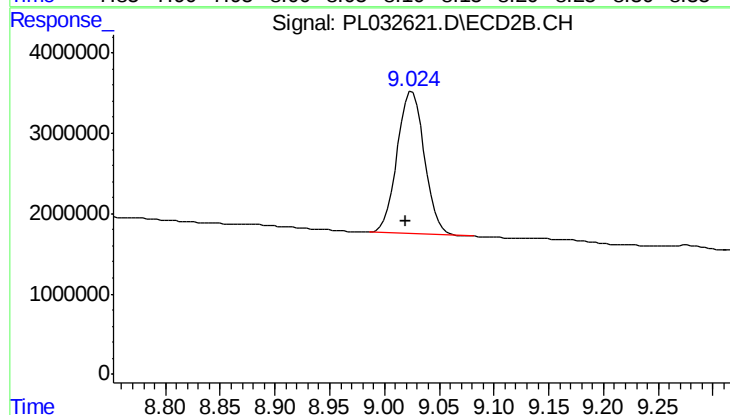

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.006 min
Response: 30188190
Conc: 15.87 ng/ml