

Data Path : P:\HPCHEM1\ECD_L\Data\PL012918\
 Data File : PL032683.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2018 4:38
 Operator : UA\AJ
 Sample : J1290-15
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-43-0-2.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 08:28:38 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 04:03:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.994	111.2E6	16731465	12.438	13.360
28)	SA Decachlor...	8.115	9.027	92783634	19138656	7.974	10.062 #
Target Compounds							
6)	B beta-BHC	4.337f	0.000	10815924	0	1.894	N.D. #
7)	B delta-BHC	0.000	5.030	0	1631377	N.D.	0.734 #
9)	A Endosulfan I	0.000	6.162f	0	1711224	N.D.	0.948 #
11)	B alpha-Chl...	0.000	6.162	0	1711224	N.D.	0.903 #
15)	B Endosulfa...	6.139f	0.000	23187890	0	1.976	N.D. #
16)	A 4,4'-DDD	0.000	6.745f	0	4435551	N.D.	3.110 #
23)	Chlordane-1	0.000	5.030	0	1631377	N.D.	21.098 #
26)	Chlordane-4	0.000	6.162	0	1711224	N.D.	5.238 #
27)	Chlordane-5	6.139	0.000	23187890	0	46.898	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_L\Data\PL012918\
Data File : PL032683.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2018 4:38
Operator : UA\AJ
Sample : J1290-15
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SB-43-0-2.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 08:28:38 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 04:03:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

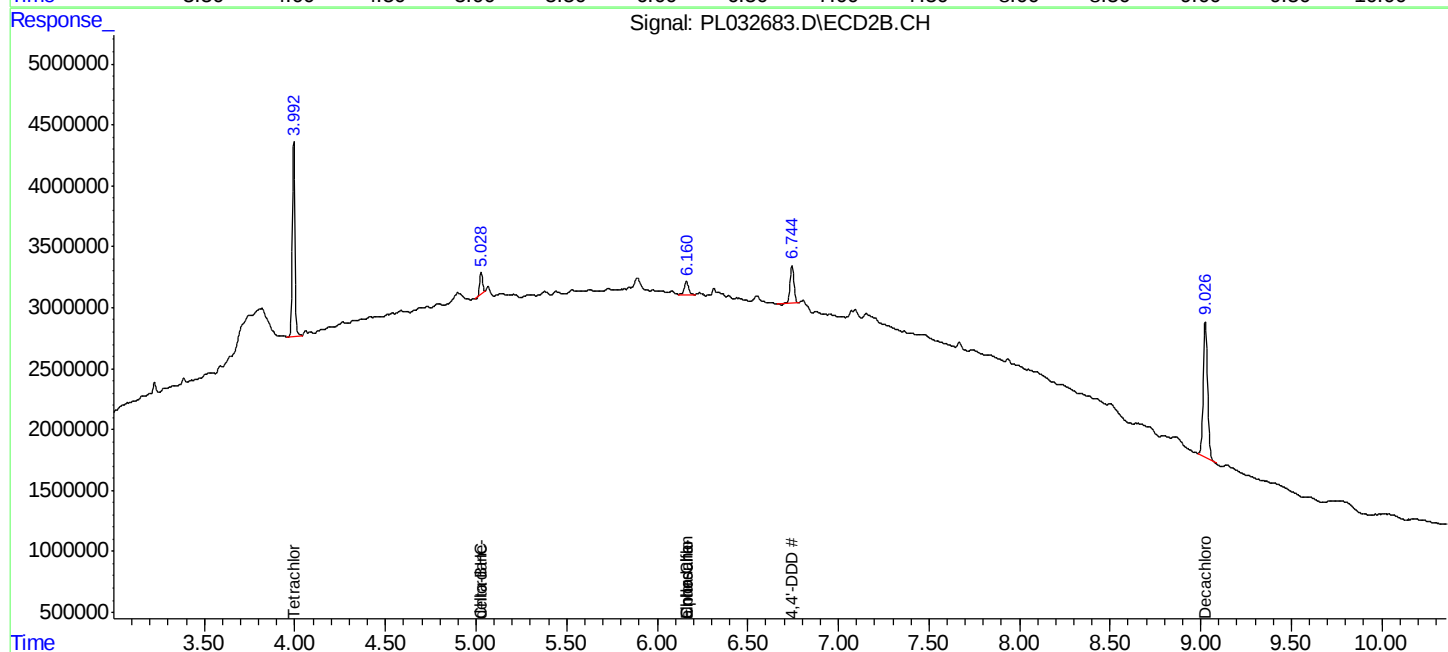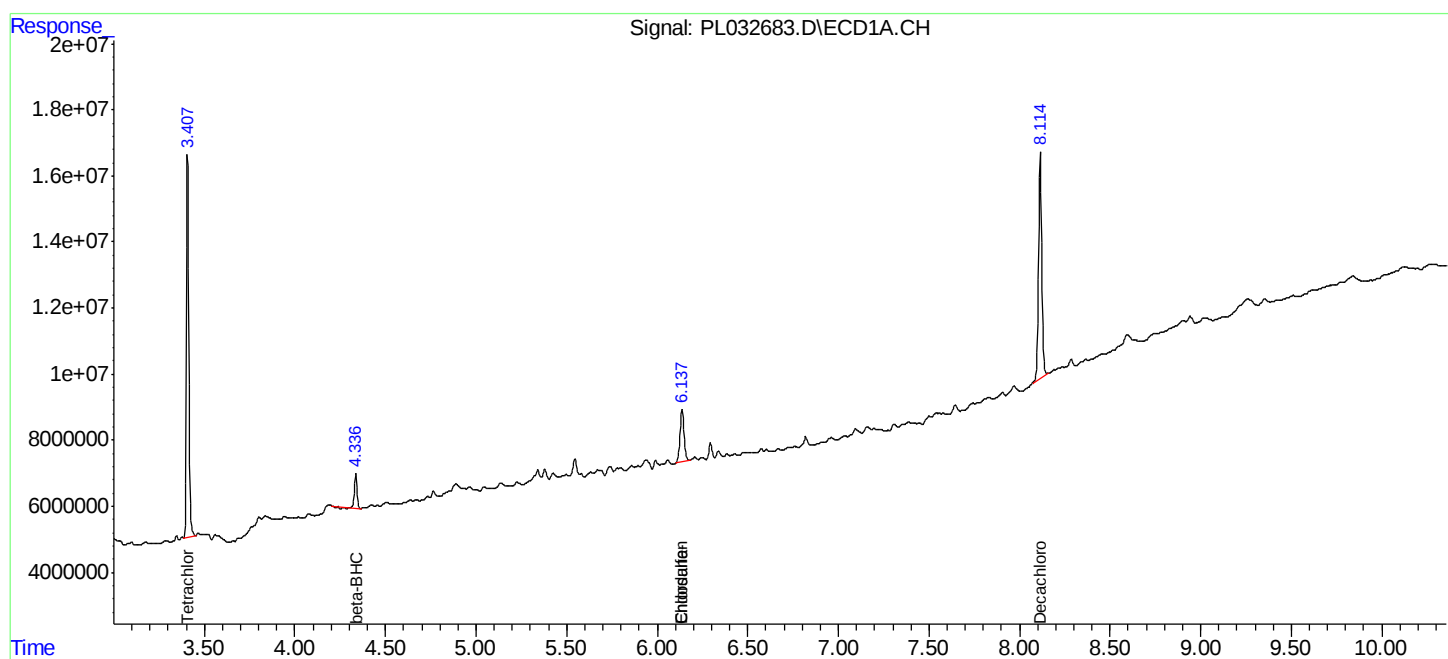


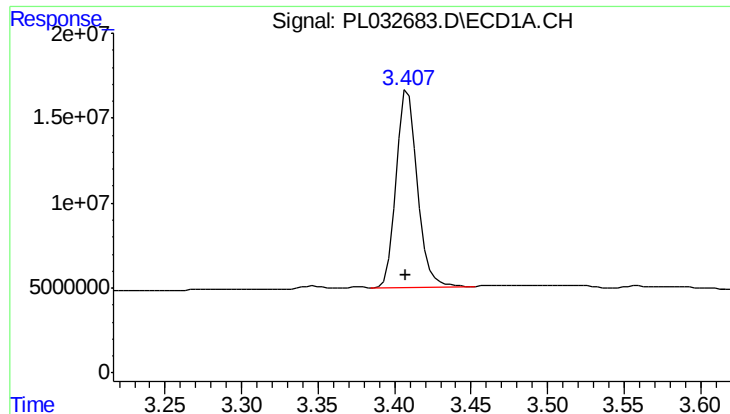

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.002 min
Response: 111200629
Conc: 12.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-43-0-2.0

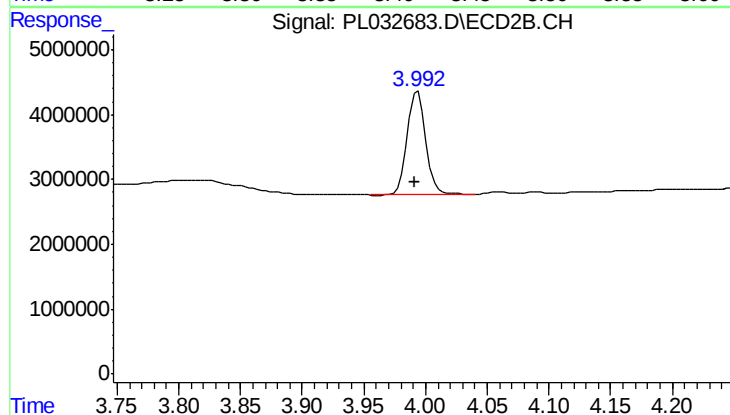


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: 0.002 min
Response: 16731465
Conc: 13.36 ng/ml

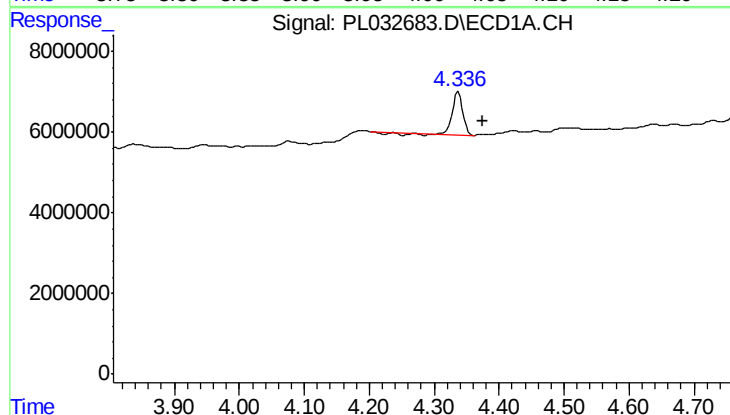


#6 beta-BHC

R.T.: 4.337 min
Delta R.T.: -0.039 min
Response: 10815924
Conc: 1.89 ng/ml

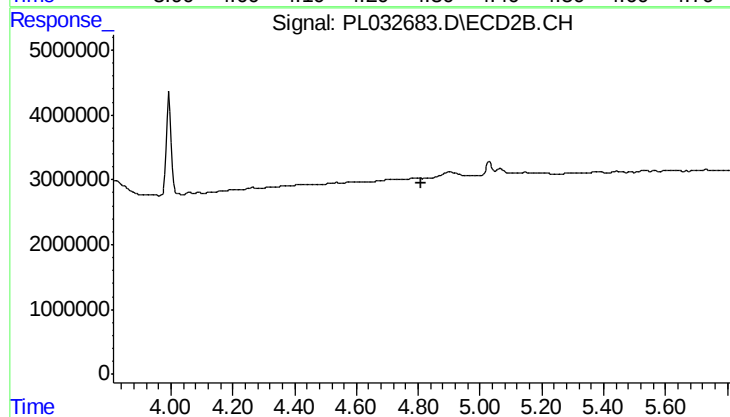

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.811 min
Response: 0
Conc: N.D.

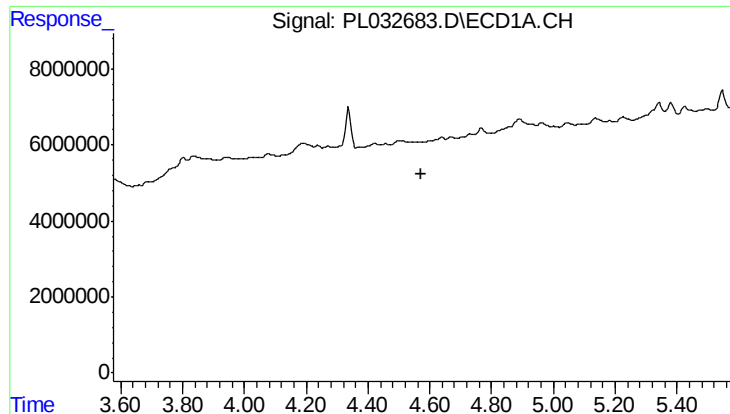

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-43-0-2.0

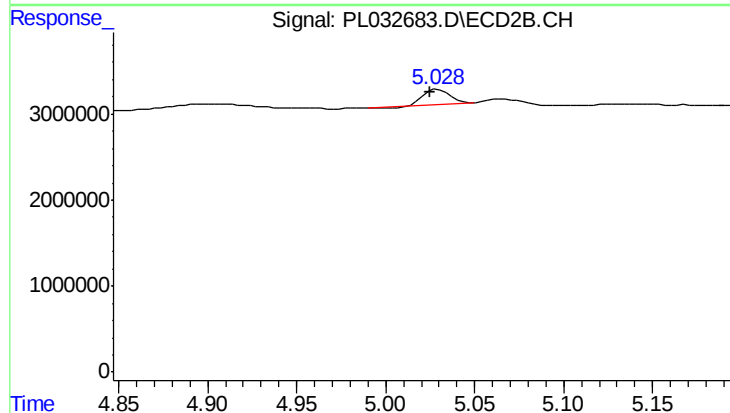


#7 delta-BHC

R.T.: 5.030 min
Delta R.T.: 0.005 min
Response: 1631377
Conc: 0.73 ng/ml

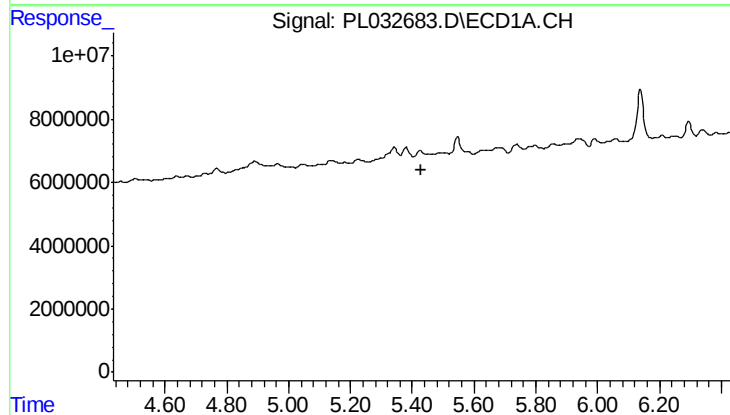


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.430 min
Response: 0
Conc: N.D.

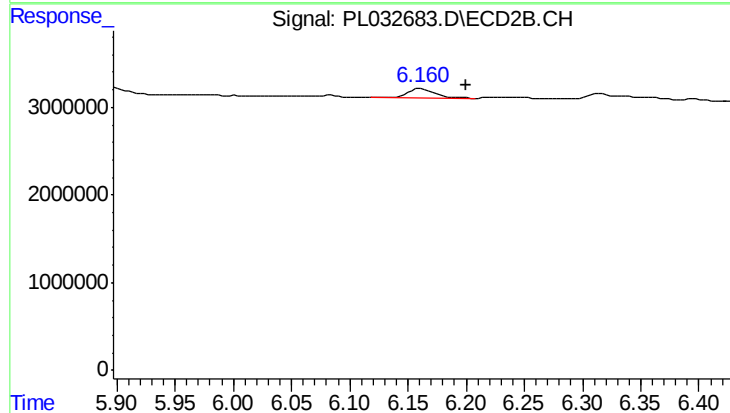

#9 Endosulfan I


R.T.: 6.162 min
Delta R.T.: -0.038 min
Response: 1711224
Conc: 0.95 ng/ml

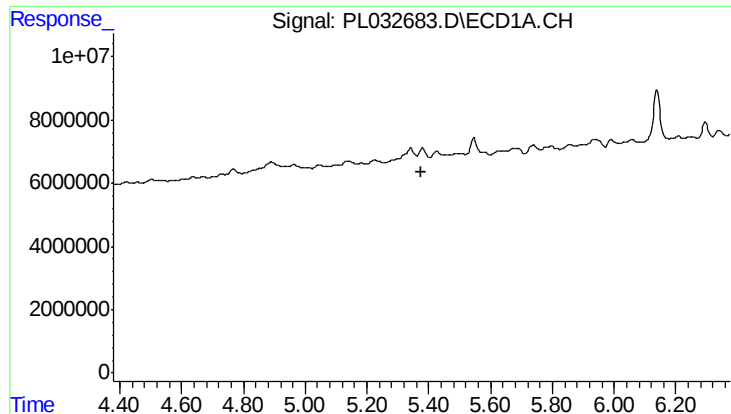

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-43-0-2.0

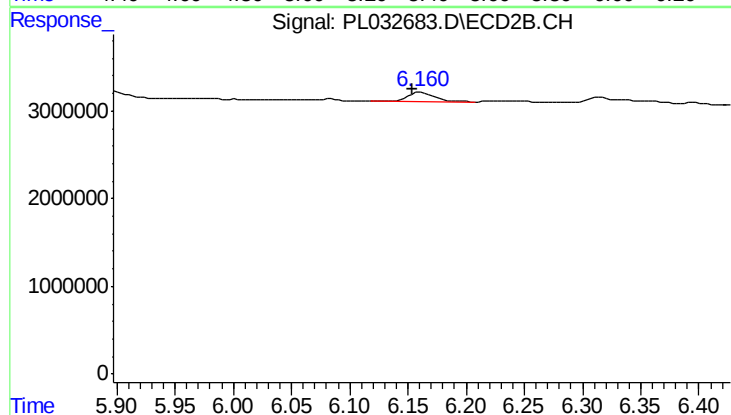


#11 alpha-Chlordane

R.T.: 6.162 min
Delta R.T.: 0.007 min
Response: 1711224
Conc: 0.90 ng/ml

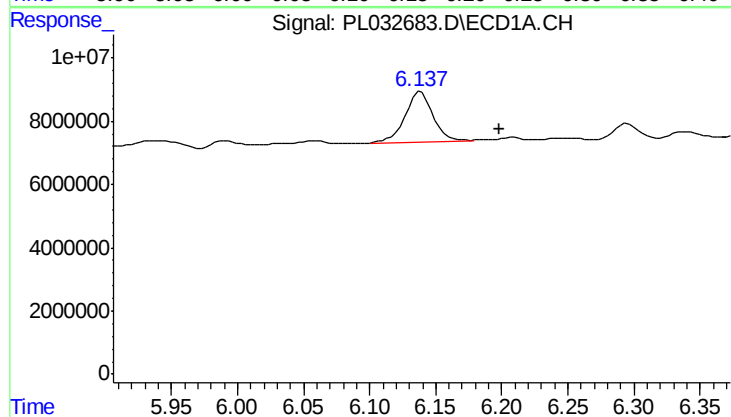


#15 Endosulfan II

R.T.: 6.139 min
Delta R.T.: -0.059 min
Response: 23187890
Conc: 1.98 ng/ml

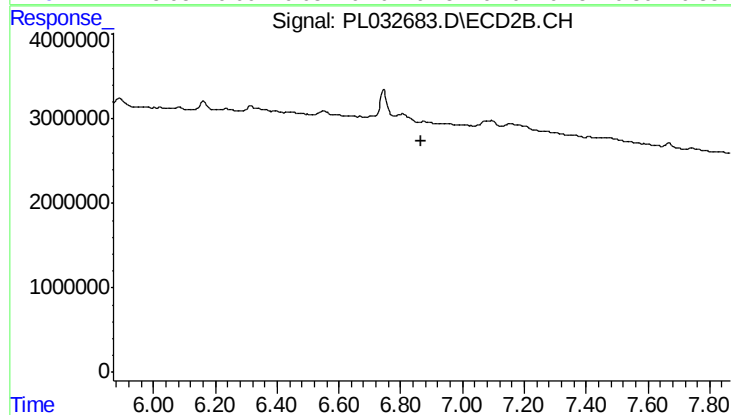

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.868 min
Response: 0
Conc: N.D.

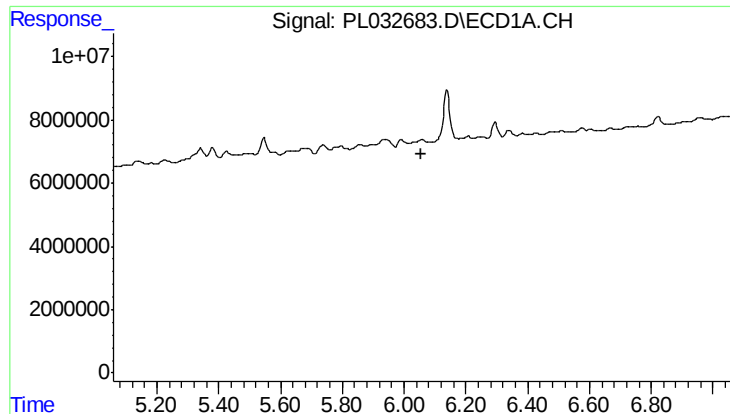

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-43-0-2.0

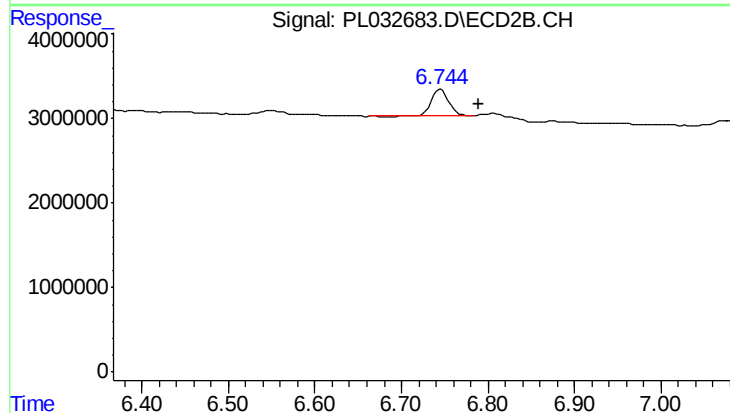


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: -0.045 min
Response: 4435551
Conc: 3.11 ng/ml

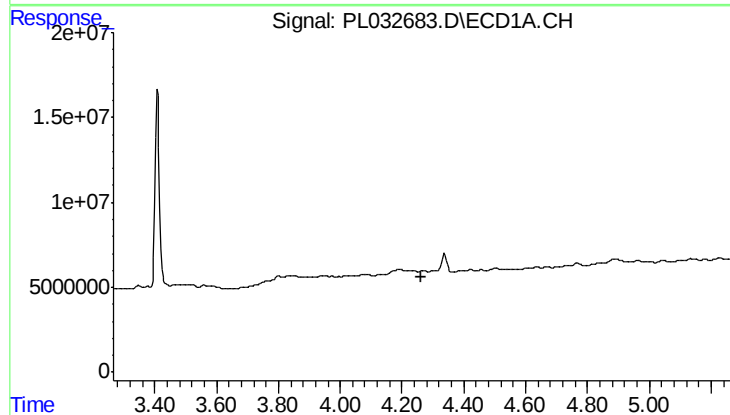


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.263 min
Response: 0
Conc: N.D.

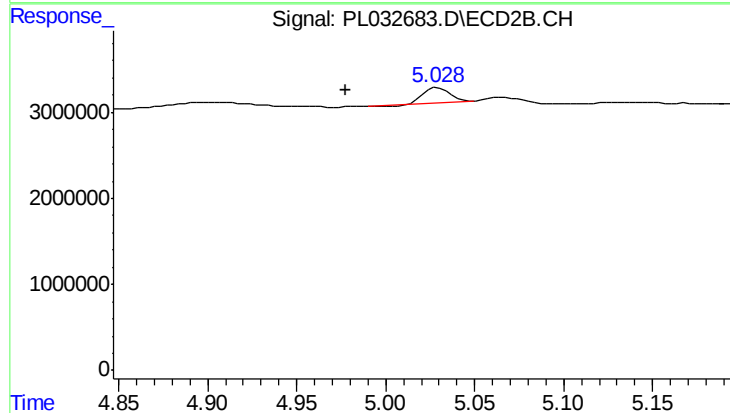

#23 Chlordane-1


R.T.: 5.030 min
Delta R.T.: 0.052 min
Response: 1631377
Conc: 21.10 ng/ml

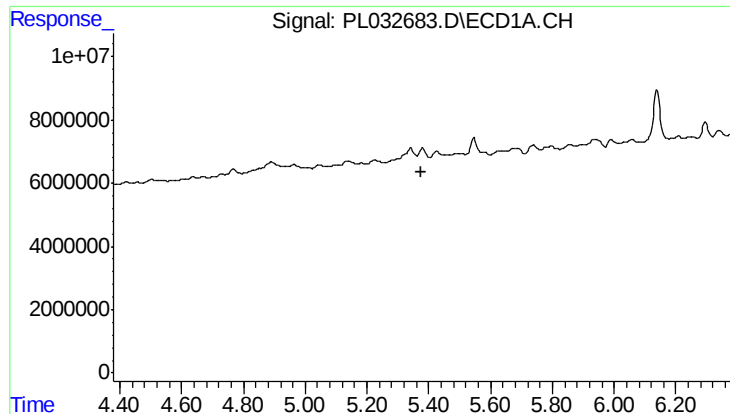

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-43-0-2.0

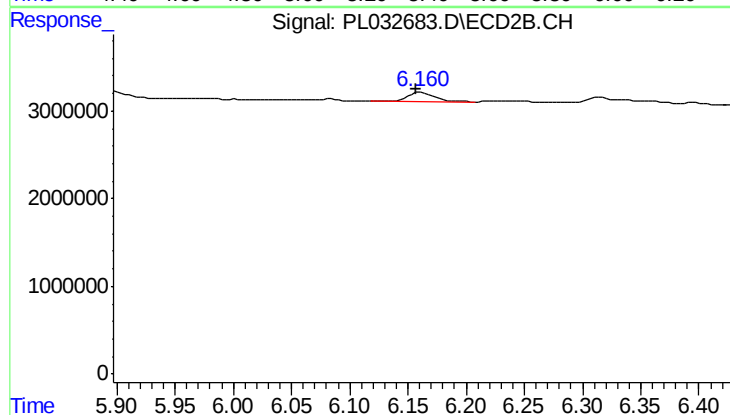


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.004 min
Response: 1711224
Conc: 5.24 ng/ml

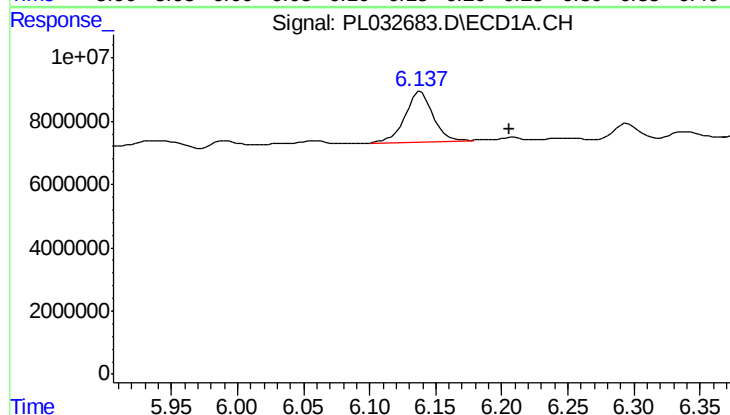


#27 Chlordane-5

R.T.: 6.139 min
Delta R.T.: -0.067 min
Response: 23187890
Conc: 46.90 ng/ml

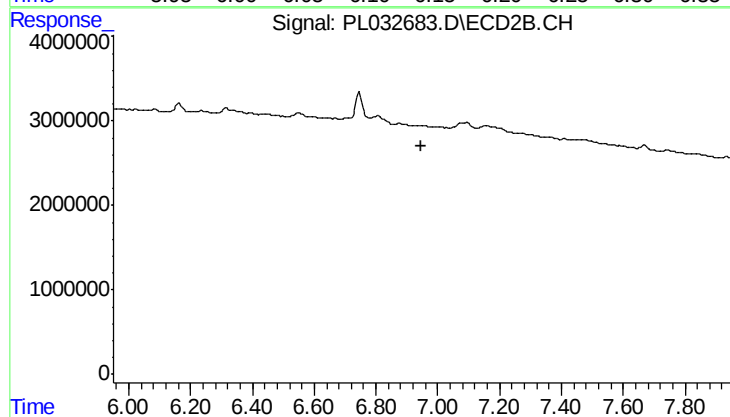

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.948 min
Response: 0
Conc: N.D.

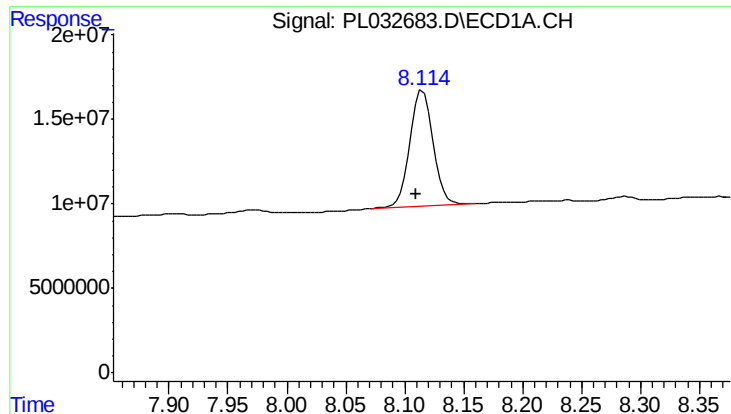

#28 Decachlorobiphenyl

R.T.: 8.115 min
Delta R.T.: 0.005 min
Response: 92783634
Conc: 7.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-43-0-2.0

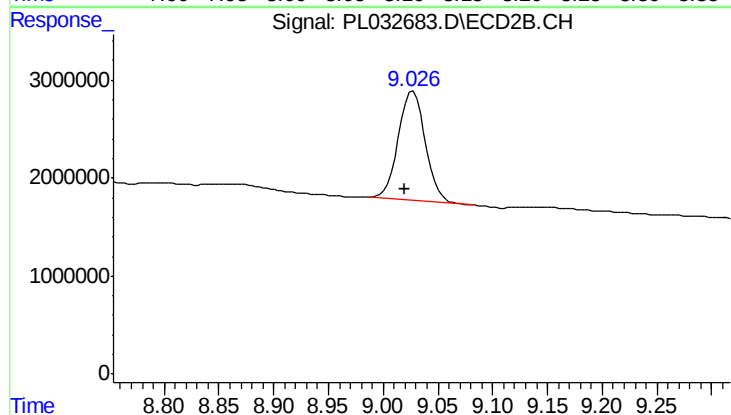

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.008 min
Response: 19138656
Conc: 10.06 ng/ml