

Data Path : P:\HPCHEM1\ECD L\Data\PL012918\
 Data File : PL032641.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2018 17:59
 Operator : UA\AJ
 Sample : J1305-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RECLAIMER-SLUDGE-PIT

Manual Integrations
 APPROVED

ugo
 1/30/2018 2:53:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 08:50:22 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 04:03:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.407	3.992	147.7E6	19094476	16.525m	15.247m
28)	SA Decachlor...	8.112	9.027	119.9E6	10473601	10.302	5.506 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD L\Data\PL012918\
Data File : PL032641.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2018 17:59
Operator : UA\AJ
Sample : J1305-05
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RECLAIMER-SLUDGE-PIT


Manual Integrations
APPROVED

ugo
1/30/2018 2:53:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 08:50:22 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 04:03:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

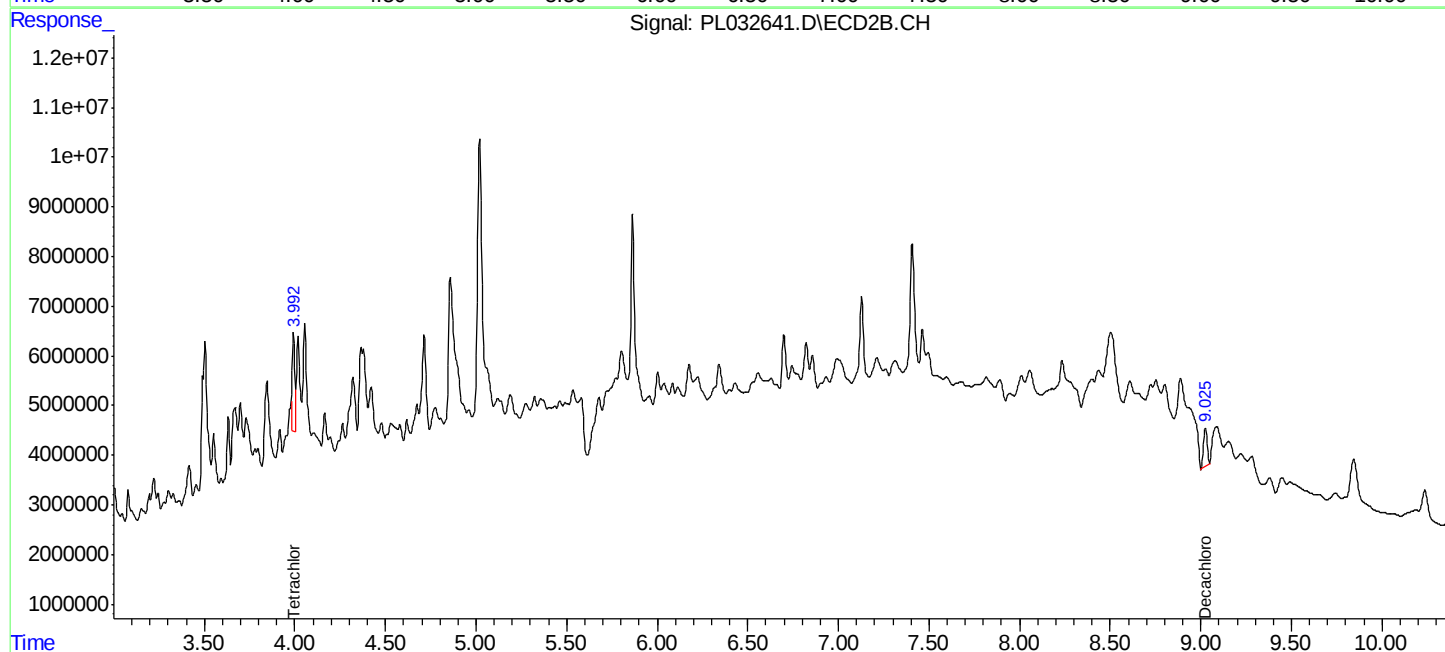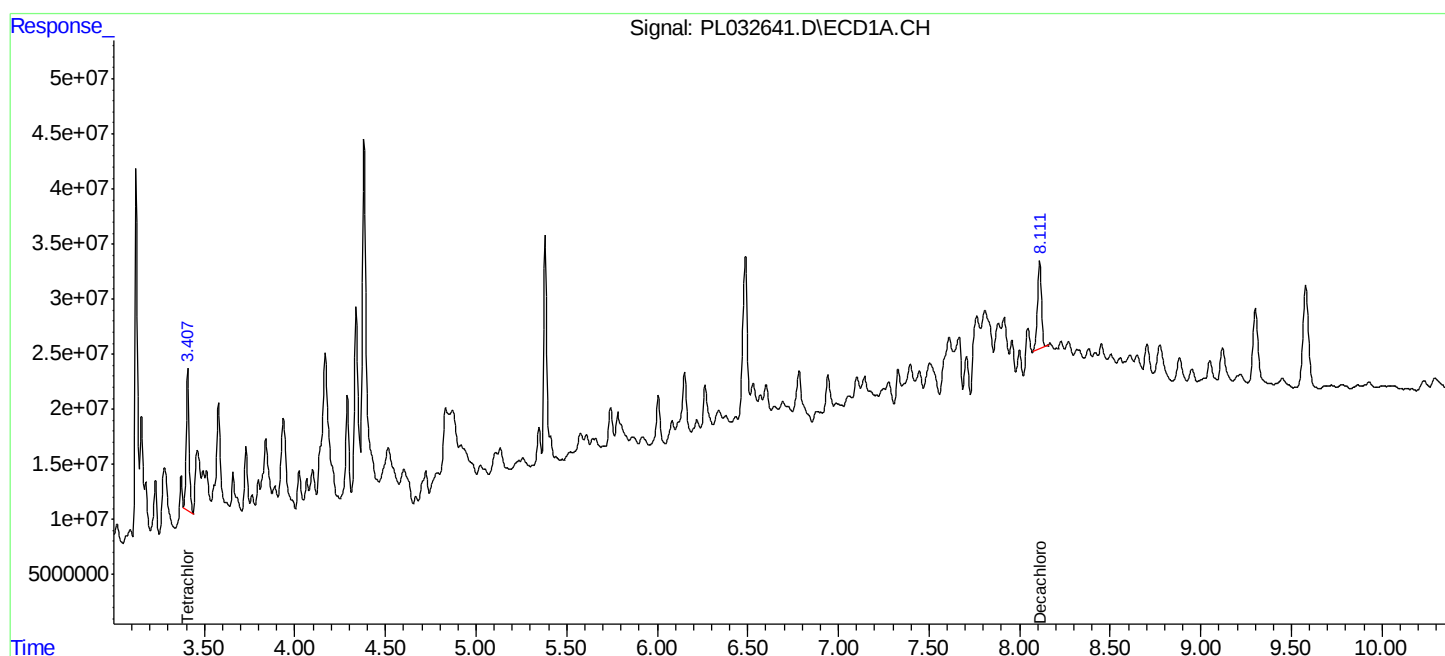

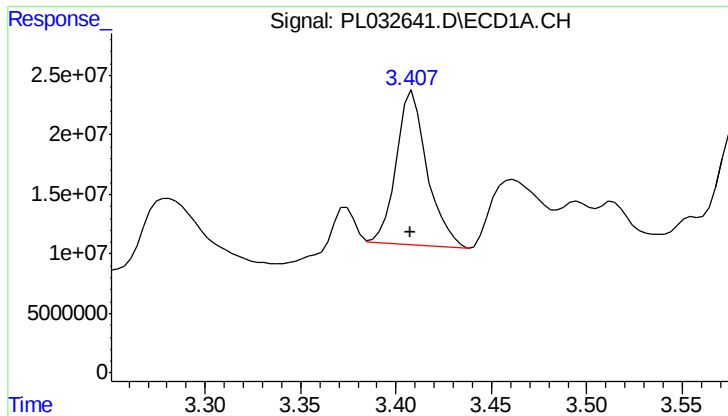


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 147732416
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
RECLAIMER-SLUDGE-PIT


Manual Integrations
APPROVED

ugo
1/30/2018 2:53:05 PM

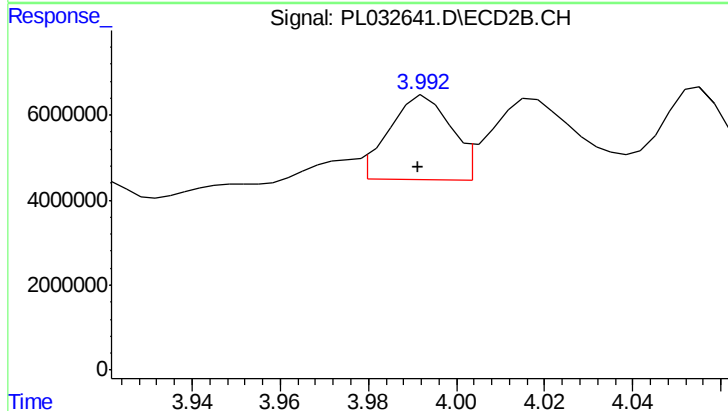


#1 Tetrachloro-m-xylene

R.T.: 3.992 min
Delta R.T.: 0.000 min
Response: 19094476
Conc: 15.25 ng/ml m

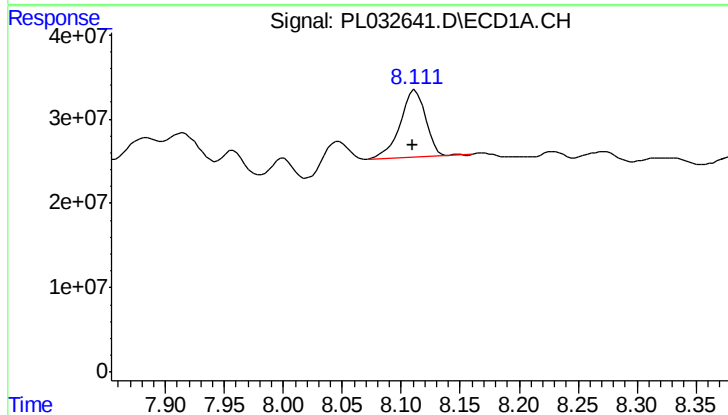

#28 Decachlorobiphenyl

R.T.: 8.112 min
Delta R.T.: 0.002 min
Response: 119867997
Conc: 10.30 ng/ml

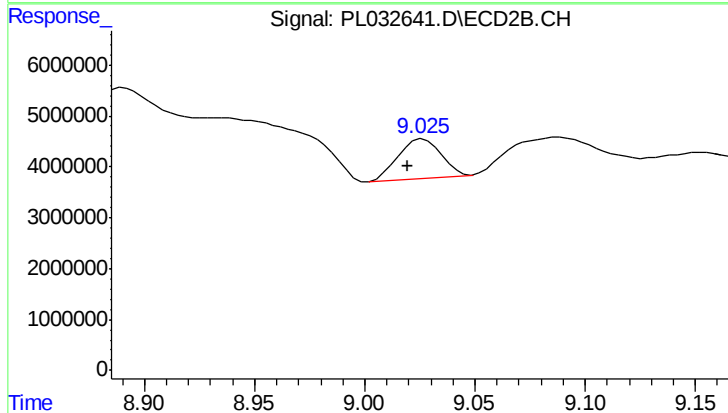

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.007 min
Response: 10473601
Conc: 5.51 ng/ml