

Data Path : P:\HPCHEM1\ECD L\Data\PL012918\
 Data File : PL032662.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2018 23:19
 Operator : UA\AJ
 Sample : J1345-02
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RECLAIMER-TANK

Manual Integrations
 APPROVED

ugo
 1/30/2018 2:53:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:00:07 2018
 Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 27 04:03:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.406	3.993	174.0E6	29272536	19.468m	23.375
28) SA Decachlor...	8.114	9.026	142.3E6	26026353	12.227	13.683

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD L\Data\PL012918\
Data File : PL032662.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2018 23:19
Operator : UA\AJ
Sample : J1345-02
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RECLAIMER-TANK


Manual Integrations
APPROVED

ugo
1/30/2018 2:53:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:00:07 2018
Quant Method : P:\HPCHEM1\ECD_L\methods\PL012618.M
Quant Title : GC Extractables
QLast Update : Sat Jan 27 04:03:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

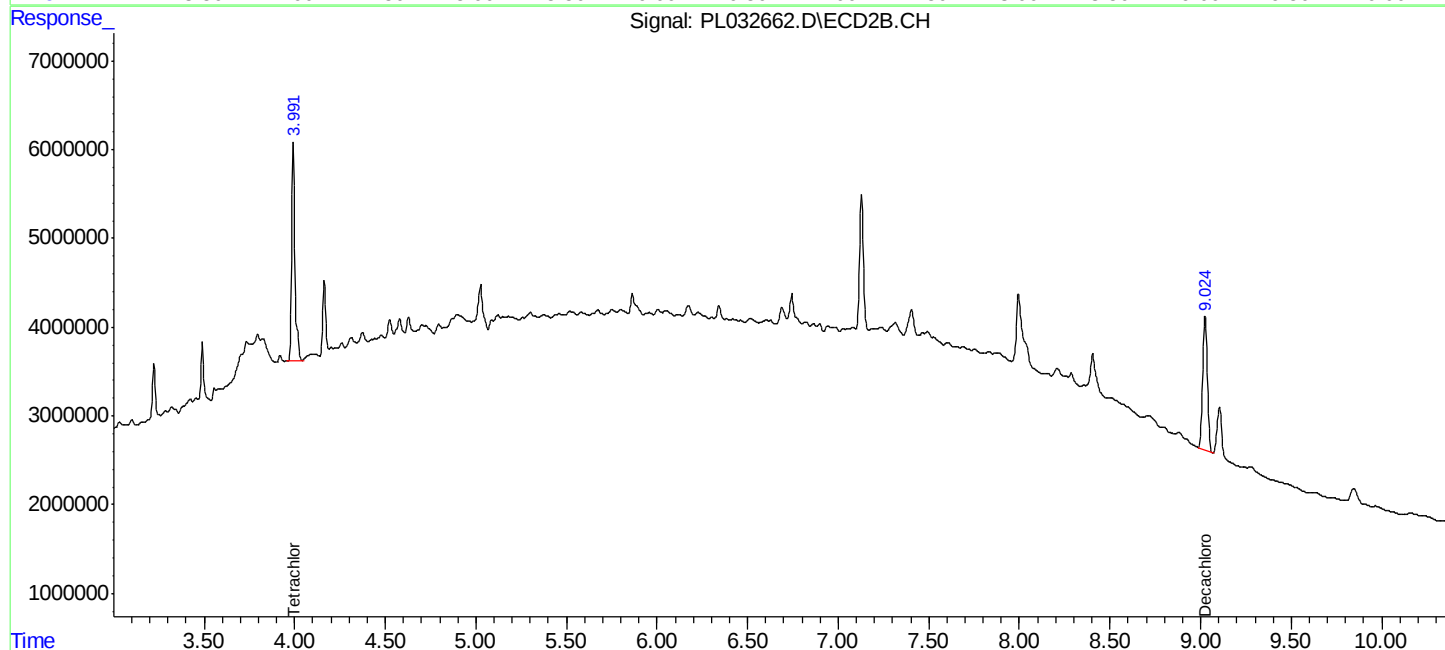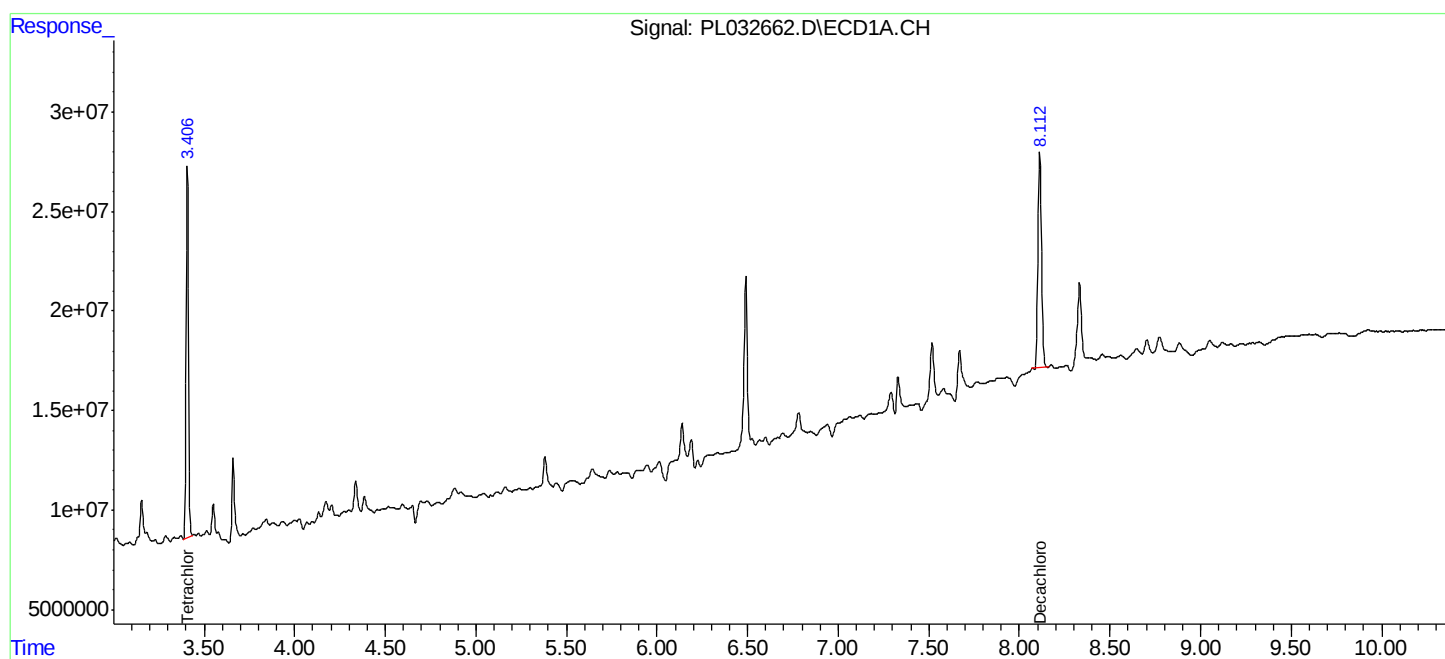

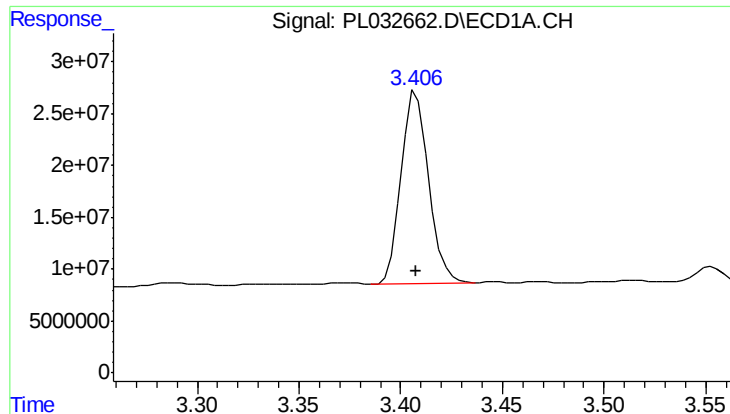


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 174042888
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
RECLAIMER-TANK


Manual Integrations
APPROVED

ugo
1/30/2018 2:53:31 PM

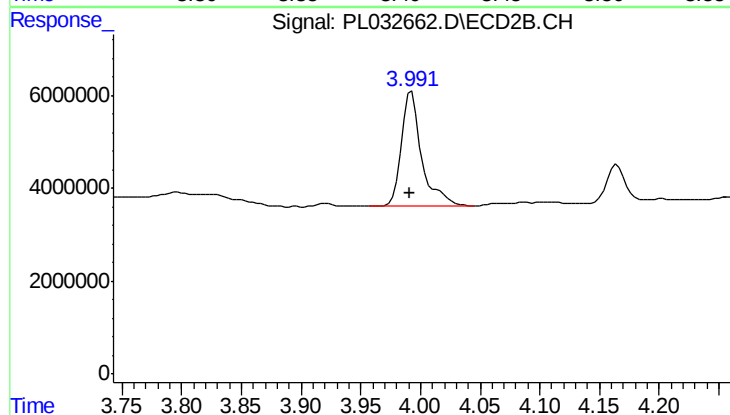


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: 0.001 min
Response: 29272536
Conc: 23.37 ng/ml

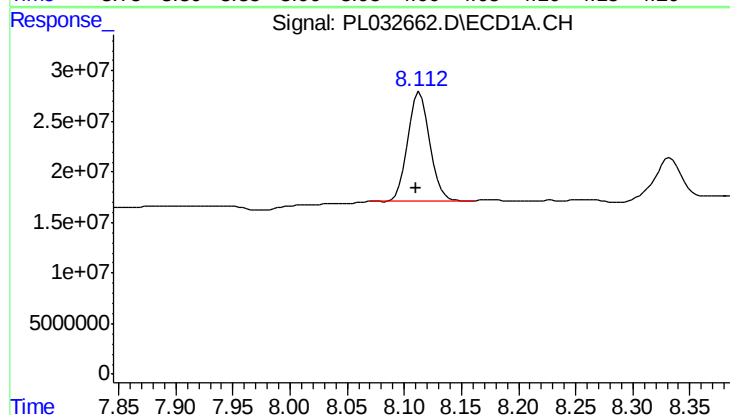

#28 Decachlorobiphenyl

R.T.: 8.114 min
Delta R.T.: 0.004 min
Response: 142272536
Conc: 12.23 ng/ml

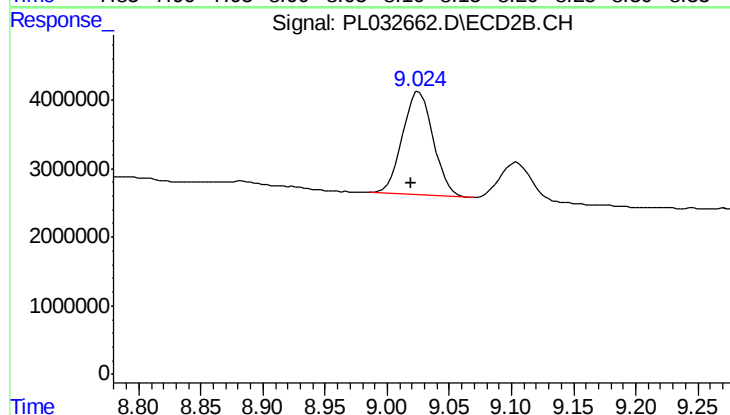

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.007 min
Response: 26026353
Conc: 13.68 ng/ml