

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
 Data File : PL056169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 10:36
 Operator : AJ\MA
 Sample : L1008-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-012420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 11:10:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.015	197.3E6	57647842	18.841	19.715
28)	SA Decachlor...	8.260	9.096	212.9E6	47219823	20.218	20.876
Target Compounds							
14)	MA Endrin	6.065	0.000	65187199	0	4.639	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
Data File : PL056169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 10:36
Operator : AJ\MA
Sample : L1008-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-012420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 11:10:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

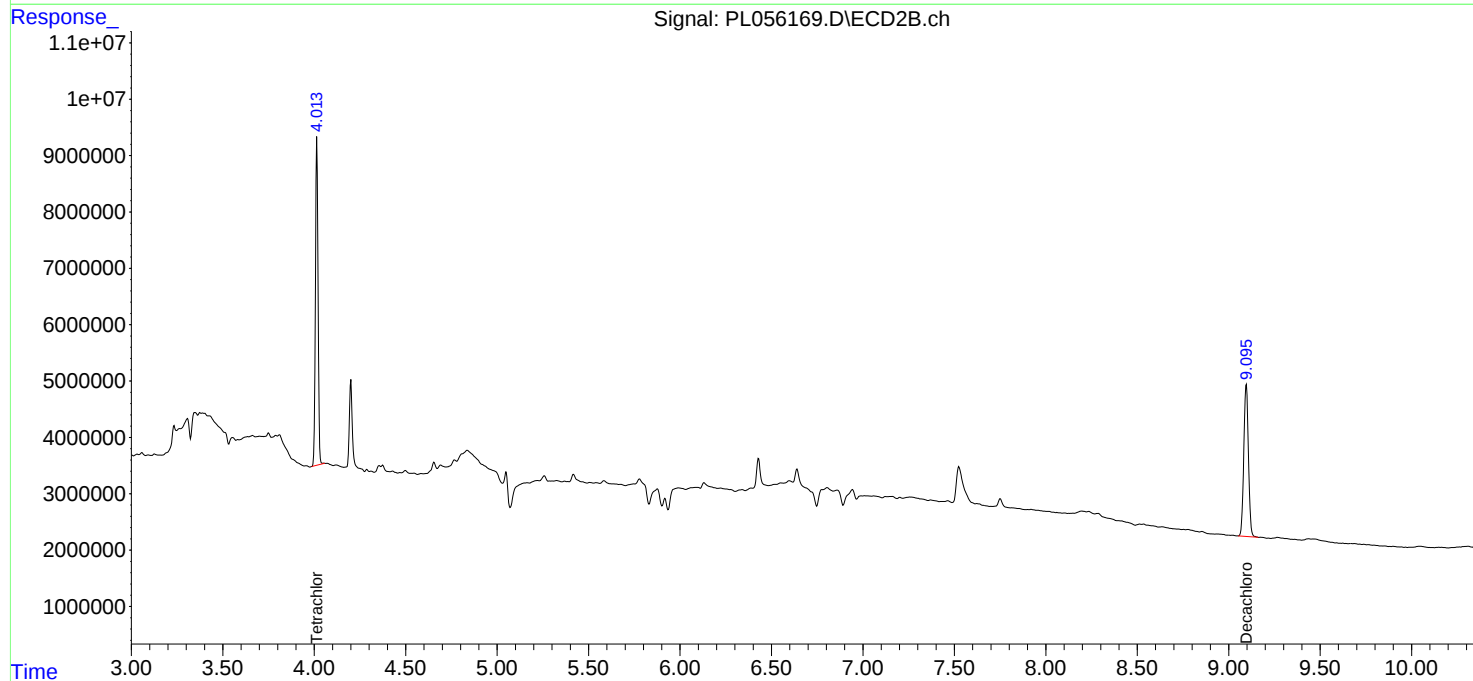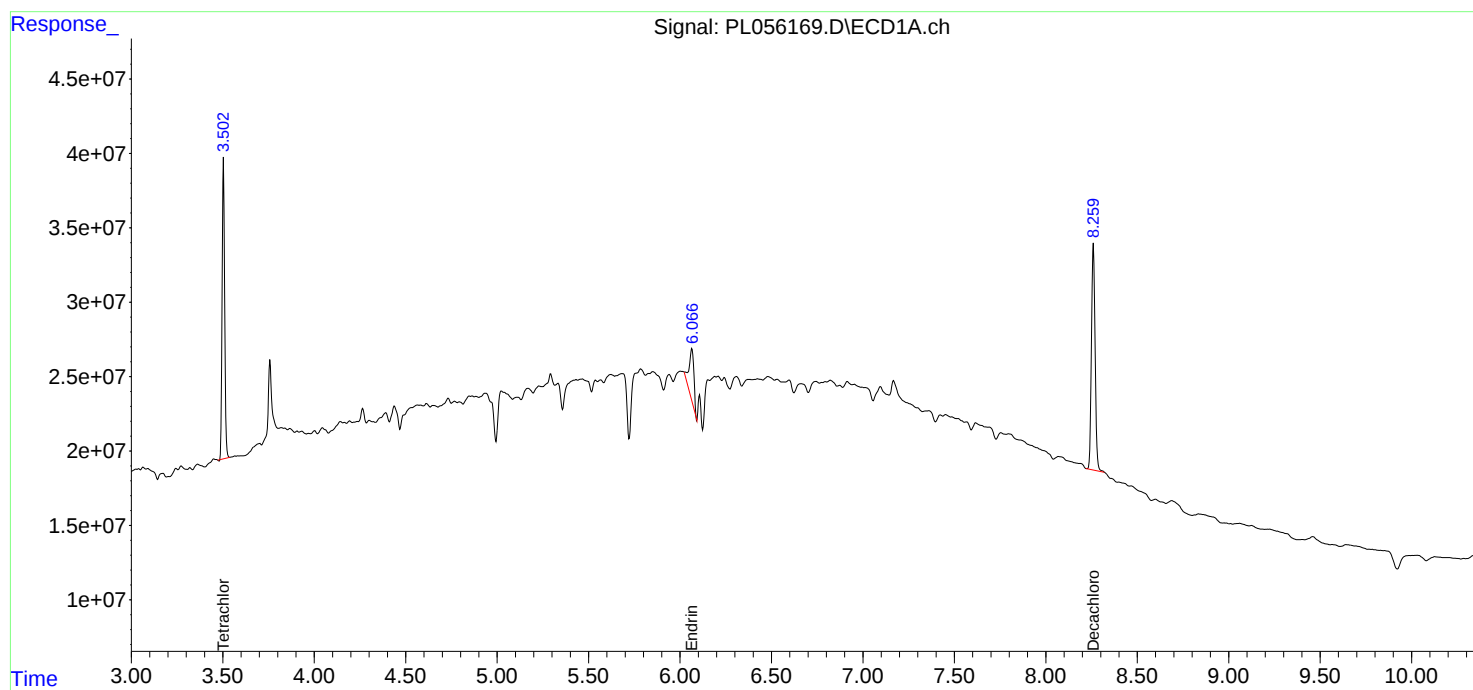


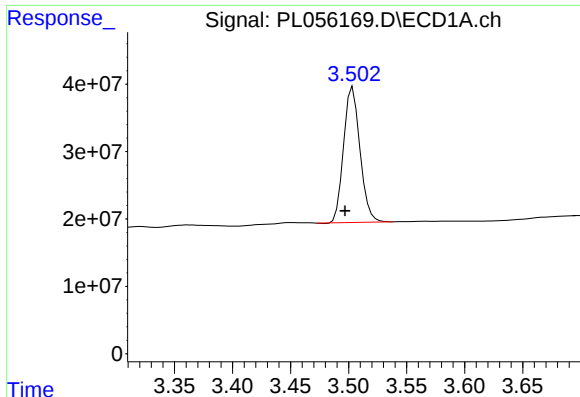

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.007 min
Response: 197324389
Conc: 18.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-012420

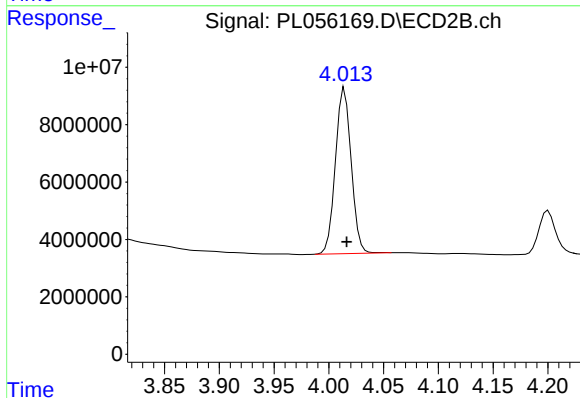


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.002 min
Response: 57647842
Conc: 19.71 ng/ml

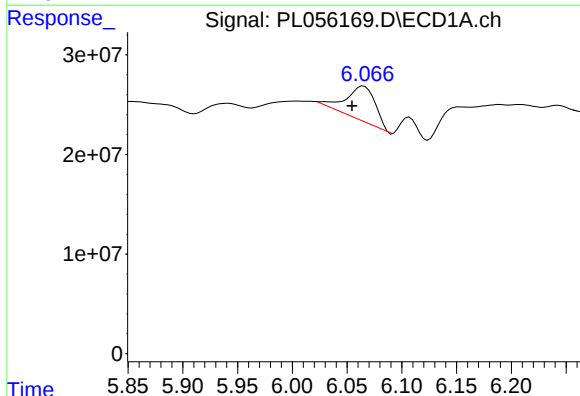


#14 Endrin

R.T.: 6.065 min
Delta R.T.: 0.011 min
Response: 65187199
Conc: 4.64 ng/ml

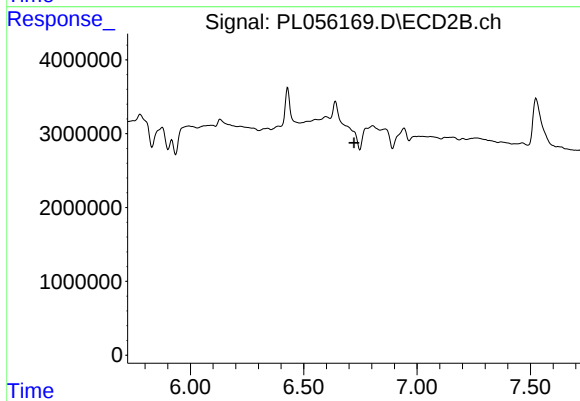

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.723 min
Response: 0
Conc: N.D.

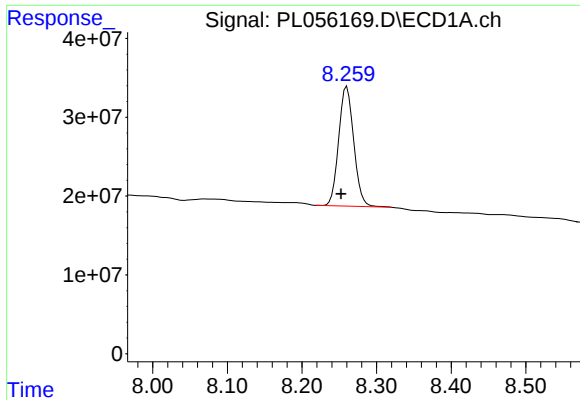

#28 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.008 min
Response: 212853635
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-012420

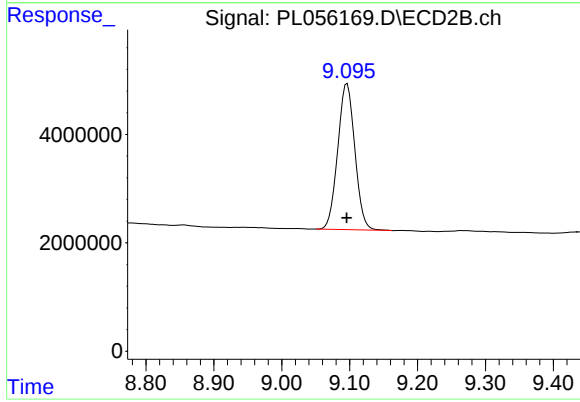

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 47219823
Conc: 20.88 ng/ml