

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
 Data File : PL056174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 13:06
 Operator : AJ\MA
 Sample : L1274-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BORING-B1-SAMPLE-S1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 15:22:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.015	132.7E6	36601974	12.671	12.517
28)	SA Decachlor...	8.253	9.094	135.3E6	34442191	12.852	15.227
Target Compounds							
23)	Chlordane-1	4.374	0.000	12914615	0	34.117	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
Data File : PL056174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 13:06
Operator : AJ\MA
Sample : L1274-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BORING-B1-SAMPLE-S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 15:22:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

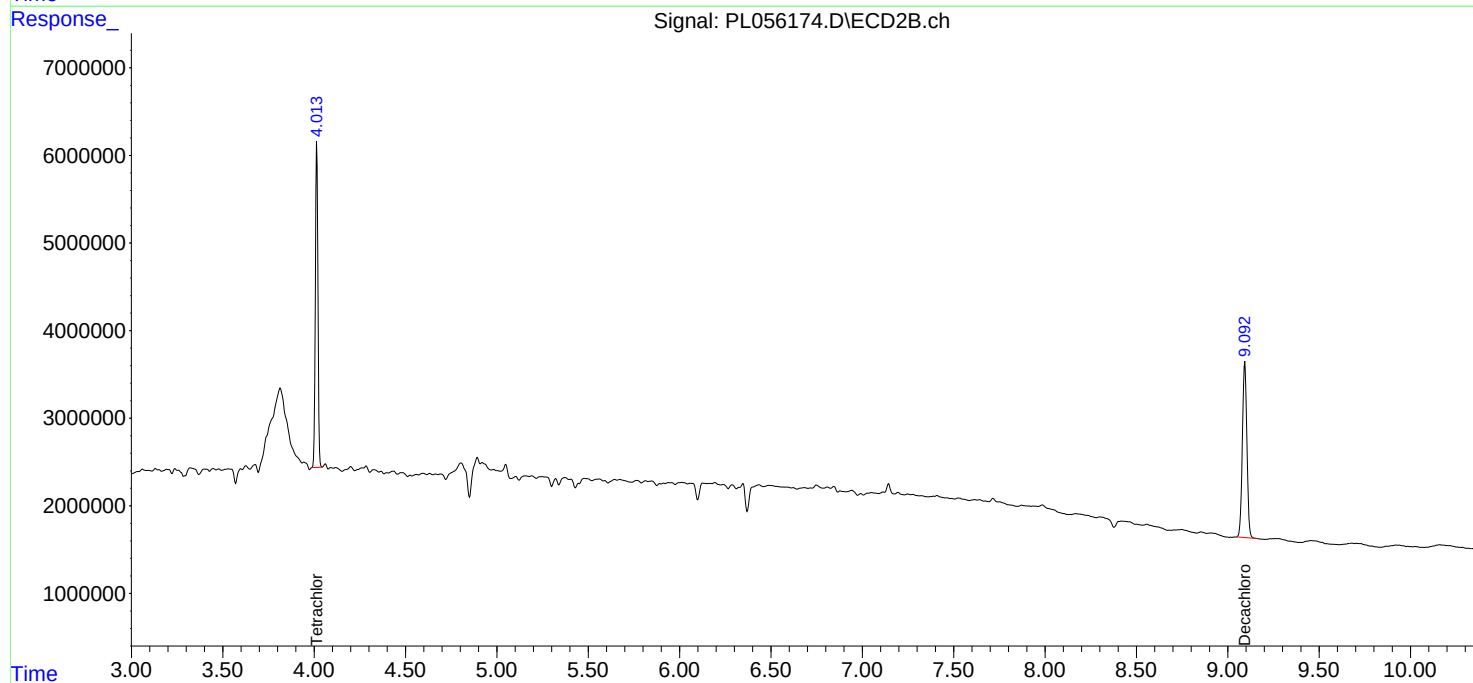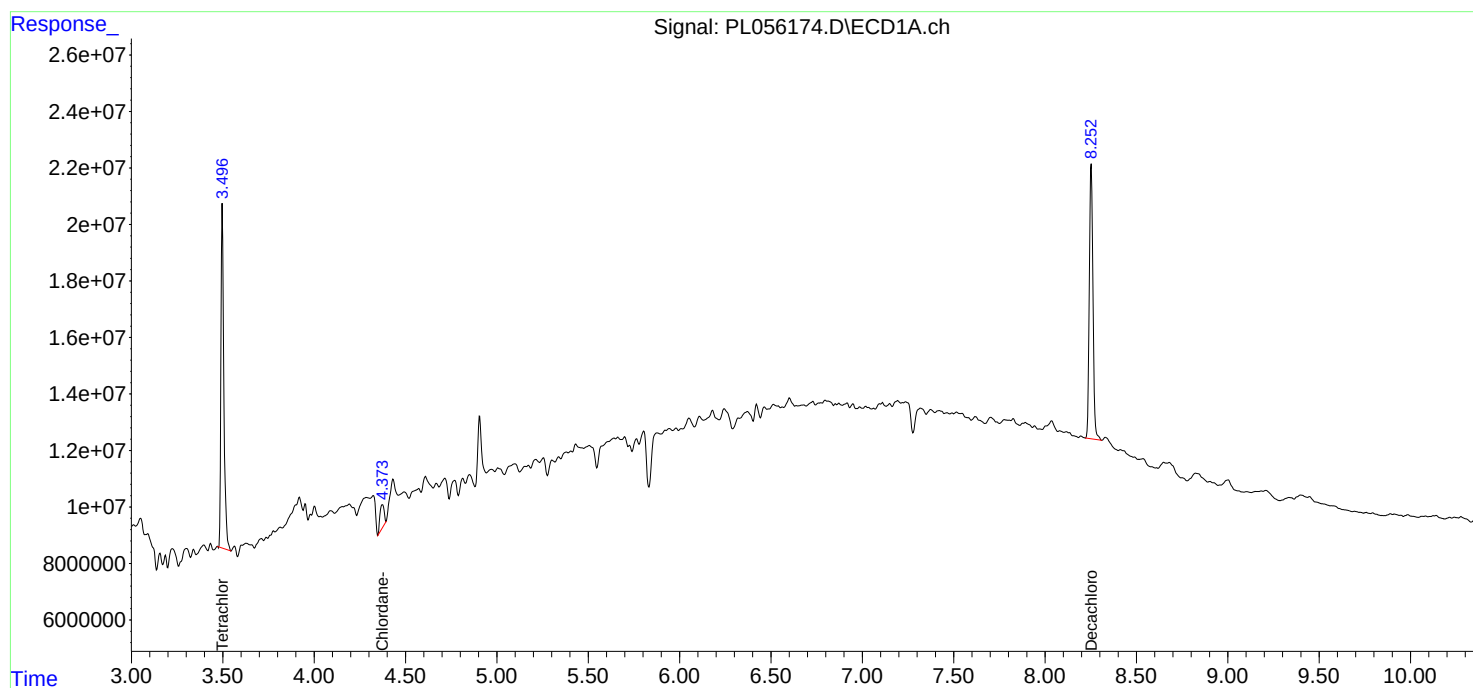


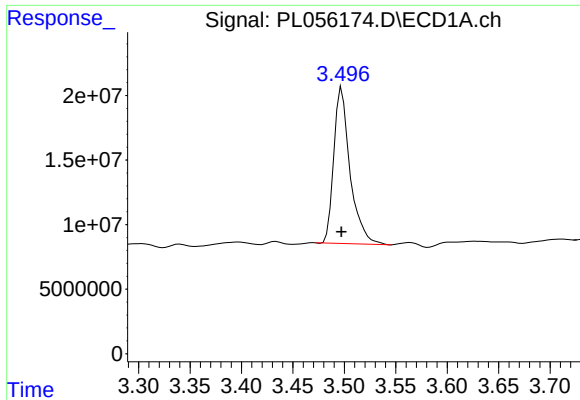

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 132701314
Conc: 12.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORING-B1-SAMPLE-S1

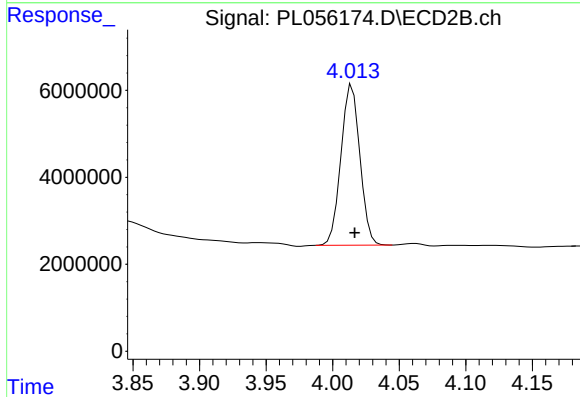


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.002 min
Response: 36601974
Conc: 12.52 ng/ml

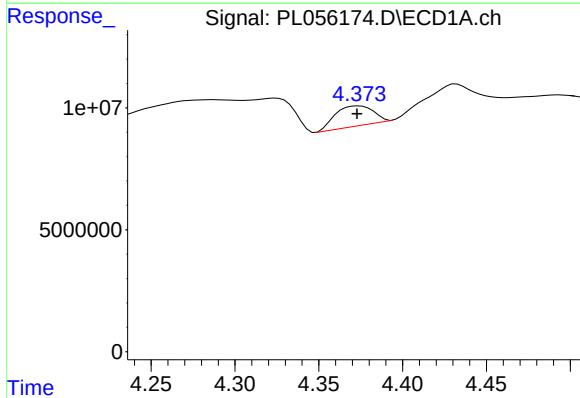


#23 Chlordane-1

R.T.: 4.374 min
Delta R.T.: 0.001 min
Response: 12914615
Conc: 34.12 ng/ml

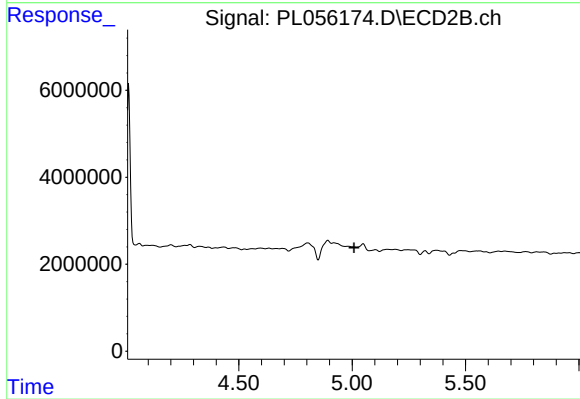

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

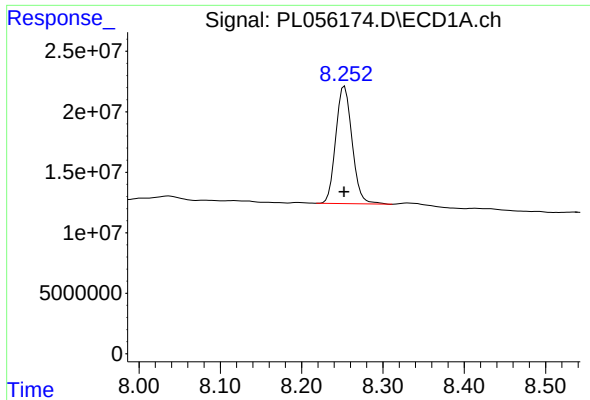

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 135303776
Conc: 12.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
BORING-B1-SAMPLE-S1

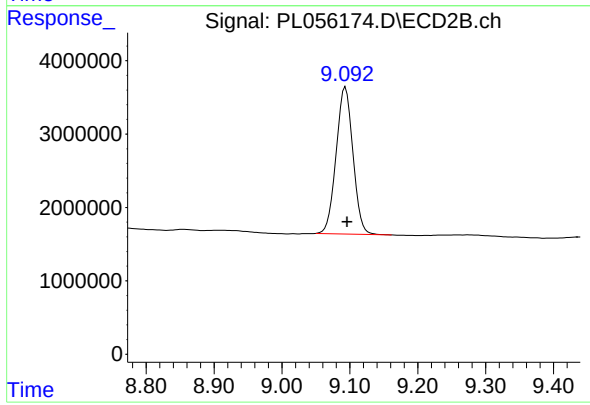

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.002 min
Response: 34442191
Conc: 15.23 ng/ml